

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122319\
 Data File : BM024277.D
 Acq On : 25 Dec 2019 05:11
 Operator : JU
 Sample : K6240-23
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFQT0

Manual Integrations
 APPROVED

mohammad
 12/26/2019 4:00:38 PM

Quant Time: Dec 25 06:51:51 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 25 03:33:48 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.43	152	305748	20.00	ng/ul	0.00
18) Naphthalene-d8	10.19	136	1268439	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.09	164	722140	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.85	188	1449801	20.00	ng/ul	0.00
78) Chrysene-d12	21.07	240	1312116	20.00	ng/ul	0.00
86) Perylene-d12	23.20	264	1583288	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.99	96	35860	5.18	ng/uL	0.00
5) Phenol-d5	6.63	99	141793	4.90	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.78	67	349370	20.12	ng/ul	0.00
9) 2-Chlorophenol-d4	6.97	132	368311	17.84	ng/ul	0.00
13) 4-Methylphenol-d8	8.16	113	262855	11.11	ng/ul	0.00
19) Nitrobenzene-d5	8.58	128	207292	22.74	ng/ul	0.00
22) 2-Nitrophenol-d4	9.30	143	232158	23.17	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.84	165	414943	21.30	ng/ul	0.00
29) 4-Chloroaniline-d4	10.35	131	528088	22.32	ng/ul	0.00
44) Dimethylphthalate-d6	13.52	166	1450080	27.15	ng/ul	0.00
47) Acenaphthylene-d8	13.78	160	1581973	24.72	ng/ul	0.00
52) 4-Nitrophenol-d4	14.37	143	41948m	4.38	ng/ul	0.02
58) Fluorene-d10	15.10	176	1170979	25.01	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.26	200	101397	11.46	ng/ul	0.00
71) Anthracene-d10	16.95	188	1865729	28.28	ng/ul	0.00
79) Pyrene-d10	19.26	212	1964285	31.43	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.06	264	2249287	28.60	ng/ul	0.00

Target Compounds

					Ovalue
2) 1,4-Dioxane	3.02	88	53934	7.035	ng/uL 92
6) Phenol	6.66	94	51776	1.732	ng/ul 97
45) Dimethylphthalate	13.56	163	102034	1.839	ng/ul 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122319\
Data File : BM024277.D
Acq On : 25 Dec 2019 05:11
Operator : JU
Sample : K6240-23
Misc :
ALS Vial : 26 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BFQT0

Manual Integrations
APPROVED

mohammad
12/26/2019 4:00:38 PM

Quant Time: Dec 25 06:51:51 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Dec 25 03:33:48 2019
Response via : Initial Calibration

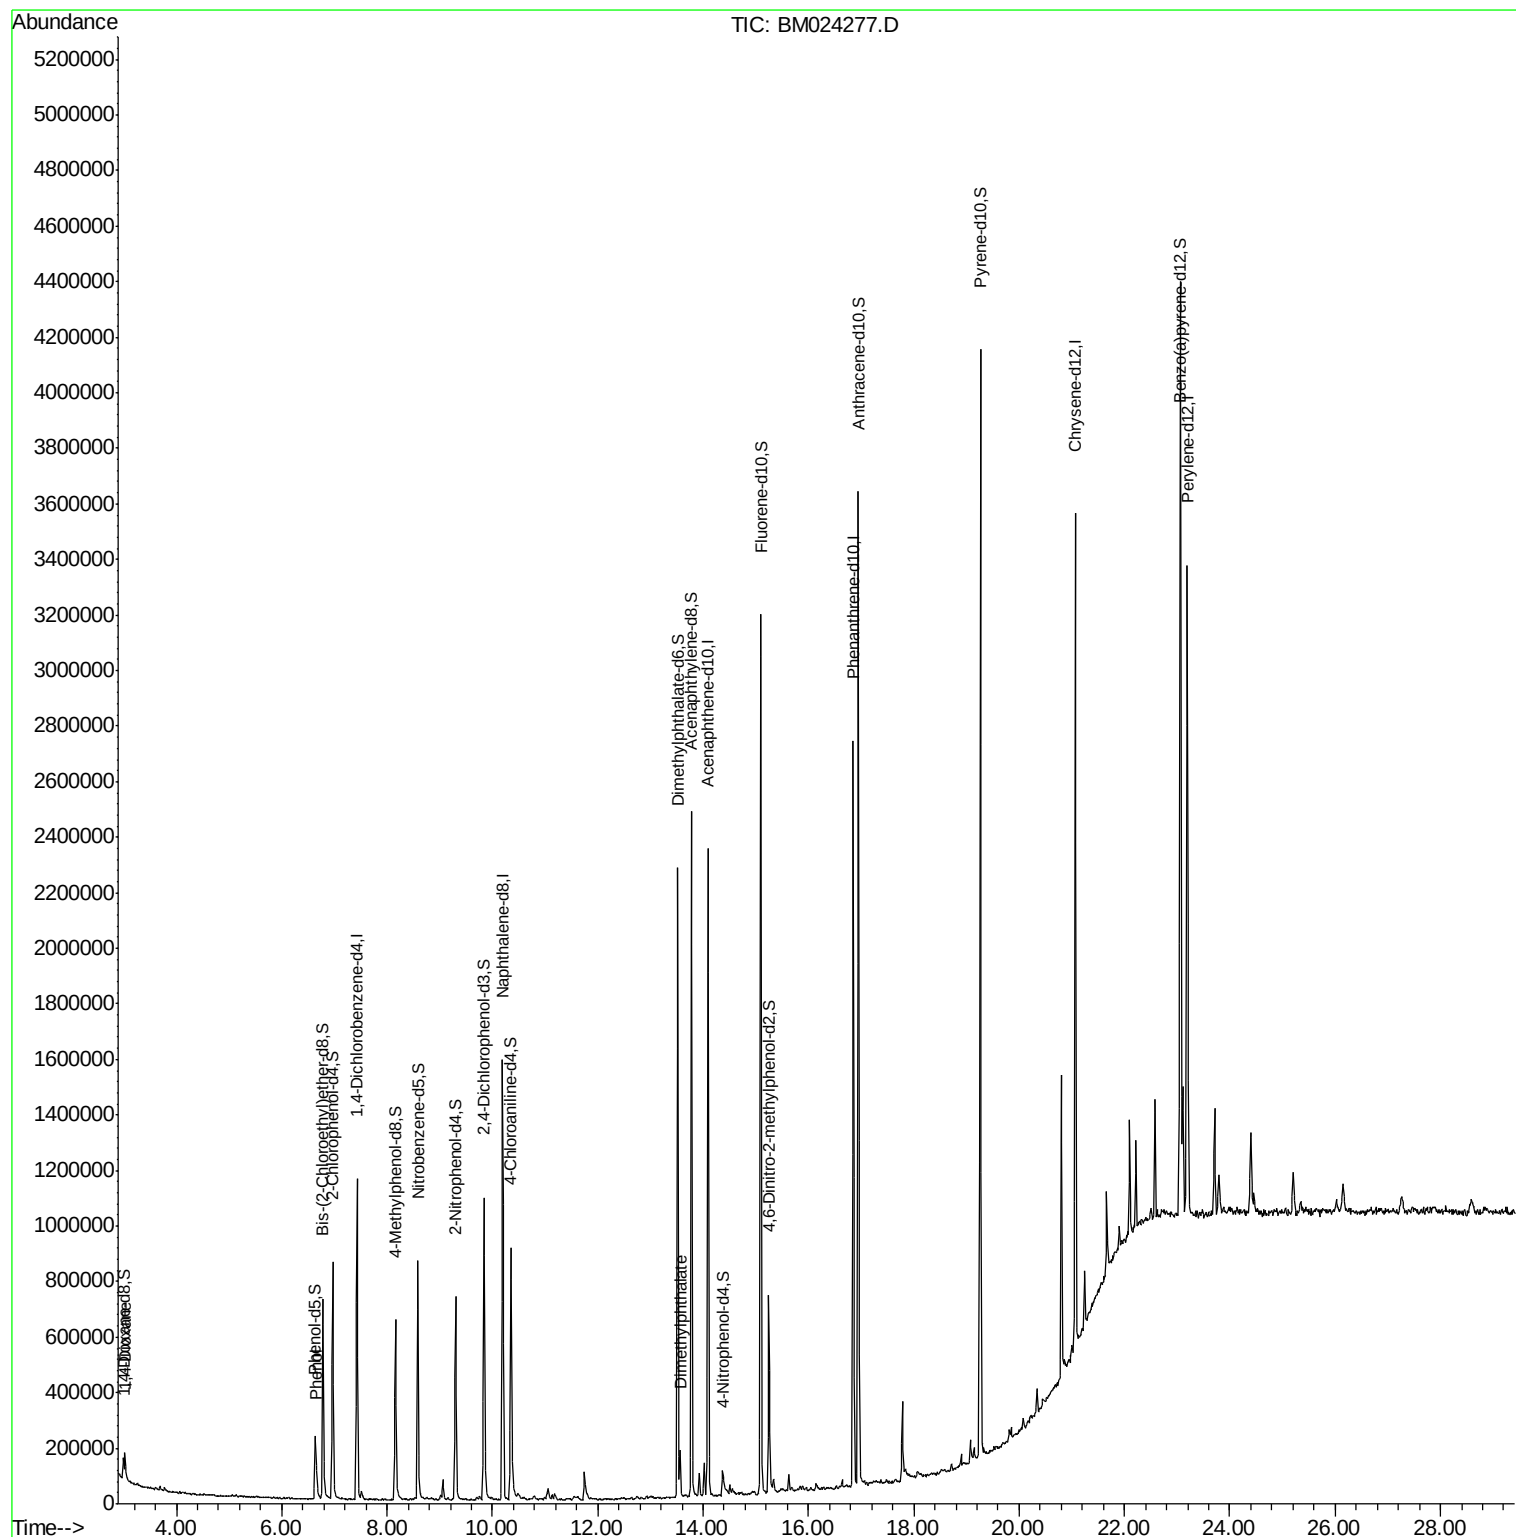

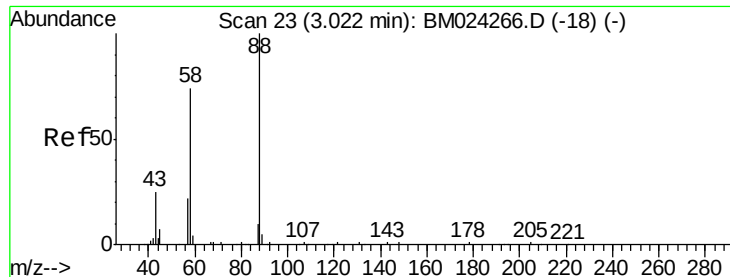

#2

1,4-Dioxane

Concen: 7.035 ng/uL

RT: 3.02 min Scan# 23

Delta R.T. -0.00 min

Lab File: BM024277.D

Acq: 25 Dec 2019 05:11

Instrument :

BNA_M





ClientSampleId :

BFQT0

Tot Ion:	88	Resp:	53934
Ion	Ratio	Lower	Upper
88	100		
43	32.4	25.9	38.9
58	70.4	48.8	73.2

Manual Integrations
APPROVED

mohammad
12/26/2019 4:00:38 PM

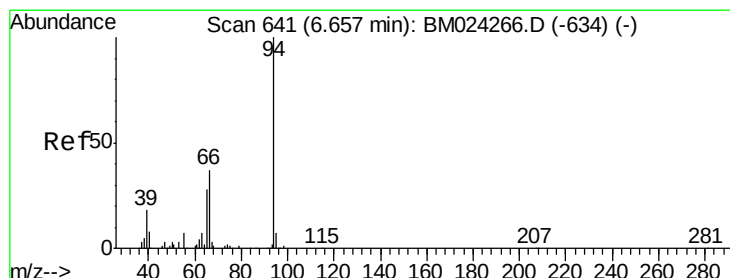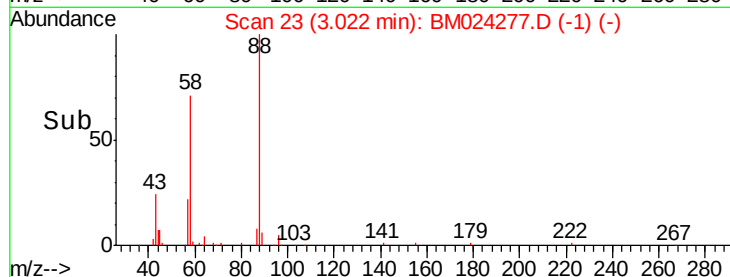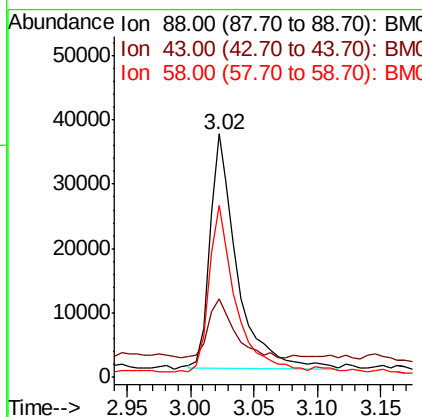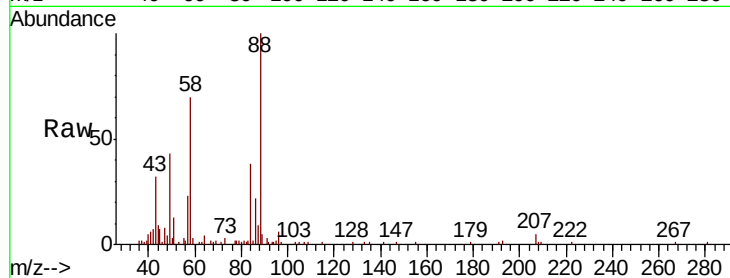

#6

Phenol

Concen: 1.732 ng/uL




RT: 6.66 min Scan# 641


Delta R.T. -0.00 min

Lab File: BM024277.D

Acq: 25 Dec 2019 05:11

Tgt Ion:	94	Resp:	51776
Ion	Ratio	Lower	Upper
94	100		
65	25.9	22.6	33.8
66	36.9	30.7	46.1

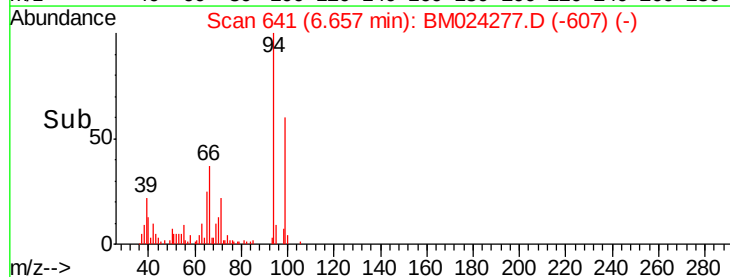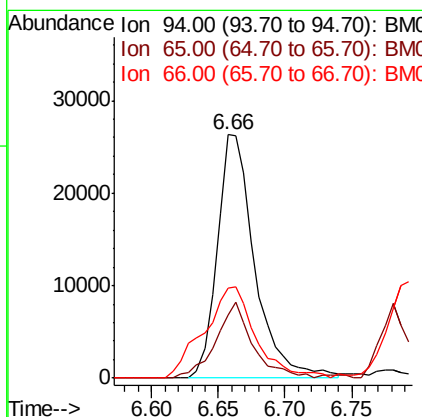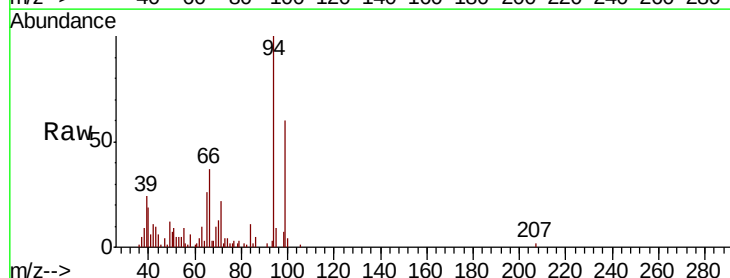

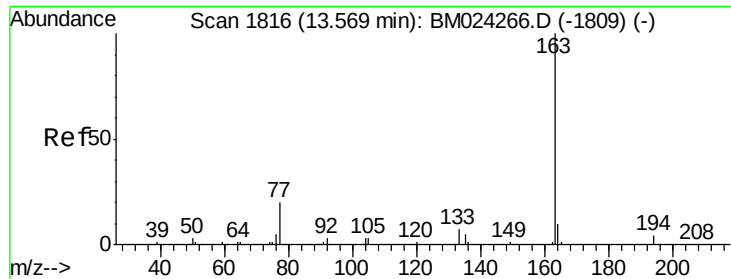

#45
 Dimethylphthalate
 Concen: 1.839 ng/ul
 RT: 13.56 min Scan# 1815
 Delta R.T. -0.01 min
 Lab File: BM024277.D
 Acq: 25 Dec 2019 05:11

Instrument :
 BNA_M
 ClientSampleId :
 BFQT0

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.4	3.2	4.8
164	10.5	7.8	11.6

Manual Integrations
 APPROVED

mohammad
 12/26/2019 4:00:38 PM

