

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122319\
 Data File : BM024234.D
 Acq On : 24 Dec 2019 02:10
 Operator : JU
 Sample : K6236-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFEX2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.999	17	19	28	rVB	29075	47266	1.31%	0.108%
2	3.499	102	104	108	rVB4	10113	10808	0.30%	0.025%
3	3.604	118	122	132	rVB2	27856	54953	1.52%	0.126%
4	3.922	172	176	183	rVB	19121	27778	0.77%	0.064%
5	4.081	200	203	205	rBV3	5580	6386	0.18%	0.015%
6	4.128	208	211	214	rVB4	8274	7469	0.21%	0.017%
7	4.328	241	245	252	rVB5	8809	14797	0.41%	0.034%
8	4.599	287	291	301	rVB	36301	59924	1.66%	0.137%
9	5.557	451	454	457	rBV5	3247	4402	0.12%	0.010%
10	5.757	484	488	490	rBV5	3752	5359	0.15%	0.012%
11	6.593	626	630	631	rBV4	5684	6121	0.17%	0.014%
12	6.628	631	636	651	rVV2	480429	994629	27.54%	2.282%
13	6.787	657	663	678	rBV	425290	735497	20.36%	1.688%
14	6.969	688	694	708	rBV	582934	970243	26.86%	2.226%
15	7.428	766	772	785	rBV	927082	1474940	40.83%	3.384%
16	7.516	785	787	793	rVB5	5165	8943	0.25%	0.021%
17	8.157	890	896	913	rBV	581384	1093269	30.27%	2.508%
18	8.275	913	916	920	rVV3	15407	26947	0.75%	0.062%
19	8.587	962	969	986	rBV	503898	914323	25.31%	2.098%
20	8.763	994	999	1005	rVB7	5138	8716	0.24%	0.020%
21	9.016	1039	1042	1049	rVB2	12164	16367	0.45%	0.038%
22	9.304	1083	1091	1105	rBV	402664	750293	20.77%	1.721%
23	9.839	1174	1182	1205	rBV	577977	1164819	32.25%	2.673%
24	10.198	1236	1243	1254	rBV	1295447	2184765	60.48%	5.013%
25	10.281	1254	1257	1259	rVB4	4880	5838	0.16%	0.013%
26	10.357	1263	1270	1298	rBV	490022	1114345	30.85%	2.557%
27	11.498	1463	1464	1472	rVB5	3192	4798	0.13%	0.011%
28	11.822	1514	1519	1525	rVB7	5456	13992	0.39%	0.032%
29	13.398	1784	1787	1792	rBV5	5315	8621	0.24%	0.020%
30	13.522	1801	1808	1813	rBV	1258268	1821351	50.42%	4.179%
31	13.569	1813	1816	1830	rVB	170296	265289	7.34%	0.609%
32	13.780	1846	1852	1866	rBV	1422024	2106528	58.32%	4.833%
33	14.027	1891	1894	1898	rVB5	3619	4494	0.12%	0.010%
34	14.092	1898	1905	1924	rBV	2016428	3000164	83.06%	6.884%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122319\
 Data File : BM024234.D
 Acq On : 24 Dec 2019 02:10
 Operator : JU
 Sample : K6236-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFEX2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
 Title : SVOA CALIBRATION

35	14.363	1944	1951	1970	rBV	96714	350993	9.72%	0.805%
36	14.563	1982	1985	1991	rVB6	12350	15360	0.43%	0.035%
37	14.880	2034	2039	2042	rBV6	5322	10582	0.29%	0.024%
38	14.974	2054	2055	2060	rBV4	3779	4259	0.12%	0.010%
39	15.098	2069	2076	2086	rBV	1910416	2733429	75.67%	6.272%
40	15.251	2097	2102	2114	rBV	244882	431352	11.94%	0.990%
41	15.339	2114	2117	2122	rVB3	21681	35487	0.98%	0.081%
42	15.851	2200	2204	2207	rBV5	9253	14710	0.41%	0.034%
43	15.886	2207	2210	2214	rVB3	5722	8130	0.23%	0.019%
44	16.080	2240	2243	2246	rBV4	4040	5613	0.16%	0.013%
45	16.415	2297	2300	2304	rVB4	9872	13223	0.37%	0.030%
46	16.639	2335	2338	2343	rBV5	10324	11815	0.33%	0.027%
47	16.851	2368	2374	2384	rBV	2455366	3390561	93.86%	7.779%
48	16.951	2384	2391	2407	rVV	2076103	2931169	81.15%	6.725%
49	17.074	2409	2412	2417	rVB5	17385	27817	0.77%	0.064%
50	17.268	2438	2445	2454	rBV6	23705	52189	1.44%	0.120%
51	17.492	2481	2483	2486	rVB4	3555	4005	0.11%	0.009%
52	17.533	2486	2490	2491	rBV4	3634	4804	0.13%	0.011%
53	17.657	2509	2511	2517	rVB4	7611	11489	0.32%	0.026%
54	17.774	2526	2531	2541	rBV3	76419	137877	3.82%	0.316%
55	17.845	2541	2543	2545	rVB3	5799	4990	0.14%	0.011%
56	17.992	2566	2568	2571	rVB4	4354	5002	0.14%	0.011%
57	18.021	2571	2573	2577	rVB4	4000	5608	0.16%	0.013%
58	18.209	2601	2605	2610	rVB7	18850	26353	0.73%	0.060%
59	18.251	2610	2612	2613	rBV2	4849	3724	0.10%	0.009%
60	18.404	2632	2638	2641	rBV6	12615	22996	0.64%	0.053%
61	18.892	2718	2721	2727	rBV2	17915	27067	0.75%	0.062%
62	19.080	2748	2753	2754	rBV5	18483	24833	0.69%	0.057%
63	19.145	2762	2764	2769	rVB4	16620	18151	0.50%	0.042%
64	19.256	2778	2783	2796	rBV	2372985	3369893	93.29%	7.732%
65	20.803	3043	3046	3054	rBV2	167041	264169	7.31%	0.606%
66	21.062	3085	3090	3100	rBV	2640786	3612182	100.00%	8.288%
67	21.662	3190	3192	3198	rVB2	130942	146818	4.06%	0.337%
68	22.103	3264	3267	3272	rVB	196332	229343	6.35%	0.526%
69	23.062	3424	3430	3435	rBV	1734710	3102894	85.90%	7.119%
70	23.191	3446	3452	3461	rVB	1999208	3590878	99.41%	8.239%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122319\
Data File : BM024234.D
Acq On : 24 Dec 2019 02:10
Operator : JU
Sample : K6236-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFEX2

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Title : SVOA CALIBRATION


Sum of corrected areas: 43584199

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122319\
Data File : BM024234.D
Acq On : 24 Dec 2019 02:10
Operator : JU
Sample : K6236-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFEX2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

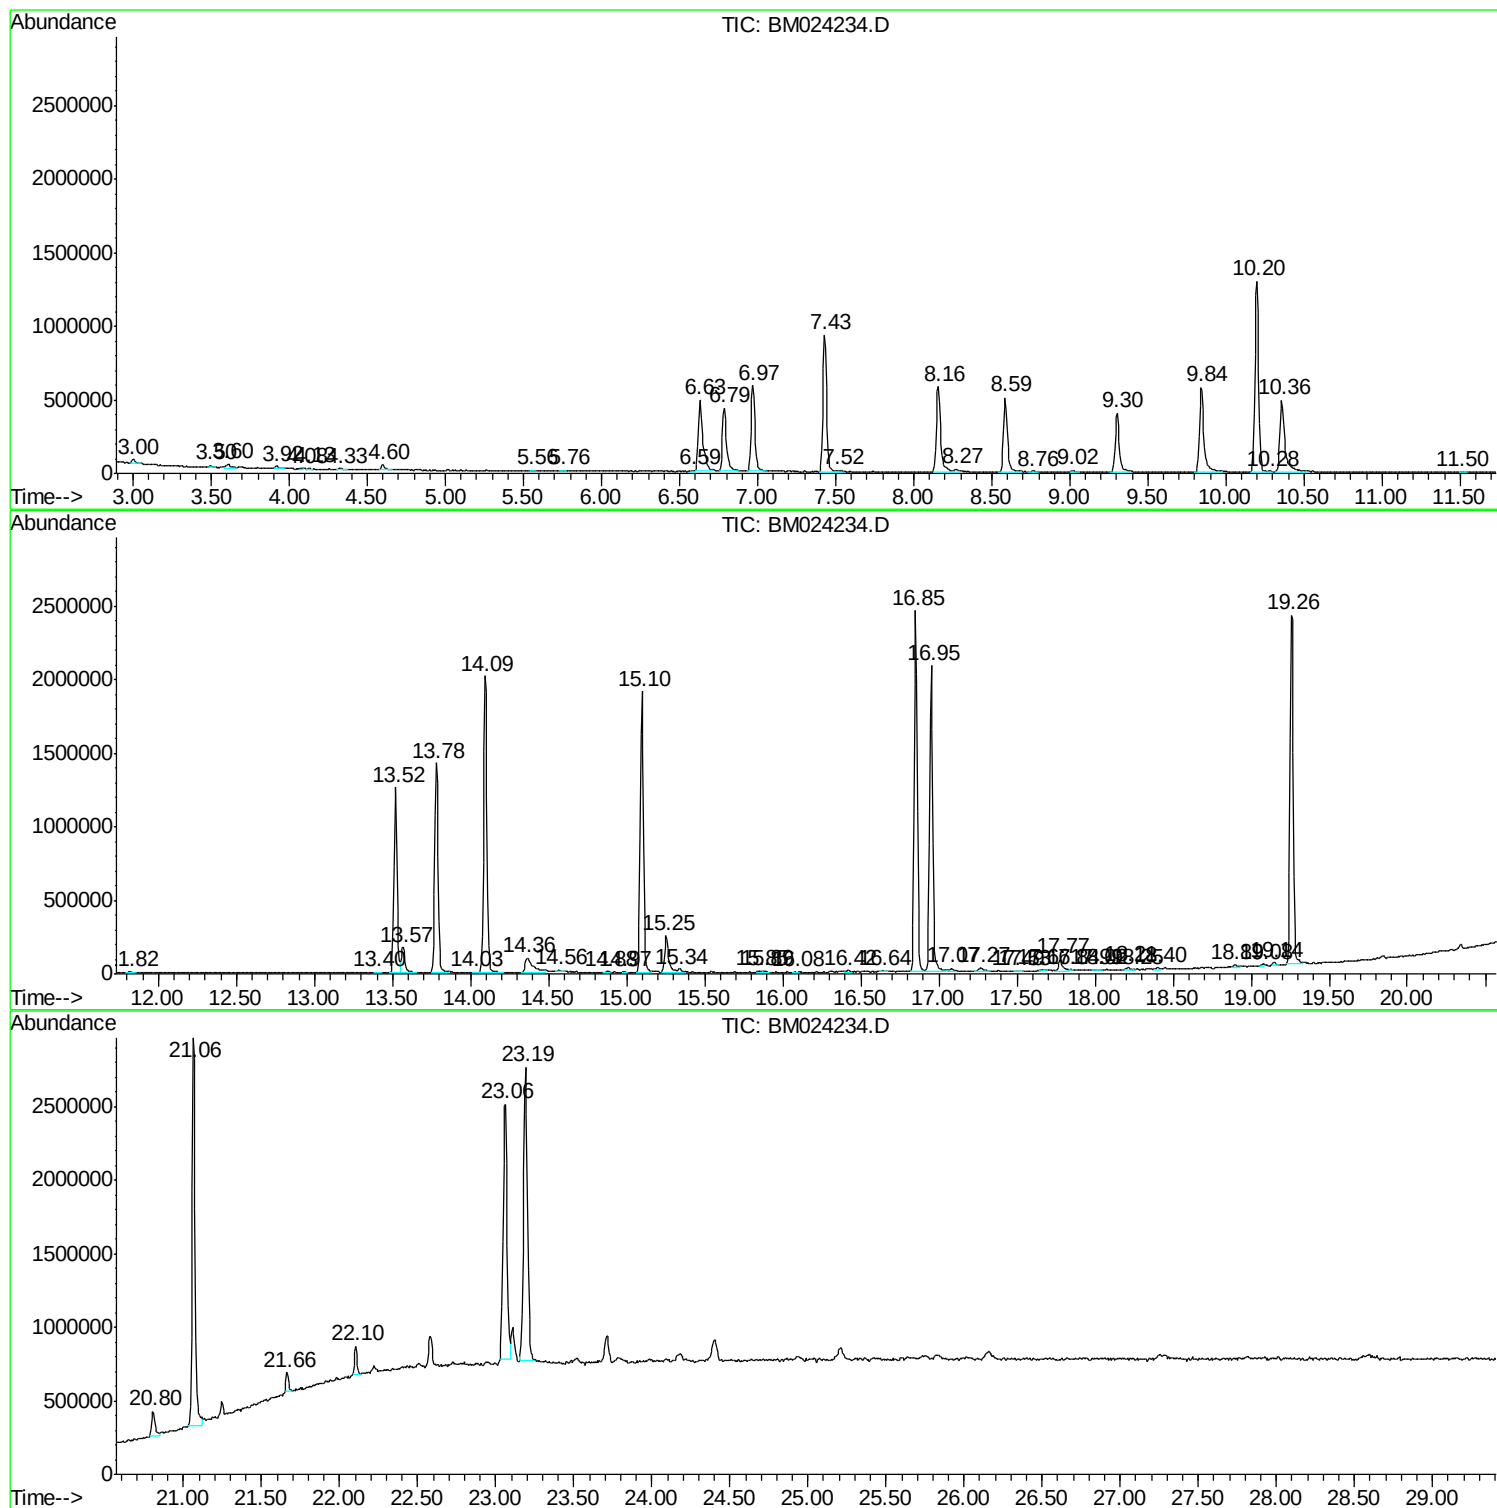

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122319\
Data File : BM024234.D
Acq On : 24 Dec 2019 02:10
Operator : JU
Sample : K6236-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFEX2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122319\
Data File : BM024234.D
Acq On : 24 Dec 2019 02:10
Operator : JU
Sample : K6236-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFEX2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc