
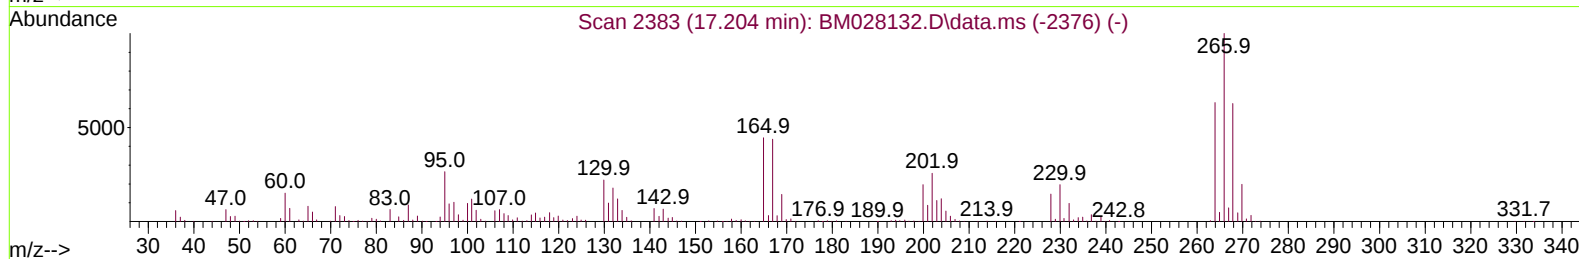
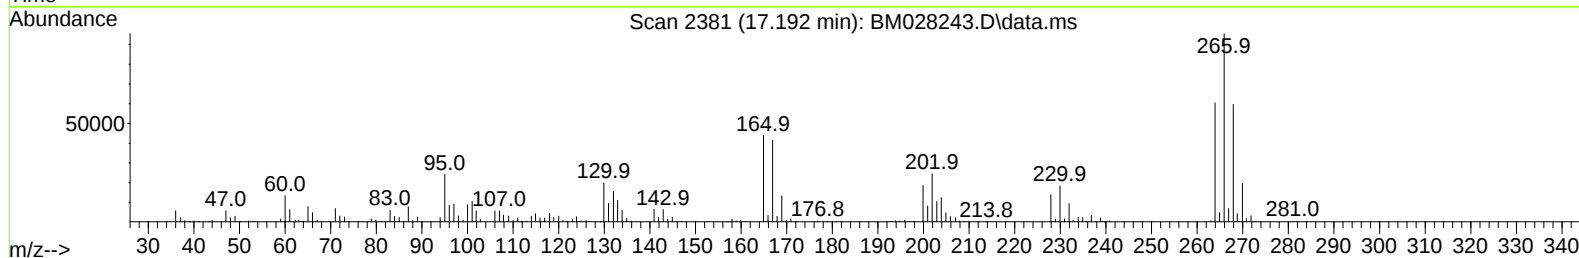


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122320\
Data File : BM028243.D
Acq On : 23 Dec 2020 08:43
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 24 04:18:56 2020
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 23 12:17:02 2020
Response via : Initial Calibration

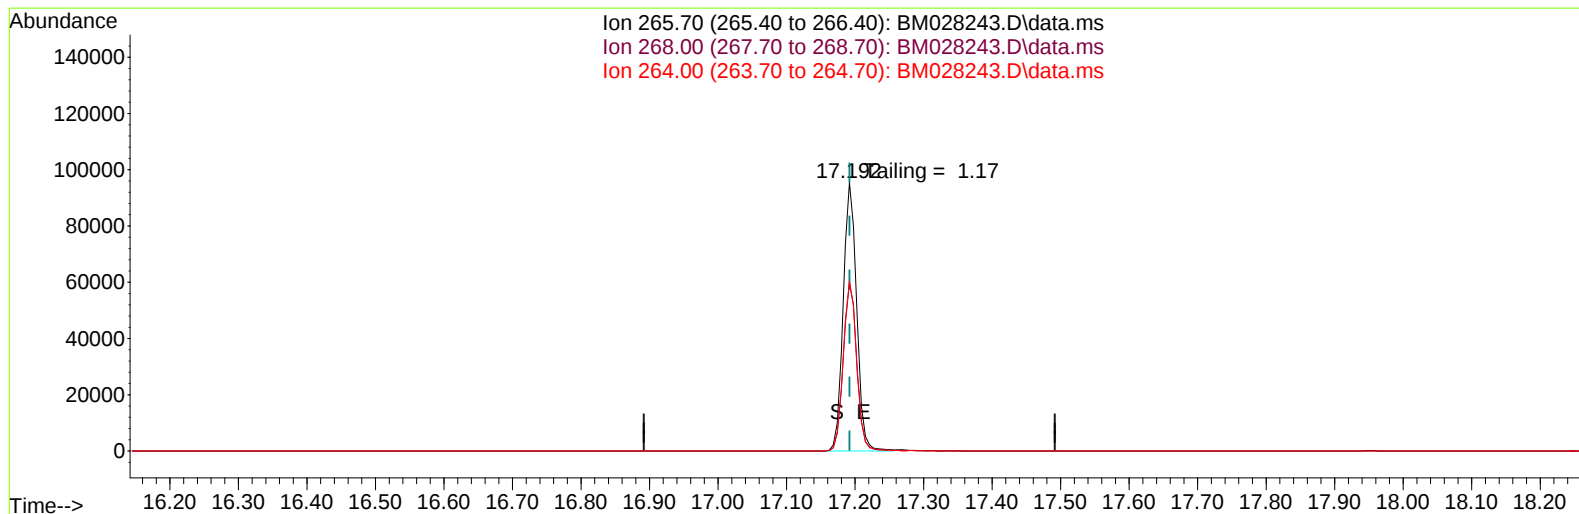

TIC: BM028243.D\data.ms

(70) Pentachlorophenol (C)




17.192min (-0.000) 94053.70 ng

response 130260

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	62.51
264.00	63.30	63.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122320\
 Data File : BM028243.D
 Acq On : 23 Dec 2020 08:43
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 24 04:18:56 2020
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 23 12:17:02 2020
 Response via : Initial Calibration

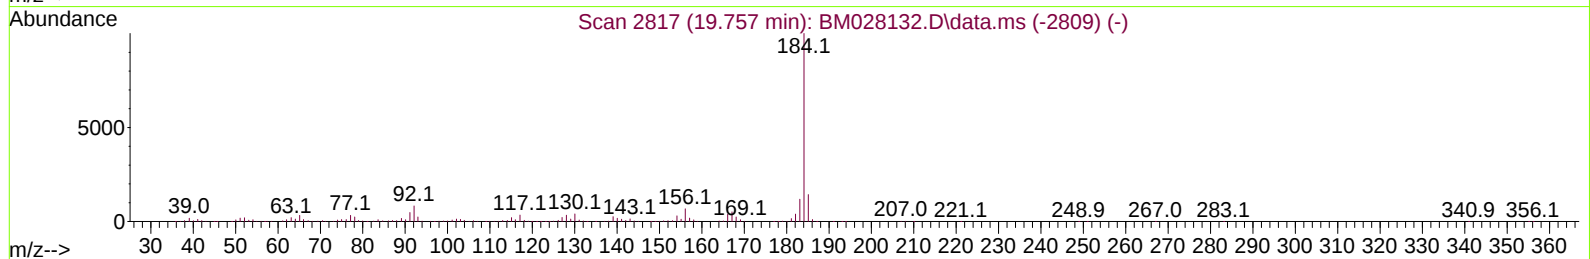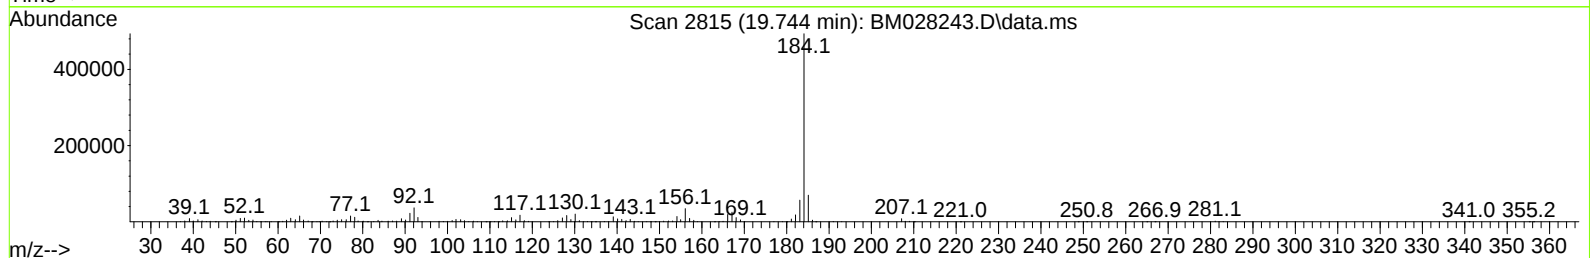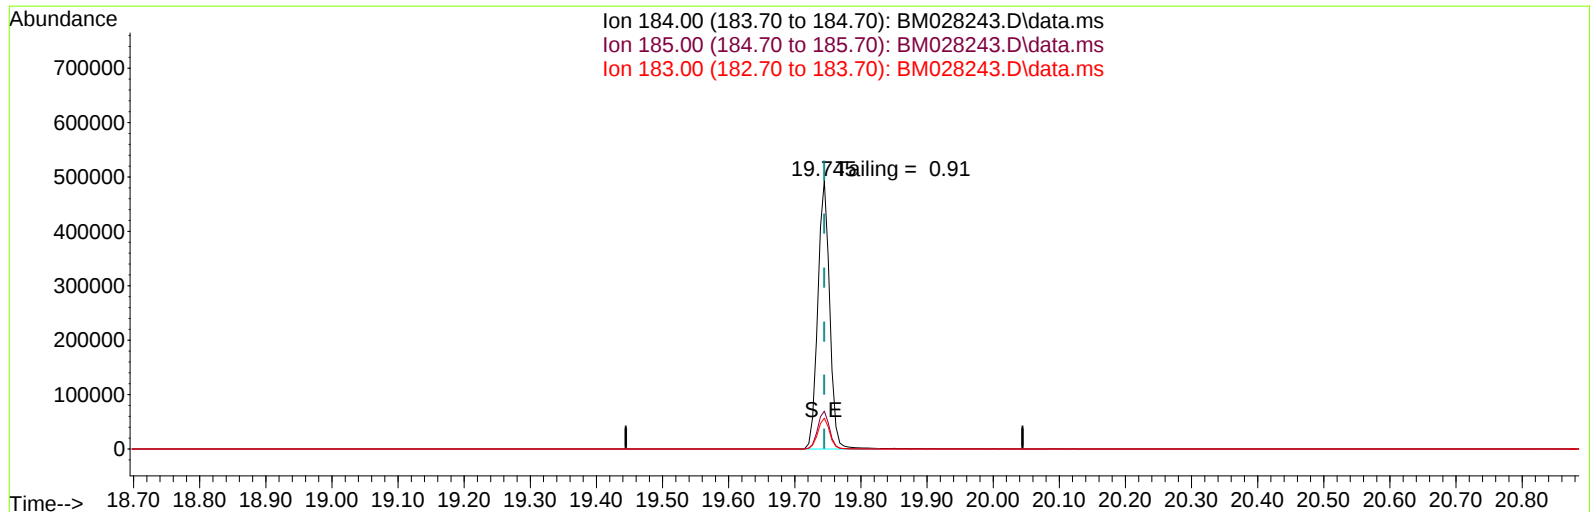

TIC: BM028243.D\data.ms

(77) Benzidine

19.744min (-0.000) 3651.43 ng

response 619420

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.15
183.00	12.10	11.54
0.00	0.00	0.00