

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122320\
 Data File : BM028255.D
 Acq On : 23 Dec 2020 17:18
 Operator : JU/CG
 Sample : L5192-01 2X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CL-02-122220

Manual Integrations
 APPROVED

mohammad
 12/24/2020 10:43:41 AM

Quant Time: Dec 24 01:54:54 2020
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 23 12:17:02 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.198	152	148692	20.00	ng	0.00
21) Naphthalene-d8	11.028	136	559912	20.00	ng	# 0.00
39) Acenaphthene-d10	14.827	164	284837	20.00	ng	0.00
64) Phenanthrene-d10	17.545	188	516421	20.00	ng	# 0.00
76) Chrysene-d12	21.662	240	458074	20.00	ng	# 0.00
86) Perylene-d12	24.027	264	477500	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.693	112	416929	46.21	ng	0.00
7) Phenol-d6	7.340	99	529483	41.09	ng	0.00
23) Nitrobenzene-d5	9.375	82	318486	28.23	ng	0.00
42) 2,4,6-Tribromophenol	16.298	330	150432	39.79	ng	0.00
45) 2-Fluorobiphenyl	13.451	172	641705	29.29	ng	0.00
79) Terphenyl-d14	20.121	244	629081	24.92	ng	0.00
Target Compounds						Qvalue
10) Phenol	7.363	94	59121	4.83	ng	86
71) Phenanthrene	17.586	178	190615	6.08	ng	99
75) Fluoranthene	19.574	202	318987	9.08	ng	97
78) Pyrene	19.933	202	284504	8.58	ng	99
81) Benzo(a)anthracene	21.645	228	165821	5.31	ng	98
83) Chrysene	21.698	228	148371	4.91	ng	97
87) Indeno(1,2,3-cd)pyrene	26.450	276	115050m	3.62	ng	
88) Benzo(b)fluoranthene	23.309	252	225741	6.94	ng	# 91
89) Benzo(k)fluoranthene	23.350	252	63895m	2.02	ng	
90) Benzo(a)pyrene	23.921	252	160580	5.50	ng	# 90
92) Benzo(g,h,i)perylene	27.203	276	112945	4.46	ng	# 87

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122320\
Data File : BM028255.D
Acq On : 23 Dec 2020 17:18
Operator : JU/CG
Sample : L5192-01 2X
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
CL-02-122220

Manual Integrations
APPROVED


mohammad
12/24/2020 10:43:41 AM

Quant Time: Dec 24 01:54:54 2020
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 23 12:17:02 2020
Response via : Initial Calibration



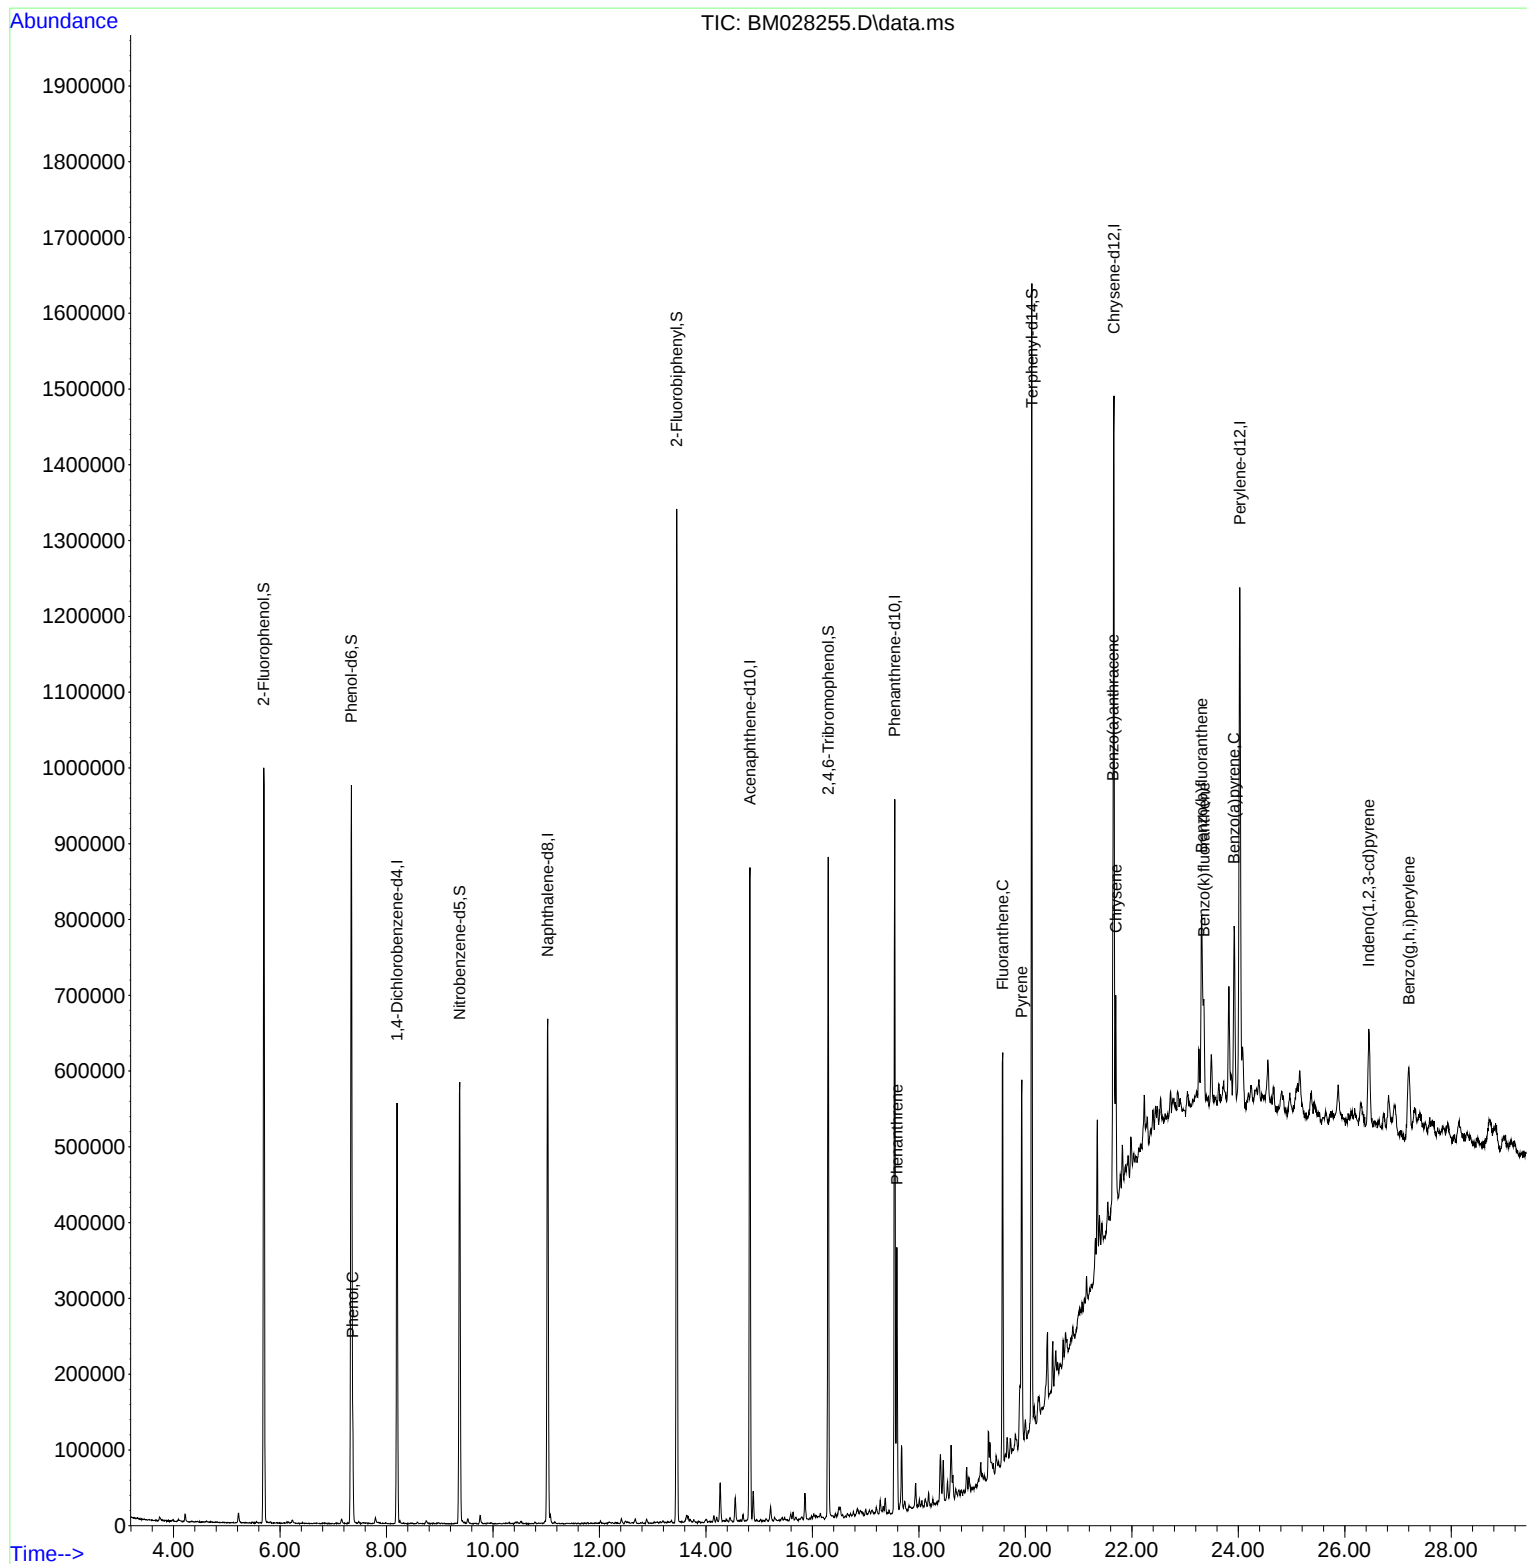





#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.198 min Scan# 852
Delta R.T. 0.000 min
Lab File: BM028255.D
Acq: 23 Dec 2020 17:18





Tgt Ion:152 Resp: 148692
Ion Ratio Lower Upper
152 100
150 156.9 120.6 181.0
115 57.3 47.2 70.8

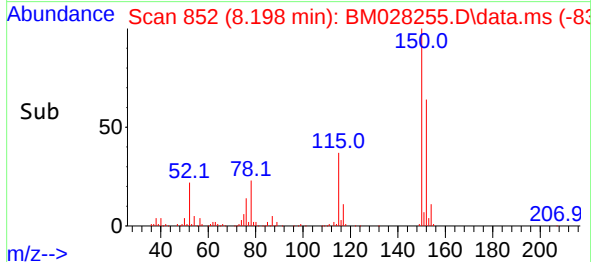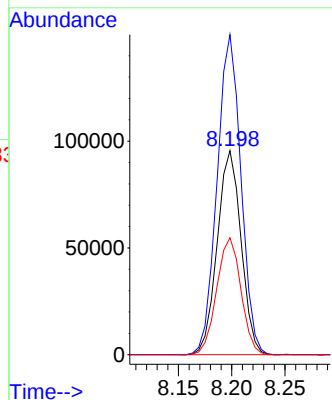

#5
2-Fluorophenol
Concen: 46.21 ng
RT: 5.693 min Scan# 426
Delta R.T. 0.000 min
Lab File: BM028255.D
Acq: 23 Dec 2020 17:18




Tgt Ion:112 Resp: 416929
Ion Ratio Lower Upper
112 100
64 61.4 50.6 76.0
63 32.2 31.0 46.6

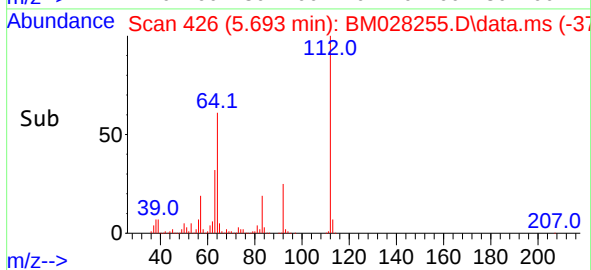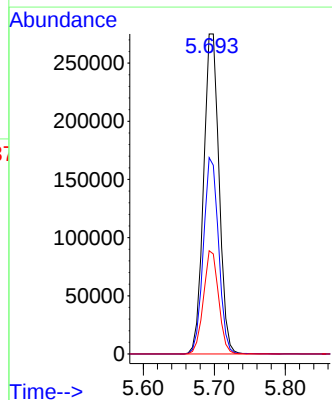

Instrument :
BNA_M
ClientSampleId :
CL-02-122220

Manual Integrations
APPROVED

mohammad
12/24/2020 10:43:41 AM







#7
Phenol-d6
Concen: 41.09 ng
RT: 7.340 min Scan# 706
Delta R.T. 0.000 min
Lab File: BM028255.D
Acq: 23 Dec 2020 17:18

Tgt Ion: 99 Resp: 529483
Ion Ratio Lower Upper
99 100
42 20.0 13.5 20.3
71 32.5 39.4 59.0#

Instrument :
BNA_M
ClientSampleId :
CL-02-122220




Manual Integrations
APPROVED


mohammad
12/24/2020 10:43:41 AM

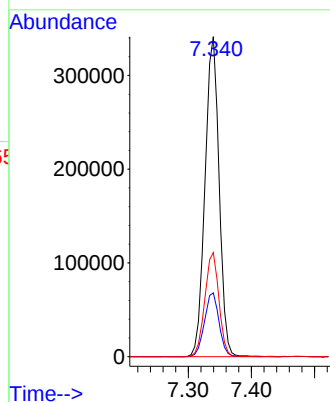

#10
Phenol
Concen: 4.83 ng
RT: 7.363 min Scan# 710
Delta R.T. -0.006 min
Lab File: BM028255.D
Acq: 23 Dec 2020 17:18


Tgt Ion: 94 Resp: 59121
Ion Ratio Lower Upper
94 100
65 29.9 16.4 56.4
66 39.0 30.2 70.2

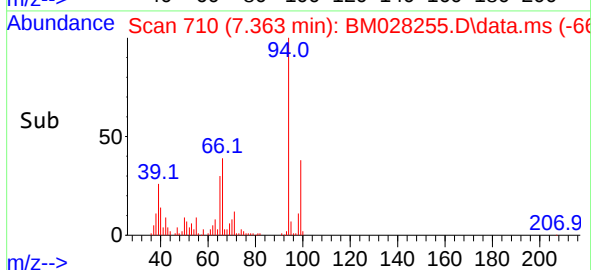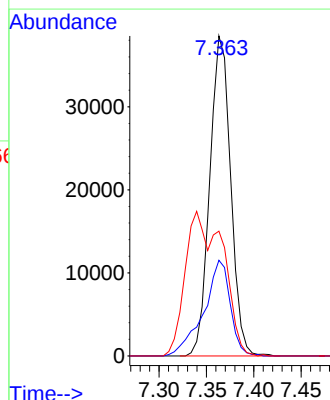



#21
Naphthalene-d8
Concen: 20.00 ng
RT: 11.028 min Scan# 1333
Delta R.T. 0.000 min
Lab File: BM028255.D
Acq: 23 Dec 2020 17:18




Instrument :
BNA_M
ClientSampleId :
CL-02-122220




Tgt Ion:	136	Resp:	559912
Ion Ratio	Lower	Upper	
136	100		
137	10.7	8.6	12.8
54	9.1	4.6	7.0#
68	6.1	4.1	6.1

Manual Integrations
APPROVED



mohammad
12/24/2020 10:43:41 AM

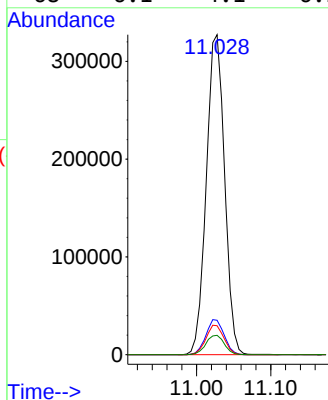


#23
Nitrobenzene-d5
Concen: 28.23 ng
RT: 9.375 min Scan# 1052
Delta R.T. 0.000 min
Lab File: BM028255.D
Acq: 23 Dec 2020 17:18




Tgt Ion:	82	Resp:	318486
Ion Ratio	Lower	Upper	
82	100		
128	46.0	27.4	41.0#
54	54.4	31.4	47.0#

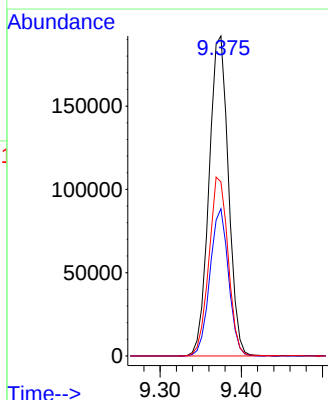



#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.827 min Scan# 1979
Delta R.T. 0.000 min
Lab File: BM028255.D
Acq: 23 Dec 2020 17:18




Instrument :
BNA_M
ClientSampleId :
CL-02-122220



Tgt Ion:164 Resp: 284837
Ion Ratio Lower Upper
164 100
162 101.0 80.4 120.6
160 44.7 35.9 53.9




Manual Integrations
APPROVED


mohammad
12/24/2020 10:43:41 AM

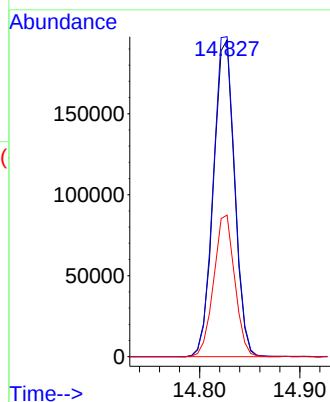

#42
2,4,6-Tribromophenol
Concen: 39.79 ng
RT: 16.298 min Scan# 2229
Delta R.T. -0.006 min
Lab File: BM028255.D
Acq: 23 Dec 2020 17:18


Tgt Ion:330 Resp: 150432
Ion Ratio Lower Upper
330 100
332 96.6 77.8 116.8
141 34.3 28.4 42.6

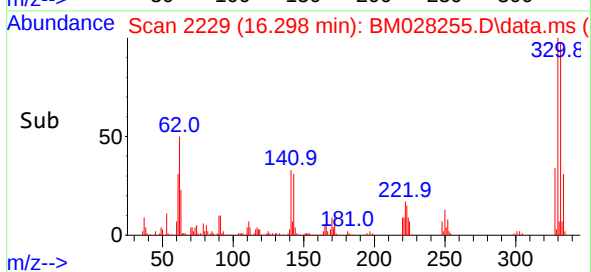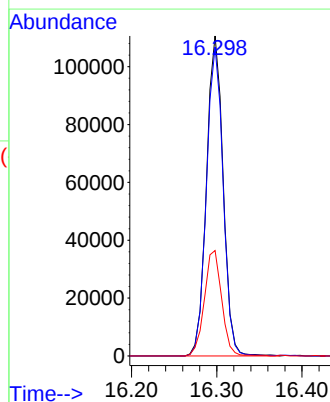



#45
2-Fluorobiphenyl
Concen: 29.29 ng
RT: 13.451 min Scan# 1745
Delta R.T. -0.006 min
Lab File: BM028255.D
Acq: 23 Dec 2020 17:18




Instrument :
BNA_M
ClientSampleId :
CL-02-122220




Tgt Ion:172 Resp: 641705
Ion Ratio Lower Upper
172 100
171 35.2 27.8 41.8
170 22.8 18.6 27.8

Manual Integrations
APPROVED



mohammad
12/24/2020 10:43:41 AM

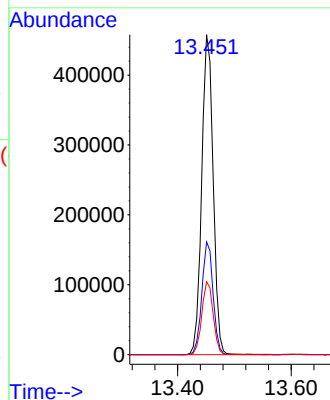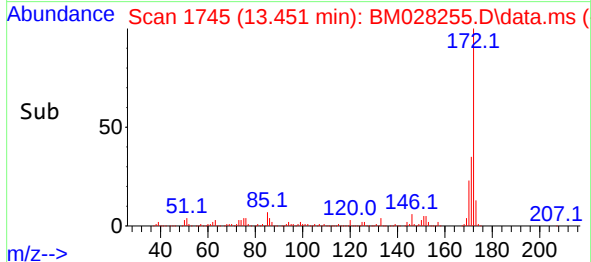


#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.545 min Scan# 2441
Delta R.T. 0.000 min
Lab File: BM028255.D
Acq: 23 Dec 2020 17:18



Tgt Ion:188 Resp: 516421
Ion Ratio Lower Upper
188 100
94 10.2 6.2 9.4#
80 11.1 7.5 11.3

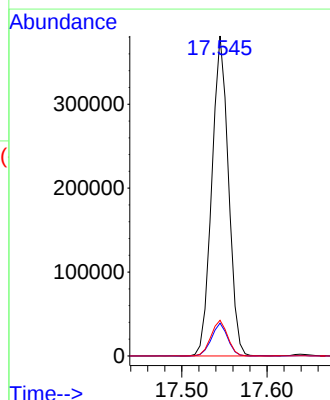







#71
Phenanthrene
Concen: 6.08 ng
RT: 17.586 min Scan# 2448
Delta R.T. -0.006 min
Lab File: BM028255.D
Acq: 23 Dec 2020 17:18

Tgt Ion:178 Resp: 190615
Ion Ratio Lower Upper
178 100
176 18.6 15.0 22.6
179 15.6 12.2 18.4

Instrument :
BNA_M
ClientSampled :
CL-02-122220




Manual Integrations
APPROVED


mohammad
12/24/2020 10:43:41 AM

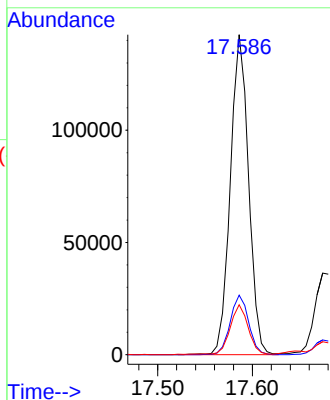

#75
Fluoranthene
Concen: 9.08 ng
RT: 19.574 min Scan# 2786
Delta R.T. 0.000 min
Lab File: BM028255.D
Acq: 23 Dec 2020 17:18


Tgt Ion:202 Resp: 318987
Ion Ratio Lower Upper
202 100
101 11.9 0.0 28.5
203 17.4 0.0 37.3

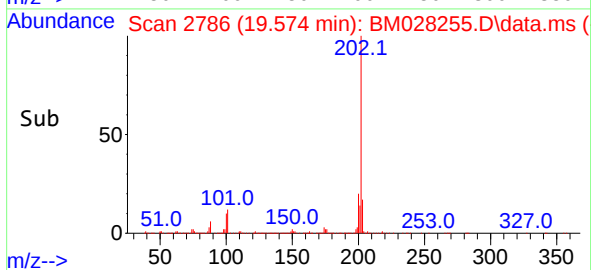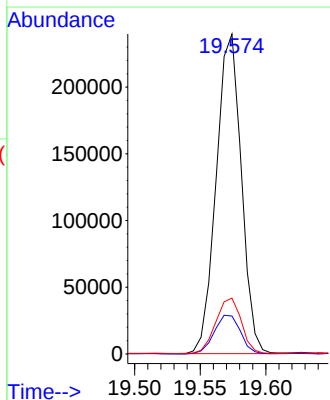



#76
Chrysene-d12
Concen: 20.00 ng
RT: 21.662 min Scan# 3141
Delta R.T. 0.000 min
Lab File: BM028255.D
Acq: 23 Dec 2020 17:18




Instrument :
BNA_M
ClientSampleId :
CL-02-122220



Tgt Ion:240 Resp: 458074
Ion Ratio Lower Upper
240 100
120 12.4 6.4 9.6#
236 24.0 20.1 30.1




Manual Integrations
APPROVED


mohammad
12/24/2020 10:43:41 AM

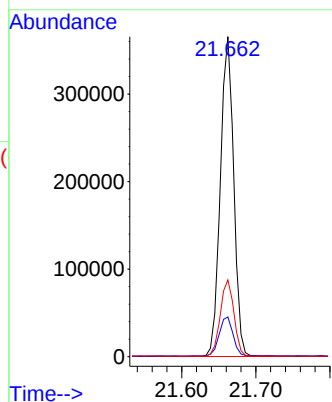

#78
Pyrene
Concen: 8.58 ng
RT: 19.933 min Scan# 2847
Delta R.T. 0.000 min
Lab File: BM028255.D
Acq: 23 Dec 2020 17:18

Tgt Ion:202 Resp: 284504
Ion Ratio Lower Upper
202 100
200 19.9 16.6 24.8
203 17.7 13.8 20.6

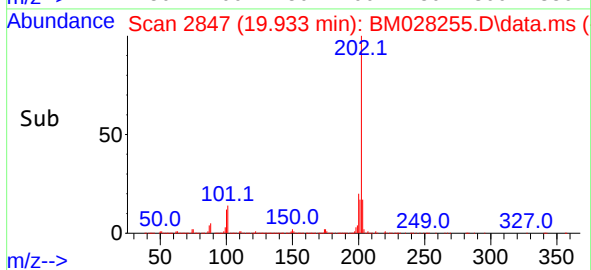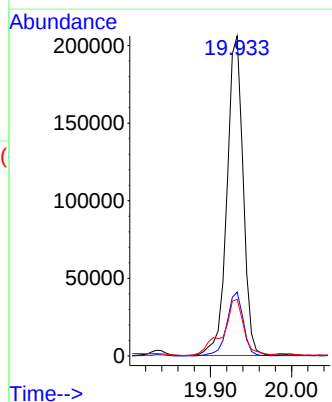







#79
 Terphenyl-d14
 Concen: 24.92 ng
 RT: 20.121 min Scan# 2879
 Delta R.T. 0.000 min
 Lab File: BM028255.D
 Acq: 23 Dec 2020 17:18

Tgt Ion:244 Resp: 629081
 Ion Ratio Lower Upper
 244 100
 212 6.6 5.8 8.8
 122 10.9 6.5 9.7#

Instrument :
 BNA_M
 ClientSampled :
 CL-02-122220




Manual Integrations
 APPROVED


mohammad
 12/24/2020 10:43:41 AM

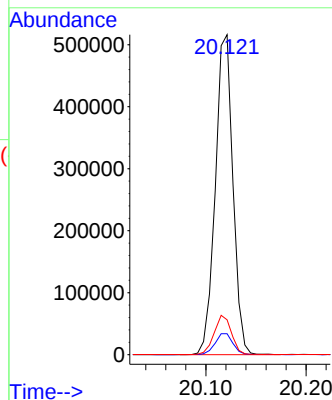

#81
 Benzo(a)anthracene
 Concen: 5.31 ng
 RT: 21.645 min Scan# 3138
 Delta R.T. 0.000 min
 Lab File: BM028255.D
 Acq: 23 Dec 2020 17:18

Tgt Ion:228 Resp: 165821
 Ion Ratio Lower Upper
 228 100
 226 27.3 21.1 31.7
 229 20.7 15.7 23.5

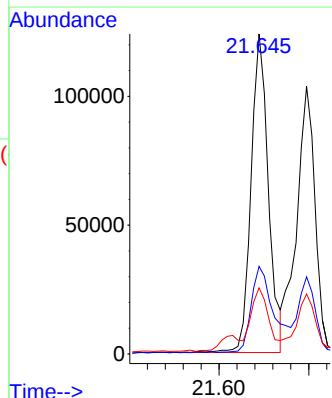







#83
Chrysene
Concen: 4.91 ng
RT: 21.698 min Scan# 3147
Delta R.T. 0.000 min
Lab File: BM028255.D
Acq: 23 Dec 2020 17:18

Tgt Ion:	228	Resp:	148371
Ion	Ratio	Lower	Upper
228	100		
226	28.8	23.4	35.0
229	22.4	15.7	23.5

Instrument :
BNA_M
ClientSampled :
CL-02-122220




Manual Integrations
APPROVED


mohammad
12/24/2020 10:43:41 AM

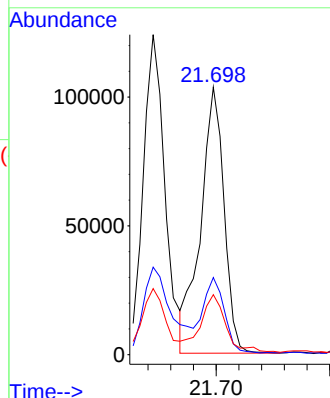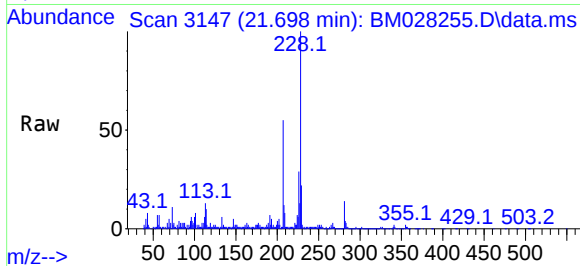


#86
Perylene-d12
Concen: 20.00 ng
RT: 24.027 min Scan# 3543
Delta R.T. 0.006 min
Lab File: BM028255.D
Acq: 23 Dec 2020 17:18

Tgt Ion:	264	Resp:	477500
Ion	Ratio	Lower	Upper
264	100		
260	23.0	19.0	28.4
265	22.0	17.7	26.5


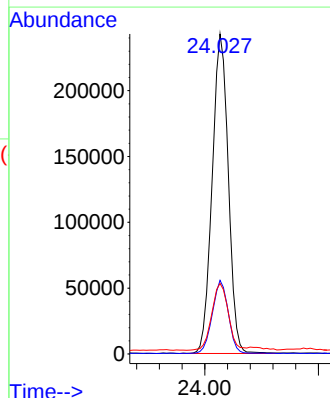
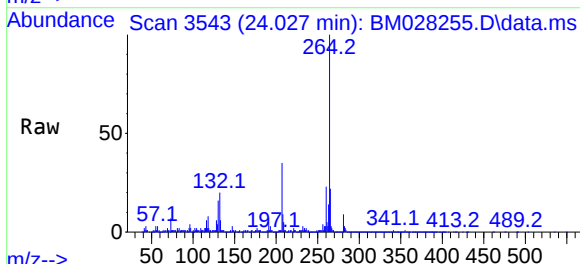





#87
Indeno(1,2,3-cd)pyrene
Concen: 3.62 ng m
RT: 26.450 min Scan# 3955
Delta R.T. -0.006 min
Lab File: BM028255.D
Acq: 23 Dec 2020 17:18





Tgt Ion: 276 Resp: 115050
Ion Ratio Lower Upper
276 100
138 1.8 14.2 21.4#
277 2.2 19.8 29.8#

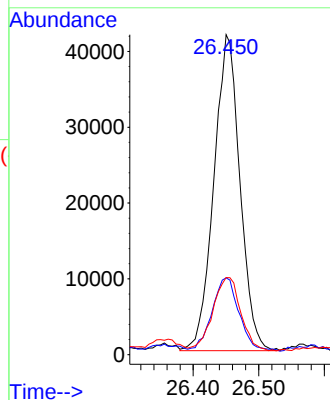

#88
Benzo(b)fluoranthene
Concen: 6.94 ng
RT: 23.309 min Scan# 3421
Delta R.T. 0.000 min
Lab File: BM028255.D
Acq: 23 Dec 2020 17:18




Tgt Ion: 252 Resp: 225741
Ion Ratio Lower Upper
252 100
253 24.2 17.4 26.0
125 14.0 5.7 8.5#

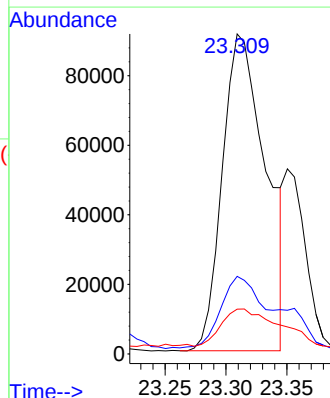

Instrument :
BNA_M
ClientSampleId :
CL-02-122220


Manual Integrations
APPROVED

mohammad
12/24/2020 10:43:41 AM



#89
Benzo(k)fluoranthene
Concen: 2.02 ng m
RT: 23.350 min Scan# 3428
Delta R.T. -0.006 min
Lab File: BM028255.D
Acq: 23 Dec 2020 17:18




Instrument :
BNA_M
ClientSampleId :
CL-02-122220




Tgt Ion:252 Resp: 63895
Ion Ratio Lower Upper
252 100
253 23.6 17.4 26.0
125 14.6 5.6 8.4#

Manual Integrations
APPROVED



mohammad
12/24/2020 10:43:41 AM

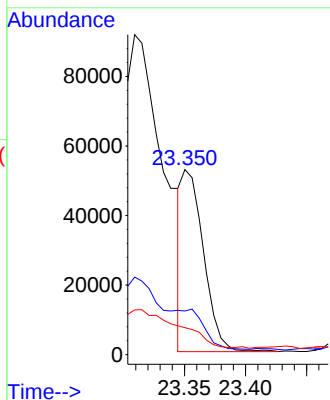


#90
Benzo(a)pyrene
Concen: 5.50 ng
RT: 23.921 min Scan# 3525
Delta R.T. 0.000 min
Lab File: BM028255.D
Acq: 23 Dec 2020 17:18




Tgt Ion:252 Resp: 160580
Ion Ratio Lower Upper
252 100
253 24.7 17.4 26.2
125 16.0 6.6 9.8#

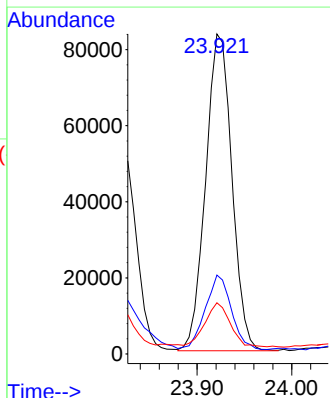



#92
Benzo(g,h,i)perylene
Concen: 4.46 ng
RT: 27.203 min Scan# 4083
Delta R.T. 0.000 min
Lab File: BM028255.D
Acq: 23 Dec 2020 17:18

Instrument :
BNA_M
ClientSampleId :
CL-02-122220



Tgt Ion: 276 Resp: 112945
Ion Ratio Lower Upper
276 100
277 24.9 18.6 28.0
138 27.1 12.2 18.2#

Manual Integrations
APPROVED

mohammad
12/24/2020 10:43:41 AM

