

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122320\
 Data File : BM028245.D
 Acq On : 23 Dec 2020 10:35
 Operator : JU/CG
 Sample : PB133742BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB133742BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM028245.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.693	419	426	438	rBV	2590188	3825673	66.74%	12.260%
2	7.340	697	706	720	rBV	2433295	3909886	68.21%	12.529%
3	8.193	844	851	859	rBV	488068	768113	13.40%	2.461%
4	9.375	1042	1052	1061	rBV	1523524	2516400	43.90%	8.064%
5	11.022	1325	1332	1340	rBV	629756	1041366	18.17%	3.337%
6	13.451	1738	1745	1753	rBV	3560053	5155718	89.94%	16.522%
7	14.822	1971	1978	1986	rBV	874838	1243346	21.69%	3.984%
8	16.298	2222	2229	2245	rBV	2472099	3476996	60.66%	11.142%
9	17.545	2434	2441	2450	rBV	928803	1275390	22.25%	4.087%
10	20.121	2873	2879	2884	rBV	4591275	5732222	100.00%	18.369%
11	21.656	3135	3140	3146	rBV	902580	1145415	19.98%	3.671%
12	24.015	3535	3541	3550	rVB2	563213	1115223	19.46%	3.574%




Sum of corrected areas: 31205748

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122320\
Data File : BM028245.D
Acq On : 23 Dec 2020 10:35
Operator : JU/CG
Sample : PB133742BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB133742BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

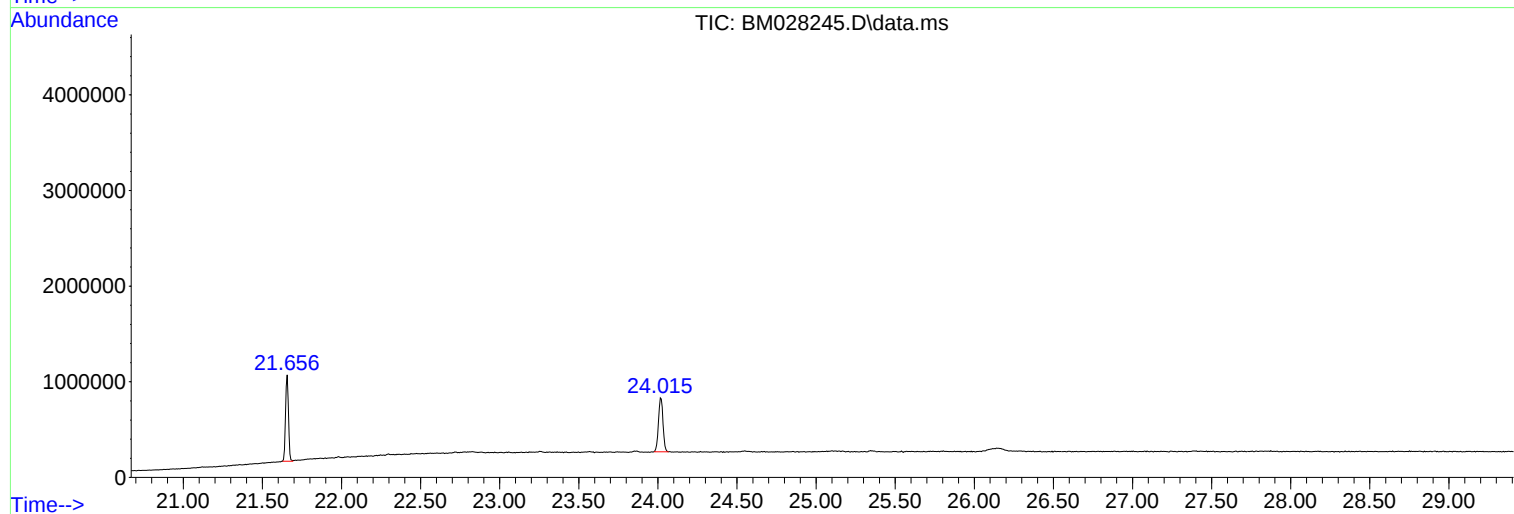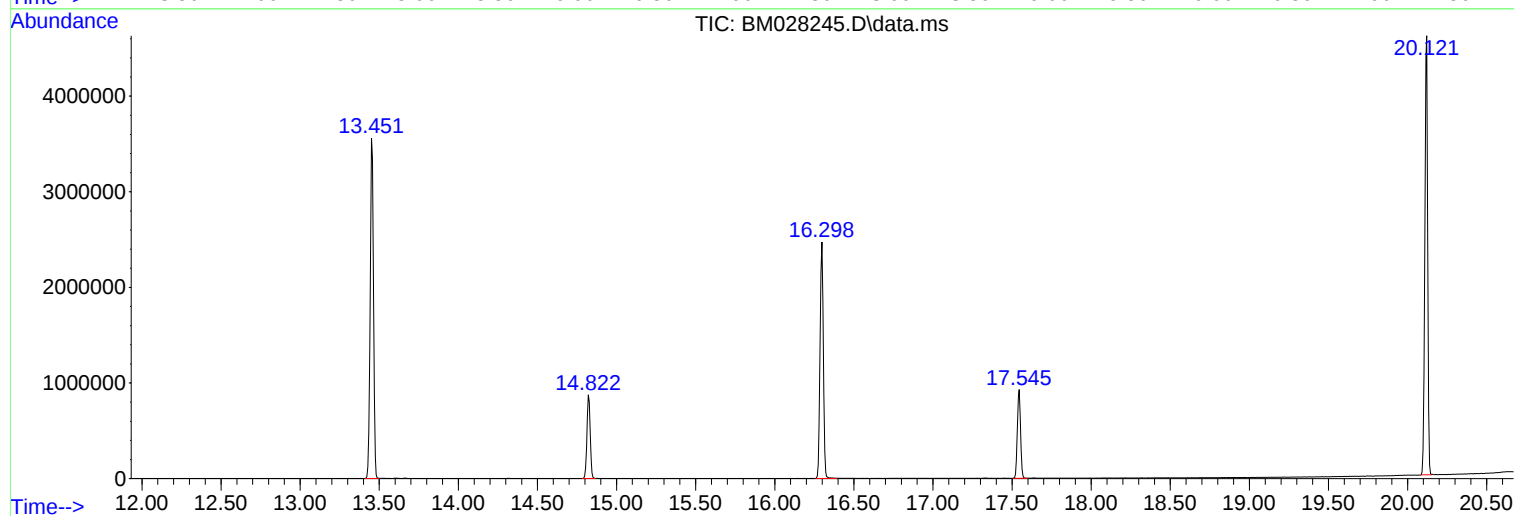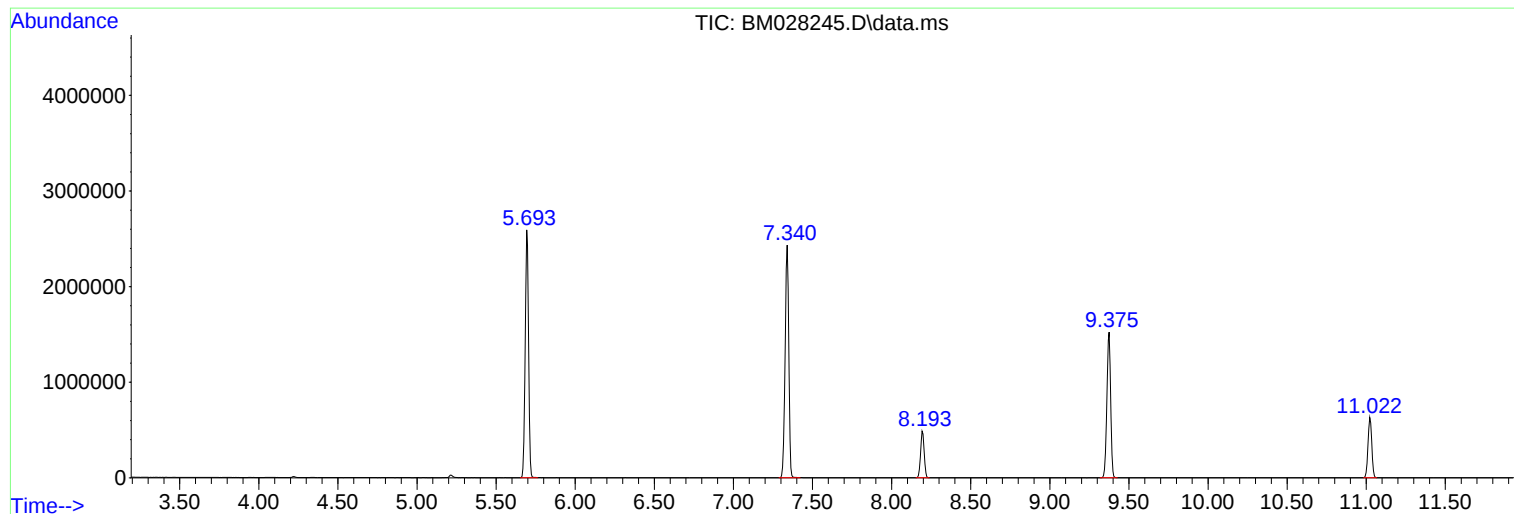

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122320\
Data File : BM028245.D
Acq On : 23 Dec 2020 10:35
Operator : JU/CG
Sample : PB133742BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB133742BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122320\
Data File : BM028245.D
Acq On : 23 Dec 2020 10:35
Operator : JU/CG
Sample : PB133742BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB133742BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------