

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122320\
 Data File : BM028254.D
 Acq On : 23 Dec 2020 16:42
 Operator : JU/CG
 Sample : L5189-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 09

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM028254.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.216	340	345	354	rVB	70818	103370	2.46%	0.380%
2	5.699	420	427	435	rBV	2095215	3030641	72.11%	11.153%
3	7.340	698	706	720	rBV	1948271	3309105	78.73%	12.177%
4	7.787	777	782	791	rBV	27227	49129	1.17%	0.181%
5	8.199	840	852	858	rBV	495037	766303	18.23%	2.820%
6	9.375	1043	1052	1063	rBV	1237528	2009596	47.82%	7.395%
7	11.028	1326	1333	1339	rBV	606842	1010334	24.04%	3.718%
8	13.451	1737	1745	1754	rBV	2538941	3743739	89.08%	13.777%
9	14.269	1877	1884	1891	rBV	199106	282559	6.72%	1.040%
10	14.822	1972	1978	1986	rVB2	773606	1156301	27.51%	4.255%
11	16.298	2219	2229	2240	rBV	1872894	2643591	62.90%	9.728%
12	17.545	2435	2441	2446	rBV	845270	1189343	28.30%	4.377%
13	17.586	2446	2448	2455	rVV	61925	76762	1.83%	0.282%
14	18.398	2582	2586	2592	rBV4	47862	80070	1.91%	0.295%
15	18.604	2615	2621	2625	rBV4	22457	42521	1.01%	0.156%
16	19.569	2780	2785	2791	rVB	174685	242225	5.76%	0.891%
17	19.927	2842	2846	2853	rVB	218332	292573	6.96%	1.077%
18	20.116	2873	2878	2885	rBV	3260792	4202842	100.00%	15.466%
19	21.345	3084	3087	3092	rBV	264933	332453	7.91%	1.223%
20	21.657	3135	3140	3145	rBV	972737	1391218	33.10%	5.120%
21	24.027	3537	3543	3550	rVB2	642758	1219328	29.01%	4.487%

Sum of corrected areas: 27174003

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122320\
Data File : BM028254.D
Acq On : 23 Dec 2020 16:42
Operator : JU/CG
Sample : L5189-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
09










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.216	2.70 ng	103370	1,4-Dichlorobenzene-d4	8.199

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	45		
2	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	10		
3	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
4	Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9		
5	5-Hexen-2-one	98	C6H10O	000109-49-9	9		

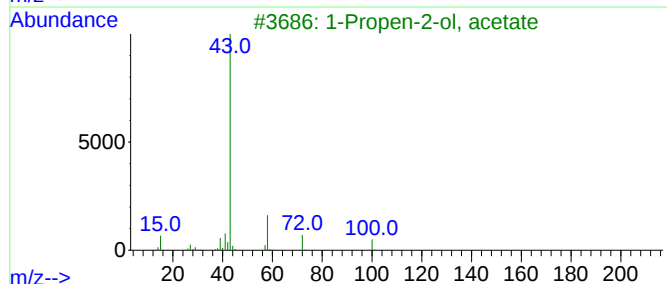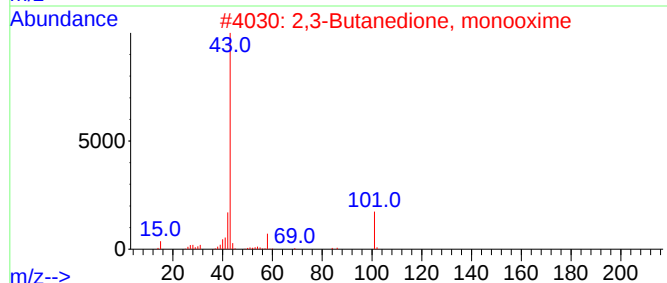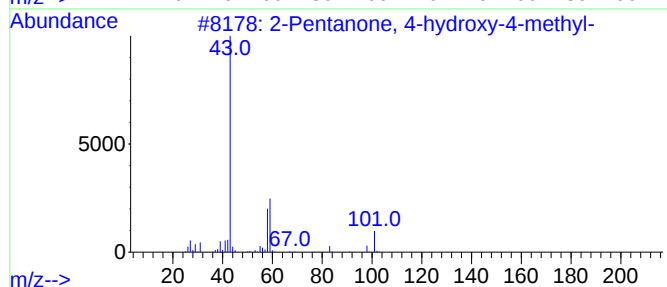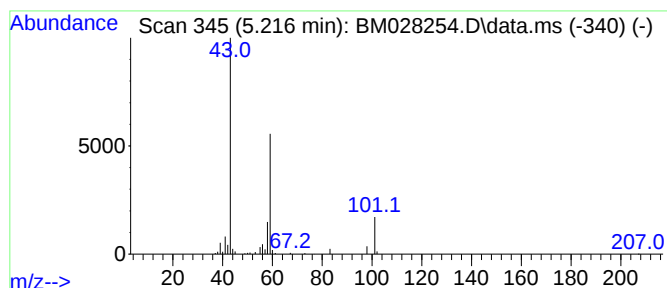

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122320\
Data File : BM028254.D
Acq On : 23 Dec 2020 16:42
Operator : JU/CG
Sample : L5189-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
09










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 5-Eicosene, (E)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.345	4.78 ng	332453	Chrysene-d12	21.663

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			5-Eicosene, (E)-	280	C20H40	074685-30-6	99
2			3-Eicosene, (E)-	280	C20H40	074685-33-9	98
3			Heptadecyl heptafluorobutyrate	452	C21H35F7O2	959085-66-6	94
4			Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	94
5			9-Eicosene, (E)-	280	C20H40	074685-29-3	93

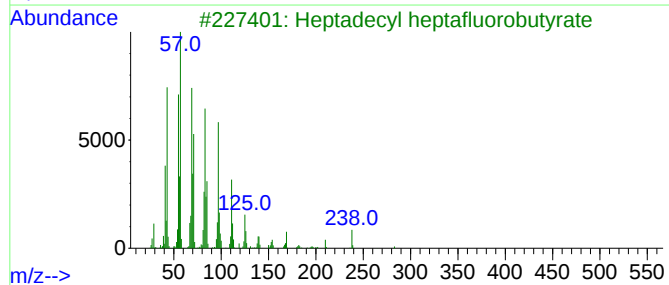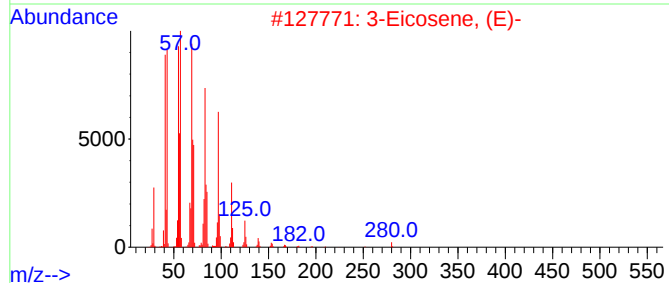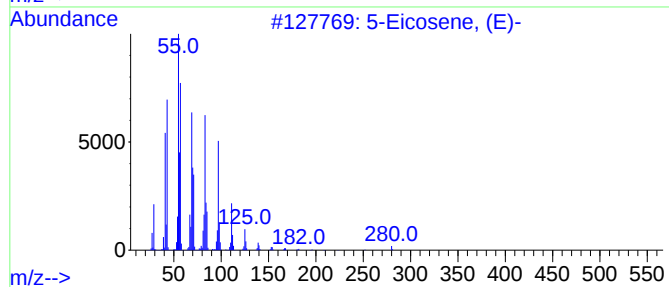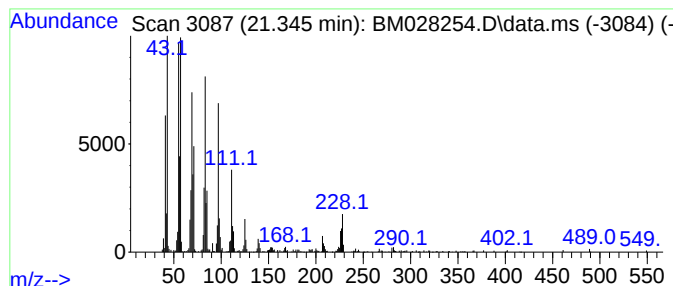

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122320\
Data File : BM028254.D
Acq On : 23 Dec 2020 16:42
Operator : JU/CG
Sample : L5189-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
09

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.216	2.7	ng	103370	1	8.199	766303	20.0
5-Eicosene, (E)-	21.345	4.8	ng	332453	5	21.663	1391220	20.0