

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122320\
 Data File : BM028255.D
 Acq On : 23 Dec 2020 17:18
 Operator : JU/CG
 Sample : L5192-01 2X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CL-02-122220

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121620.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM028255.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.222	340	346	354	rVB	12785	21323	1.13%	0.104%
2	5.693	419	426	436	rBV	996812	1496846	79.42%	7.279%
3	7.340	698	706	724	rVB	974109	1706262	90.53%	8.297%
4	8.198	839	852	859	rBV	555243	877777	46.57%	4.269%
5	9.375	1044	1052	1060	rBV	582428	970786	51.51%	4.721%
6	9.757	1112	1117	1126	rBV2	11373	19691	1.04%	0.096%
7	11.028	1326	1333	1339	rBV	663851	1140708	60.52%	5.547%
8	13.451	1737	1745	1753	rBV	1338612	1860101	98.69%	9.046%
9	14.269	1877	1884	1890	rBV	51703	79349	4.21%	0.386%
10	14.551	1927	1932	1941	rBV2	31739	52647	2.79%	0.256%
11	14.827	1971	1979	1985	rBV	861201	1284612	68.16%	6.247%
12	14.886	1985	1989	1995	rVB	39776	56176	2.98%	0.273%
13	15.216	2037	2045	2054	rBV	19475	34757	1.84%	0.169%
14	15.857	2149	2154	2161	rBV2	35389	57851	3.07%	0.281%
15	16.298	2223	2229	2239	rBV	870366	1208209	64.10%	5.875%
16	17.274	2390	2395	2399	rBV2	18502	28247	1.50%	0.137%
17	17.368	2407	2411	2416	rVB	20413	30779	1.63%	0.150%
18	17.545	2435	2441	2445	rBV	940353	1306846	69.34%	6.355%
19	17.586	2445	2448	2454	rVV	347116	450008	23.88%	2.188%
20	17.674	2455	2463	2469	rVV	84479	134137	7.12%	0.652%
21	17.939	2503	2508	2514	rVB2	31295	45570	2.42%	0.222%
22	18.180	2545	2549	2554	rBV3	18257	24753	1.31%	0.120%
23	18.404	2582	2587	2592	rBV2	62343	108031	5.73%	0.525%
24	18.457	2592	2596	2601	rVB	53512	76250	4.05%	0.371%
25	18.539	2606	2610	2614	rVV	23139	30155	1.60%	0.147%
26	18.604	2615	2621	2625	rVV3	69547	124333	6.60%	0.605%
27	18.639	2625	2627	2632	rVB	31817	35014	1.86%	0.170%
28	18.692	2632	2636	2642	rBV7	13740	27803	1.48%	0.135%
29	18.898	2667	2671	2675	rBV	30133	40401	2.14%	0.196%
30	18.939	2675	2678	2683	rVB4	16408	23948	1.27%	0.116%
31	19.304	2736	2740	2743	rBV2	62060	89781	4.76%	0.437%
32	19.333	2743	2745	2749	rVB5	29883	35596	1.89%	0.173%
33	19.574	2780	2786	2791	rBV	542619	738594	39.19%	3.592%
34	19.656	2797	2800	2805	rVB4	27279	37919	2.01%	0.184%
35	19.898	2836	2841	2842	rBV2	78975	112119	5.95%	0.545%
36	19.933	2842	2847	2854	rVB	477170	683309	36.25%	3.323%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122320\
Data File : BM028255.D
Acq On : 23 Dec 2020 17:18
Operator : JU/CG
Sample : L5192-01 2X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CL-02-122220

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121620.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	20.121	2873	2879	2883	rBV	1504170	1884824	100.00%	9.166%
38	20.415	2925	2929	2933	rVB	85356	118708	6.30%	0.577%
39	20.515	2942	2946	2949	rBV2	62628	74474	3.95%	0.362%
40	21.350	3084	3088	3092	rBV	177679	215388	11.43%	1.047%
41	21.662	3134	3141	3145	rBV2	1060888	1792816	95.12%	8.718%
42	21.698	3145	3147	3154	rVB	268257	303788	16.12%	1.477%
43	24.027	3538	3543	3549	rVB2	624032	1123089	59.59%	5.461%




Sum of corrected areas: 20563775

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122320\
Data File : BM028255.D
Acq On : 23 Dec 2020 17:18
Operator : JU/CG
Sample : L5192-01 2X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CL-02-122220

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

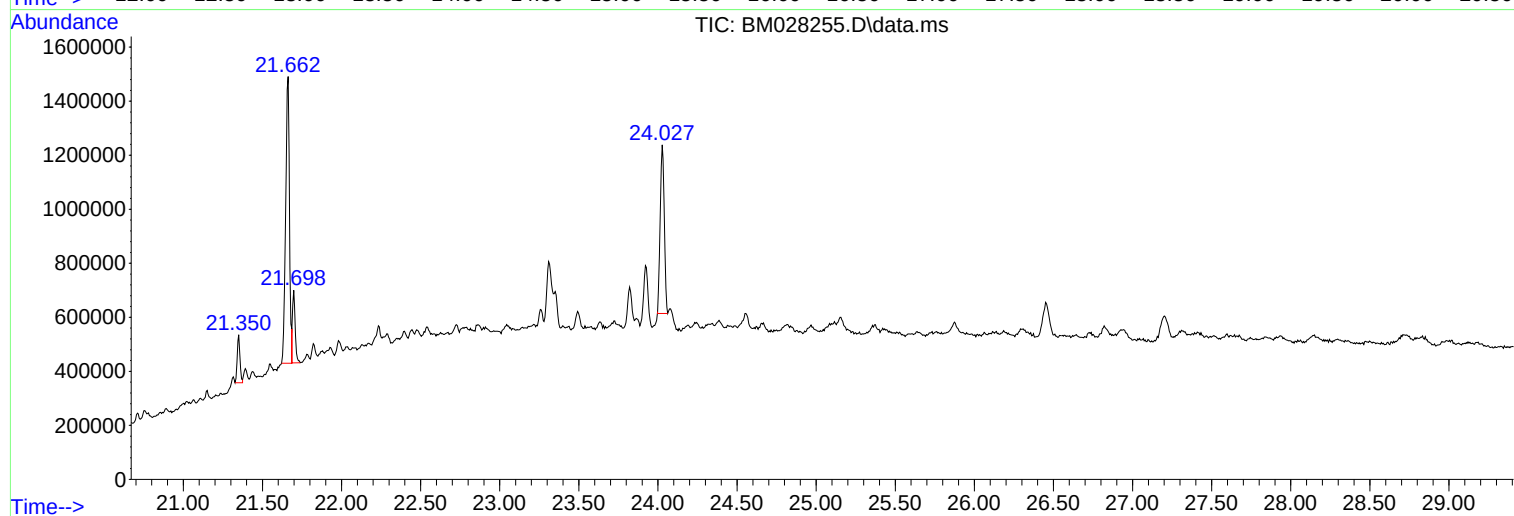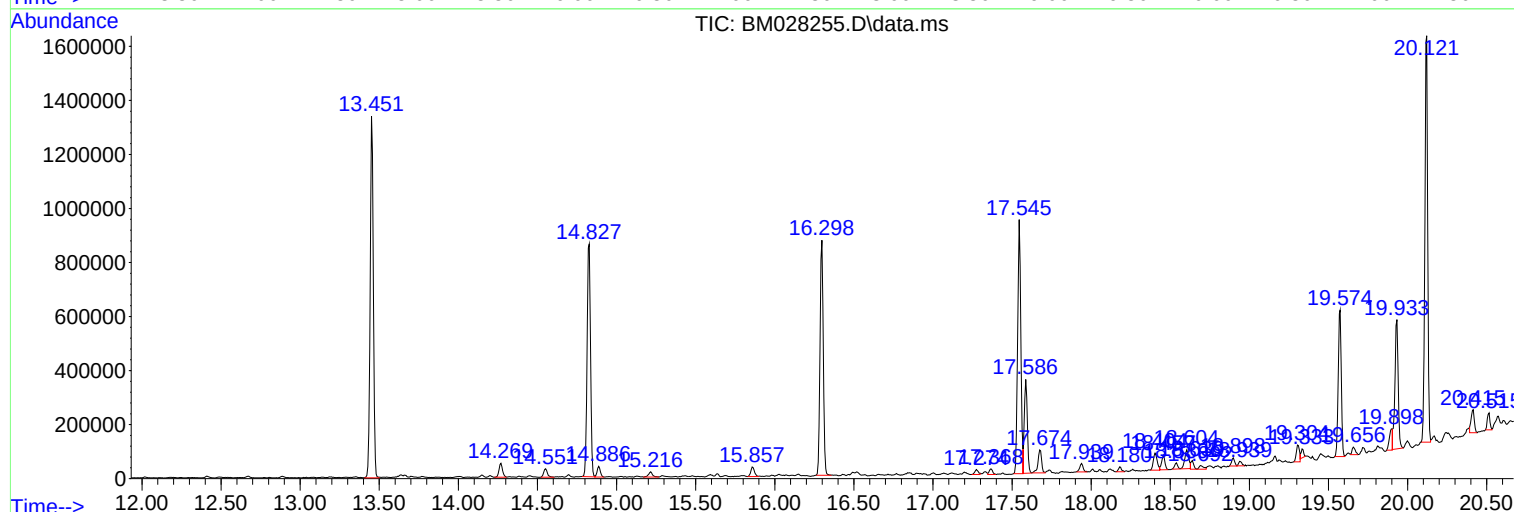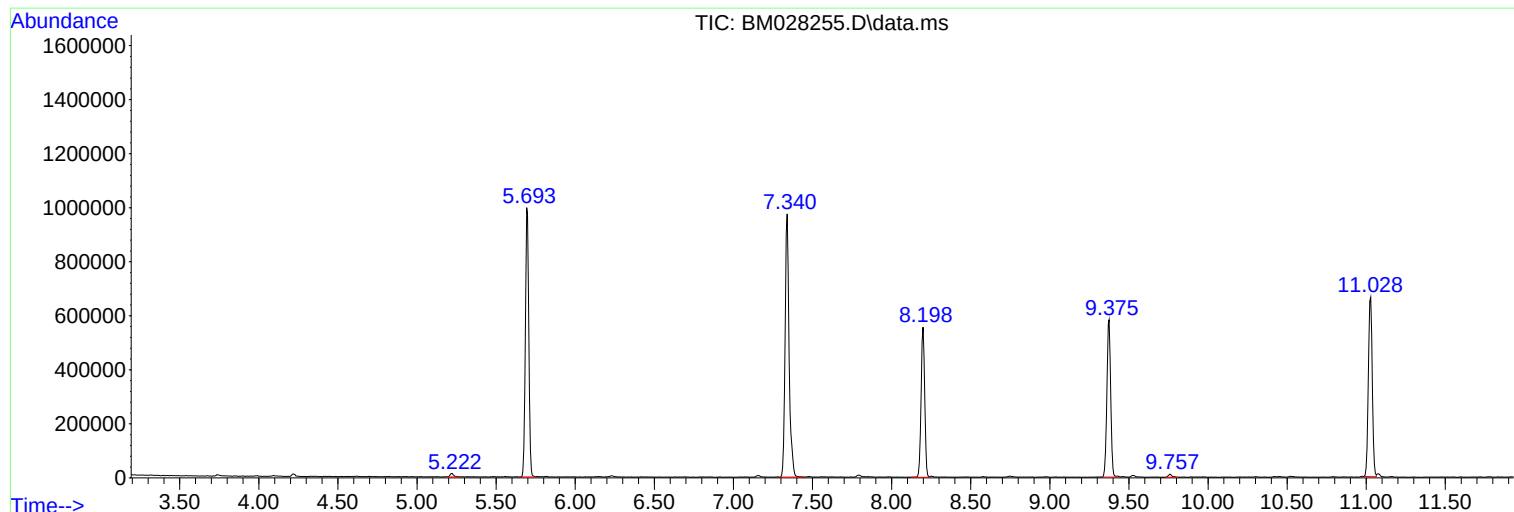

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122320\
Data File : BM028255.D
Acq On : 23 Dec 2020 17:18
Operator : JU/CG
Sample : L5192-01 2X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CL-02-122220

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122320\
Data File : BM028255.D
Acq On : 23 Dec 2020 17:18
Operator : JU/CG
Sample : L5192-01 2X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CL-02-122220

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------