


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122320\
 Data File : BM028243.D
 Acq On : 23 Dec 2020 08:43
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM121620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 23 12:17:02 2020

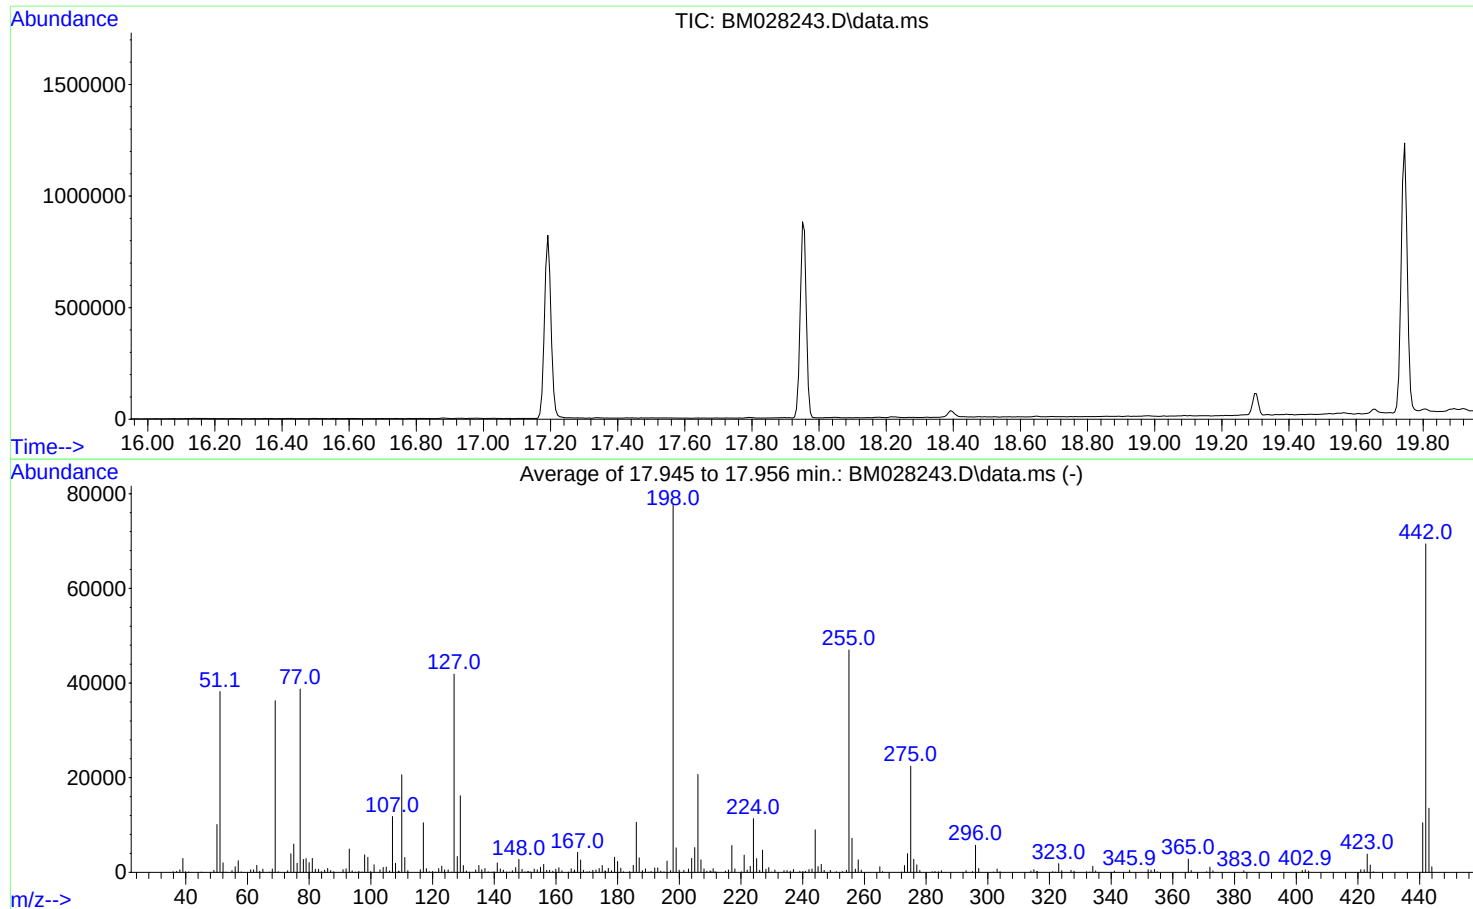

AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.2	38219	PASS
68	69	0.00	2	2.0	722	PASS
69	198	0.00	100	46.7	36269	PASS
70	69	0.00	2	0.4	151	PASS
127	198	10	80	53.9	41885	PASS
197	198	0.00	2	0.5	382	PASS
198	198	100	100	100.0	77731	PASS
199	198	5	9	6.6	5162	PASS
275	198	10	60	28.8	22405	PASS
365	198	1	100	3.6	2822	PASS
441	198	0.01	100	13.5	10475	PASS
442	198	50	100	89.3	69405	PASS
443	442	15	24	19.6	13573	PASS