

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
 Data File : BM049175.D
 Acq On : 24 Dec 2024 09:23
 Operator : RC/JU
 Sample : PB165769BL
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK769

Quant Time: Dec 24 21:39:16 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 18 15:33:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.548	152	9540	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.308	136	27510	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.186	164	15319	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.034	188	1515167	0.400	ng/ul	0.08
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.15
23) Perylene-d12	23.288	264	37664	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.139	96	41103	3.736	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.920	152	7204	0.195	ng/ul	0.00
18) Fluoranthene-d10	18.973	212	15314	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.185	166	2589	0.050	ng/ul#	15
26) Benzo(a)pyrene	23.157	252	6490	0.056	ng/ul#	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049175.D
Acq On : 24 Dec 2024 09:23
Operator : RC/JU
Sample : PB165769BL
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK769

Quant Time: Dec 24 21:39:16 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration




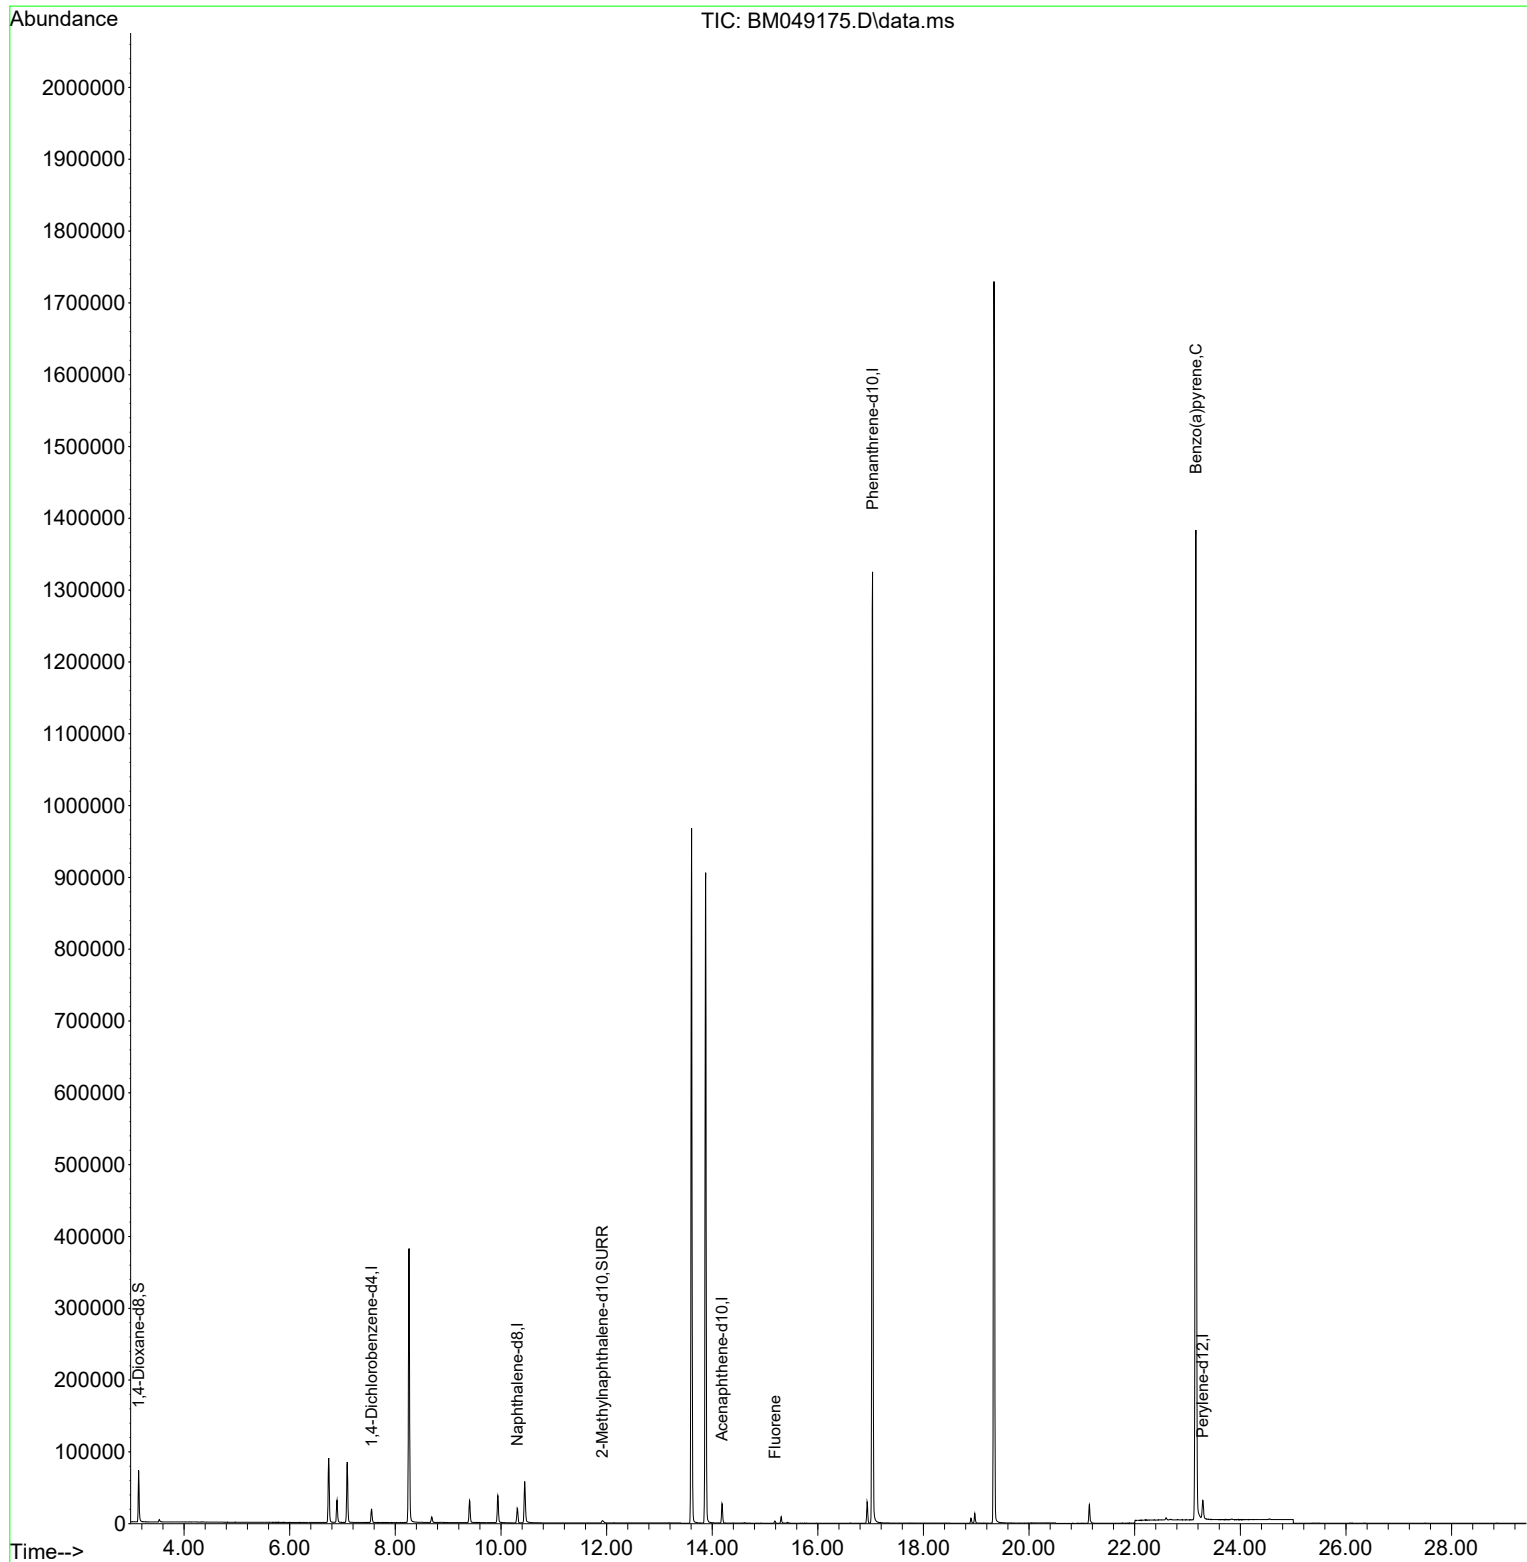


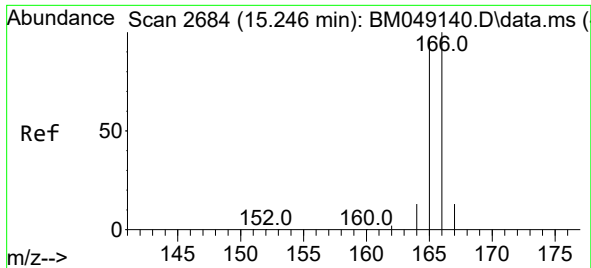

#12
Fluorene
Concen: 0.050 ng/ul
RT: 15.185 min Scan# 2
Delta R.T. -0.069 min
Lab File: BM049175.D
Acq: 24 Dec 2024 09:23

Instrument :
BNA_M
ClientSampleId :
SBLK769

Tgt Ion:166 Resp: 2589
Ion Ratio Lower Upper
166 100
165 9.2 79.7 119.5#
167 33.2 11.4 17.0#

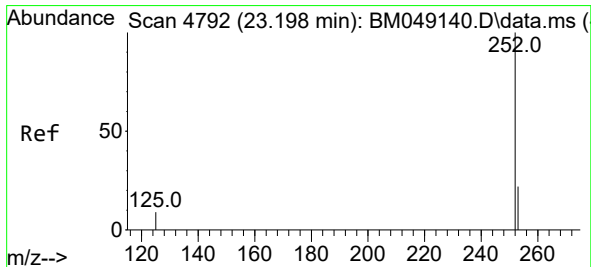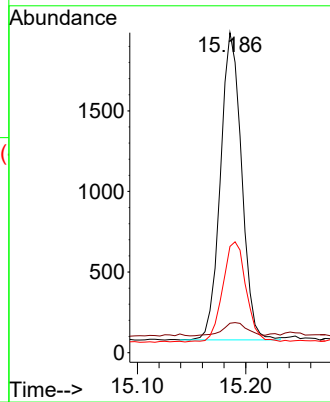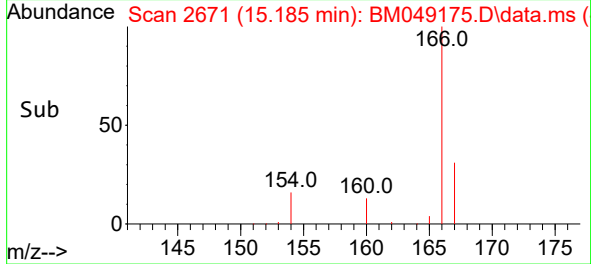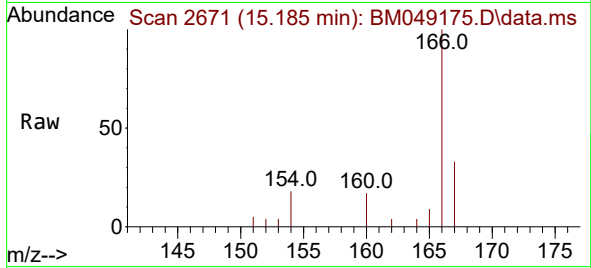

#26
Benzo(a)pyrene
Concen: 0.056 ng/ul
RT: 23.157 min Scan# 4778
Delta R.T. -0.053 min
Lab File: BM049175.D
Acq: 24 Dec 2024 09:23

Tgt Ion:252 Resp: 6490
Ion Ratio Lower Upper
252 100
253 39.1 22.4 33.6#
125 29.7 14.8 22.2#

