

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
 Data File : BM049185.D
 Acq On : 24 Dec 2024 15:19
 Operator : RC/JU
 Sample : P5302-17
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E2AQ0

Quant Time: Dec 24 21:41:02 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 18 15:33:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.552	152	7681	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.308	136	23995	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.186	164	13386	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.035	188	1658580	0.400	ng/ul	0.08
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.15
23) Perylene-d12	23.291	264	31905	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.143	96	33566	3.789	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.909	152	8582	0.266	ng/ul	-0.02
18) Fluoranthene-d10	18.973	212	19476	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
26) Benzo(a)pyrene	23.157	252	5999	0.061	ng/ul#	56


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049185.D
Acq On : 24 Dec 2024 15:19
Operator : RC/JU
Sample : P5302-17
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2AQ0


Quant Time: Dec 24 21:41:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

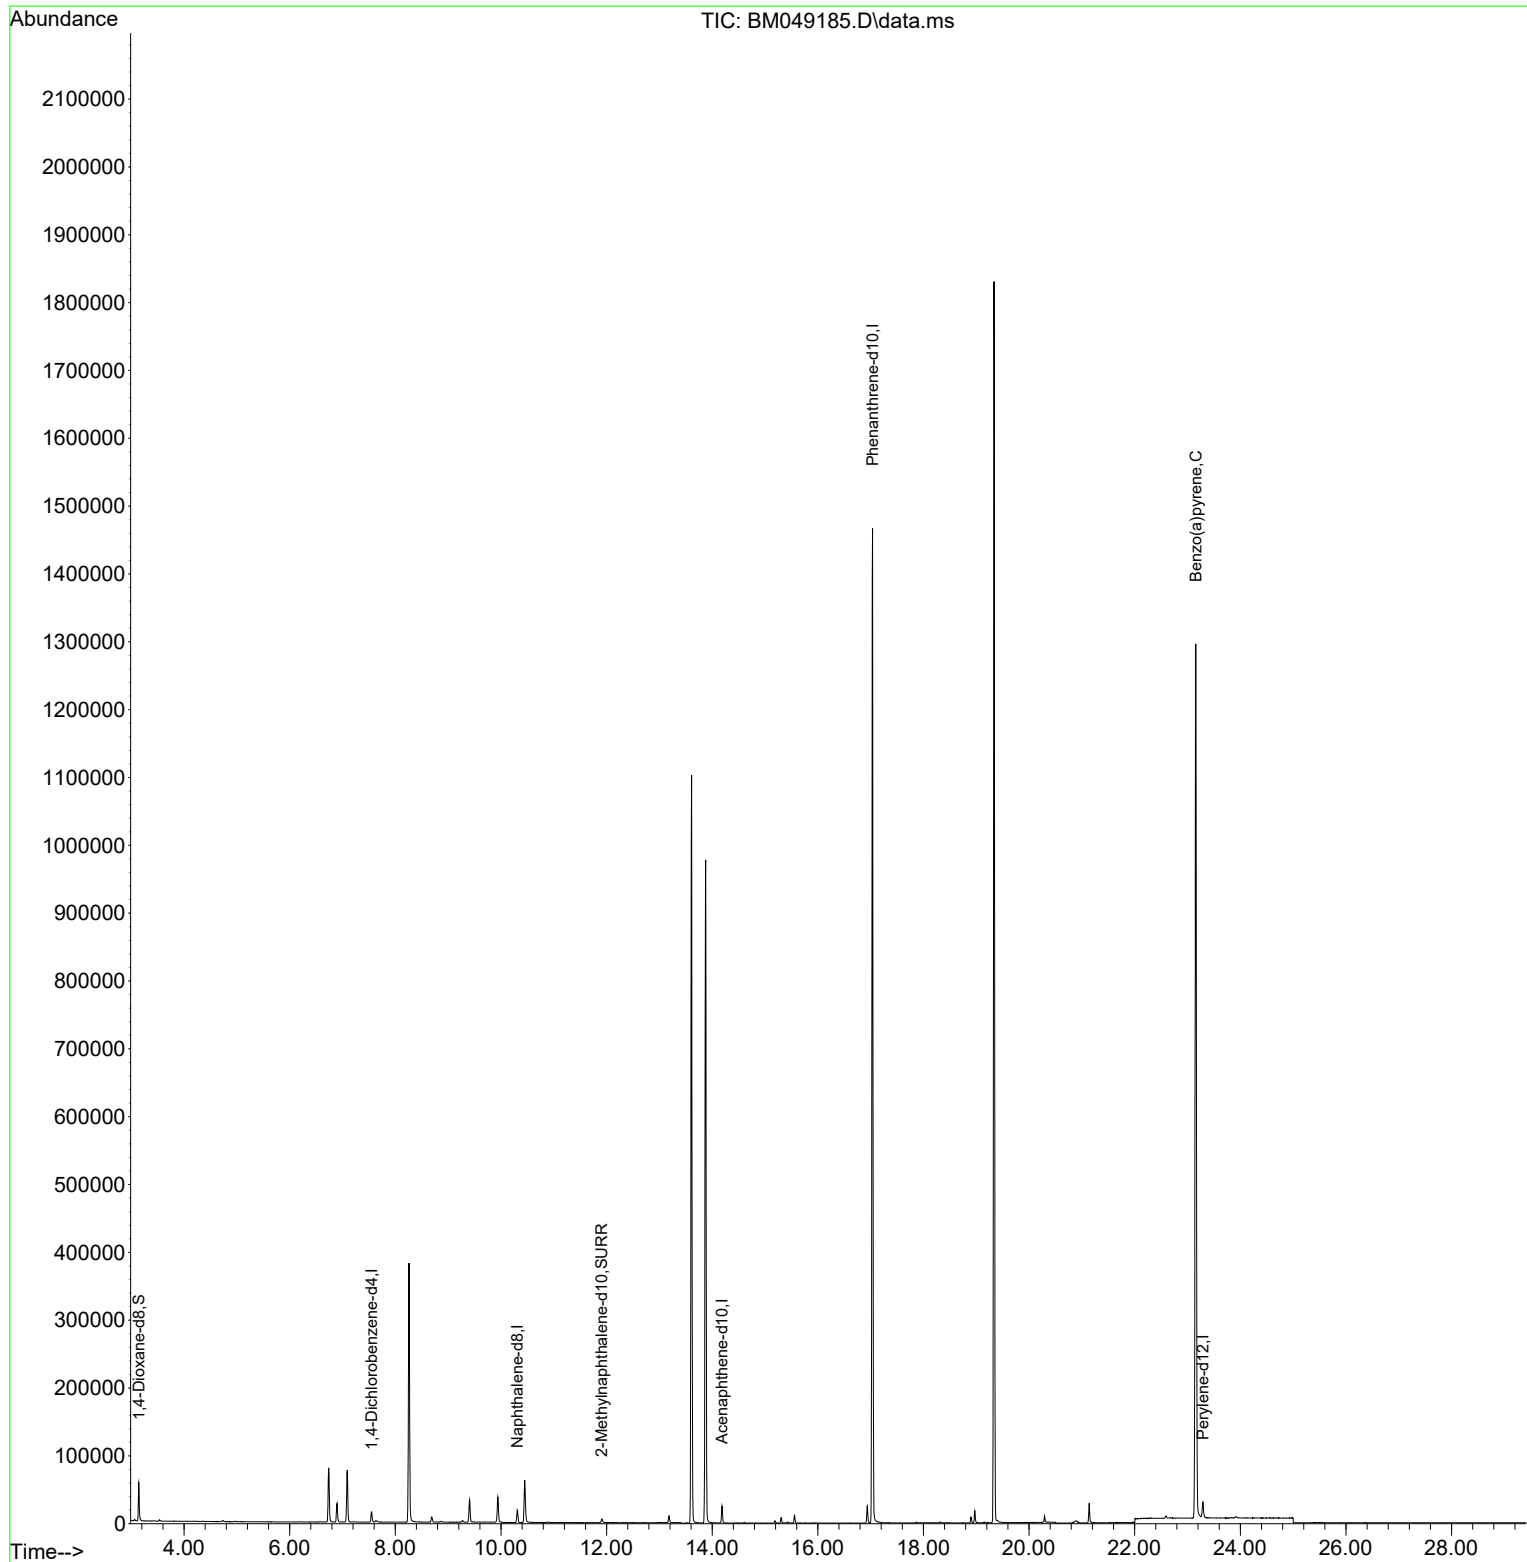

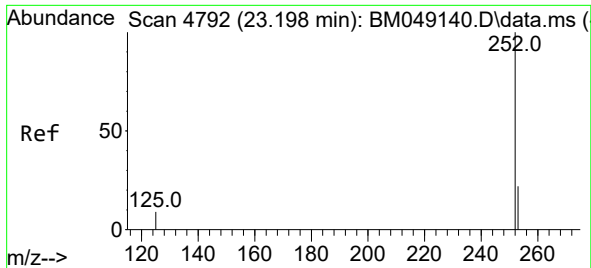

#26
Benzo(a)pyrene
Concen: 0.061 ng/ul
RT: 23.157 min Scan# 41
Delta R.T. -0.052 min
Lab File: BM049185.D
Acq: 24 Dec 2024 15:19

Instrument :
BNA_M
ClientSampleId :
E2AQ0

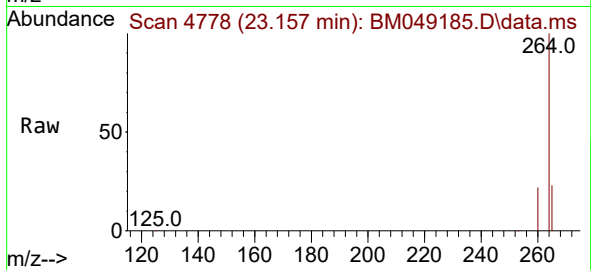

Tgt Ion:252 Resp: 5999
Ion Ratio Lower Upper
252 100
253 48.7 22.4 33.6#
125 41.4 14.8 22.2#

