

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
 Data File : BM049192.D
 Acq On : 24 Dec 2024 20:05
 Operator : RC/JU
 Sample : PB165752BL
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK752

Quant Time: Dec 24 21:42:12 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 18 15:33:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.548	152	5362	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.308	136	16185	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.186	164	8804	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.035	188	1626684	0.400	ng/ul	# 0.08
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.15
23) Perylene-d12	23.291	264	21086	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.139	96	39885	6.450	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.914	152	8452	0.389	ng/ul	-0.01
18) Fluoranthene-d10	18.973	212	17574	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
26) Benzo(a)pyrene	23.157	252	6498	0.101	ng/ul#	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049192.D
Acq On : 24 Dec 2024 20:05
Operator : RC/JU
Sample : PB165752BL
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK752


Quant Time: Dec 24 21:42:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

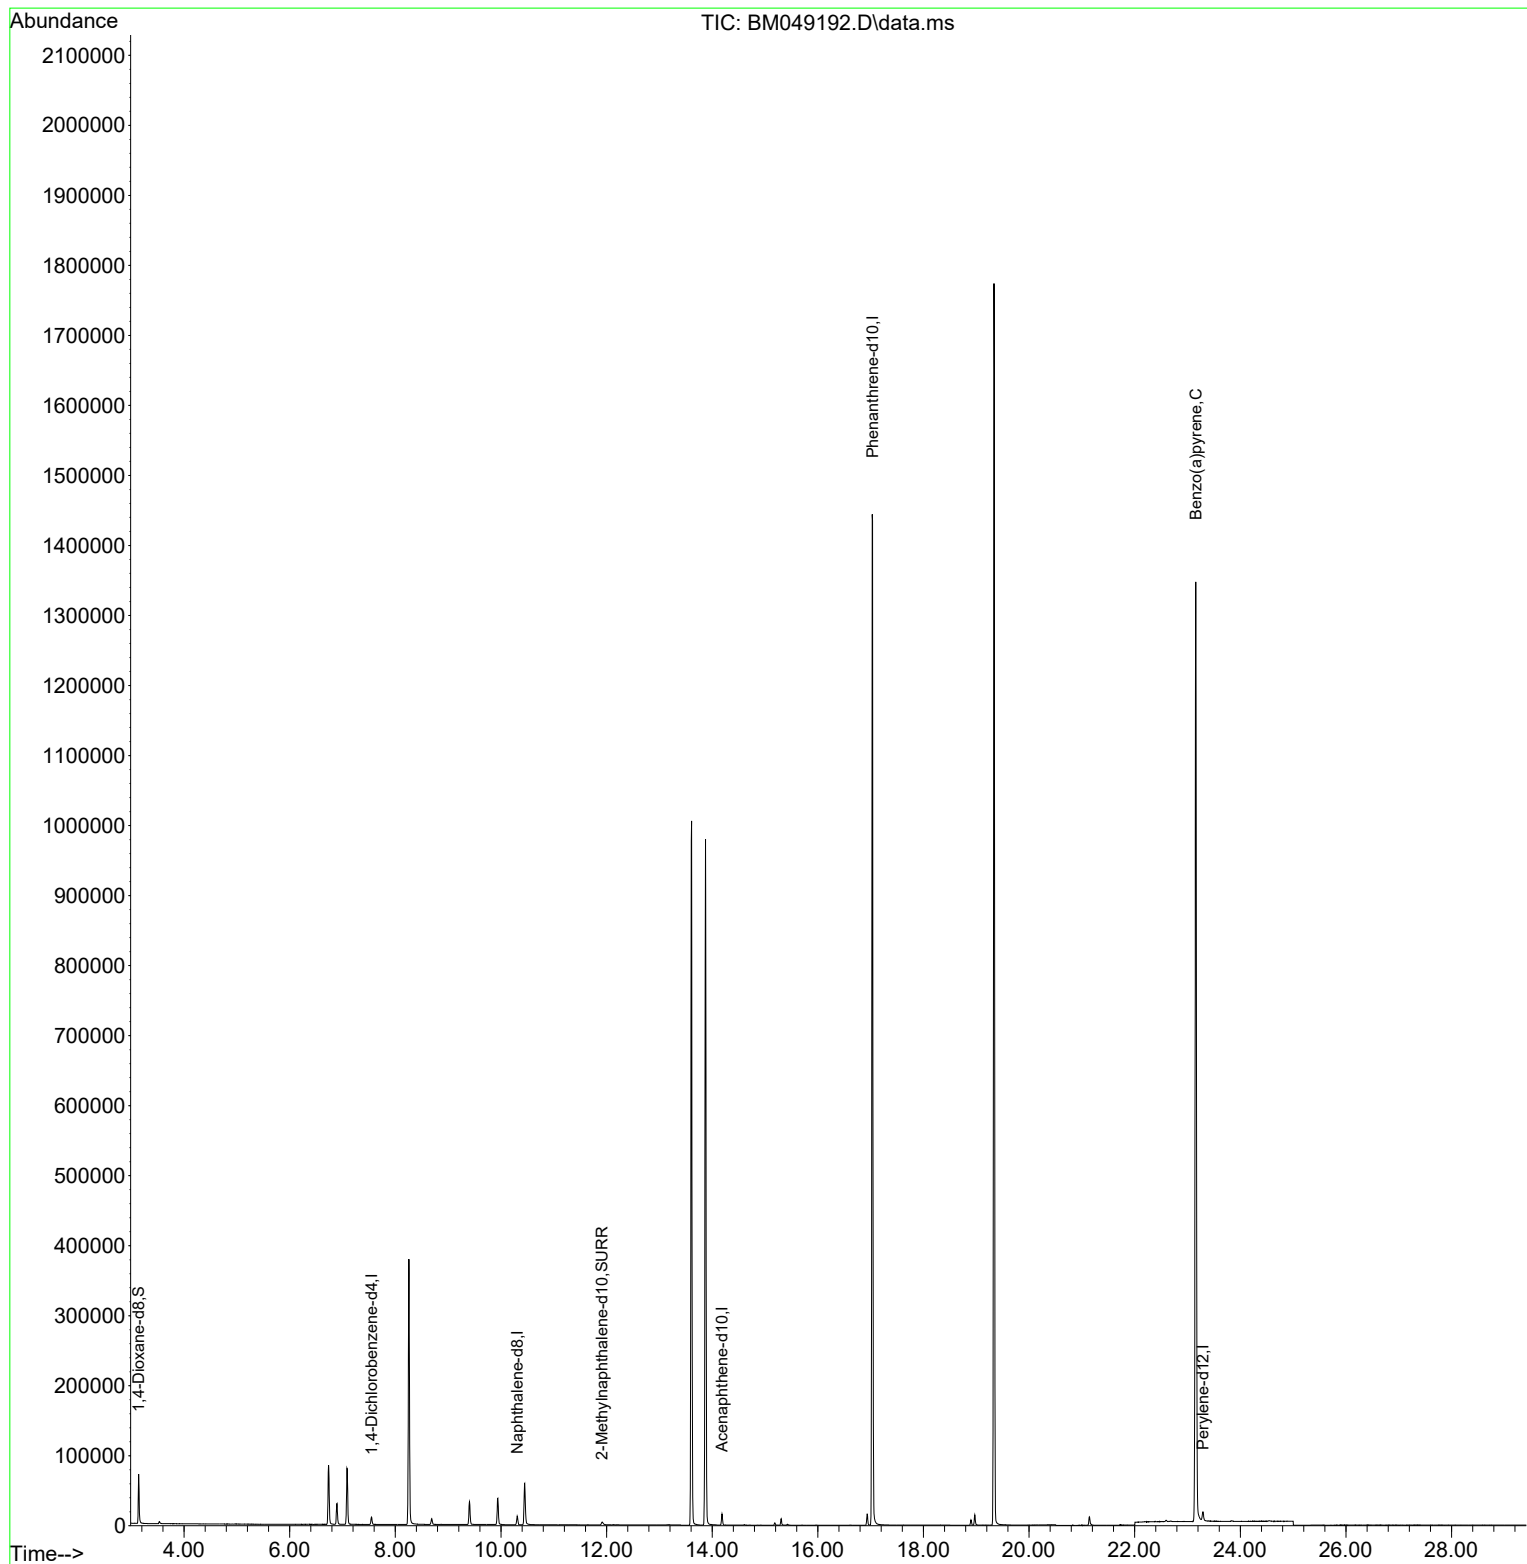

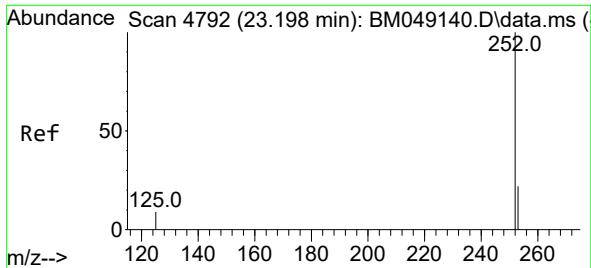

#26
Benzo(a)pyrene
Concen: 0.101 ng/ul
RT: 23.157 min Scan# 41
Delta R.T. -0.052 min
Lab File: BM049192.D
Acq: 24 Dec 2024 20:05

Instrument :
BNA_M
ClientSampleId :
SBLK752

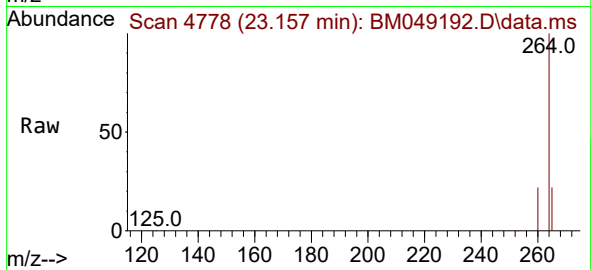

Tgt Ion:252 Resp: 6498
Ion Ratio Lower Upper
252 100
253 42.5 22.4 33.6#
125 30.8 14.8 22.2#

