




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049141.D
Acq On : 23 Dec 2024 11:27
Operator : RC/JU
Sample : PB165769BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK769

Manual IntegrationsAPPROVED

Quant Time: Dec 23 11:56:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

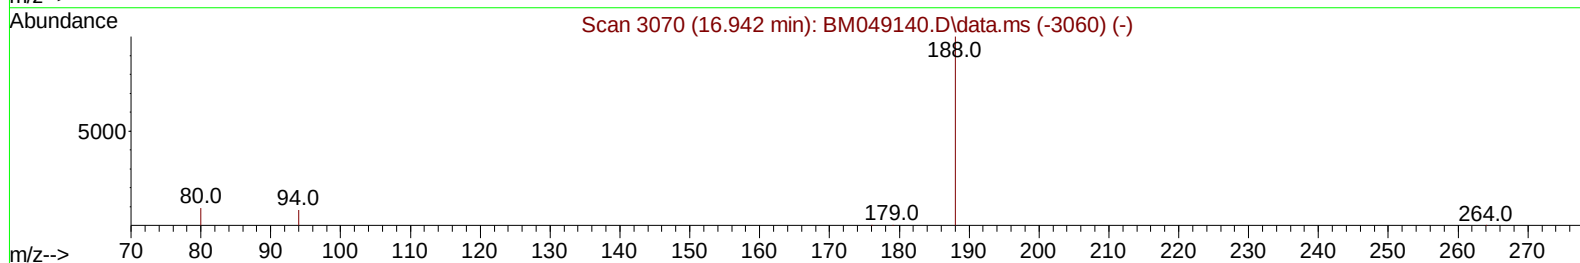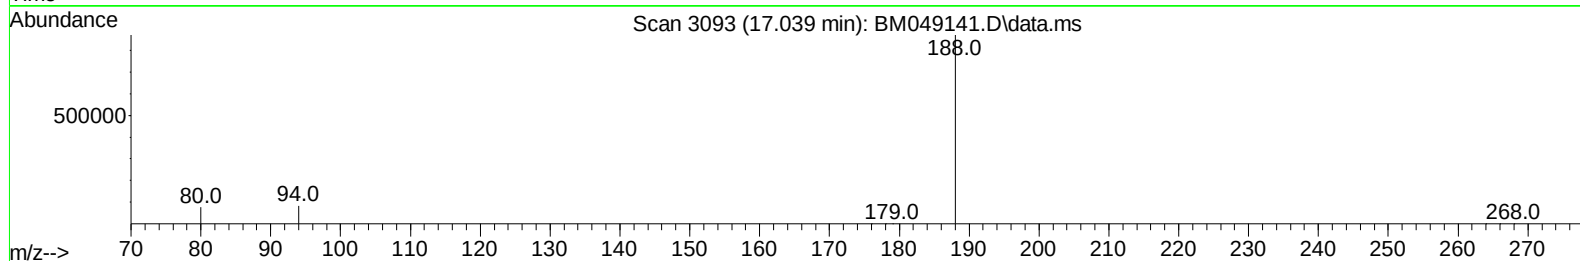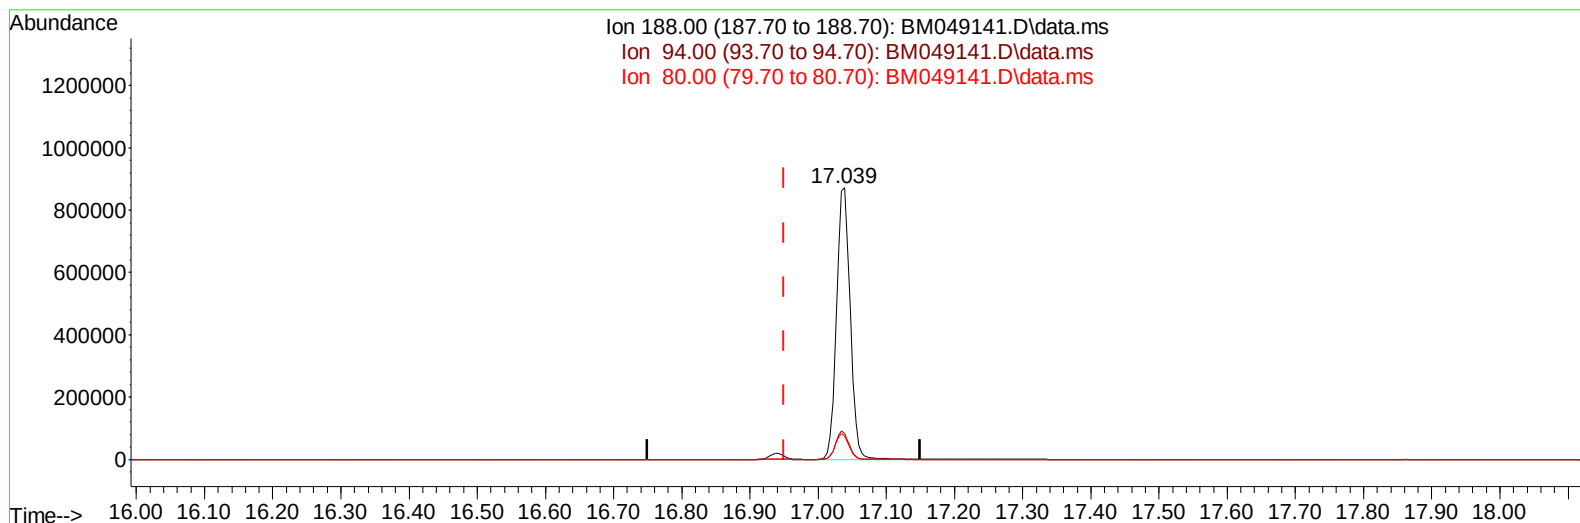

TIC: BM049141.D\data.ms

(13) Phenanthrene-d10 (I)

17.039min (+ 0.089) 0.40 ng/u1

response 1209360

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	9.80	9.66
80.00	10.70	8.71
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049141.D
Acq On : 23 Dec 2024 11:27
Operator : RC/JU
Sample : PB165769BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK769

Manual IntegrationsAPPROVED

Quant Time: Dec 23 11:56:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

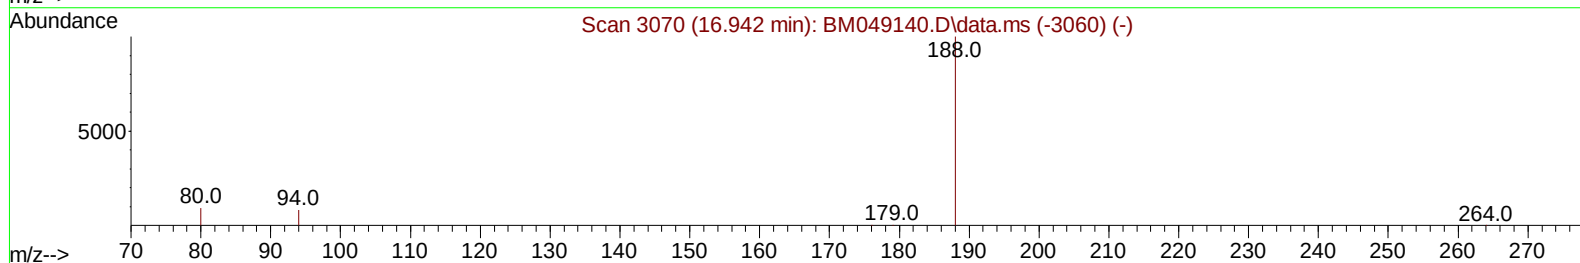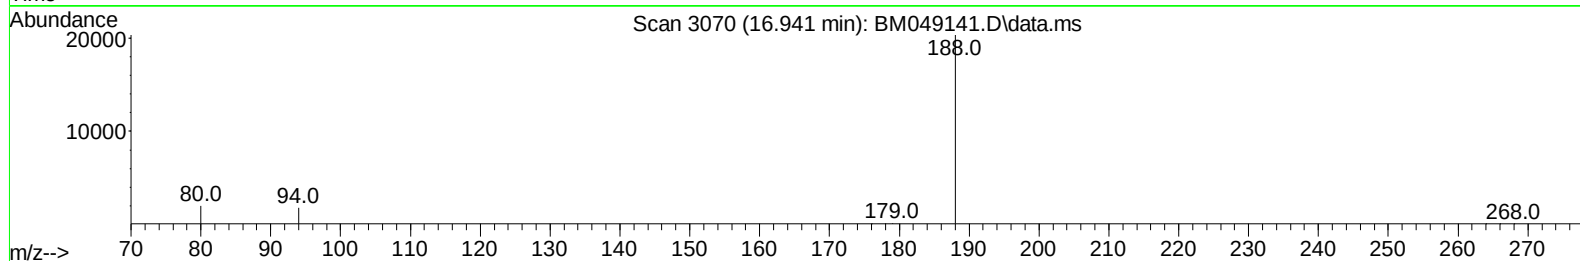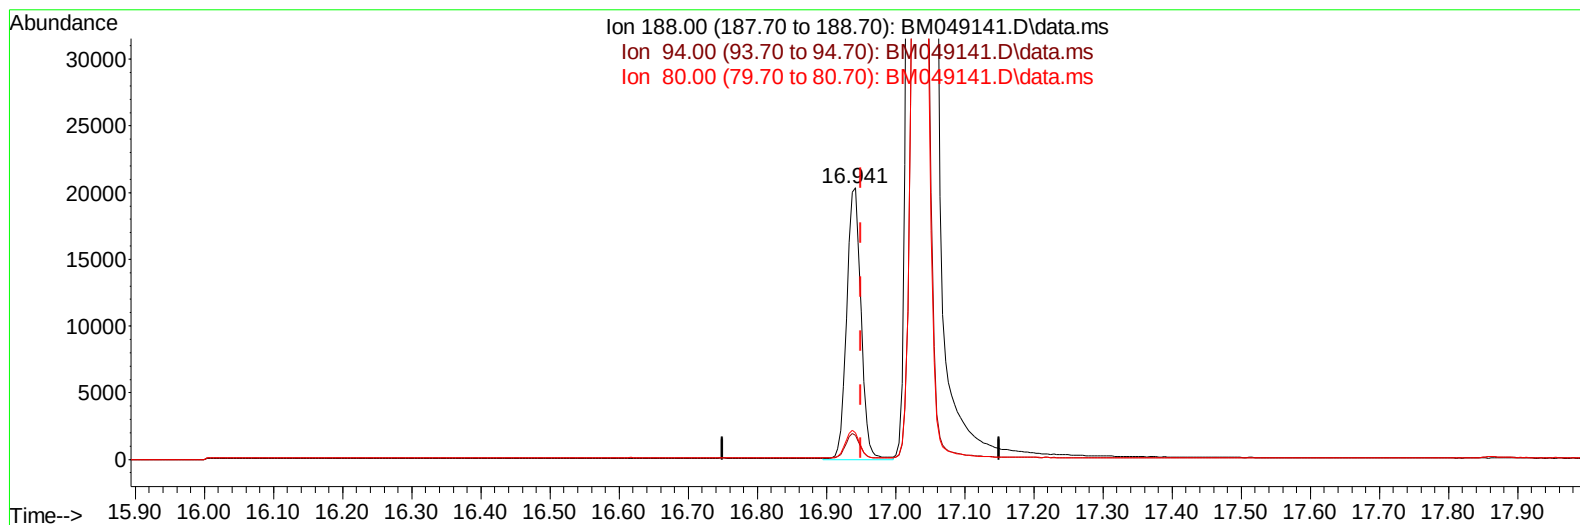

TIC: BM049141.D\data.ms

(13) Phenanthrene-d10 (I)

16.941min (-0.008) 0.40 ng/ul m

response 29152

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	9.80	8.76
80.00	10.70	9.74
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049141.D
Acq On : 23 Dec 2024 11:27
Operator : RC/JU
Sample : PB165769BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK769

Manual IntegrationsAPPROVED

Quant Time: Dec 23 11:56:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

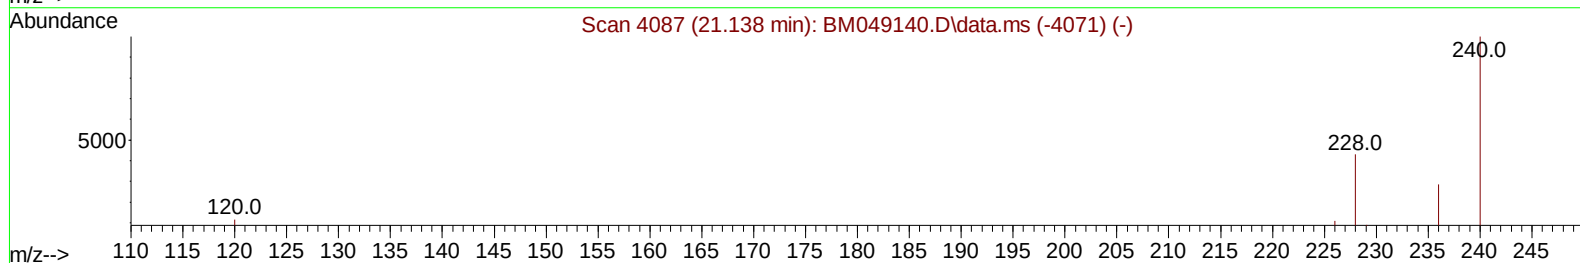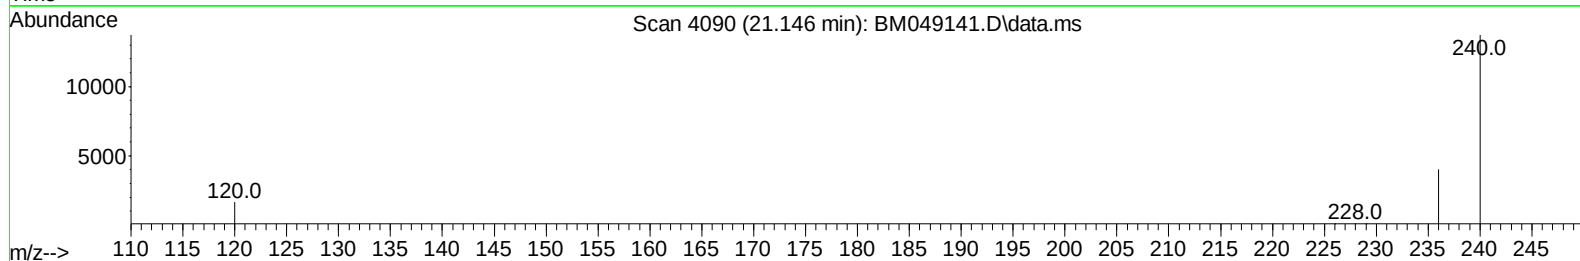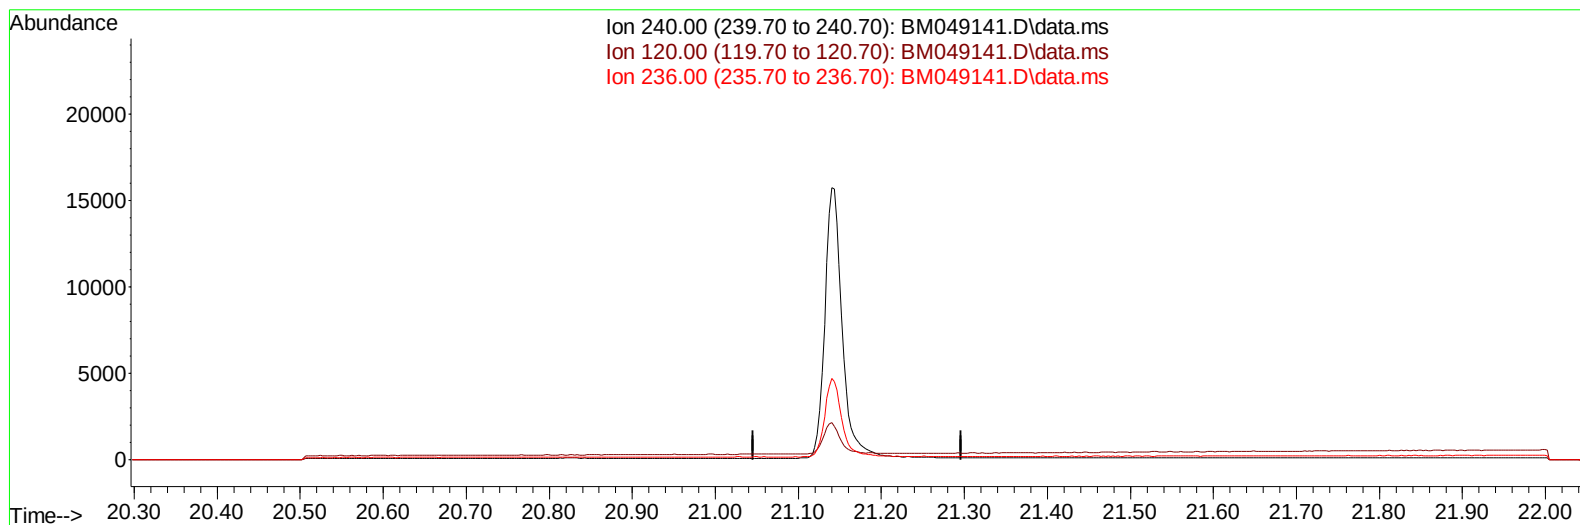

TIC: BM049141.D\data.ms

(17) Chrysene-d12

21.146min (-21.146) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	14.50	0.00#
236.00	29.80	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049141.D
Acq On : 23 Dec 2024 11:27
Operator : RC/JU
Sample : PB165769BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK769

Manual IntegrationsAPPROVED

Quant Time: Dec 23 11:56:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

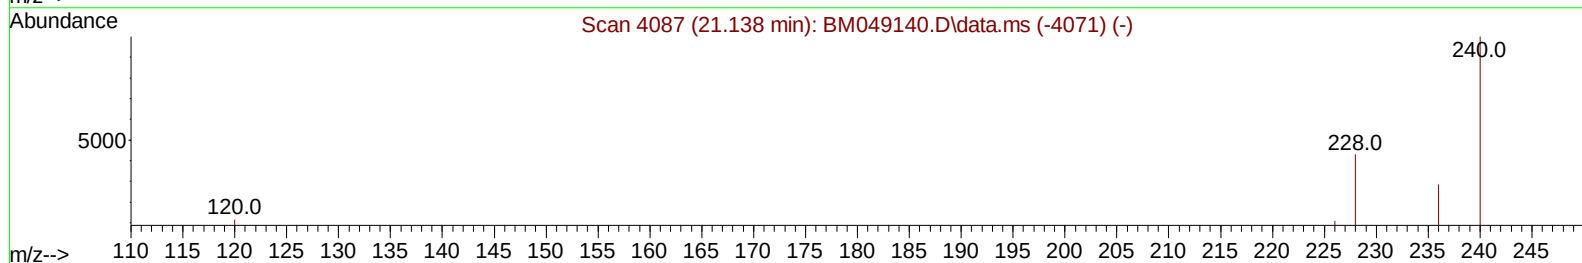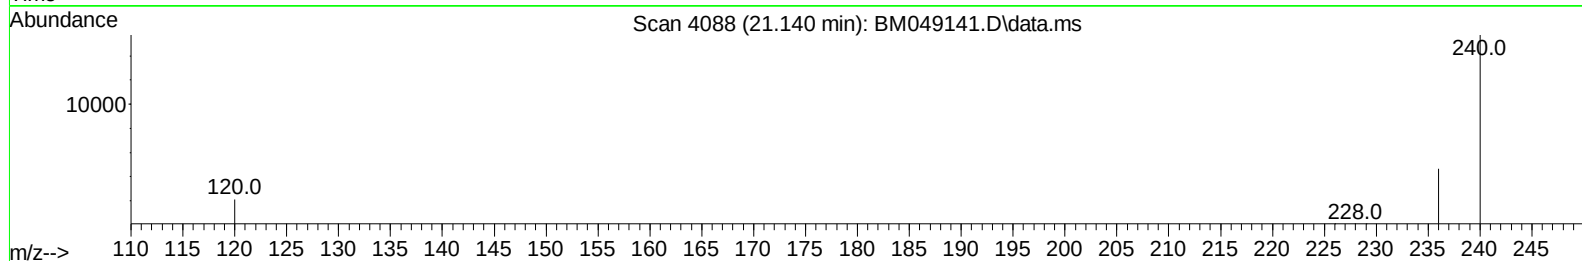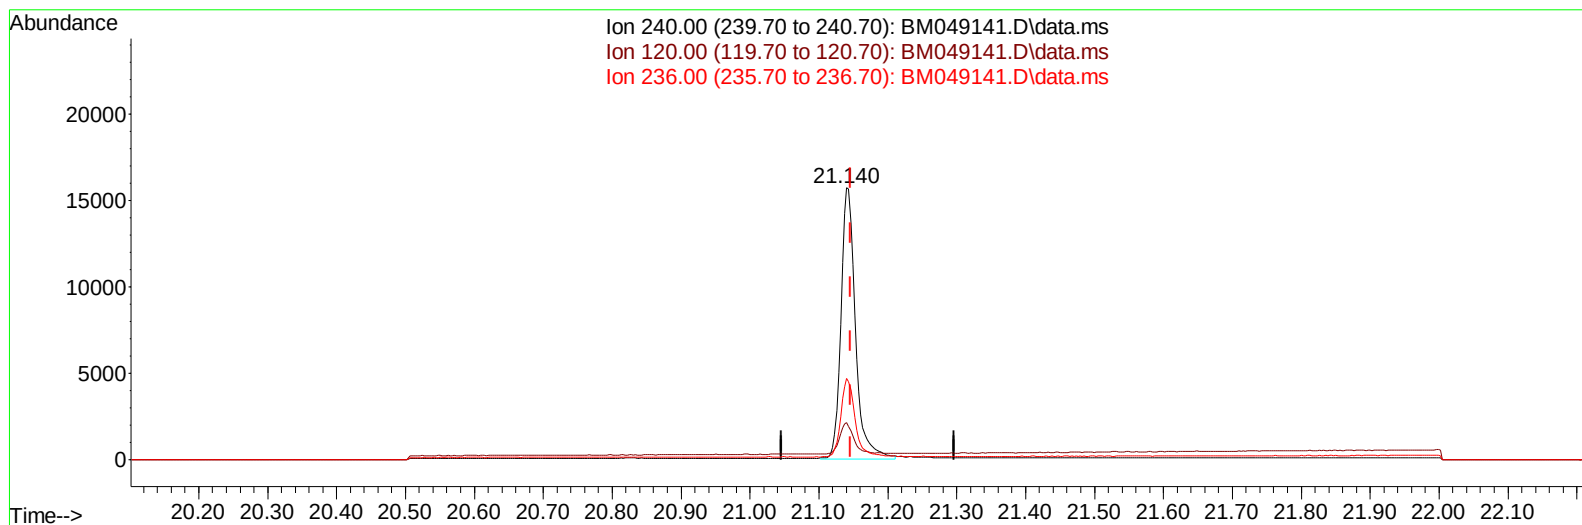

TIC: BM049141.D\data.ms

(17) Chrysene-d12

21.140min (-0.006) 0.40 ng/ul m

response 22904

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	14.50	13.56
236.00	29.80	29.77
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049141.D
Acq On : 23 Dec 2024 11:27
Operator : RC/JU
Sample : PB165769BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK769

Manual IntegrationsAPPROVED

Quant Time: Dec 23 11:56:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

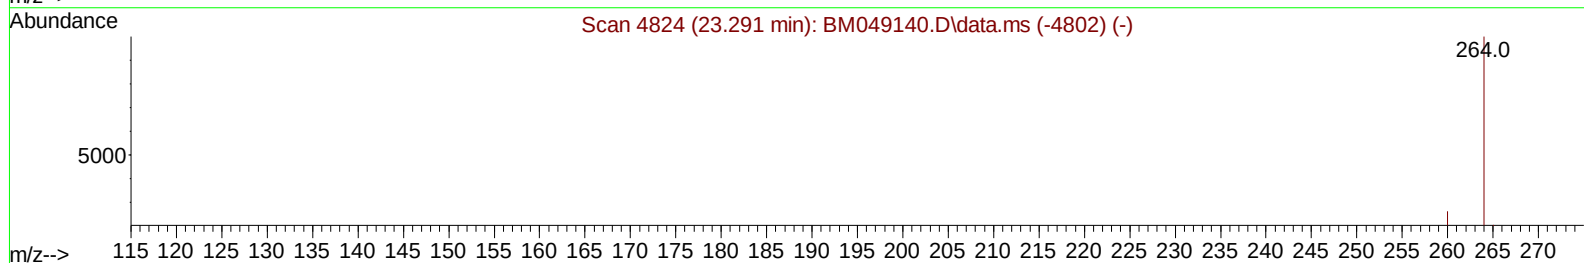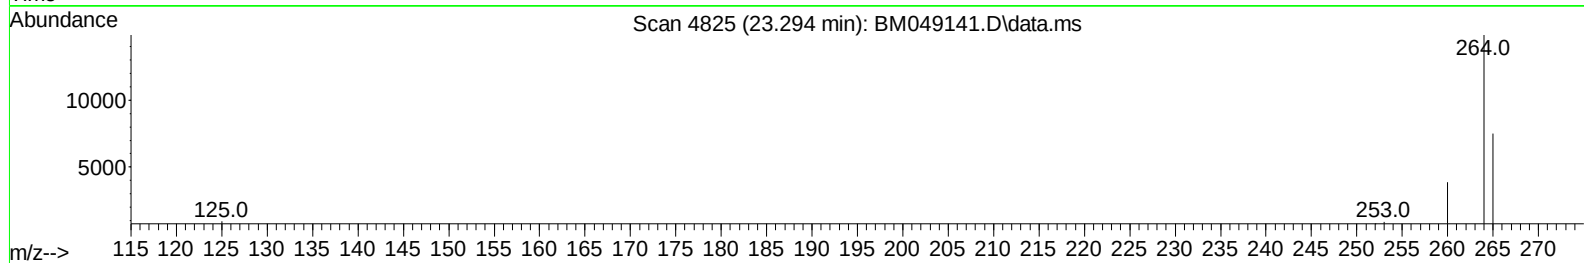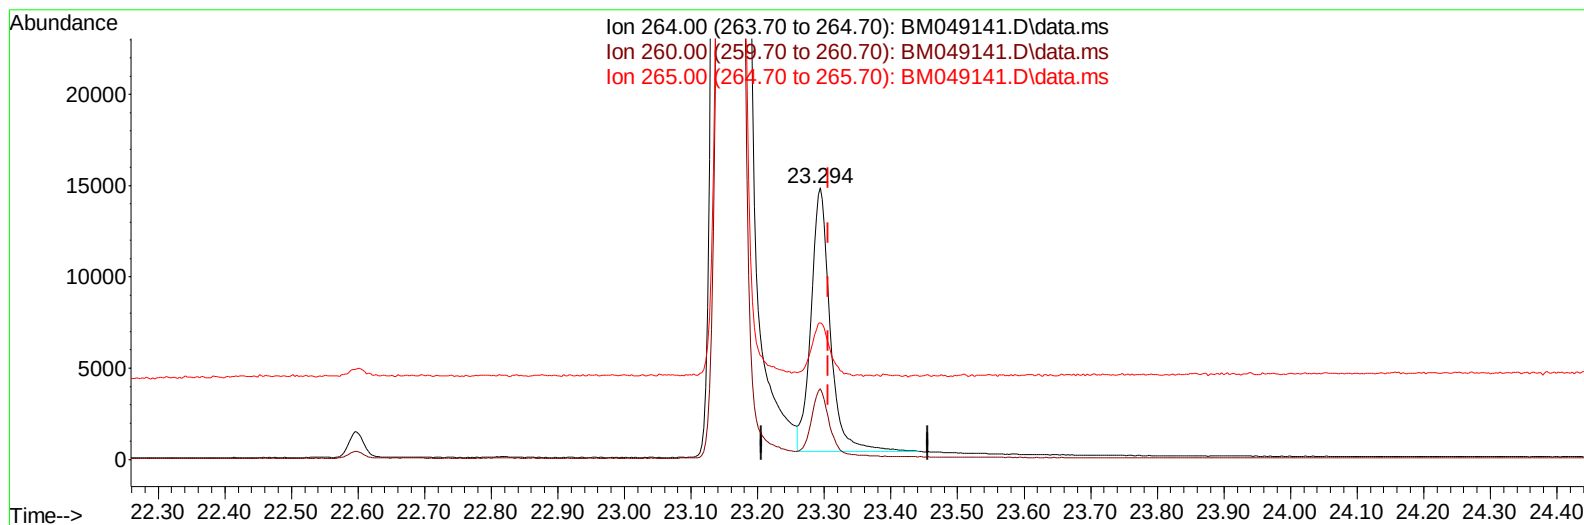

TIC: BM049141.D\data.ms

(23) Perylene-d12 (I)

23.294min (-0.012) 0.40 ng/u1

response 28964

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.80	26.07
265.00	78.30	50.39#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049141.D
Acq On : 23 Dec 2024 11:27
Operator : RC/JU
Sample : PB165769BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK769

Manual IntegrationsAPPROVED

Quant Time: Dec 23 11:56:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

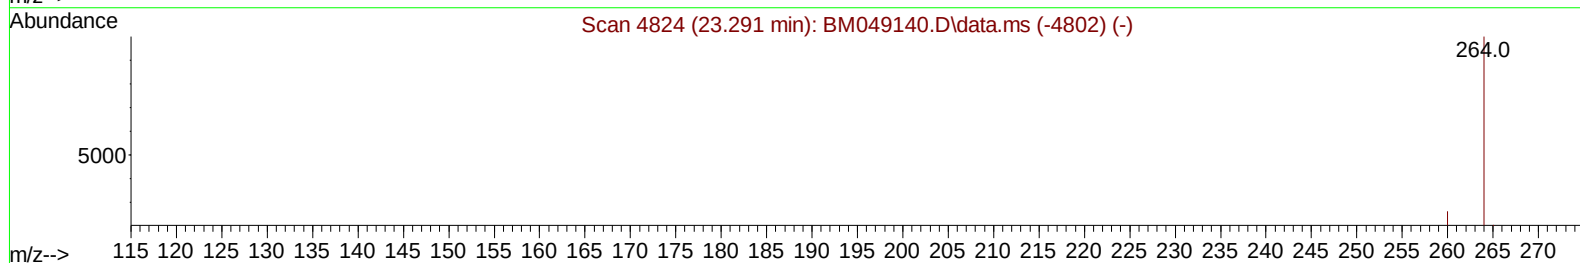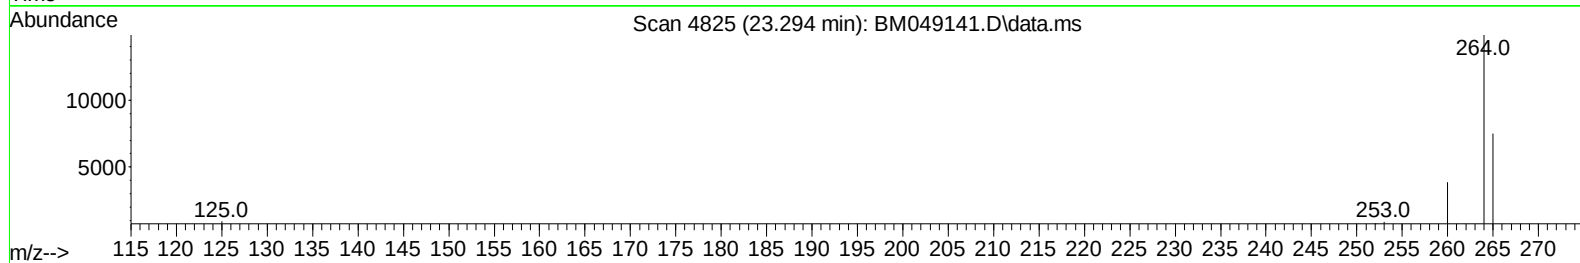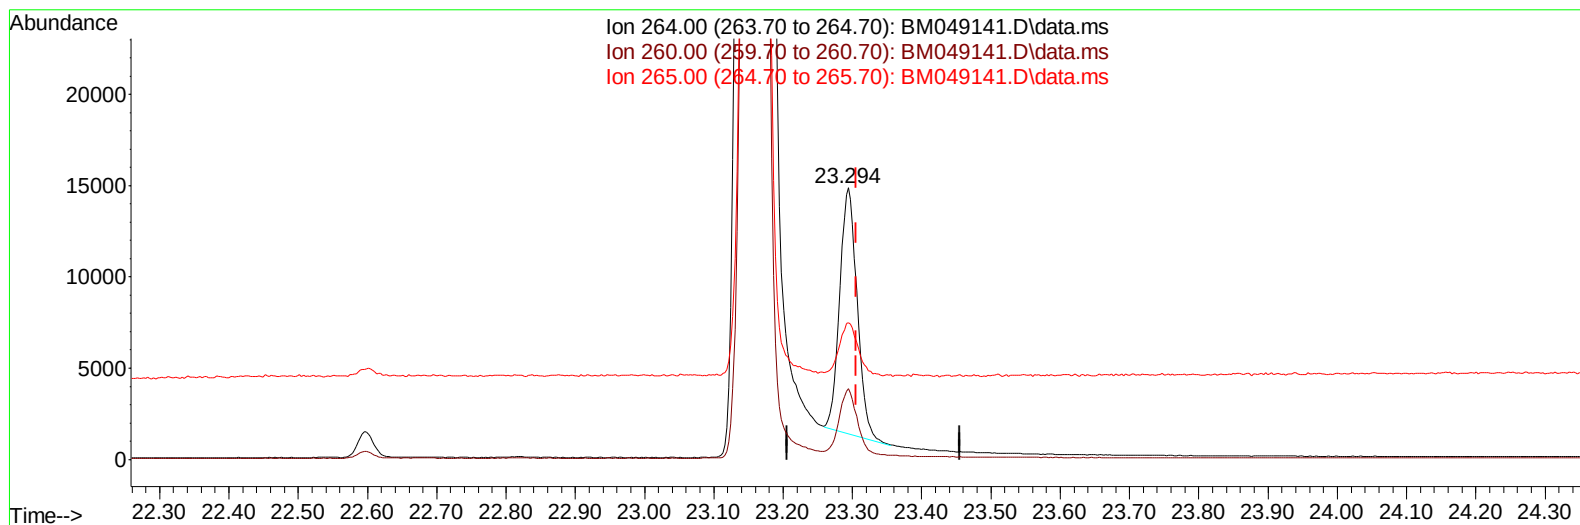

TIC: BM049141.D\data.ms

(23) Perylene-d12 (I)

23.294min (-0.012) 0.40 ng/ul m

response 23600

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.80	26.07
265.00	78.30	50.39#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
 Data File : BM049141.D
 Acq On : 23 Dec 2024 11:27
 Operator : RC/JU
 Sample : PB165769BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK769

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/24/2024
 Supervised By :mohammad ahmed 12/26/2024

Quant Time: Dec 23 11:56:21 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 18 15:33:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.552	152	8771	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.314	136	25083	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.191	164	13559	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.941	188	29152m	0.400	ng/ul	0.00
17) Chrysene-d12	21.140	240	22904m	0.400	ng/ul	0.00
23) Perylene-d12	23.294	264	23600m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.143	96	39264	3.882	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.919	152	6835	0.203	ng/ul	0.00
18) Fluoranthene-d10	18.977	212	13257	0.204	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049141.D
Acq On : 23 Dec 2024 11:27
Operator : RC/JU
Sample : PB165769BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK769

Manual IntegrationsAPPROVED

Quant Time: Dec 23 11:56:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

