




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049158.D
Acq On : 23 Dec 2024 22:43
Operator : RC/JU
Sample : PB165813BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK813

Manual IntegrationsAPPROVED

Quant Time: Dec 23 23:17:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

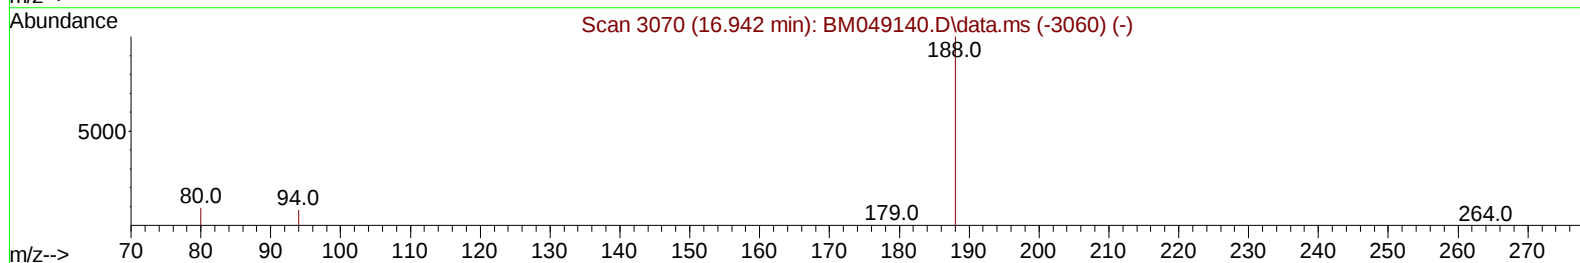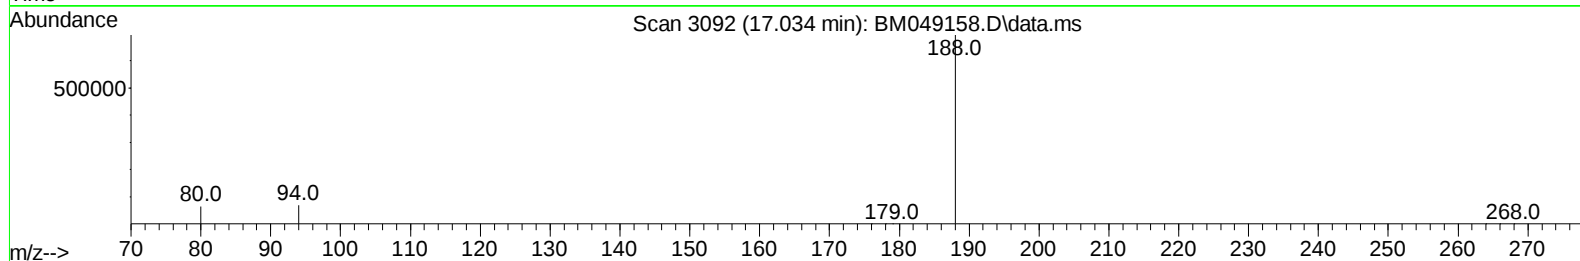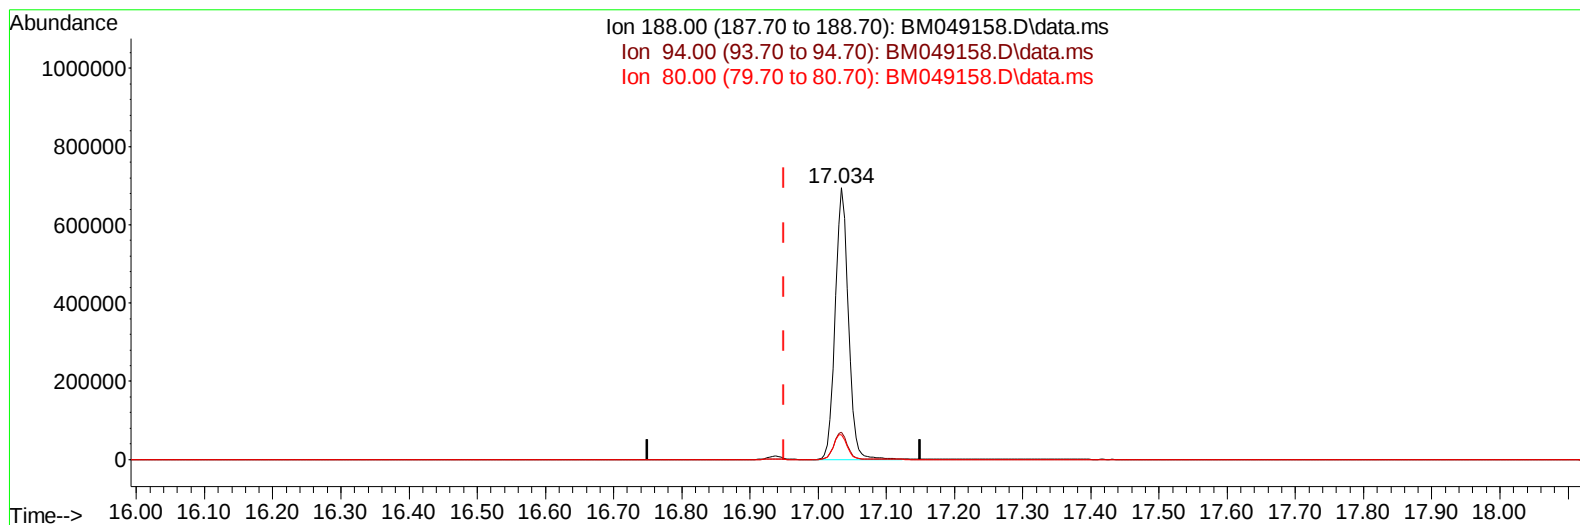

TIC: BM049158.D\data.ms

(13) Phenanthrene-d10 (I)

17.034min (+ 0.084) 0.40 ng/u1

response 930874

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	9.80	10.00
80.00	10.70	9.19
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049158.D
Acq On : 23 Dec 2024 22:43
Operator : RC/JU
Sample : PB165813BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK813

Manual IntegrationsAPPROVED

Quant Time: Dec 23 23:17:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

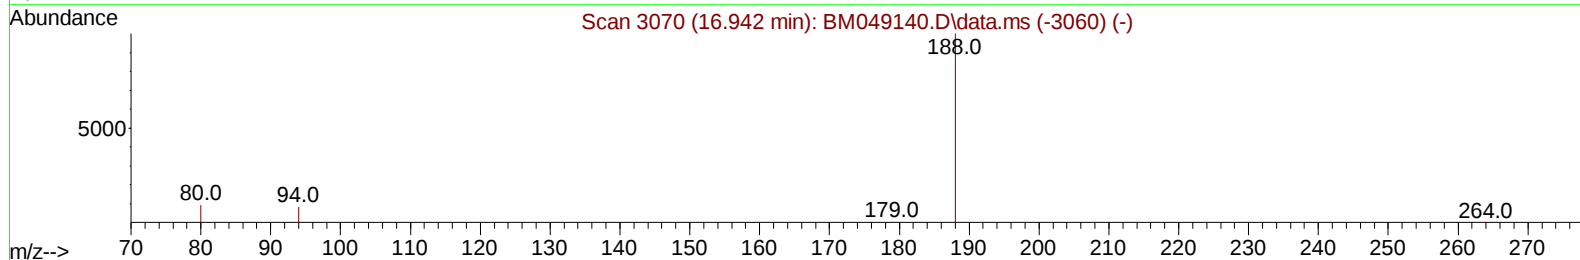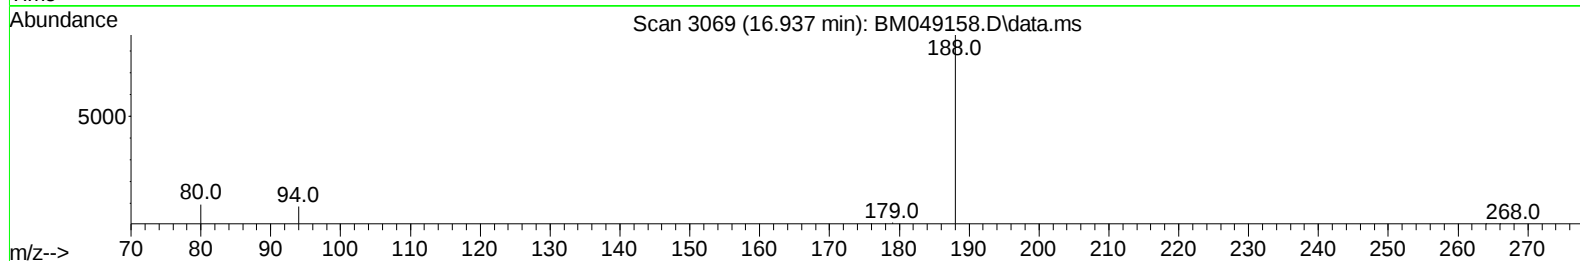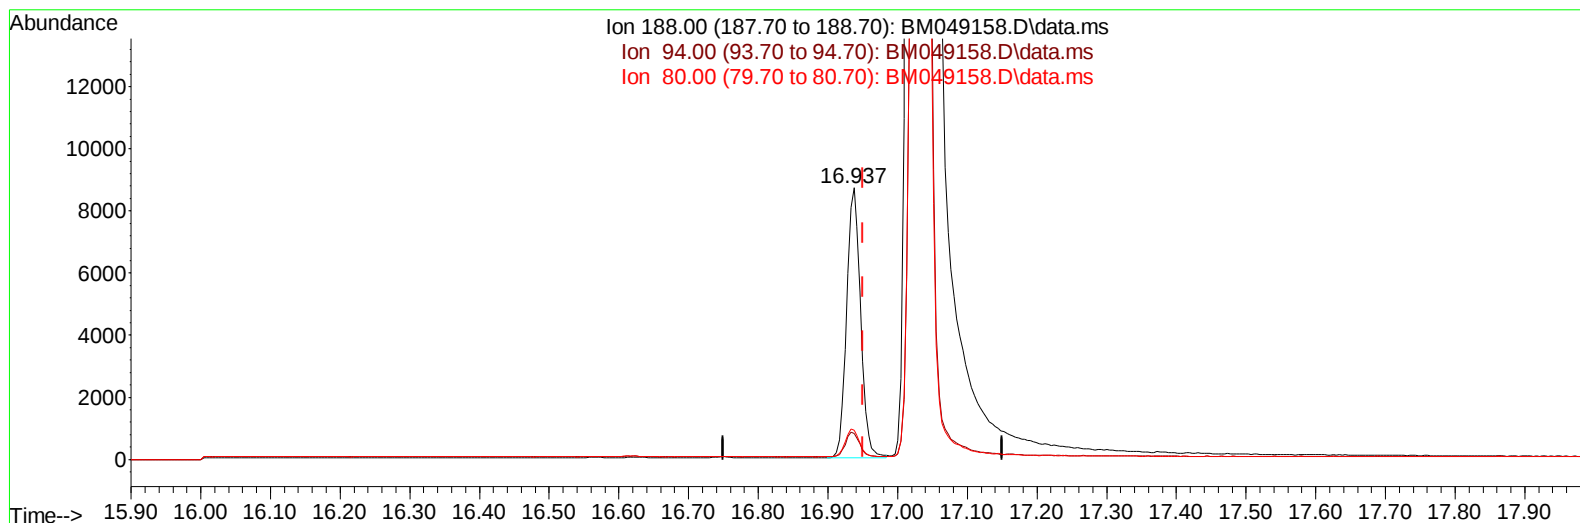

TIC: BM049158.D\data.ms

(13) Phenanthrene-d10 (I)

16.937min (-0.013) 0.40 ng/u1 m

response 12068

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	9.80	9.60
80.00	10.70	10.76
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049158.D
Acq On : 23 Dec 2024 22:43
Operator : RC/JU
Sample : PB165813BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK813

Manual IntegrationsAPPROVED

Quant Time: Dec 23 23:17:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

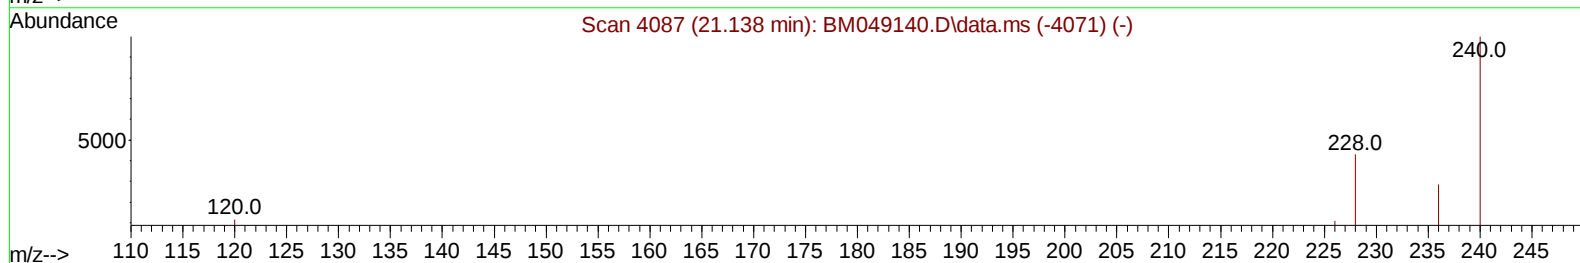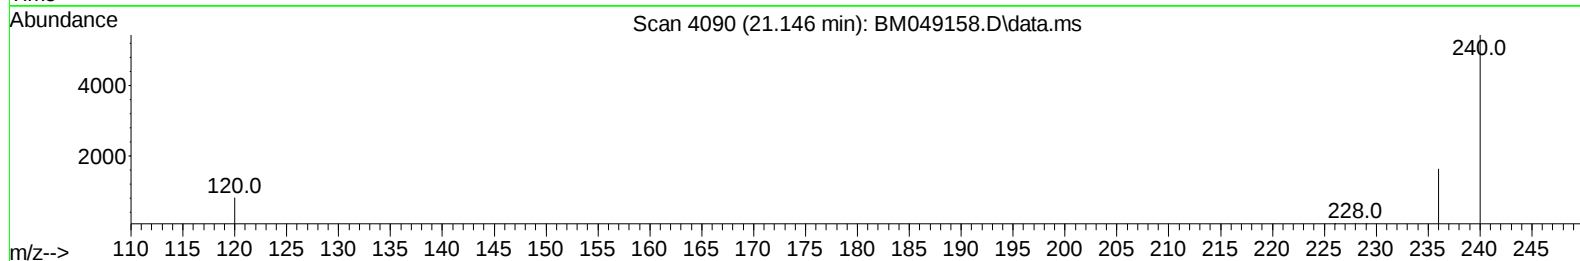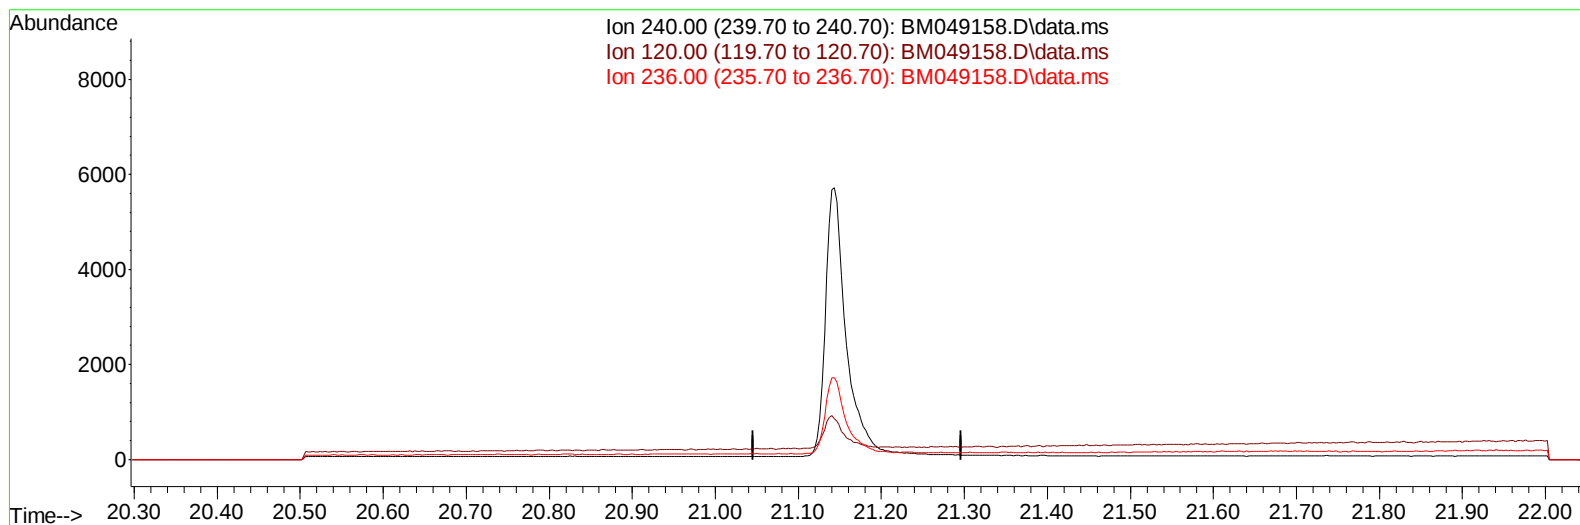

TIC: BM049158.D\data.ms

(17) Chrysene-d12

21.146min (-21.146) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	14.50	0.00#
236.00	29.80	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049158.D
Acq On : 23 Dec 2024 22:43
Operator : RC/JU
Sample : PB165813BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK813

Manual IntegrationsAPPROVED

Quant Time: Dec 23 23:17:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

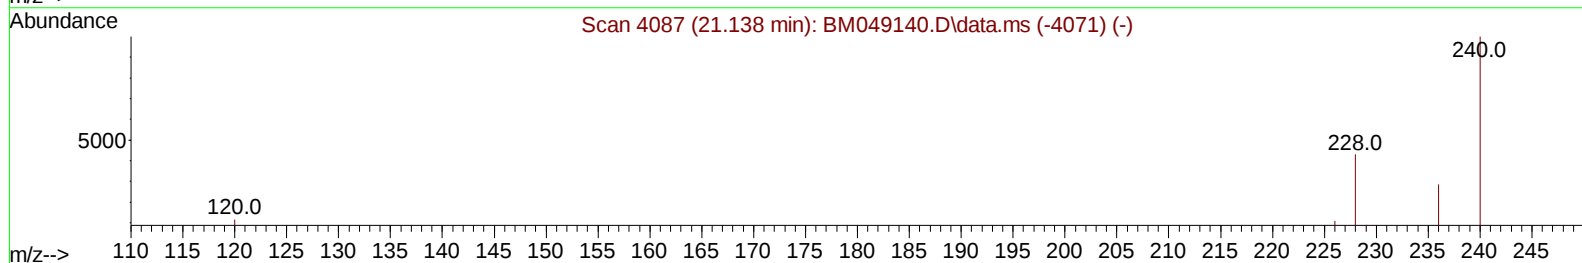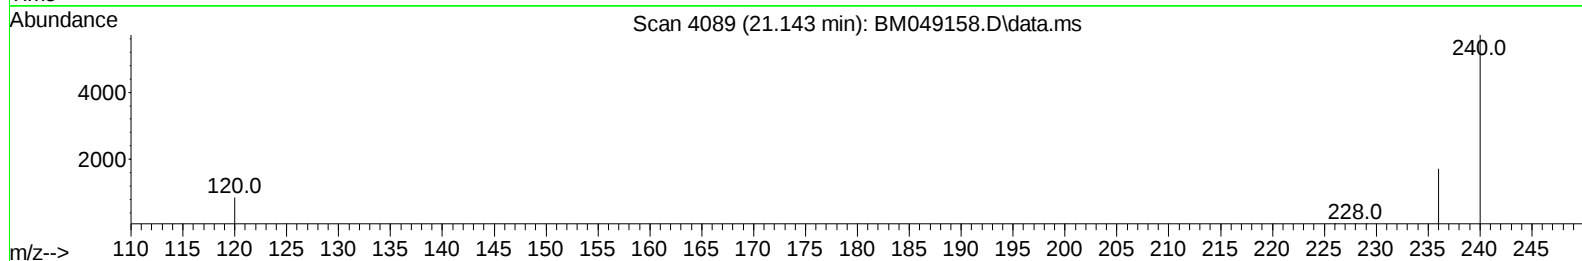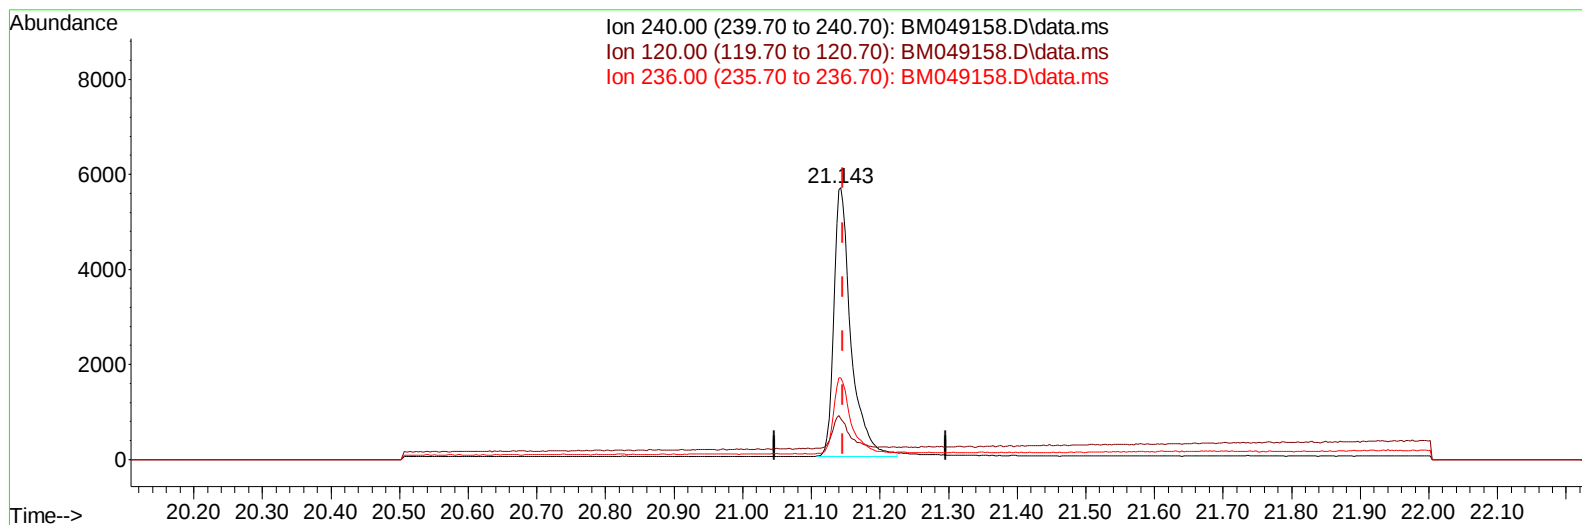

TIC: BM049158.D\data.ms

(17) Chrysene-d12

21.143min (-0.003) 0.40 ng/ul m

response 9840

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	14.50	14.91
236.00	29.80	30.19
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049158.D
Acq On : 23 Dec 2024 22:43
Operator : RC/JU
Sample : PB165813BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK813

Manual IntegrationsAPPROVED

Quant Time: Dec 23 23:17:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

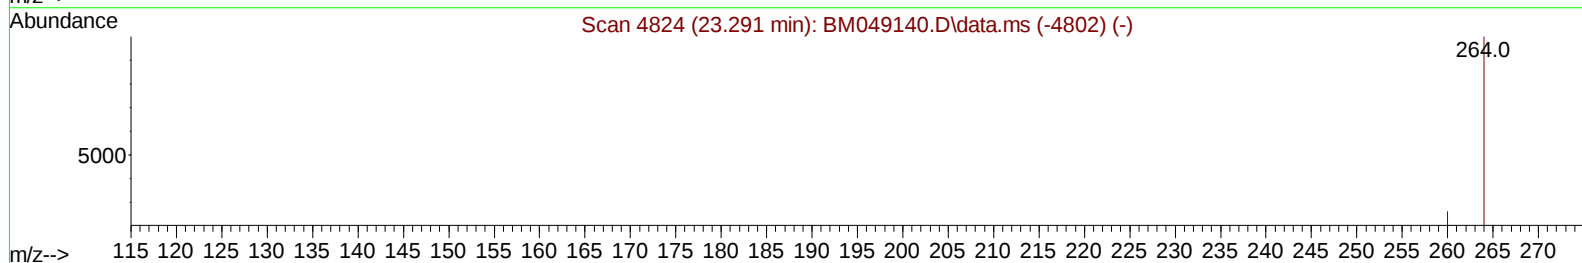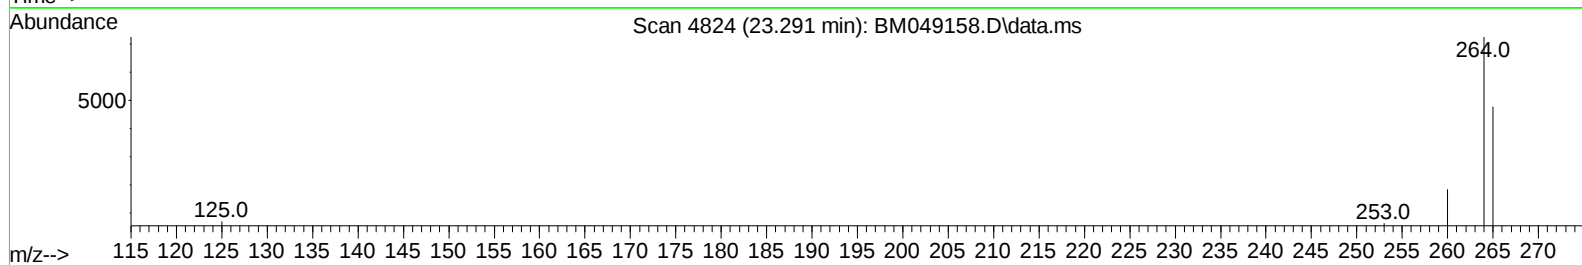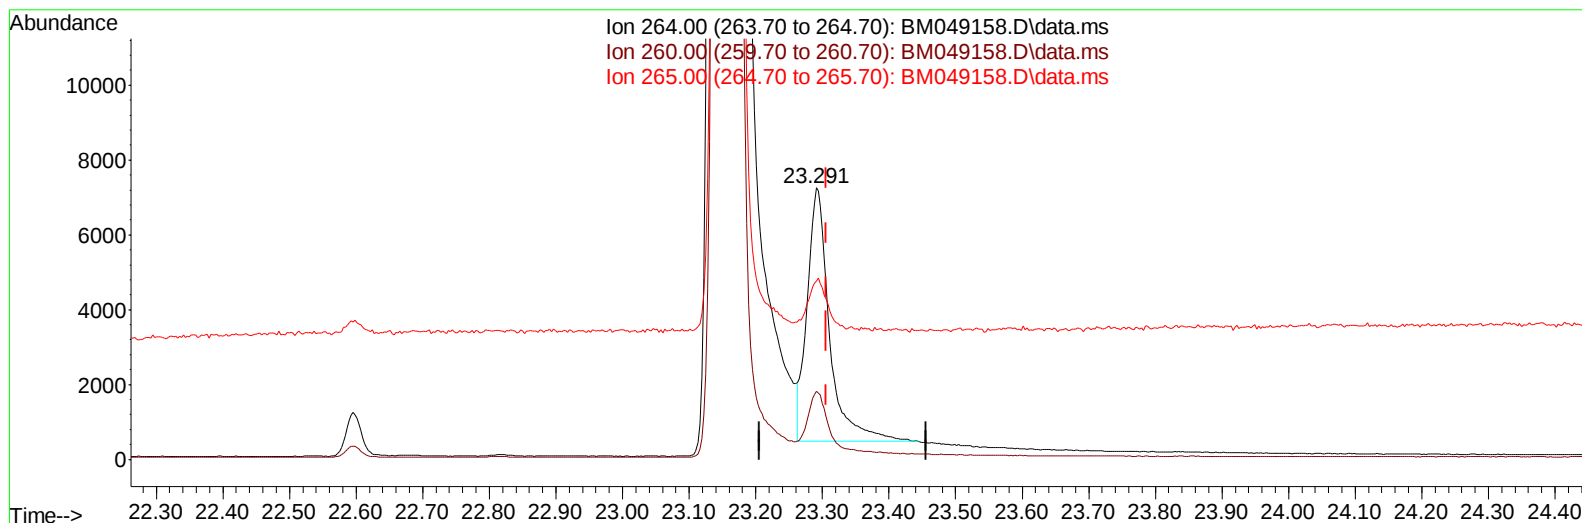

TIC: BM049158.D\data.ms

(23) Perylene-d12 (I)

23.291min (-0.015) 0.40 ng/u1

response 15997

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.80	25.17
265.00	78.30	65.72
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049158.D
Acq On : 23 Dec 2024 22:43
Operator : RC/JU
Sample : PB165813BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK813

Manual IntegrationsAPPROVED

Quant Time: Dec 23 23:17:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

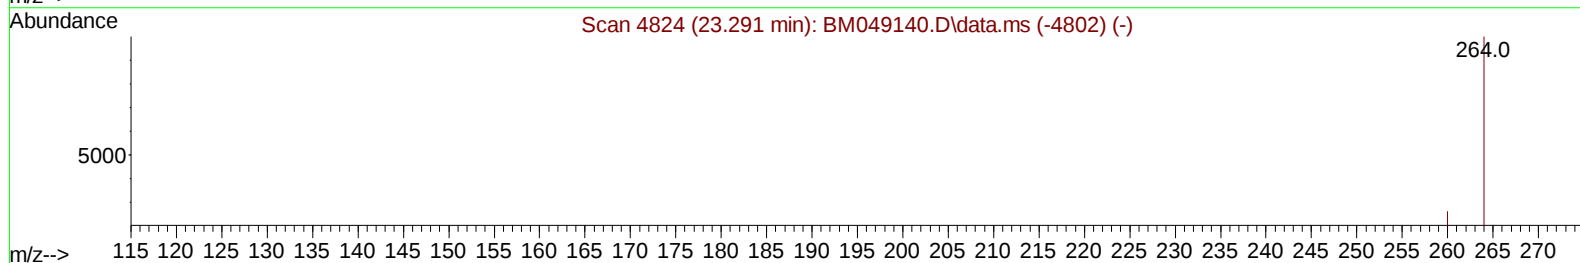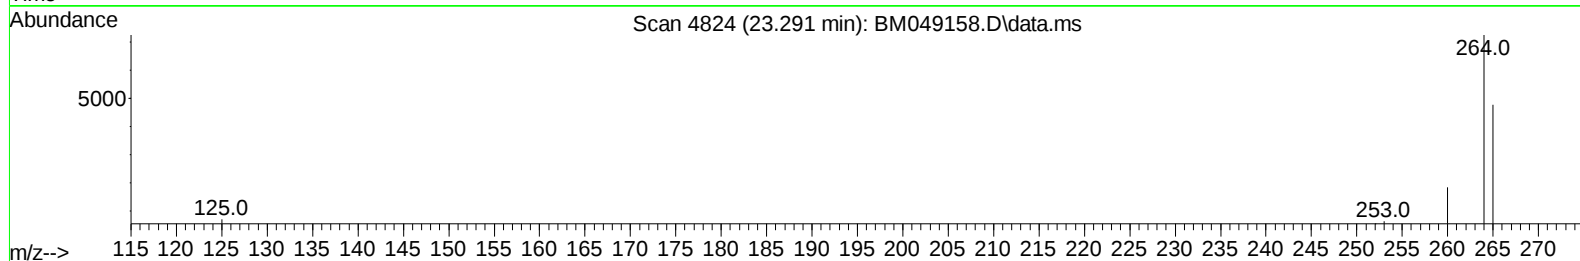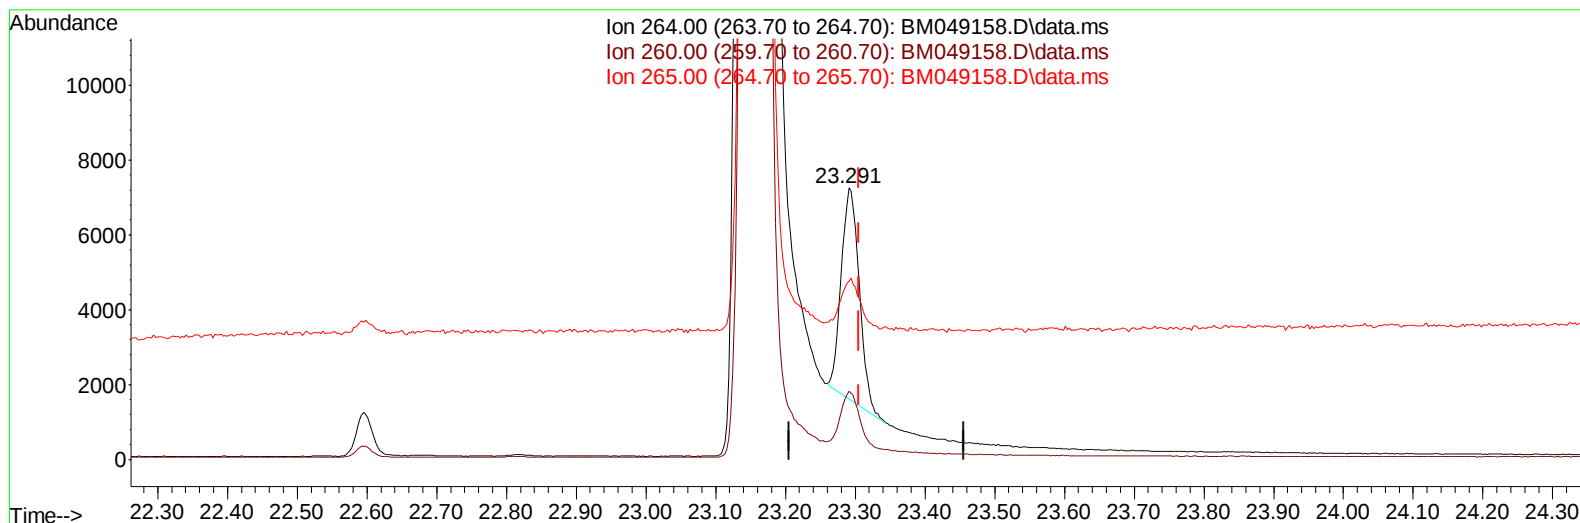

TIC: BM049158.D\data.ms

(23) Perylene-d12 (I)

23.291min (-0.015) 0.40 ng/ul m

response 10102

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.80	25.17
265.00	78.30	65.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
 Data File : BM049158.D
 Acq On : 23 Dec 2024 22:43
 Operator : RC/JU
 Sample : PB165813BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK813

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/24/2024
 Supervised By :mohammad ahmed 12/26/2024

Quant Time: Dec 23 23:17:02 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 18 15:33:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.552	152	3632	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.314	136	10154	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.191	164	5482	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.937	188	12068m	0.400	ng/ul	-0.01
17) Chrysene-d12	21.143	240	9840m	0.400	ng/ul	0.00
23) Perylene-d12	23.291	264	10102m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.138	96	28058	6.698	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.925	152	4508	0.330	ng/ul	0.00
18) Fluoranthene-d10	18.973	212	9767	0.350	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049158.D
Acq On : 23 Dec 2024 22:43
Operator : RC/JU
Sample : PB165813BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK813

Manual IntegrationsAPPROVED

Quant Time: Dec 23 23:17:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

