




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049163.D
Acq On : 24 Dec 2024 01:41
Operator : RC/JU
Sample : P5302-08
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2AR8

Manual IntegrationsAPPROVED

Quant Time: Dec 24 02:06:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

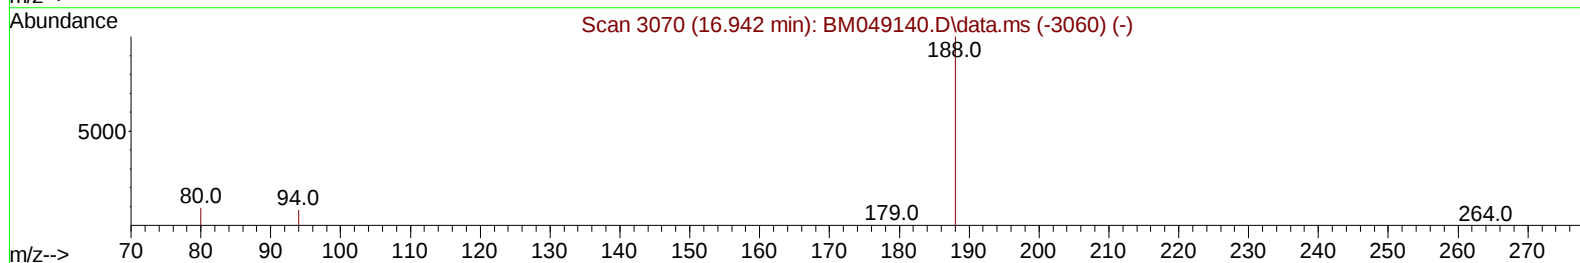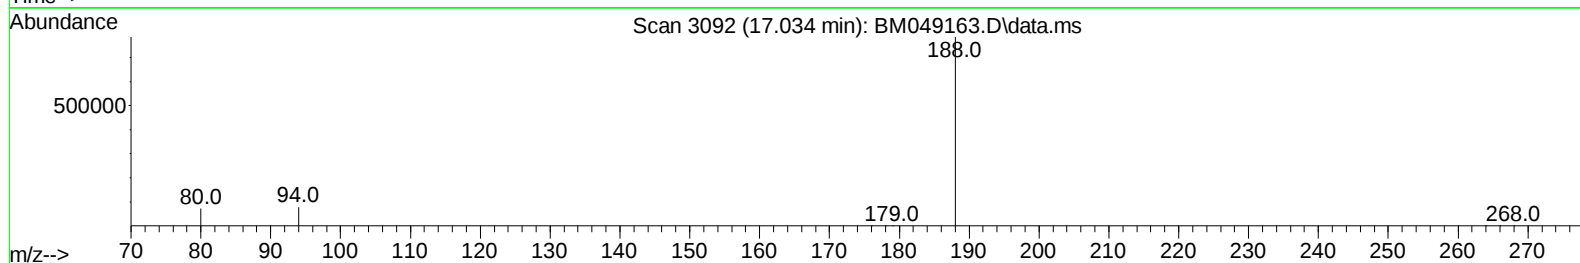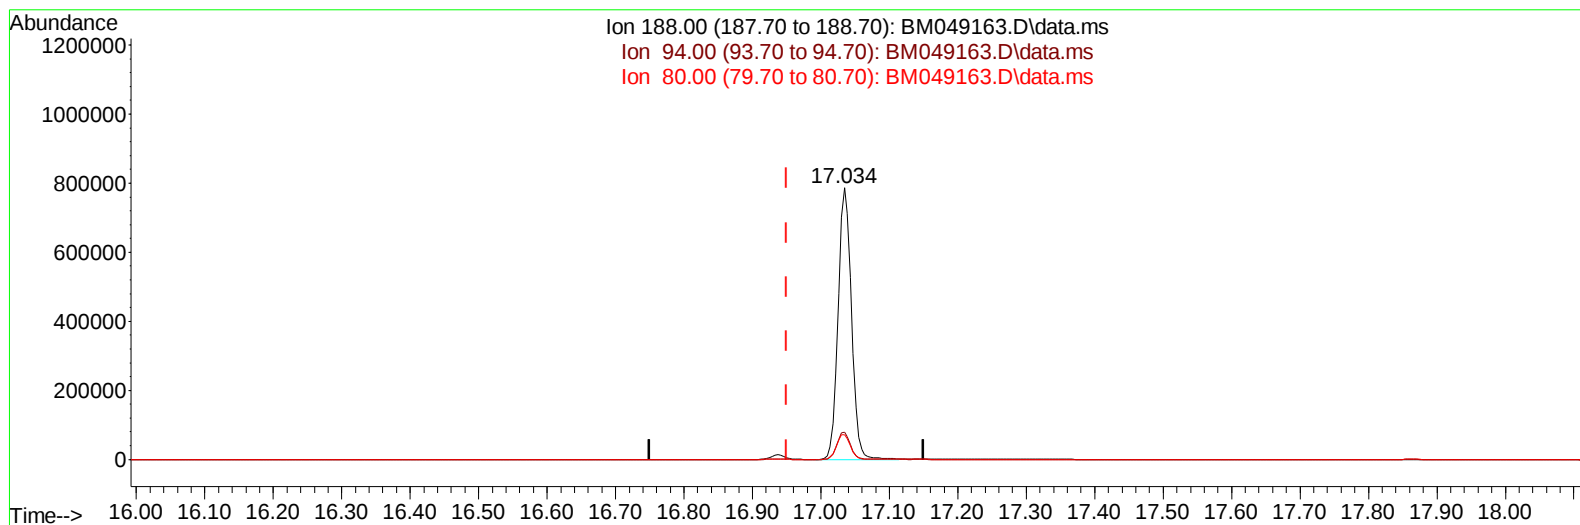

TIC: BM049163.D\data.ms

(13) Phenanthrene-d10 (I)

17.034min (+ 0.084) 0.40 ng/u1

response 1068592

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	9.80	9.95
80.00	10.70	9.12
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049163.D
Acq On : 24 Dec 2024 01:41
Operator : RC/JU
Sample : P5302-08
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2AR8

Manual IntegrationsAPPROVED

Quant Time: Dec 24 02:06:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

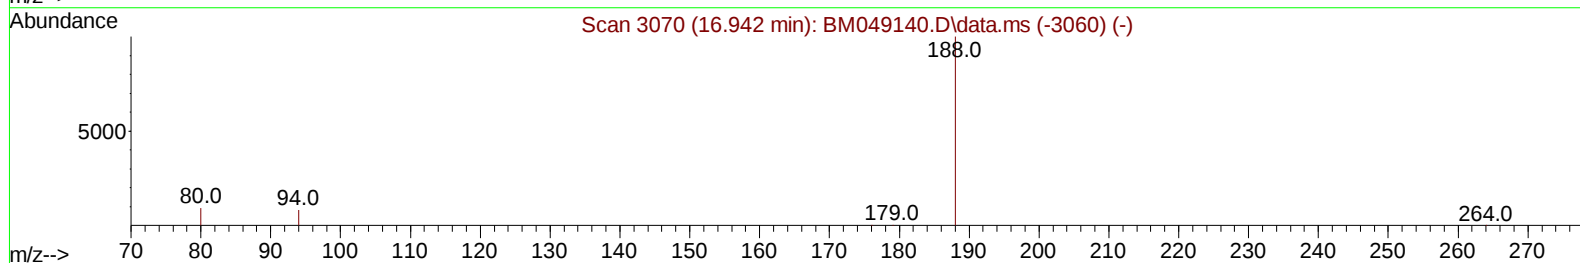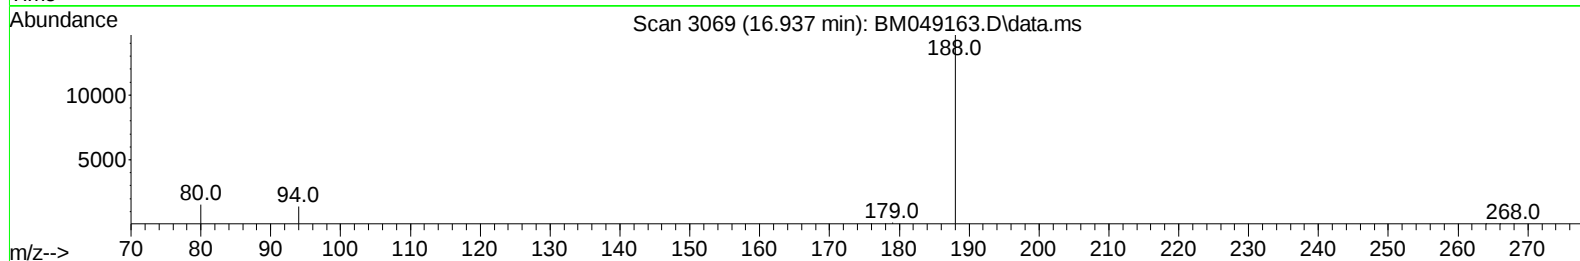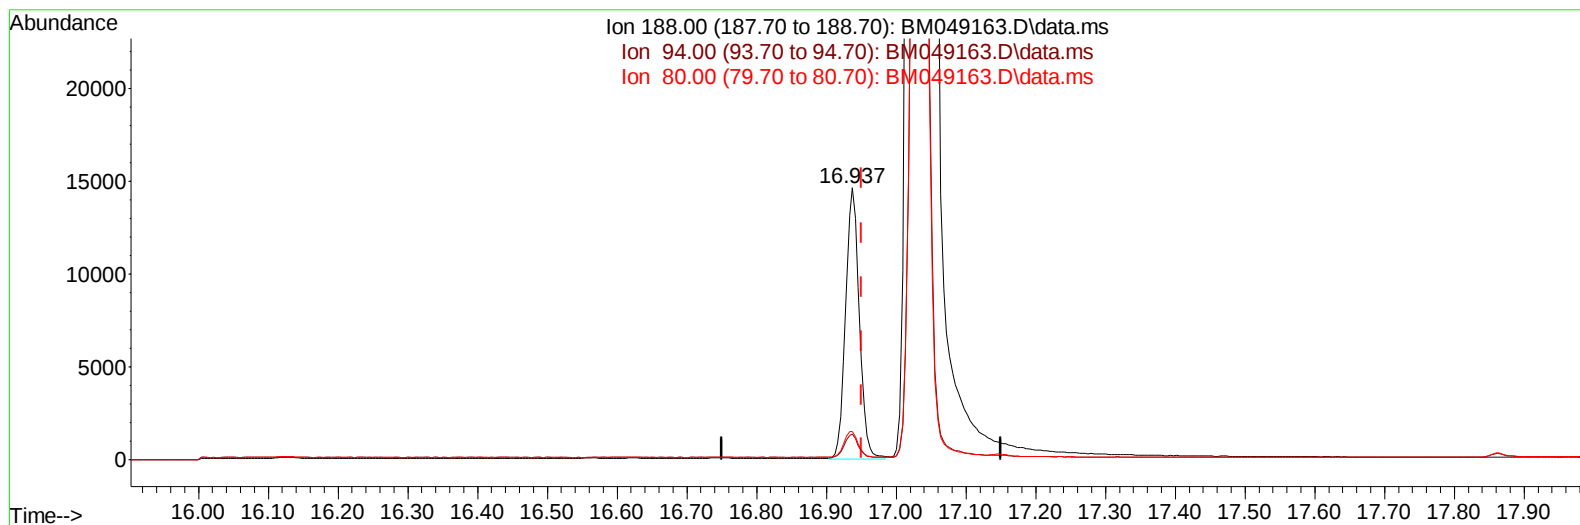

TIC: BM049163.D\data.ms

(13) Phenanthrene-d10 (I)

16.937min (-0.013) 0.40 ng/ul m

response 20048

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	9.80	9.40
80.00	10.70	10.39
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049163.D
Acq On : 24 Dec 2024 01:41
Operator : RC/JU
Sample : P5302-08
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2AR8

Manual IntegrationsAPPROVED

Quant Time: Dec 24 02:06:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

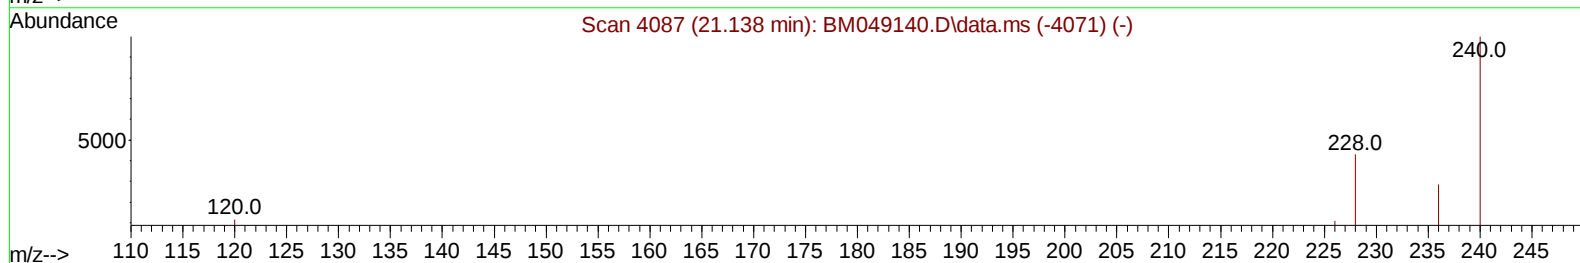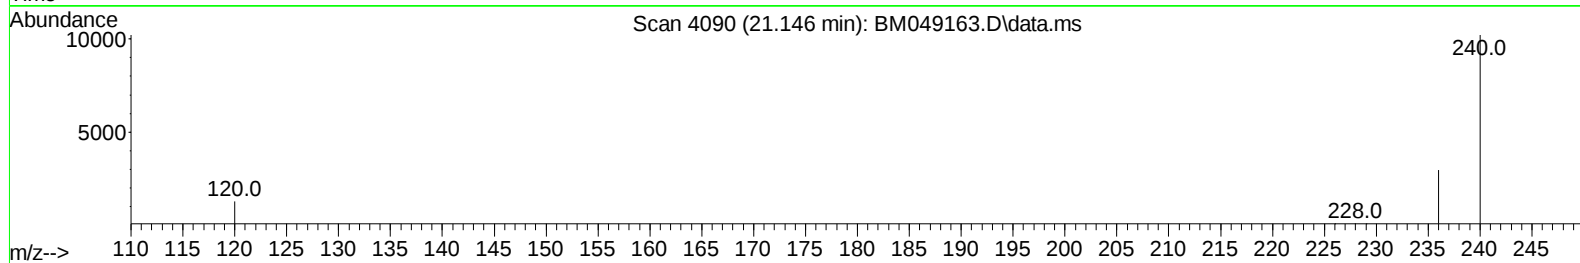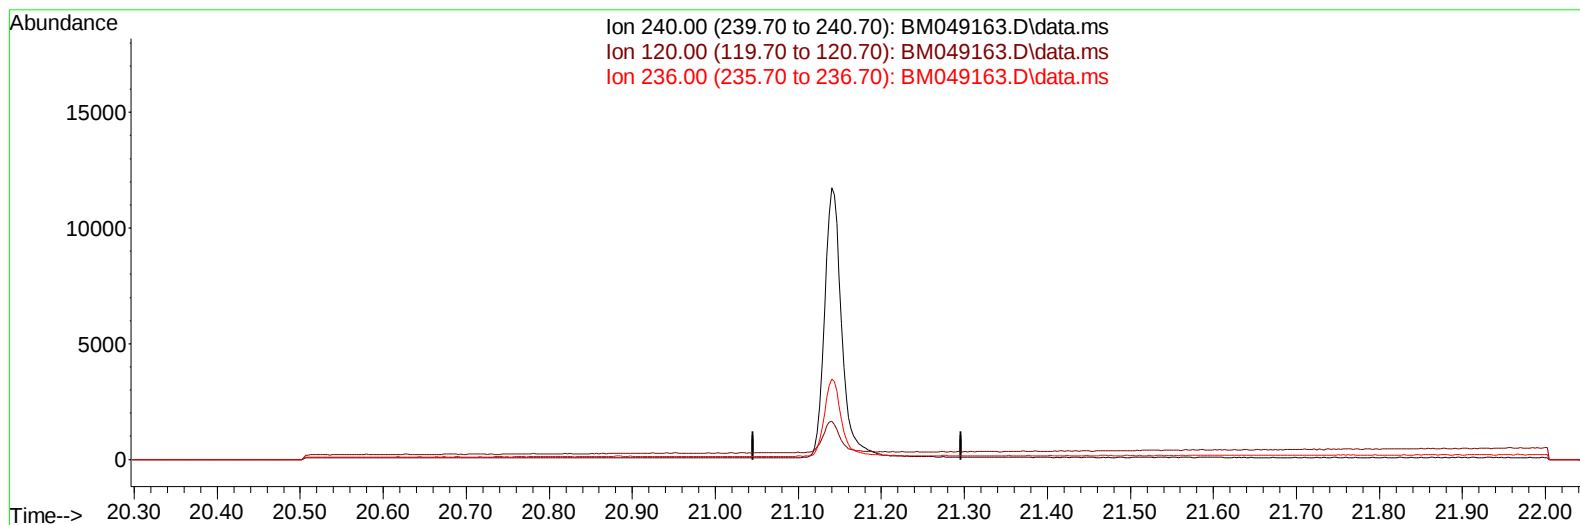

TIC: BM049163.D\data.ms

(17) Chrysene-d12

21.146min (-21.146) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	14.50	0.00#
236.00	29.80	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049163.D
Acq On : 24 Dec 2024 01:41
Operator : RC/JU
Sample : P5302-08
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2AR8

Manual IntegrationsAPPROVED

Quant Time: Dec 24 02:06:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

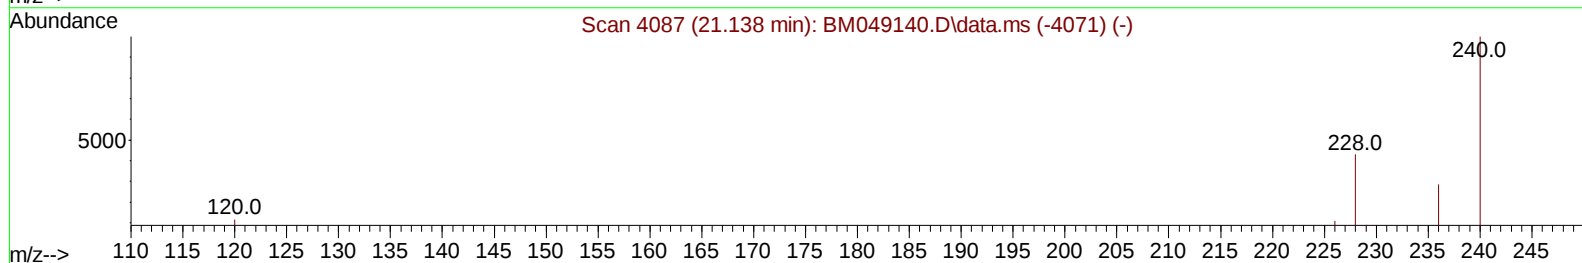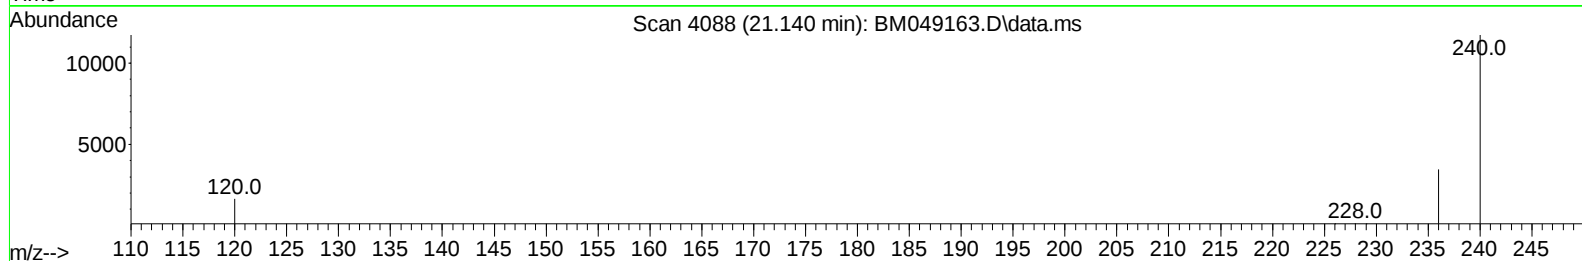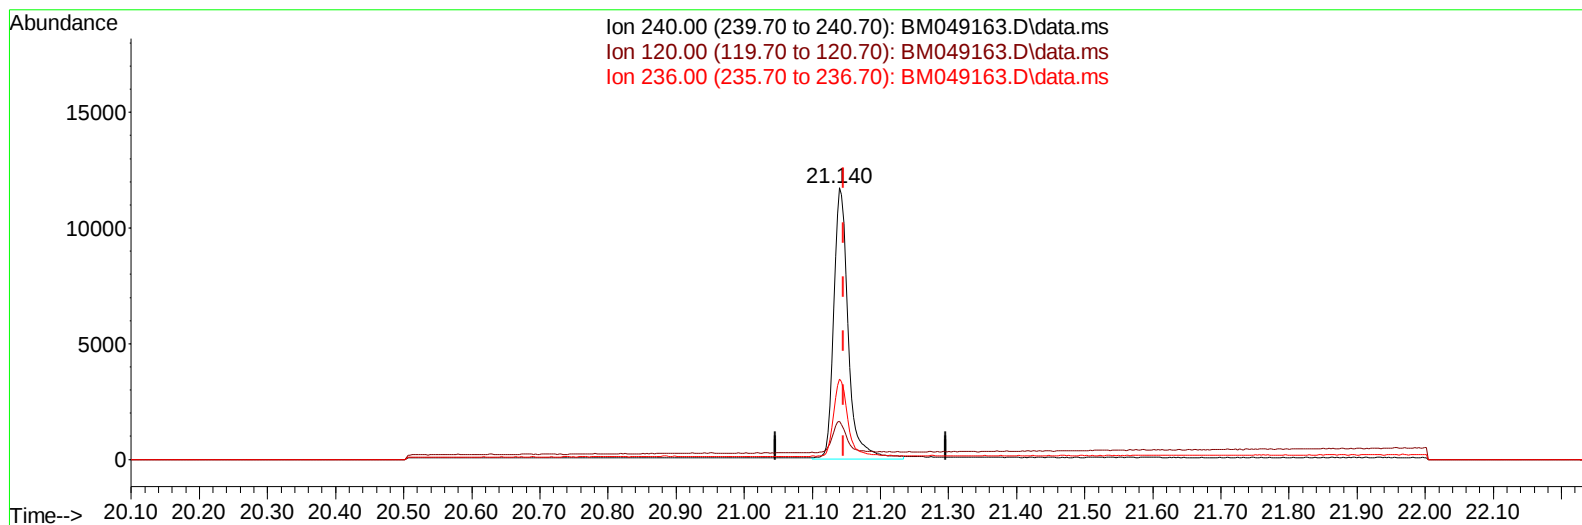

TIC: BM049163.D\data.ms

(17) Chrysene-d12

21.140min (-0.006) 0.40 ng/u1 m

response 17333

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	14.50	14.04
236.00	29.80	29.61
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049163.D
Acq On : 24 Dec 2024 01:41
Operator : RC/JU
Sample : P5302-08
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2AR8

Manual IntegrationsAPPROVED

Quant Time: Dec 24 02:06:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

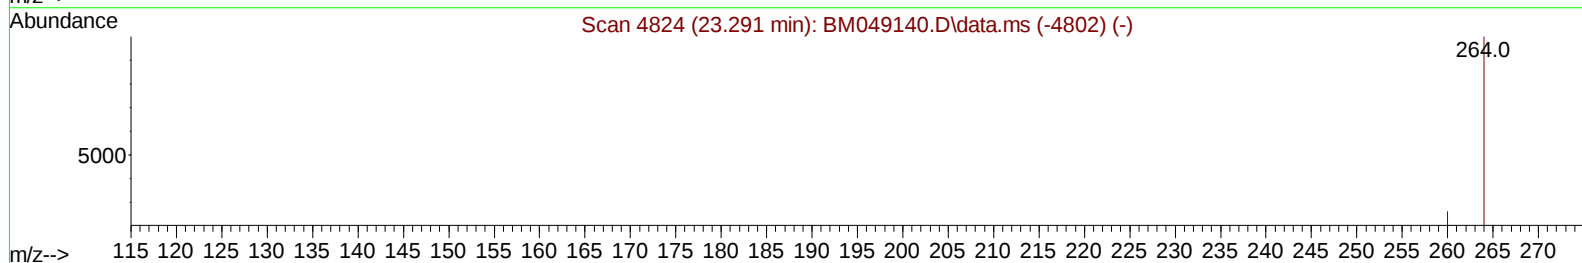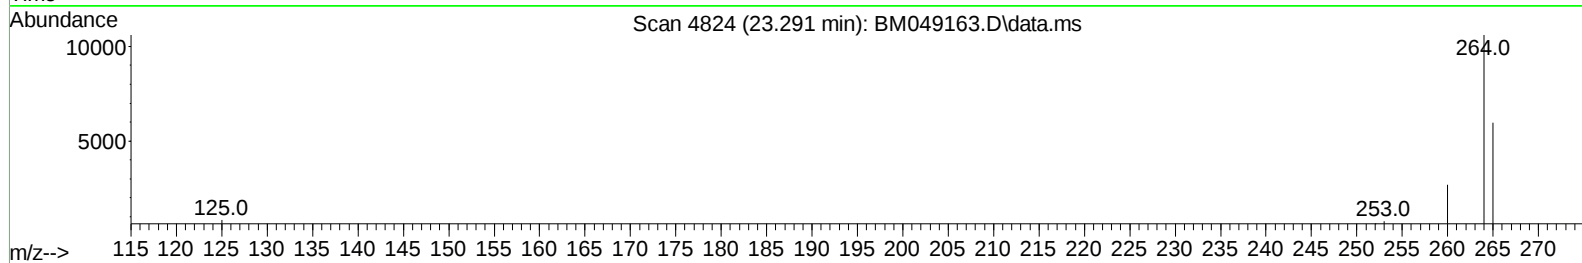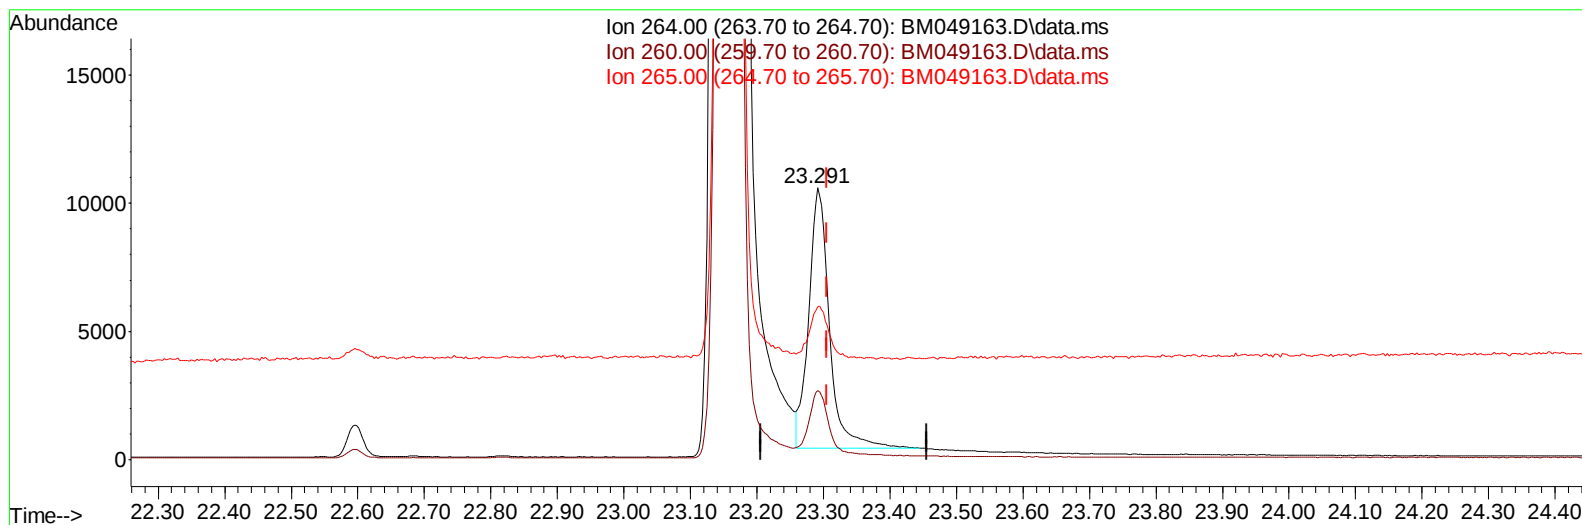

TIC: BM049163.D\data.ms

(23) Perylene-d12 (I)

23.291min (-0.015) 0.40 ng/u1

response 22026

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.80	25.45
265.00	78.30	56.23#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049163.D
Acq On : 24 Dec 2024 01:41
Operator : RC/JU
Sample : P5302-08
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2AR8

Manual IntegrationsAPPROVED

Quant Time: Dec 24 02:06:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

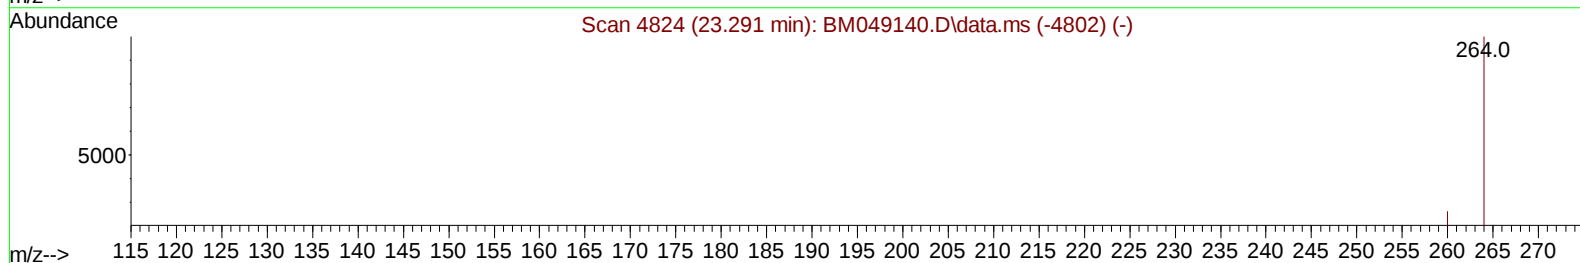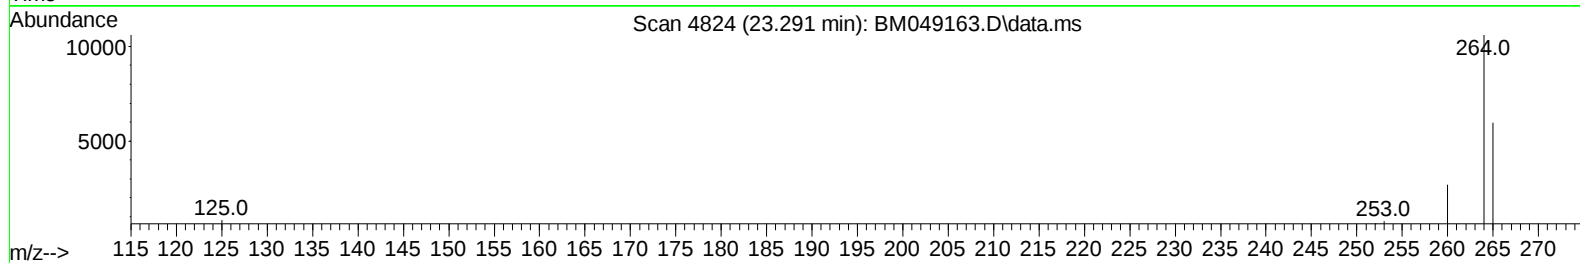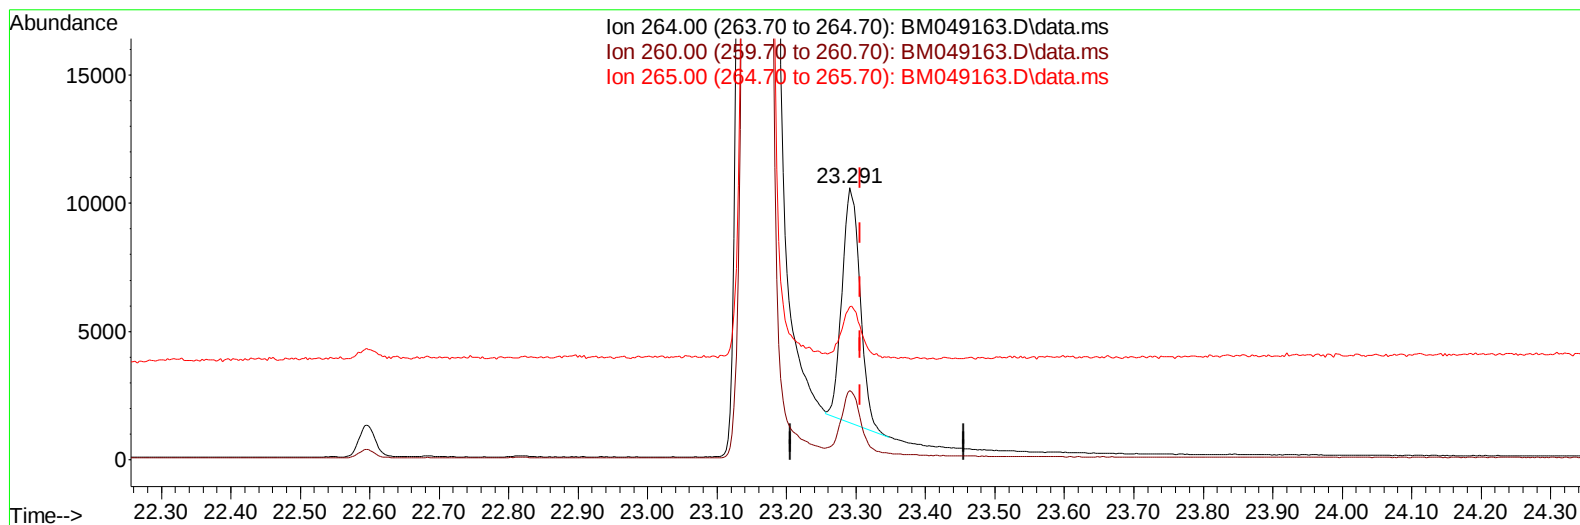

TIC: BM049163.D\data.ms

(23) Perylene-d12 (I)

23.291min (-0.015) 0.40 ng/ul m

response 16633

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.80	25.45
265.00	78.30	56.23#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
 Data File : BM049163.D
 Acq On : 24 Dec 2024 01:41
 Operator : RC/JU
 Sample : P5302-08
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E2AR8

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/24/2024
 Supervised By :mohammad ahmed 12/26/2024

Quant Time: Dec 24 02:06:57 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 18 15:33:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.552	152	5601	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.314	136	16423	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.186	164	9103	0.400	ng/ul	-0.01
13) Phenanthrene-d10	16.937	188	20048m	0.400	ng/ul	-0.01
17) Chrysene-d12	21.140	240	17333m	0.400	ng/ul	0.00
23) Perylene-d12	23.291	264	16633m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.143	96	18611	2.881	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.914	152	4940	0.224	ng/ul	-0.01
18) Fluoranthene-d10	18.973	212	11861	0.241	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049163.D
Acq On : 24 Dec 2024 01:41
Operator : RC/JU
Sample : P5302-08
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2AR8

Manual IntegrationsAPPROVED

Quant Time: Dec 24 02:06:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

