




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049193.D
Acq On : 24 Dec 2024 20:40
Operator : RC/JU
Sample : P5353-03
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2928

Manual IntegrationsAPPROVED

Quant Time: Dec 24 21:42:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/25/2024
Supervised By :mohammad ahmed 12/26/2024

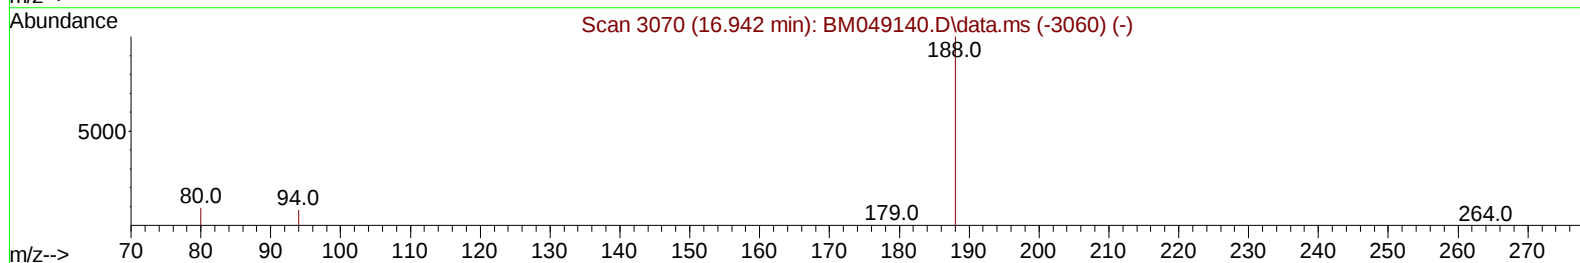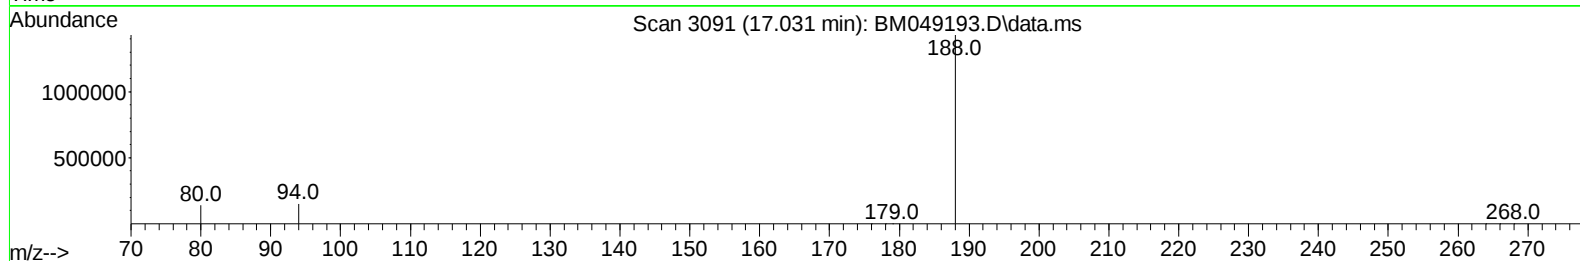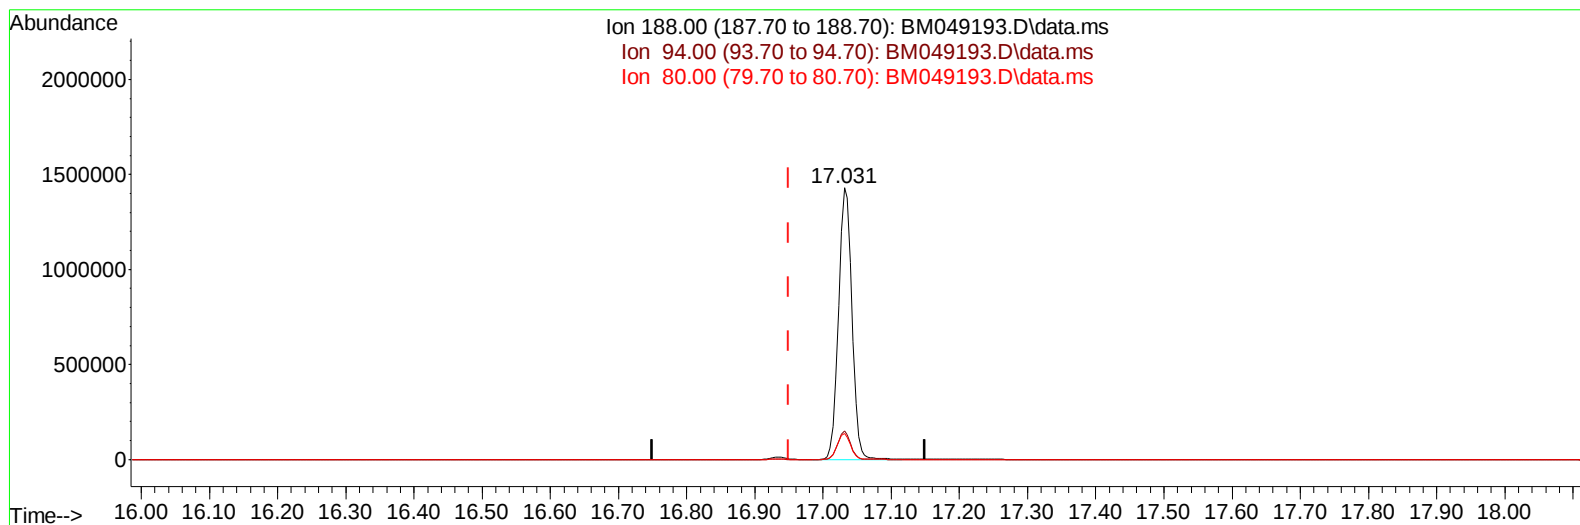

TIC: BM049193.D\data.ms

(13) Phenanthrene-d10 (I)

17.031min (+ 0.081) 0.40 ng/u1

response 1949335

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	9.80	10.45
80.00	10.70	9.68
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049193.D
Acq On : 24 Dec 2024 20:40
Operator : RC/JU
Sample : P5353-03
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2928

Manual IntegrationsAPPROVED

Quant Time: Dec 24 21:42:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/25/2024
Supervised By :mohammad ahmed 12/26/2024

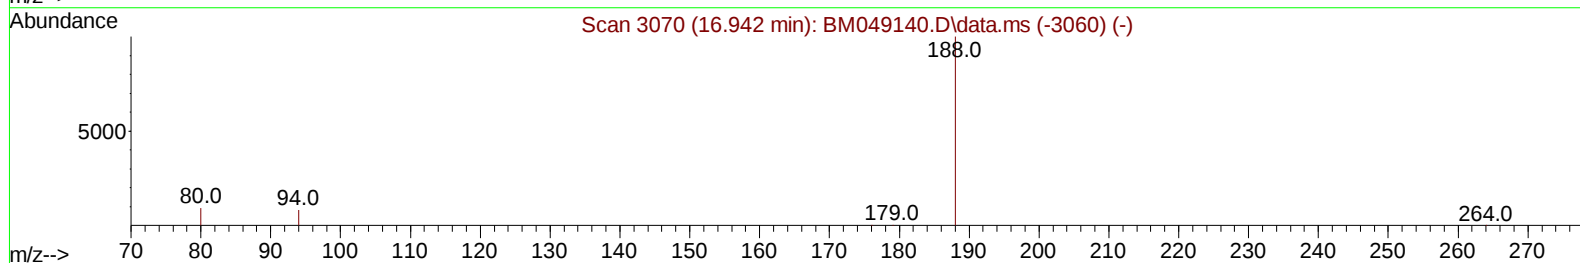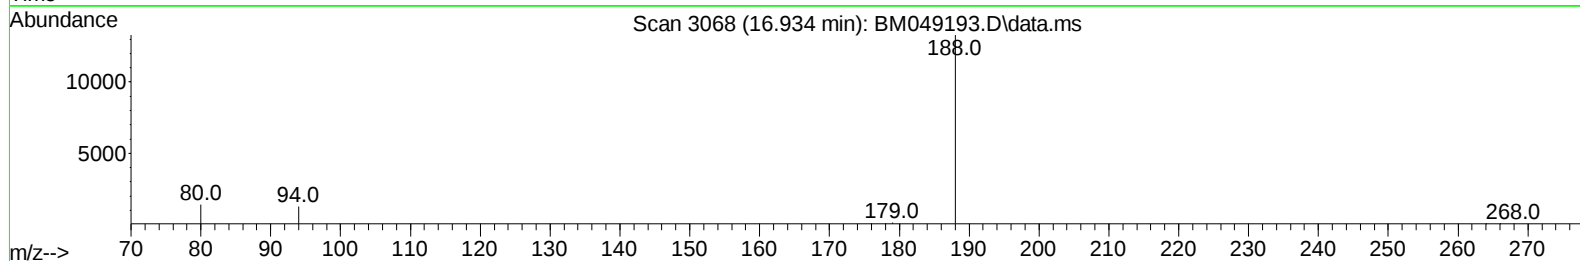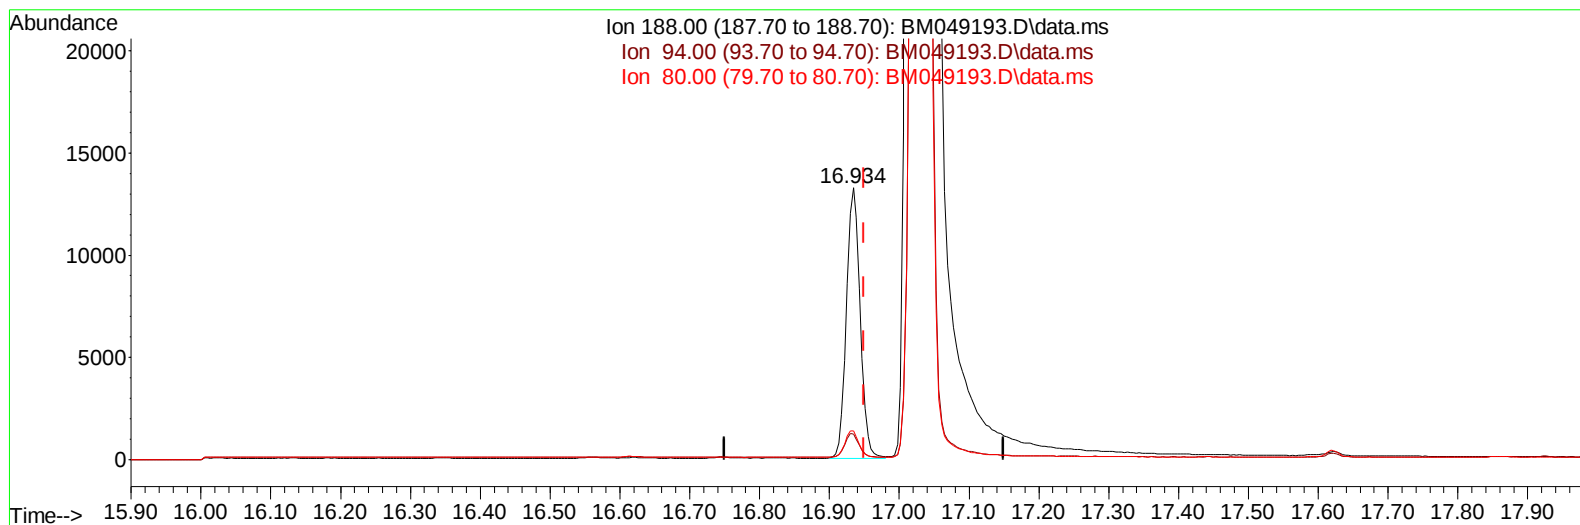

TIC: BM049193.D\data.ms

(13) Phenanthrene-d10 (I)

16.934min (-0.016) 0.40 ng/ul m

response 18176

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	9.80	9.36
80.00	10.70	10.42
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049193.D
Acq On : 24 Dec 2024 20:40
Operator : RC/JU
Sample : P5353-03
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2928

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/25/2024
Supervised By :mohammad ahmed 12/26/2024

Quant Time: Dec 24 21:42:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

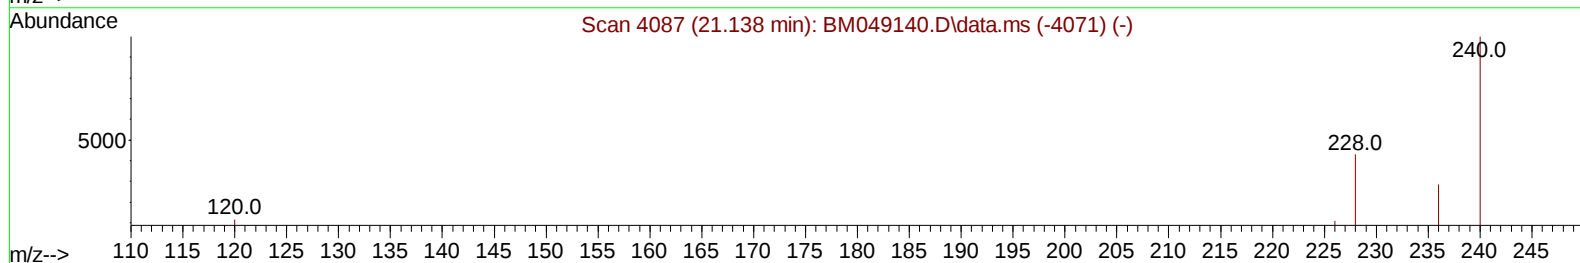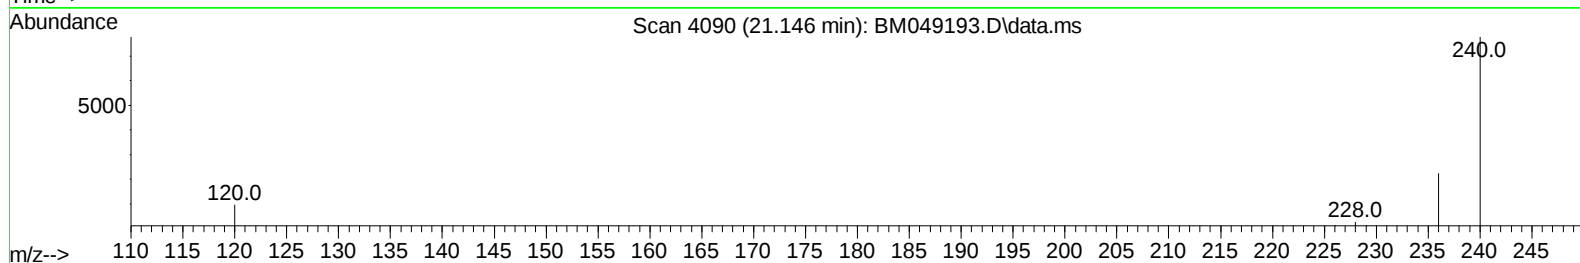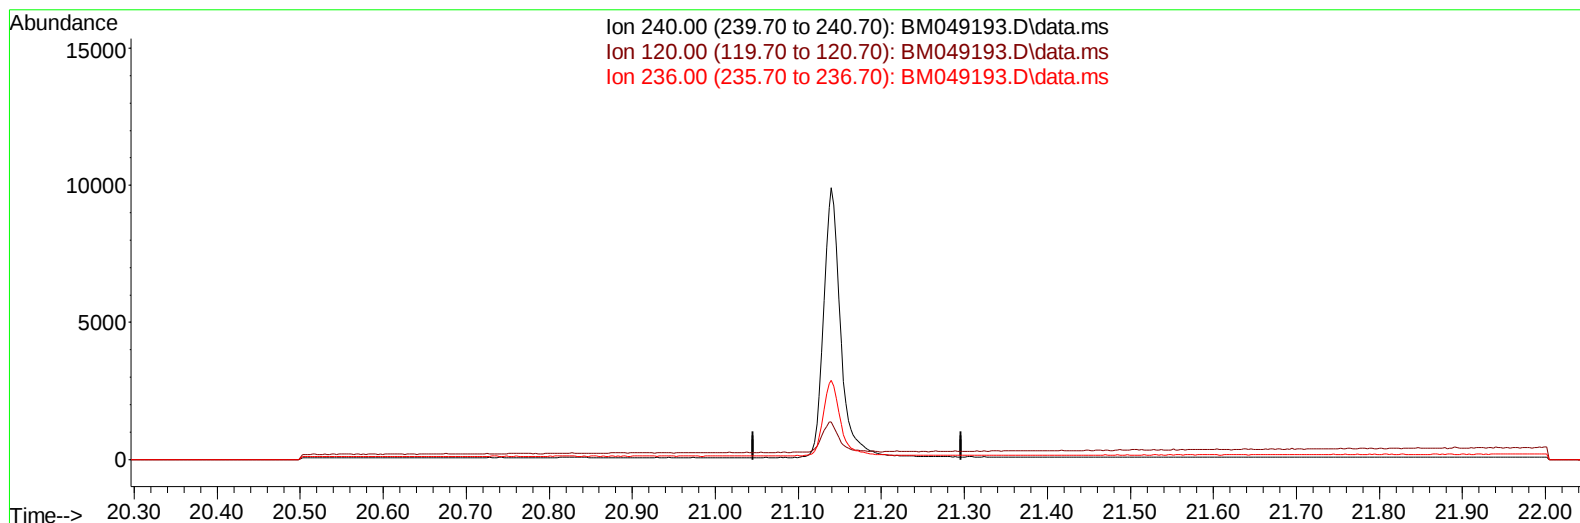

TIC: BM049193.D\data.ms

(17) Chrysene-d12

21.146min (-21.146) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	14.50	0.00#
236.00	29.80	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049193.D
Acq On : 24 Dec 2024 20:40
Operator : RC/JU
Sample : P5353-03
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2928

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/25/2024
Supervised By :mohammad ahmed 12/26/2024

Quant Time: Dec 24 21:42:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

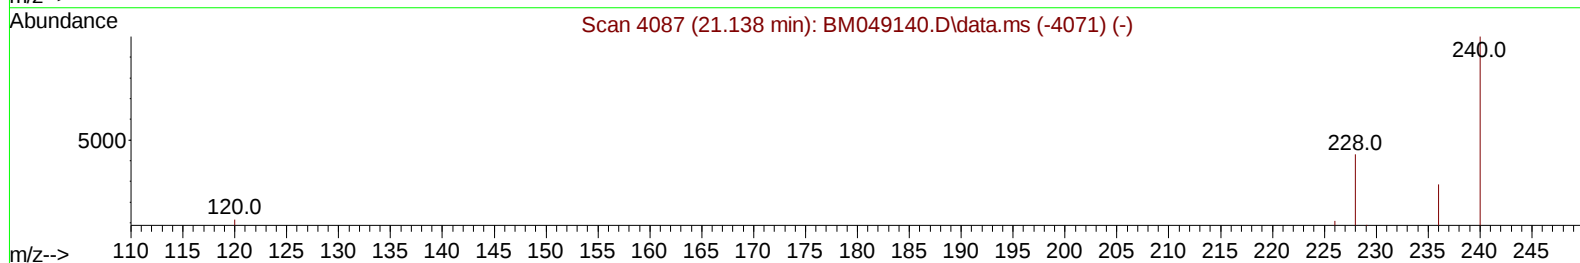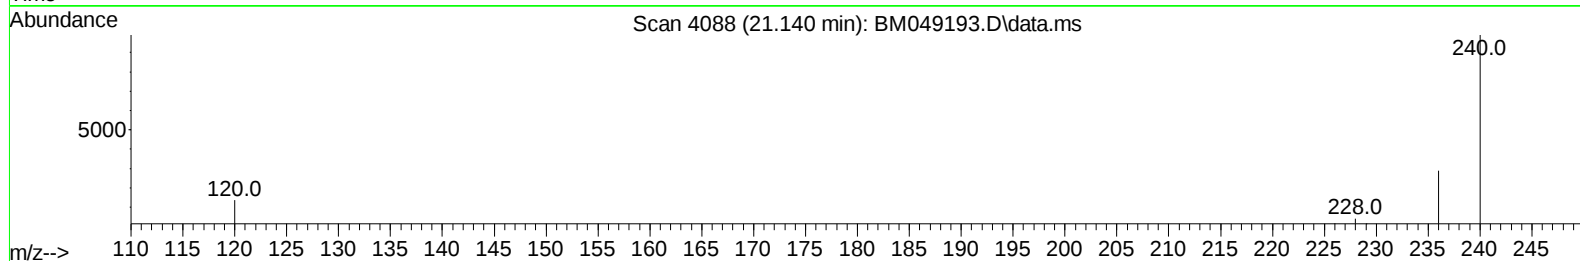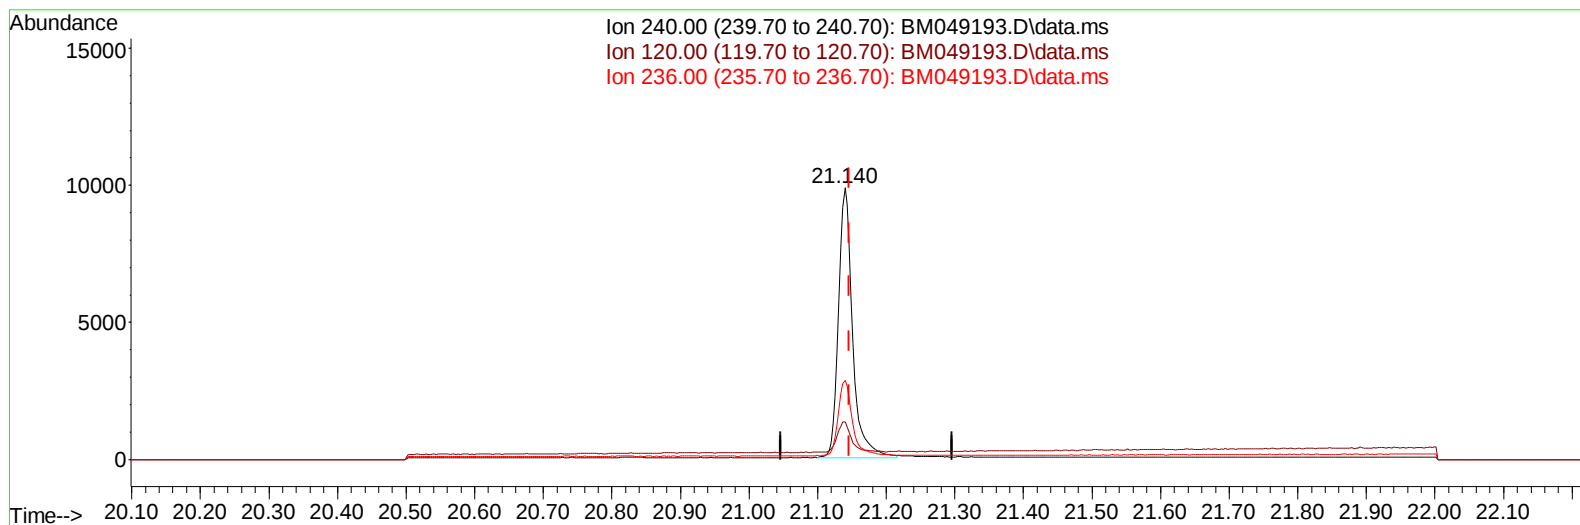

TIC: BM049193.D\data.ms

(17) Chrysene-d12

21.140min (-0.006) 0.40 ng/ul m

response 14041

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	14.50	13.75
236.00	29.80	29.11
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049193.D
Acq On : 24 Dec 2024 20:40
Operator : RC/JU
Sample : P5353-03
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2928

Manual IntegrationsAPPROVED

Quant Time: Dec 24 21:42:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/25/2024
Supervised By :mohammad ahmed 12/26/2024

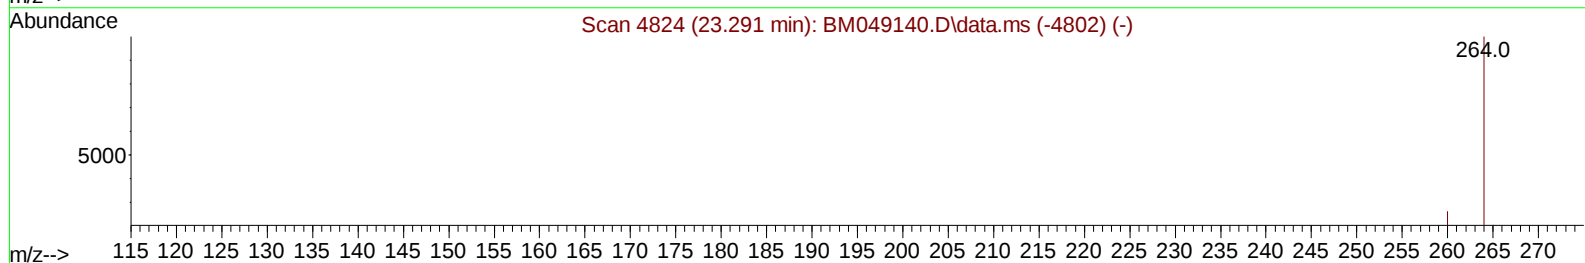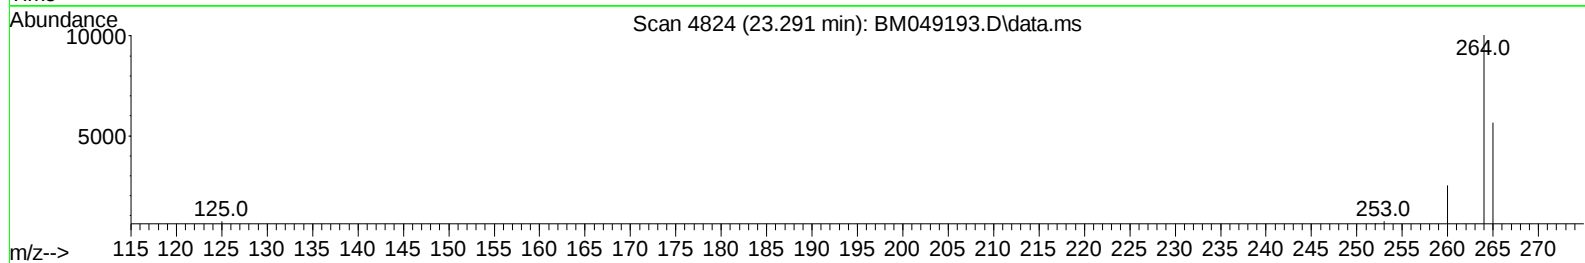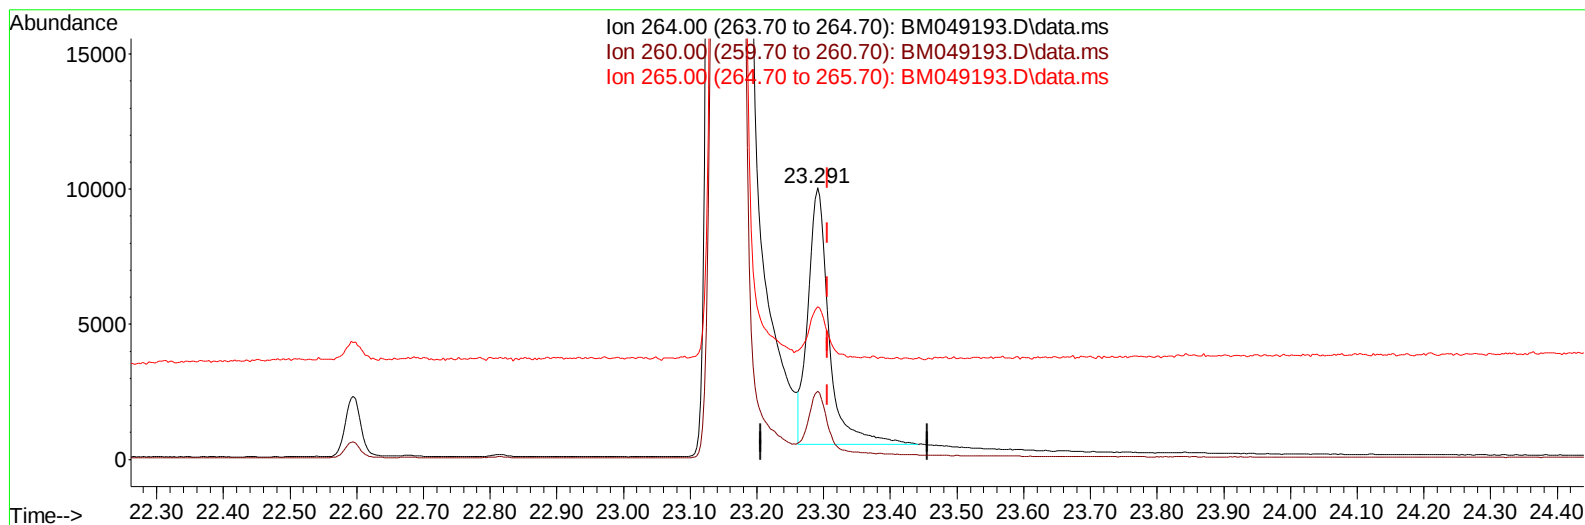

TIC: BM049193.D\data.ms

(23) Perylene-d12 (I)

23.291min (-0.015) 0.40 ng/u1

response 20542

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.80	25.18
265.00	78.30	56.25#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049193.D
Acq On : 24 Dec 2024 20:40
Operator : RC/JU
Sample : P5353-03
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2928

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/25/2024
Supervised By :mohammad ahmed 12/26/2024

Quant Time: Dec 24 21:42:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

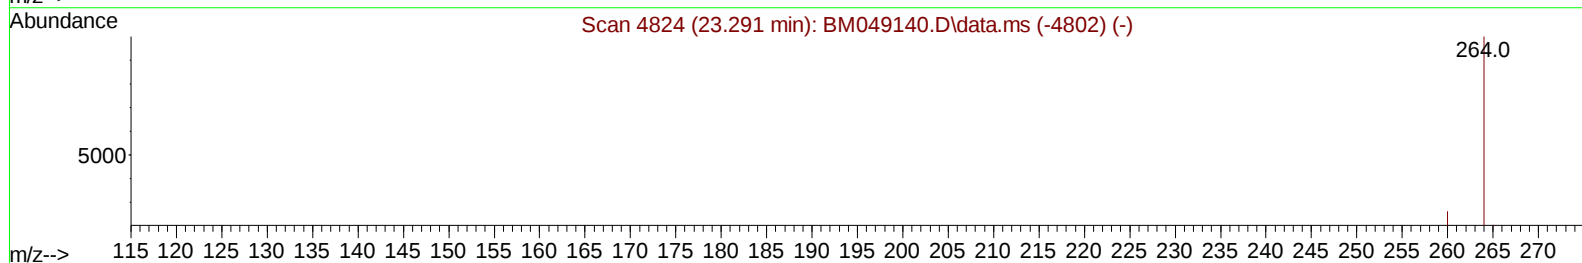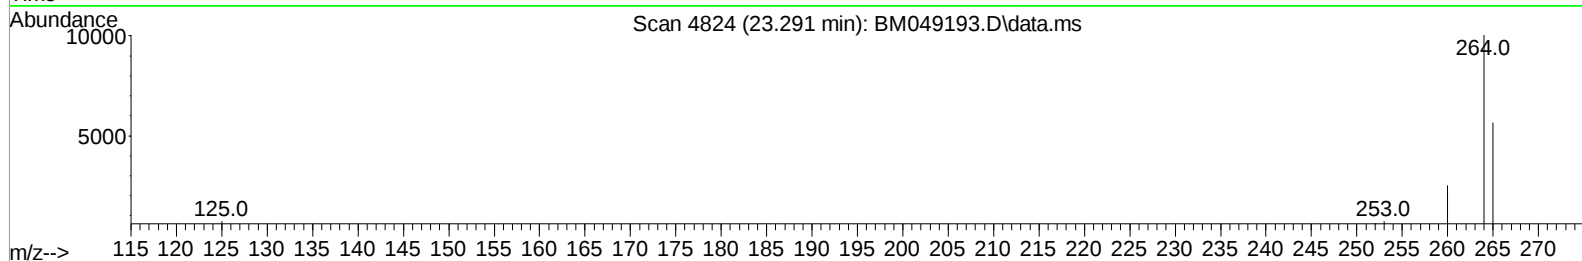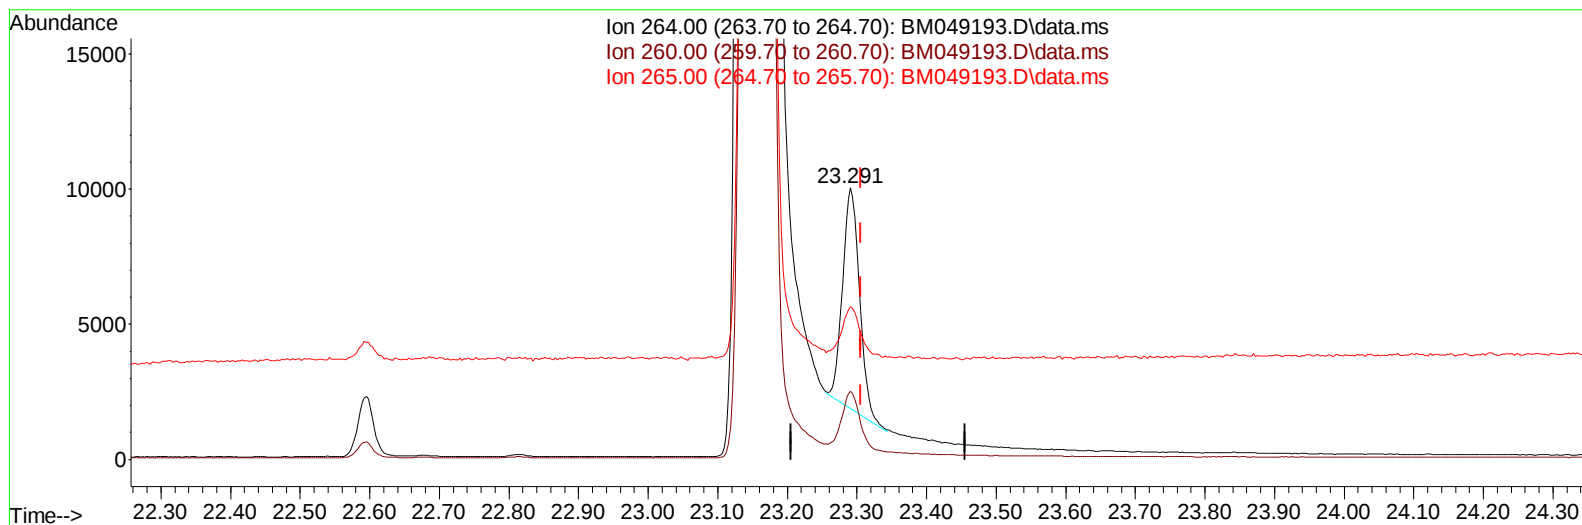

TIC: BM049193.D\data.ms

(23) Perylene-d12 (I)

23.291min (-0.015) 0.40 ng/ul m

response 13781

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.80	25.18
265.00	78.30	56.25#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
 Data File : BM049193.D
 Acq On : 24 Dec 2024 20:40
 Operator : RC/JU
 Sample : P5353-03
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E2928

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/25/2024
 Supervised By :mohammad ahmed 12/26/2024

Quant Time: Dec 24 21:42:18 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 18 15:33:13 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.548	152		4809	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.309	136		14566	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.187	164		8141	0.400	ng/ul	-0.01
13) Phenanthrene-d10	16.934	188		18176m	0.400	ng/ul	-0.02
17) Chrysene-d12	21.140	240		14041m	0.400	ng/ul	0.00
23) Perylene-d12	23.291	264		13781m	0.400	ng/ul	-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.143	96		32636	5.884	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.910	152		8575	0.438	ng/ul	-0.02
18) Fluoranthene-d10	18.969	212		20488	0.514	ng/ul	-0.01
Target Compounds				Qvalue			
5) Naphthalene	10.359	128		1121	0.031	ng/ul#	76
19) Fluoranthene	19.002	202		1278	0.025	ng/ul#	83
21) Benzo(a)anthracene	21.125	228		1350	0.028	ng/ul#	89
22) Chrysene	21.175	228		1484	0.028	ng/ul#	88
24) Benzo(b)fluoranthene	22.653	252		1899	0.043	ng/ul#	28
25) Benzo(k)fluoranthene	22.697	252		1738	0.036	ng/ul#	26
27) Indeno(1,2,3-cd)pyrene	25.437	276		2264	0.038	ng/ul#	55
28) Dibenzo(a,h)anthracene	25.450	278		1490	0.032	ng/ul#	33
29) Benzo(g,h,i)perylene	26.084	276		1826	0.038	ng/ul#	64

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049193.D
Acq On : 24 Dec 2024 20:40
Operator : RC/JU
Sample : P5353-03
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2928

Manual IntegrationsAPPROVED

Quant Time: Dec 24 21:42:18 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/25/2024
Supervised By :mohammad ahmed 12/26/2024

