




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049194.D
Acq On : 24 Dec 2024 21:16
Operator : RC/JU
Sample : P5379-01
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YE692

Manual IntegrationsAPPROVED

Quant Time: Dec 24 23:08:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/25/2024
Supervised By :mohammad ahmed 12/26/2024

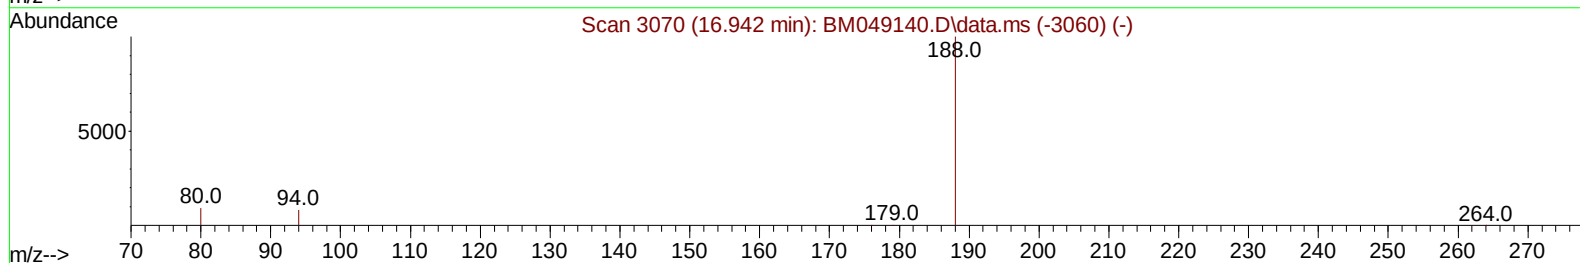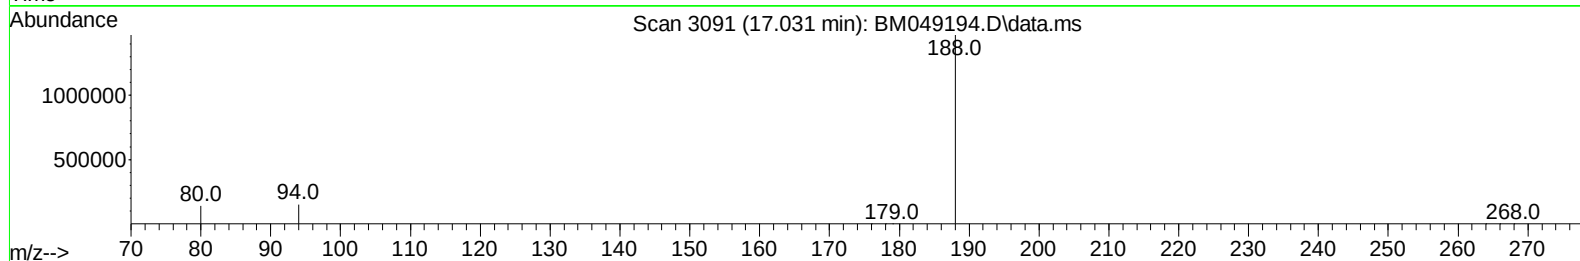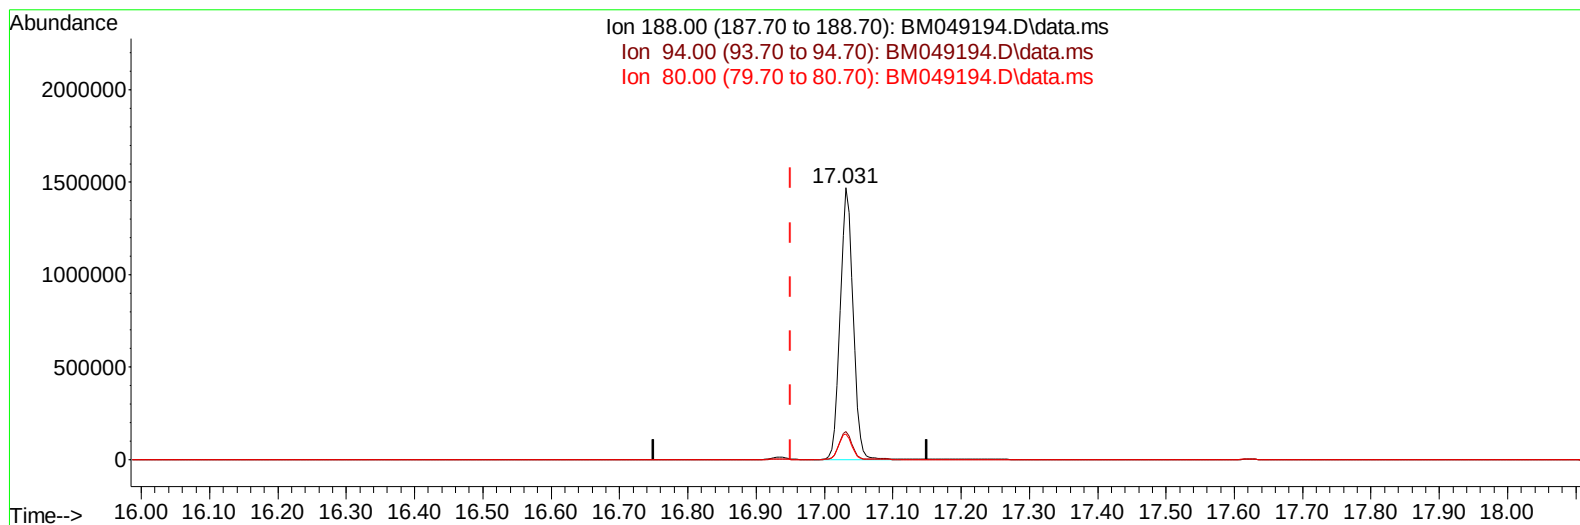

TIC: BM049194.D\data.ms

(13) Phenanthrene-d10 (I)

17.031min (+ 0.081) 0.40 ng/u1

response 1912865

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	9.80	10.27
80.00	10.70	9.45
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049194.D
Acq On : 24 Dec 2024 21:16
Operator : RC/JU
Sample : P5379-01
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YE692

Manual IntegrationsAPPROVED

Quant Time: Dec 24 23:08:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/25/2024
Supervised By :mohammad ahmed 12/26/2024

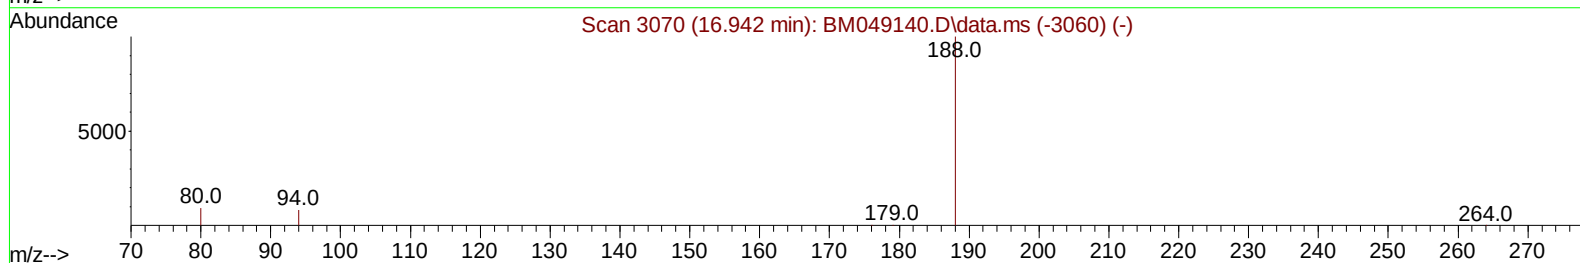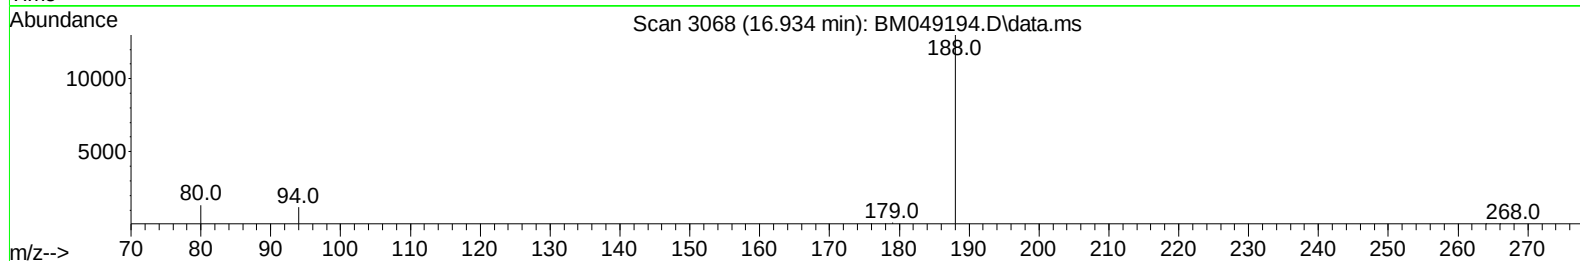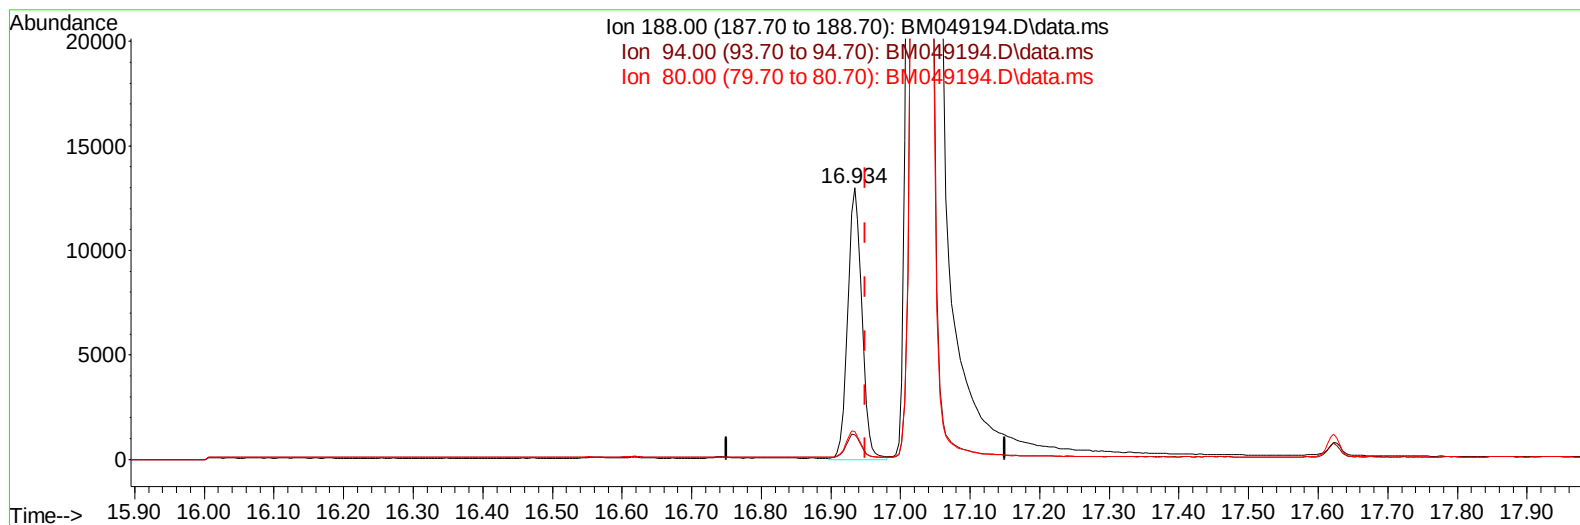

TIC: BM049194.D\data.ms

(13) Phenanthrene-d10 (I)

16.934min (-0.016) 0.40 ng/ul m

response 18410

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	9.80	9.11
80.00	10.70	10.26
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049194.D
Acq On : 24 Dec 2024 21:16
Operator : RC/JU
Sample : P5379-01
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YE692

Manual IntegrationsAPPROVED

Quant Time: Dec 24 23:08:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/25/2024
Supervised By :mohammad ahmed 12/26/2024

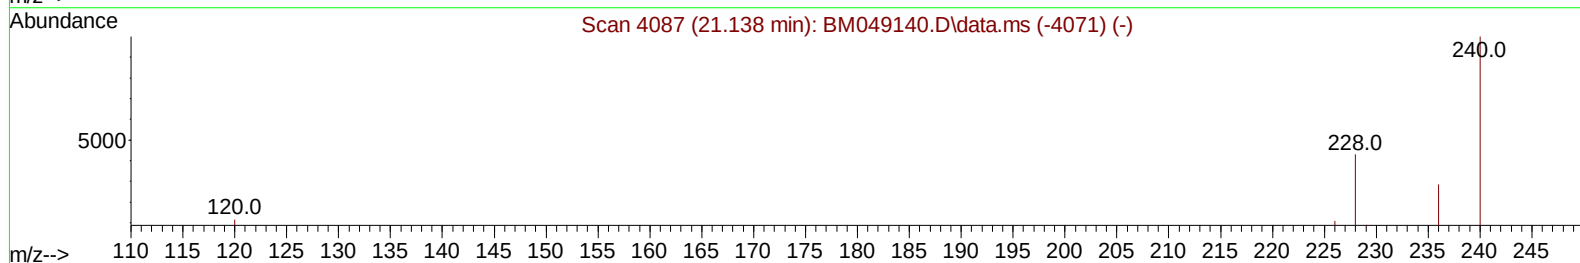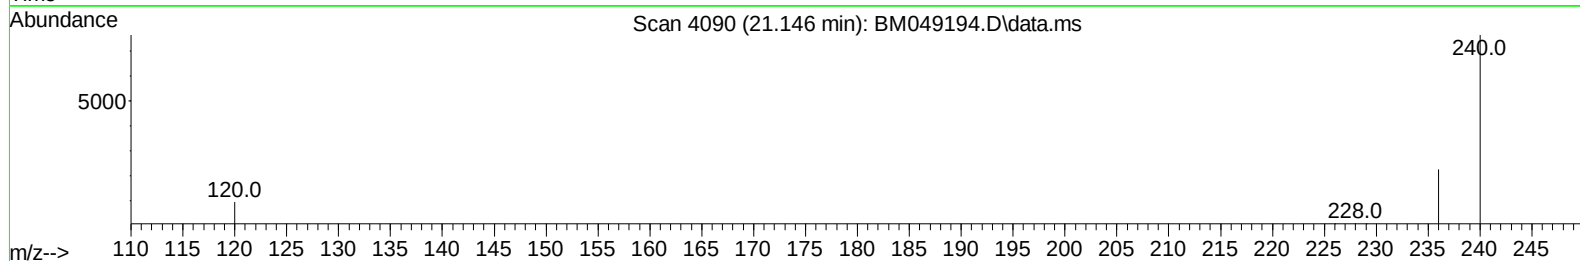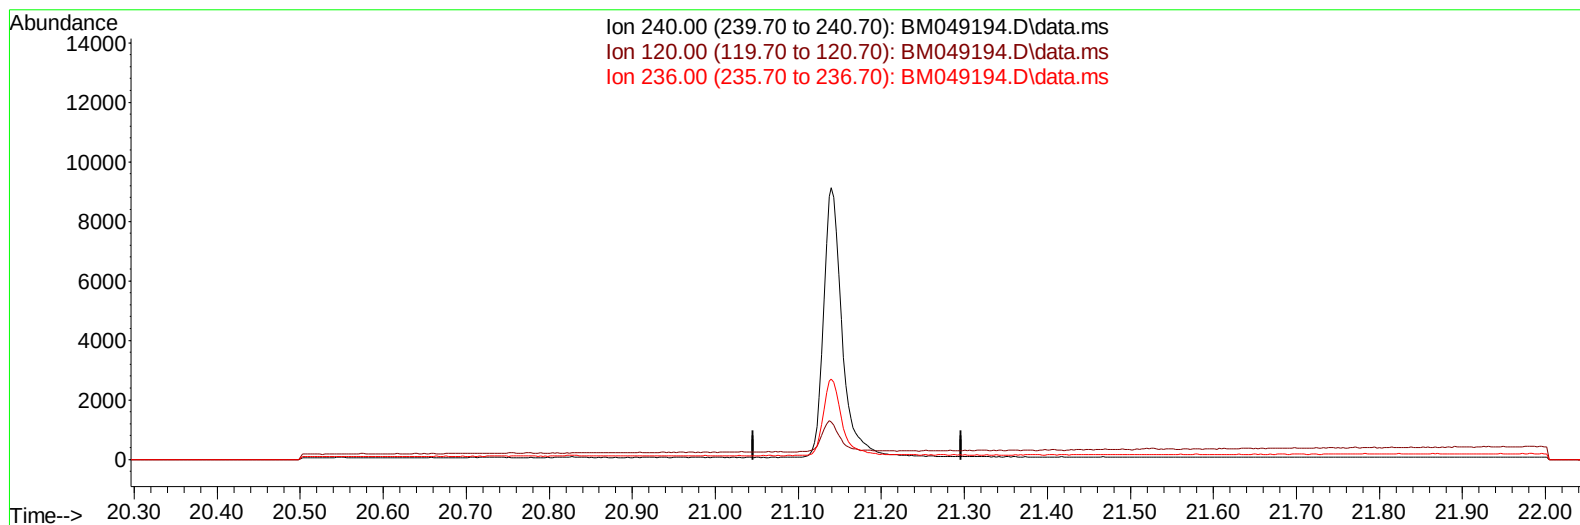

TIC: BM049194.D\data.ms

(17) Chrysene-d12

21.146min (-21.146) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	14.50	0.00#
236.00	29.80	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049194.D
Acq On : 24 Dec 2024 21:16
Operator : RC/JU
Sample : P5379-01
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YE692

Manual IntegrationsAPPROVED

Quant Time: Dec 24 23:08:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/25/2024
Supervised By :mohammad ahmed 12/26/2024

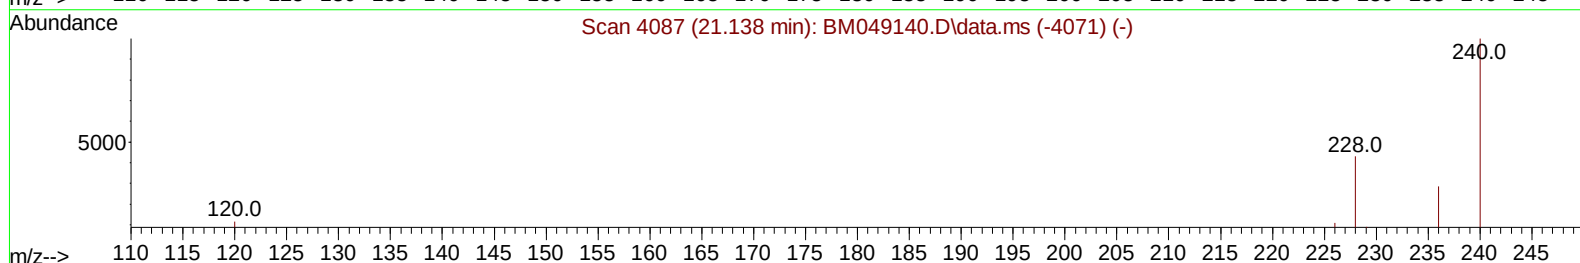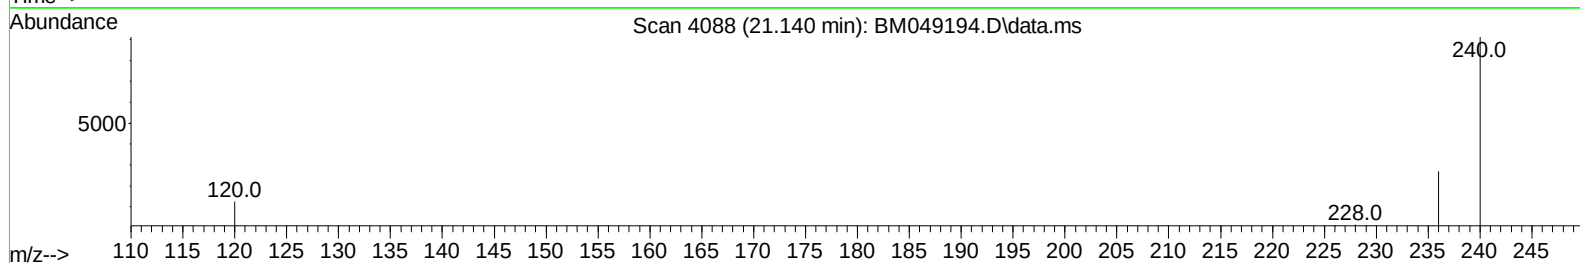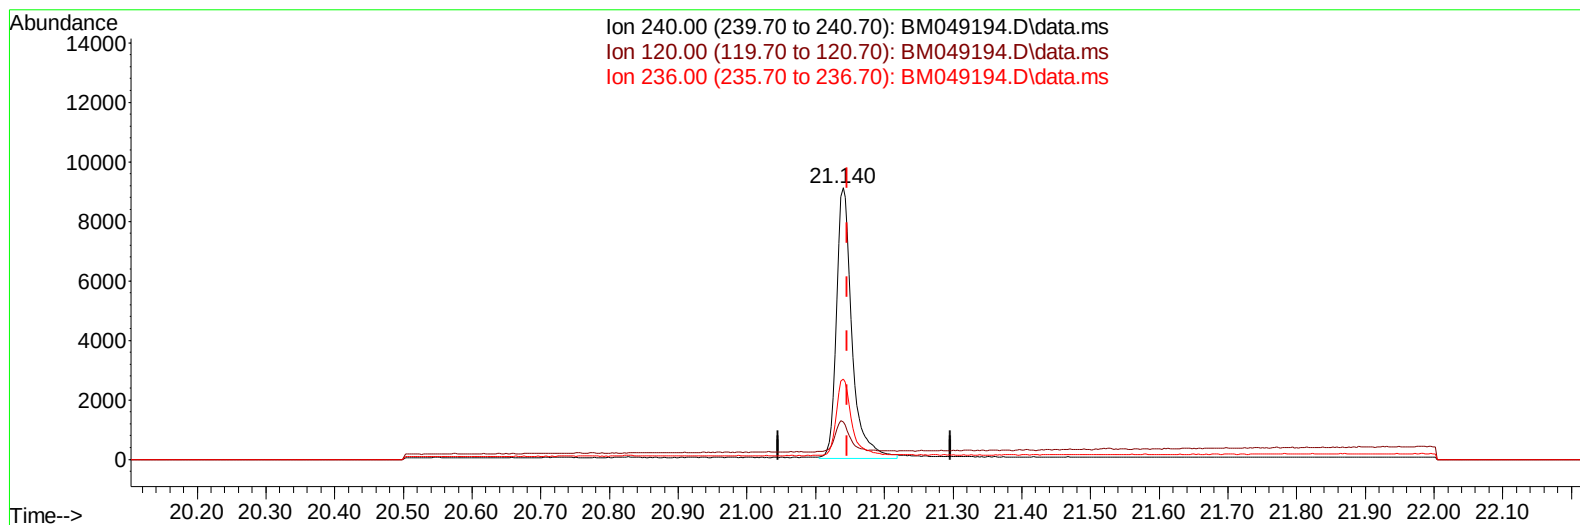

TIC: BM049194.D\data.ms

(17) Chrysene-d12

21.140min (-0.006) 0.40 ng/ul m

response 14229

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	14.50	13.71
236.00	29.80	29.66
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049194.D
Acq On : 24 Dec 2024 21:16
Operator : RC/JU
Sample : P5379-01
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YE692

Manual IntegrationsAPPROVED

Quant Time: Dec 24 23:08:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/25/2024
Supervised By :mohammad ahmed 12/26/2024

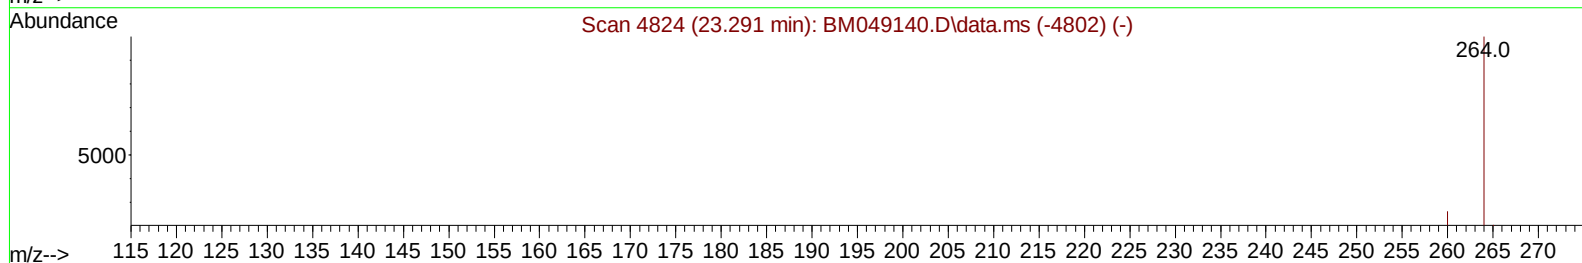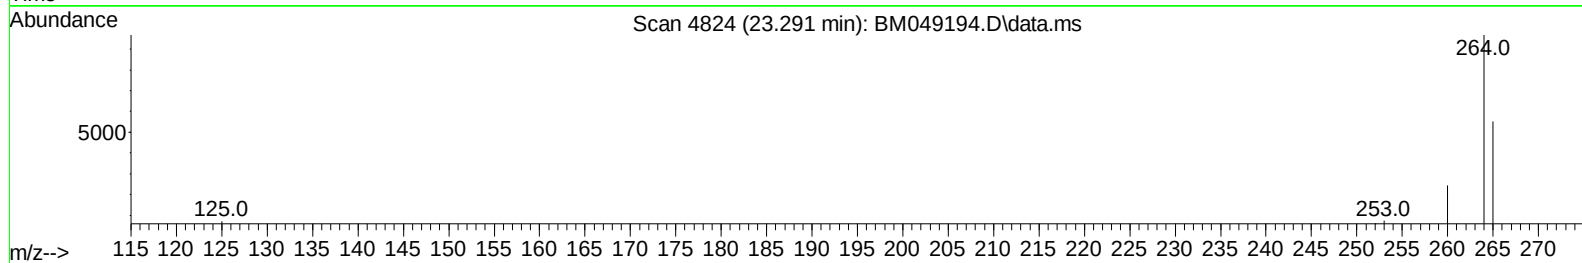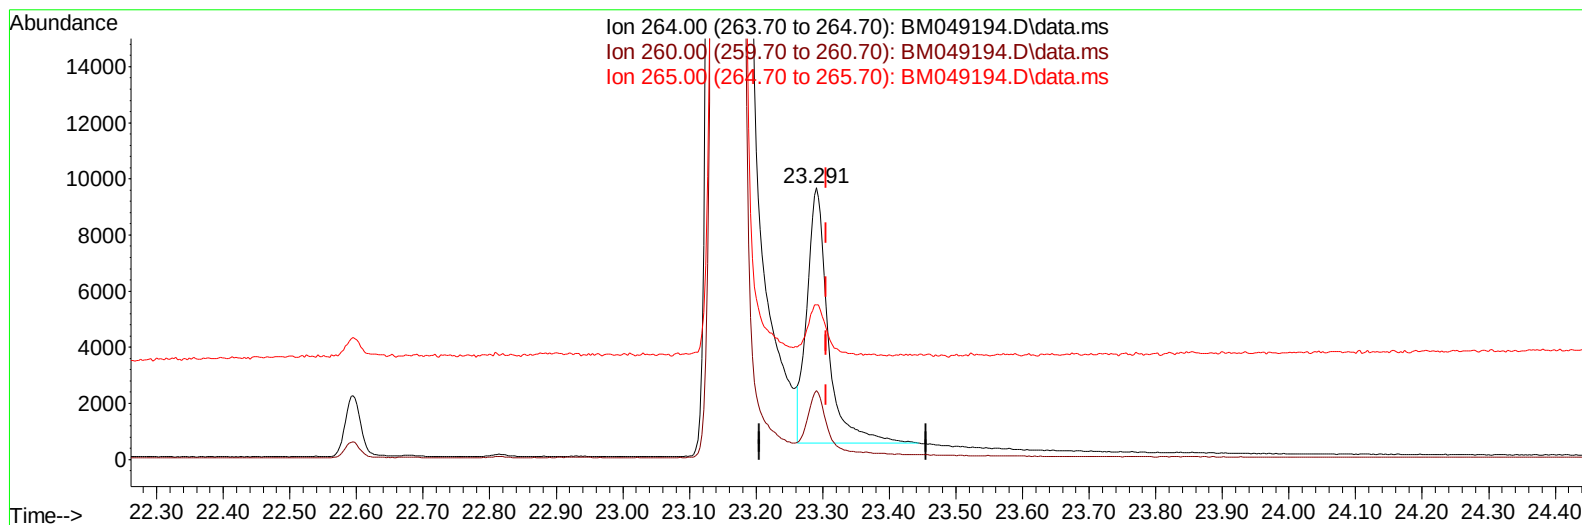

TIC: BM049194.D\data.ms

(23) Perylene-d12 (I)

23.291min (-0.015) 0.40 ng/u1

response 20280

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.80	25.36
265.00	78.30	56.98#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049194.D
Acq On : 24 Dec 2024 21:16
Operator : RC/JU
Sample : P5379-01
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YE692

Manual IntegrationsAPPROVED

Quant Time: Dec 24 23:08:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/25/2024
Supervised By :mohammad ahmed 12/26/2024

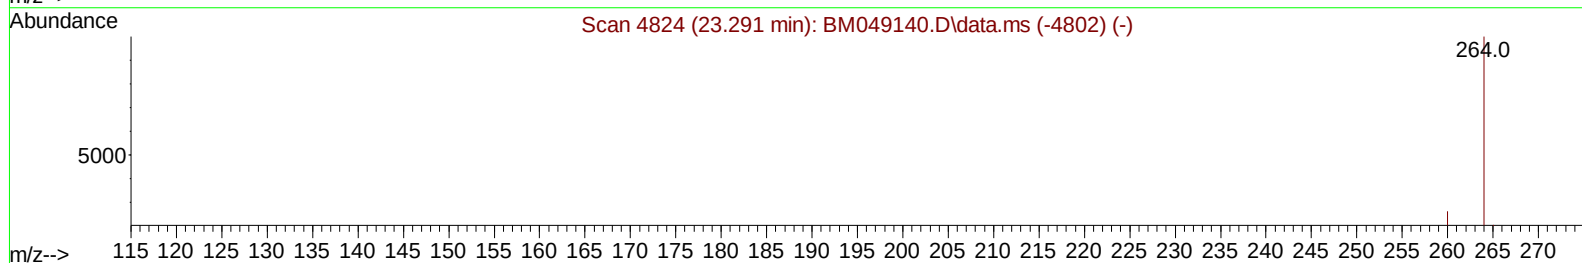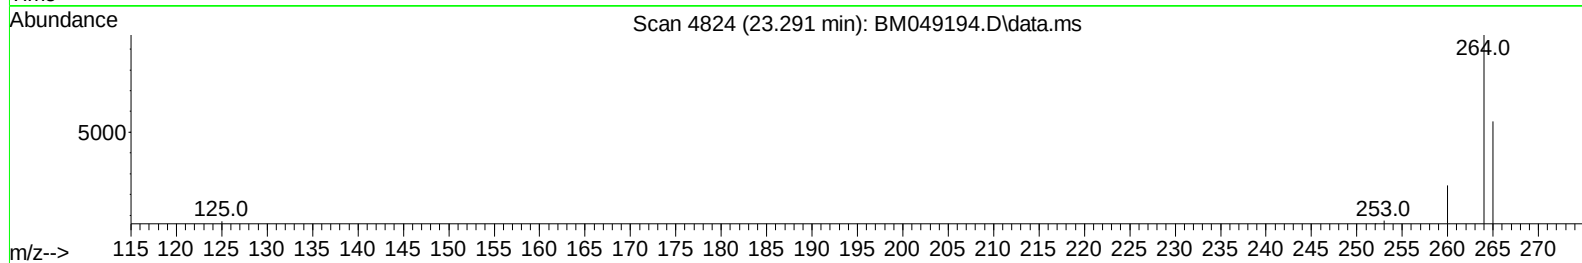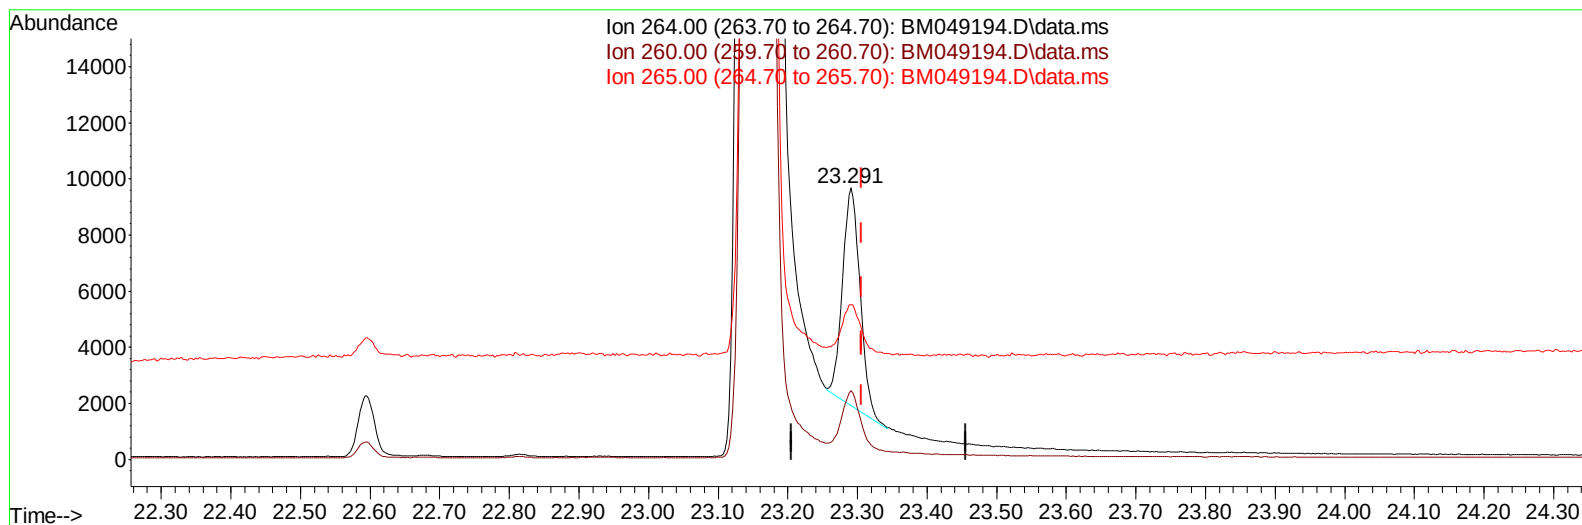

TIC: BM049194.D\data.ms

(23) Perylene-d12 (I)

23.291min (-0.015) 0.40 ng/ul m

response 13556

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	25.80	25.36
265.00	78.30	56.98#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
 Data File : BM049194.D
 Acq On : 24 Dec 2024 21:16
 Operator : RC/JU
 Sample : P5379-01
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YE692

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/25/2024
 Supervised By :mohammad ahmed 12/26/2024

Quant Time: Dec 24 23:08:30 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 18 15:33:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.548	152	5035	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.309	136	15090	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.183	164	8334	0.400	ng/ul	-0.02
13) Phenanthrene-d10	16.934	188	18410m	0.400	ng/ul	-0.02
17) Chrysene-d12	21.140	240	14229m	0.400	ng/ul	0.00
23) Perylene-d12	23.291	264	13556m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.143	96	31107	5.357	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.910	152	8997	0.444	ng/ul	-0.02
18) Fluoranthene-d10	18.974	212	20746	0.514	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049194.D
Acq On : 24 Dec 2024 21:16
Operator : RC/JU
Sample : P5379-01
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YE692

Manual IntegrationsAPPROVED

Quant Time: Dec 24 23:08:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/25/2024
Supervised By :mohammad ahmed 12/26/2024

