

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
 Data File : BM049153.D
 Acq On : 23 Dec 2024 19:10
 Operator : RC/JU
 Sample : P5353-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E2927

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/24/2024
 Supervised By :mohammad ahmed 12/26/2024

Quant Time: Dec 23 22:58:43 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 18 15:33:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.552	152	3818	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.314	136	11047	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.191	164	6060	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.937	188	12955m	0.400	ng/ul	-0.01
17) Chrysene-d12	21.143	240	10140m	0.400	ng/ul	0.00
23) Perylene-d12	23.291	264	10071m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.143	96	27097	6.154	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.920	152	6491	0.437	ng/ul	0.00
18) Fluoranthene-d10	18.973	212	14962	0.520	ng/ul	0.00
Target Compounds						Qvalue
5) Naphthalene	10.363	128	642	0.023	ng/ul#	63

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049153.D
Acq On : 23 Dec 2024 19:10
Operator : RC/JU
Sample : P5353-01
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
E2927

Quant Time: Dec 23 22:58:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

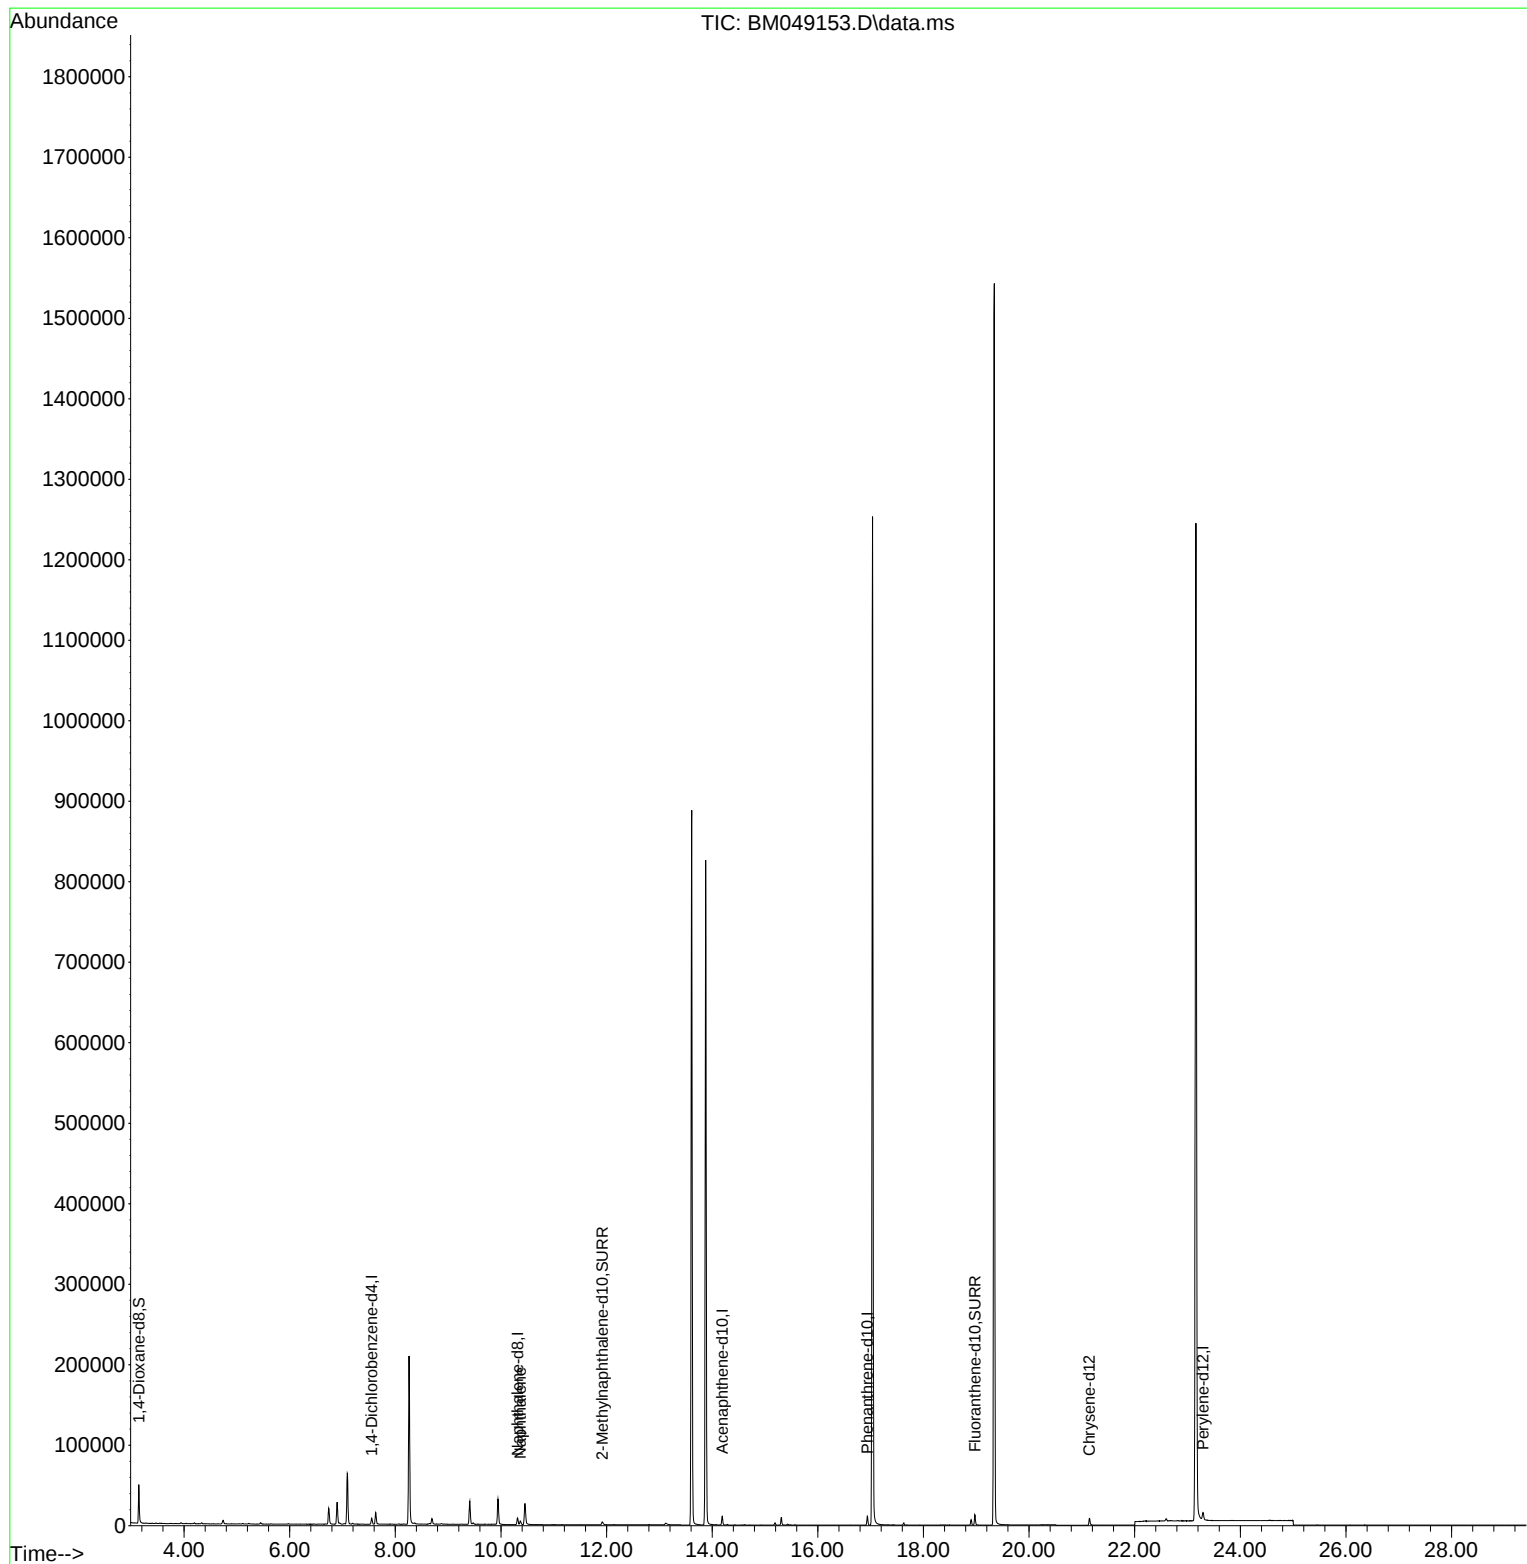

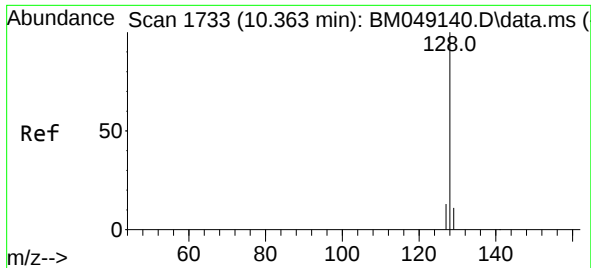

#5
Naphthalene
Concen: 0.023 ng/ul
RT: 10.363 min Scan# 11
Delta R.T. -0.016 min
Lab File: BM049153.D
Acq: 23 Dec 2024 19:10

Instrument :
BNA_M
ClientSampleId :
E2927

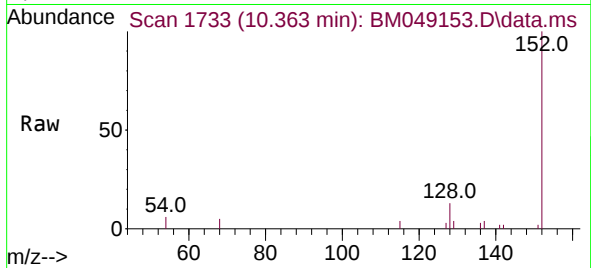

Tgt Ion:128 Resp: 64
Ion Ratio Lower Upper
128 100
129 29.7 9.7 14.5
127 25.0 10.6 16.0

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/24/2024
Supervised By :mohammad ahmed 12/26/2024

