

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
 Data File : BM049195.D
 Acq On : 24 Dec 2024 21:52
 Operator : RC/JU
 Sample : P5305-02
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E2AT7

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/25/2024
 Supervised By :mohammad ahmed 12/26/2024

Quant Time: Dec 24 23:10:30 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 18 15:33:13 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.548	152	6967	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.309	136	21054	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.183	164	11698	0.400	ng/ul	-0.02
13) Phenanthrene-d10	16.934	188	25471m	0.400	ng/ul	-0.02
17) Chrysene-d12	21.140	240	19193m	0.400	ng/ul	0.00
23) Perylene-d12	23.291	264	18791m	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.143	96	37116	4.619	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.910	152	10393	0.367	ng/ul	-0.02
18) Fluoranthene-d10	18.969	212	23062	0.424	ng/ul	-0.01
Target Compounds						Qvalue
5) Naphthalene	10.359	128	1090	0.021	ng/ul#	73

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122324\
Data File : BM049195.D
Acq On : 24 Dec 2024 21:52
Operator : RC/JU
Sample : P5305-02
Misc :
ALS Vial : 60 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
E2AT7

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/25/2024
Supervised By :mohammad ahmed 12/26/2024


Quant Time: Dec 24 23:10:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 18 15:33:13 2024
Response via : Initial Calibration

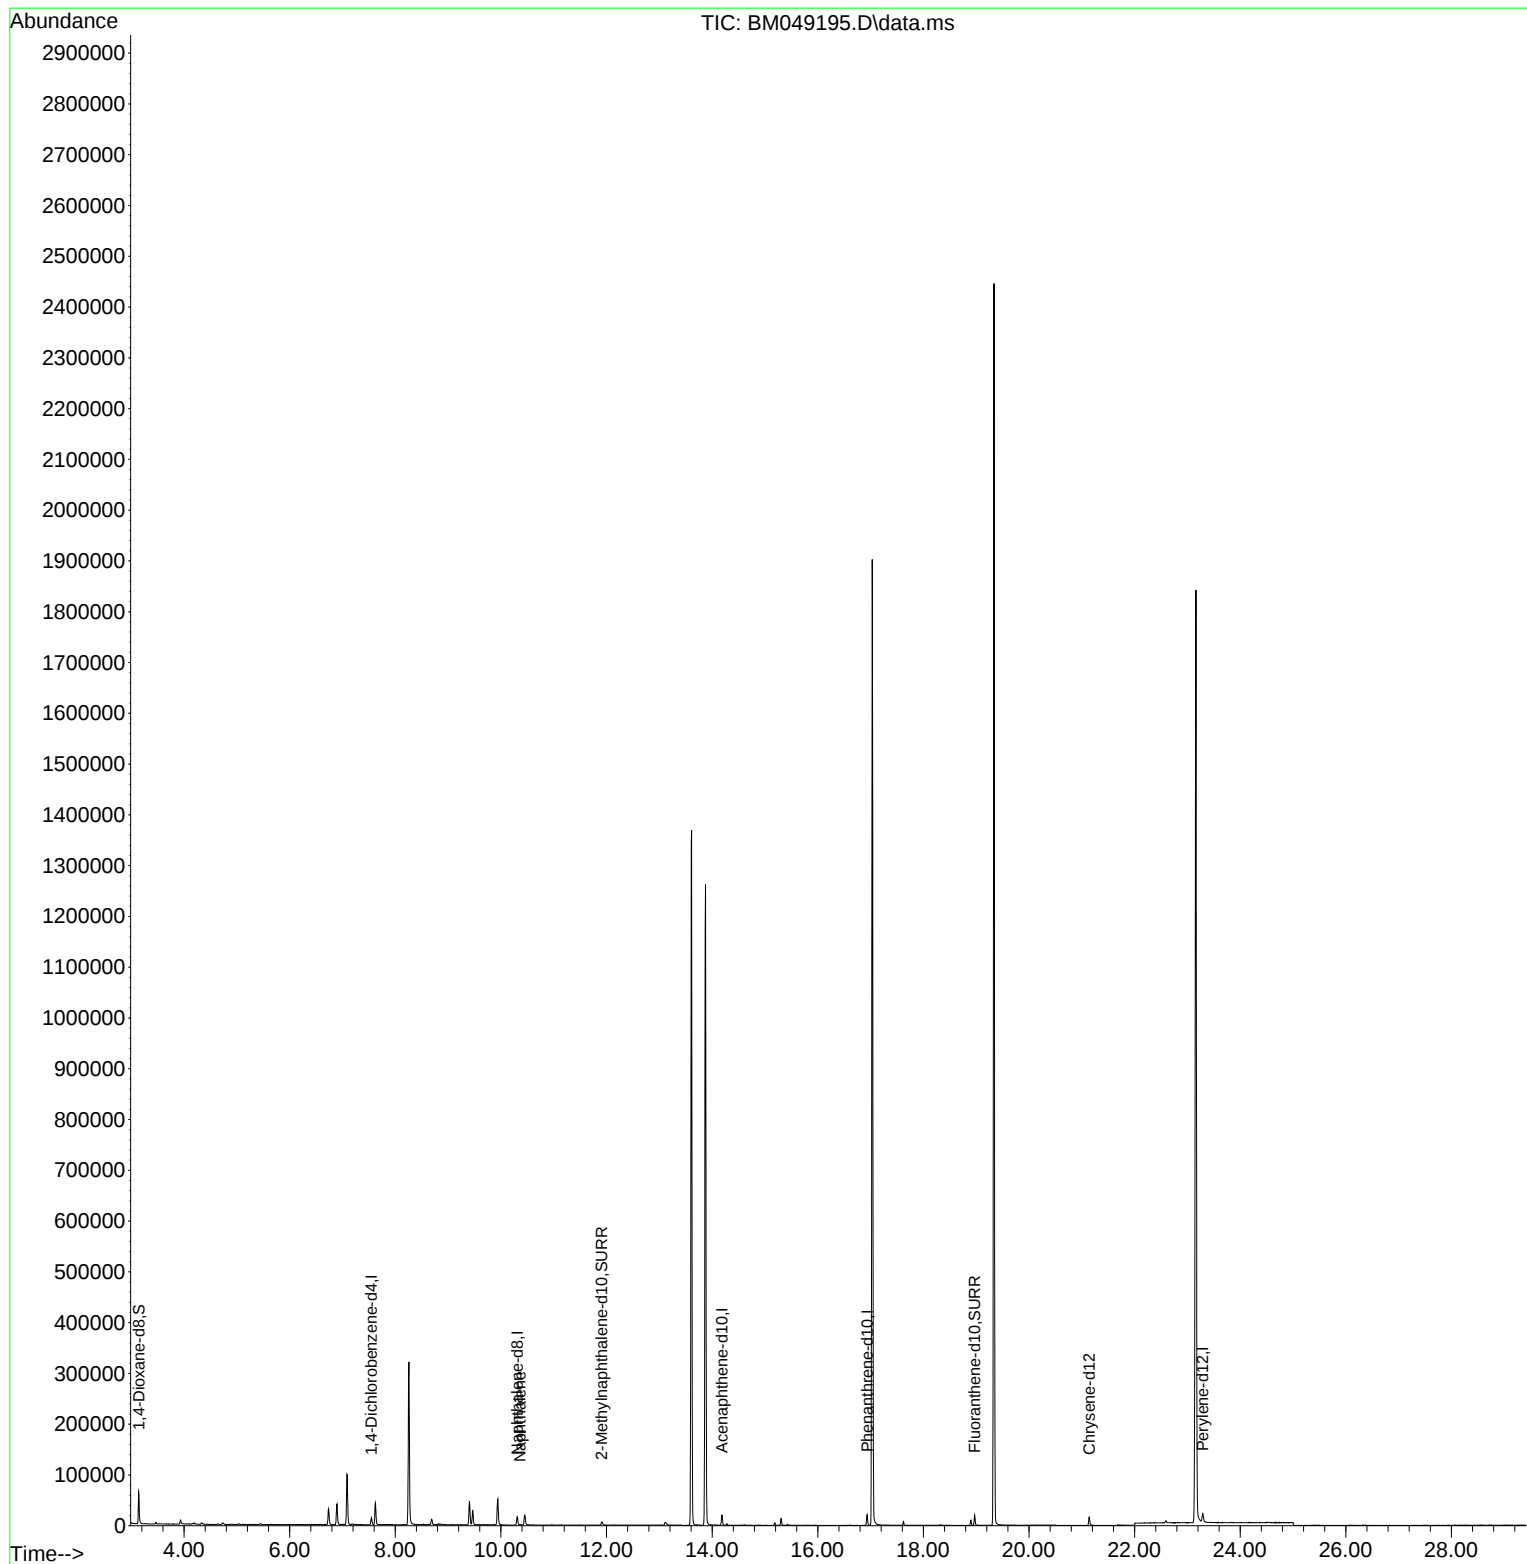

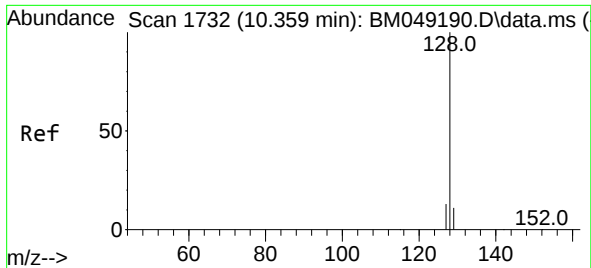

#5
Naphthalene
Concen: 0.021 ng/ul
RT: 10.359 min Scan# 11
Delta R.T. -0.021 min
Lab File: BM049195.D
Acq: 24 Dec 2024 21:52

Instrument :
BNA_M
ClientSampleId :
E2AT7

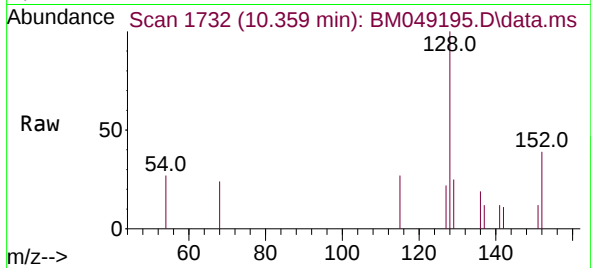

Tgt Ion:128 Resp: 1090
Ion Ratio Lower Upper
128 100
129 24.7 9.7 14.5
127 22.3 10.6 16.0

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/25/2024
Supervised By :mohammad ahmed 12/26/2024

