


Data Path : Z:\HPCHEM1\BNA M\DATA\BM122415\
 Data File : BM003744.D
 Acq On : 23 Dec 2015 13:42
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM122415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 24 10:08:49 2015

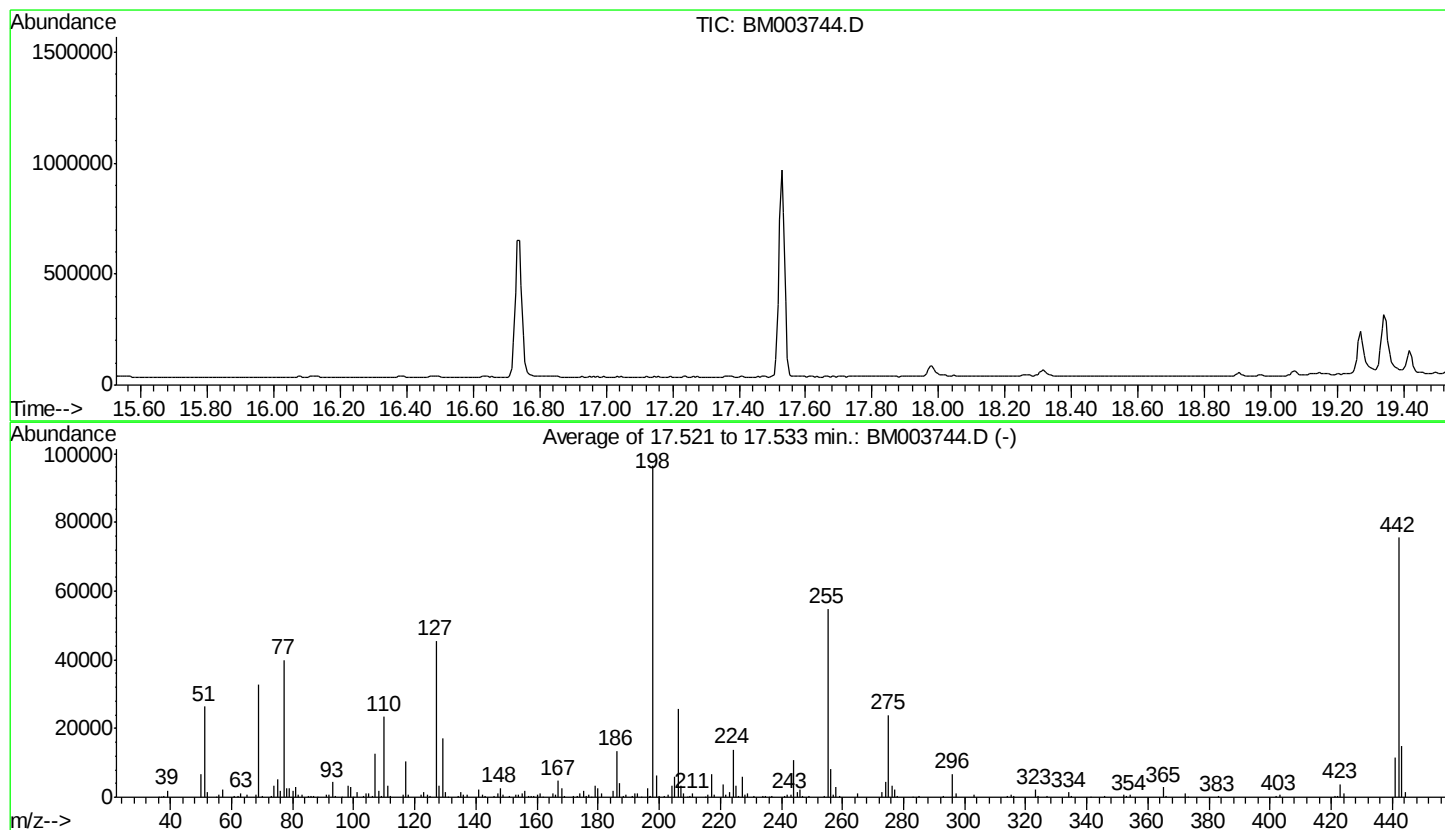

AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.4	26434	PASS
68	69	0.00	2	1.9	633	PASS
69	198	0.00	100	34.0	32837	PASS
70	69	0.00	2	0.6	212	PASS
127	198	10	80	47.1	45480	PASS
197	198	0.00	2	0.4	348	PASS
198	198	100	100	100.0	96504	PASS
199	198	5	9	6.7	6432	PASS
275	198	10	60	24.8	23896	PASS
365	198	1	100	3.0	2894	PASS
441	442	0.01	24	15.2	11465	PASS
442	198	50	100	78.3	75541	PASS
443	442	15	24	20.0	15089	PASS