


Data Path : Z:\HPCHEM1\BNA M\DATA\BM122415\
 Data File : BM003755.D
 Acq On : 23 Dec 2015 23:47
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM122415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 24 10:08:49 2015

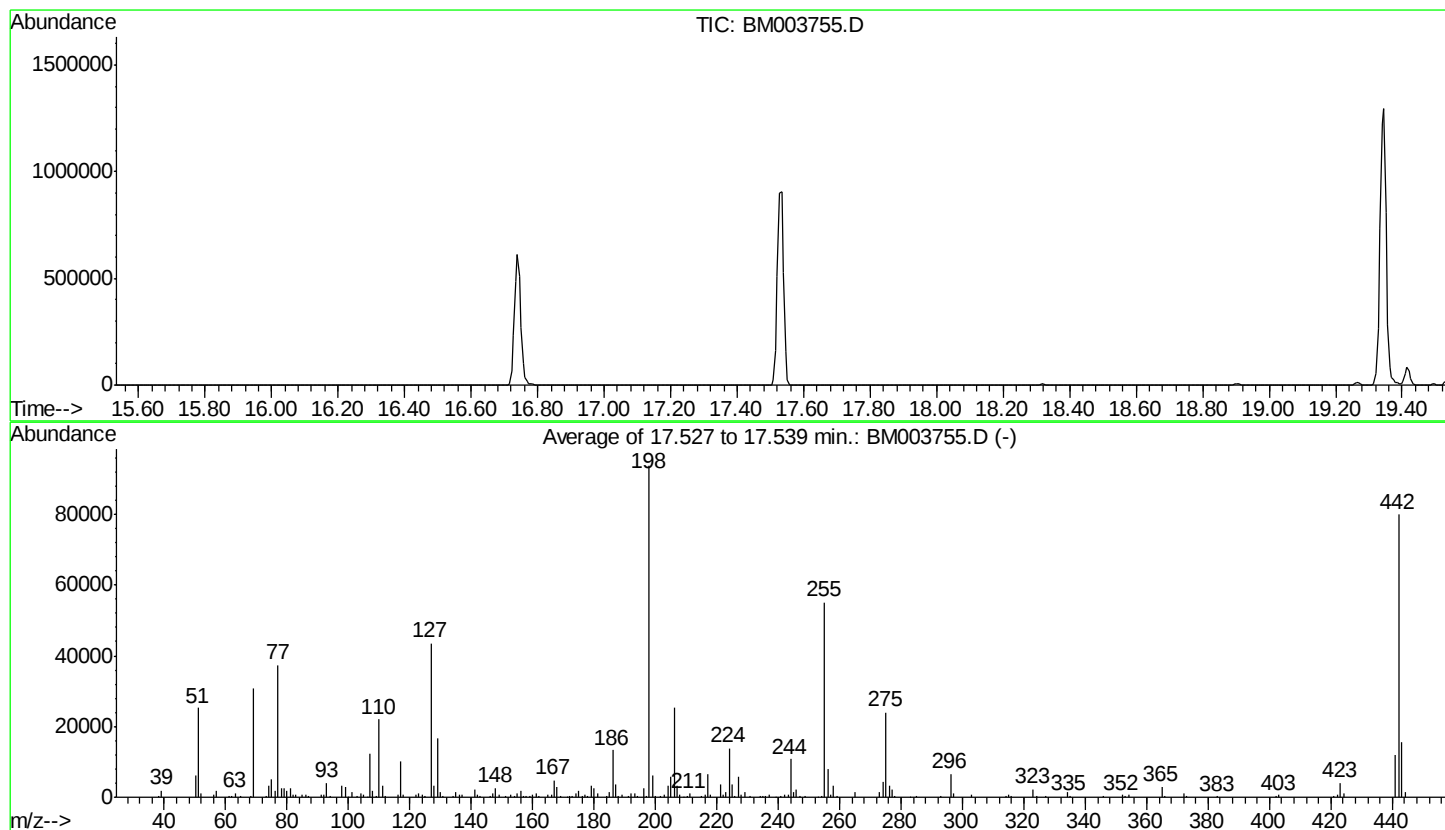

AutoFind: Scans 2455, 2456, 2457; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.9	25226	PASS
68	69	0.00	2	1.3	406	PASS
69	198	0.00	100	32.9	30842	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.5	43594	PASS
197	198	0.00	2	0.5	493	PASS
198	198	100	100	100.0	93781	PASS
199	198	5	9	6.6	6182	PASS
275	198	10	60	25.6	24050	PASS
365	198	1	100	3.1	2942	PASS
441	442	0.01	24	15.1	12061	PASS
442	198	50	100	85.1	79853	PASS
443	442	15	24	19.4	15509	PASS