

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
 Data File : BM008615.D
 Acq On : 24 Dec 2016 04:01
 Operator : UM/SJ
 Sample : H5995-08
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA870

Quant Time: Dec 24 04:58:43 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 24 04:56:03 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	434	0.40	ng/ul	-0.09
2) Naphthalene-d8	10.42	136	1404	0.40	ng/ul	-0.08
6) Acenaphthene-d10	14.28	164	944	0.40	ng/ul	-0.03
10) Phenanthrene-d10	17.14	188	85315	0.40	ng/ul	0.05
16) Chrysene-d12	21.27	240	1563	0.40	ng/ul	0.00
20) Perylene-d12	23.48	264	2228	0.40	ng/ul	-0.02
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.01	152	498	0.23	ng/ul	-0.09
14) Fluoranthene-d10	19.08	212	955	0.00	ng/ul	-0.02
Target Compounds				Qvalue		
3) Naphthalene	10.46	128	5743	1.45	ng/ul	98
5) 2-Methylnaphthalene	12.08	142	4966	1.87	ng/ul	97
7) Acenaphthylene	14.00	152	433	0.10	ng/ul#	1
8) Acenaphthene	14.35	153	808	0.25	ng/ul#	87
9) Fluorene	15.34	166	1982	0.54	ng/ul#	87
17) Pyrene	19.45	202	309	0.05	ng/ul#	1
23) Benzo(a)pyrene	23.33	252	469	0.06	ng/ul#	25


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
Data File : BM008615.D
Acq On : 24 Dec 2016 04:01
Operator : UM/SJ
Sample : H5995-08
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA870

Quant Time: Dec 24 04:58:43 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 24 04:56:03 2016
Response via : Initial Calibration

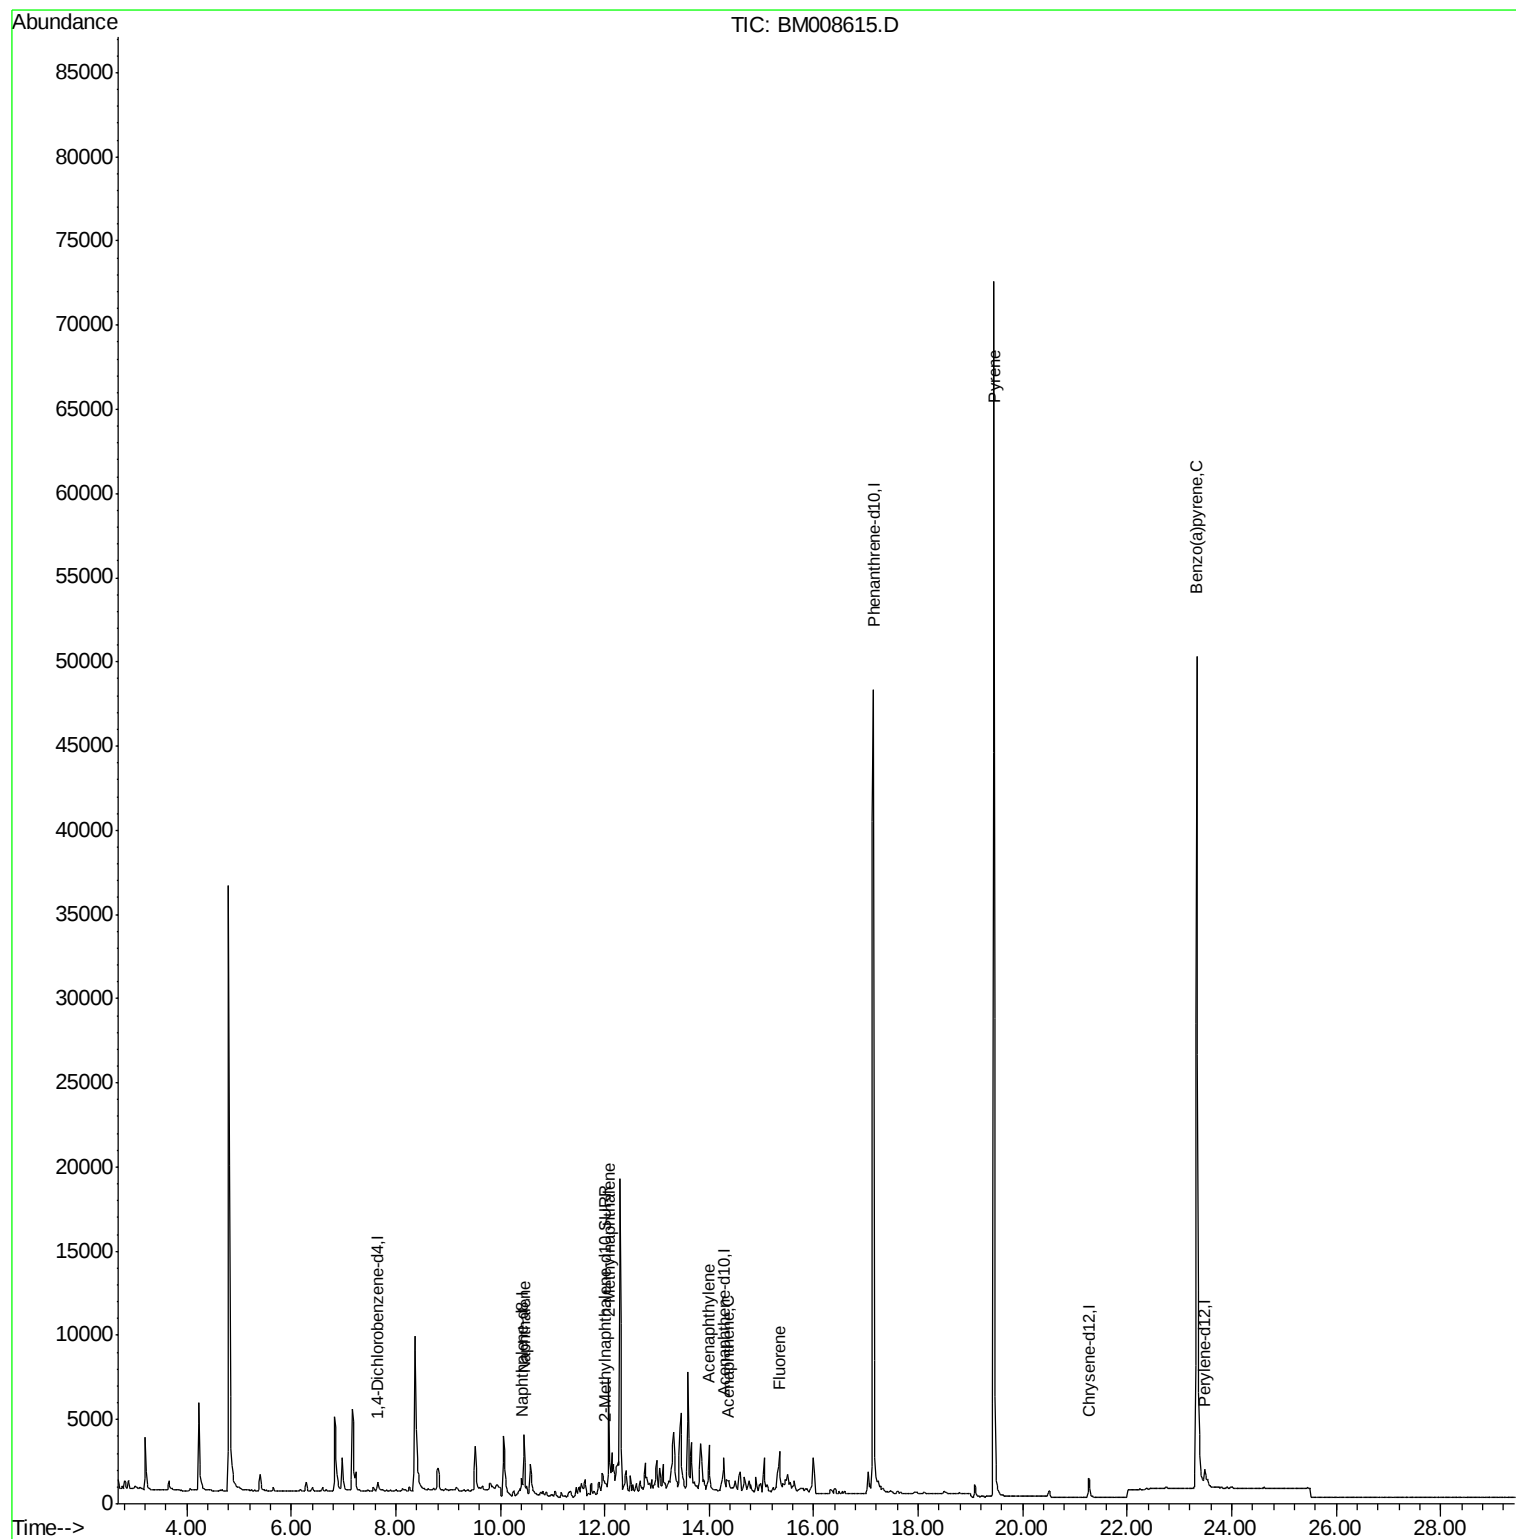

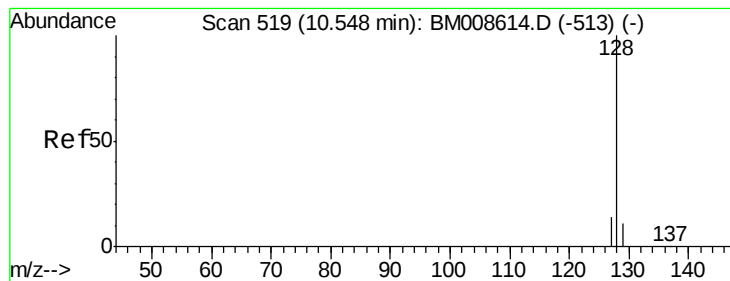

#3

Naphthalene

Concen: 1.45 ng/ul

RT: 10.46 min Scan# 512

Delta R.T. -0.08 min

Lab File: BM008615.D

Acq: 24 Dec 2016 04:01

Instrument :

BNA_M

ClientSampleId :

DA870


Tgt Ion:128 Resp: 5743

Ion Ratio Lower Upper

128 100

129 14.0 11.3 16.9




127 14.9 12.8 19.2

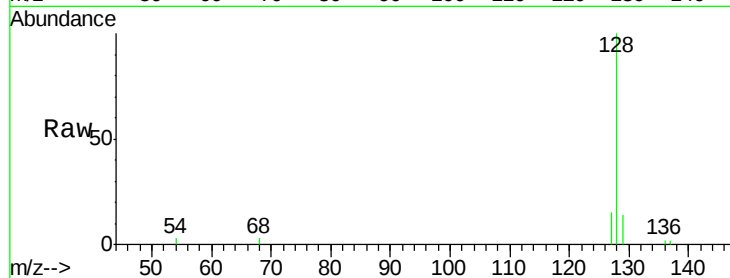

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

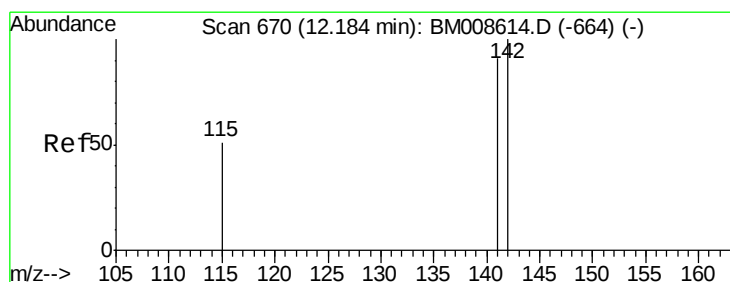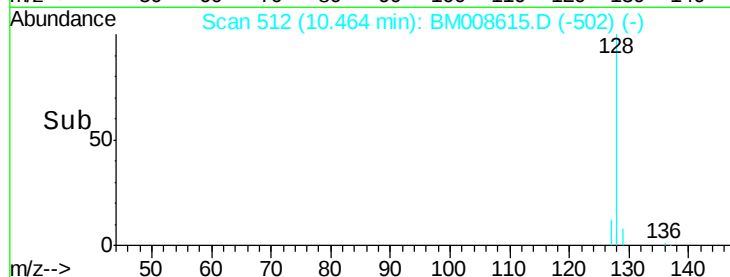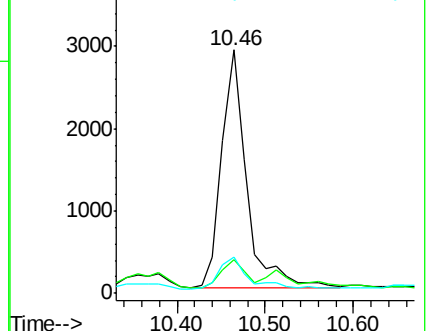

#5

2-Methylnaphthalene

Concen: 1.87 ng/ul

RT: 12.08 min Scan# 660

Delta R.T. -0.10 min

Lab File: BM008615.D


Acq: 24 Dec 2016 04:01

Tgt Ion:142 Resp: 4966

Ion Ratio Lower Upper



142 100


141 93.2 72.6 108.8

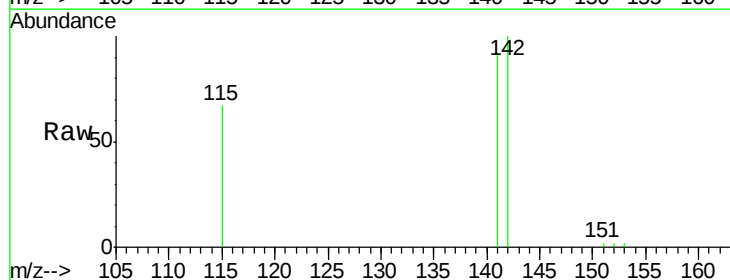

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

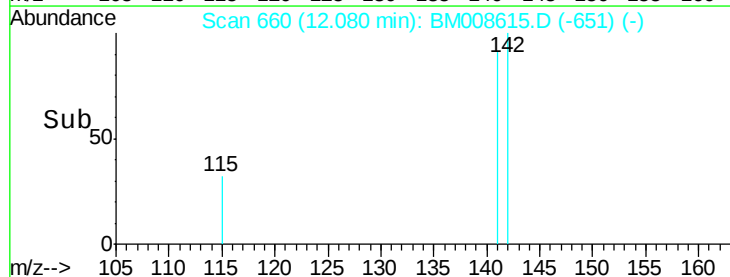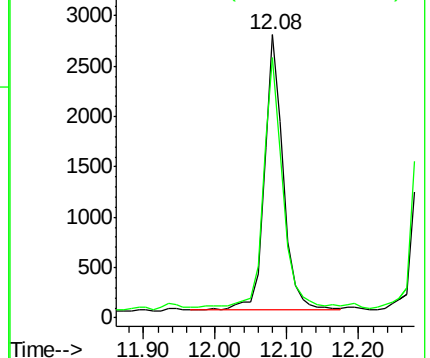

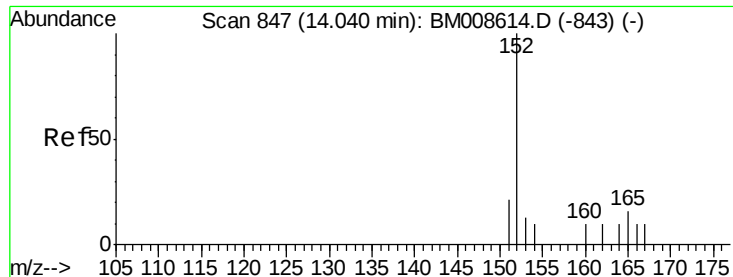

#7

Acenaphthylene

Concen: 0.10 ng/ul

RT: 14.00 min Scan# 844

Delta R.T. -0.04 min

Lab File: BM008615.D

Acq: 24 Dec 2016 04:01

Instrument :

BNA_M

ClientSampleId :

DA870


Tgt Ion:152 Resp: 433

Ion Ratio Lower Upper

152 100

151 53.0 17.1 25.7#




153 89.3 12.8 19.2#

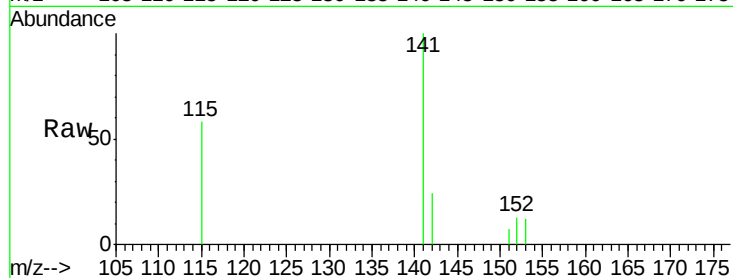

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

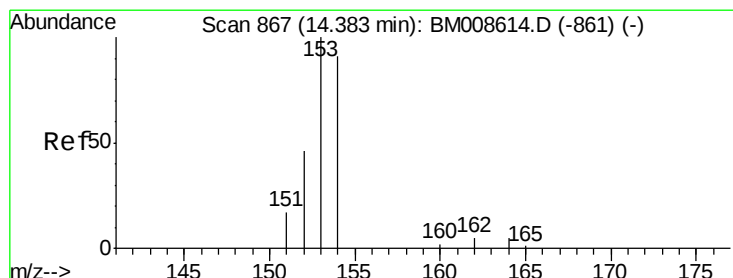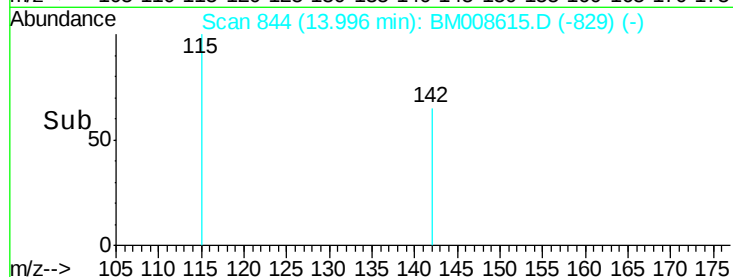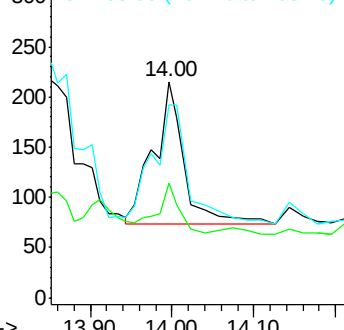

#8

Acenaphthene

Concen: 0.25 ng/ul

RT: 14.35 min Scan# 865

Delta R.T. -0.03 min

Lab File: BM008615.D

Acq: 24 Dec 2016 04:01


Tgt Ion:153 Resp: 808

Ion Ratio Lower Upper

153 100

152 67.7 40.3 60.5#



154 83.8 71.4 107.2

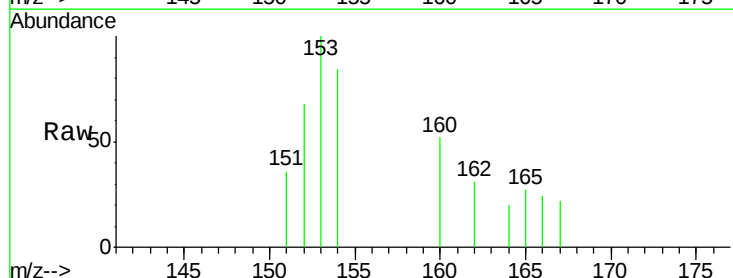


Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E



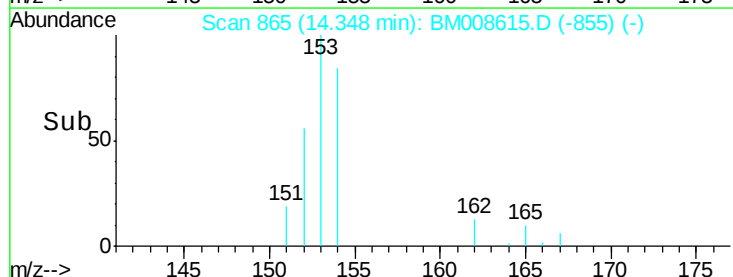
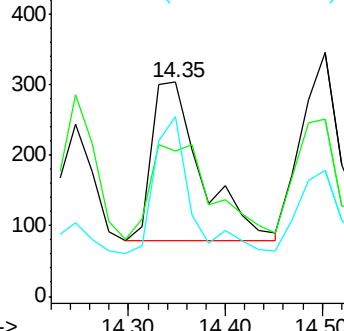


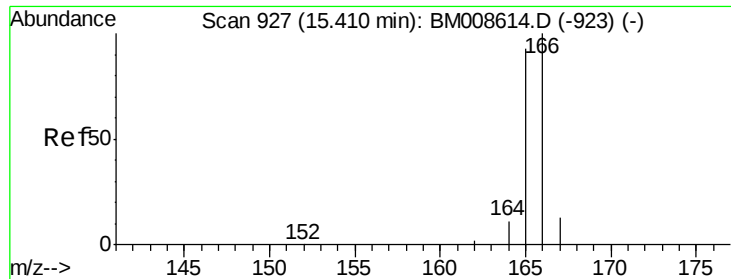

#9
Fluorene
 Concen: 0.54 ng/ul
 RT: 15.34 min Scan# 923
 Delta R.T. -0.07 min
 Lab File: BM008615.D
 Acq: 24 Dec 2016 04:01




Instrument :
 BNA_M
 ClientSampleId :
 DA870




Tgt Ion:166 Resp: 1982
 Ion Ratio Lower Upper
 166 100
 165 103.7 73.4 110.2
 167 26.0 14.6 22.0#

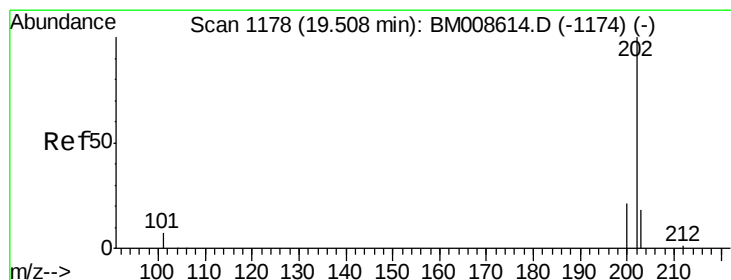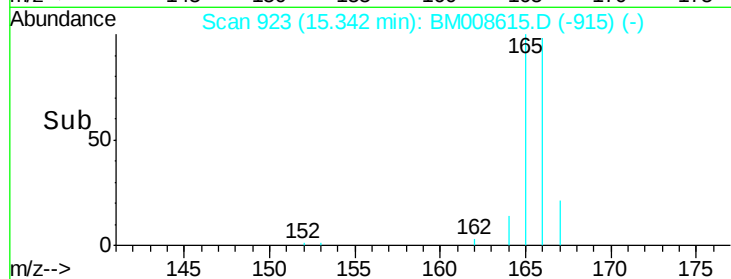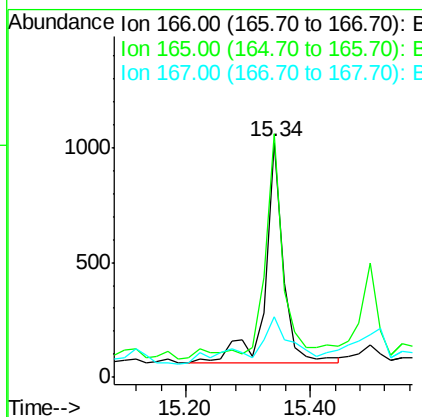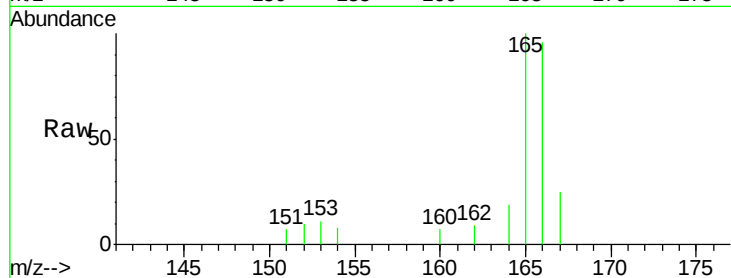

#17
Pyrene
 Concen: 0.05 ng/ul
 RT: 19.45 min Scan# 1173
 Delta R.T. -0.06 min
 Lab File: BM008615.D
 Acq: 24 Dec 2016 04:01

Tgt Ion:202 Resp: 309
 Ion Ratio Lower Upper
 202 100
 200 37.9 18.2 27.4#
 203 169.6 15.6 23.4#

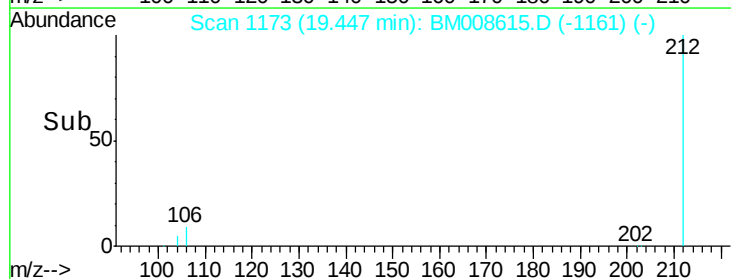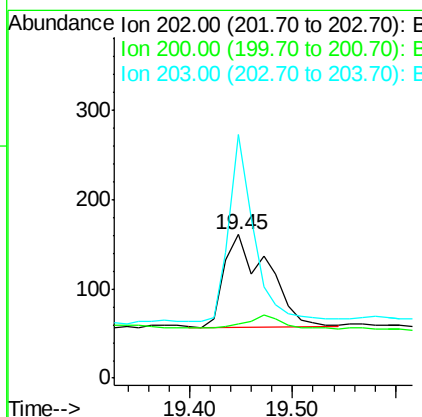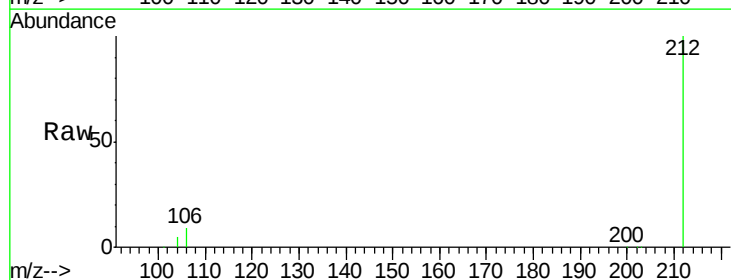

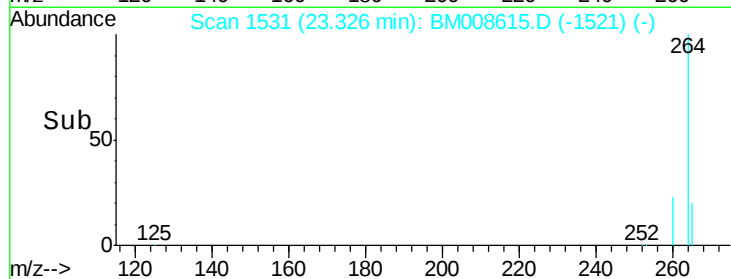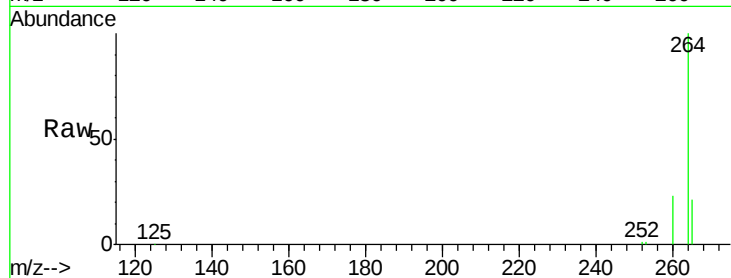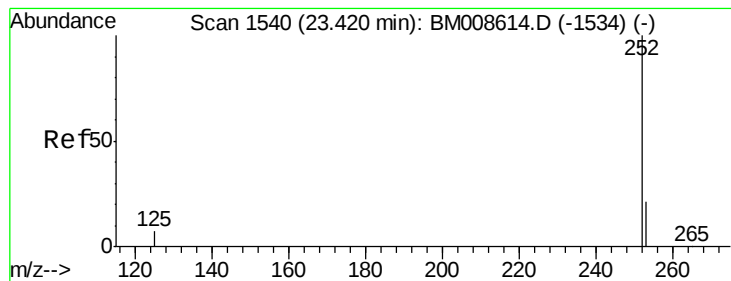

#23

Benzo(a)pyrene

Concen: 0.06 ng/ul

RT: 23.33 min Scan# 1531

Delta R.T. -0.09 min

Lab File: BM008615.D

Acq: 24 Dec 2016 04:01

Instrument :

BNA_M

ClientSampleId :

DA870

Tgt Ion: 252 Resp: 469

Ion Ratio Lower Upper

252 100

253 79.9 28.5 42.7#

125 57.7 18.1 27.1#

