

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
Data File : BM008614.D
Acq On : 24 Dec 2016 02:50
Operator : UM/SJ
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_M
LabSampleId :
SSTD0.464

Manual Integrations
APPROVED

sohil
12/26/2016 6:25:01 PM

Quant Time: Dec 24 04:56:22 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 23 23:37:39 2016
Response via : Initial Calibration

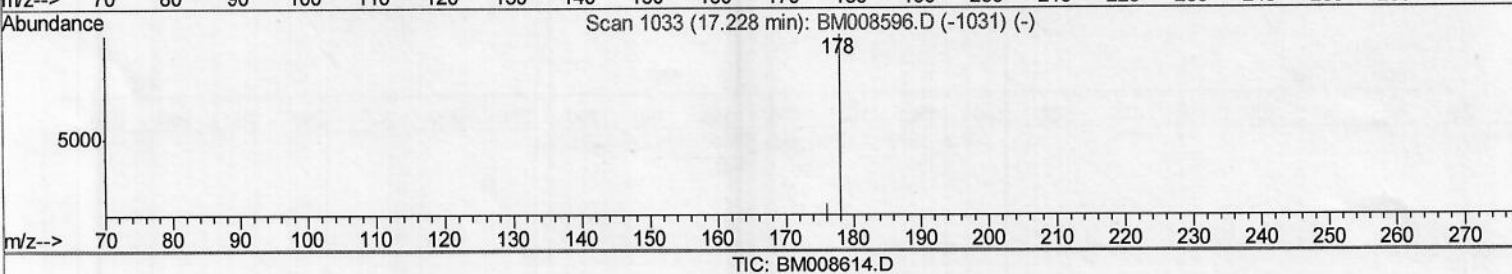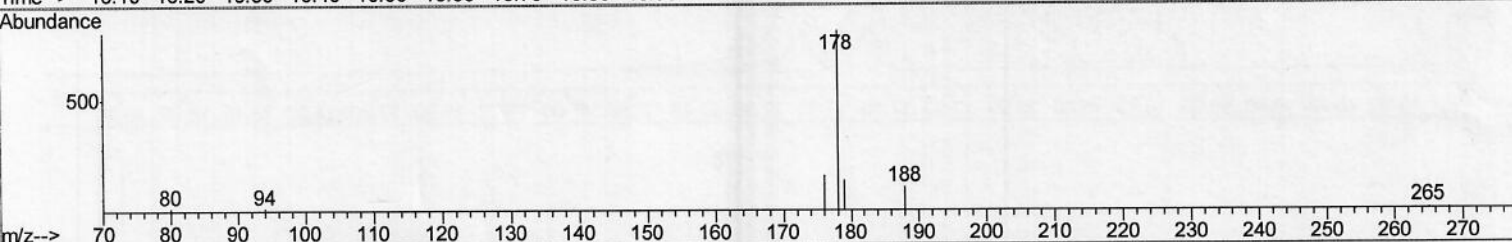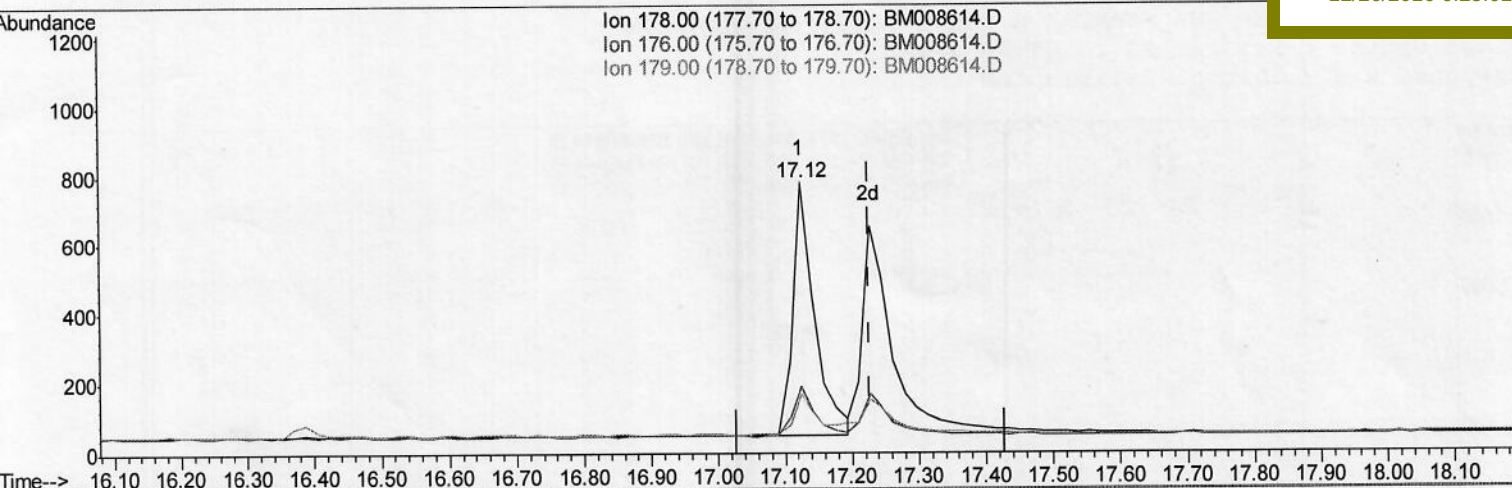

TIC: BM008614.D

(13) Anthracene

17.125min (-0.103) 0.41ng/ul

response 1659

Ion	Exp%	Act%
178.00	100	100
176.00	22.60	24.27
179.00	18.40	21.20
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
 Data File : BM008614.D
 Acq On : 24 Dec 2016 02:50
 Operator : UM/SJ
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 LabSampleId :
 SSTD0.464

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:25:01 PM

Quant Time: Dec 24 04:56:22 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 23:37:39 2016
 Response via : Initial Calibration

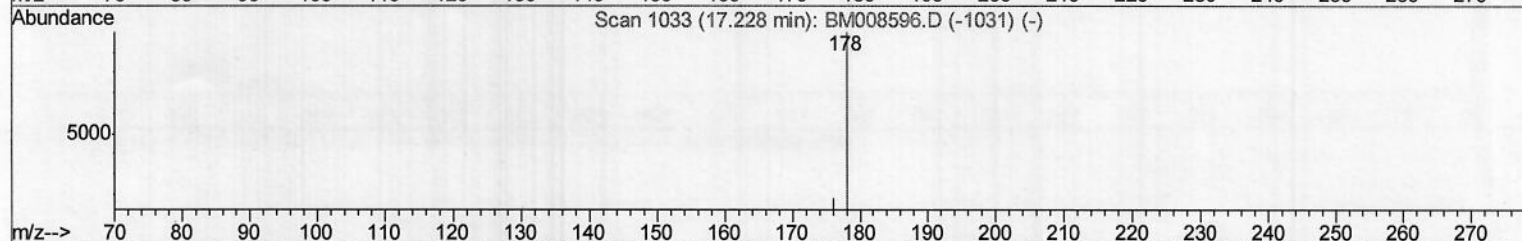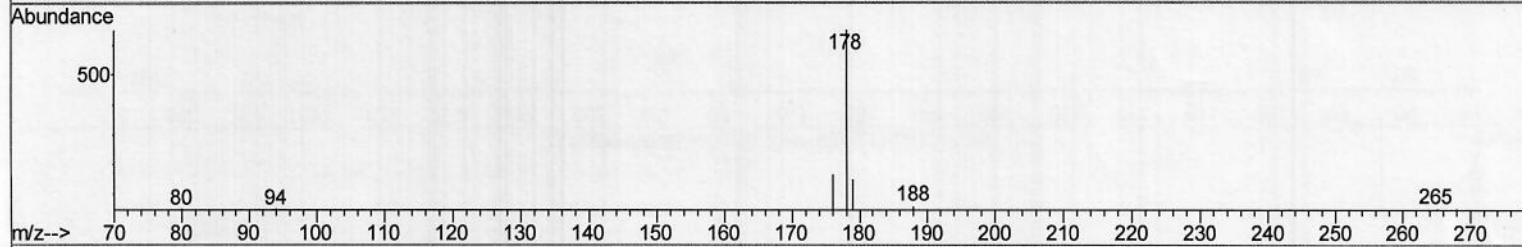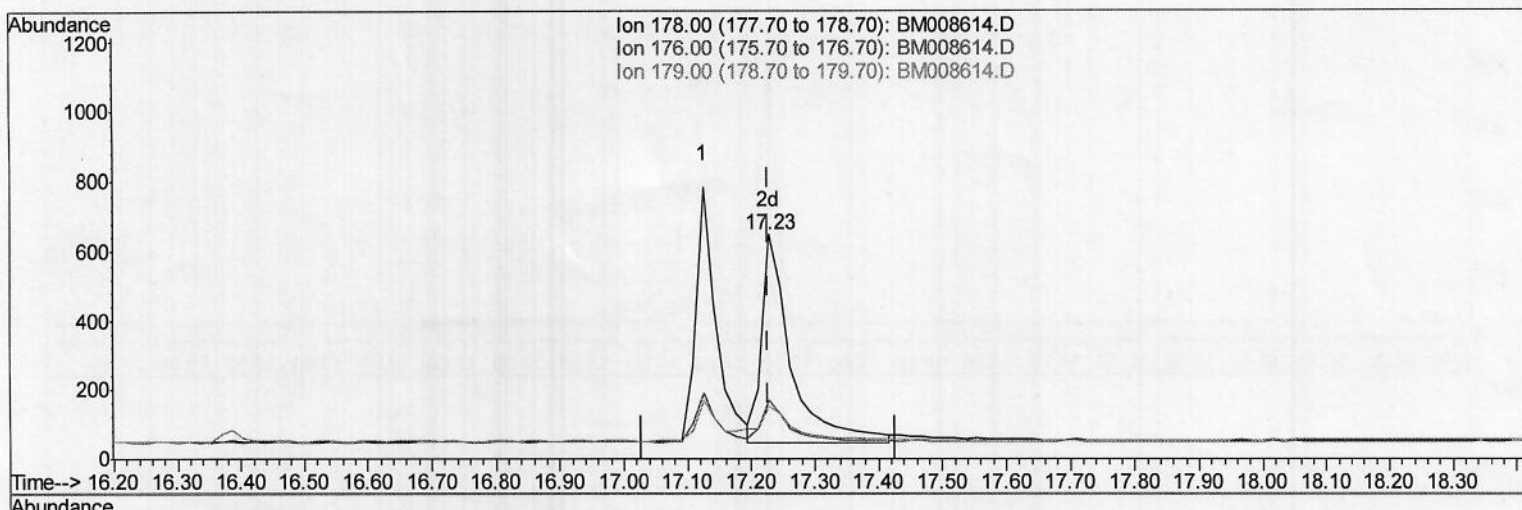

TIC: BM008614.D

(13) Anthracene

17.228min (-0.000) 0.47ng/ul m

response 1922

Ion	Exp%	Act%
178.00	100	100
176.00	22.60	25.69
179.00	18.40	22.92#
0.00	0.00	0.00

9.1
 12 | 27 | 16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
 Data File : BM008614.D
 Acq On : 24 Dec 2016 02:50
 Operator : UM/SJ
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
LabSampleId :
 SSTD0.464

Manual Integrations
APPROVED

sohil
 12/26/2016 6:25:01 PM

Quant Time: Dec 24 04:56:22 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 23:37:39 2016
 Response via : Initial Calibration

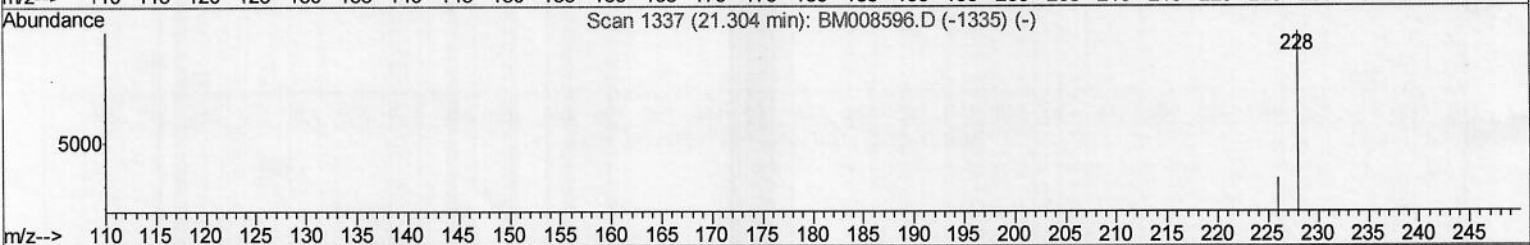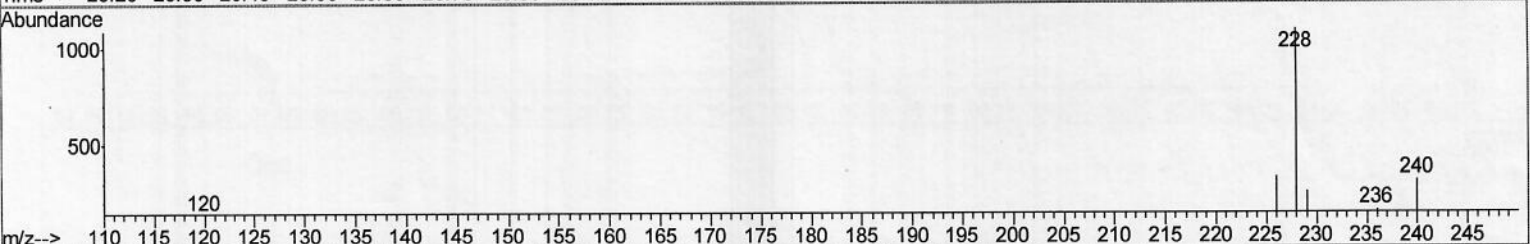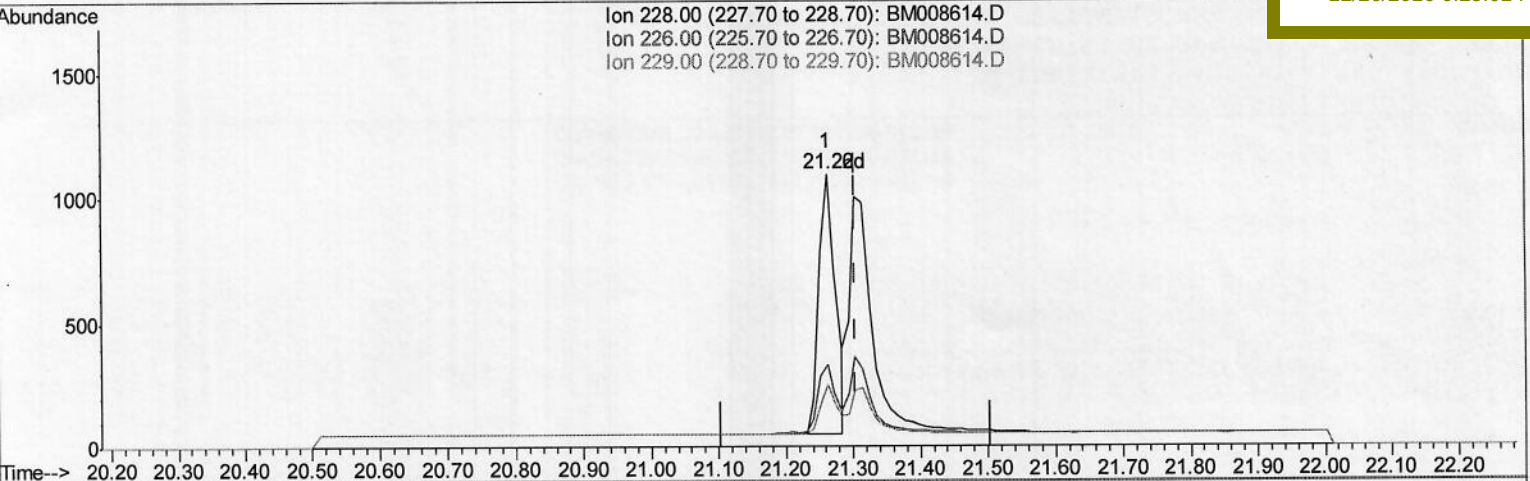

TIC: BM008614.D

(19) Chrysene

21.262min (-0.042) 0.36ng/ul

response 1817

Ion	Exp%	Act%
228.00	100	100
226.00	29.20	30.42
229.00	22.10	23.07
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
 Data File : BM008614.D
 Acq On : 24 Dec 2016 02:50
 Operator : UM/SJ
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 LabSampleId :
 SSTD0.464

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:25:01 PM

Quant Time: Dec 24 04:56:22 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 23:37:39 2016
 Response via : Initial Calibration

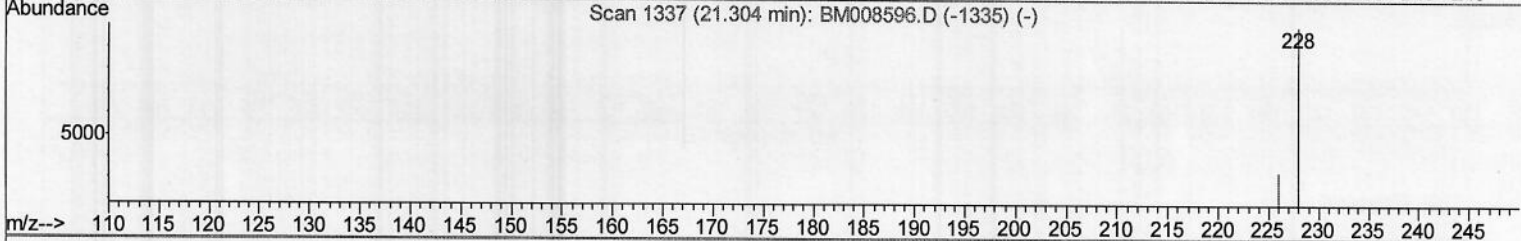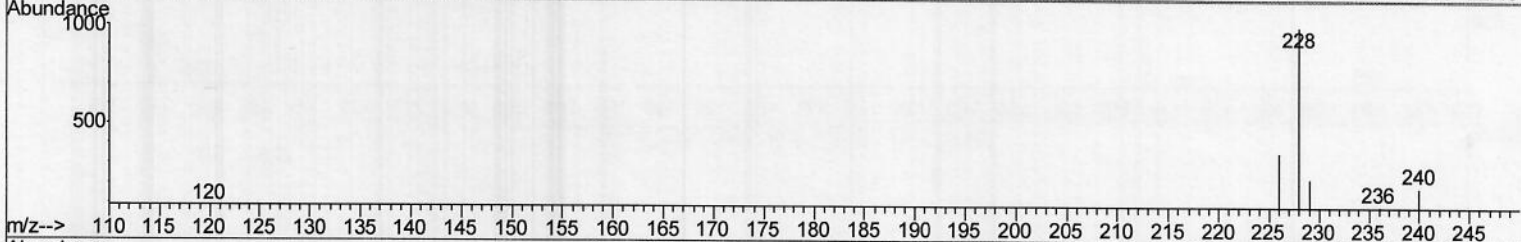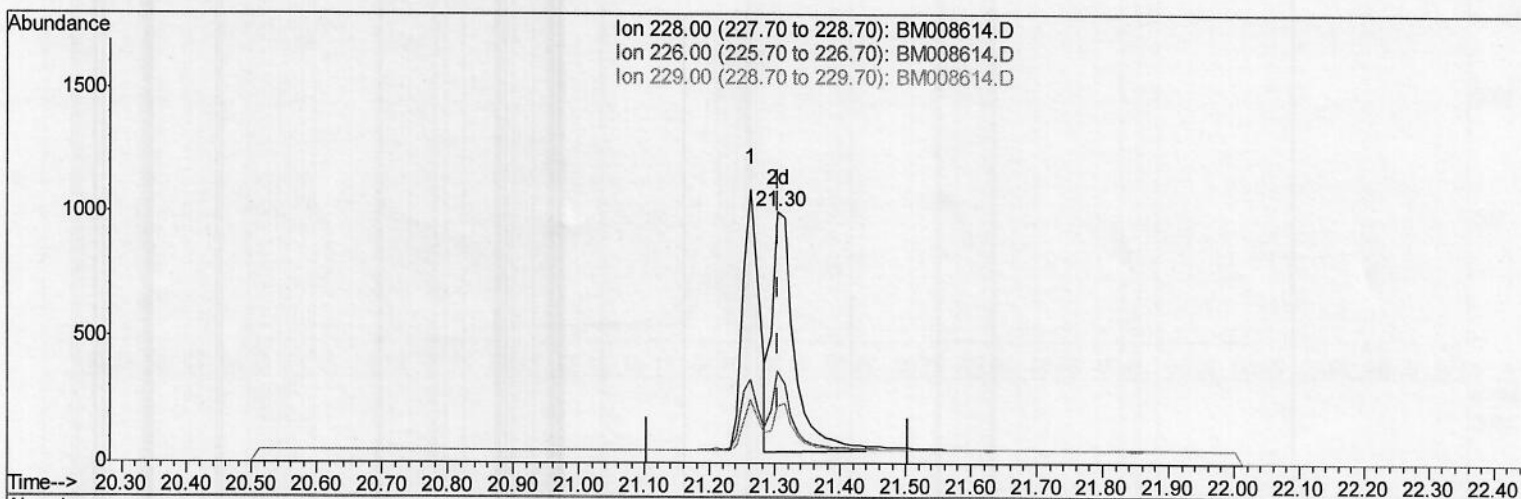

(19) Chrysene

21.304min (-0.000) 0.46ng/ul m

response 2322

Ion	Exp%	Act%
228.00	100	100
226.00	29.20	36.36#
229.00	22.10	22.88
0.00	0.00	0.00

29.5
 12/27/16

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
 Data File : BM008614.D
 Acq On : 24 Dec 2016 02:50
 Operator : UM/SJ
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 LabSampleId :
 SSTD0.464

Quant Time: Dec 24 04:57:17 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 23:37:39 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:25:01 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	366	0.40	ng/ul	0.00
2) Naphthalene-d8	10.50	136	1313	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.31	164	747	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.09	188	1380	0.40	ng/ul	0.00
16) Chrysene-d12	21.27	240	1389	0.40	ng/ul	0.00
20) Perylene-d12	23.50	264	1347	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.10	152	750	0.37	ng/ul	0.00
14) Fluoranthene-d10	19.11	212	1530	0.40	ng/ul	0.00
Target Compounds				Qvalue		
3) Naphthalene	10.55	128	1465	0.40	ng/ul#	78
5) 2-Methylnaphthalene	12.18	142	912	0.37	ng/ul	94
7) Acenaphthylene	14.04	152	1404	0.42	ng/ul#	88
8) Acenaphthene	14.38	153	1045	0.41	ng/ul	96
9) Fluorene	15.41	166	1112	0.38	ng/ul#	96
11) Pentachlorophenol	16.80	266	137	0.32	ng/ul	96
12) Phenanthrene	17.12	178	1659	0.39	ng/ul#	94
13) Anthracene	17.23	178	1922m	0.47	ng/ul	
15) Fluoranthene	19.14	202	2176	0.42	ng/ul	96
17) Pyrene	19.51	202	2321	0.43	ng/ul	96
18) Benzo(a)anthracene	21.26	228	1817	0.40	ng/ul	96
19) Chrysene	21.30	228	2322m	0.46	ng/ul	
21) Benzo(b)fluoranthene	22.84	252	1956	0.37	ng/ul	95
22) Benzo(k)fluoranthene	22.88	252	2222	0.43	ng/ul	94
23) Benzo(a)pyrene	23.42	252	2020	0.41	ng/ul	93
24) Indeno(1,2,3-cd)pyrene	25.77	276	2346	0.40	ng/ul#	93
25) Dibenzo(a,h)anthracene	25.77	278	1868	0.40	ng/ul#	88
26) Benzo(g,h,i)perylene	26.44	276	2054	0.41	ng/ul	95

2 9.5
 12/27/16

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
 Data File : BM008614.D
 Acq On : 24 Dec 2016 02:50
 Operator : UM/SJ
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 LabSampleId :
 SSTD0.464

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:25:01 PM

Quant Time: Dec 24 04:57:17 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 23 23:37:39 2016
 Response via : Initial Calibration

