

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122416\
 Data File : BM008632.D
 Acq On : 24 Dec 2016 14:40
 Operator : UM/SJ
 Sample : H5995-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Quant Time: Dec 26 13:41:49 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 03:21:10 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
ClientSampleId :
 DA874

Manual Integrations
APPROVED

sohil
 12/26/2016 6:26:52 PM

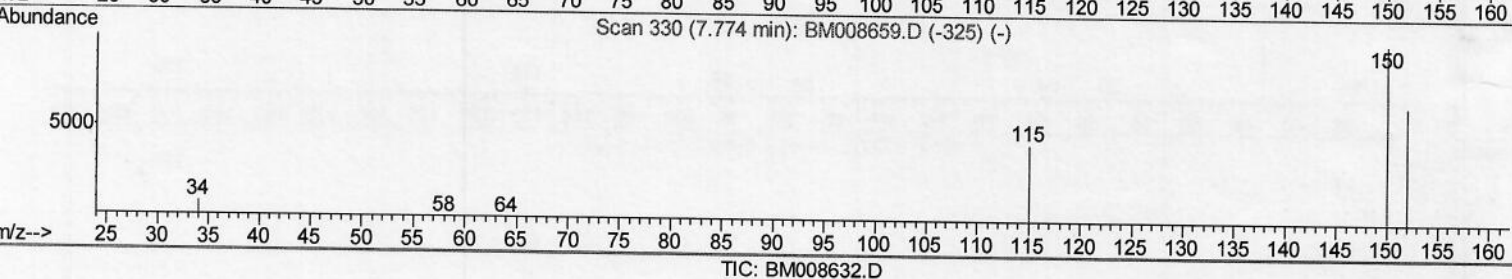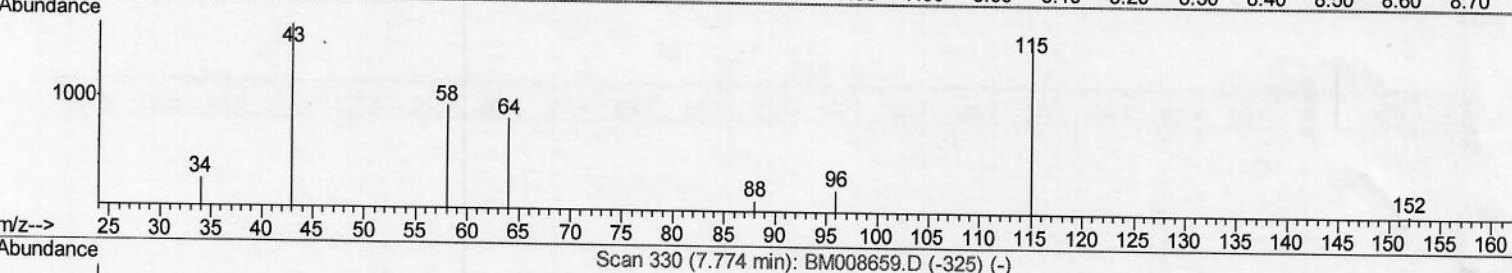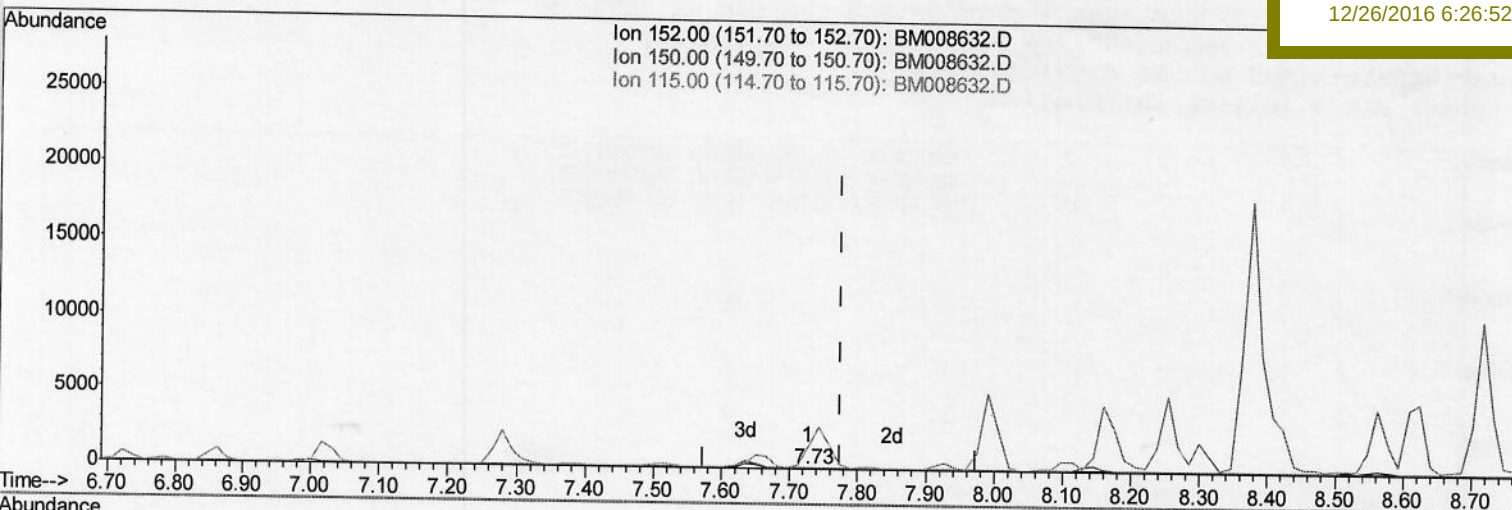

(1) 1,4-Dichlorobenzene-d4 (I)

7.728min (-0.046) 0.40ng/ul

response 31

Ion	Exp%	Act%
152.00	100	100
150.00	143.40	71.43#
115.00	64.90	2046.75#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM122416\
 Data File : BM008632.D
 Acq On : 24 Dec 2016 14:40
 Operator : UM/SJ
 Sample : H5995-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 Client Sample ID :
 DA874

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:26:52 PM

Quant Time: Dec 26 13:41:49 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 03:21:10 2016
 Response via : Initial Calibration

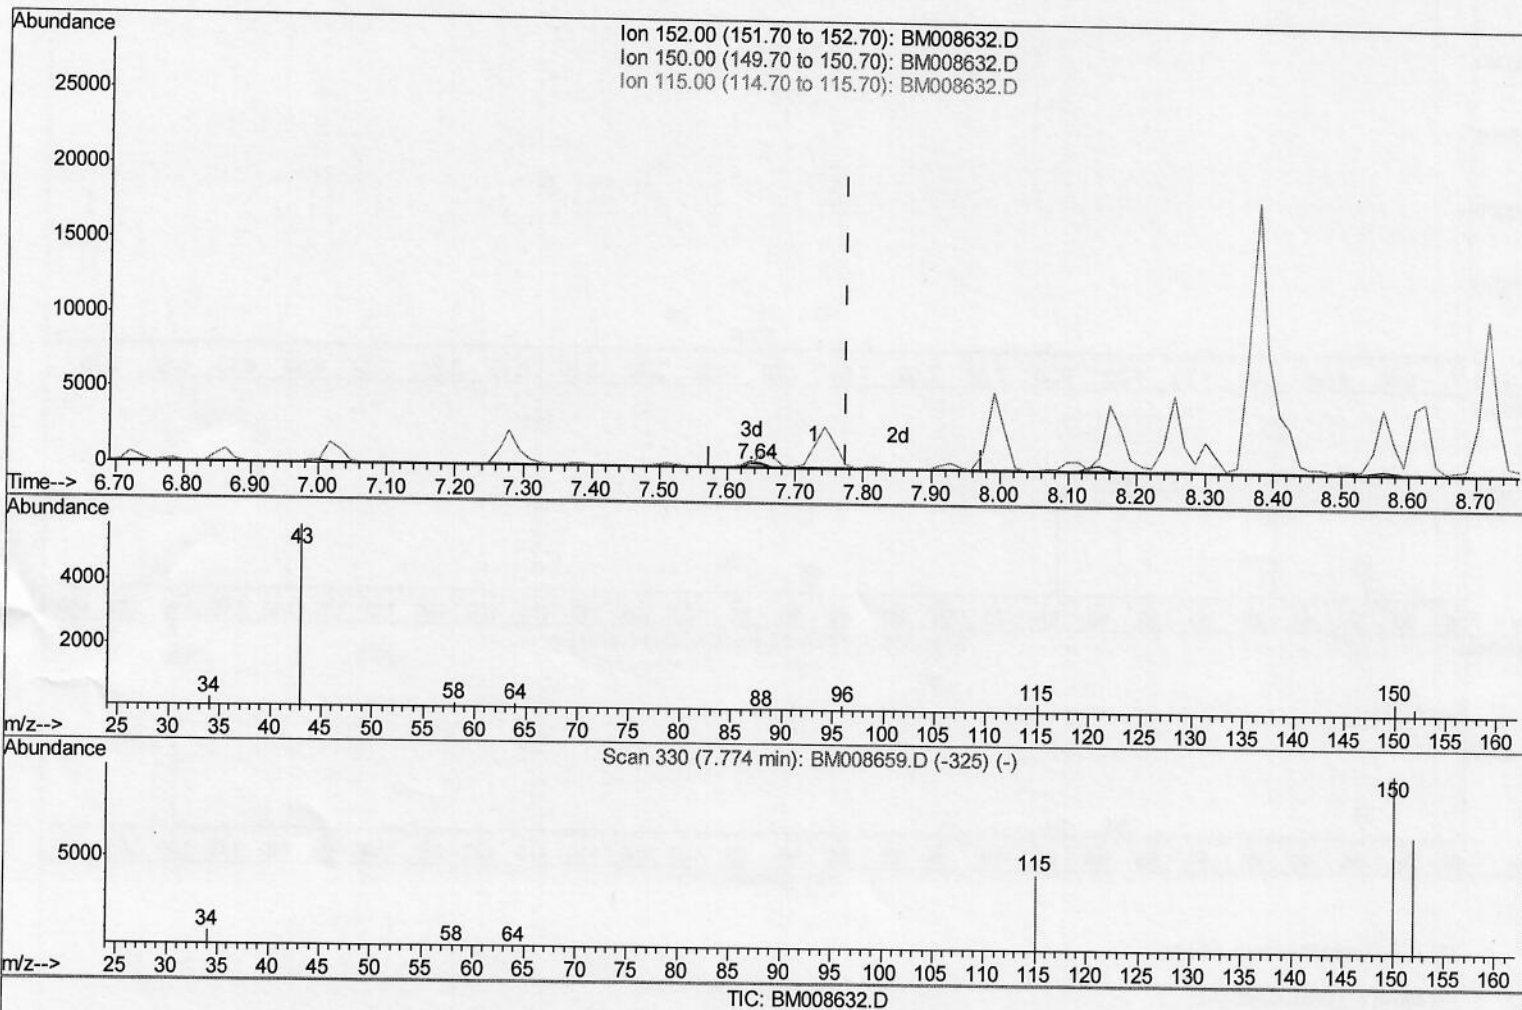

(1) 1,4-Dichlorobenzene-d4 (I)

7.635min (-0.139) 0.40ng/ul m

response 553

Ion Exp% Act%

152.00 100 100

150.00 143.40 151.45

115.00 64.90 105.47#

0.00 0.00 0.00

> 5.5
 12/27/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122416\
 Data File : BM008632.D
 Acq On : 24 Dec 2016 14:40
 Operator : UM/SJ
 Sample : H5995-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA874

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:26:52 PM

Quant Time: Dec 26 13:42:18 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 03:21:10 2016
 Response via : Initial Calibration

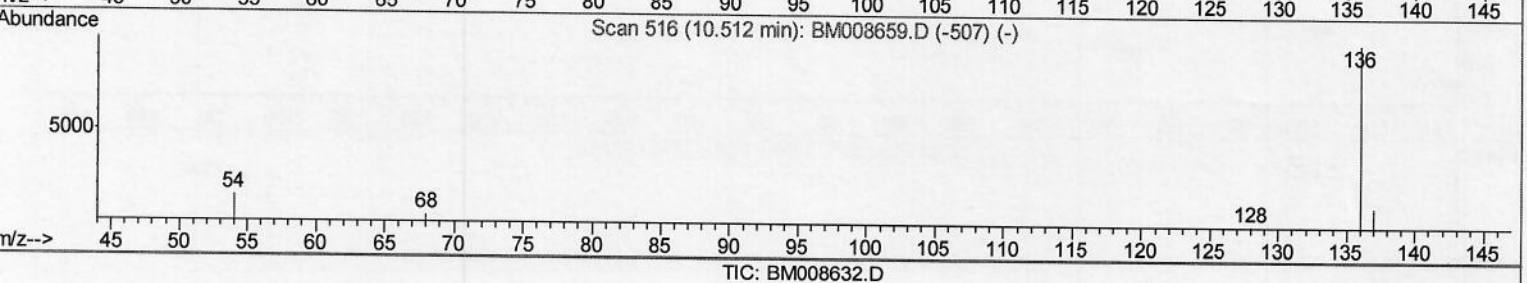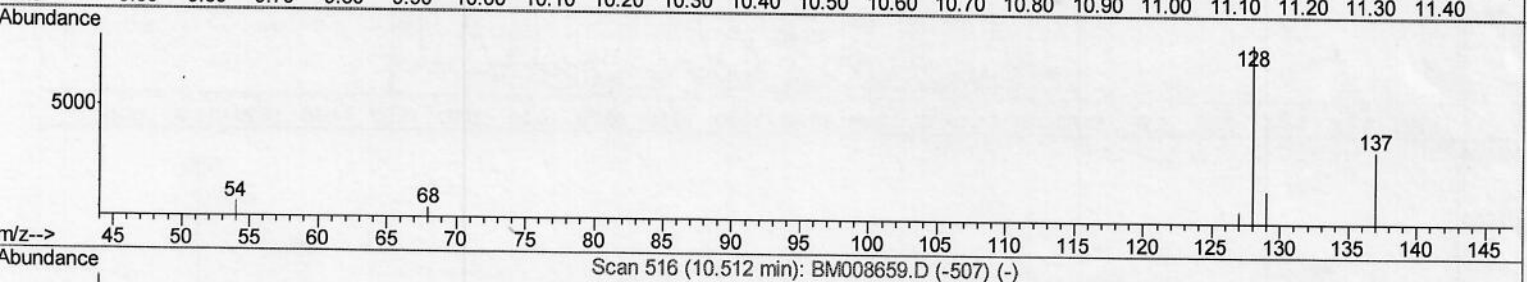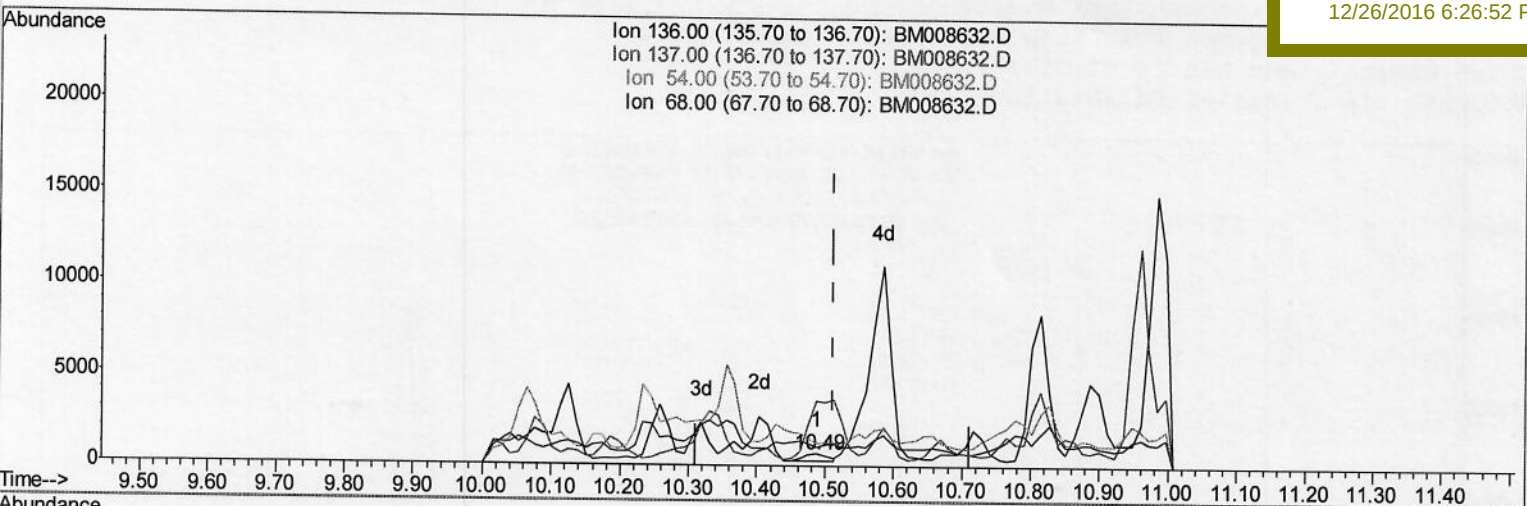

(2) Naphthalene-d8 (I)
 10.488min (-0.024) 0.40ng/ul
 response 892

Ion	Exp%	Act%
136.00	100	100
137.00	13.90	518.56#
54.00	15.50	182.18#
68.00	9.90	155.38#

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122416\
 Data File : BM008632.D
 Acq On : 24 Dec 2016 14:40
 Operator : UM/SJ
 Sample : H5995-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 Client Sampled :
 DA874

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:26:52 PM

Quant Time: Dec 26 13:42:18 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 03:21:10 2016
 Response via : Initial Calibration

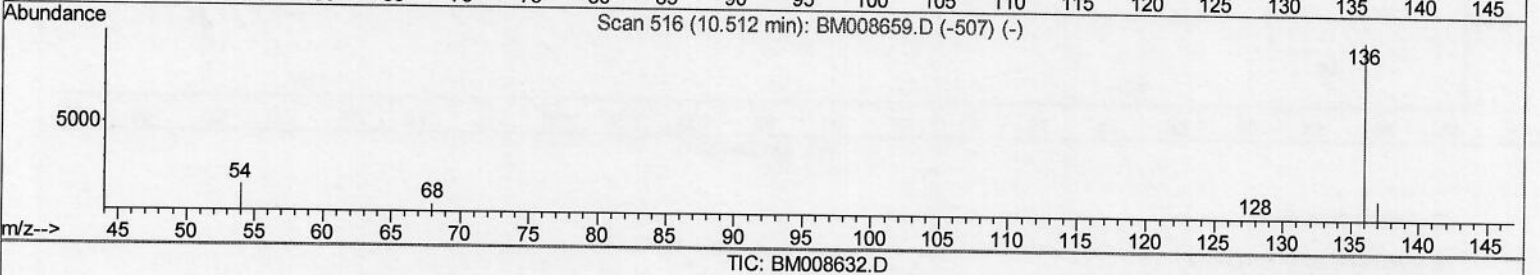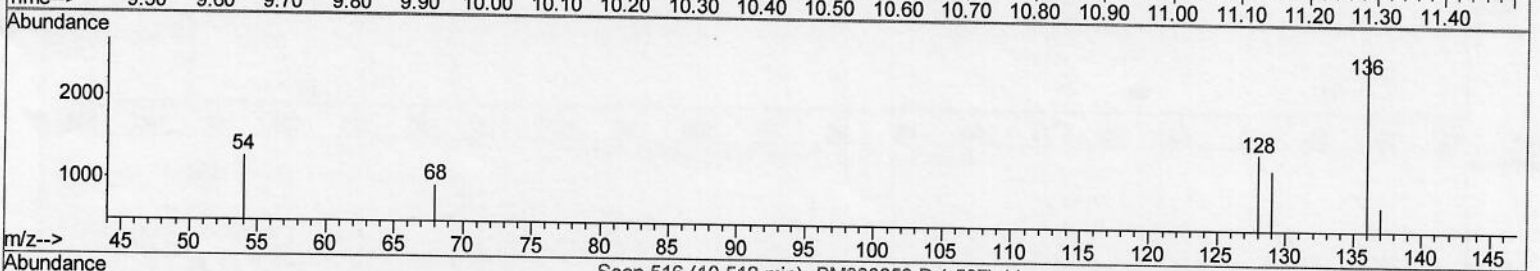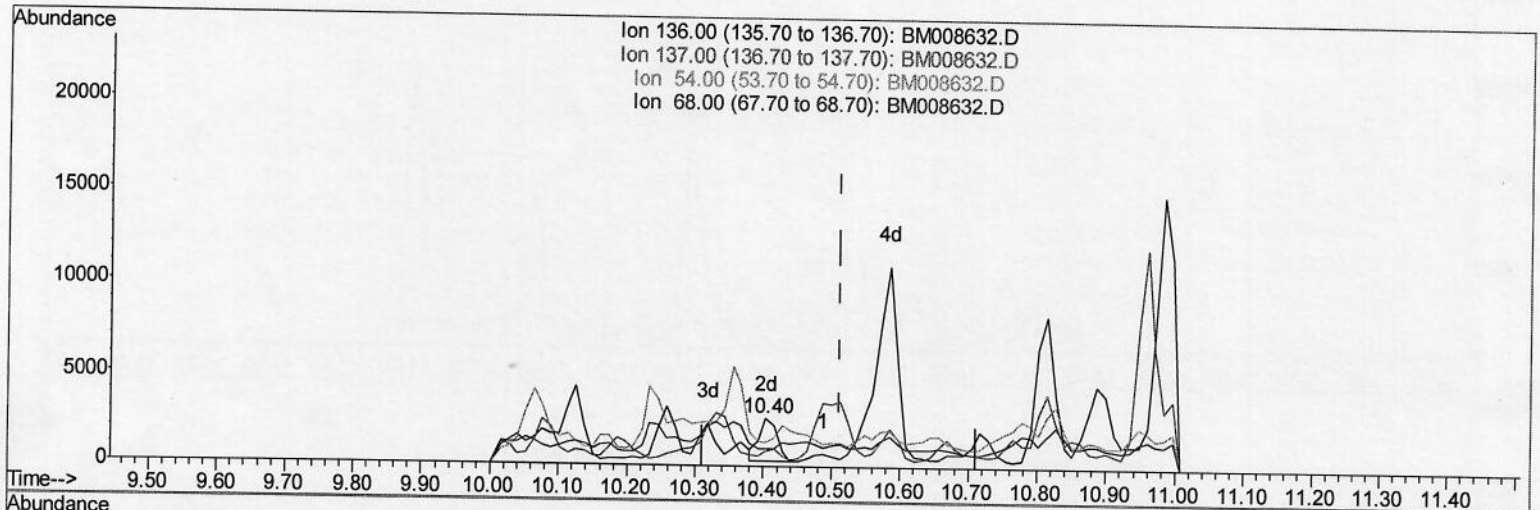

(2) Naphthalene-d8 (I)

10.403min (-0.109) 0.40ng/ul m

response 4350

Ion	Exp%	Act%
136.00	100	100
137.00	13.90	29.42#
54.00	15.50	47.43#
68.00	9.90	34.56#

5.5
 12/27/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122416\
Data File : BM008632.D
Acq On : 24 Dec 2016 14:40
Operator : UM/SJ
Sample : H5995-09
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA874

Manual Integrations
APPROVED

sohil
12/26/2016 6:26:52 PM

Quant Time: Dec 26 13:42:49 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 26 03:21:10 2016
Response via : Initial Calibration

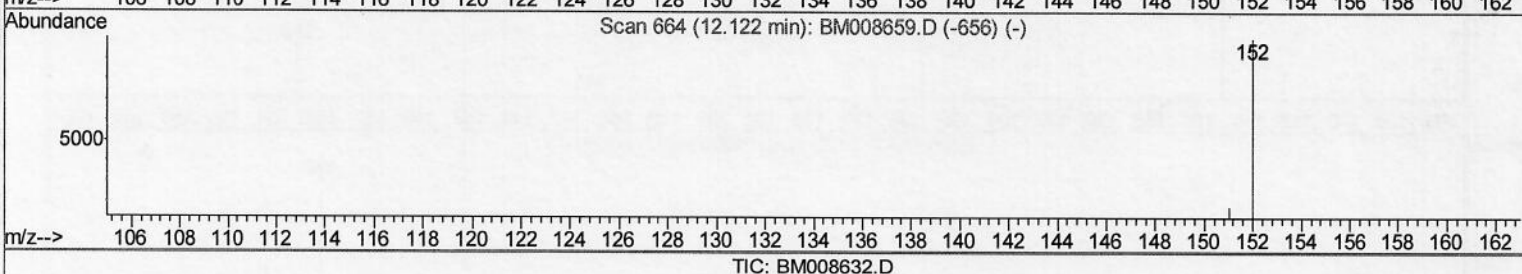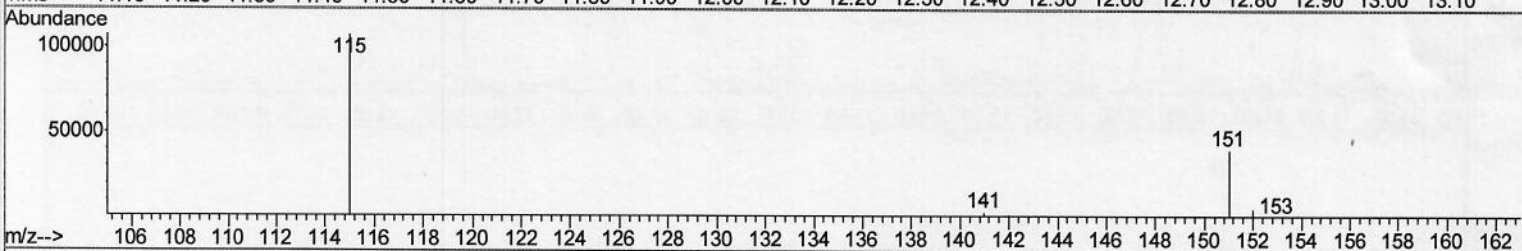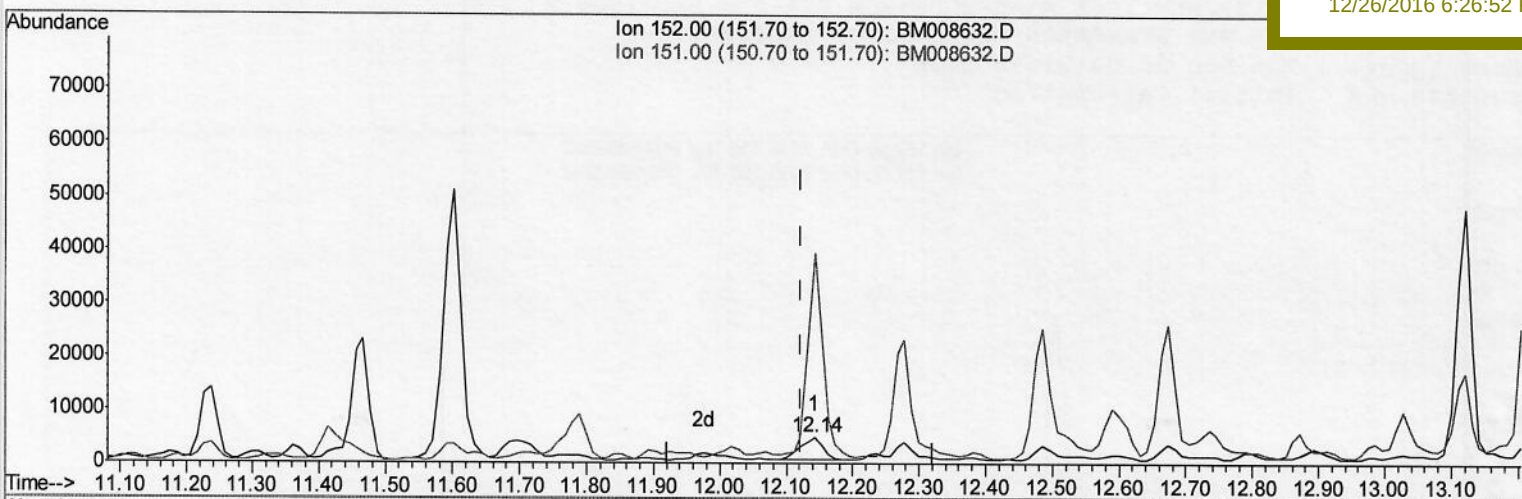

(4) 2-Methylnaphthalene-d10 (SURR)

12.143min (+0.021) 1.53ng/ul

response 10212

Ion	Exp%	Act%
152.00	100	100
151.00	19.30	604.51#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122416\
 Data File : BM008632.D
 Acq On : 24 Dec 2016 14:40
 Operator : UM/SJ
 Sample : H5995-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA874

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:26:52 PM

Quant Time: Dec 26 13:42:49 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 03:21:10 2016
 Response via : Initial Calibration

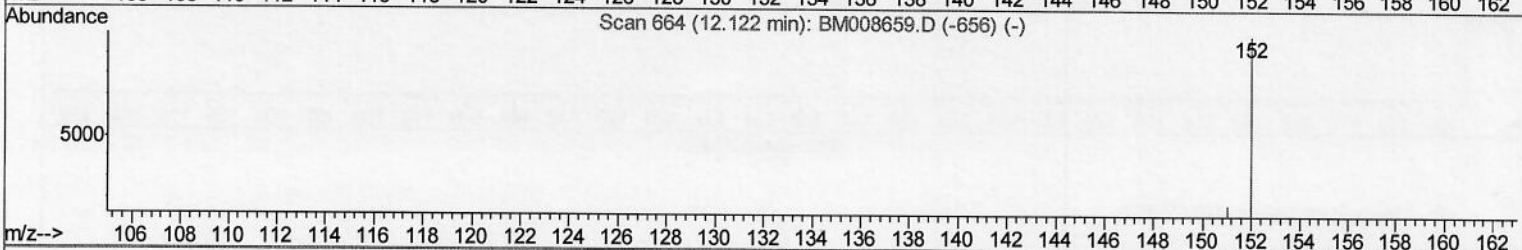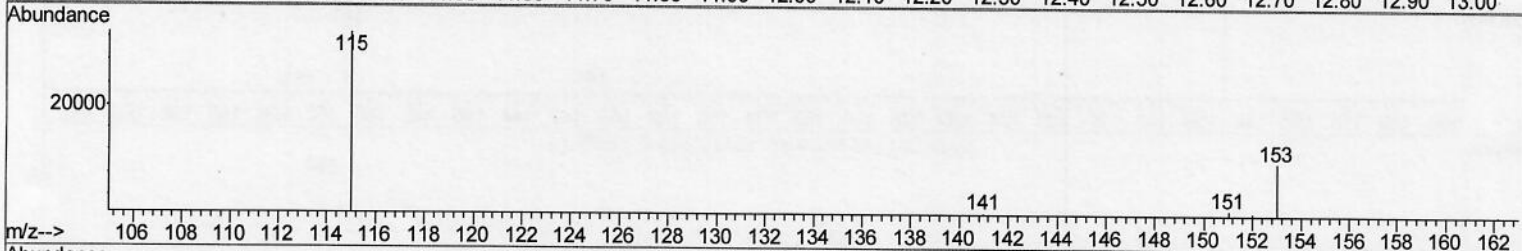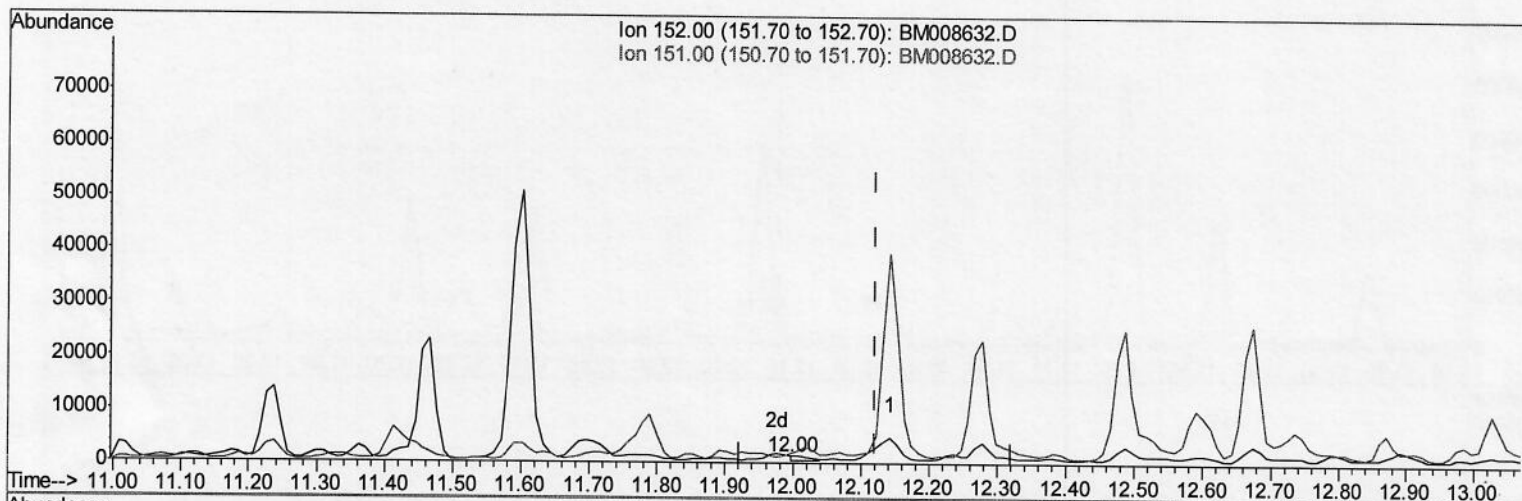

TIC: BM008632.D

(4) 2-Methylnaphthalene-d10 (SURR)

11.997min (-0.125) 0.19ng/ul m

response 1283

Ion Exp% Act%

152.00 100 100

151.00 19.30 4811.61#

0.00 0.00 0.00

0.00 0.00 0.00

9.9
 12/27/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122416\
 Data File : BM008632.D
 Acq On : 24 Dec 2016 14:40
 Operator : UM/SJ
 Sample : H5995-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA874

Quant Time: Dec 26 13:42:49 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 03:21:10 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:26:52 PM

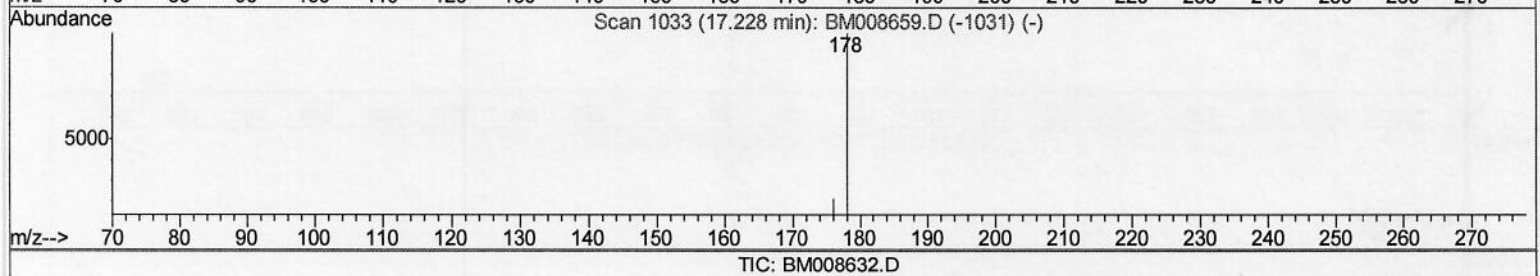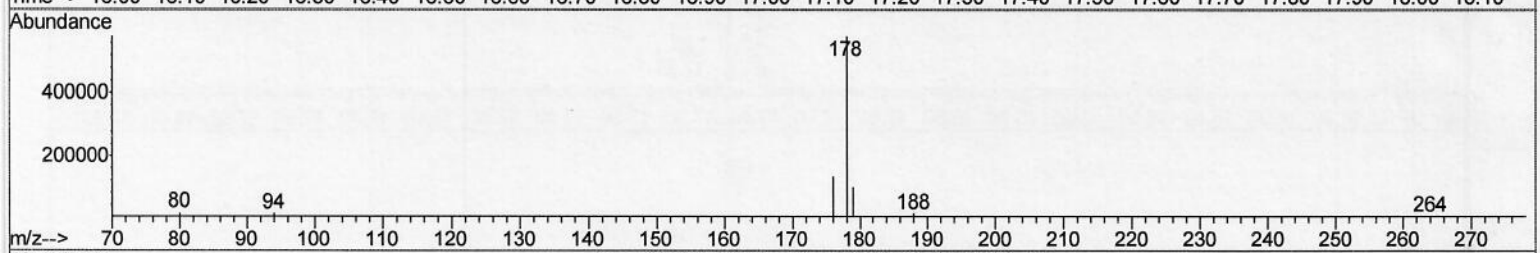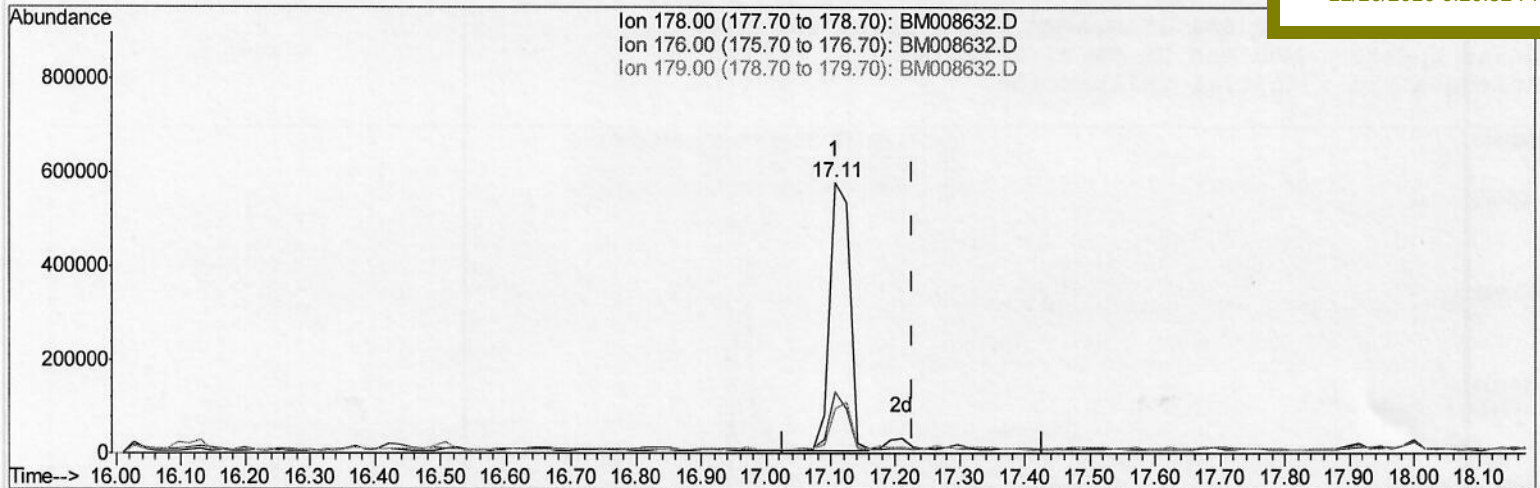

TIC: BM008632.D

(13) Anthracene

17.108min (-0.120) 11.83ng/ul

response 1243638

Ion	Exp%	Act%
178.00	100	100
176.00	22.60	22.84
179.00	18.40	16.39
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122416\
 Data File : BM008632.D
 Acq On : 24 Dec 2016 14:40
 Operator : UM/SJ
 Sample : H5995-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 Client Sample ID :
 DA874

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:26:52 PM

Quant Time: Dec 26 13:42:49 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 03:21:10 2016
 Response via : Initial Calibration

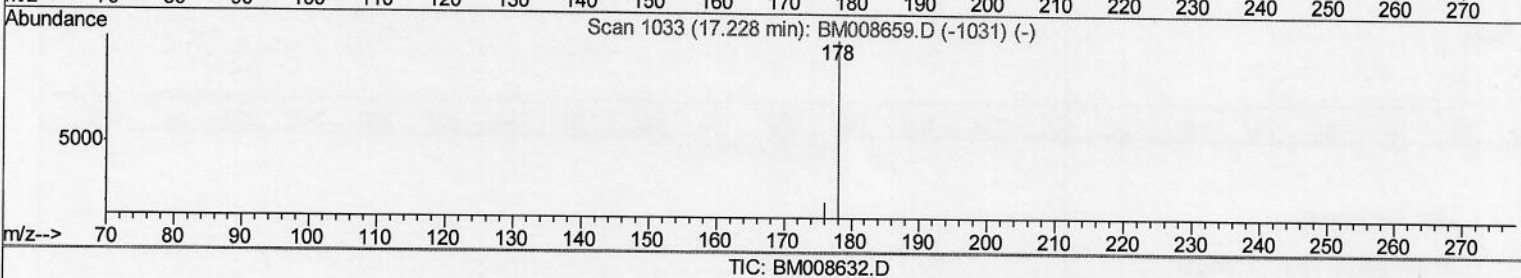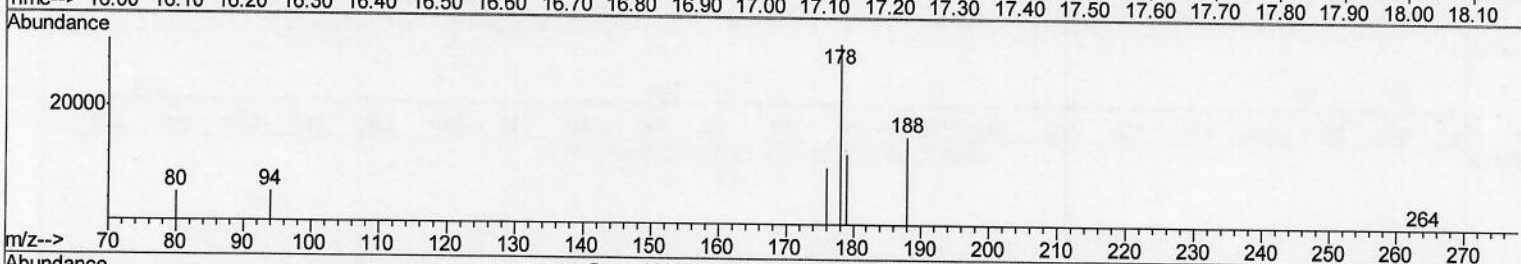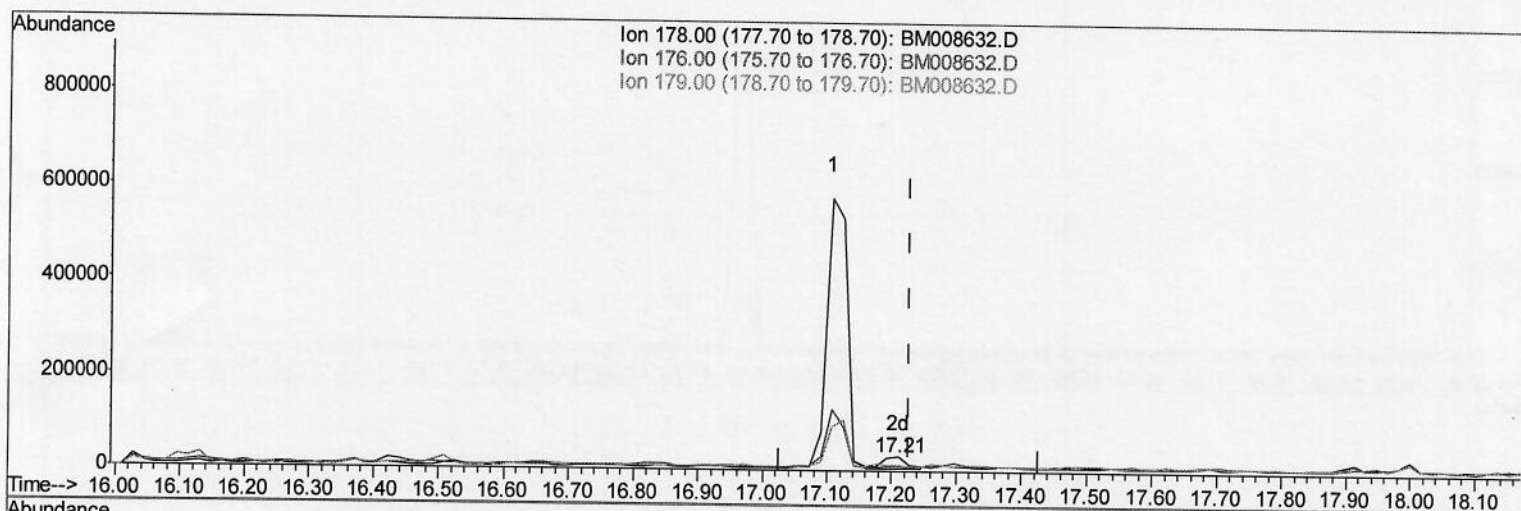

TIC: BM008632.D

(13) Anthracene

17.211min (-0.017) 0.67ng/ul m

response 70339

Ion	Exp%	Act%
178.00	100	100
176.00	22.60	32.08#
179.00	18.40	39.06#
0.00	0.00	0.00

5.7
 12/27/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122416\
Data File : BM008632.D
Acq On : 24 Dec 2016 14:40
Operator : UM/SJ
Sample : H5995-09
Misc :
ALS Vial : 37 Sample Multiplier: 1

Quant Time: Dec 26 13:42:49 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 26 03:21:10 2016
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DA874

Manual Integrations
APPROVED

sohil
12/26/2016 6:26:52 PM

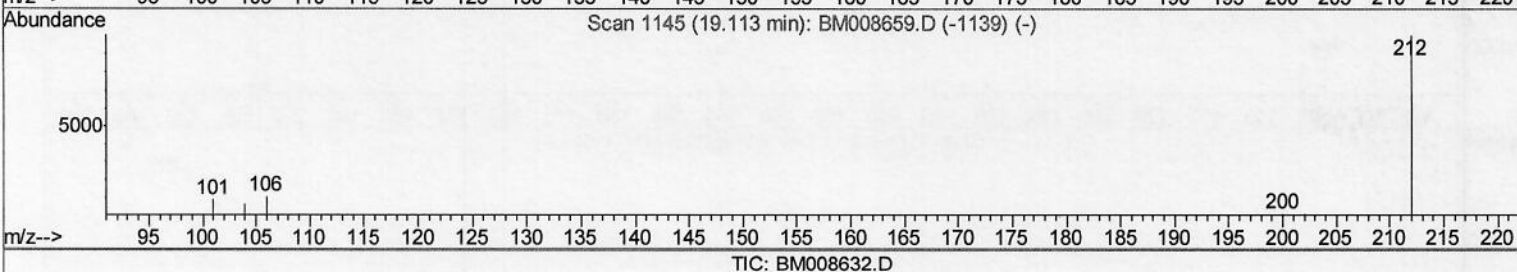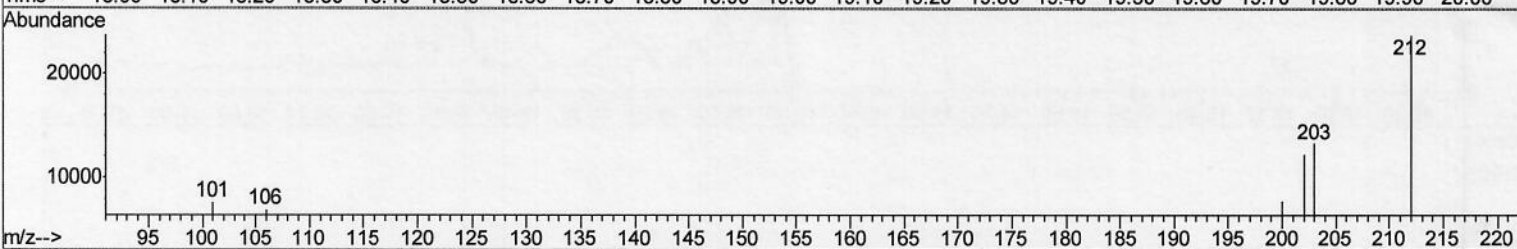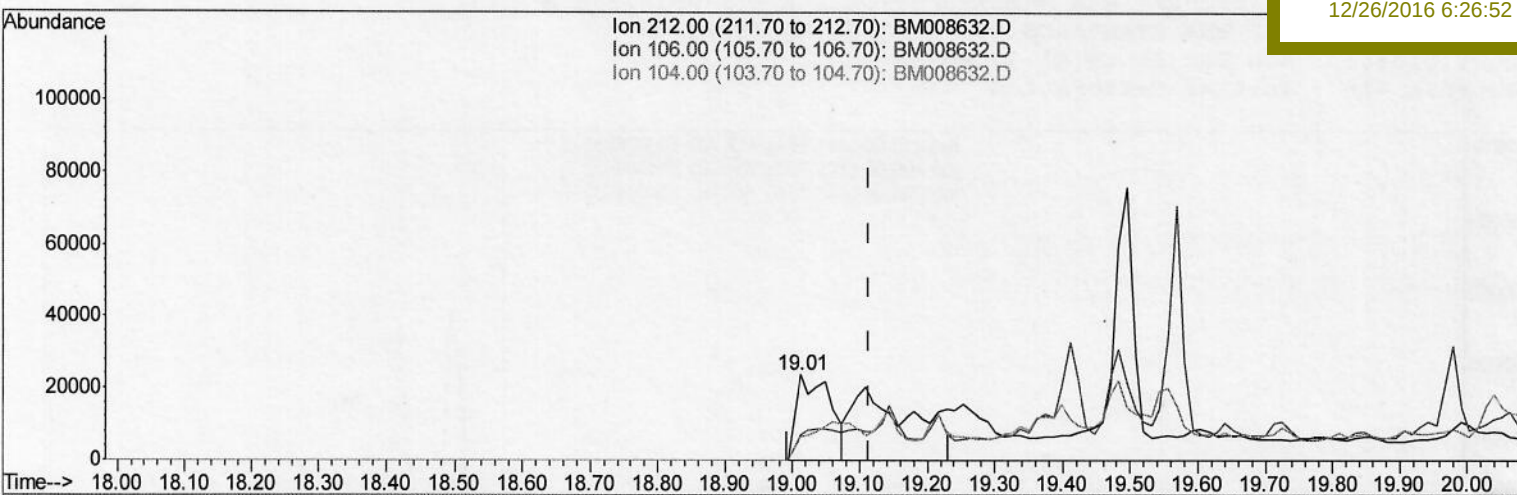

(14) Fluoranthene-d10 (SURR)

19.012min (-0.102) 0.90ng/ul

response 88111

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122416\
 Data File : BM008632.D
 Acq On : 24 Dec 2016 14:40
 Operator : UM/SJ
 Sample : H5995-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 DA874

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:26:52 PM

Quant Time: Dec 26 13:42:49 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 03:21:10 2016
 Response via : Initial Calibration

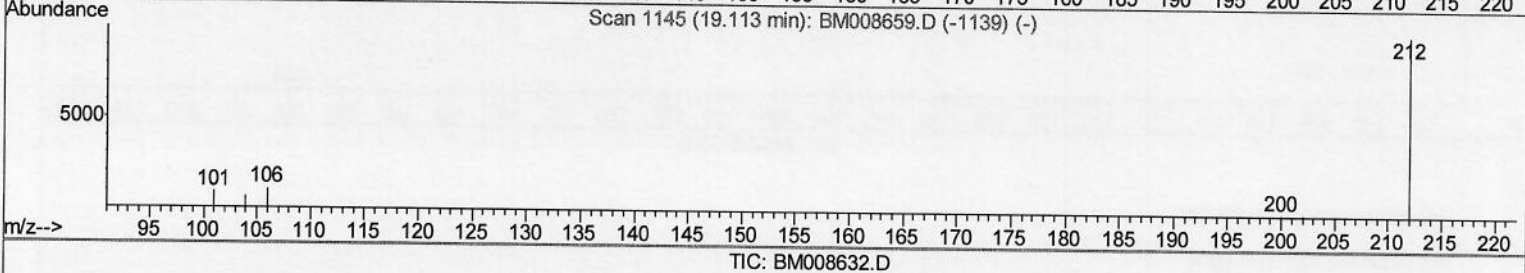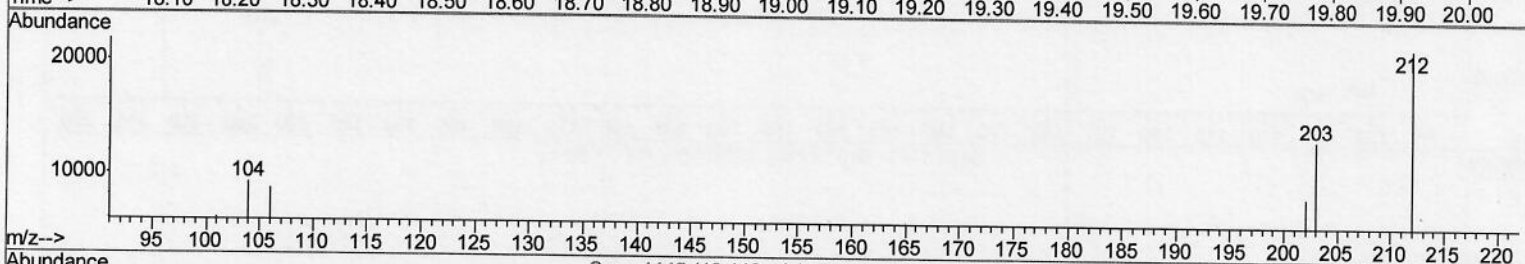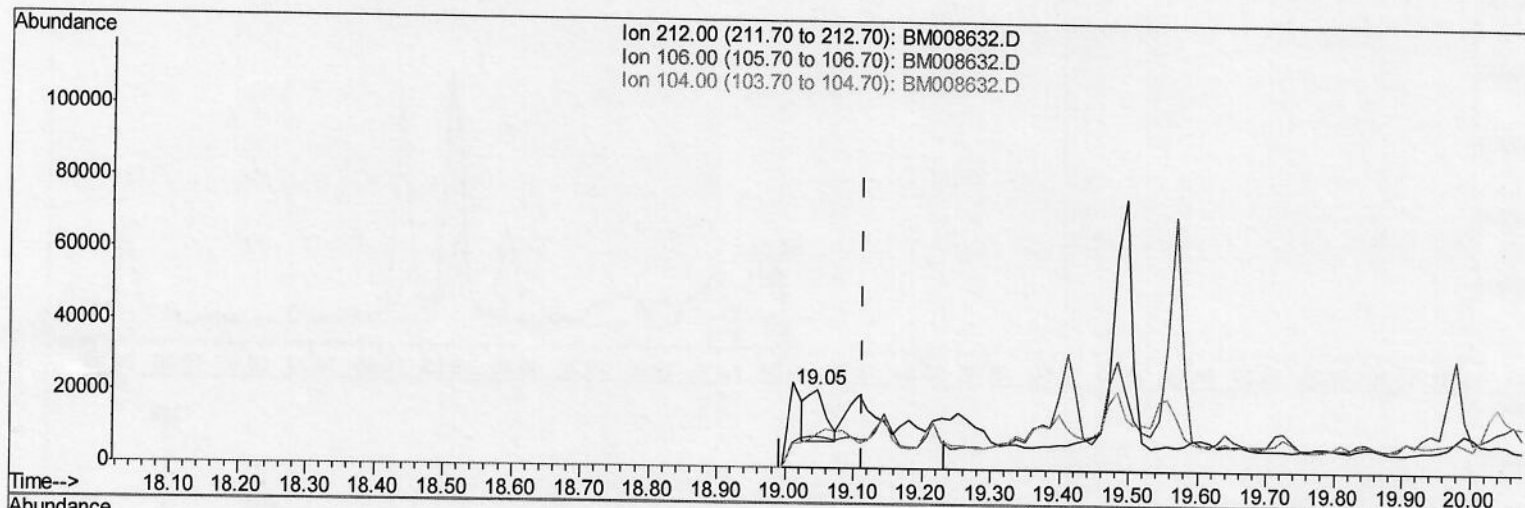

(14) Fluoranthene-d10 (SURR)

19.048min (-0.065) 0.27ng/ul m

response 26545

Ion Exp% Act%

212.00 100 100

106.00 18.30 0.00#

104.00 15.60 0.00#

0.00 0.00 0.00

79.9
 12/27/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122416\
 Data File : BM008632.D
 Acq On : 24 Dec 2016 14:40
 Operator : UM/SJ
 Sample : H5995-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Quant Time: Dec 26 13:42:49 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 03:21:10 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 DA874

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:26:52 PM

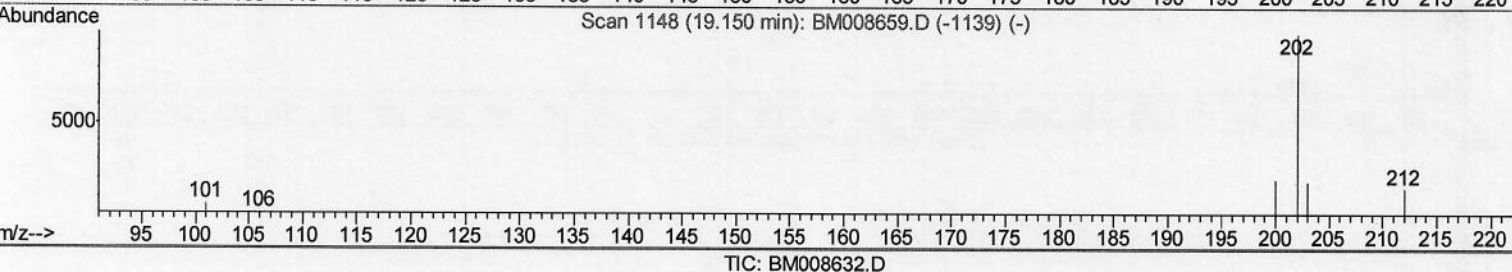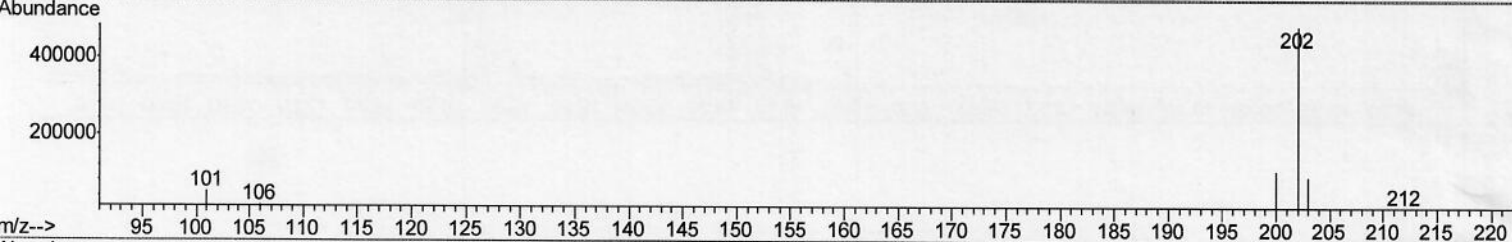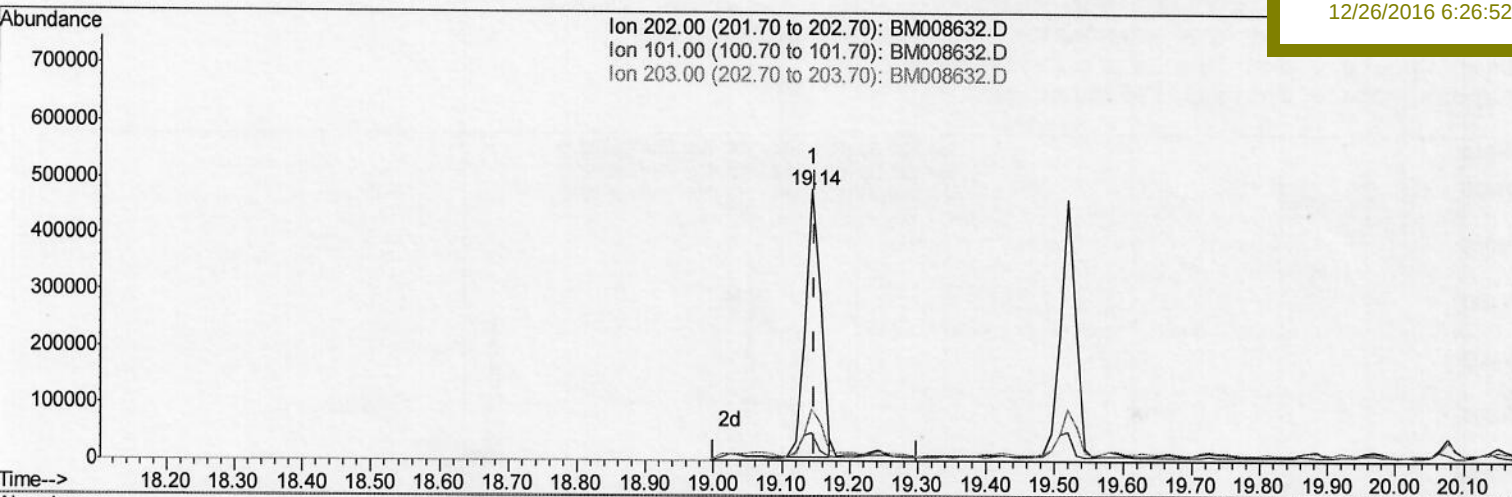

(15) Fluoranthene (C)

19.145min (-0.005) 5.61ng/ul

response 745120

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	10.69
203.00	19.50	19.09
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122416\
 Data File : BM008632.D
 Acq On : 24 Dec 2016 14:40
 Operator : UM/SJ
 Sample : H5995-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA874

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:26:52 PM

Quant Time: Dec 26 13:42:49 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 03:21:10 2016
 Response via : Initial Calibration

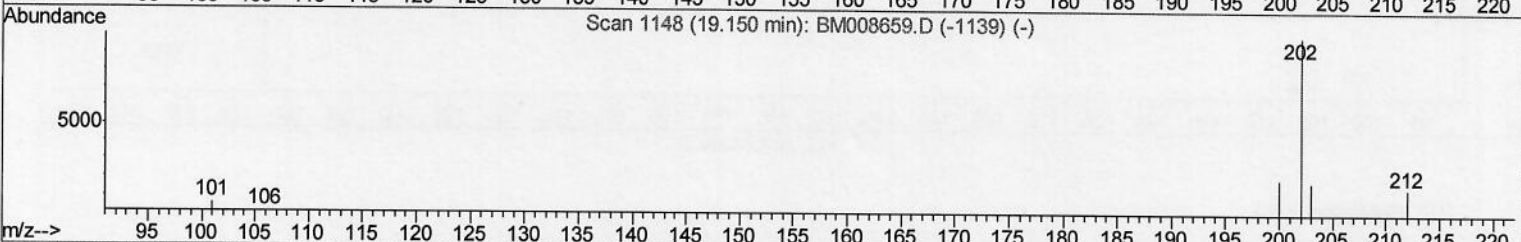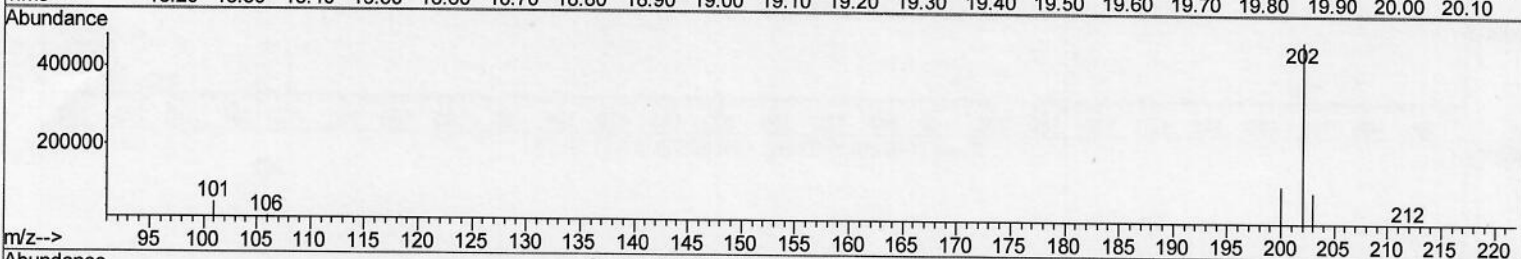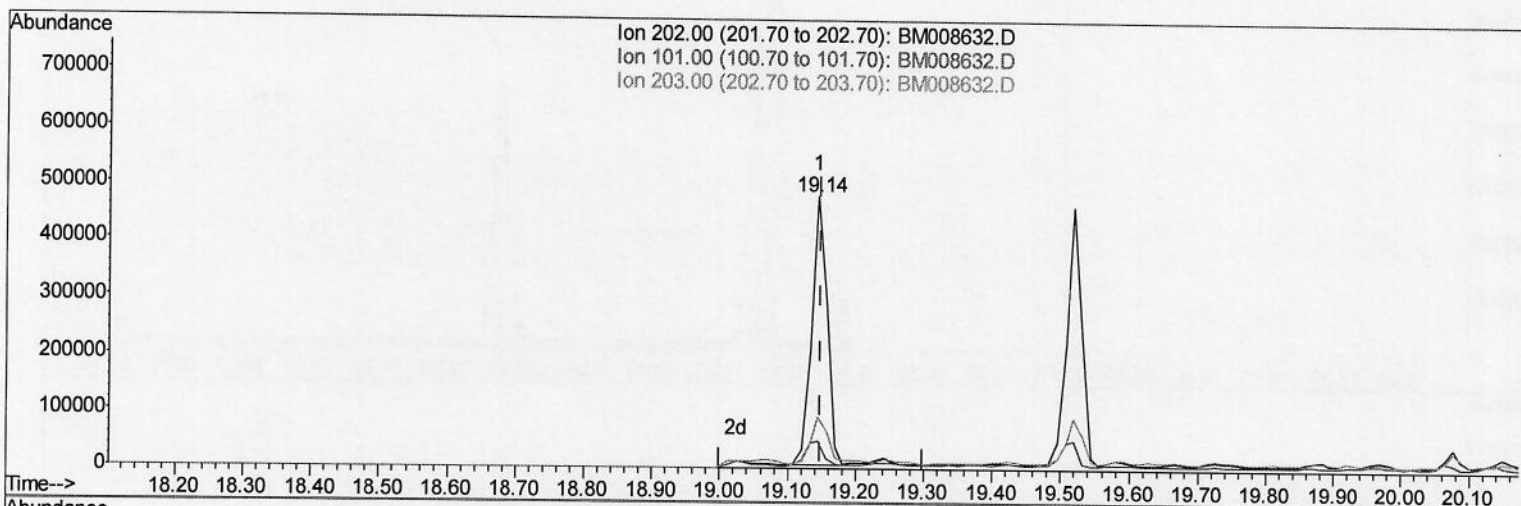

TIC: BM008632.D

(15) Fluoranthene (C)

19.145min (-0.005) 5.64ng/ul m

response 748457

Ion Exp% Act%

202.00 100 100

101.00 10.30 10.69

203.00 19.50 19.09

0.00 0.00 0.00

25.7
 12/29/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122416\
 Data File : BM008632.D
 Acq On : 24 Dec 2016 14:40
 Operator : UM/SJ
 Sample : H5995-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA874

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:26:52 PM

Quant Time: Dec 26 13:42:49 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 03:21:10 2016
 Response via : Initial Calibration

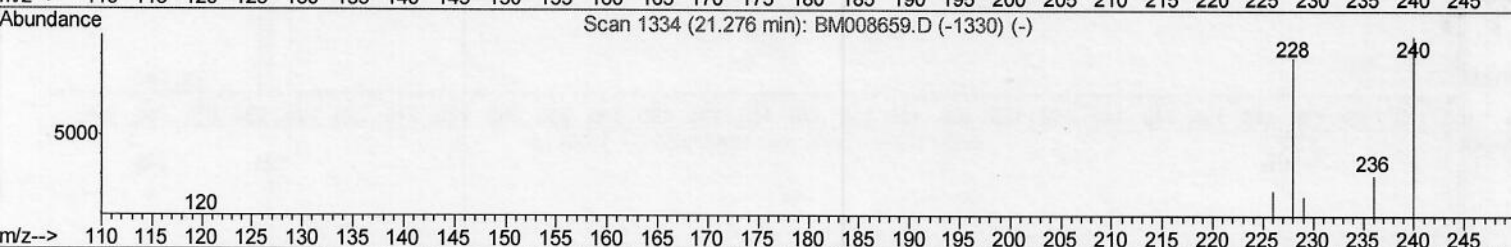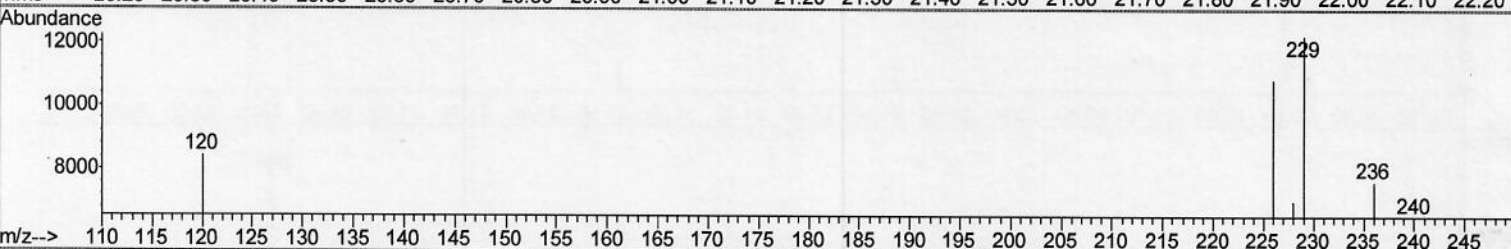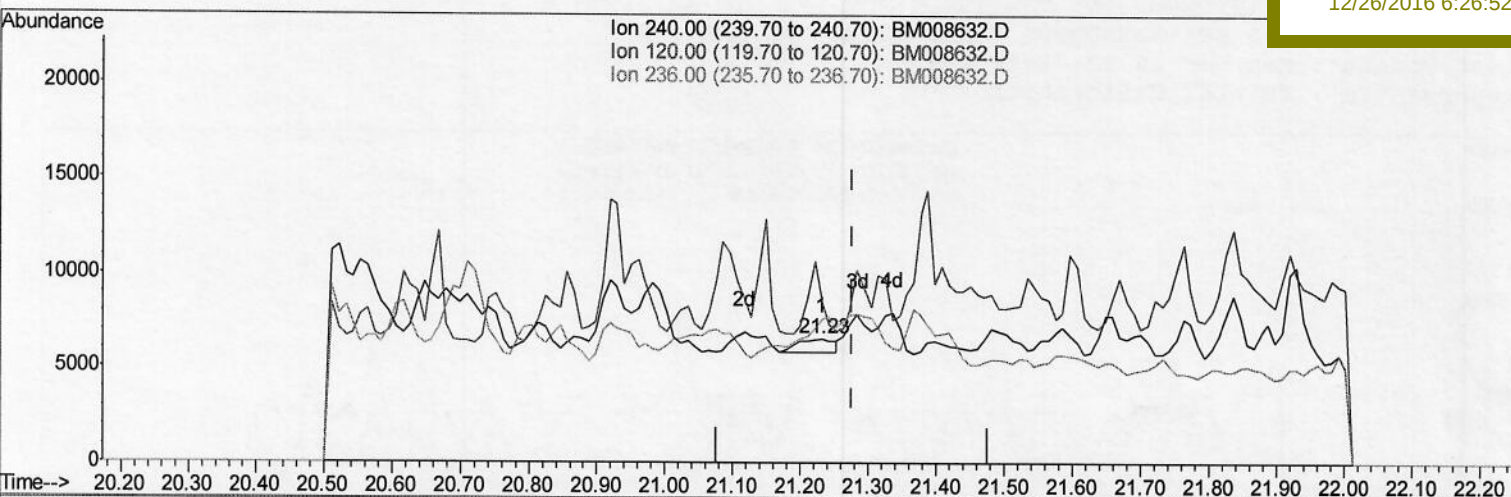

TIC: BM008632.D

(16) Chrysene-d12 (I)
 21.231min (-0.045) 0.40ng/ul
 response 2710

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	128.58#
236.00	34.90	116.12#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122416\
 Data File : BM008632.D
 Acq On : 24 Dec 2016 14:40
 Operator : UM/SJ
 Sample : H5995-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA874

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:26:52 PM

Quant Time: Dec 26 13:42:49 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 03:21:10 2016
 Response via : Initial Calibration

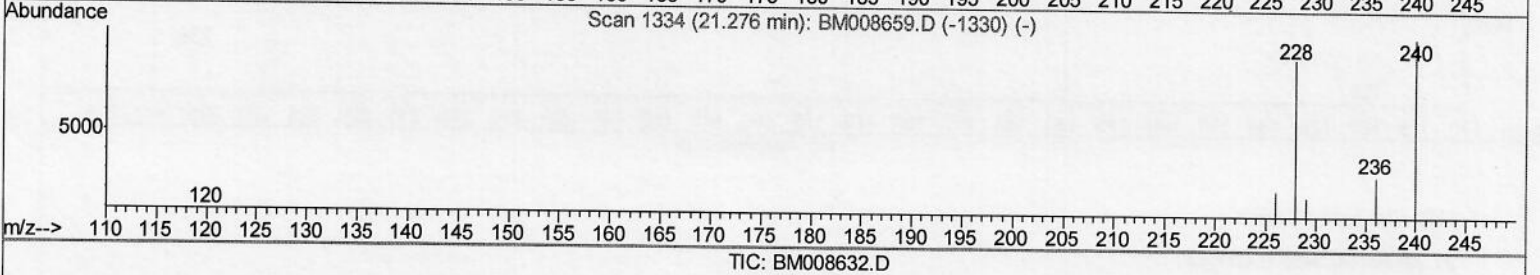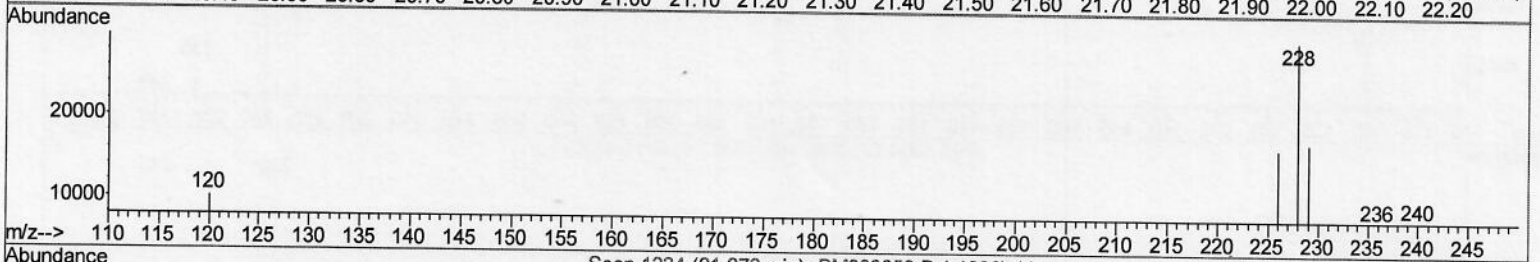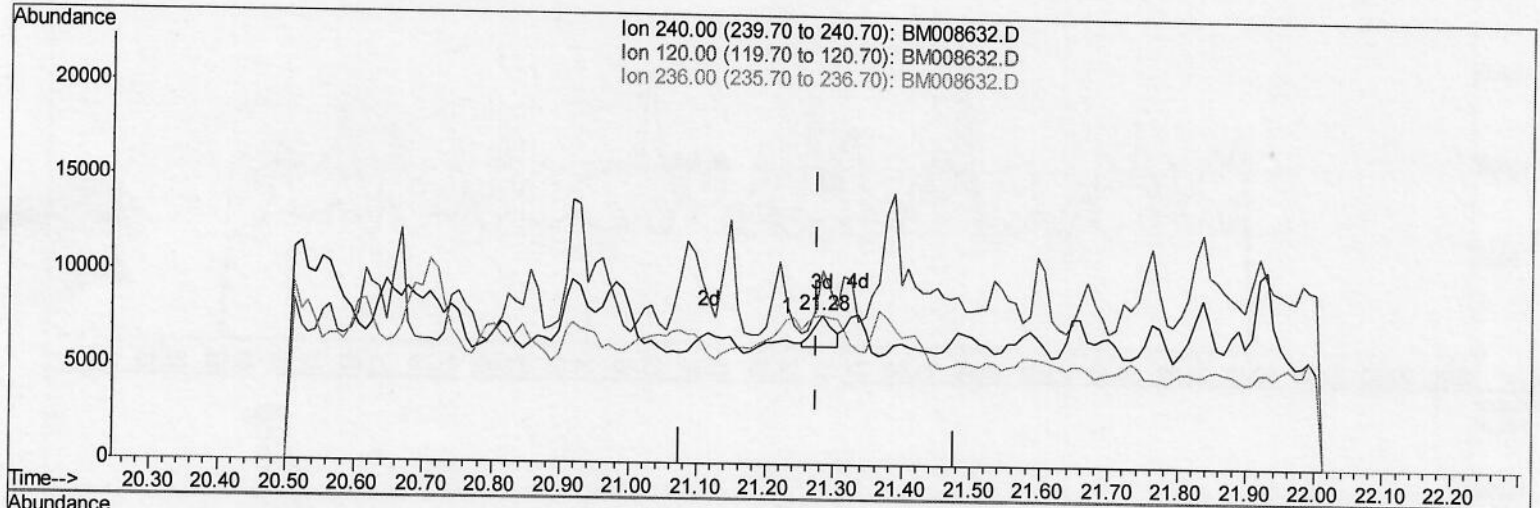

(16) Chrysene-d12 (I)

21.283min (+0.007) 0.40ng/ul m

response 3036

Ion Exp% Act%

240.00 100 100

120.00 20.60 129.51#

236.00 34.90 99.96#

0.00 0.00 0.00

7 5.9
 12/24/16

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA_M\Data\BM122416\
Data File : BM008632.D
Acq On : 24 Dec 2016 14:40
Operator : UM/SJ
Sample : H5995-09
Misc :
ALS Vial : 37 Sample Multiplier: 1




Quant Time: Dec 26 13:46:33 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 26 03:21:10 2016
Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :

DA874

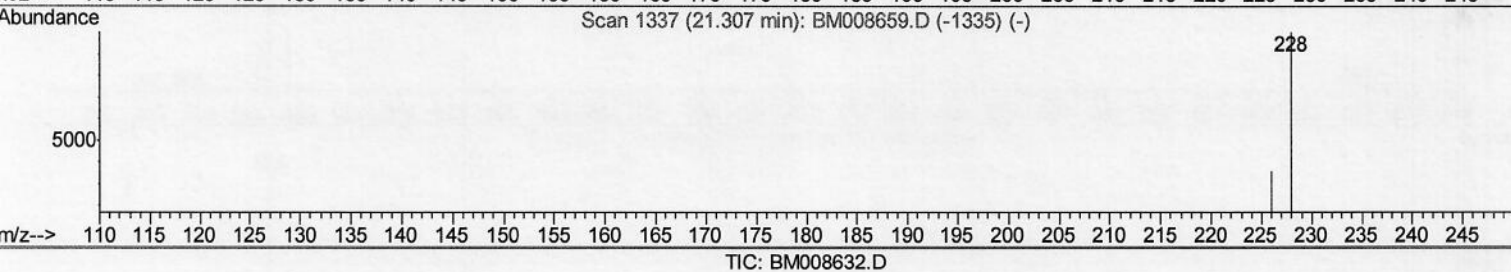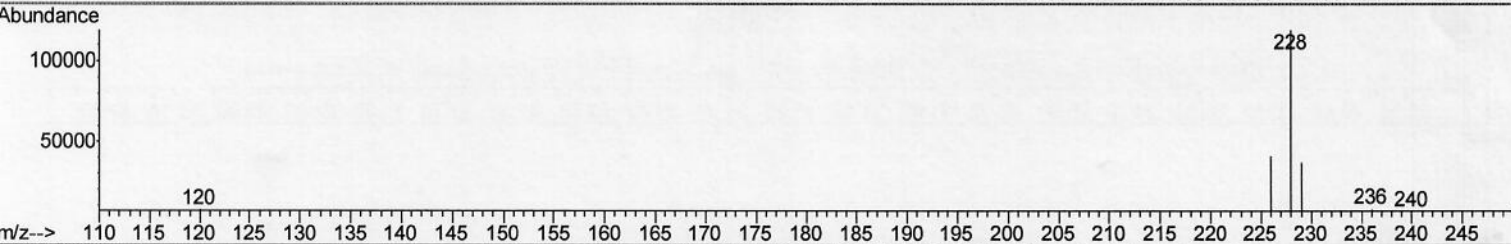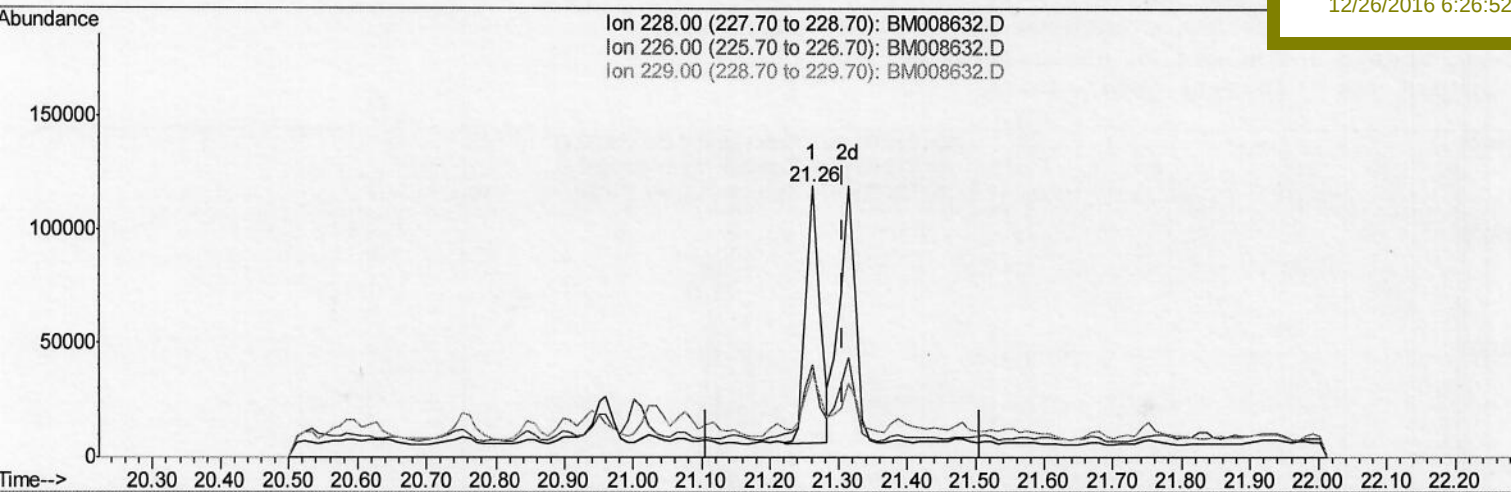Manual Integrations
APPROVEDsohil
12/26/2016 6:26:52 PM

(19) Chrysene

21.262min (-0.045) 14.94ng/ul

response 163021

Ion	Exp%	Act%
228.00	100	100
226.00	29.20	33.76
229.00	22.10	30.67#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122416\
 Data File : BM008632.D
 Acq On : 24 Dec 2016 14:40
 Operator : UM/SJ
 Sample : H5995-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 DA874

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:26:52 PM

Quant Time: Dec 26 13:46:33 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 03:21:10 2016
 Response via : Initial Calibration

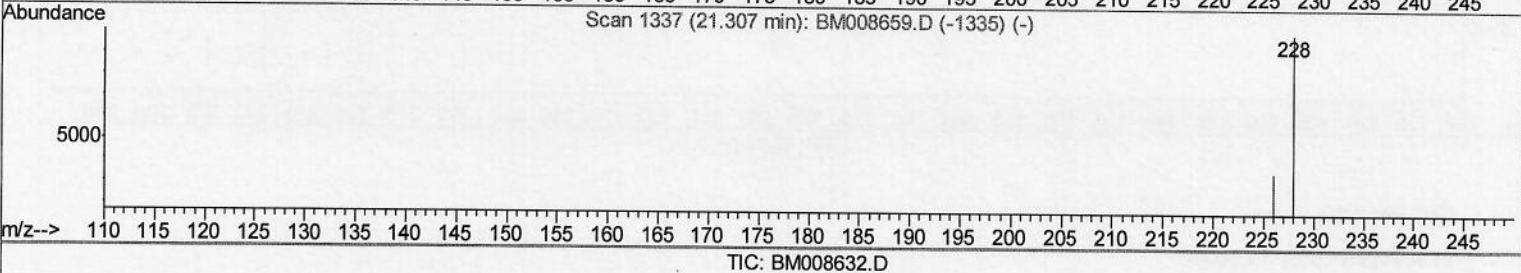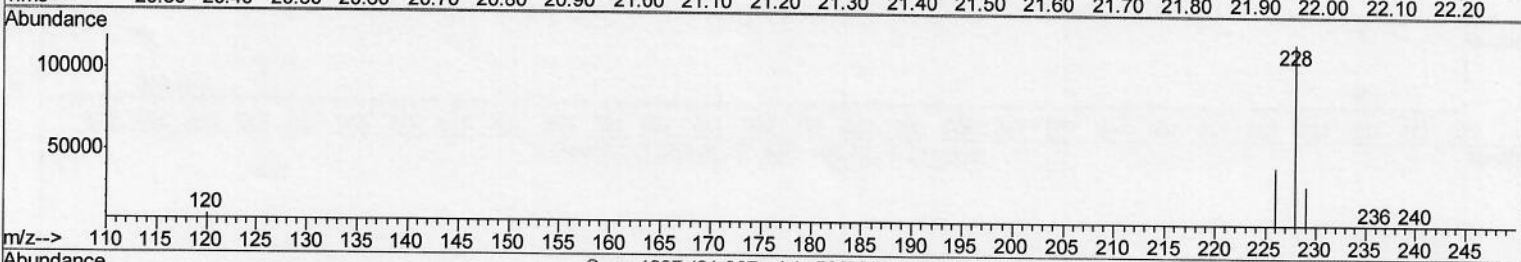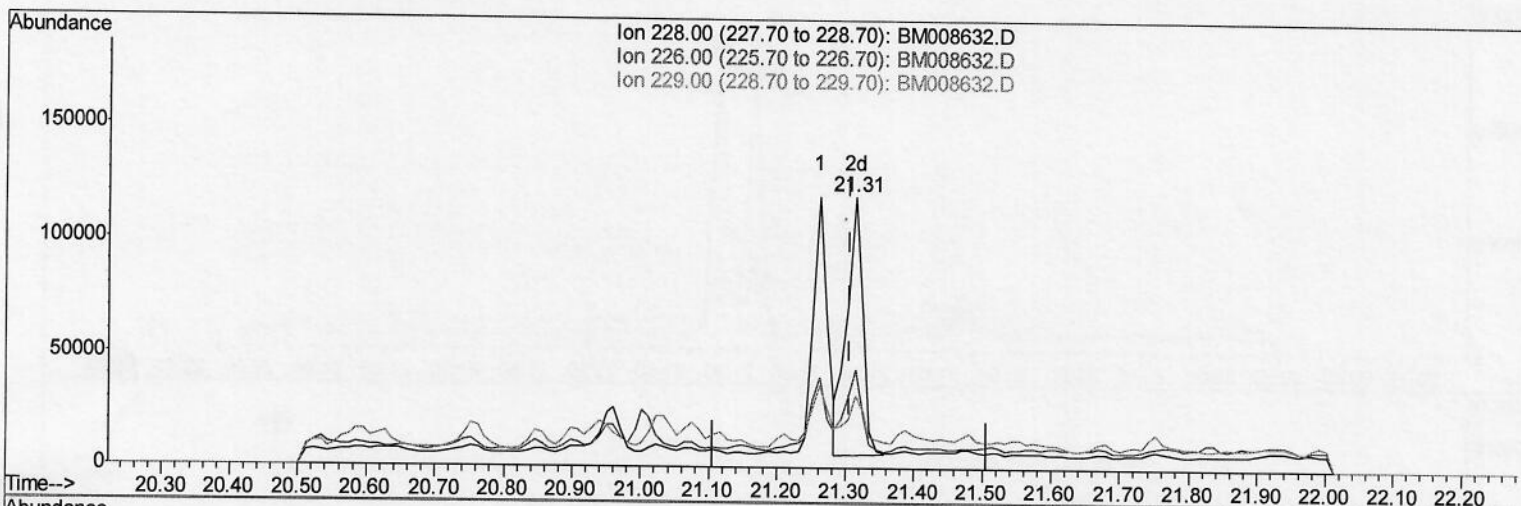

(19) Chrysene

21.315min (+0.007) 16.71ng/ul m

response 182393

Ion	Exp%	Act%
228.00	100	100
226.00	29.20	36.31#
229.00	22.10	26.70#
0.00	0.00	0.00

29.7
 12/27/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122416\
 Data File : BM008632.D
 Acq On : 24 Dec 2016 14:40
 Operator : UM/SJ
 Sample : H5995-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 DA874

Manual Integrations
APPROVED

sohil
 12/26/2016 6:26:52 PM

Quant Time: Dec 26 13:46:33 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 03:21:10 2016
 Response via : Initial Calibration

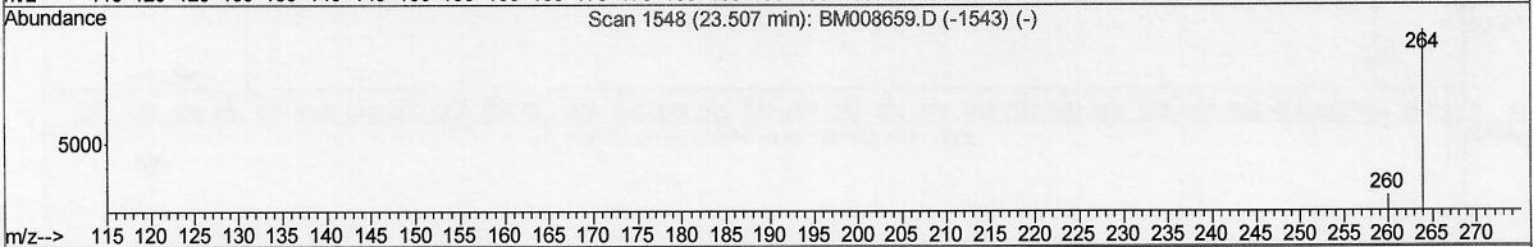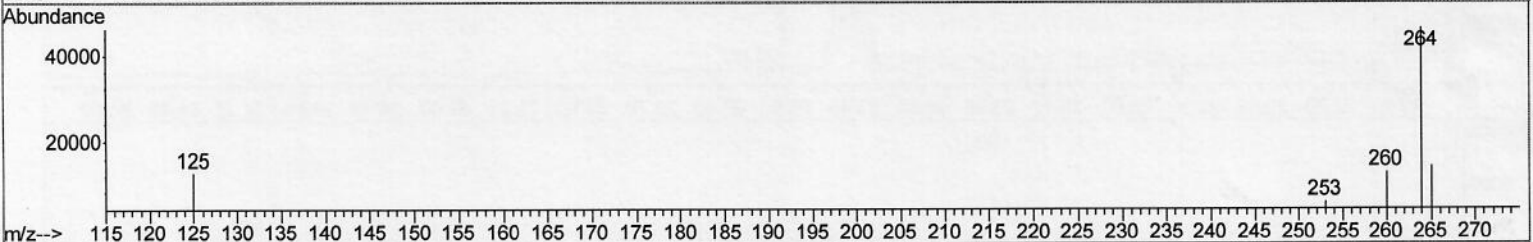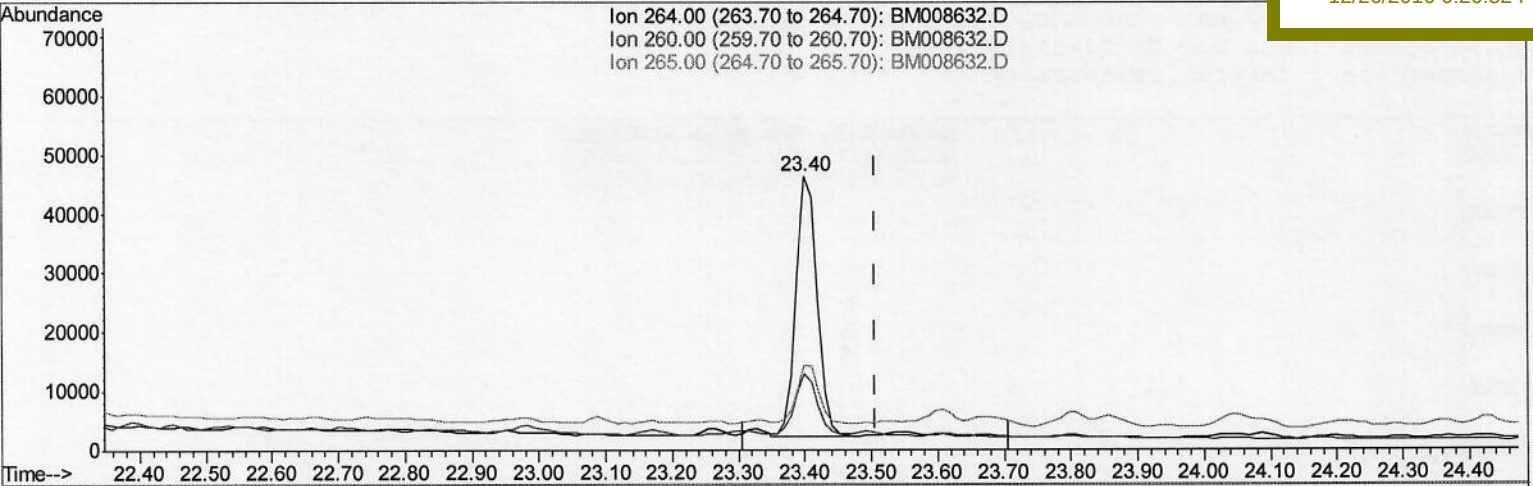

TIC: BM008632.D

(20) Perylene-d12 (I)
 23.399min (-0.107) 0.40ng/ul
 response 97447

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	27.76
265.00	103.50	30.78#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122416\
 Data File : BM008632.D
 Acq On : 24 Dec 2016 14:40
 Operator : UM/SJ
 Sample : H5995-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 Client Sample ID :
 DA874

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:26:52 PM

Quant Time: Dec 26 13:46:33 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 03:21:10 2016
 Response via : Initial Calibration

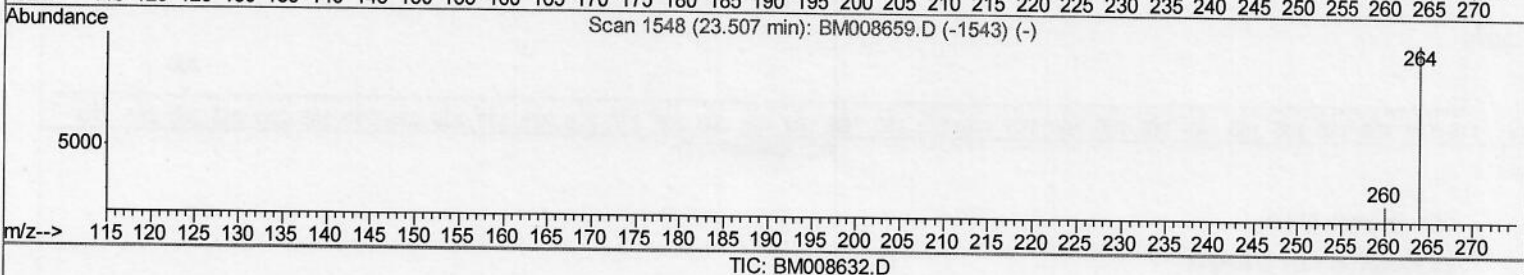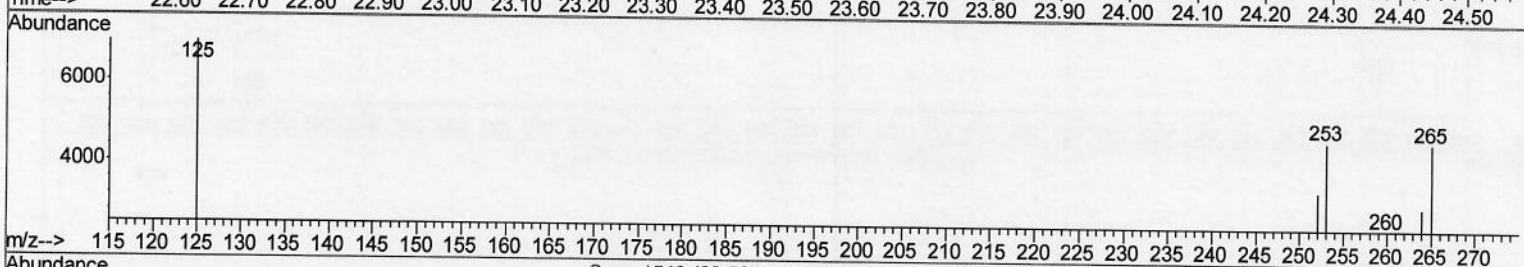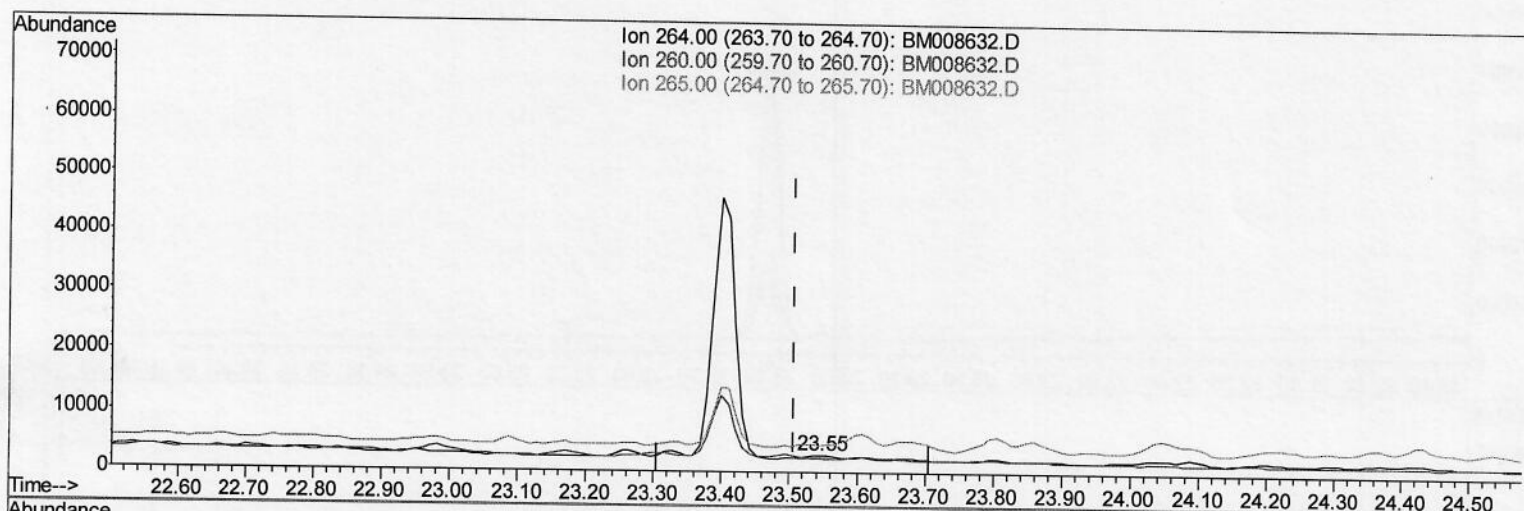

(20) Perylene-d12 (I)

23.545min (+0.038) 0.40ng/ul m

response 1480

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	82.15#
265.00	103.50	152.43#
0.00	0.00	0.00

29.7
 12/27/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122416\
 Data File : BM008632.D
 Acq On : 24 Dec 2016 14:40
 Operator : UM/SJ
 Sample : H5995-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 DA874

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:26:52 PM

Quant Time: Dec 26 13:47:47 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 03:21:10 2016
 Response via : Initial Calibration

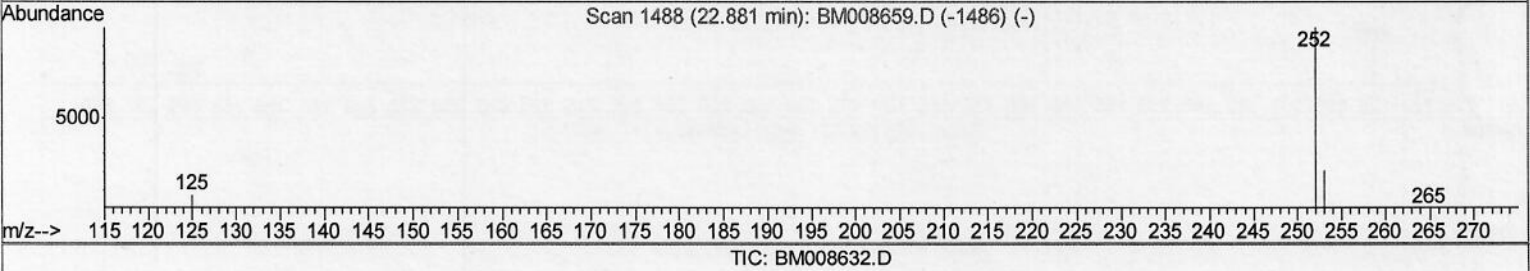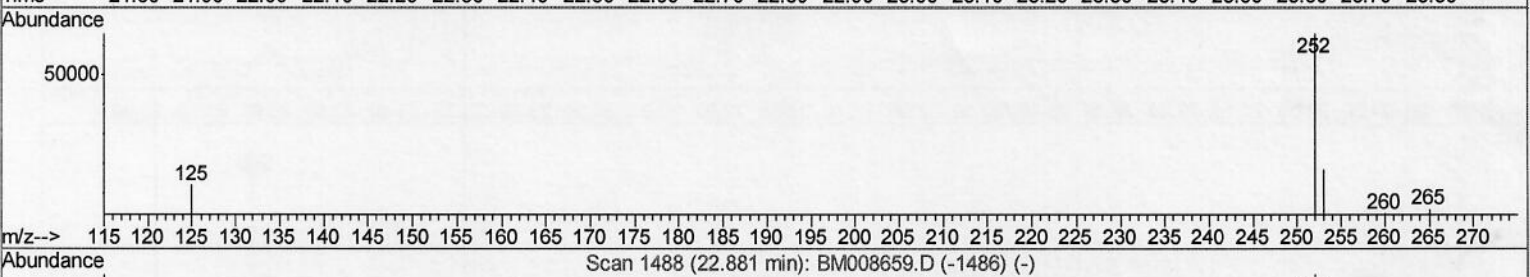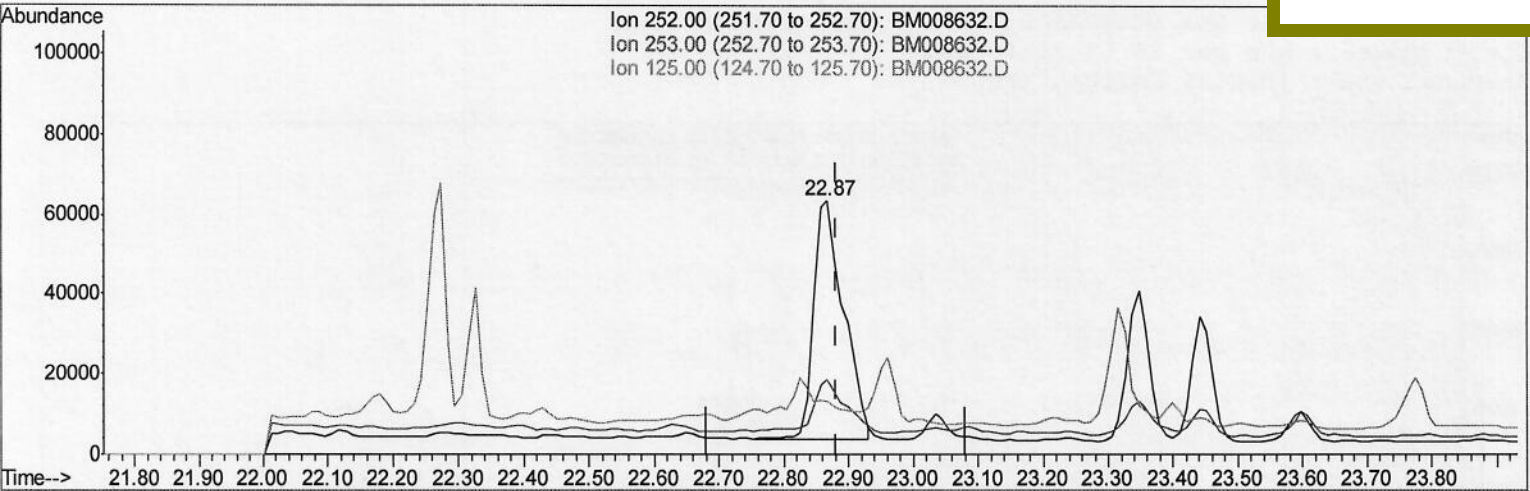

(22) Benzo(k)fluoranthene
 22.868min (-0.014) 33.23ng/ul
 response 188937

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	28.96
125.00	17.10	20.27
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122416\
 Data File : BM008632.D
 Acq On : 24 Dec 2016 14:40
 Operator : UM/SJ
 Sample : H5995-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA874

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:26:52 PM

Quant Time: Dec 26 13:47:47 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 03:21:10 2016
 Response via : Initial Calibration

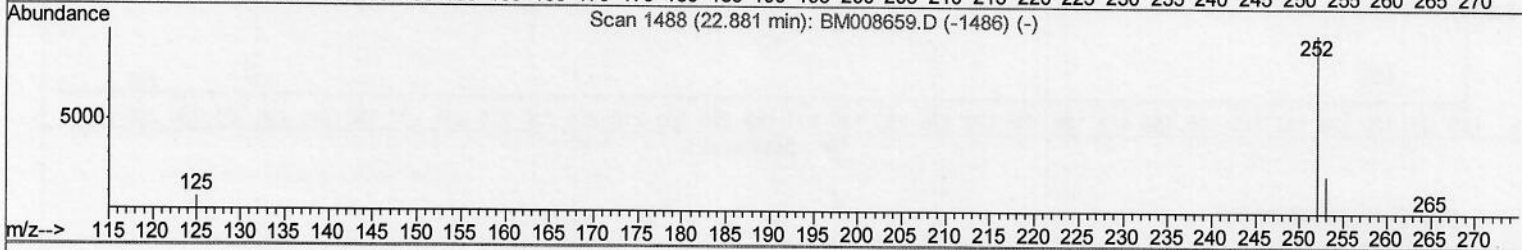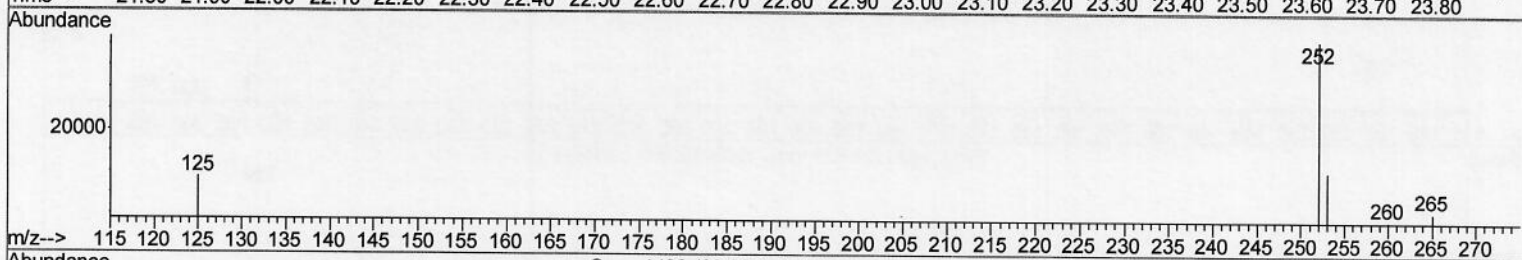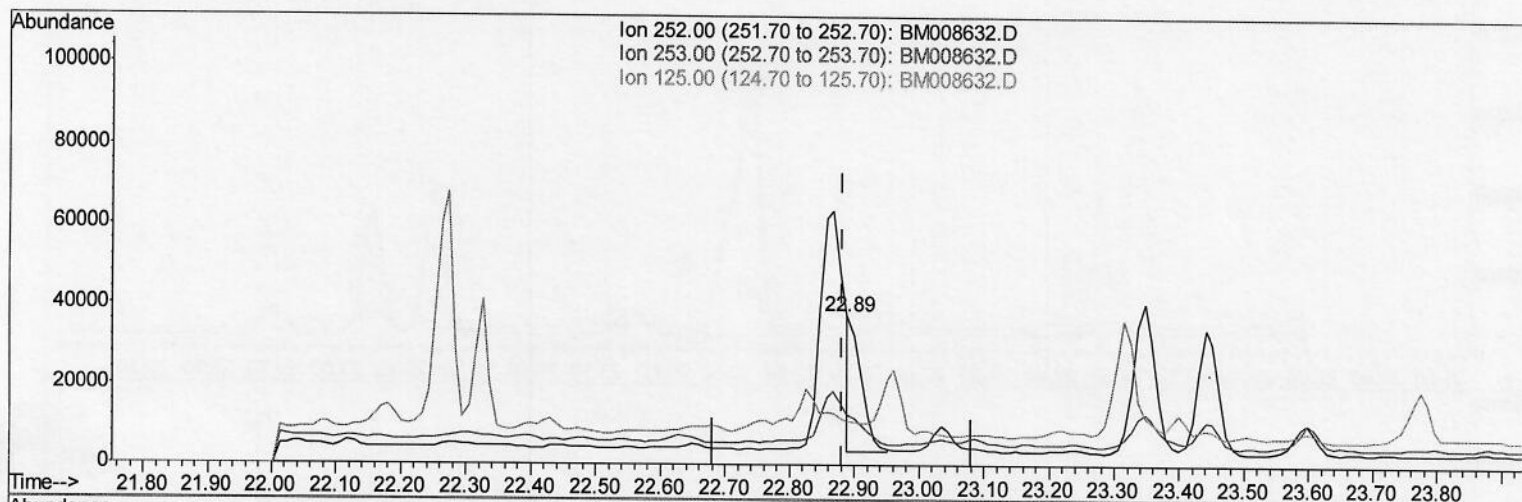

(22) Benzo(k)fluoranthene

22.888min (+0.007) 6.98ng/ul m

response 39686

Ion Exp% Act%

252.00 100 100

253.00 30.60 33.95

125.00 17.10 29.36#

0.00 0.00 0.00

7 5.5
 12/27/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122416\
 Data File : BM008632.D
 Acq On : 24 Dec 2016 14:40
 Operator : UM/SJ
 Sample : H5995-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA874

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:26:52 PM

Quant Time: Dec 26 13:47:47 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 03:21:10 2016
 Response via : Initial Calibration

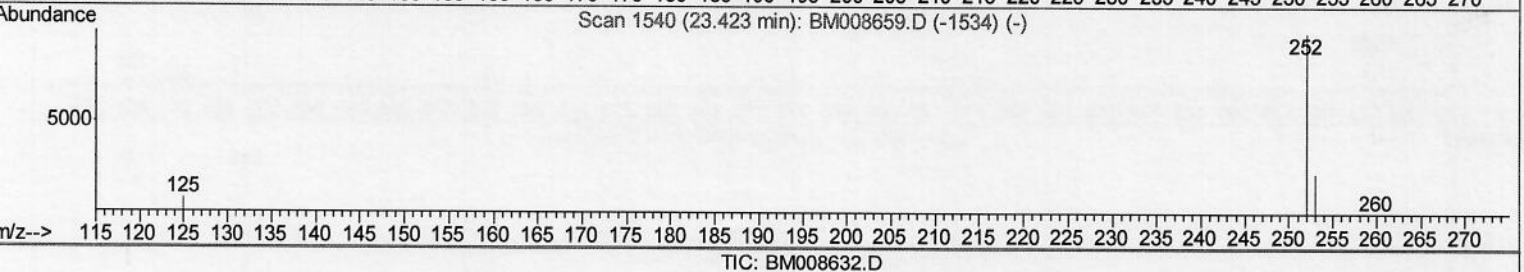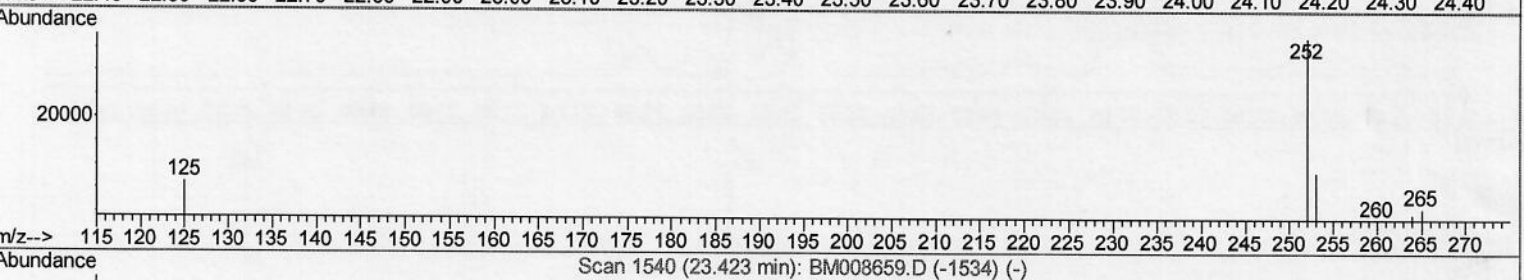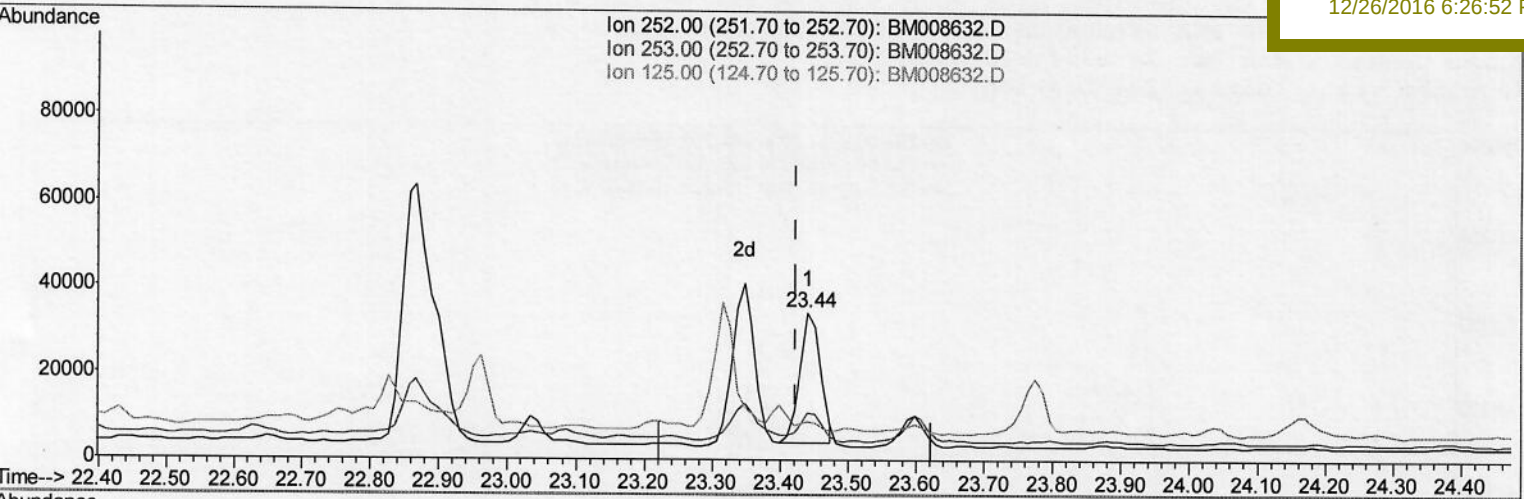

(23) Benzo(a)pyrene (C)

23.441min (+0.018) 11.89ng/ul

response 64244

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	32.31
125.00	22.60	26.60
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122416\
 Data File : BM008632.D
 Acq On : 24 Dec 2016 14:40
 Operator : UM/SJ
 Sample : H5995-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA874

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:26:52 PM

Quant Time: Dec 26 13:47:47 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 03:21:10 2016
 Response via : Initial Calibration

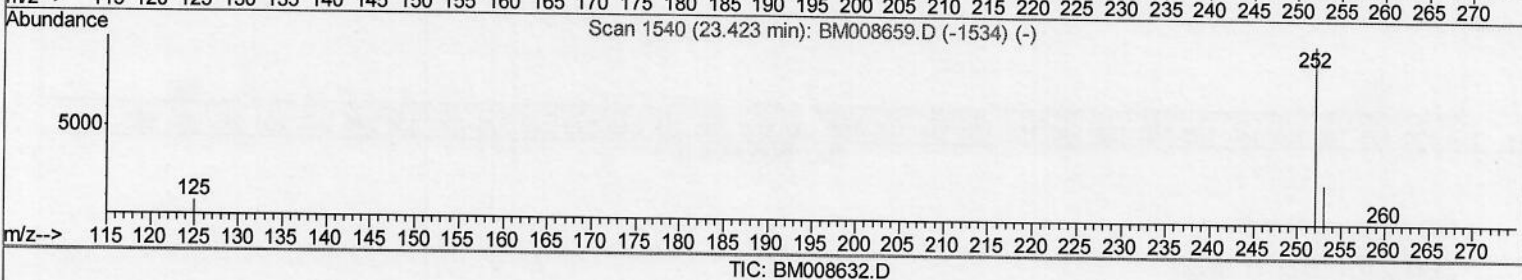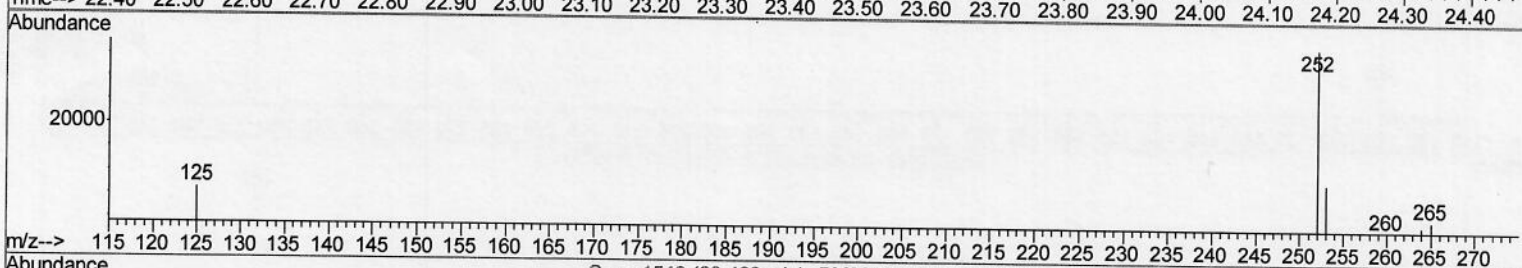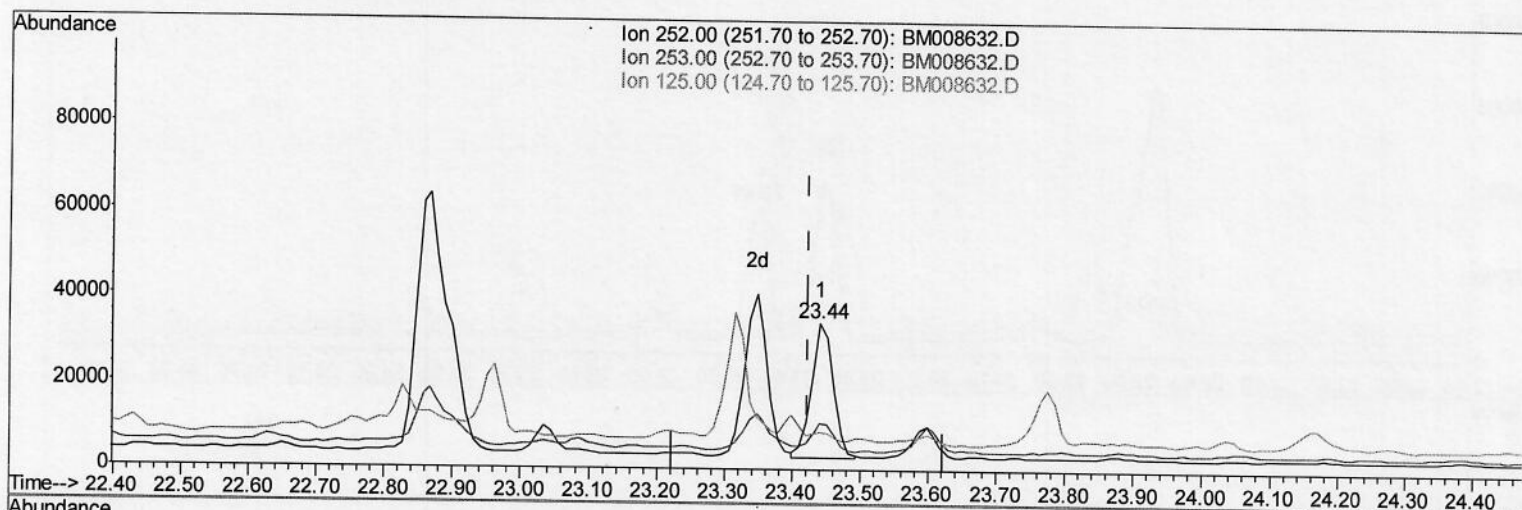

(23) Benzo(a)pyrene (C)

23.441min (+0.018) 13.12ng/ul m

response 70885

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	32.31
125.00	22.60	26.60
0.00	0.00	0.00

5.9
 12/27/16

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM122416\
 Data File : BM008632.D
 Acq On : 24 Dec 2016 14:40
 Operator : UM/SJ
 Sample : H5995-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA874

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:26:52 PM

Quant Time: Dec 26 13:47:47 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 03:21:10 2016
 Response via : Initial Calibration

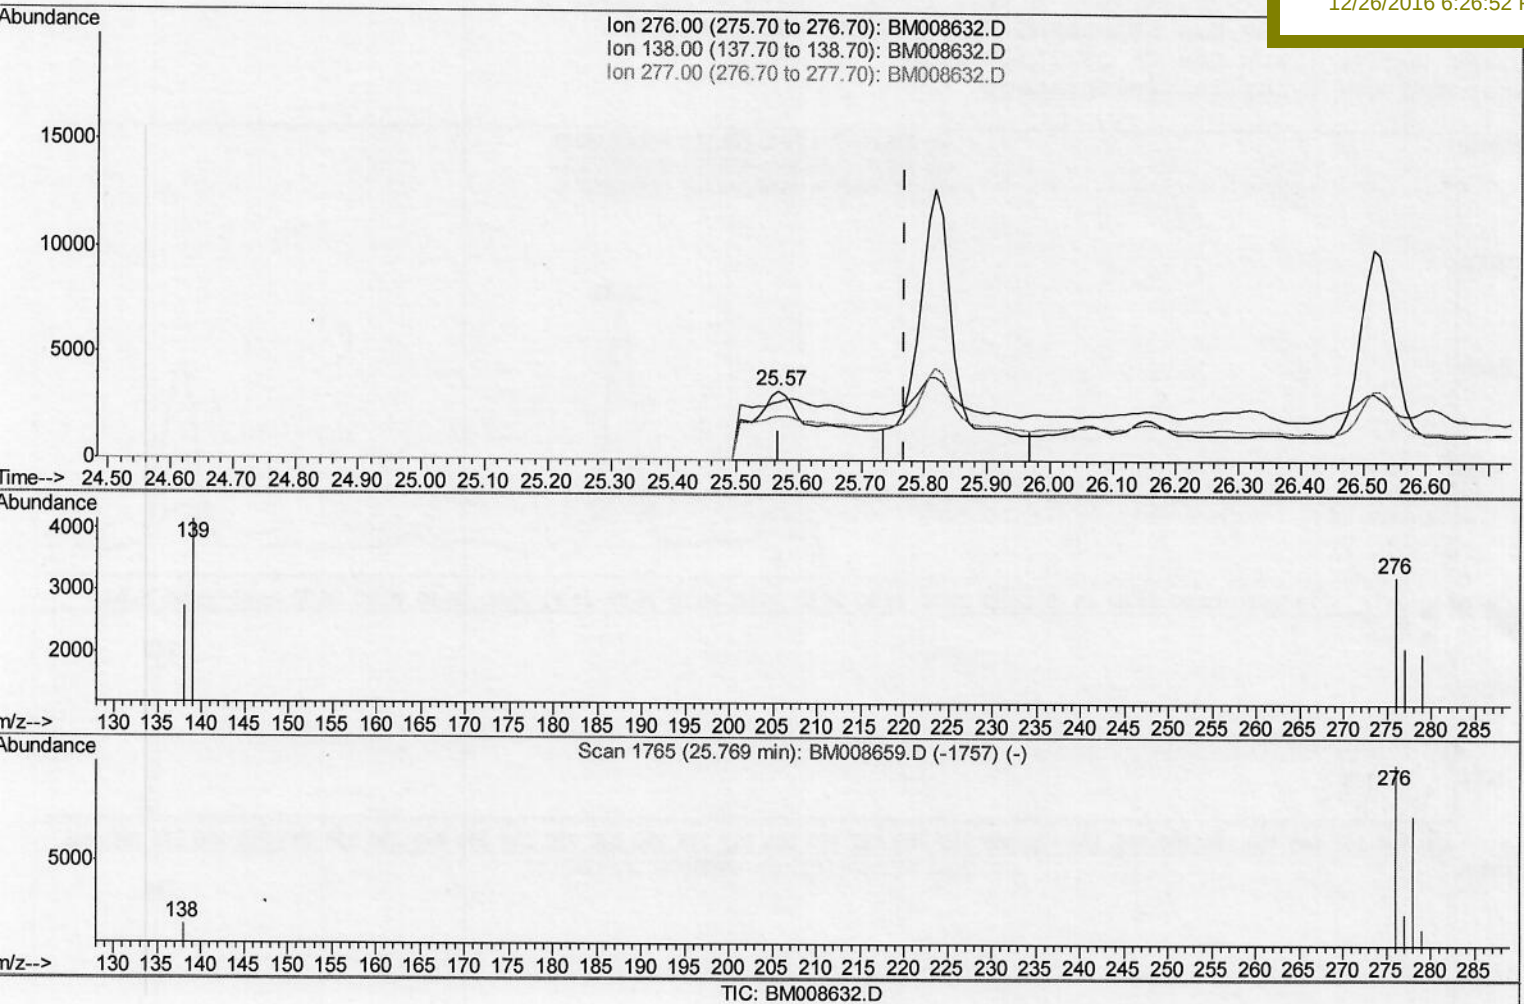

(24) Indeno(1,2,3-cd)pyrene

25.568min (-0.201) 4.36ng/ul

response 28092

Ion	Exp%	Act%
276.00	100	100
138.00	23.90	0.00#
277.00	24.50	101.62#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\Data\BM122416\
 Data File : BM008632.D
 Acq On : 24 Dec 2016 14:40
 Operator : UM/SJ
 Sample : H5995-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 Client Sampled :
 DA874

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:26:52 PM

Quant Time: Dec 26 13:47:47 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 03:21:10 2016
 Response via : Initial Calibration

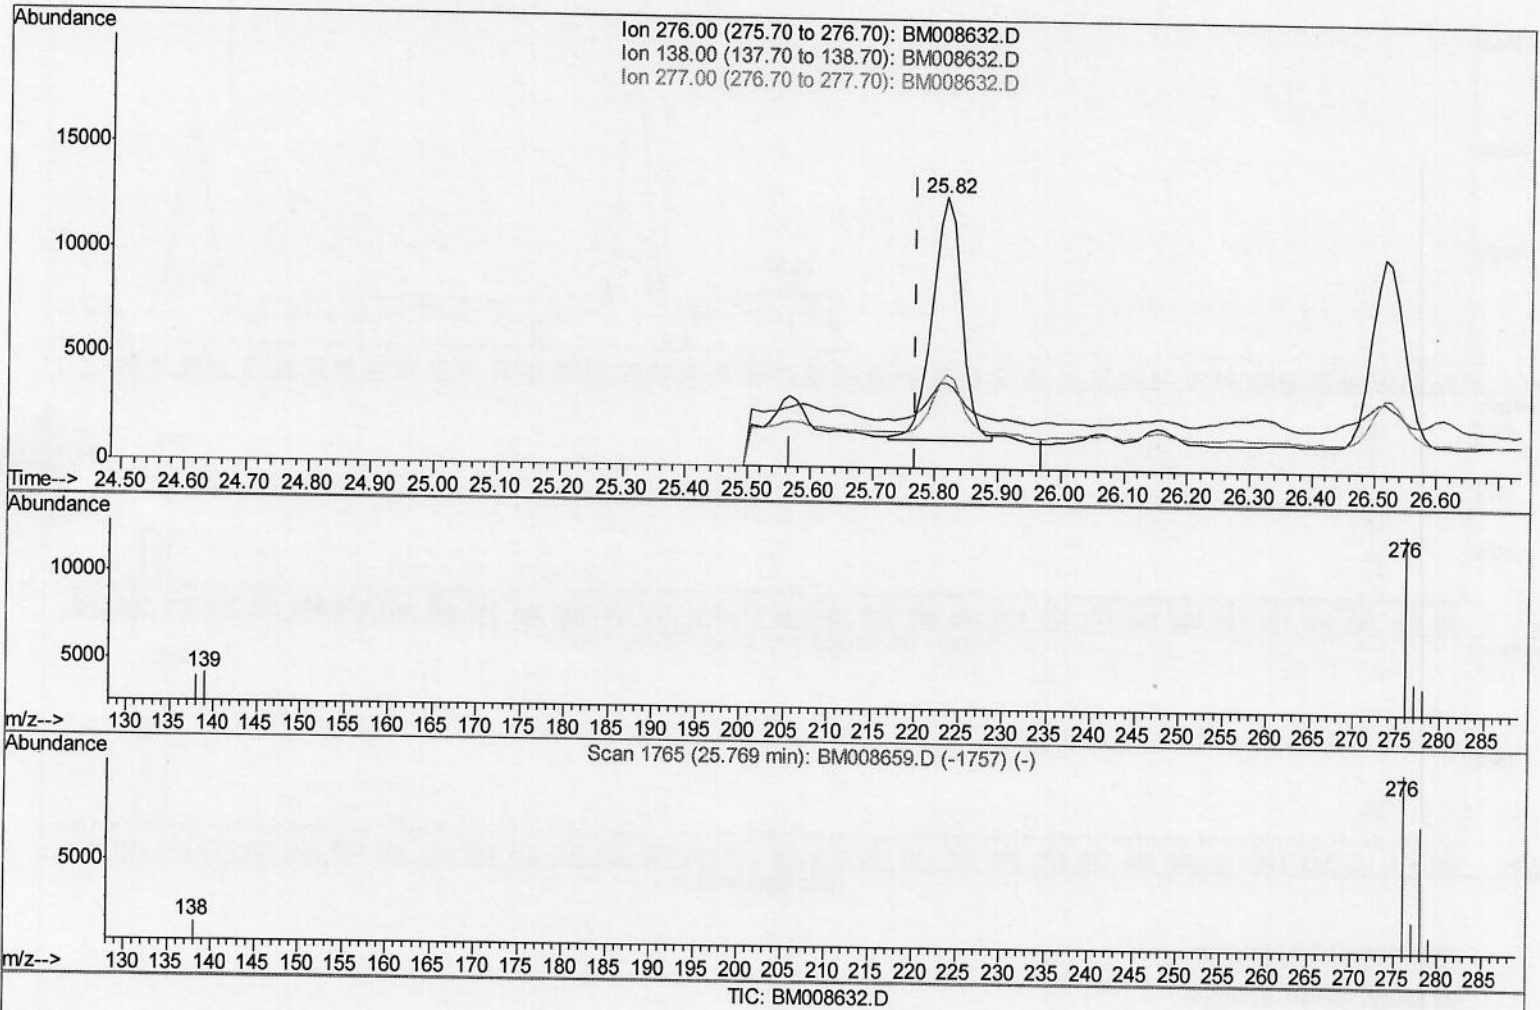

(24) Indeno(1,2,3-cd)pyrene

25.818min (+0.049) 5.76ng/ul m

response 37115

Ion Exp% Act%

276.00 100 100

138.00 23.90 0.00#

277.00 24.50 76.91#

0.00 0.00 0.00

> 5.7
 12/27/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122416\
Data File : BM008632.D
Acq On : 24 Dec 2016 14:40
Operator : UM/SJ
Sample : H5995-09
Misc :
ALS Vial : 37 Sample Multiplier: 1

Quant Time: Dec 26 13:47:47 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 26 03:21:10 2016
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DA874

Manual Integrations
APPROVED

sohil
12/26/2016 6:26:52 PM

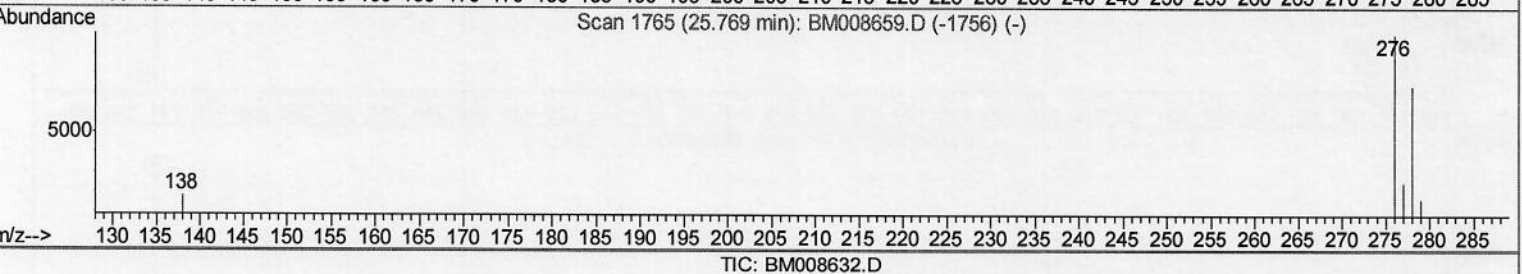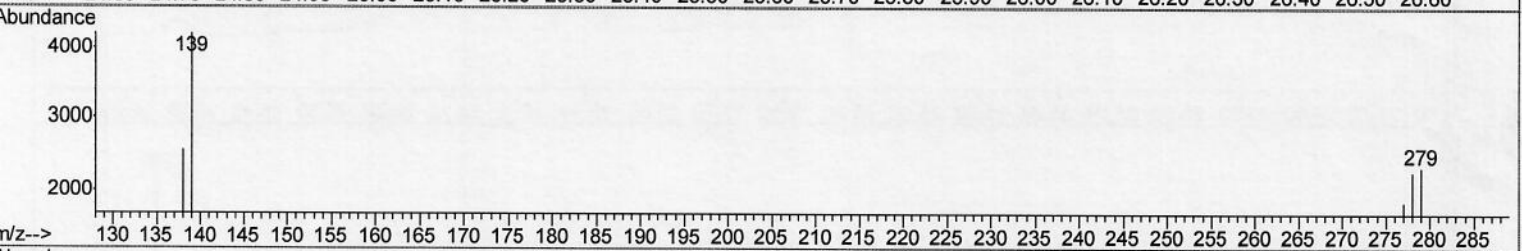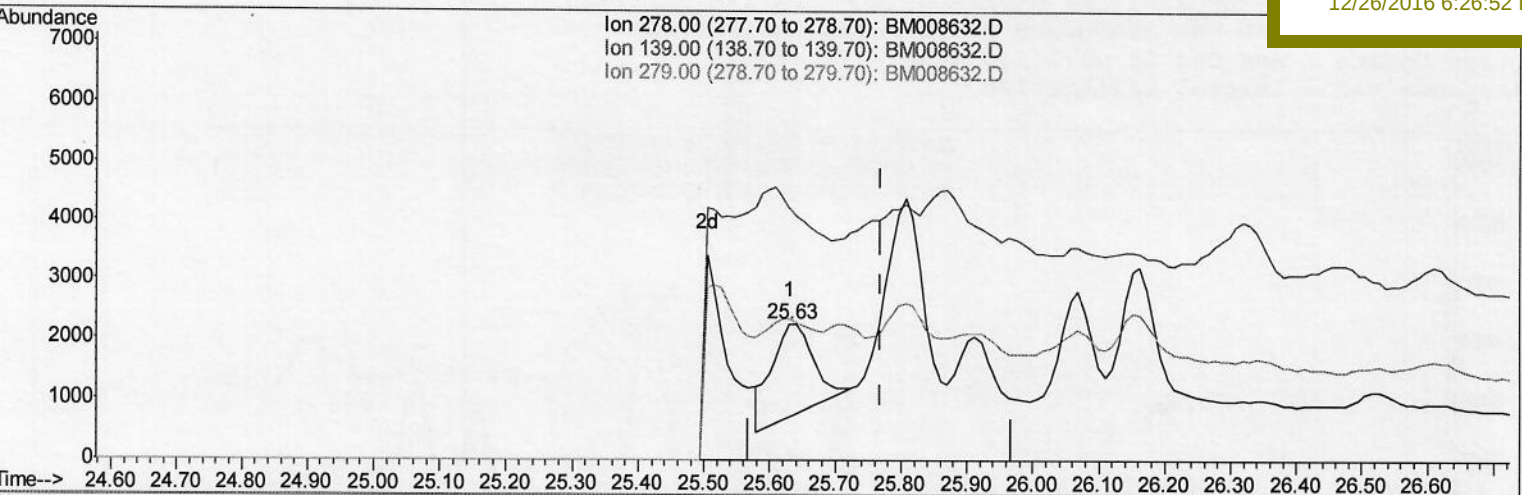

(25) Dibenzo(a,h)anthracene

25.630min (-0.139) 1.32ng/ul

response 6779

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	186.75#
279.00	32.40	102.93#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122416\
 Data File : BM008632.D
 Acq On : 24 Dec 2016 14:40
 Operator : UM/SJ
 Sample : H5995-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA874

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:26:52 PM

Quant Time: Dec 26 13:47:47 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 03:21:10 2016
 Response via : Initial Calibration

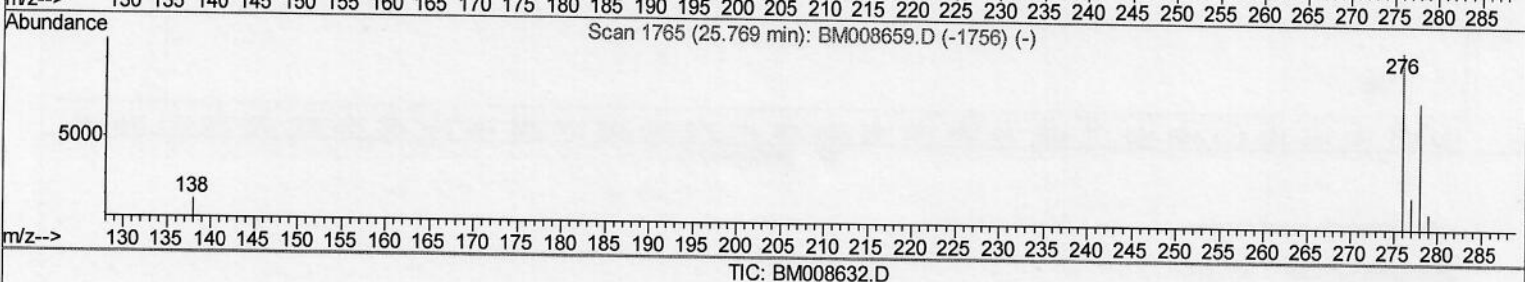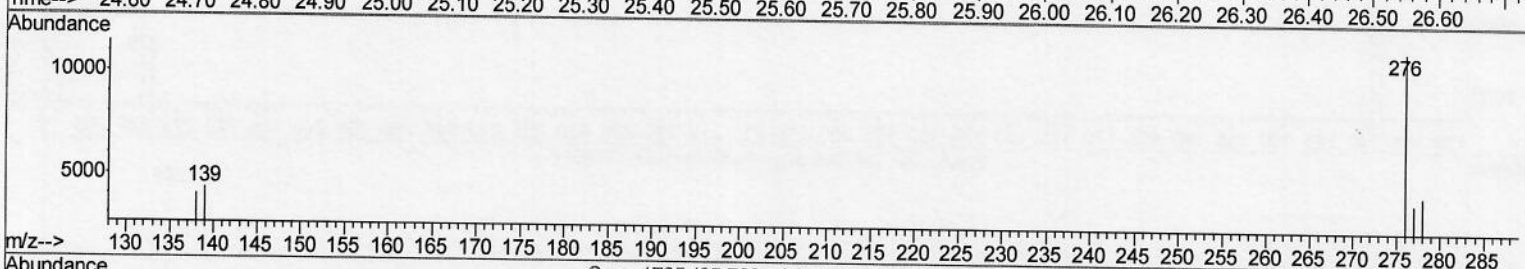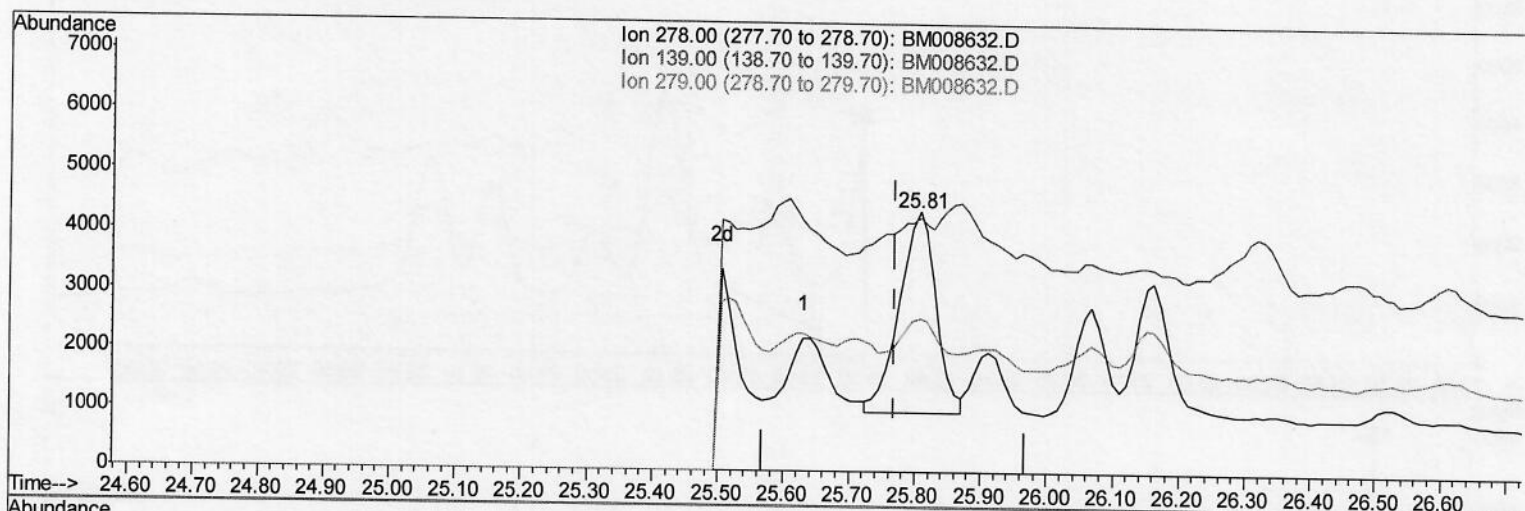

(25) Dibenzo(a,h)anthracene

25.807min (+0.038) 2.57ng/ul m

response 13229

Ion Exp% Act%

278.00 100 100

139.00 21.70 97.88#

279.00 32.40 59.33#

0.00 0.00 0.00

75.9
 12/29/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122416\
 Data File : BM008632.D
 Acq On : 24 Dec 2016 14:40
 Operator : UM/SJ
 Sample : H5995-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA874

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:26:52 PM

Quant Time: Dec 26 13:47:47 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 03:21:10 2016
 Response via : Initial Calibration

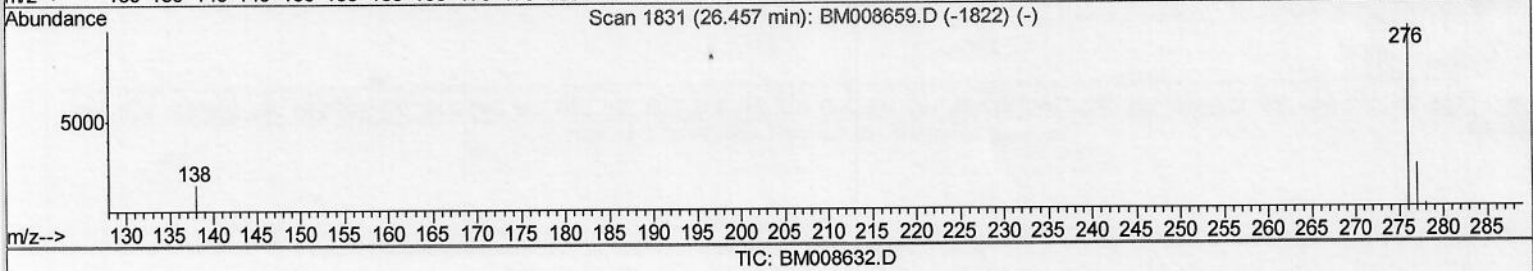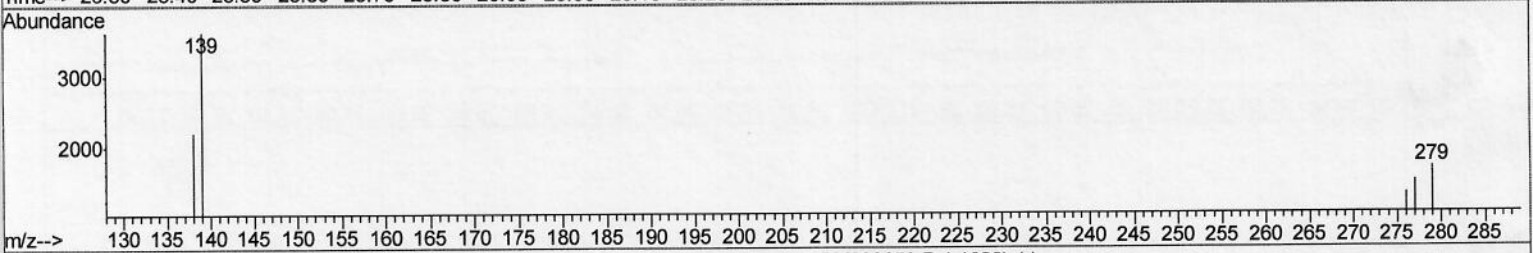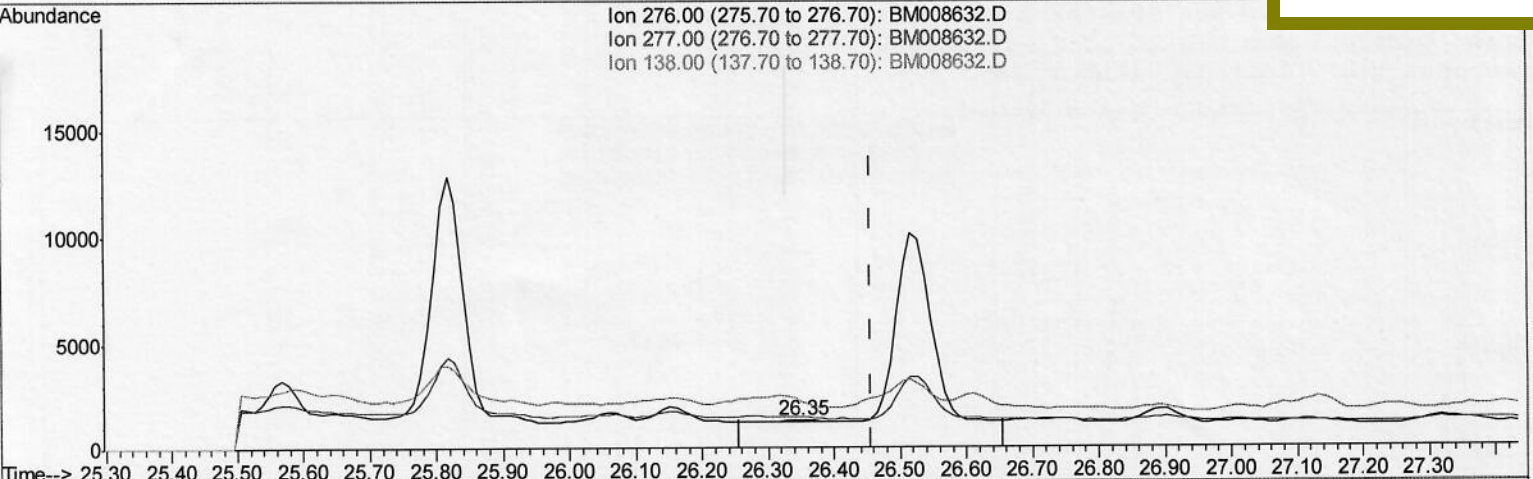

(26) Benzo(g,h,i)perylene
 26.349min (-0.107) 0.06ng/ul
 response 330

Ion	Exp%	Act%
276.00	100	100
277.00	27.30	114.47#
138.00	25.60	170.82#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\Data\BM122416\
 Data File : BM008632.D
 Acq On : 24 Dec 2016 14:40
 Operator : UM/SJ
 Sample : H5995-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA874

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:26:52 PM

Quant Time: Dec 26 13:47:47 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 03:21:10 2016
 Response via : Initial Calibration

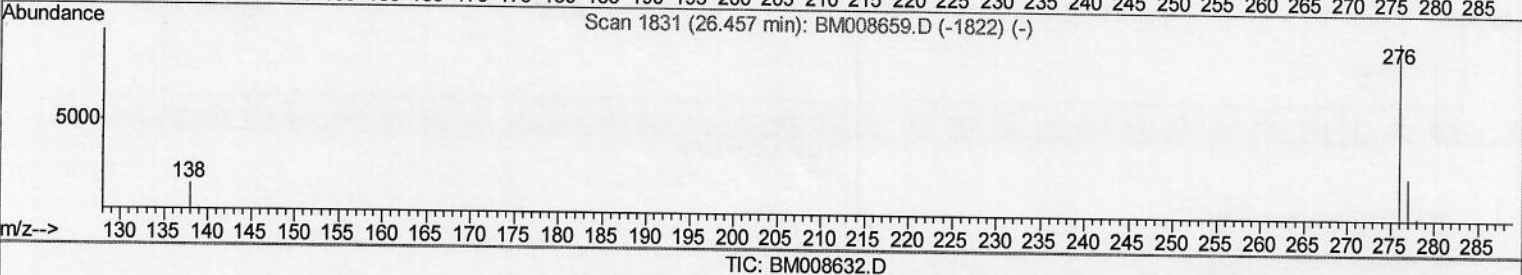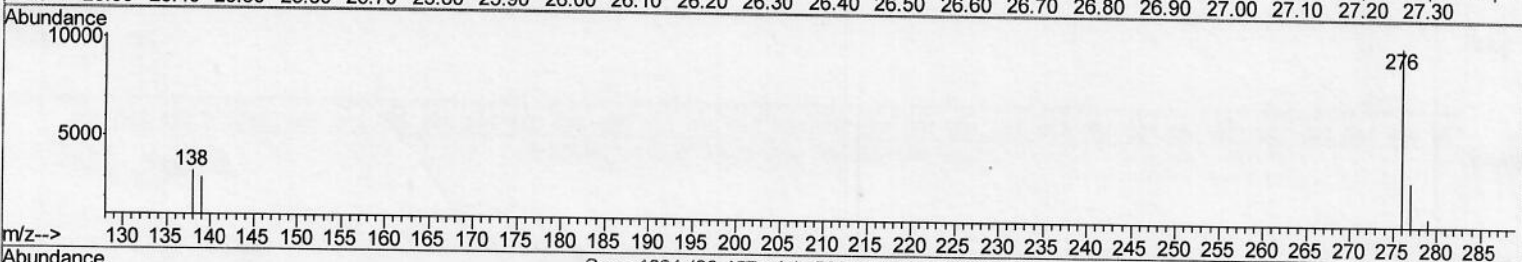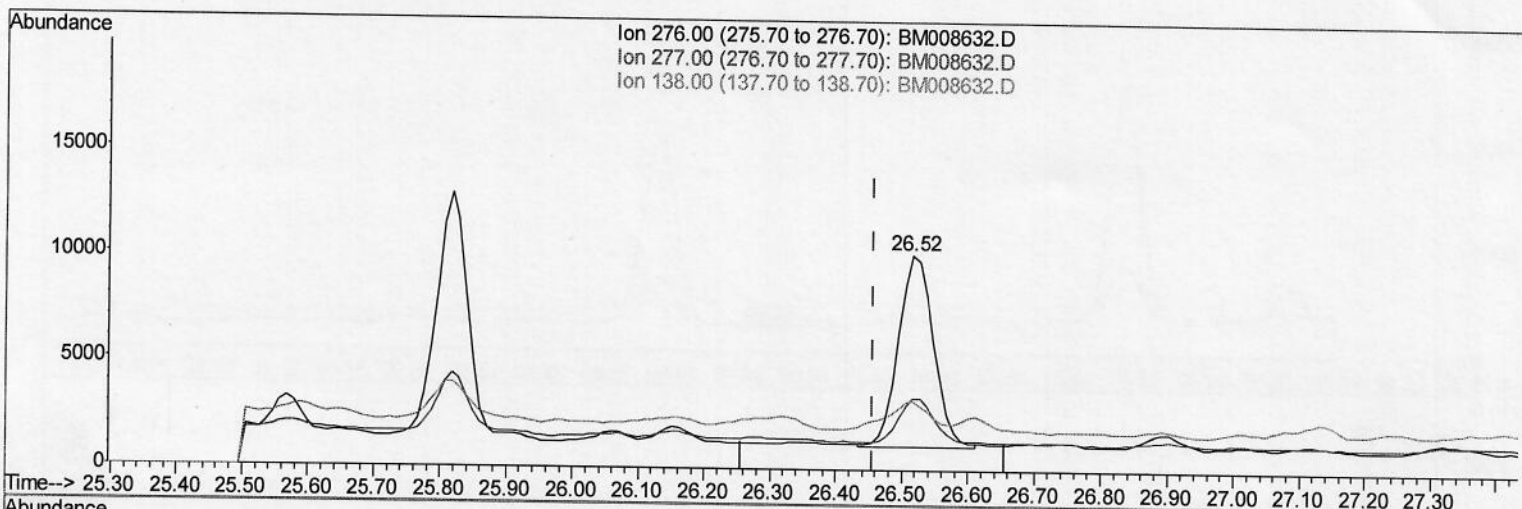

(26) Benzo(g,h,i)perylene

26.516min (+0.059) 6.08ng/ul m

response 33590

Ion Exp% Act%

276.00 100 100

277.00 27.30 33.48#

138.00 25.60 32.31#

0.00 0.00 0.00

75.7
 12/27/16

Data Path : Z:\HPCHEM1\BNA_M\Data\BM122416\
 Data File : BM008632.D
 Acq On : 24 Dec 2016 14:40
 Operator : UM/SJ
 Sample : H5995-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA874

Quant Time: Dec 26 13:50:47 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 03:21:10 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:26:52 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	553m	0.40	ng/ul	-0.14
2) Naphthalene-d8	10.40	136	4350m	0.40	ng/ul	-0.11
6) Acenaphthene-d10	14.28	164	11077	0.40	ng/ul	-0.05
10) Phenanthrene-d10	17.02	188	35463	0.40	ng/ul	-0.07
16) Chrysene-d12	21.28	240	3036m	0.40	ng/ul	0.00
20) Perylene-d12	23.55	264	1480m	0.40	ng/ul	0.04

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.00	152	1283m	0.19	ng/ul	-0.12
14) Fluoranthene-d10	19.05	212	26545m	0.27	ng/ul	-0.07

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Naphthalene	10.46	128	225481	18.42	ng/ul	96
5) 2-Methylnaphthalene	12.09	142	984353	119.50	ng/ul	98
7) Acenaphthylene	14.02	152	81710	1.63	ng/ul#	1
8) Acenaphthene	14.38	153	90485	2.40	ng/ul#	42
9) Fluorene	15.38	166	83655	1.94	ng/ul#	25
12) Phenanthrene	17.11	178	1243638	11.48	ng/ul	99
13) Anthracene	17.21	178	70339m	0.67	ng/ul	
15) Fluoranthene	19.14	202	748457m	5.64	ng/ul	
17) Pyrene	19.52	202	697784	59.46	ng/ul	100
18) Benzo(a)anthracene	21.26	228	162465	16.30	ng/ul#	86
19) Chrysene	21.31	228	182393m	16.71	ng/ul	
21) Benzo(b)fluoranthene	22.87	252	151727	26.02	ng/ul	94
22) Benzo(k)fluoranthene	22.89	252	39686m	6.98	ng/ul	
23) Benzo(a)pyrene	23.44	252	70885m	13.12	ng/ul	
24) Indeno(1,2,3-cd)pyrene	25.82	276	37115m	5.76	ng/ul	
25) Dibenzo(a,h)anthracene	25.81	278	13229m	2.57	ng/ul	
26) Benzo(g,h,i)perylene	26.52	276	33590m	6.08	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA_M\Data\BM122416\
 Data File : BM008632.D
 Acq On : 24 Dec 2016 14:40
 Operator : UM/SJ
 Sample : H5995-09
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA874

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:26:52 PM

Quant Time: Dec 26 13:50:47 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 03:21:10 2016
 Response via : Initial Calibration

