

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
 Data File : BM008637.D
 Acq On : 24 Dec 2016 17:38
 Operator : UM/SJ
 Sample : H5995-13DL 2X
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA881DL

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:27:51 PM

Quant Time: Dec 26 00:37:00 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Dec 25 23:48:32 2016
 Response via : Initial Calibration

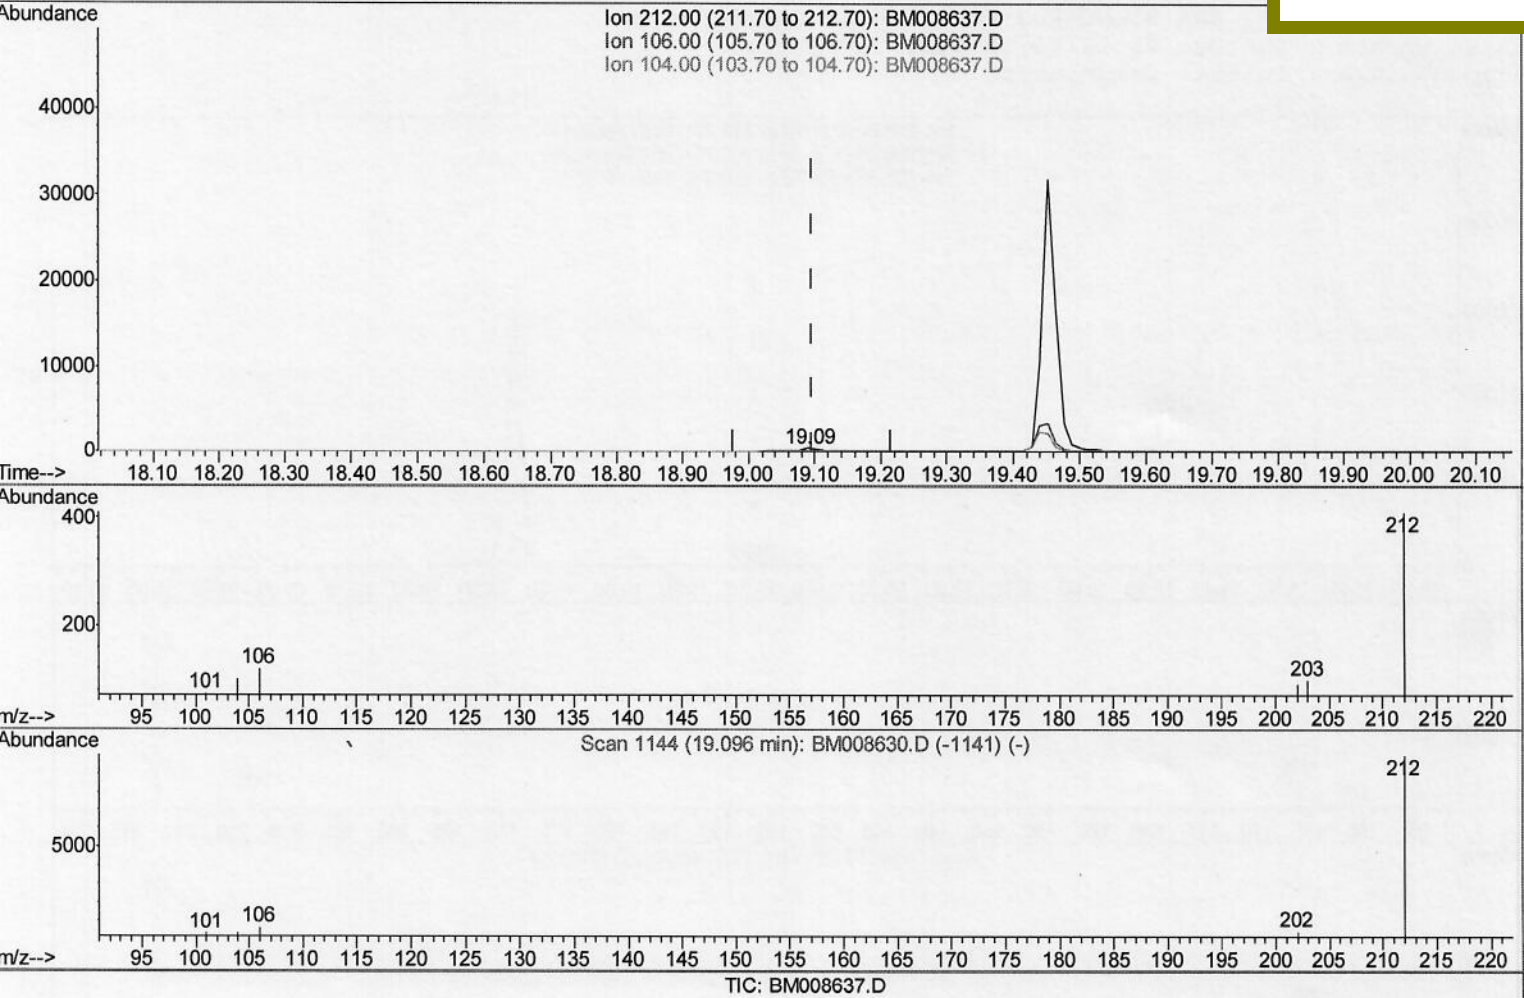

(14) Fluoranthene-d10 (SURR)

19.089min (-0.007) 0.30ng/ul

response 1170

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	64.87#
104.00	15.60	55.30#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
 Data File : BM008637.D
 Acq On : 24 Dec 2016 17:38
 Operator : UM/SJ
 Sample : H5995-13DL 2X
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA881DL

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:27:51 PM

Quant Time: Dec 26 00:37:00 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Dec 25 23:48:32 2016
 Response via : Initial Calibration

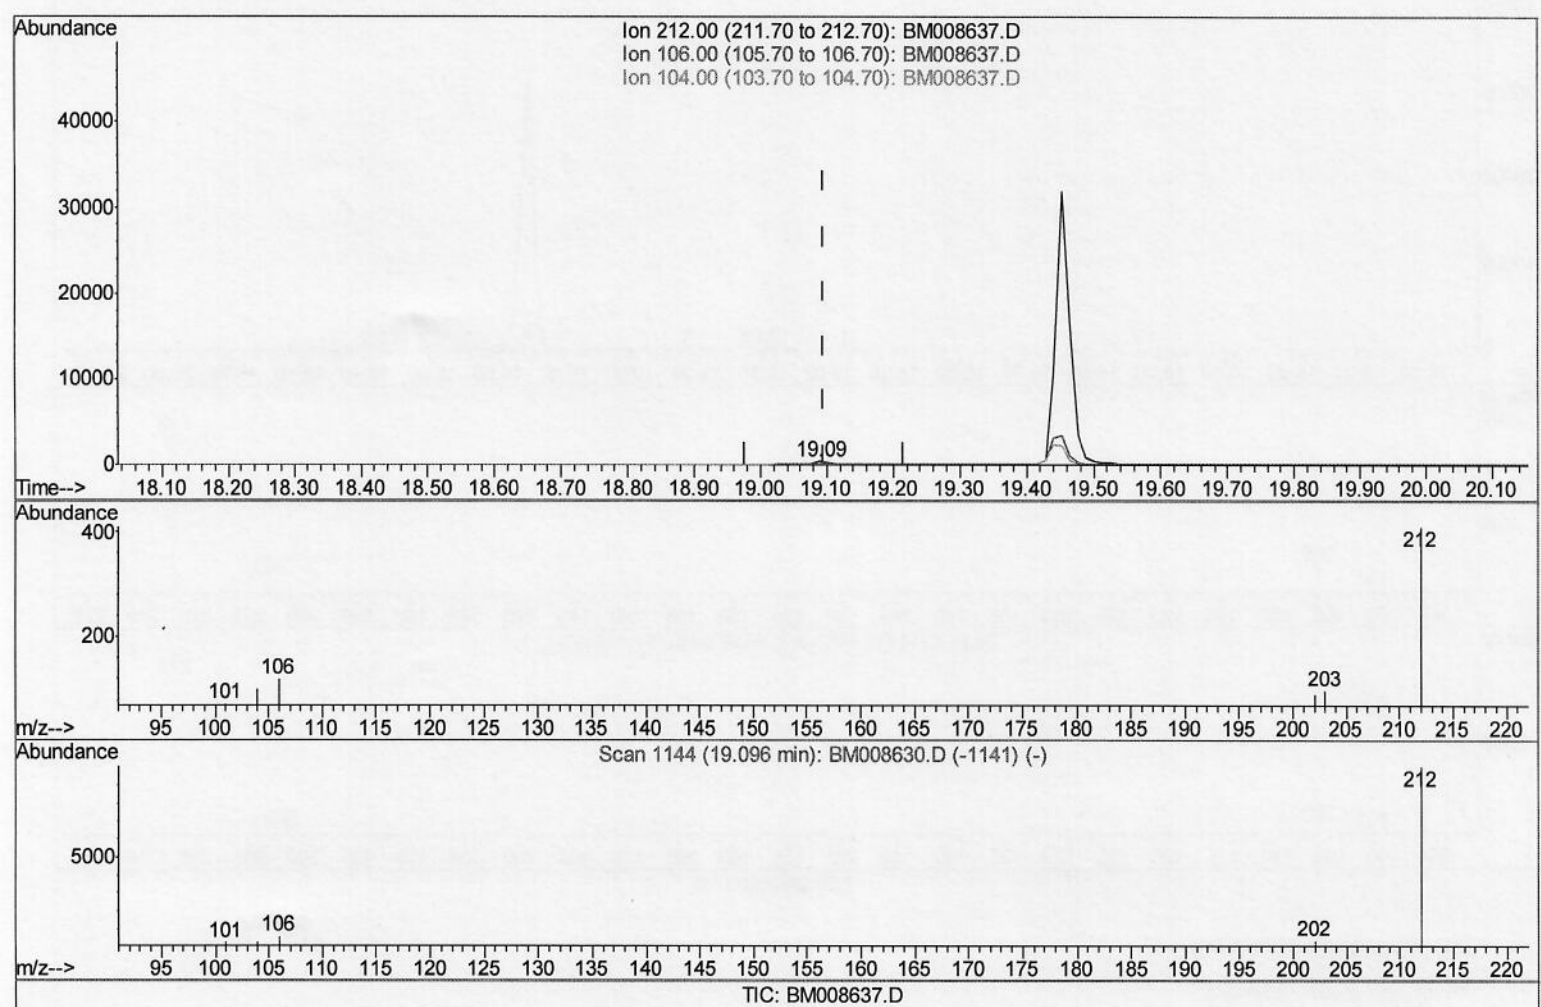

(14) Fluoranthene-d10 (SURR)

19.089min (-0.007) 0.14ng/ul m

response 555

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	136.76#
104.00	15.60	116.58#
0.00	0.00	0.00

> 5.5
 12/27/16

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
Data File : BM008637.D
Acq On : 24 Dec 2016 17:38
Operator : UM/SJ
Sample : H5995-13DL 2X
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA881DL

Quant Time: Dec 26 00:37:47 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Dec 25 23:48:32 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

sohil
12/26/2016 6:27:51 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	418	0.40	ng/ul	-0.03
2) Naphthalene-d8	10.43	136	1324	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.30	164	763	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.04	188	1430	0.40	ng/ul	-0.02
16) Chrysene-d12	21.27	240	1483	0.40	ng/ul	0.00
20) Perylene-d12	23.49	264	1777	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.05	152	232	0.11	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	555m	0.14	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

> 9.5
12/27/16

Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
 Data File : BM008637.D
 Acq On : 24 Dec 2016 17:38
 Operator : UM/SJ
 Sample : H5995-13DL 2X
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA881DL

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:27:51 PM

Quant Time: Dec 26 00:37:47 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Dec 25 23:48:32 2016
 Response via : Initial Calibration

