

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
Data File : BM008639.D
Acq On : 24 Dec 2016 18:50
Operator : UM/SJ
Sample : H6040-13DL 2X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :

BNA_M

ClientSampleId :

DA8W6DL

Manual Integrations
APPROVED

sohil

12/26/2016 6:27:54 PM




Quant Time: Dec 26 00:01:43 2016

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sun Dec 25 23:48:32 2016

Response via : Initial Calibration

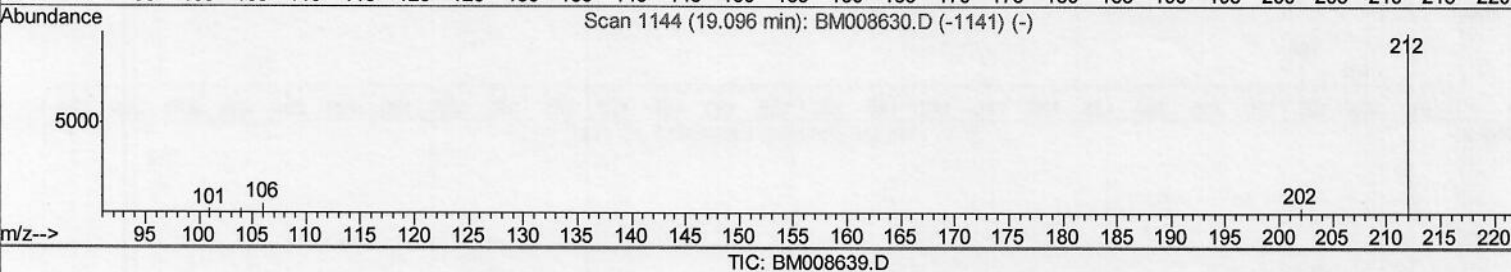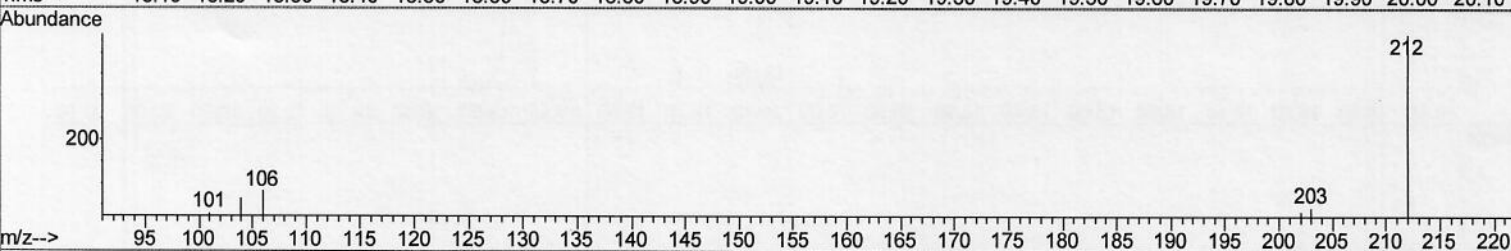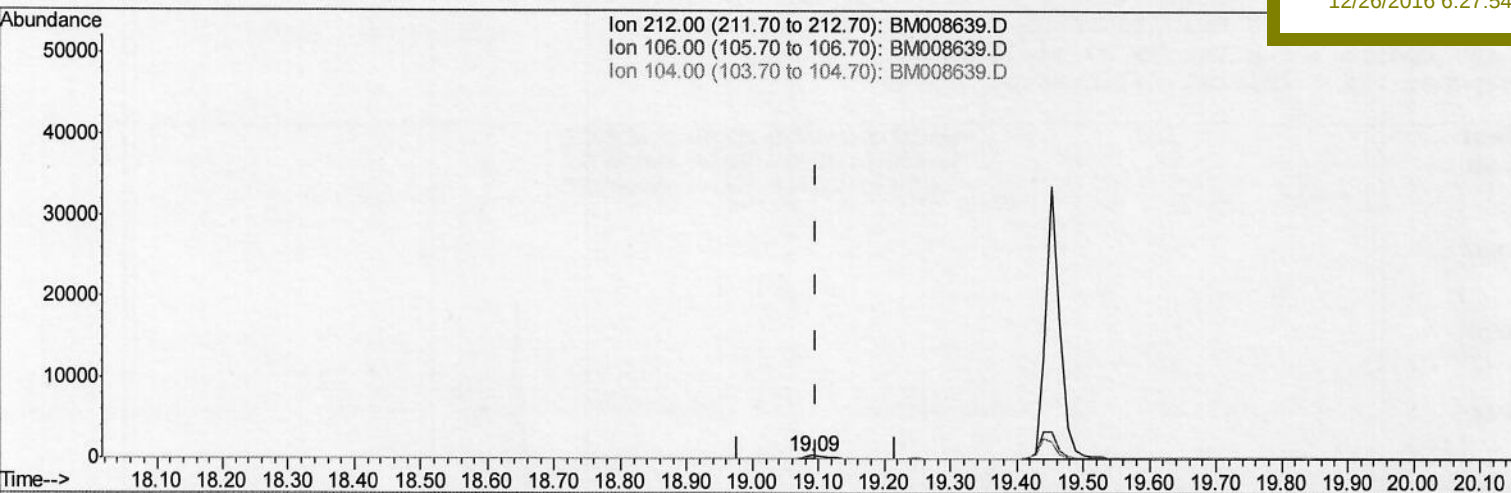

(14) Fluoranthene-d10 (SURR)

19.089min (-0.007) 0.27ng/ul

response 1103

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	51.95#
104.00	15.60	56.30#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
 Data File : BM008639.D
 Acq On : 24 Dec 2016 18:50
 Operator : UM/SJ
 Sample : H6040-13DL 2X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8W6DL

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:27:54 PM

Quant Time: Dec 26 00:01:43 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Dec 25 23:48:32 2016
 Response via : Initial Calibration

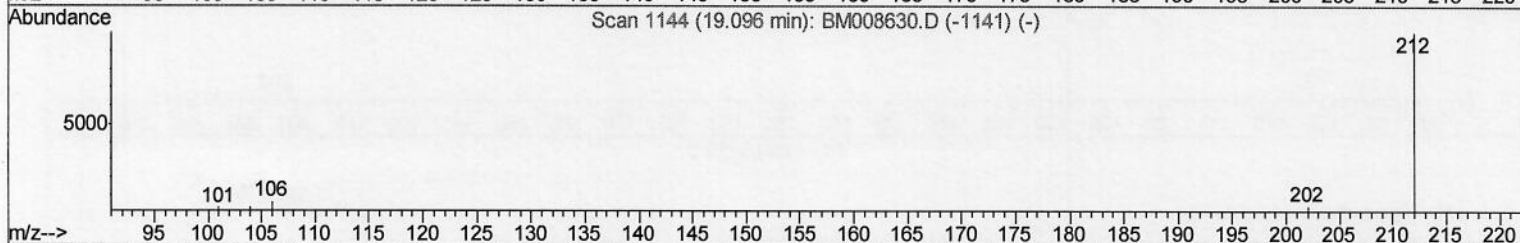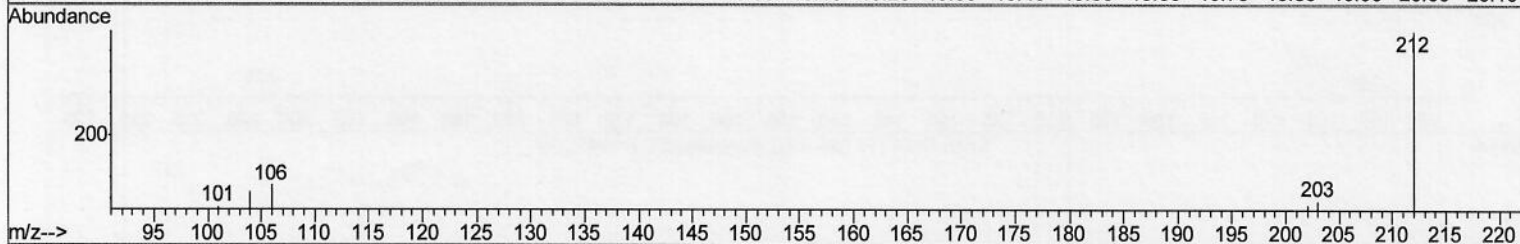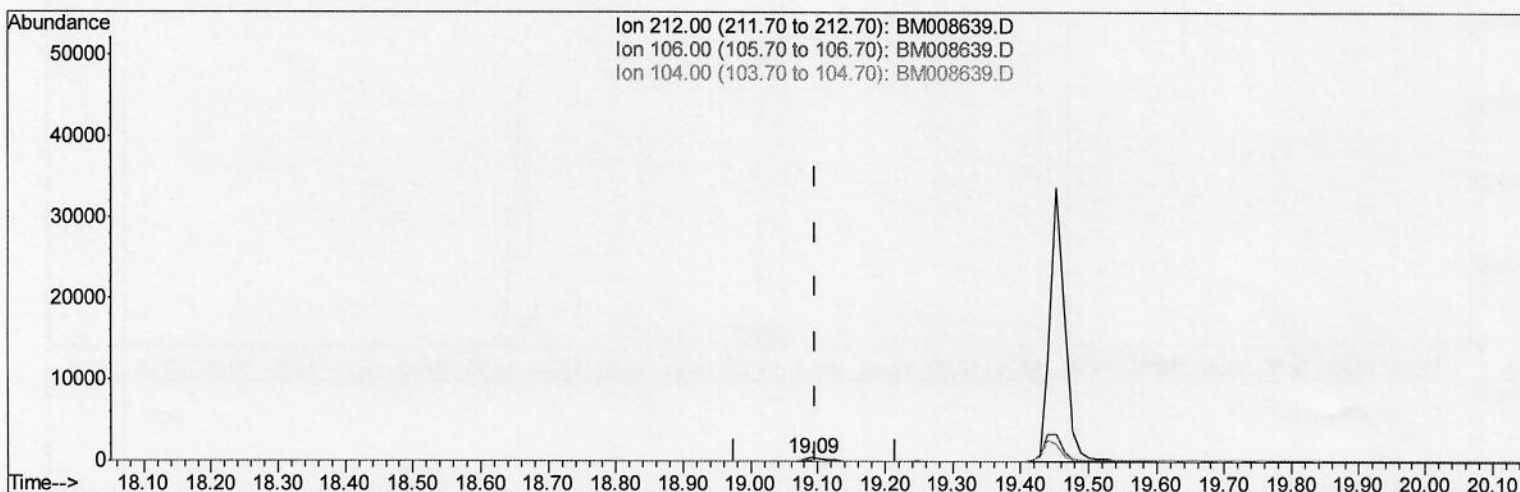

TIC: BM008639.D

(14) Fluoranthene-d10 (SURR)

19.089min (-0.007) 0.16ng/ul m

response 658

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	87.08#
104.00	15.60	94.38#
0.00	0.00	0.00

25.7
 12/27/16

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
Data File : BM008639.D
Acq On : 24 Dec 2016 18:50
Operator : UM/SJ
Sample : H6040-13DL 2X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA8W6DL

Manual Integrations
APPROVED

sohil
12/26/2016 6:27:54 PM

Quant Time: Dec 26 00:42:06 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Dec 25 23:48:32 2016
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	475	0.40	ng/ul	-0.03
2) Naphthalene-d8	10.43	136	1442	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.30	164	835	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.04	188	1510	0.40	ng/ul	-0.02
16) Chrysene-d12	21.27	240	1548	0.40	ng/ul	0.00
20) Perylene-d12	23.49	264	1928	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.06	152	240	0.11	ng/ul	0.01
14) Fluoranthene-d10	19.09	212	658m	0.16	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

5.9
12/27/16

Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
 Data File : BM008639.D
 Acq On : 24 Dec 2016 18:50
 Operator : UM/SJ
 Sample : H6040-13DL 2X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA8W6DL

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:27:54 PM

Quant Time: Dec 26 00:42:06 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Dec 25 23:48:32 2016
 Response via : Initial Calibration

