

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
 Data File : BM008646.D
 Acq On : 24 Dec 2016 23:33
 Operator : UM/SJ
 Sample : H6069-06DL 2X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA7J2DL

Quant Time: Dec 26 00:59:05 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 00:55:42 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:28:03 PM

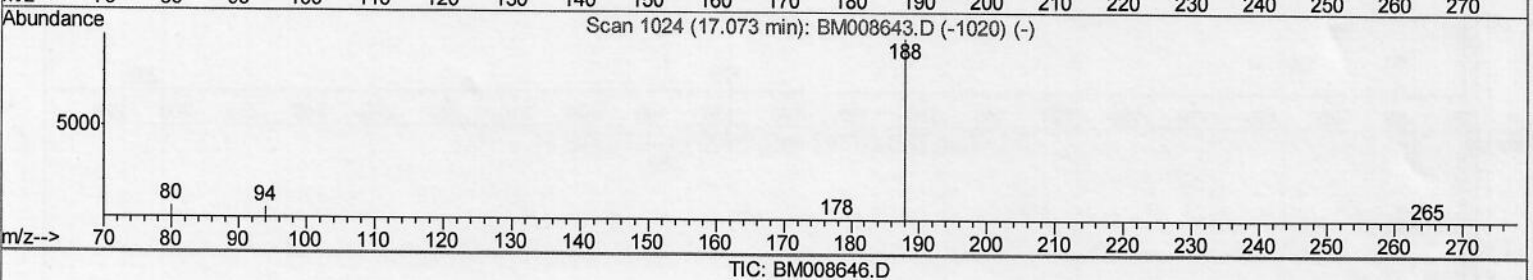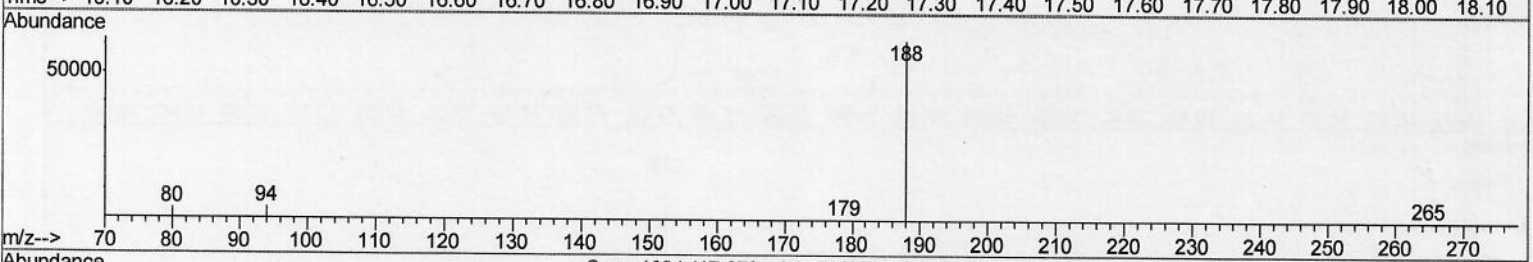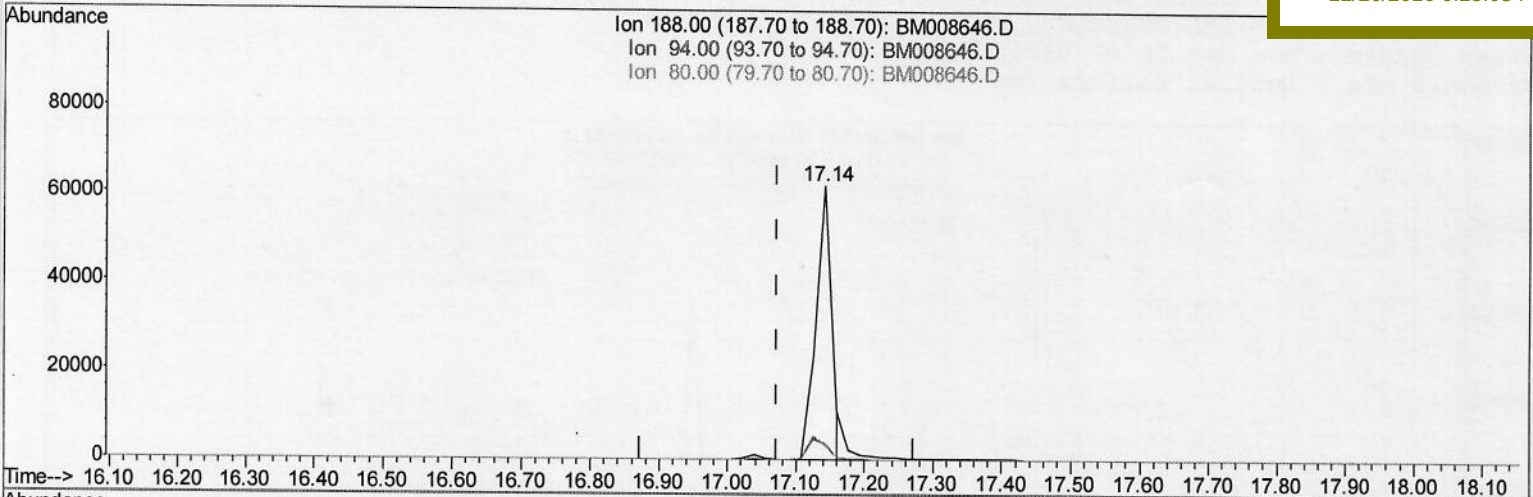

(10) Phenanthrene-d10 (I)

17.142min (+0.069) 0.40ng/ul

response 98178

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	5.96#
80.00	11.80	5.25#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
 Data File : BM008646.D
 Acq On : 24 Dec 2016 23:33
 Operator : UM/SJ
 Sample : H6069-06DL 2X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA7J2DL

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:28:03 PM

Quant Time: Dec 26 00:59:05 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 00:55:42 2016
 Response via : Initial Calibration

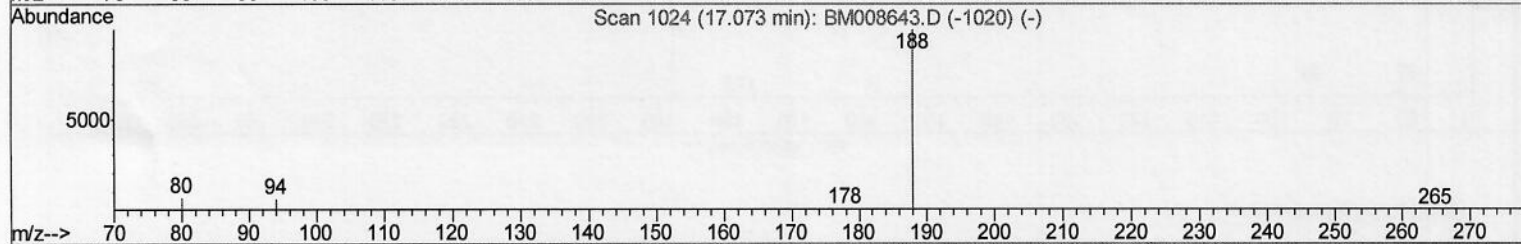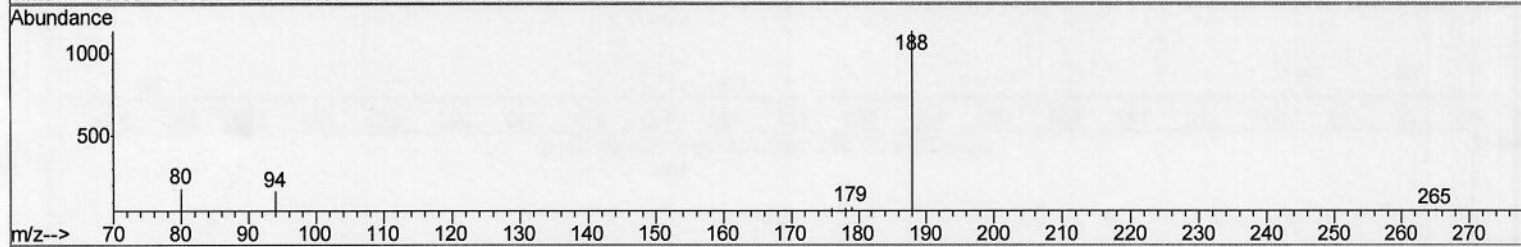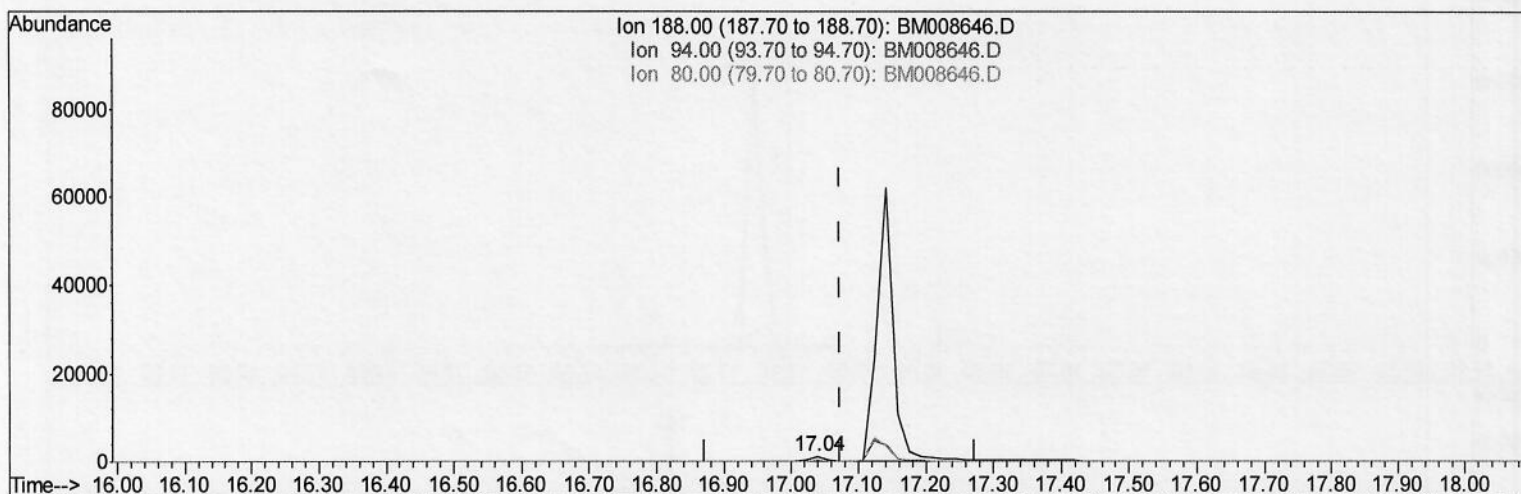

TIC: BM008646.D

(10) Phenanthrene-d10 (I)

17.039min (-0.034) 0.40ng/ul m

response 1869

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	14.42#
80.00	11.80	16.19#
0.00	0.00	0.00

Handwritten: 5.5
 12/27/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
 Data File : BM008646.D
 Acq On : 24 Dec 2016 23:33
 Operator : UM/SJ
 Sample : H6069-06DL 2X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA7J2DL

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:28:03 PM

Quant Time: Dec 26 00:59:05 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 00:55:42 2016
 Response via : Initial Calibration

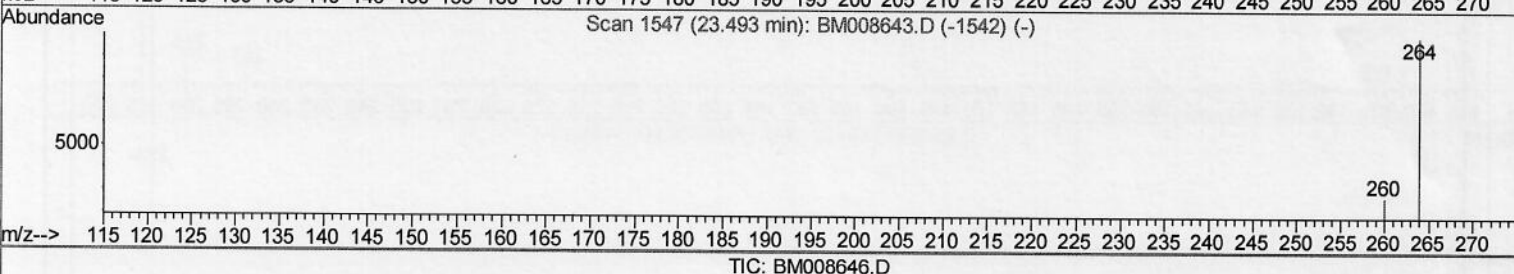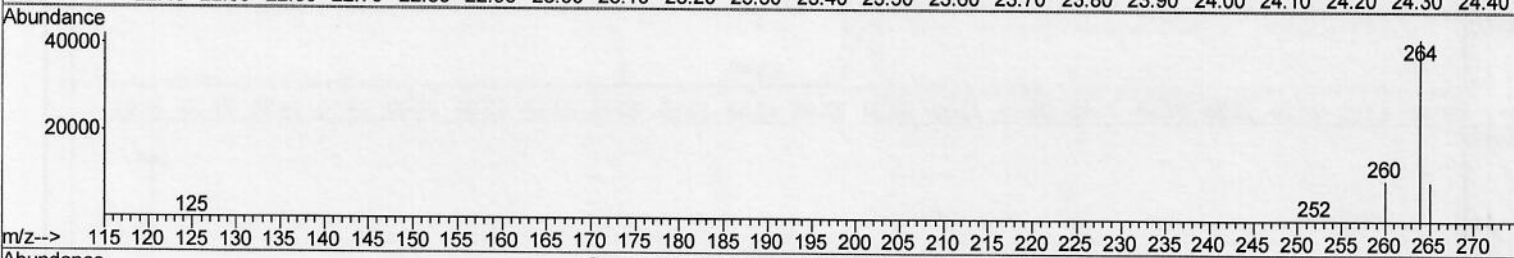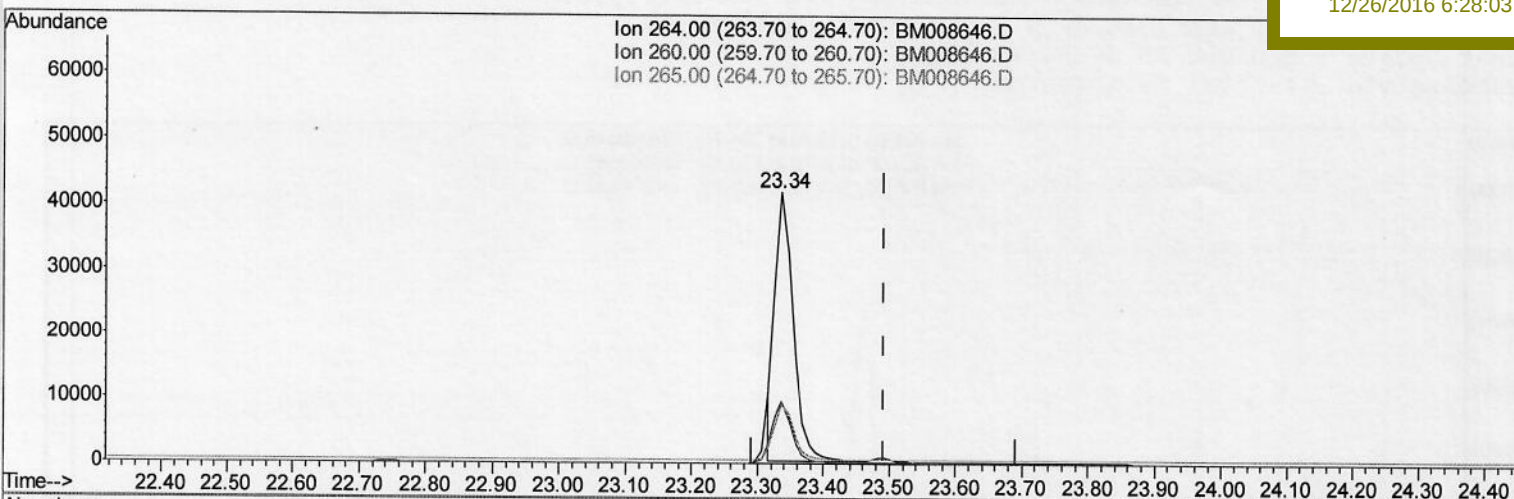

(20) Perylene-d12 (I)

23.337min (-0.156) 0.40ng/ui

response 80531

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	22.64#
265.00	103.50	21.58#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
Data File : BM008646.D
Acq On : 24 Dec 2016 23:33
Operator : UM/SJ
Sample : H6069-06DL 2X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA7J2DL

Manual Integrations
APPROVED

sohil
12/26/2016 6:28:03 PM

Quant Time: Dec 26 00:59:05 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 26 00:55:42 2016
Response via : Initial Calibration

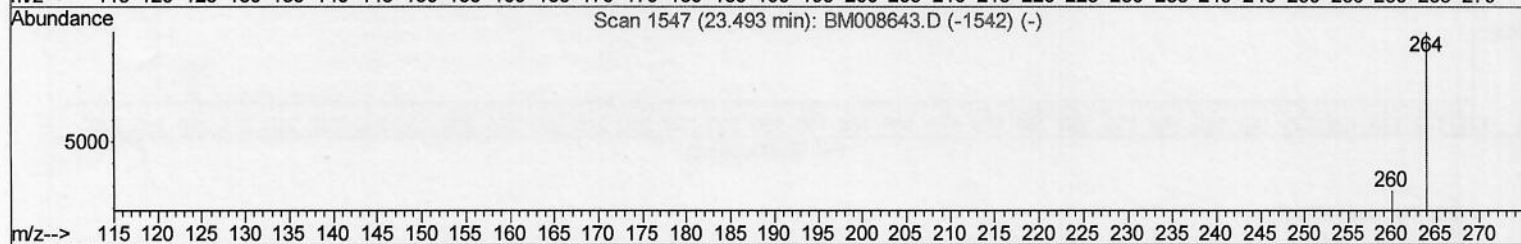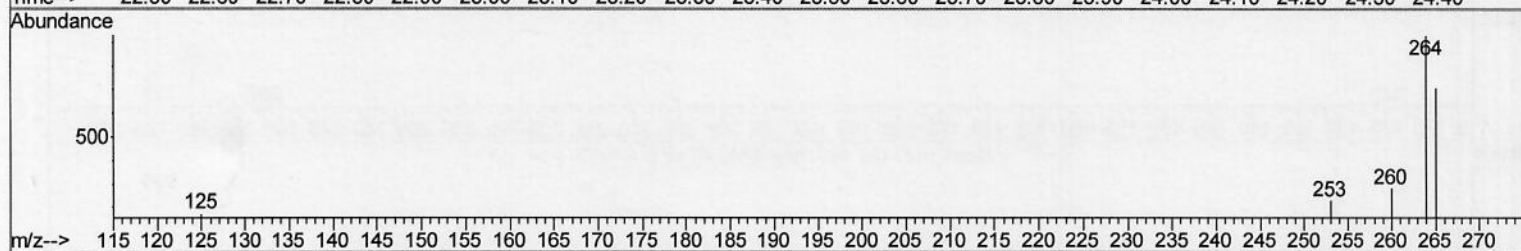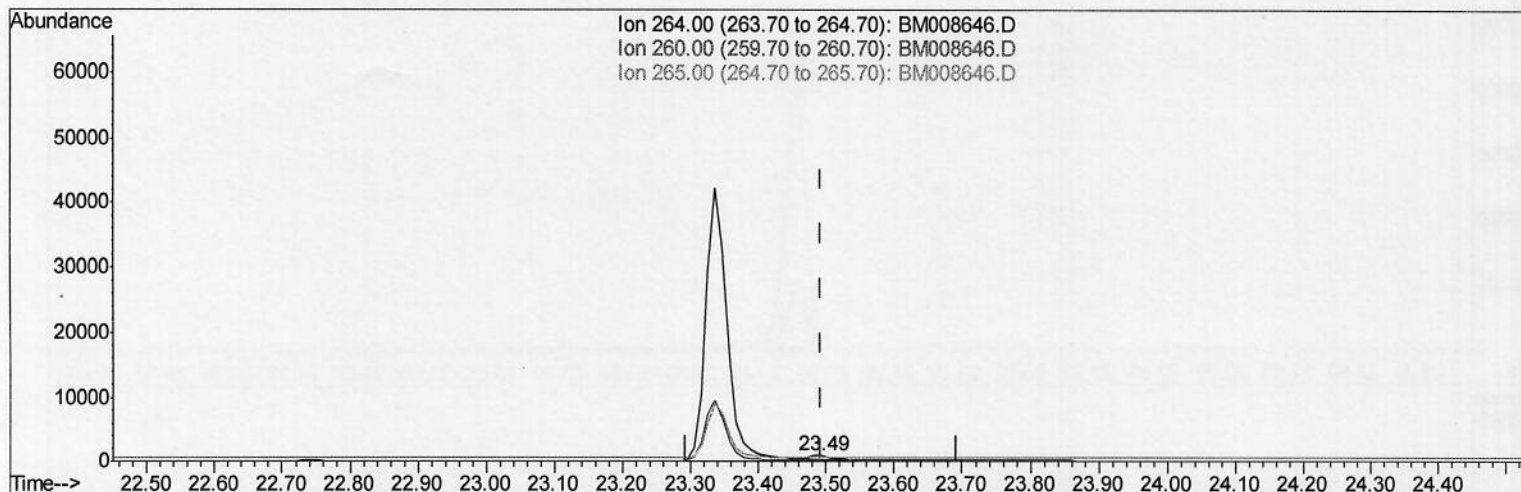

TIC: BM008646.D

(20) Perylene-d12 (I)

23.493min (+0.000) 0.40ng/ul m

response 1165

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	30.08
265.00	103.50	75.73#
0.00	0.00	0.00

> 5.5
12/27/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
Data File : BM008646.D
Acq On : 24 Dec 2016 23:33
Operator : UM/SJ
Sample : H6069-06DL 2X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA7J2DL

Manual Integrations
APPROVED

sohil
12/26/2016 6:28:03 PM

Quant Time: Dec 26 01:32:23 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 26 00:55:42 2016
Response via : Initial Calibration

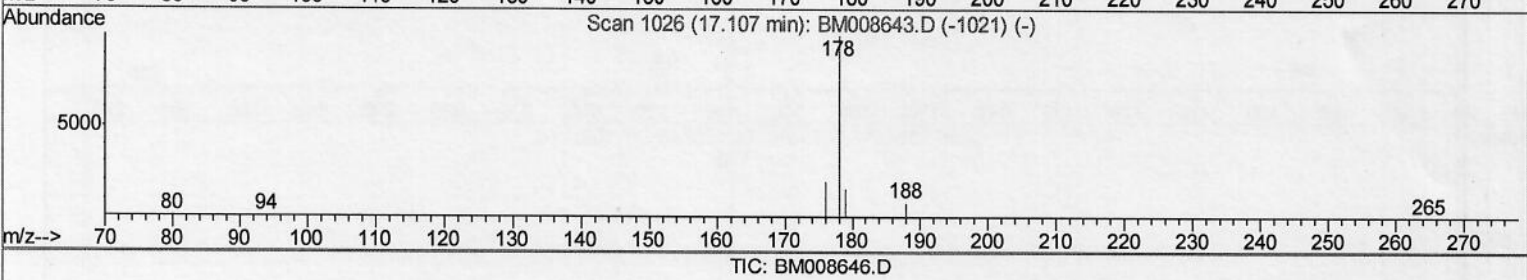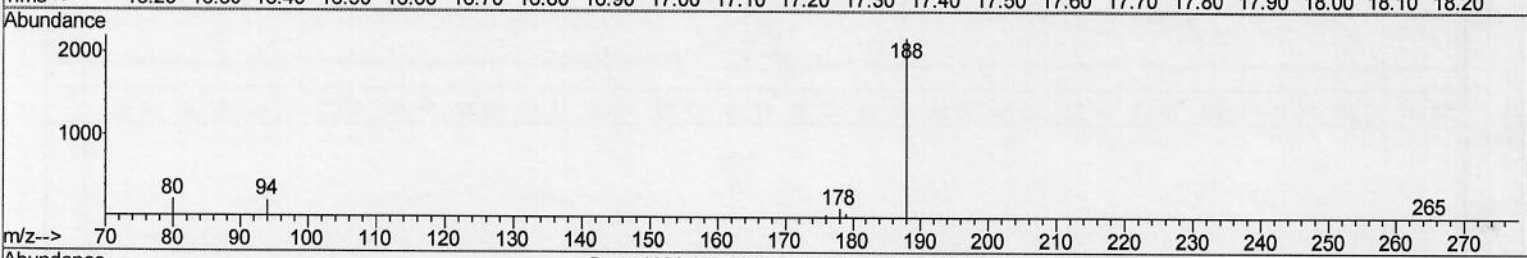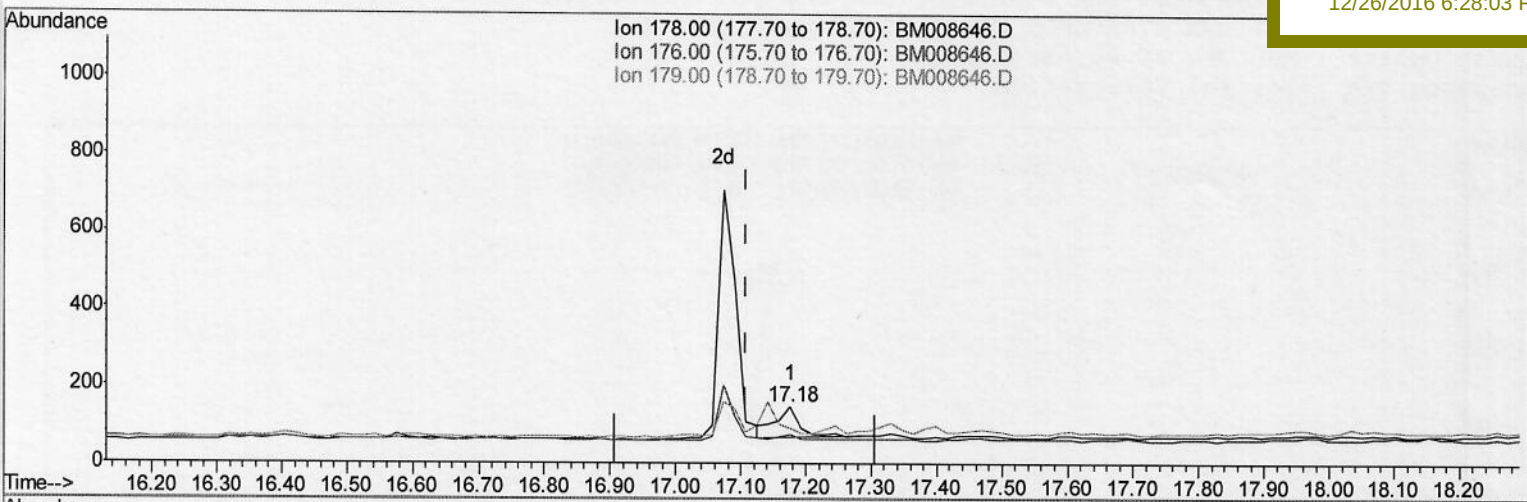

(12) Phenanthrene

17.176min (+0.069) 0.04ng/ul

response 207

Ion	Exp%	Act%
178.00	100	100
176.00	23.00	50.34#
179.00	17.00	61.38#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
 Data File : BM008646.D
 Acq On : 24 Dec 2016 23:33
 Operator : UM/SJ
 Sample : H6069-06DL 2X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA7J2DL

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:28:03 PM

Quant Time: Dec 26 01:32:23 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 00:55:42 2016
 Response via : Initial Calibration

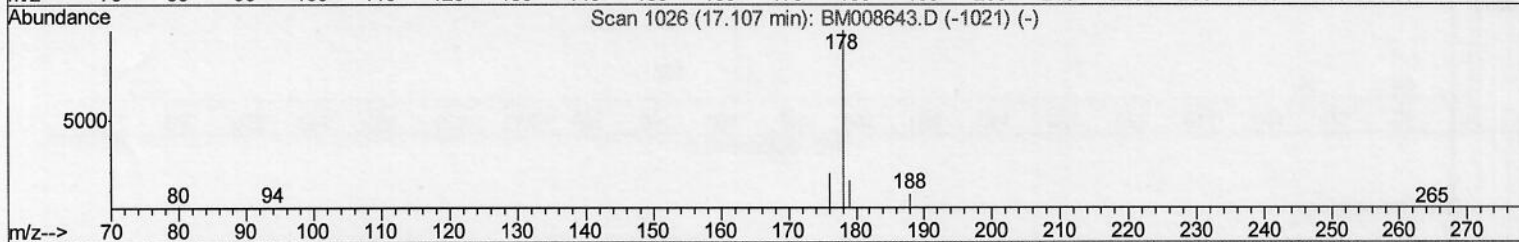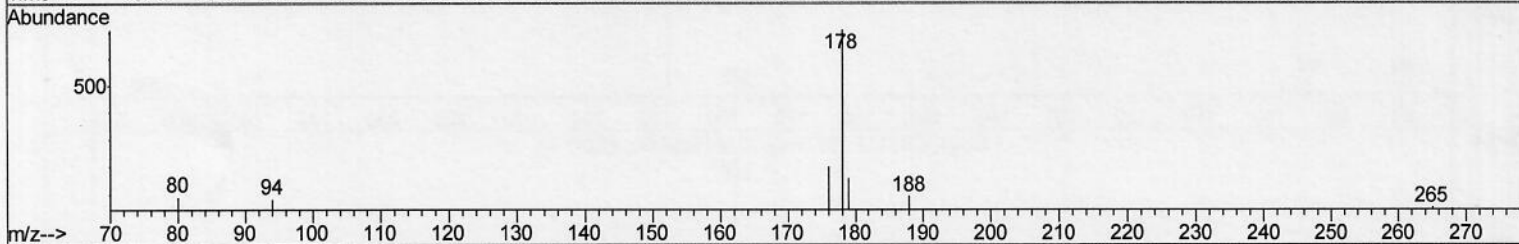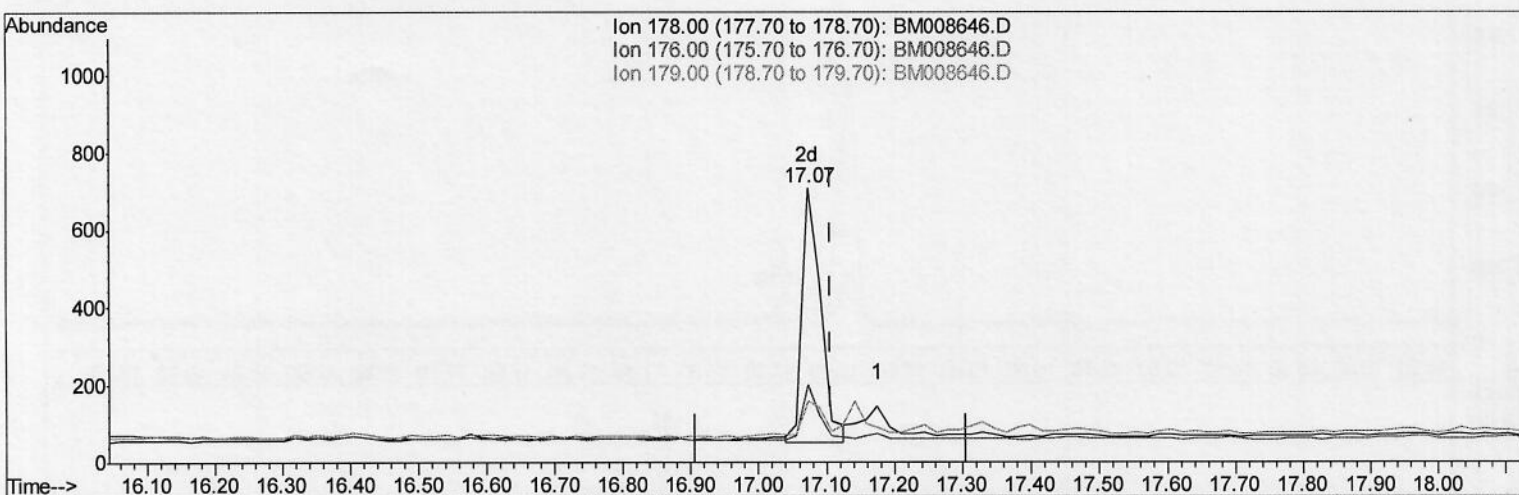

TIC: BM008646.D

(12) Phenanthrene

17.073min (-0.034) 0.22ng/ul m

response 1264

Ion	Exp%	Act%
178.00	100	100
176.00	23.00	28.39#
179.00	17.00	22.46#
0.00	0.00	0.00

9.9
 12/27/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
 Data File : BM008646.D
 Acq On : 24 Dec 2016 23:33
 Operator : UM/SJ
 Sample : H6069-06DL 2X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Quant Time: Dec 26 01:32:23 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 00:55:42 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 DA7J2DL

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:28:03 PM

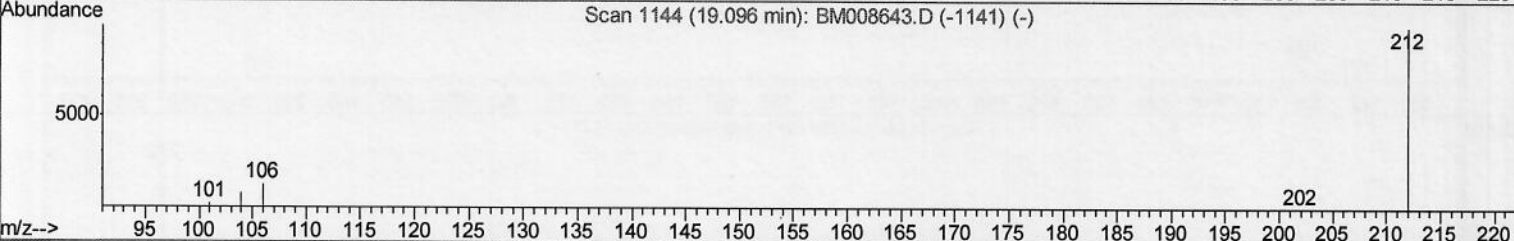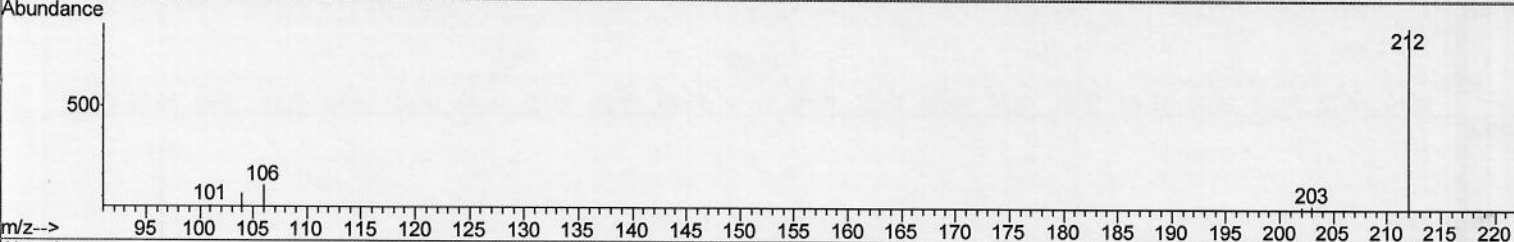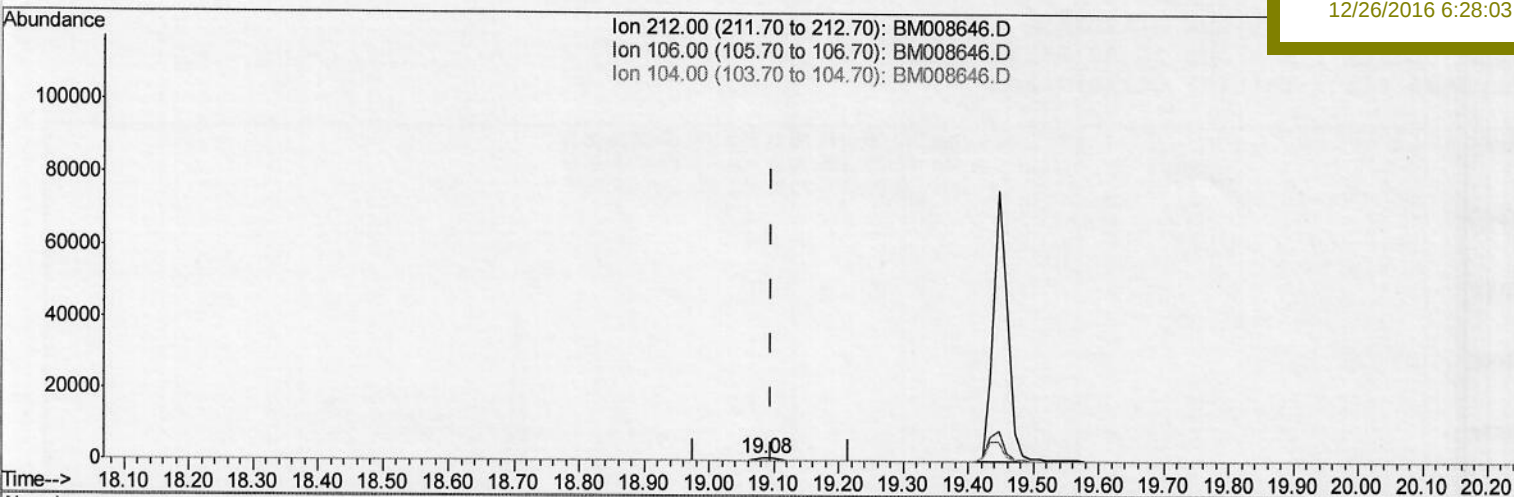

TIC: BM008646.D

(14) Fluoranthene-d10 (SURR)

19.084min (-0.012) 0.22ng/ul

response 1147

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
Data File : BM008646.D
Acq On : 24 Dec 2016 23:33
Operator : UM/SJ
Sample : H6069-06DL 2X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DA7J2DL

Manual Integrations
APPROVED

sohil
12/26/2016 6:28:03 PM

Quant Time: Dec 26 01:32:23 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 26 00:55:42 2016
Response via : Initial Calibration

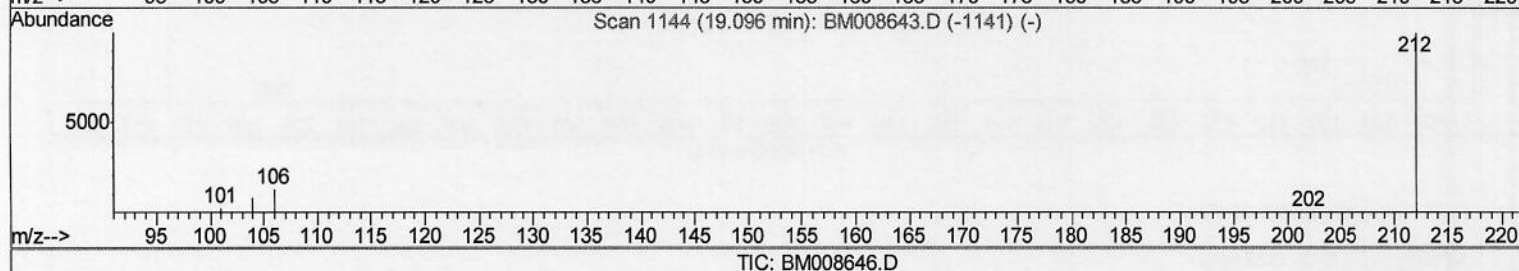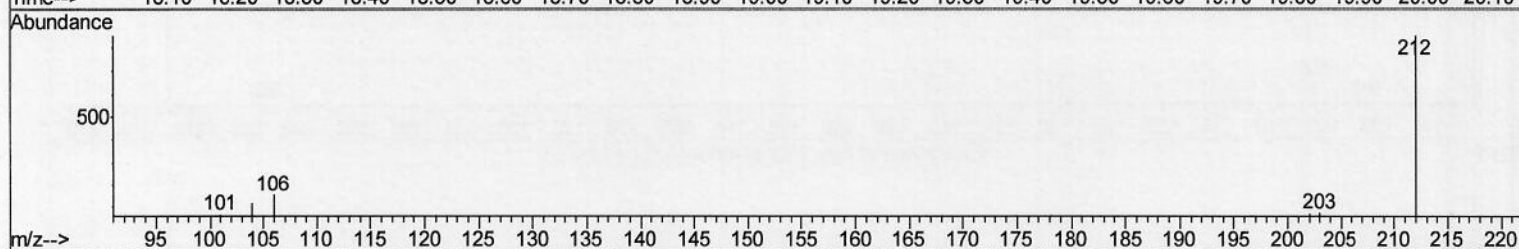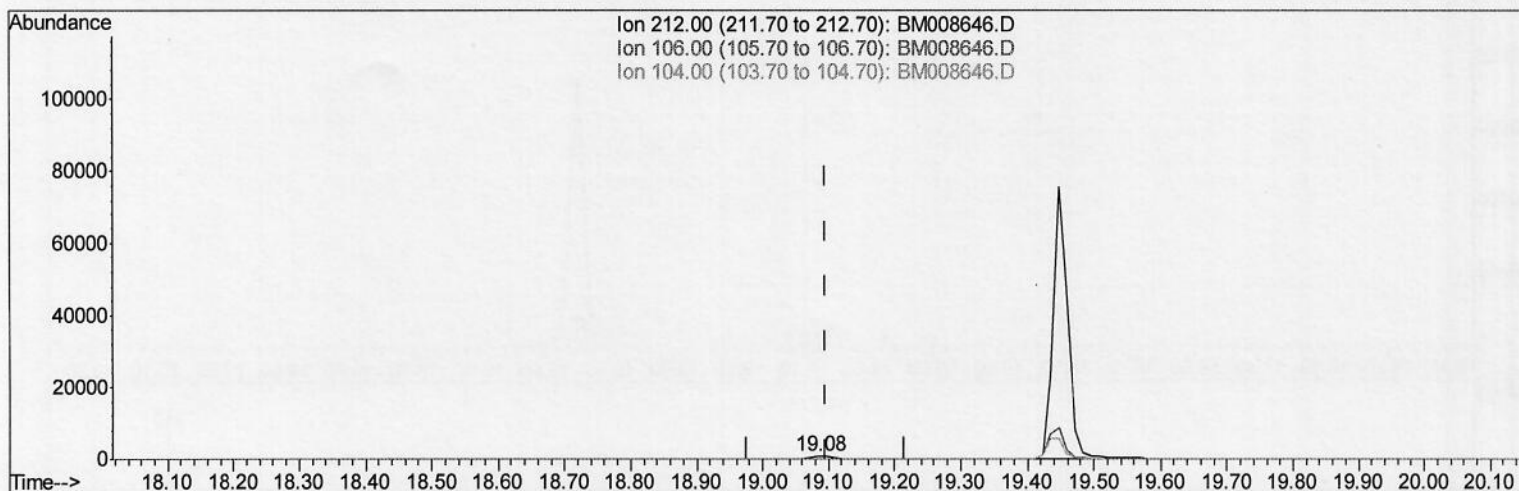

(14) Fluoranthene-d10 (SURR)

19.084min (-0.012) 0.28ng/ul m

response 1435

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

25.7
12/24/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
 Data File : BM008646.D
 Acq On : 24 Dec 2016 23:33
 Operator : UM/SJ
 Sample : H6069-06DL 2X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA7J2DL

Quant Time: Dec 26 01:32:23 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 00:55:42 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:28:03 PM

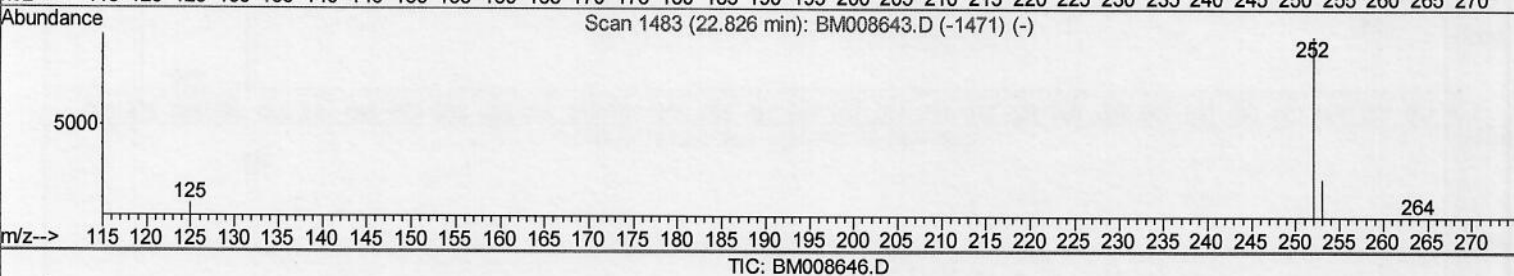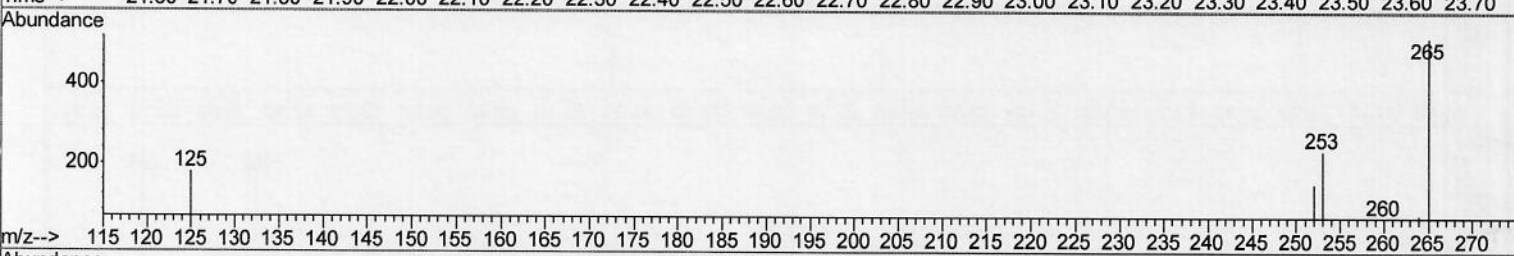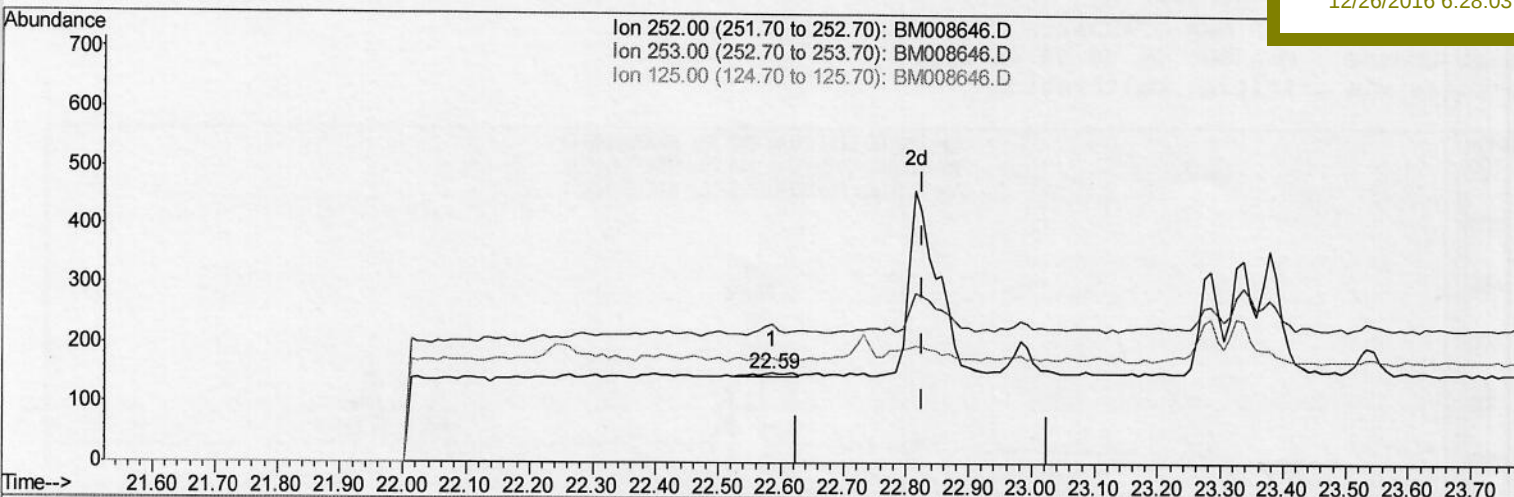

(21) Benzo(b)fluoranthene

22.586min (-0.240) 0.01ng/ui

response 25

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	155.33#
125.00	17.50	117.33#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
 Data File : BM008646.D
 Acq On : 24 Dec 2016 23:33
 Operator : UM/SJ
 Sample : H6069-06DL 2X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA7J2DL

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:28:03 PM

Quant Time: Dec 26 01:32:23 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 00:55:42 2016
 Response via : Initial Calibration

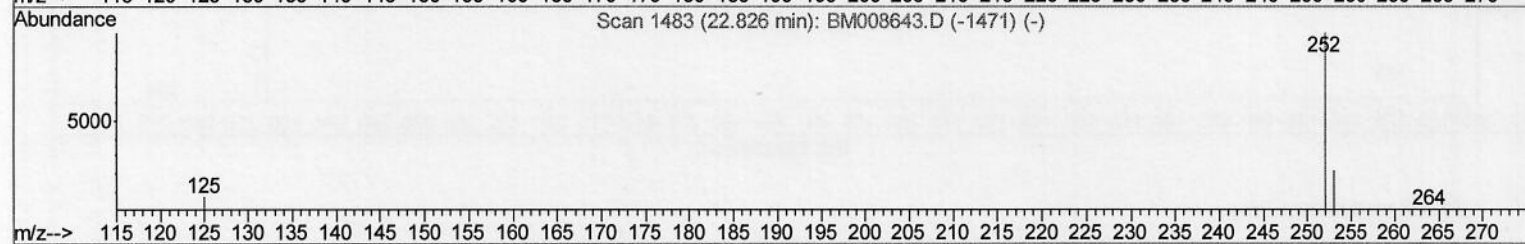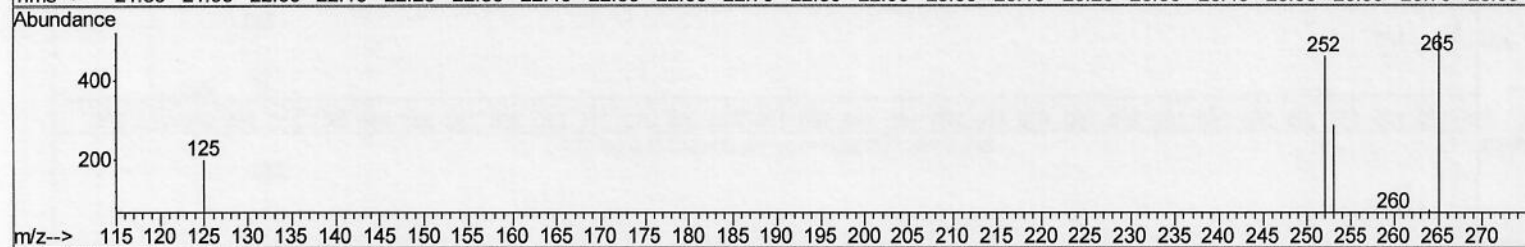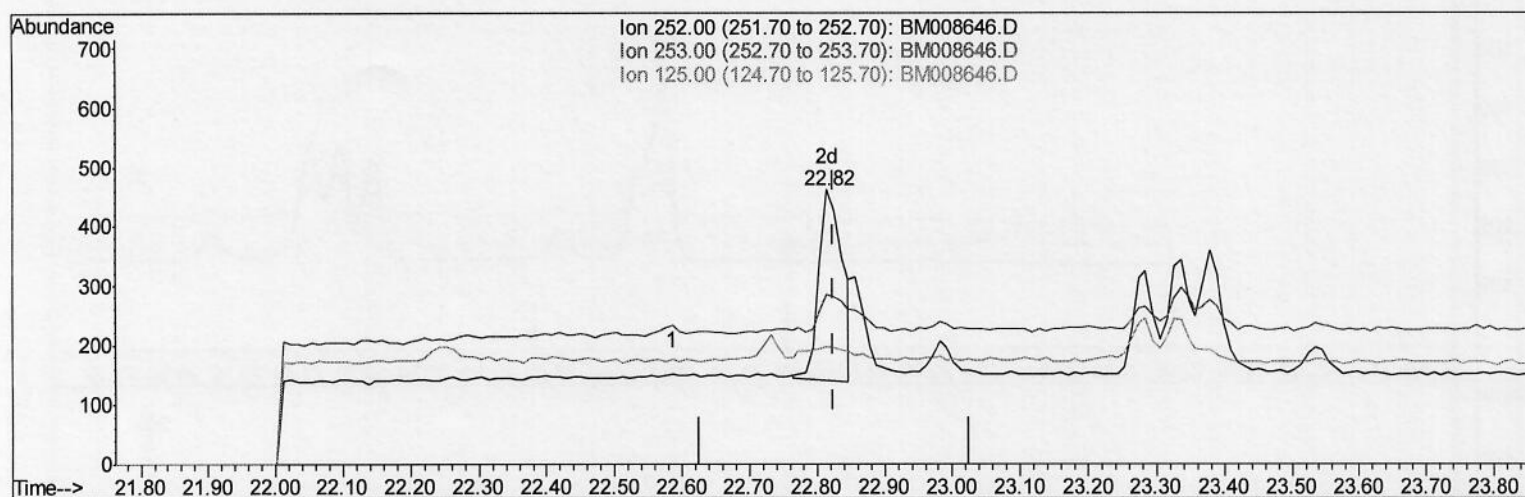

(21) Benzo(b)fluoranthene

22.815min (-0.010) 0.17ng/ul m

response 781

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	61.82
125.00	17.50	42.95#
0.00	0.00	0.00

> 5.9
 12/24/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
 Data File : BM008646.D
 Acq On : 24 Dec 2016 23:33
 Operator : UM/SJ
 Sample : H6069-06DL 2X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA7J2DL

Quant Time: Dec 26 01:32:23 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 00:55:42 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:28:03 PM

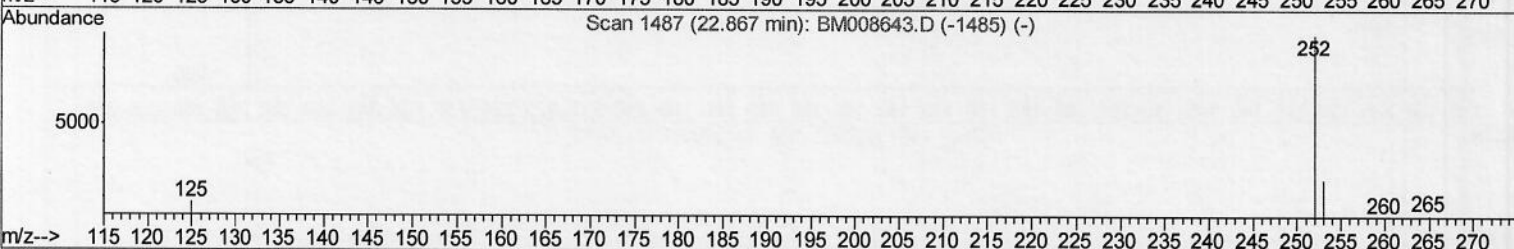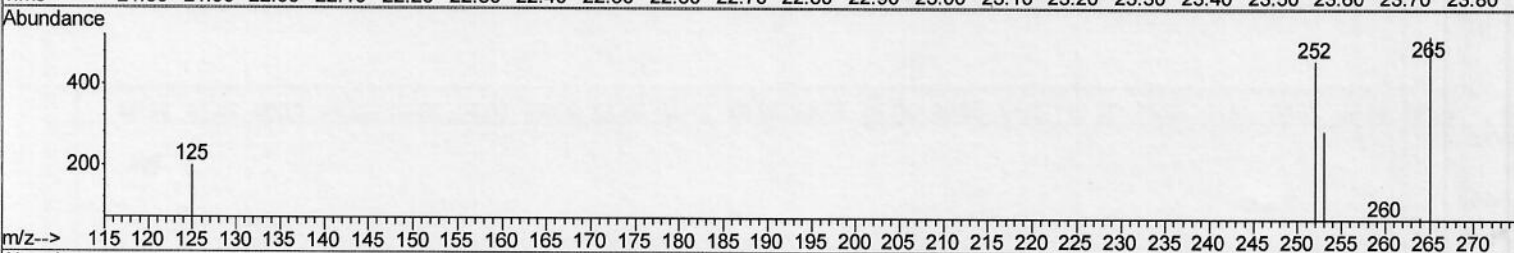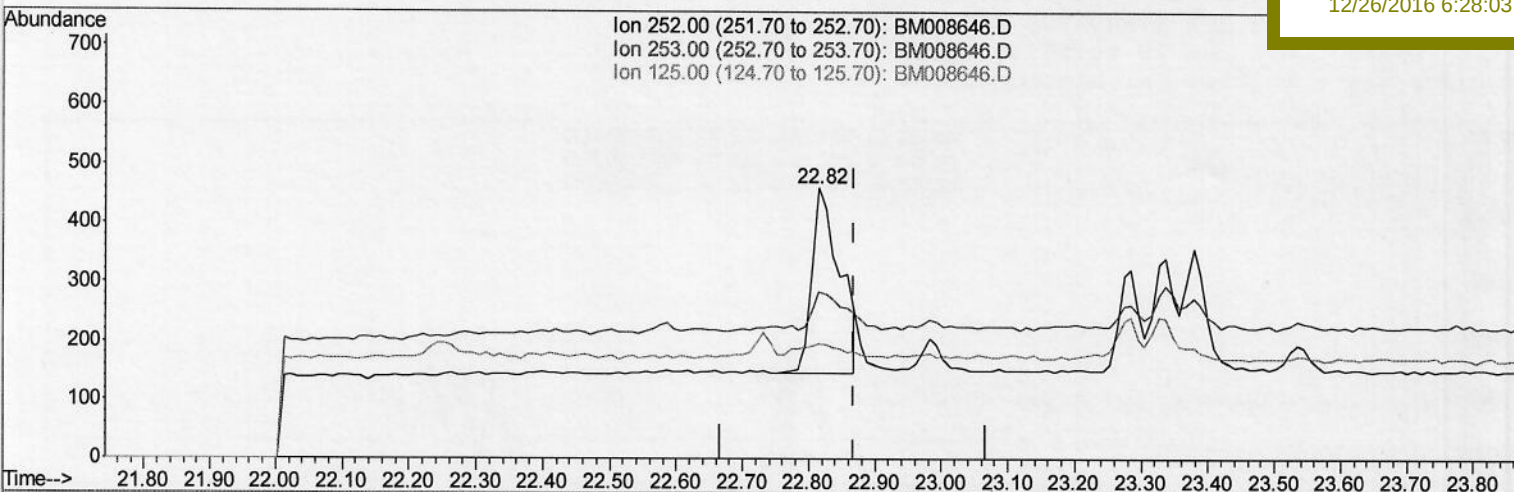

TIC: BM008646.D

(22) Benzo(k)fluoranthene

22.815min (-0.052) 0.21ng/ul

response 934

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	61.82#
125.00	17.10	42.95#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
 Data File : BM008646.D
 Acq On : 24 Dec 2016 23:33
 Operator : UM/SJ
 Sample : H6069-06DL 2X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 Client Sampled :
 DA7J2DL

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:28:03 PM

Quant Time: Dec 26 01:32:23 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 00:55:42 2016
 Response via : Initial Calibration

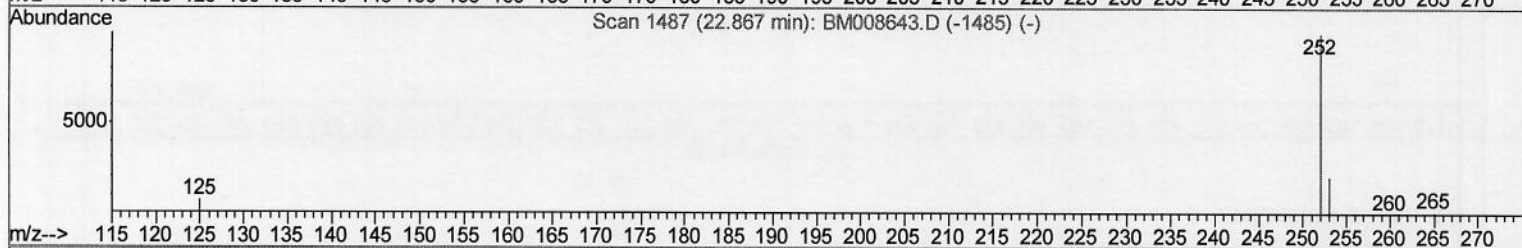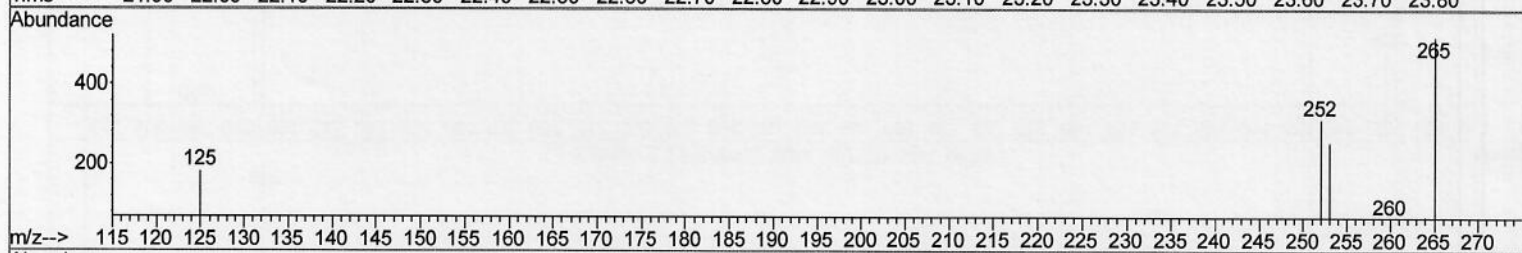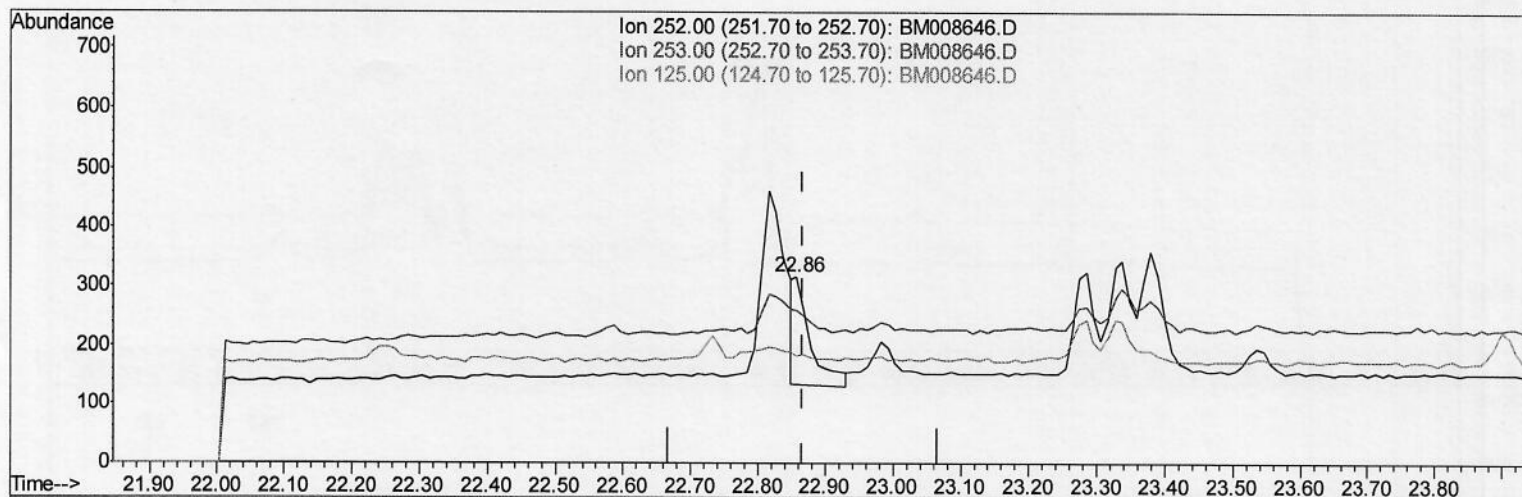

TIC: BM008646.D

(22) Benzo(k)fluoranthene

22.857min (-0.010) 0.07ng/ul m

response 317

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	81.90#
125.00	17.10	58.10#
0.00	0.00	0.00

> 5.9
 12/27/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
 Data File : BM008646.D
 Acq On : 24 Dec 2016 23:33
 Operator : UM/SJ
 Sample : H6069-06DL 2X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Quant Time: Dec 26 01:32:23 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 00:55:42 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 DA7J2DL

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:28:03 PM

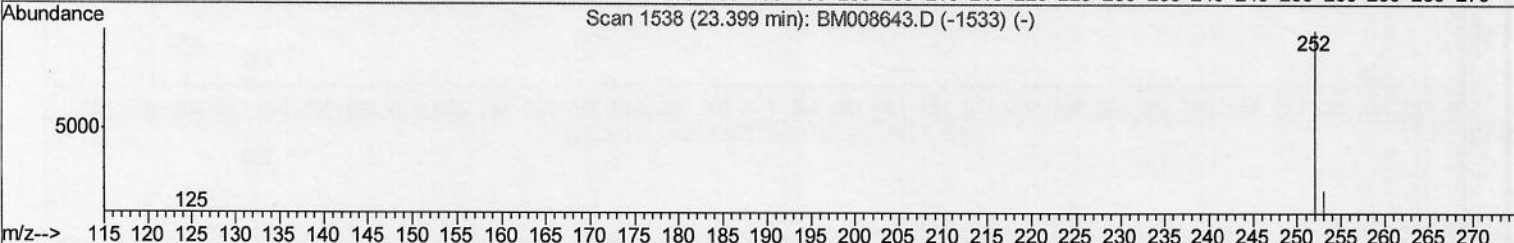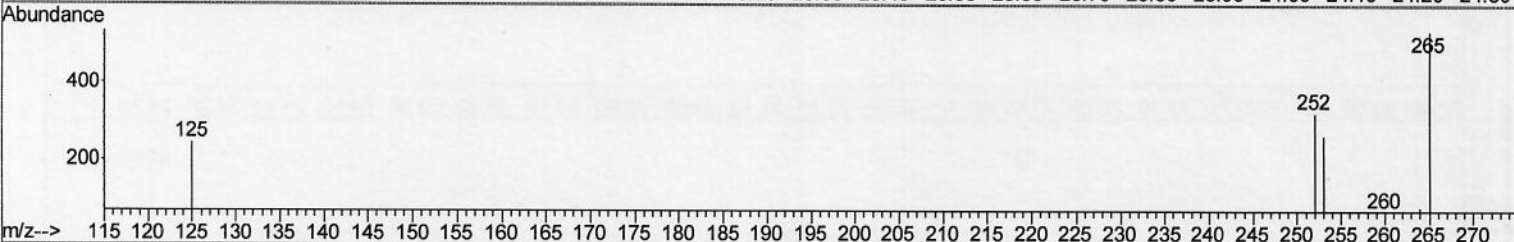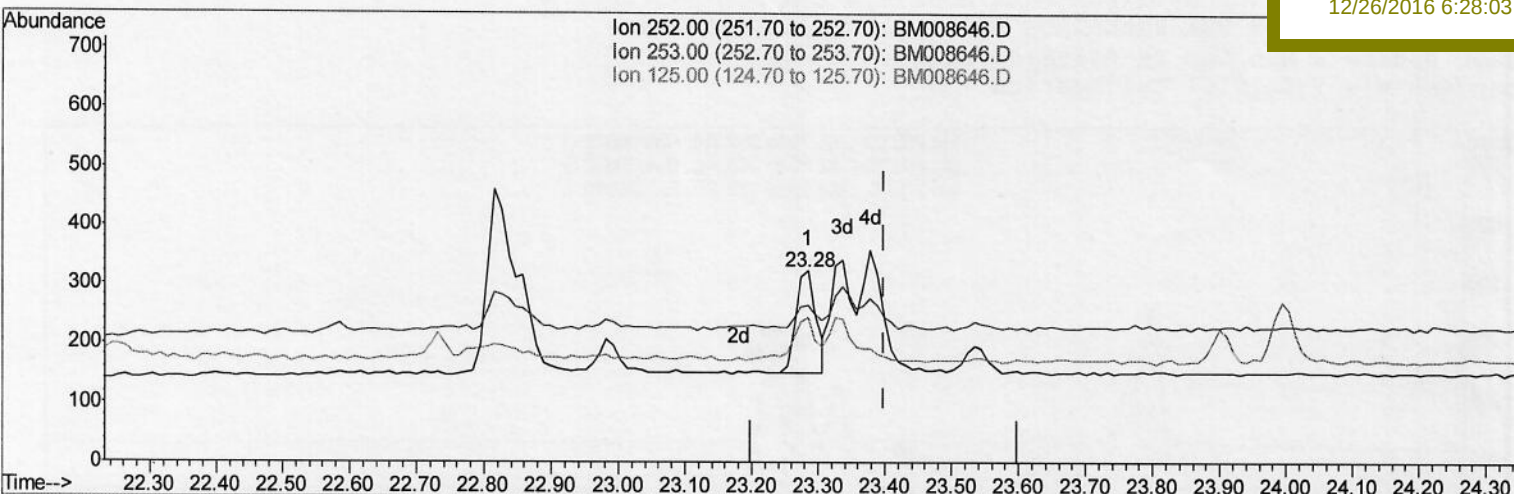

TIC: BM008646.D

(23) Benzo(a)pyrene (C)

23.284min (-0.115) 0.08ng/ul

response 358

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	81.99#
125.00	22.60	75.47#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
Data File : BM008646.D
Acq On : 24 Dec 2016 23:33
Operator : UM/SJ
Sample : H6069-06DL 2X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_M
Client Sampled :
DA7J2DL

Manual Integrations
APPROVED

sohil
12/26/2016 6:28:03 PM

Quant Time: Dec 26 01:32:23 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 26 00:55:42 2016
Response via : Initial Calibration

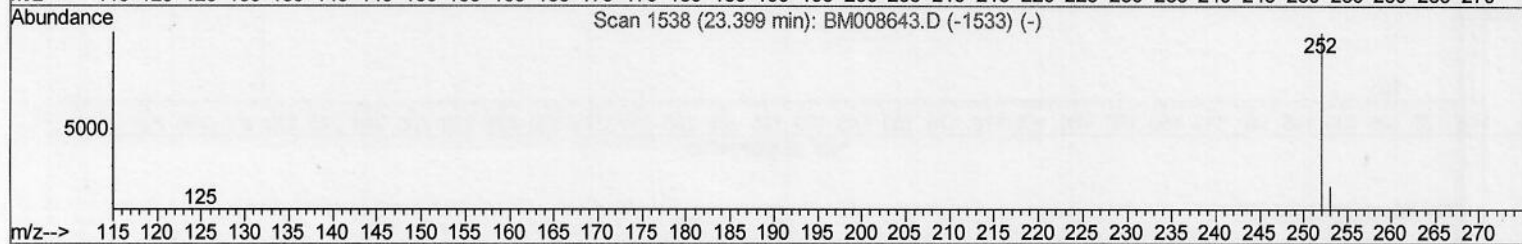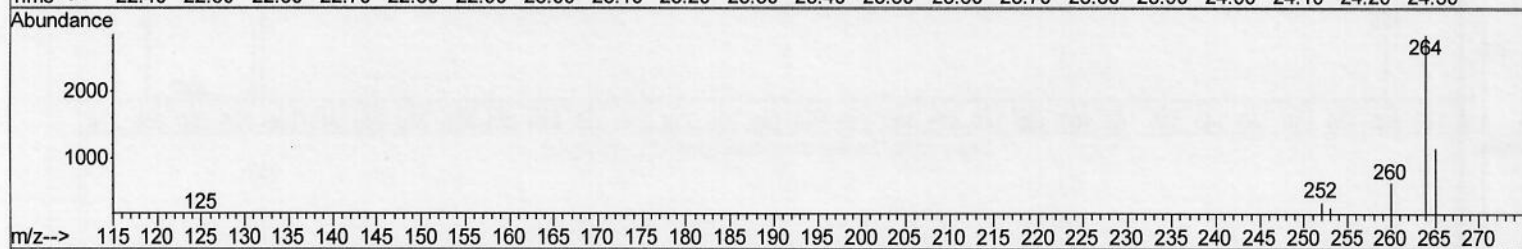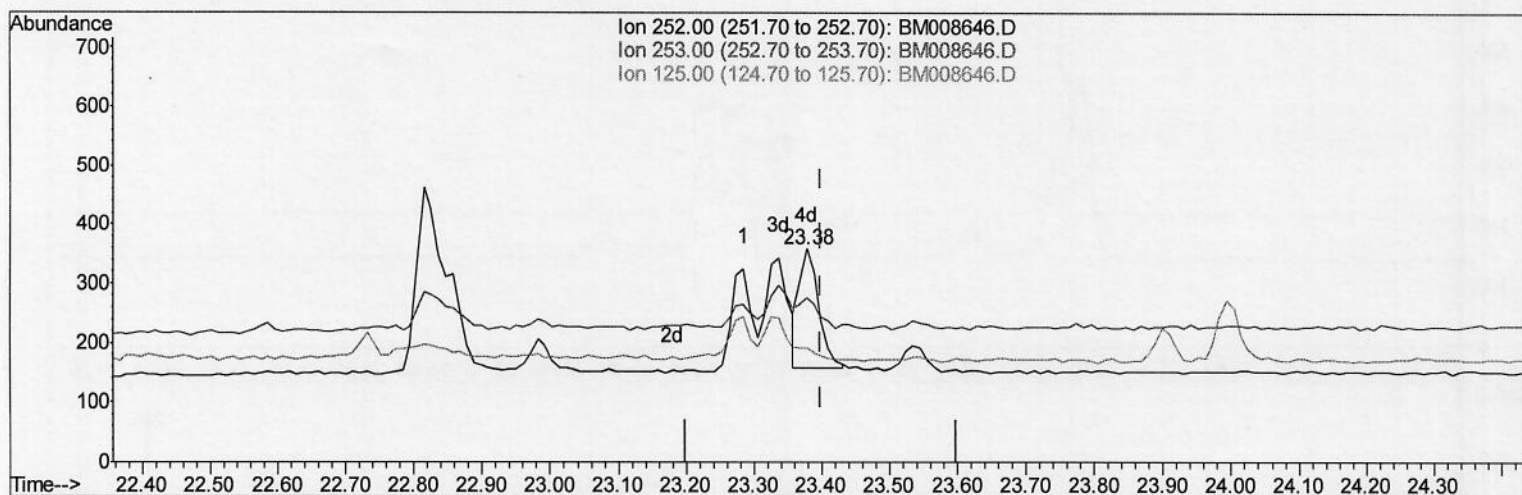

TIC: BM008646.D

(23) Benzo(a)pyrene (C)

23.378min (-0.021) 0.09ng/ul m

response 397

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	76.82#
125.00	22.60	53.35#
0.00	0.00	0.00

7 5.9
12/29/16

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
 Data File : BM008646.D
 Acq On : 24 Dec 2016 23:33
 Operator : UM/SJ
 Sample : H6069-06DL 2X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA7J2DL

Quant Time: Dec 26 01:32:23 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 00:55:42 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:28:03 PM

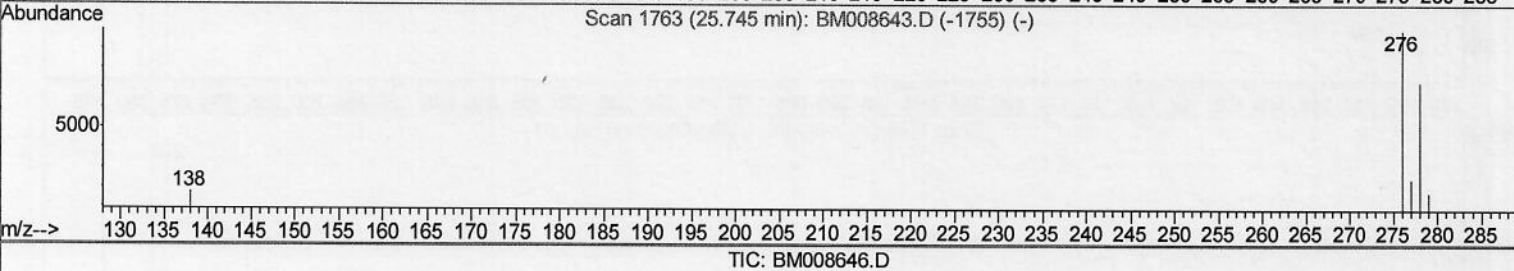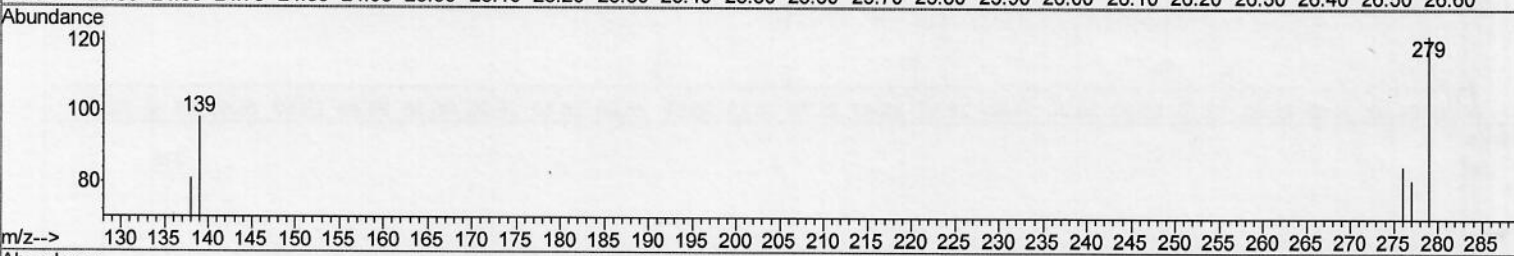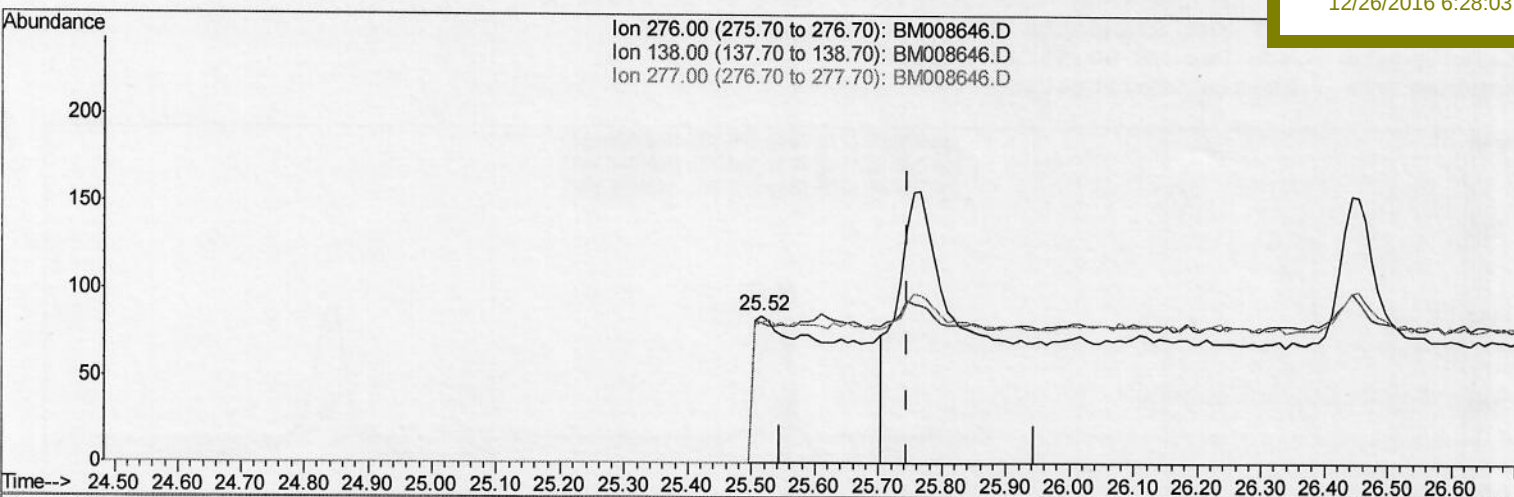

(24) Indeno(1,2,3-cd)pyrene

25.515min (-0.229) 0.18ng/ui

response 919

Ion	Exp%	Act%
276.00	100	100
138.00	23.90	0.00#
277.00	24.50	57.56#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
 Data File : BM008646.D
 Acq On : 24 Dec 2016 23:33
 Operator : UM/SJ
 Sample : H6069-06DL 2X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA7J2DL

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:28:03 PM

Quant Time: Dec 26 01:32:23 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 00:55:42 2016
 Response via : Initial Calibration

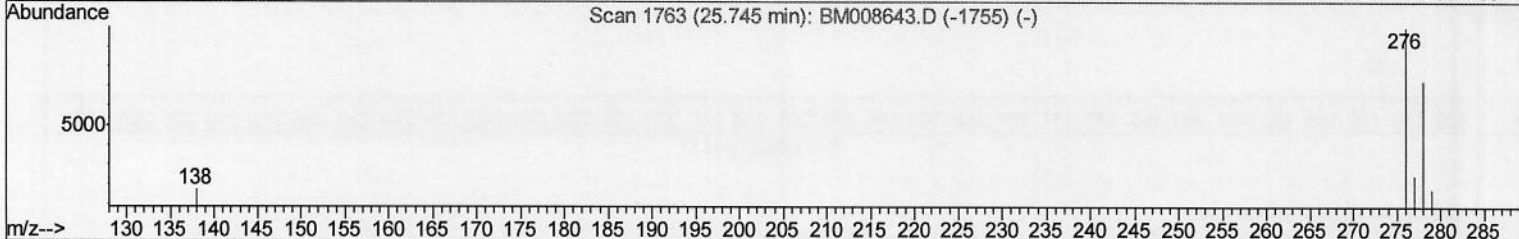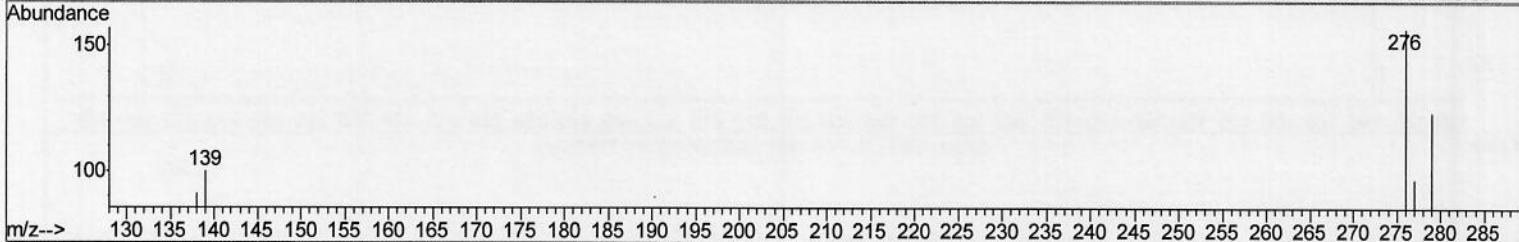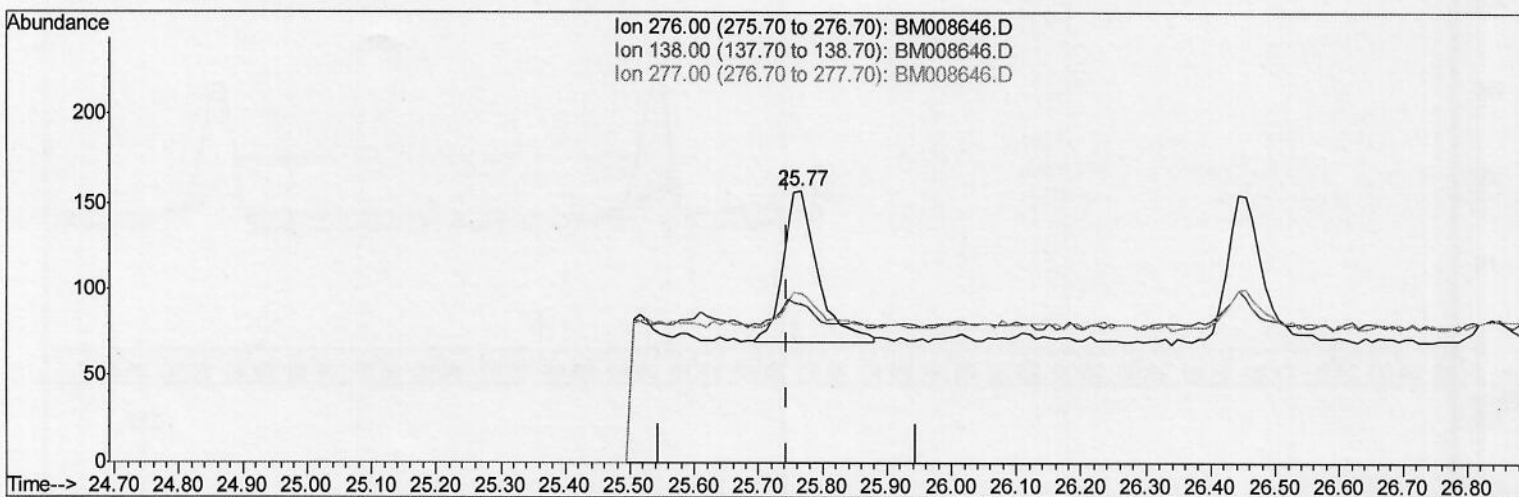

TIC: BM008646.D

(24) Indeno(1,2,3-cd)pyrene

25.765min (+0.021) 0.07ng/ul m

response 332

Ion	Exp%	Act%
276.00	100	100
138.00	23.90	0.00#
277.00	24.50	159.34#
0.00	0.00	0.00

25.7
 12127116

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
 Data File : BM008646.D
 Acq On : 24 Dec 2016 23:33
 Operator : UM/SJ
 Sample : H6069-06DL 2X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Quant Time: Dec 26 01:32:23 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 00:55:42 2016
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 DA7J2DL

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:28:03 PM

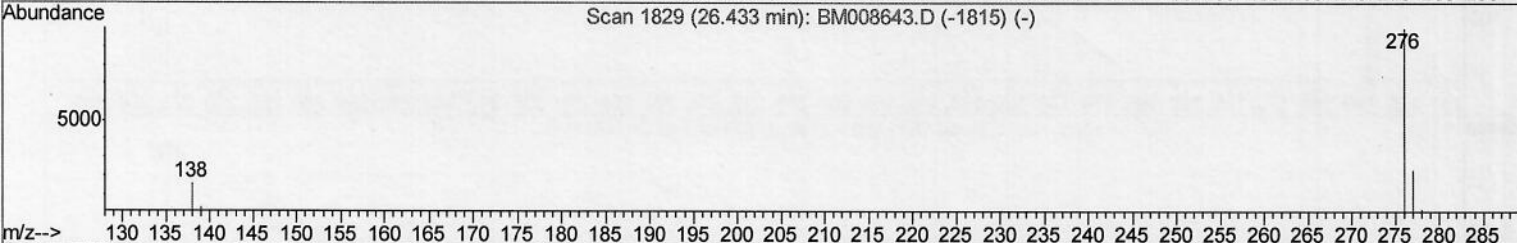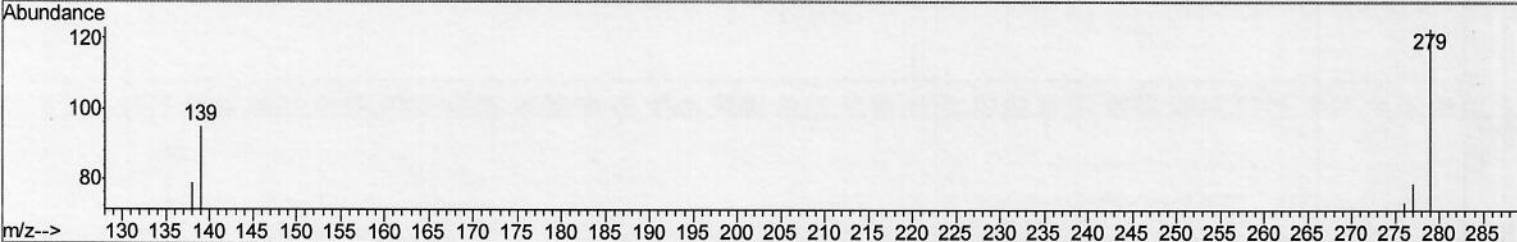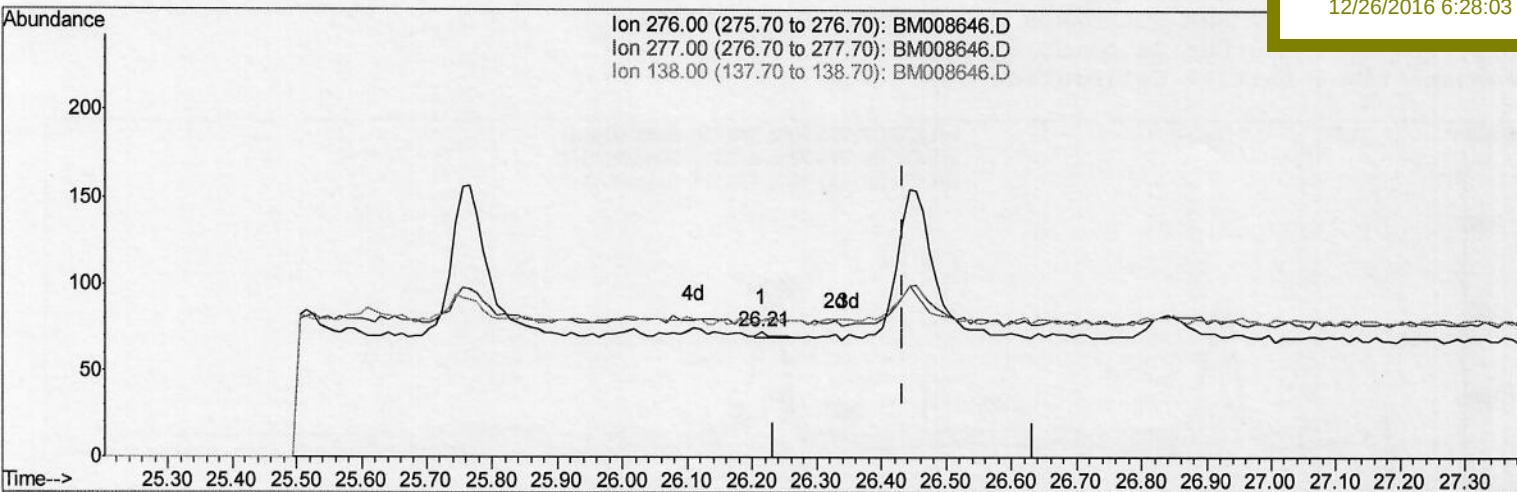

TIC: BM008646.D

(26) Benzo(g,h,i)perylene
 26.214min (-0.219) 0.00ng/ul
 response 5

Ion	Exp%	Act%
276.00	100	100
277.00	27.30	108.22#
138.00	25.60	108.22#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
 Data File : BM008646.D
 Acq On : 24 Dec 2016 23:33
 Operator : UM/SJ
 Sample : H6069-06DL 2X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA7J2DL

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:28:03 PM

Quant Time: Dec 26 01:32:23 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 00:55:42 2016
 Response via : Initial Calibration

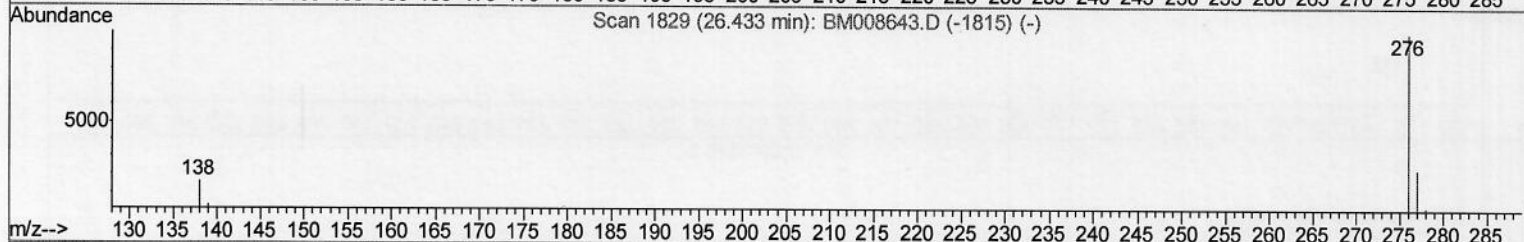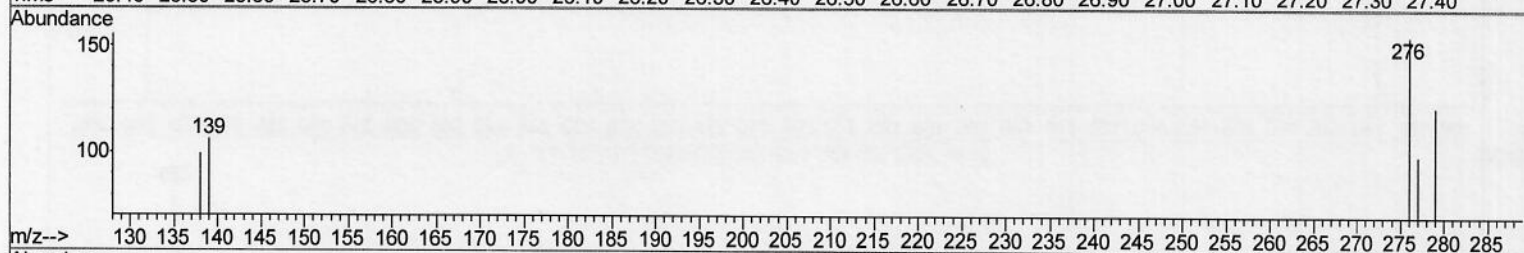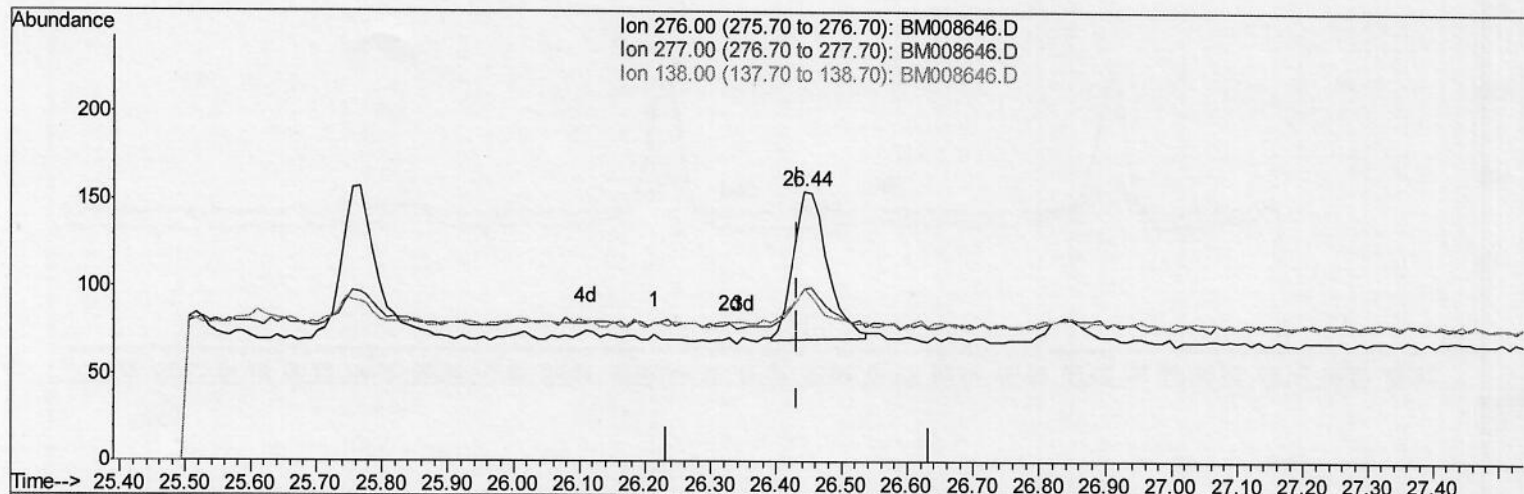

TIC: BM008646.D

(26) Benzo(g,h,i)perylene

26.443min (+0.011) 0.07ng/ul m

response 310

Ion	Exp%	Act%
276.00	100	100
277.00	27.30	63.87#
138.00	25.60	63.87#
0.00	0.00	0.00

7 9.5
 12/27/16

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
 Data File : BM008646.D
 Acq On : 24 Dec 2016 23:33
 Operator : UM/SJ
 Sample : H6069-06DL 2X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA7J2DL

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:28:03 PM

Quant Time: Dec 26 01:34:19 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 00:55:42 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	443	0.40	ng/ul	-0.08
2) Naphthalene-d8	10.43	136	1425	0.40	ng/ul	-0.05
6) Acenaphthene-d10	14.28	164	906	0.40	ng/ul	-0.03
10) Phenanthrene-d10	17.04	188	1869m	0.40	ng/ul	-0.03
16) Chrysene-d12	21.26	240	1620	0.40	ng/ul	0.00
20) Perylene-d12	23.49	264	1165m	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.04	152	515	0.24	ng/ul	-0.04
14) Fluoranthene-d10	19.08	212	1435m	0.28	ng/ul	-0.01

Target Compounds

						Qvalue
3) Naphthalene	10.46	128	539	0.13	ng/ul#	66
5) 2-Methylnaphthalene	12.11	142	548	0.20	ng/ul	99
12) Phenanthrene	17.07	178	1264m	0.22	ng/ul	
15) Fluoranthene	19.12	202	1152	0.16	ng/ul	88
17) Pyrene	19.47	202	1210	0.19	ng/ul#	78
18) Benzo(a)anthracene	21.25	228	526	0.10	ng/ul#	62
19) Chrysene	21.30	228	602	0.10	ng/ul#	65
21) Benzo(b)fluoranthene	22.82	252	781m	0.17	ng/ul	
22) Benzo(k)fluoranthene	22.86	252	317m	0.07	ng/ul	
23) Benzo(a)pyrene	23.38	252	397m	0.09	ng/ul	
24) Indeno(1,2,3-cd)pyrene	25.77	276	332m	0.07	ng/ul	
26) Benzo(g,h,i)perylene	26.44	276	310m	0.07	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122416\
 Data File : BM008646.D
 Acq On : 24 Dec 2016 23:33
 Operator : UM/SJ
 Sample : H6069-06DL 2X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DA7J2DL

Manual Integrations
 APPROVED

sohil
 12/26/2016 6:28:03 PM

Quant Time: Dec 26 01:34:19 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM121916.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 26 00:55:42 2016
 Response via : Initial Calibration

