

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122515\
 Data File : BM003791.D
 Acq On : 24 Dec 2015 23:01
 Operator : UM/SJ
 Sample : G4939-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 L-2-5(0-2)

Quant Time: Dec 25 01:04:29 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM120915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 09 18:52:47 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	51034	20.00	ng	-0.04
21) Naphthalene-d8	10.47	136	204335	20.00	ng	-0.05
38) Acenaphthene-d10	14.33	164	101893	20.00	ng	-0.04
63) Phenanthrene-d10	17.08	188	191590	20.00	ng	-0.04
75) Chrysene-d12	21.28	240	196020	20.00	ng	-0.04
86) Perylene-d12	23.52	264	208435	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.27	112	442528	154.17	ng	-0.03
7) Phenol-d6	6.86	99	569001	142.75	ng	-0.03
23) Nitrobenzene-d5	8.84	82	342365	103.89	ng	-0.04
41) 2,4,6-Tribromophenol	15.83	330	118441	116.39	ng	-0.04
44) 2-Fluorobiphenyl	12.95	172	670314	89.63	ng	-0.04
78) Terphenyl-d14	19.72	244	543201	65.35	ng	-0.04
Target Compounds						
49) Dimethylphthalate	13.79	163	93280	11.11	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122515\
Data File : BM003791.D
Acq On : 24 Dec 2015 23:01
Operator : UM/SJ
Sample : G4939-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
L-2-5(0-2)

Quant Time: Dec 25 01:04:29 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 18:52:47 2015
Response via : Initial Calibration

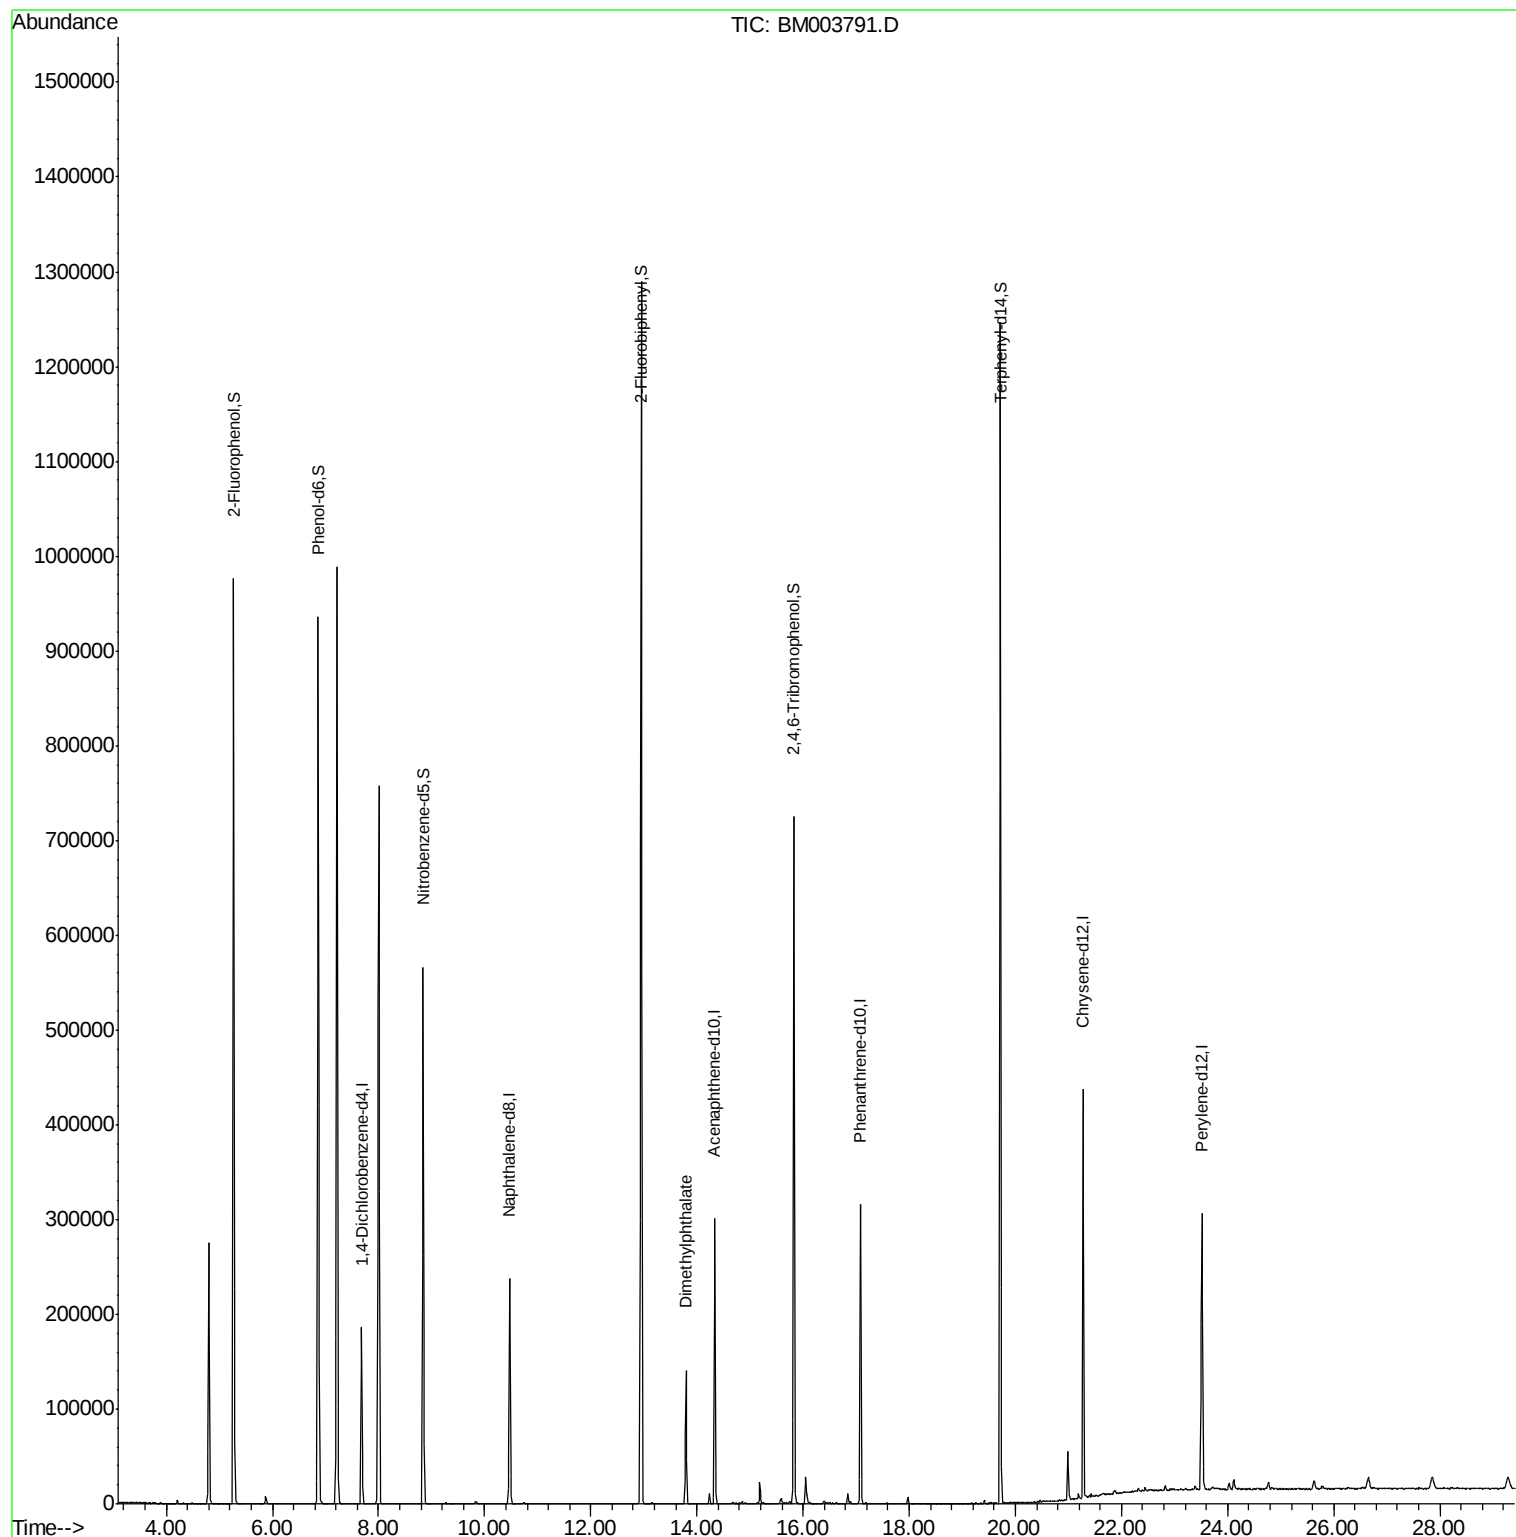

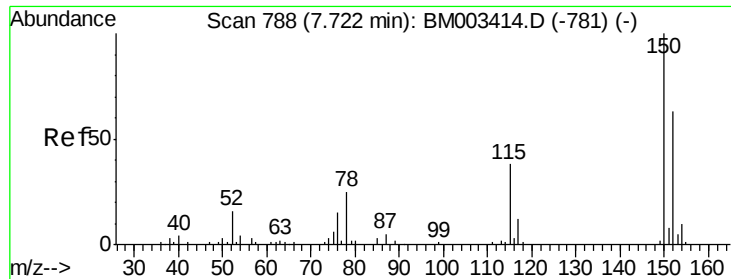


#1



1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.68 min Scan# 781
Delta R.T. -0.04 min
Lab File: BM003791.D
Acq: 24 Dec 2015 23:01

Instrument :
BNA_M
ClientSampleId :
L-2-5(0-2)

Tgt Ion:152 Resp: 51034
Ion Ratio Lower Upper
152 100
150 155.7 119.5 179.3
115 60.3 43.0 64.4

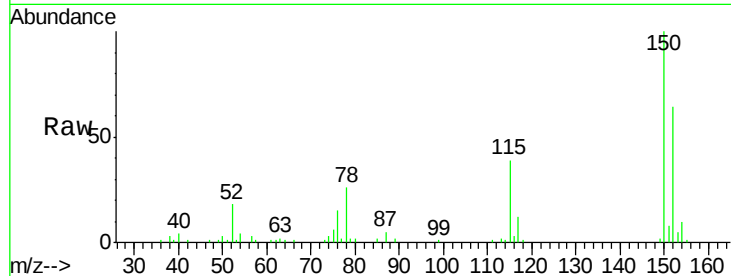


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

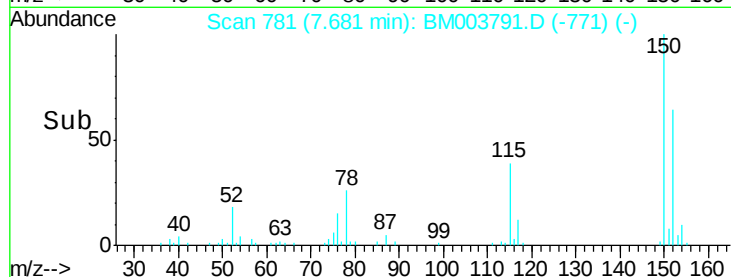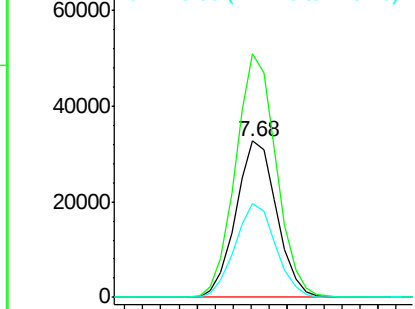



#5


2-Fluorophenol
Concen: 154.17 ng
RT: 5.27 min Scan# 371
Delta R.T. -0.03 min
Lab File: BM003791.D
Acq: 24 Dec 2015 23:01

Tgt Ion:112 Resp: 442528
Ion Ratio Lower Upper
112 100
64 52.7 38.6 57.8
63 27.4 19.3 28.9

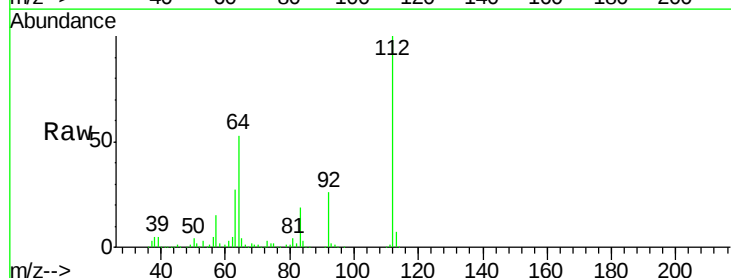

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

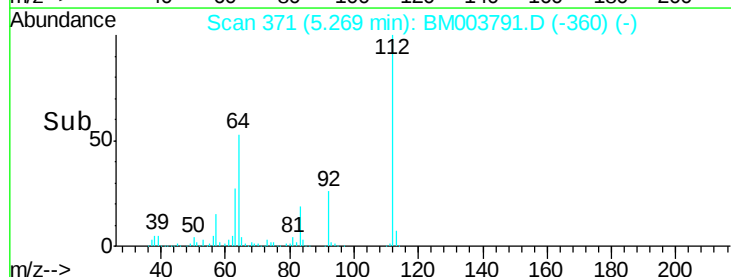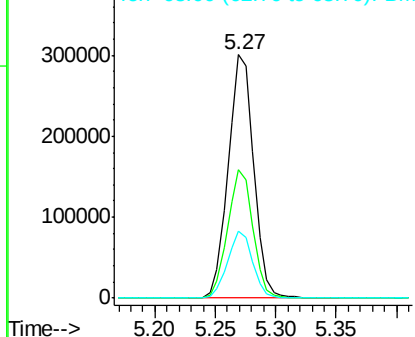

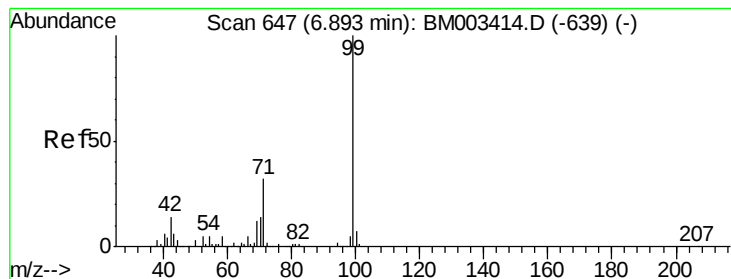

#7

Phenol-d6

Concen: 142.75 ng

RT: 6.86 min Scan# 642

Delta R.T. -0.03 min

Lab File: BM003791.D

Acq: 24 Dec 2015 23:01

Instrument :

BNA_M

ClientSampleId :

L-2-5(0-2)


Tgt Ion: 99 Resp: 569001

Ion Ratio Lower Upper

99 100

42 14.1 11.0 16.4

71 33.3 23.4 35.2



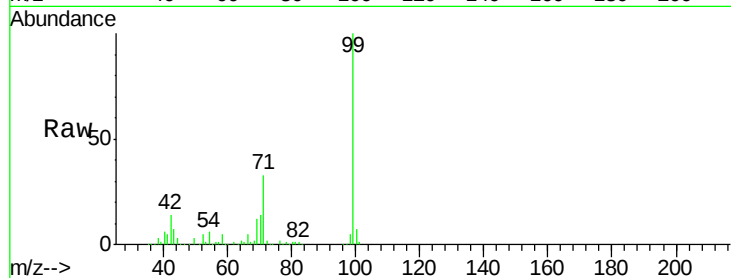


Abundance Ion 99.00 (98.70 to 99.70): BM003414.D (-639) (-)

Ion 42.00 (41.70 to 42.70): BM003414.D (-639) (-)

Ion 71.00 (70.70 to 71.70): BM003414.D (-639) (-)

6.86

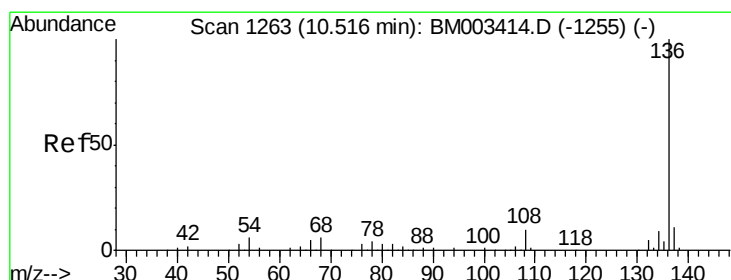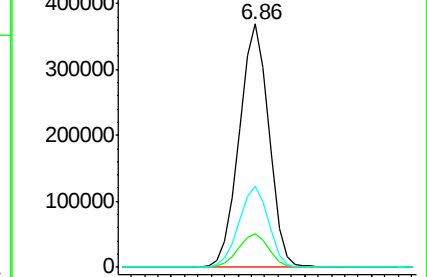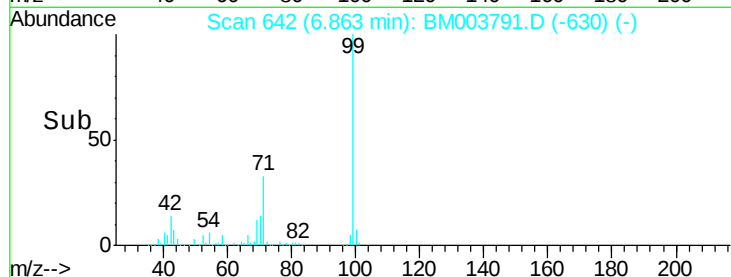

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.47 min Scan# 1255

Delta R.T. -0.05 min

Lab File: BM003791.D

Acq: 24 Dec 2015 23:01

Tgt Ion: 136 Resp: 204335


Ion Ratio Lower Upper

136 100

137 11.0 8.7 13.1

54 6.5 4.6 6.8

68 5.9 3.7 5.5#

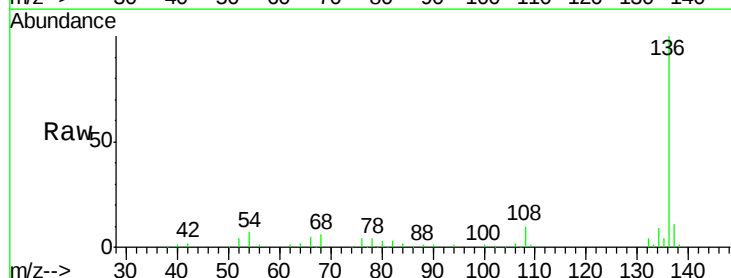



Abundance Ion 136.00 (135.70 to 136.70): BM003414.D (-1255) (-)


Ion 137.00 (136.70 to 137.70): BM003414.D (-1255) (-)

Ion 54.00 (53.70 to 54.70): BM003414.D (-1255) (-)

Ion 68.00 (67.70 to 68.70): BM003414.D (-1255) (-)

10.47

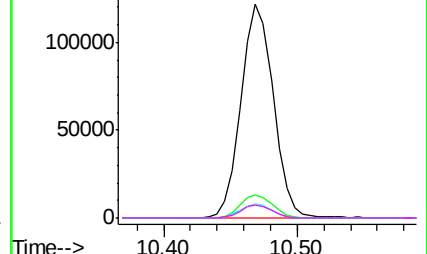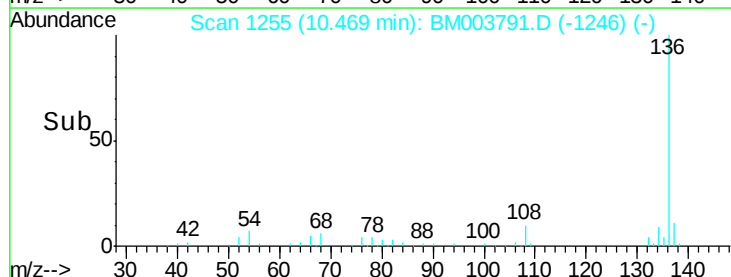


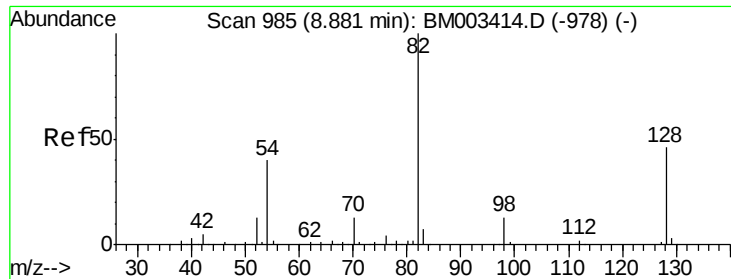

#23
 Nitrobenzene-d5
 Concen: 103.89 ng
 RT: 8.84 min Scan# 978
 Delta R.T. -0.04 min
 Lab File: BM003791.D
 Acq: 24 Dec 2015 23:01

Instrument :
 BNA_M
 ClientSampled :
 L-2-5(0-2)




Tgt Ion	Ratio	Lower	Upper
82	100		
128	45.1	32.8	49.2
54	41.8	40.6	60.8

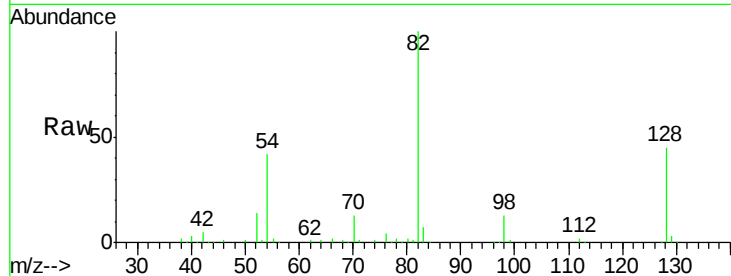

Abundance Ion 82.00 (81.70 to 82.70): BM003791.D (-978) (-)


Ion 128.00 (127.70 to 128.70): BM003791.D (-978) (-)

Ion 54.00 (53.70 to 54.70): BM003791.D (-978) (-)

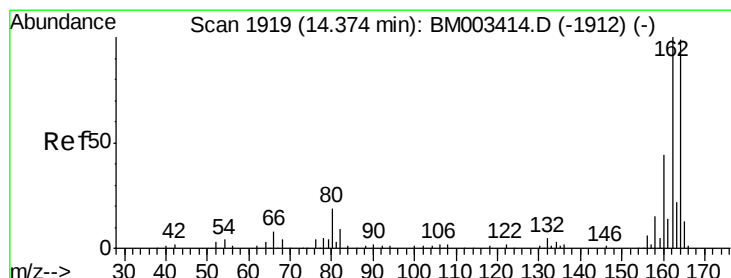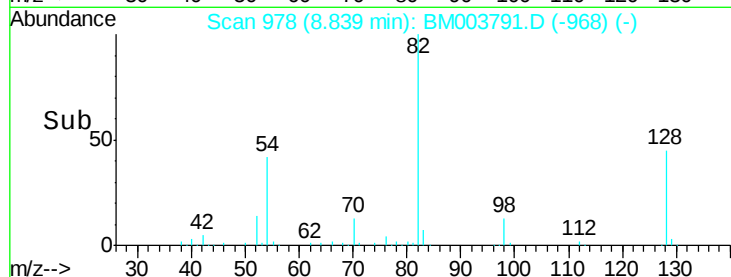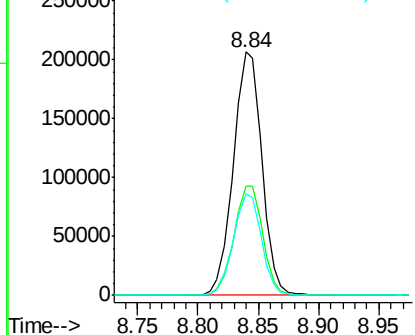

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.33 min Scan# 1912
 Delta R.T. -0.04 min
 Lab File: BM003791.D
 Acq: 24 Dec 2015 23:01



Tgt Ion	Ratio	Lower	Upper
164	100		
162	101.6	82.4	123.6
160	46.0	35.8	53.6

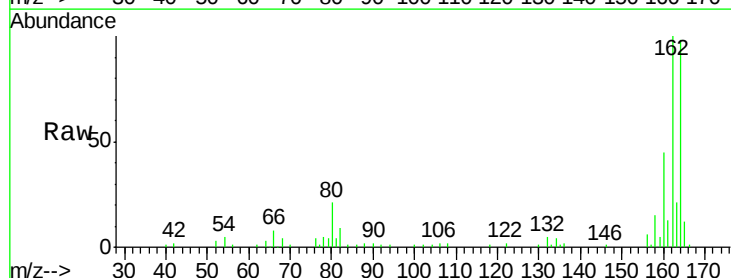

Abundance Ion 164.00 (163.70 to 164.70): BM003791.D (-1912) (-)

Ion 162.00 (161.70 to 162.70): BM003791.D (-1912) (-)

Ion 160.00 (159.70 to 160.70): BM003791.D (-1912) (-)

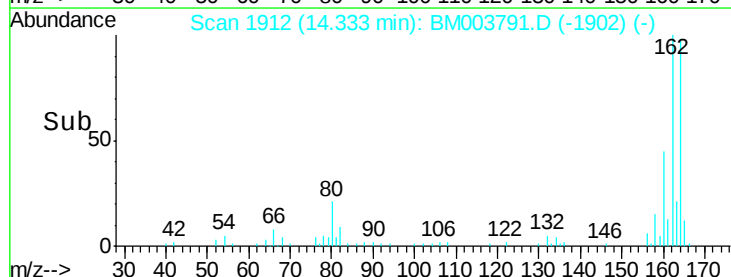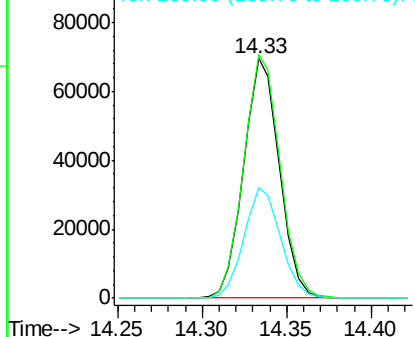



#41

2,4,6-Tribromophenol

Concen: 116.39 ng

RT: 15.83 min Scan# 2166

Delta R.T. -0.04 min

Lab File: BM003791.D

Acq: 24 Dec 2015 23:01

Instrument :

BNA_M

ClientSampleId :

L-2-5(0-2)


Tgt Ion:330 Resp: 118441

Ion Ratio Lower Upper

330 100

332 96.1 0.0 0.0#




141 43.8 0.0 0.0#

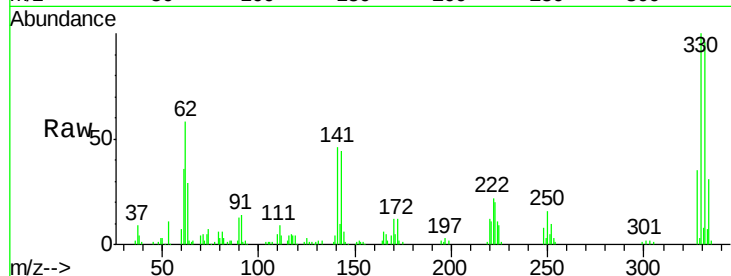

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

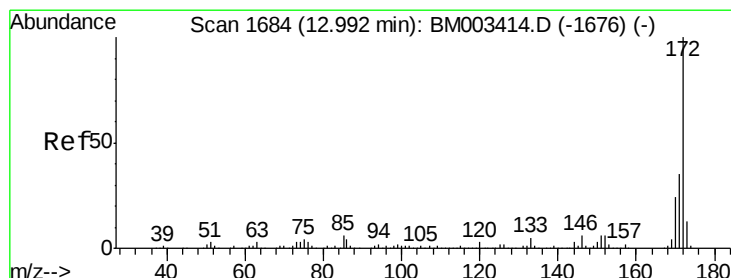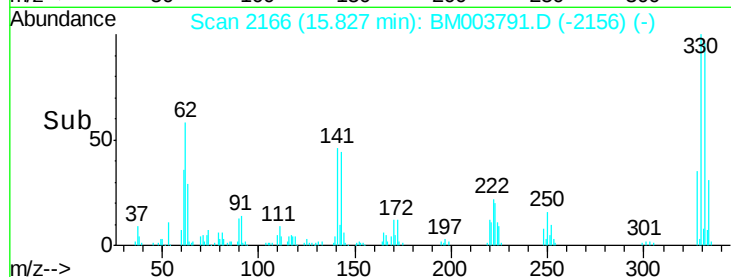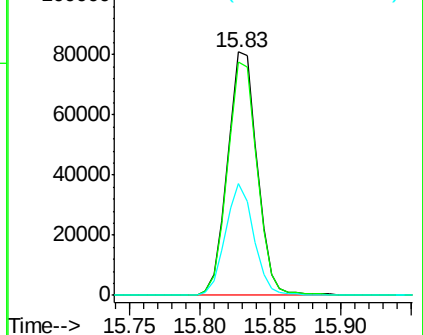

#44

2-Fluorobiphenyl

Concen: 89.63 ng

RT: 12.95 min Scan# 1677

Delta R.T. -0.04 min

Lab File: BM003791.D

Acq: 24 Dec 2015 23:01


Tgt Ion:172 Resp: 670314

Ion Ratio Lower Upper

172 100

171 35.1 28.5 42.7



170 23.1 18.8 28.2

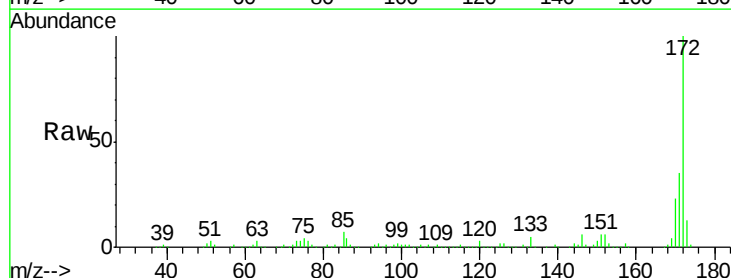


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

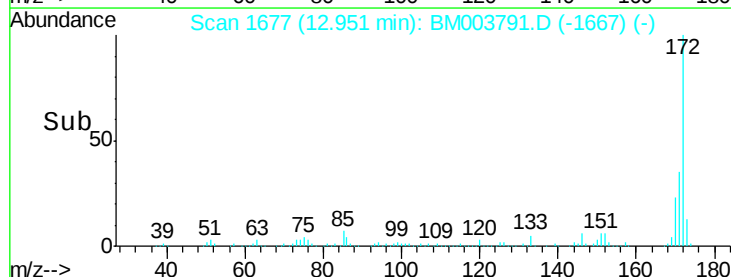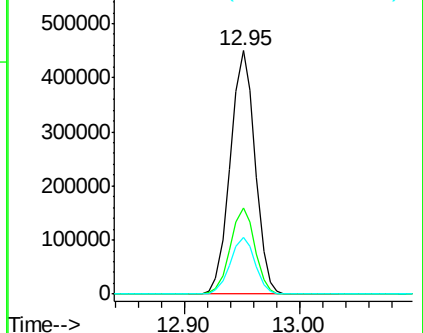

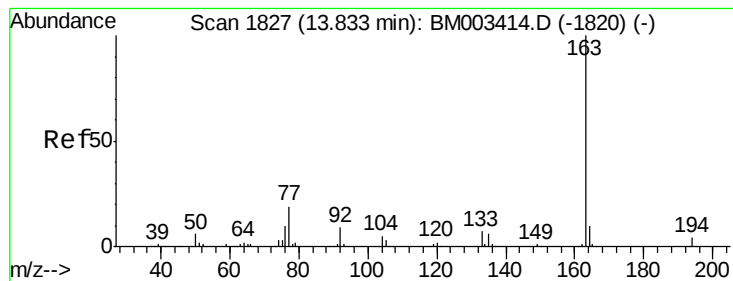

#49

Dimethylphthalate

Concen: 11.11 ng

RT: 13.79 min Scan# 1820

Delta R.T. -0.04 min

Lab File: BM003791.D

Acq: 24 Dec 2015 23:01

Instrument :

BNA_M

ClientSampleId :

L-2-5(0-2)


Tgt Ion:163 Resp: 93280

Ion Ratio Lower Upper

163 100

194 4.0 2.7 4.1




164 9.7 8.2 12.2

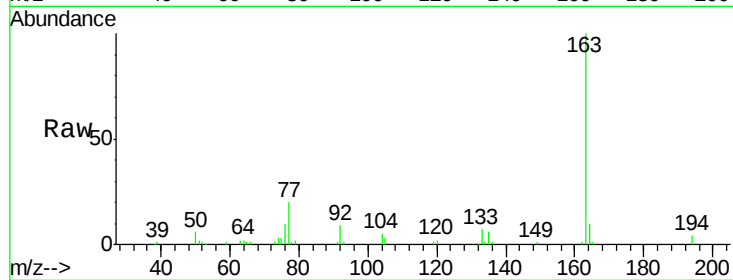

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

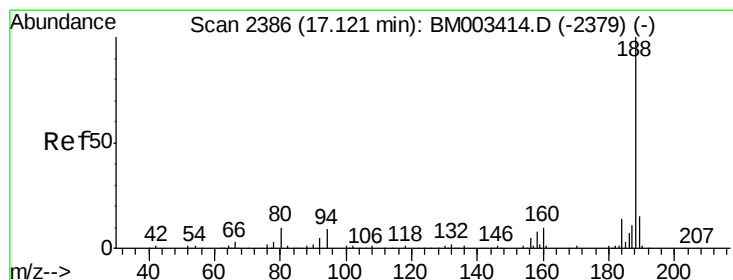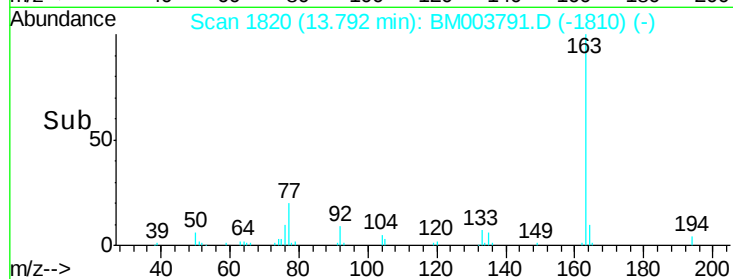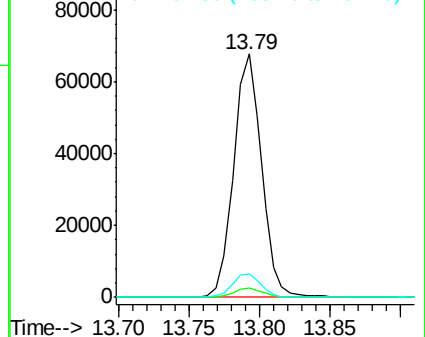

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.08 min Scan# 2379

Delta R.T. -0.04 min

Lab File: BM003791.D

Acq: 24 Dec 2015 23:01


Tgt Ion:188 Resp: 191590

Ion Ratio Lower Upper

188 100

94 9.8 8.7 13.1



80 11.0 9.3 13.9

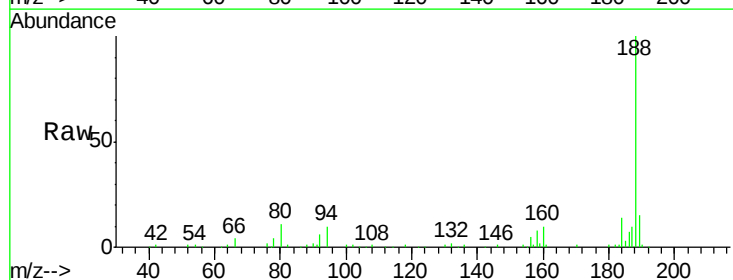


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM0

Ion 80.00 (79.70 to 80.70): BM0

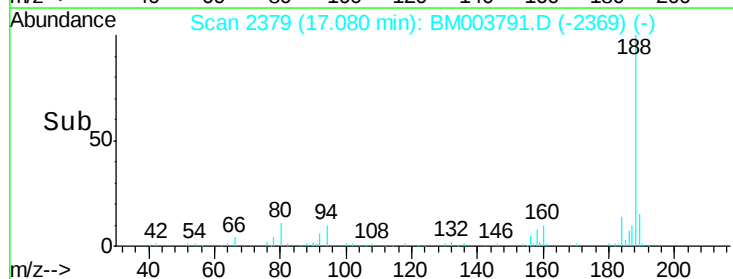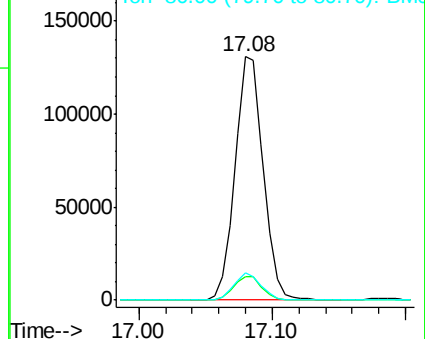

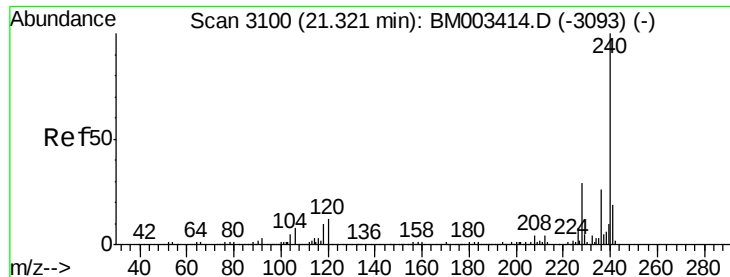

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.28 min Scan# 3093

Delta R.T. -0.04 min

Lab File: BM003791.D

Acq: 24 Dec 2015 23:01

Instrument :

BNA_M

ClientSampleId :

L-2-5(0-2)


Tgt Ion:240 Resp: 196020

Ion Ratio Lower Upper

240 100

120 11.4 8.2 12.2




236 25.5 20.0 30.0

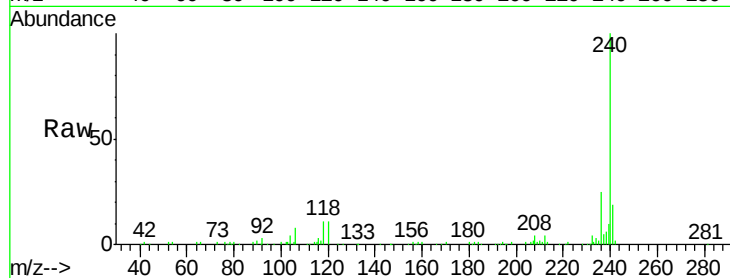

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

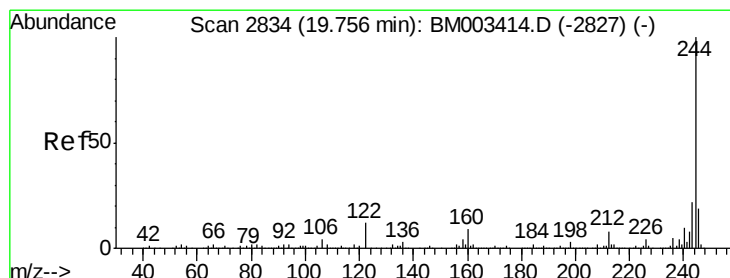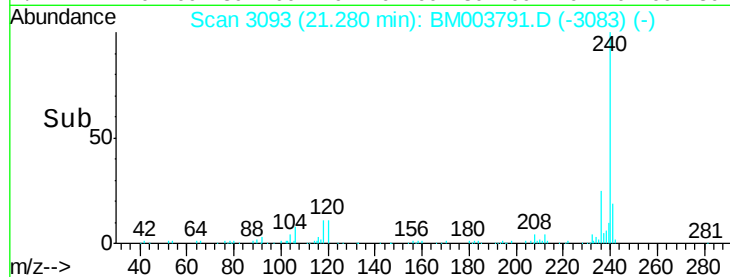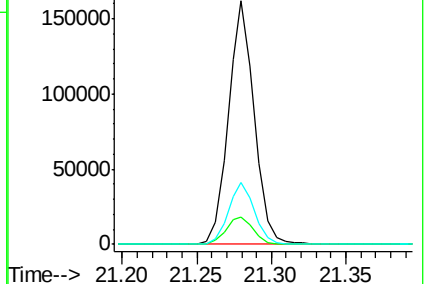

#78

Terphenyl-d14

Concen: 65.35 ng

RT: 19.72 min Scan# 2828

Delta R.T. -0.04 min

Lab File: BM003791.D

Acq: 24 Dec 2015 23:01


Tgt Ion:244 Resp: 543201

Ion Ratio Lower Upper

244 100

212 7.6 4.9 7.3#



122 11.5 6.2 9.4#

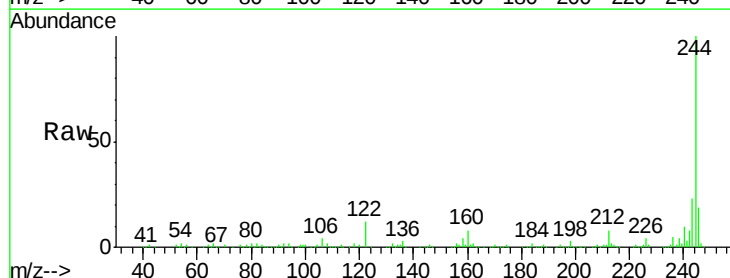


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

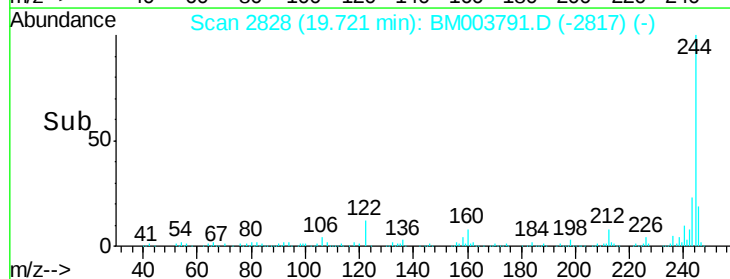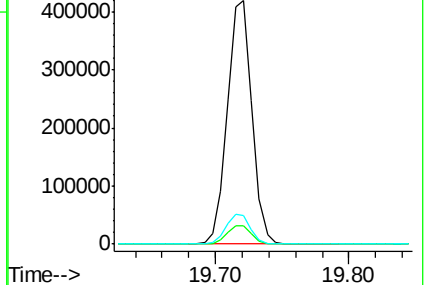

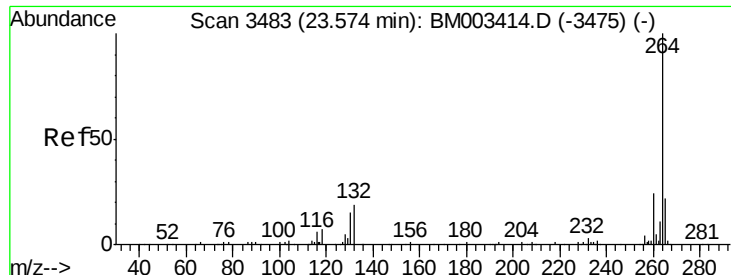

#86
Perylene-d12
Concen: 20.00 ng
RT: 23.52 min Scan# 3473
Delta R.T. -0.06 min
Lab File: BM003791.D
Acq: 24 Dec 2015 23:01

Instrument :
BNA_M
ClientSampleId :
L-2-5(0-2)

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.9	18.6	27.8
265	21.2	17.3	25.9

