
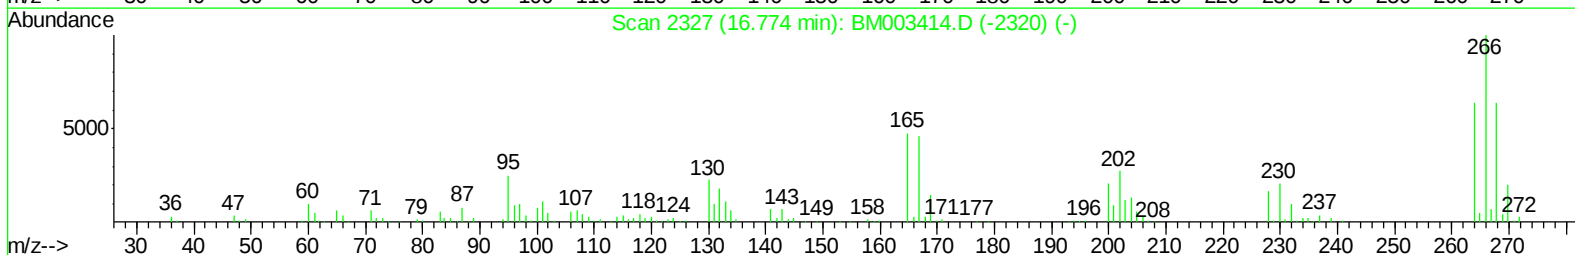
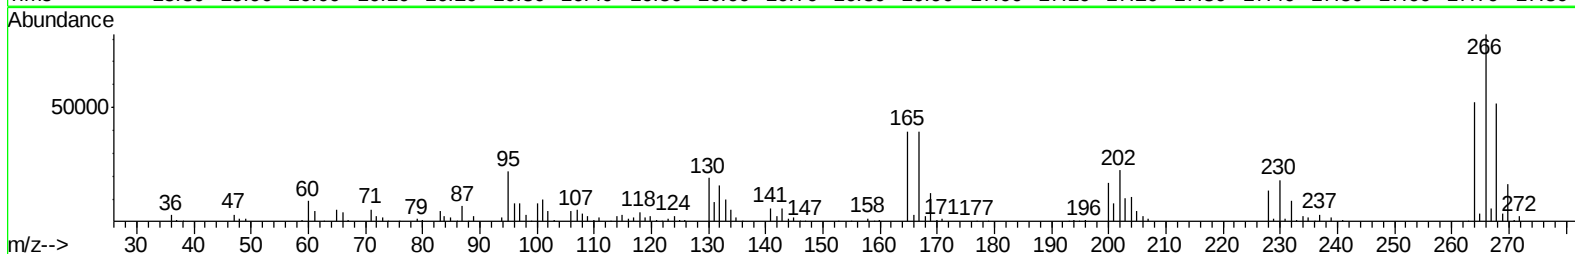


Data Path : Z:\HPCHEM1\BNA M\Data\BM122515\
Data File : BM003779.D
Acq On : 24 Dec 2015 15:42
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 24 16:16:54 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 09 18:52:47 2015
Response via : Initial Calibration

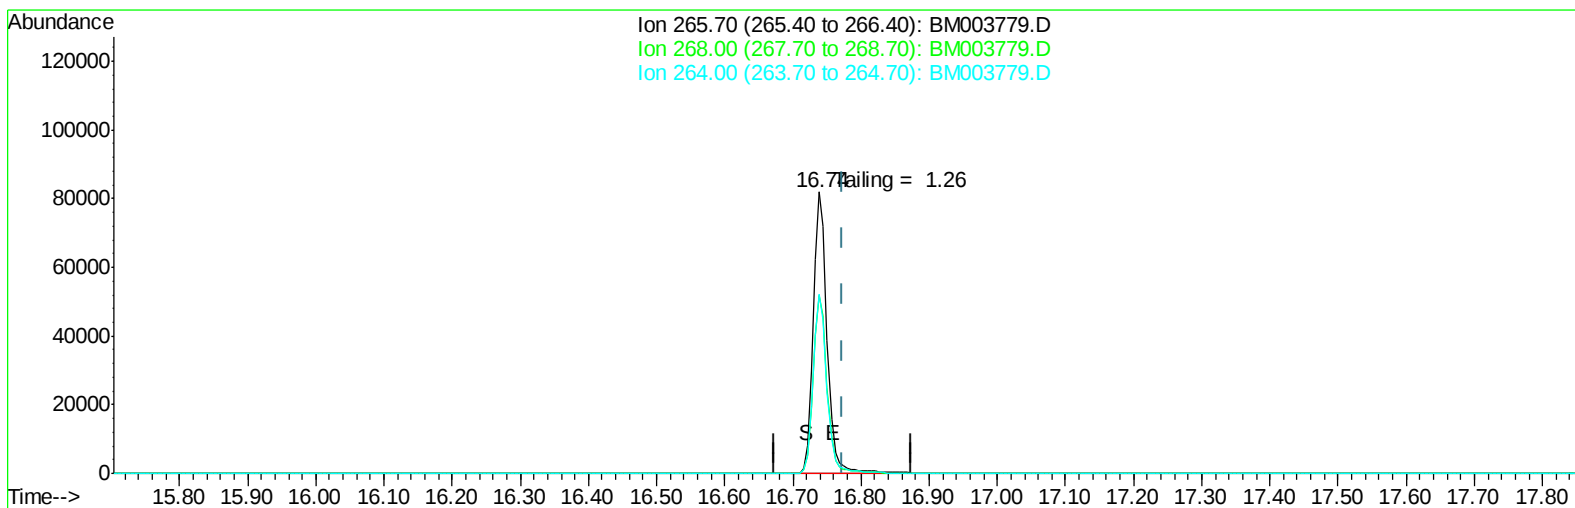

TIC: BM003779.D

(69) Pentachlorophenol (C)

16.739min (-0.035) 0.00ng

response 116785

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	63.06
264.00	61.20	63.85
0.00	0.00	0.00

