
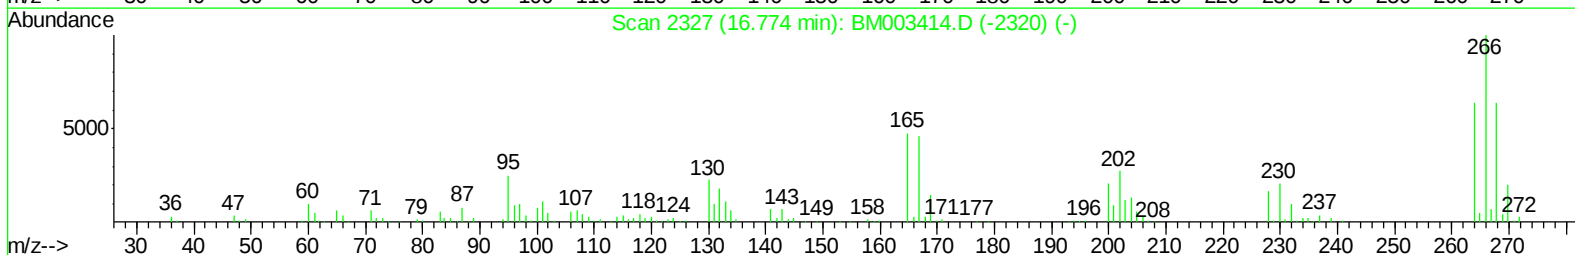
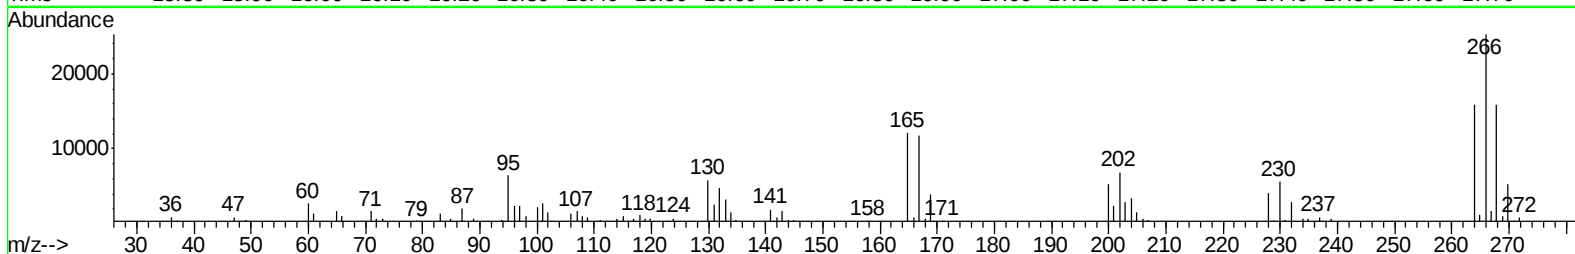


Data Path : Z:\HPCHEM1\BNA M\Data\BM122515\
 Data File : BM003797.D
 Acq On : 25 Dec 2015 02:39
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 03:21:52 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM120915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 09 18:52:47 2015
 Response via : Initial Calibration

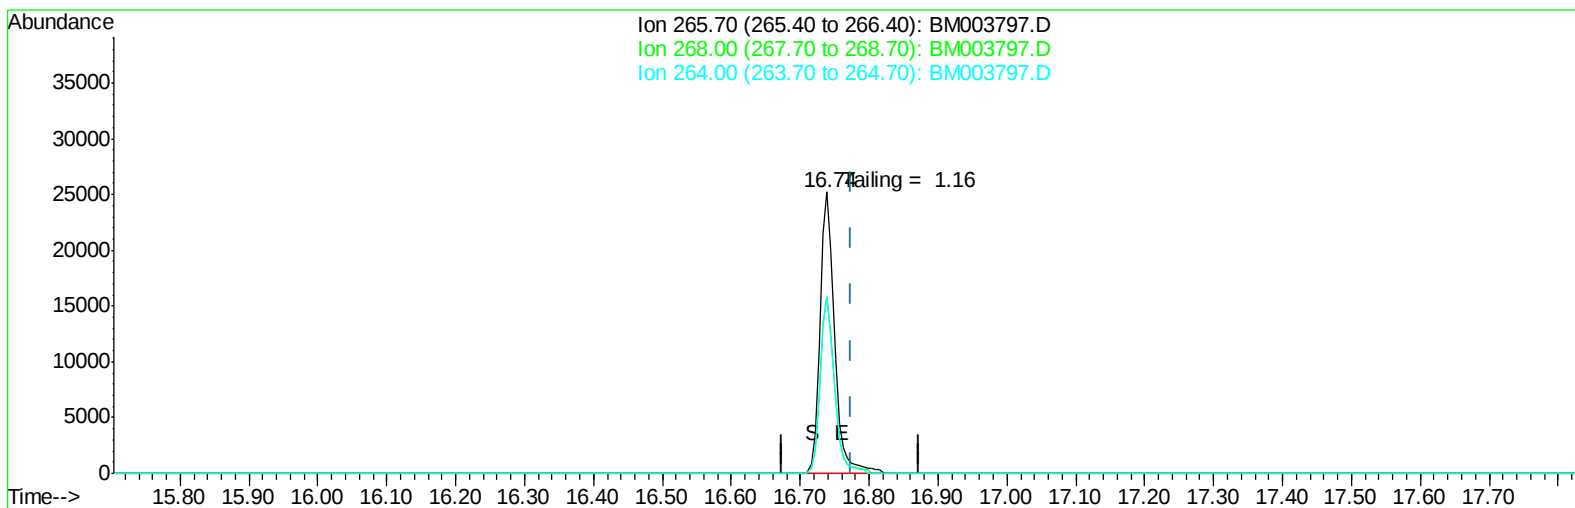

TIC: BM003797.D

(69) Pentachlorophenol (C)




16.739min (-0.035) 0.00ng

response 36974

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	62.96
264.00	61.20	62.65
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\Data\BM122515\
 Data File : BM003797.D
 Acq On : 25 Dec 2015 02:39
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 28 03:21:52 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM120915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 09 18:52:47 2015
 Response via : Initial Calibration

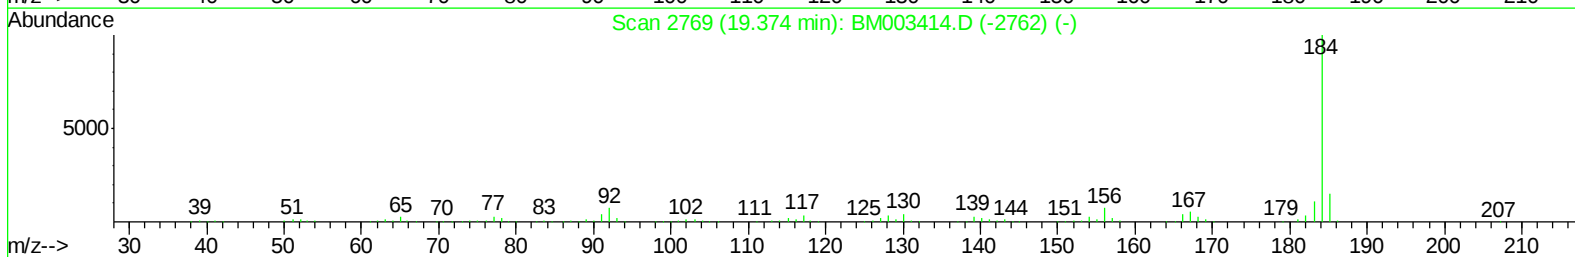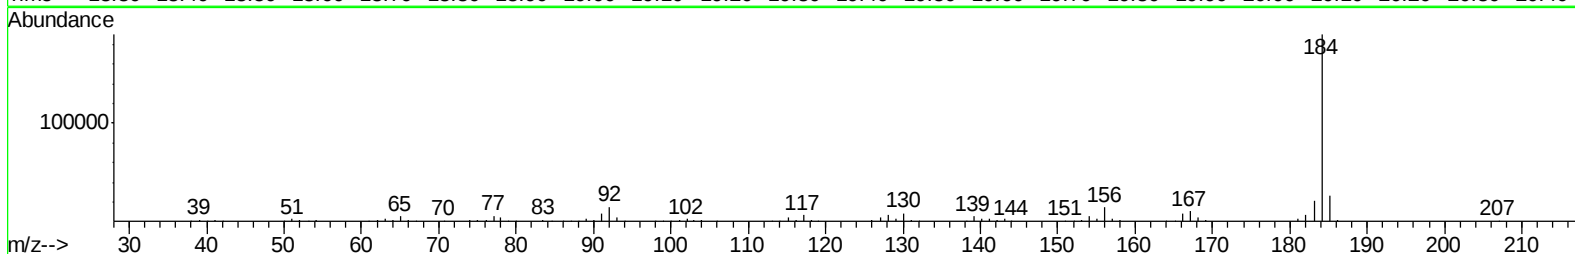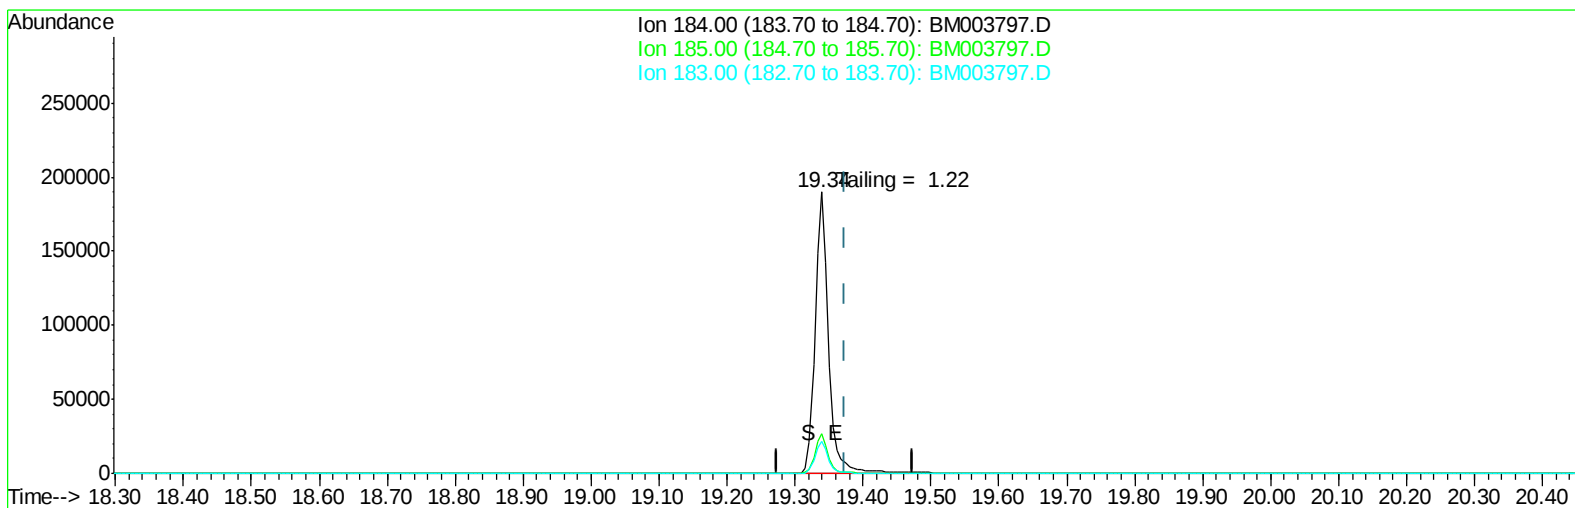

TIC: BM003797.D

(76) Benzidine

19.339min (-0.035) 0.00ng

response 261301

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	14.02
183.00	11.10	11.51
0.00	0.00	0.00