

Data Path : Z:\HPCHEM1\BNA M\DATA\BM122515\
 Data File : BM003785.D
 Acq On : 24 Dec 2015 19:22
 Operator : UM/SJ
 Sample : PB87538BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB87538BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM120915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.799	286	291	302	rBV	118505	167487	9.04%	1.401%
2	5.269	365	371	385	rBV	660461	944701	50.98%	7.901%
3	6.863	635	642	659	rBV	615263	964880	52.07%	8.070%
4	7.216	696	702	715	rBB	670141	1045105	56.40%	8.741%
5	7.681	775	781	789	rBB	192441	298263	16.10%	2.495%
6	8.004	829	836	845	rBB	521259	829166	44.75%	6.935%
7	8.839	971	978	995	rBB	368965	600532	32.41%	5.023%
8	10.469	1248	1255	1268	rBV	256582	433248	23.38%	3.624%
9	12.951	1670	1677	1689	rBV	1021804	1506375	81.30%	12.599%
10	14.333	1906	1912	1922	rBB2	364381	561388	30.30%	4.695%
11	15.827	2161	2166	2181	rBB	652633	906952	48.95%	7.586%
12	17.080	2373	2379	2393	rBV2	442792	649328	35.04%	5.431%
13	19.721	2822	2828	2836	rBV	1452253	1852928	100.00%	15.497%
14	21.280	3088	3093	3101	rBV	519056	647529	34.95%	5.416%
15	23.521	3466	3474	3484	rBV	295909	548499	29.60%	4.588%


Sum of corrected areas: 11956381

Data Path : Z:\HPCHEM1\BNA M\DATA\BM122515\
Data File : BM003785.D
Acq On : 24 Dec 2015 19:22
Operator : UM/SJ
Sample : PB87538BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB87538BL

Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

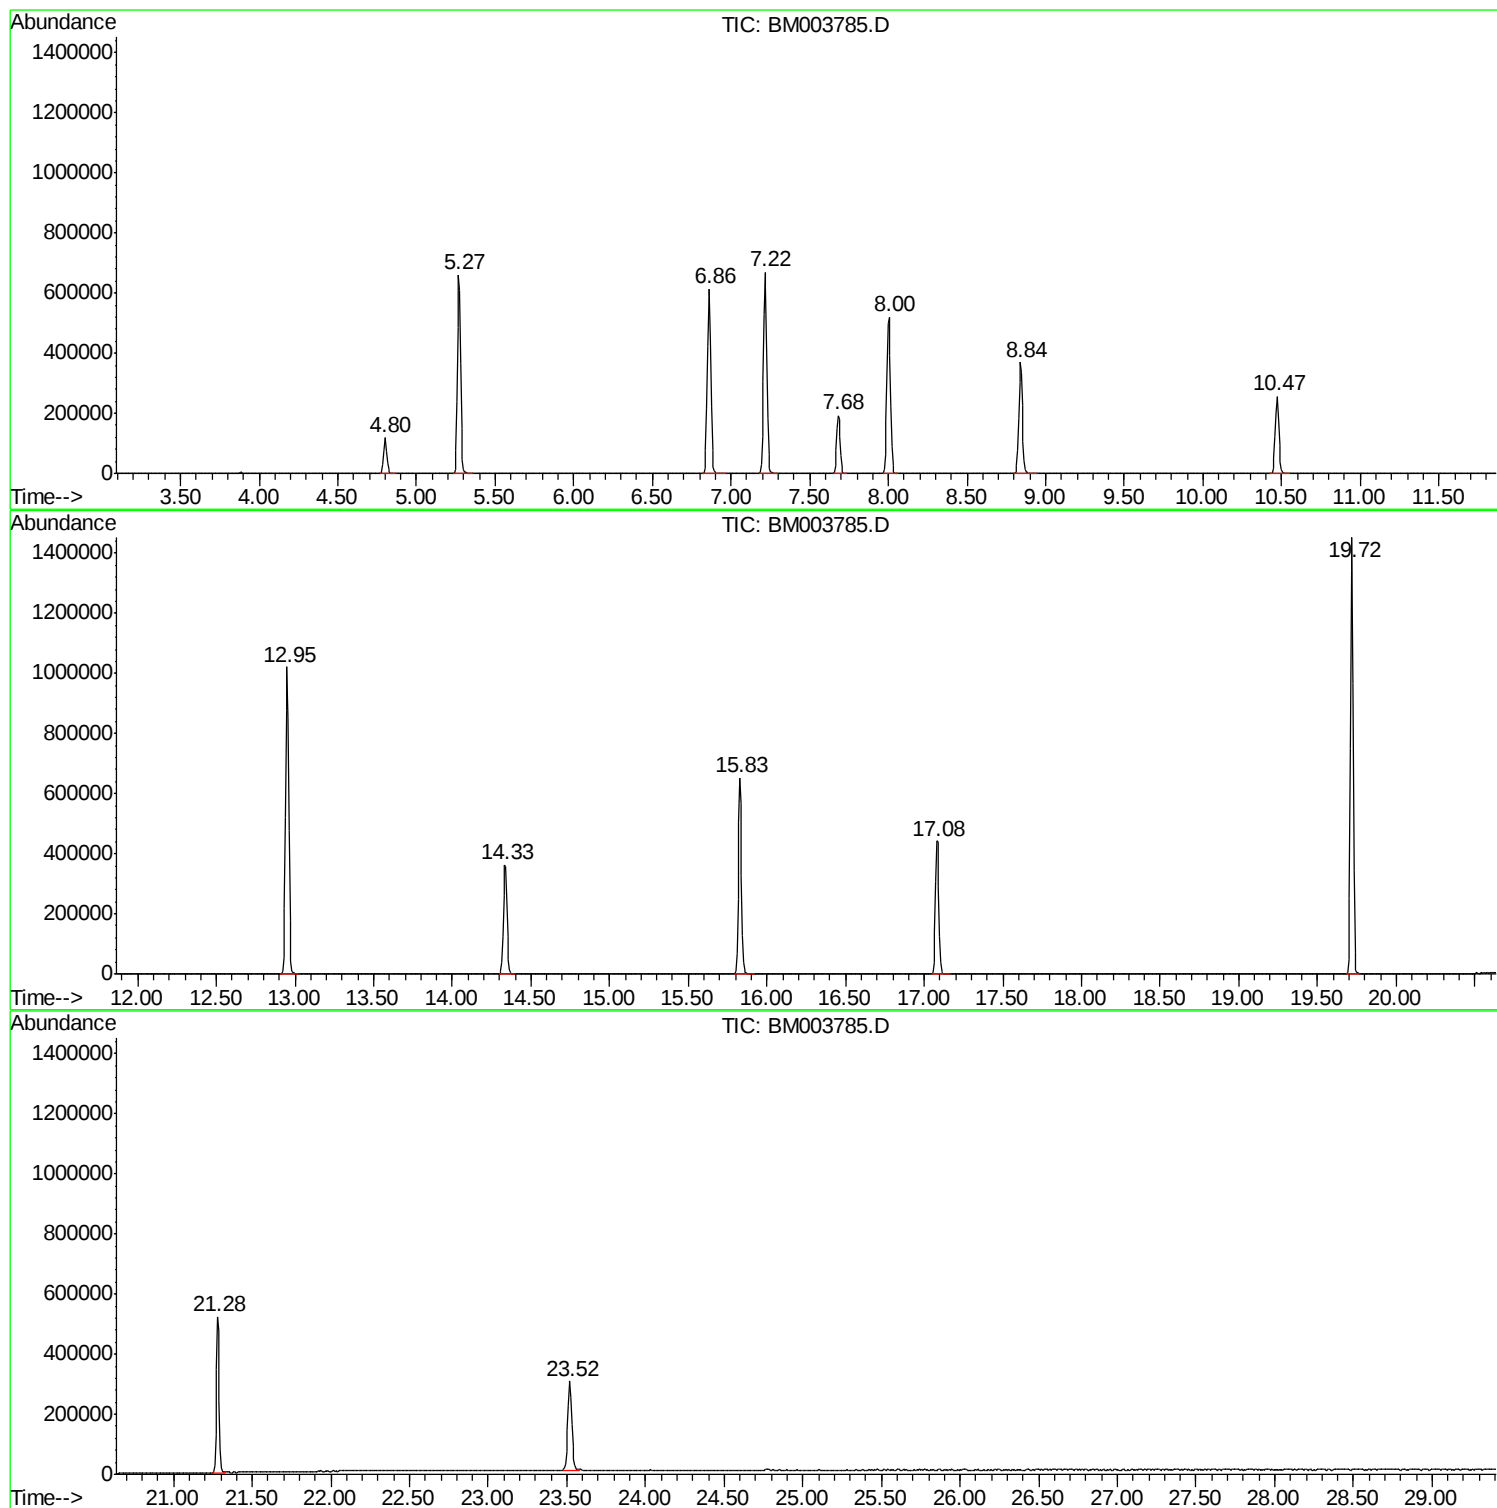

Data Path : Z:\HPCHEM1\BNA M\DATA\BM122515\
Data File : BM003785.D
Acq On : 24 Dec 2015 19:22
Operator : UM/SJ
Sample : PB87538BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB87538BL










Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.80	11.23 ng	167487	1,4-Dichlorobenzene-d4	7.68

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56	
2	Acetic acid, cyano-, 1,1-dimethyl...	141	C7H11NO2	001116-98-9	17	
3	Acetone	58	C3H6O	000067-64-1	9	
4	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9	
5	5-Hexen-2-one	98	C6H10O	000109-49-9	9	

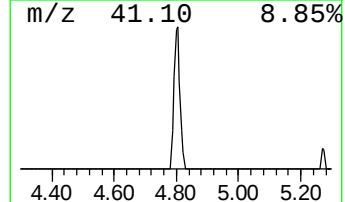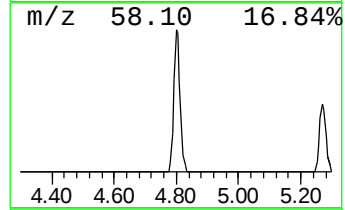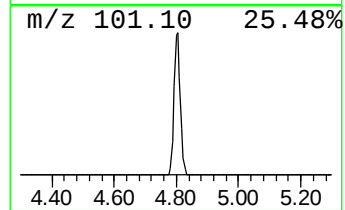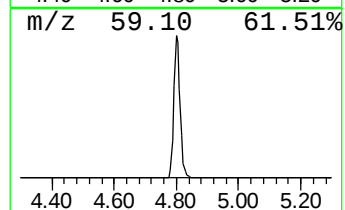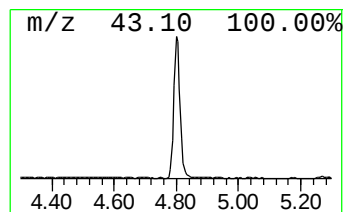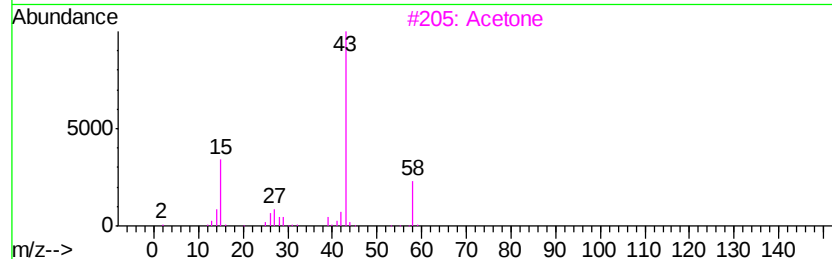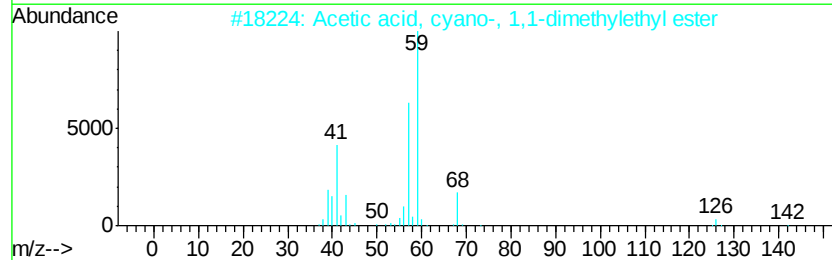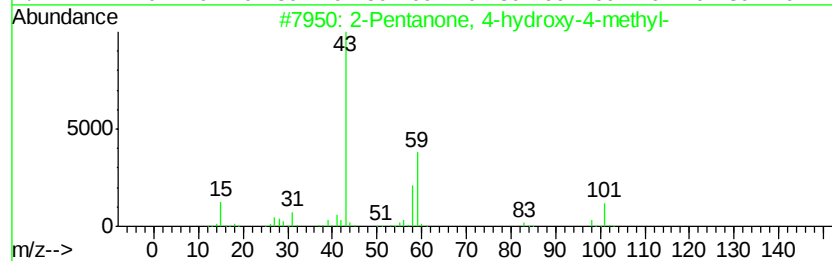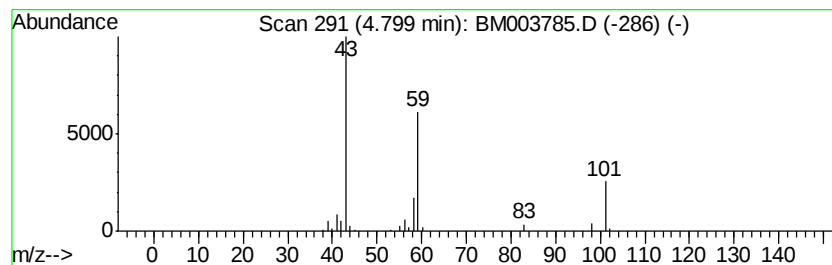

Data Path : Z:\HPCHEM1\BNA M\DATA\BM122515\
Data File : BM003785.D
Acq On : 24 Dec 2015 19:22
Operator : UM/SJ
Sample : PB87538BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB87538BL










Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown7.22 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.22	70.08 ng	1045110	1,4-Dichlorobenzene-d4	7.68

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2			5-Aminoindole	132	C8H8N2	005192-03-0	12
3			Tranvlcyproline-propionyl	189	C12H15NO	1000123-86-3	10
4			Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5			4-Chloro-6-fluoro-pyrimidine	132	C4H2ClFN2	051422-01-6	9

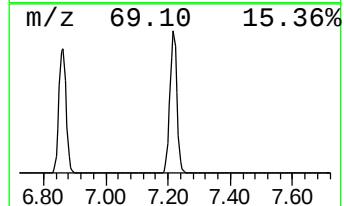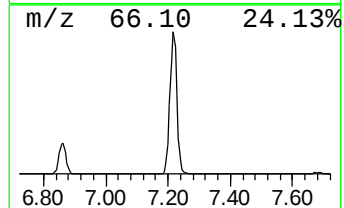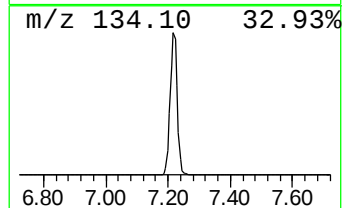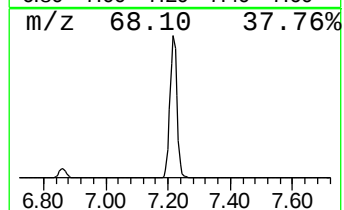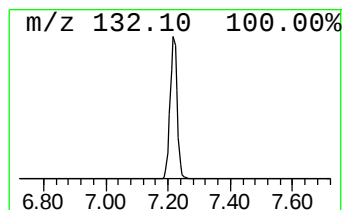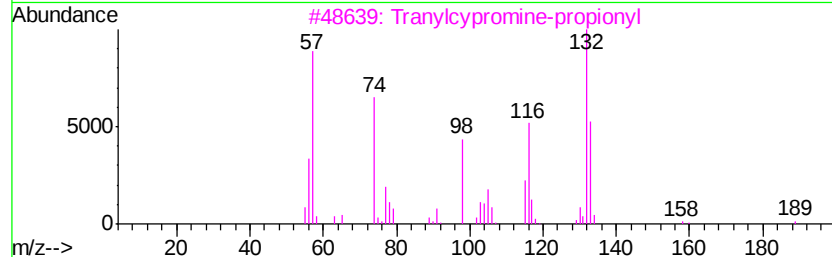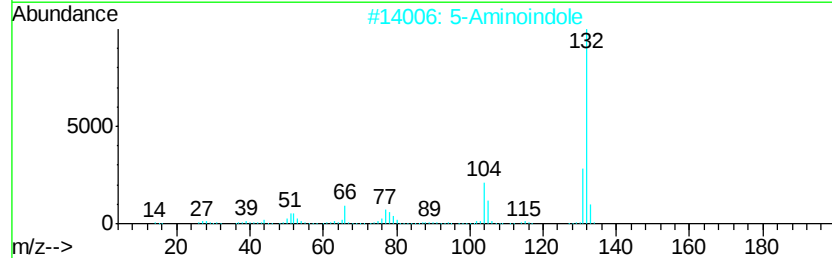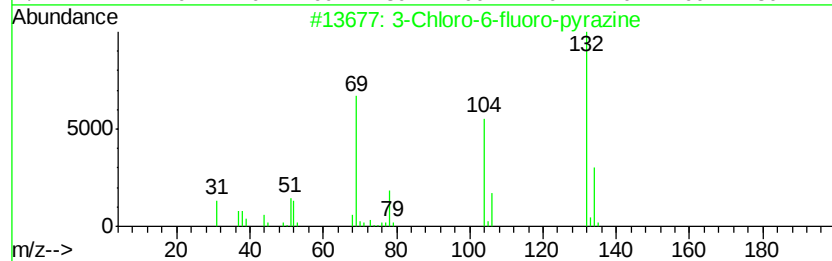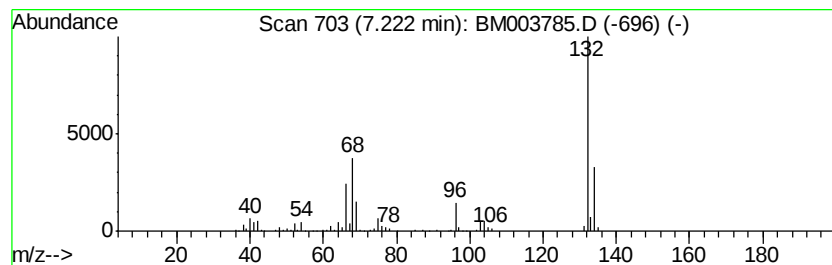

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122515\
Data File : BM003785.D
Acq On : 24 Dec 2015 19:22
Operator : UM/SJ
Sample : PB87538BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB87538BL

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM120915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.80	11.2	ng	167487	1	7.68	298263	20.0
unknown7.22	7.22	70.1	ng	1045110	1	7.68	298263	20.0