


Data Path : Z:\HPCHEM1\BNA M\DATA\BM122515\
 Data File : BM003797.D
 Acq On : 25 Dec 2015 02:39
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM120915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 09 18:52:47 2015

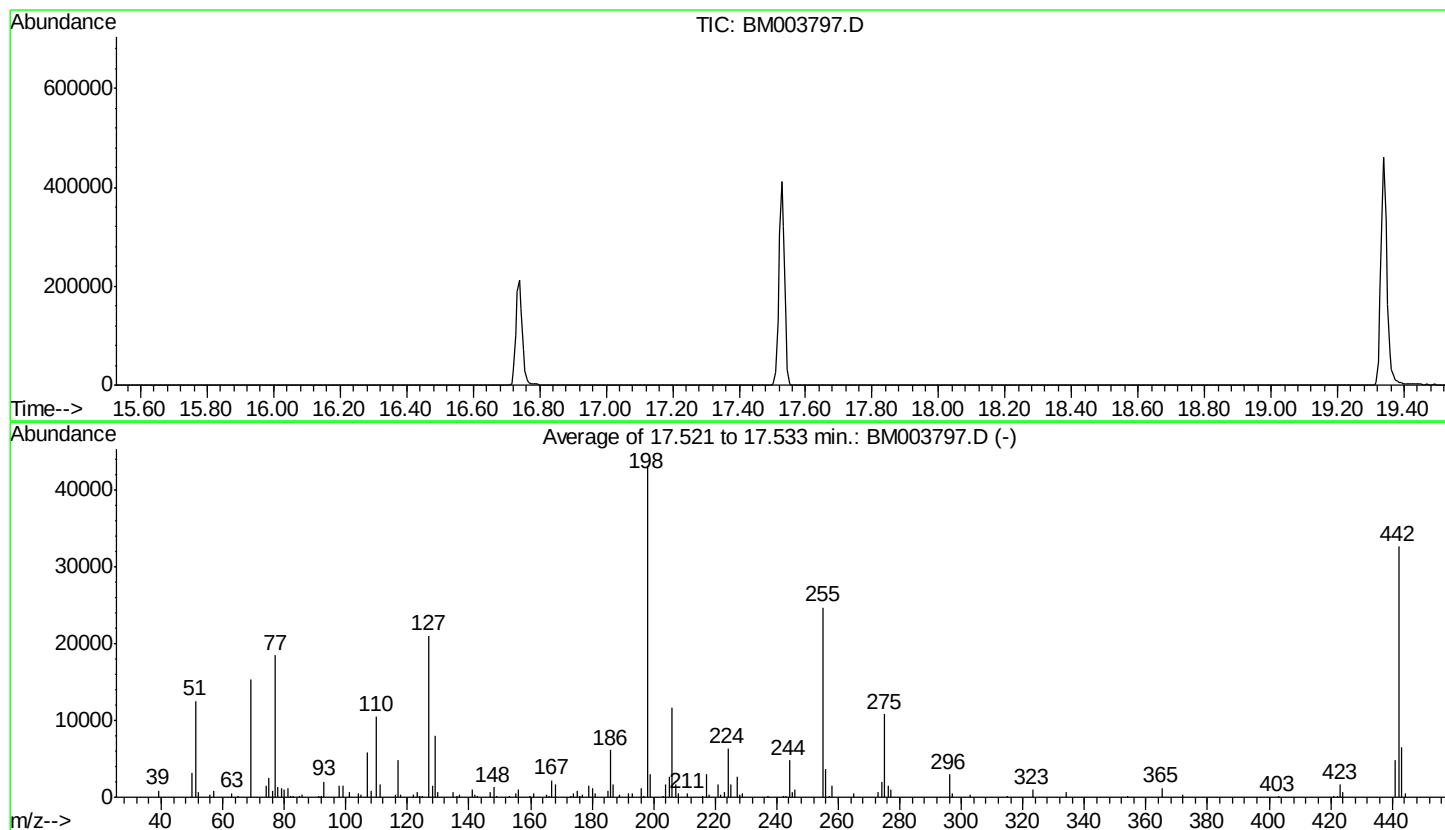

AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.1	12544	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.6	15361	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.7	20978	PASS
197	198	0.00	2	0.3	109	PASS
198	198	100	100	100.0	43090	PASS
199	198	5	9	6.8	2922	PASS
275	198	10	60	25.0	10770	PASS
365	198	1	100	2.9	1249	PASS
441	442	0.01	24	14.7	4788	PASS
442	198	50	100	75.6	32589	PASS
443	442	15	24	19.7	6423	PASS