


Data Path : Z:\HPCHEM1\BNA M\DATA\BM122515\
 Data File : BM003812.D
 Acq On : 25 Dec 2015 12:20
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM120915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 09 18:52:47 2015

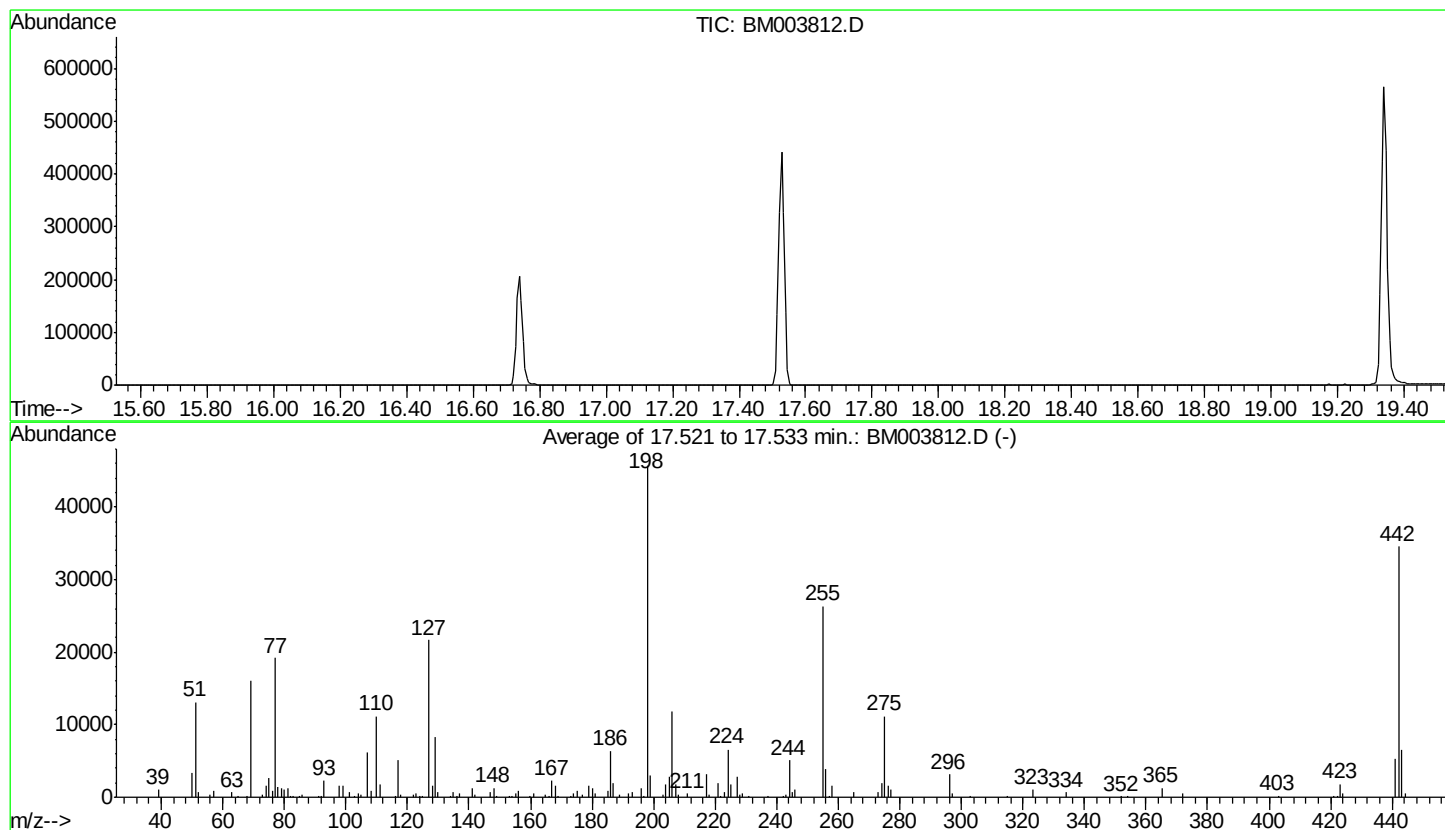

AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2448

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.7	13128	PASS
68	69	0.00	2	0.7	111	PASS
69	198	0.00	100	35.2	16076	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.4	21664	PASS
197	198	0.00	2	0.2	111	PASS
198	198	100	100	100.0	45728	PASS
199	198	5	9	6.7	3051	PASS
275	198	10	60	24.5	11205	PASS
365	198	1	100	2.8	1283	PASS
441	442	0.01	24	15.2	5246	PASS
442	198	50	100	75.5	34536	PASS
443	442	15	24	19.0	6578	PASS