

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122617\
 Data File : BM013541.D
 Acq On : 26 Dec 2017 19:02
 Operator : SJ/JU
 Sample : I7046-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COFMO

Quant Time: Dec 27 03:54:17 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 27 03:26:43 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	225444	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	1026155	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.31	164	602927	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	1224374	20.00	ng/ul	0.00
75) Chrysene-d12	21.26	240	946291	20.00	ng/ul	0.00
83) Perylene-d12	23.47	264	865642	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	23975	5.27	ng/uL	0.00
5) Phenol-d5	6.85	99	577238	29.59	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.01	67	331404	29.79	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	453804	29.77	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	501977	30.12	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	239398	29.42	ng/ul	0.00
22) 2-Nitrophenol-d4	9.54	143	265050	30.43	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	499718	27.84	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	609515	36.95	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	1682846	31.37	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	2081972	31.45	ng/ul	0.00
51) 4-Nitrophenol-d4	14.53	143	186834	20.04	ng/ul	0.00
57) Fluorene-d10	15.31	176	1381208	29.93	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.44	200	187793	24.38	ng/ul	0.00
70) Anthracene-d10	17.16	188	2000100	32.62	ng/ul	0.00
76) Pyrene-d10	19.46	212	1939274	41.13	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.33	264	1446243	32.80	ng/ul	0.00

Target Compounds


					Qvalue
6) Phenol	6.87	94	83076	4.308	ng/ul 88
44) Dimethylphthalate	13.77	163	520329	10.140	ng/ul 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM122617\
 Data File : BM013541.D
 Acq On : 26 Dec 2017 19:02
 Operator : SJ/JU
 Sample : I7046-10
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampled :
 COFMO

Quant Time: Dec 27 03:54:17 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM113017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Dec 27 03:26:43 2017
 Response via : Initial Calibration




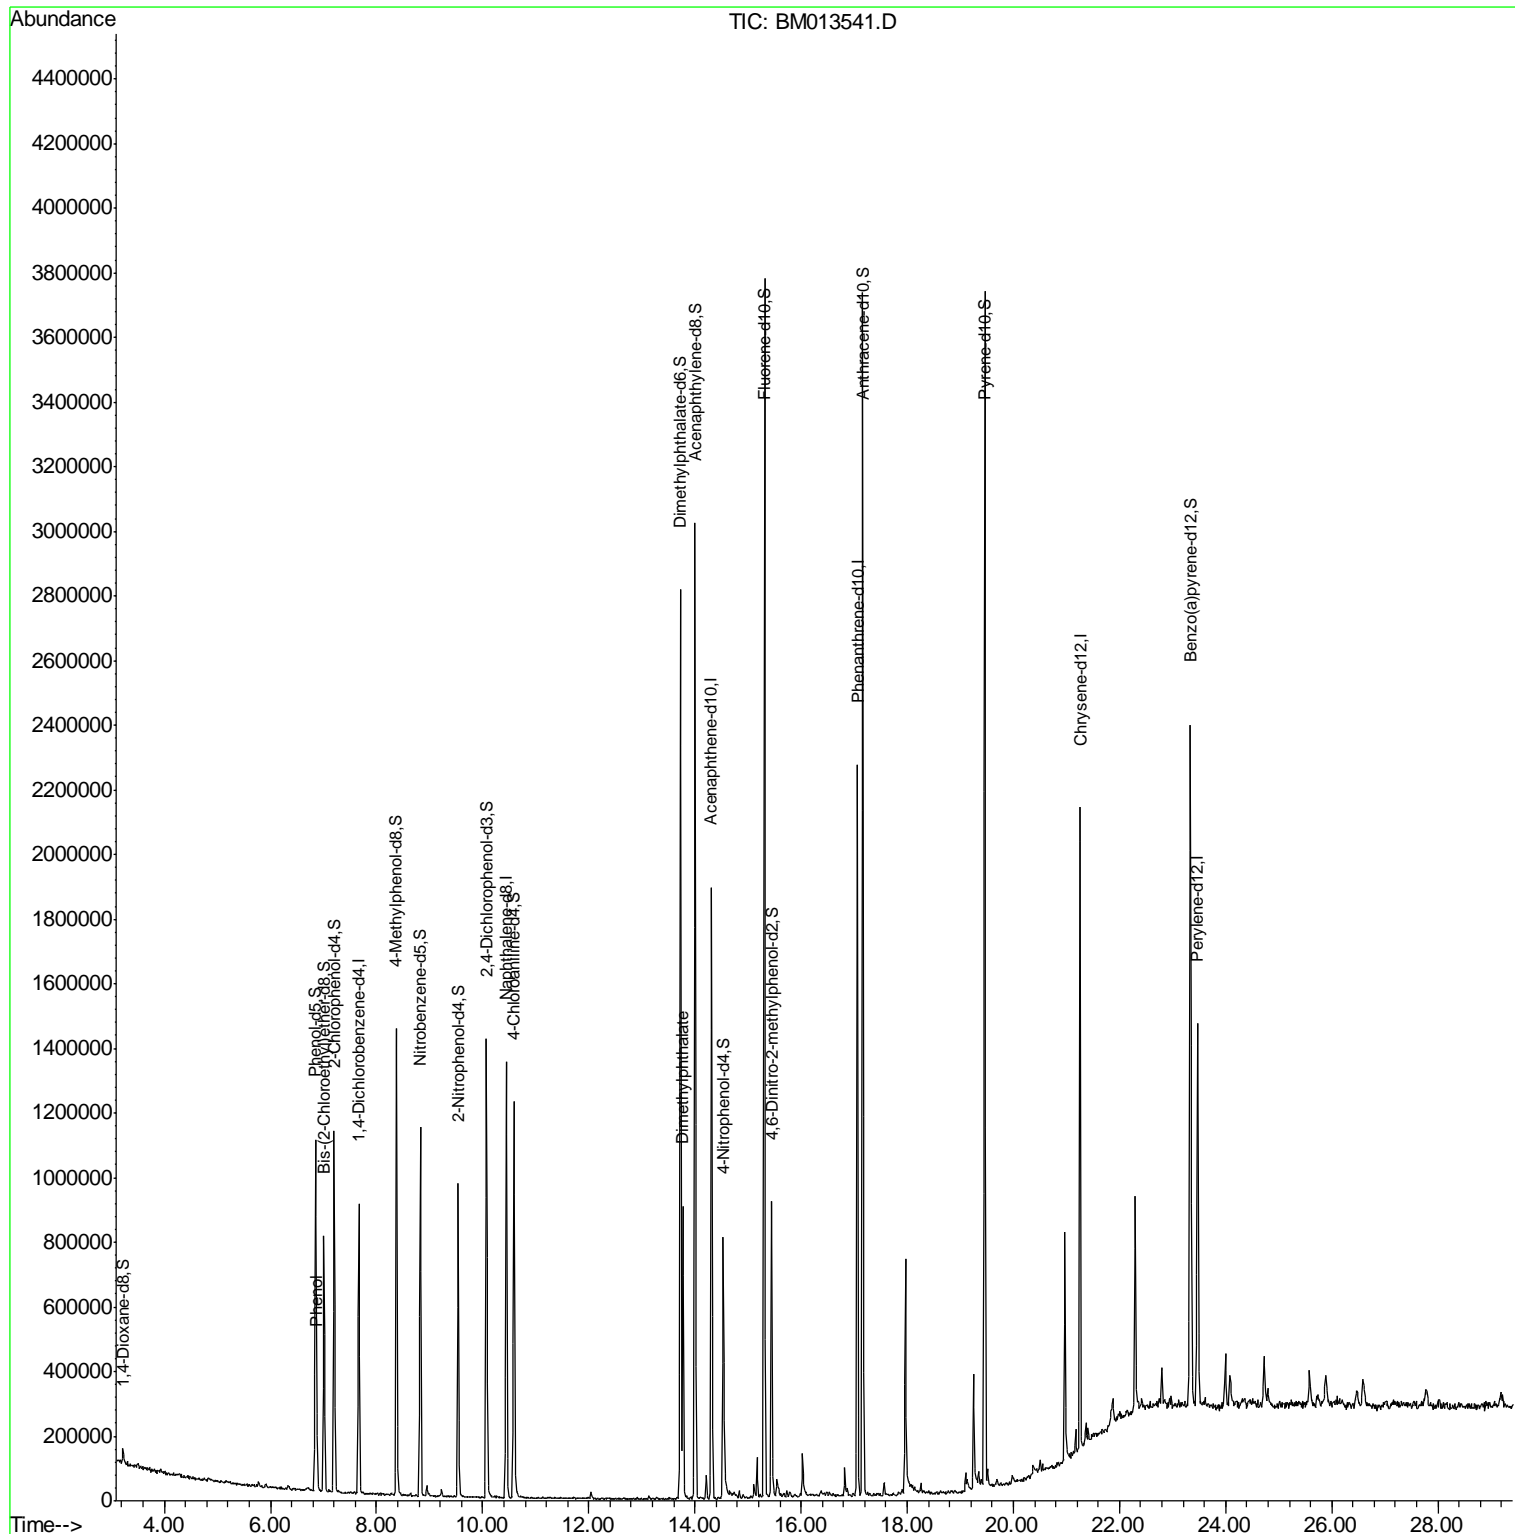


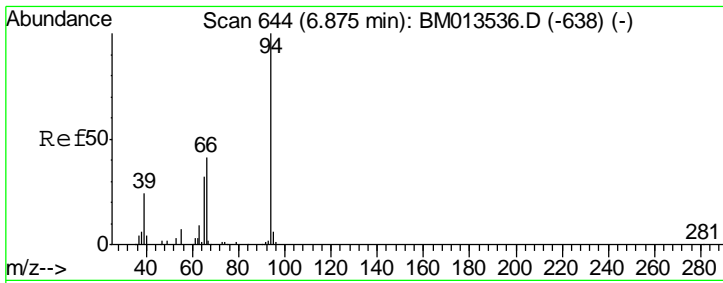

#6
 Phenol
 Concen: 4.308 ng/ul
 RT: 6.87 min Scan# 644
 Delta R.T. -0.00 min
 Lab File: BM013541.D
 Acq: 26 Dec 2017 19:02

Instrument :
 BNA_M
ClientSampled :
 COFMO

Tgt Ion	Resp	Lower	Upper
94	100		
65	32.5	28.2	42.4
66	47.2	47.2	70.8

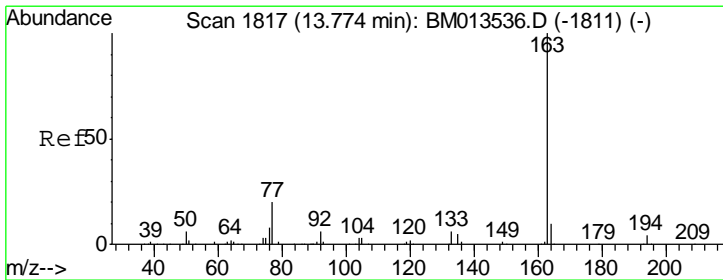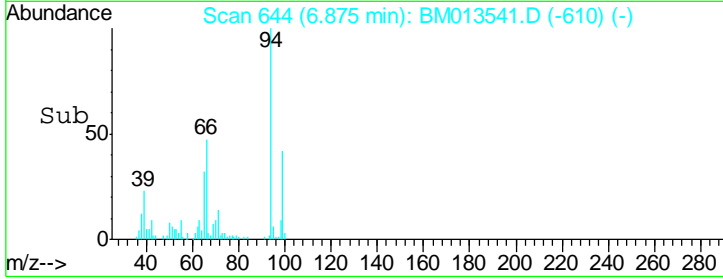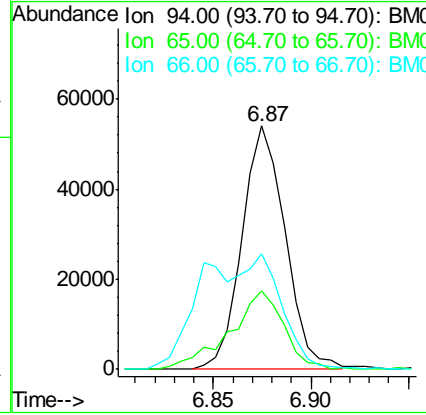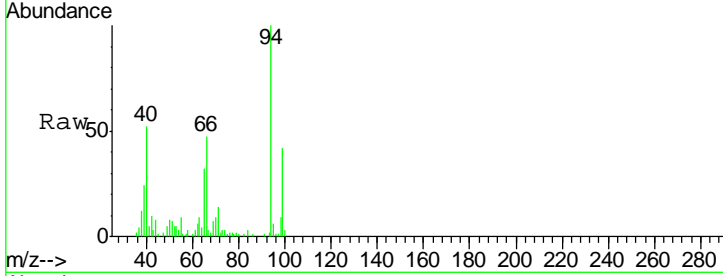

#44
 Dimethylphthalate
 Concen: 10.140 ng/ul
 RT: 13.77 min Scan# 1817
 Delta R.T. -0.00 min
 Lab File: BM013541.D
 Acq: 26 Dec 2017 19:02

Tgt Ion	Resp	Lower	Upper
163	100		
194	4.7	3.5	5.3
164	9.2	8.2	12.4

