

Data File : BM024304.D
Acq On : 26 Dec 2019 18:46
Operator : JU
Sample : PB125632BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK32

Quant Time: Dec 27 06:01:16 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 27 05:58:29 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	214895	20.00	ng/ul	0.00
18) Naphthalene-d8	10.19	136	883868	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.09	164	509290	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.85	188	1032492	20.00	ng/ul	0.00
78) Chrysene-d12	21.06	240	948847	20.00	ng/ul	0.00
86) Perylene-d12	23.19	264	1168425	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.99	96	36623	7.53	ng/uL	0.00
5) Phenol-d5	6.62	99	619352	30.44	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.78	67	422561	34.63	ng/ul	0.00
9) 2-Chlorophenol-d4	6.96	132	496283	34.20	ng/ul	0.00
13) 4-Methylphenol-d8	8.15	113	493104	29.65	ng/ul	0.00
19) Nitrobenzene-d5	8.58	128	230065	36.22	ng/ul	0.00
22) 2-Nitrophenol-d4	9.29	143	254852	36.50	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.83	165	434517	32.01	ng/ul	0.00
29) 4-Chloroaniline-d4	10.35	131	627637	38.07	ng/ul	0.00
44) Dimethylphthalate-d6	13.51	166	1401730	37.22	ng/ul	0.00
47) Acenaphthylene-d8	13.77	160	1650089	36.57	ng/ul	0.00
52) 4-Nitrophenol-d4	14.35	143	166124	24.57	ng/ul	0.00
58) Fluorene-d10	15.09	176	1185694	35.91	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.25	200	150880	23.95	ng/ul	0.00
71) Anthracene-d10	16.95	188	1764100	37.55	ng/ul	0.00
79) Pyrene-d10	19.26	212	1869295	41.36	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.06	264	2212221	38.12	ng/ul	0.00


Target Compounds					Qvalue	
46) 2,6-Dinitrotoluene	13.52	165	9724	1.261	ng/ul#	35


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM024304.D
Acq On : 26 Dec 2019 18:46
Operator : JU
Sample : PB125632BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK32

Quant Time: Dec 27 06:01:16 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Dec 27 05:58:29 2019
Response via : Initial Calibration

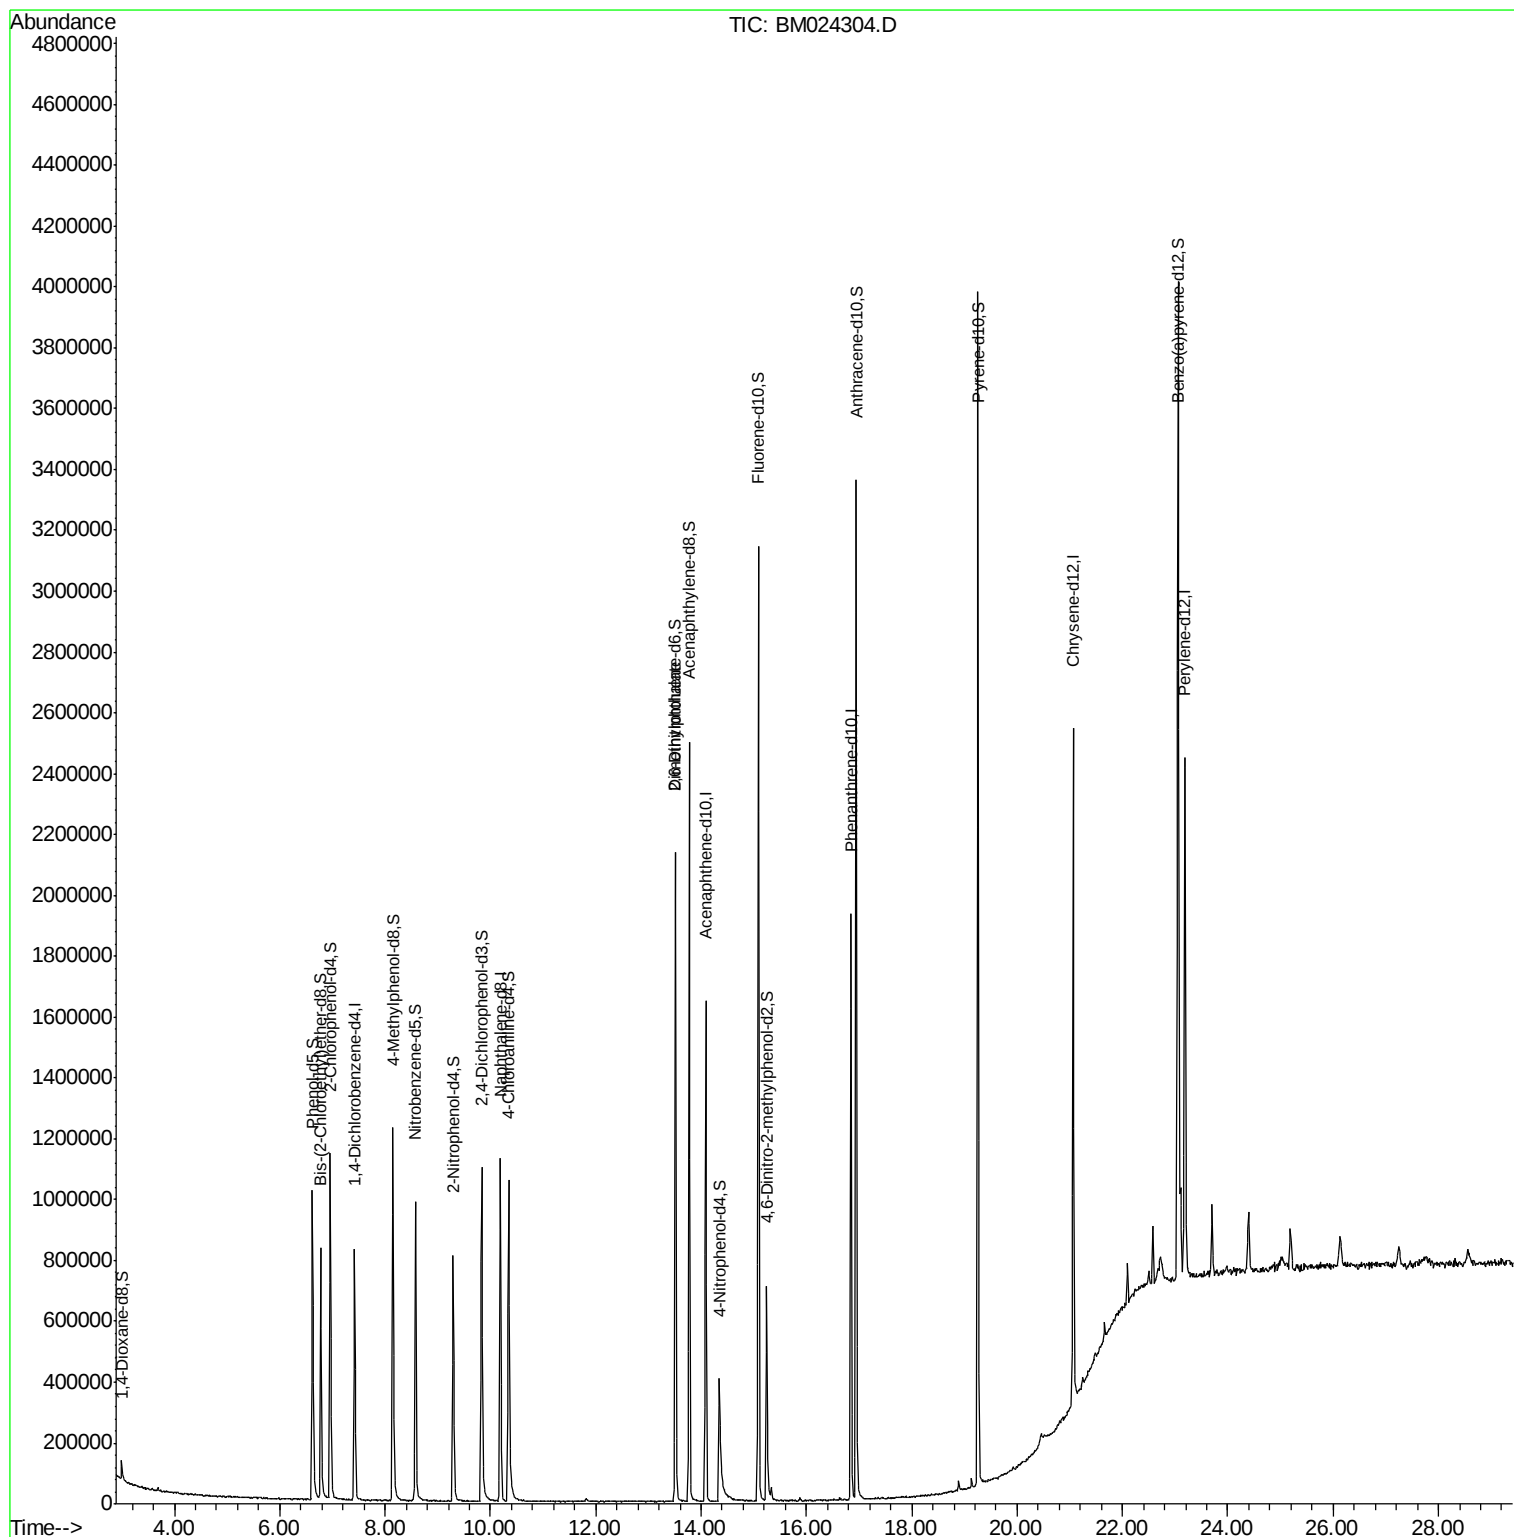

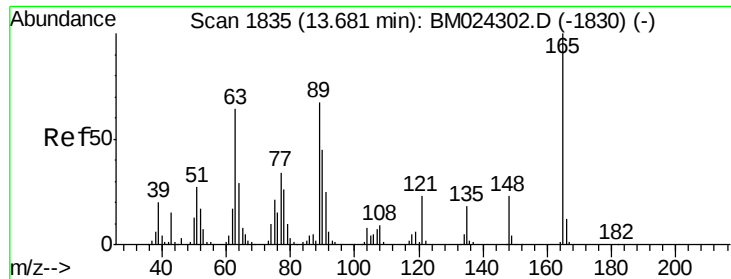

#46

2,6-Dinitrotoluene

Concen: 1.261 ng/ul

RT: 13.52 min Scan# 1807

Delta R.T. -0.16 min

Lab File: BM024304.D

Acq: 26 Dec 2019 18:46

Instrument :

BNA_M

ClientSampleId :

SBLK32



Tgt Ion:165 Resp: 9724

Ion Ratio Lower Upper

165 100

89 0.0 47.0 70.4#

121 34.0 17.1 25.7#

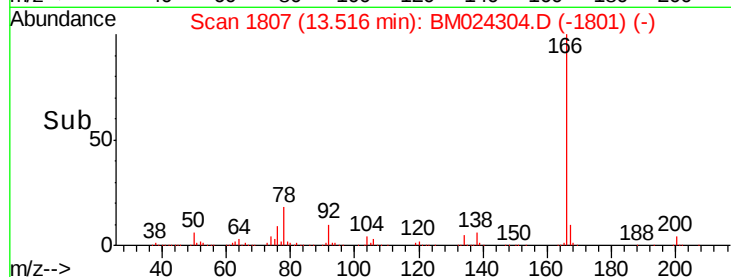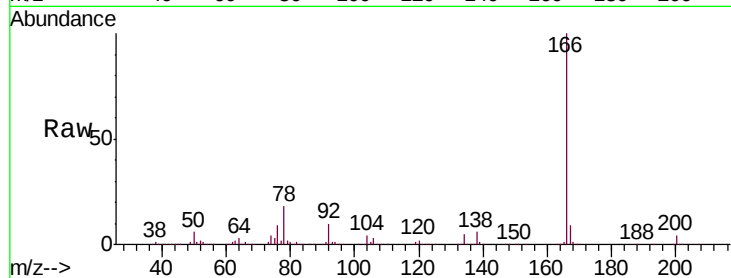

Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

