

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122619\
 Data File : BM024294.D
 Acq On : 26 Dec 2019 12:45
 Operator : JU
 Sample : K6270-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ETK79

Quant Time: Dec 26 15:06:11 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 26 03:43:38 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	206345	20.00	ng/ul	0.00
18) Naphthalene-d8	10.19	136	922151	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.09	164	555974	20.00	ng/ul	-0.01
62) Phenanthrene-d10	16.84	188	1130196	20.00	ng/ul	-0.01
78) Chrysene-d12	21.06	240	1026608	20.00	ng/ul	0.00
86) Perylene-d12	23.19	264	1226390	20.00	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.99	96	30614	6.55	ng/uL	0.00
5) Phenol-d5	6.62	99	535250	27.40	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	6.77	67	392051	33.46	ng/ul	-0.01
9) 2-Chlorophenol-d4	6.96	132	434654	31.19	ng/ul	0.00
13) 4-Methylphenol-d8	8.15	113	446503	27.96	ng/ul	-0.01
19) Nitrobenzene-d5	8.57	128	216471	32.67	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.29	143	236516	32.46	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.83	165	412346	29.11	ng/ul	0.00
29) 4-Chloroaniline-d4	10.35	131	538720	31.32	ng/ul	0.00
44) Dimethylphthalate-d6	13.52	166	1322351	32.16	ng/ul	0.00
47) Acenaphthylene-d8	13.77	160	1613756	32.76	ng/ul	0.00
52) 4-Nitrophenol-d4	14.35	143	141707	19.20	ng/ul	0.00
58) Fluorene-d10	15.09	176	1148437	31.86	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.25	200	143453	20.81	ng/ul	0.00
71) Anthracene-d10	16.94	188	1677294	32.62	ng/ul	0.00
79) Pyrene-d10	19.26	212	1782554	36.45	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.06	264	2061522	33.84	ng/ul	-0.01
Target Compounds						
6) Phenol	6.65	94	79105	3.921	ng/ul	94
45) Dimethylphthalate	13.56	163	302061	7.069	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122619\
Data File : BM024294.D
Acq On : 26 Dec 2019 12:45
Operator : JU
Sample : K6270-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETK79

Quant Time: Dec 26 15:06:11 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 26 03:43:38 2019
Response via : Initial Calibration

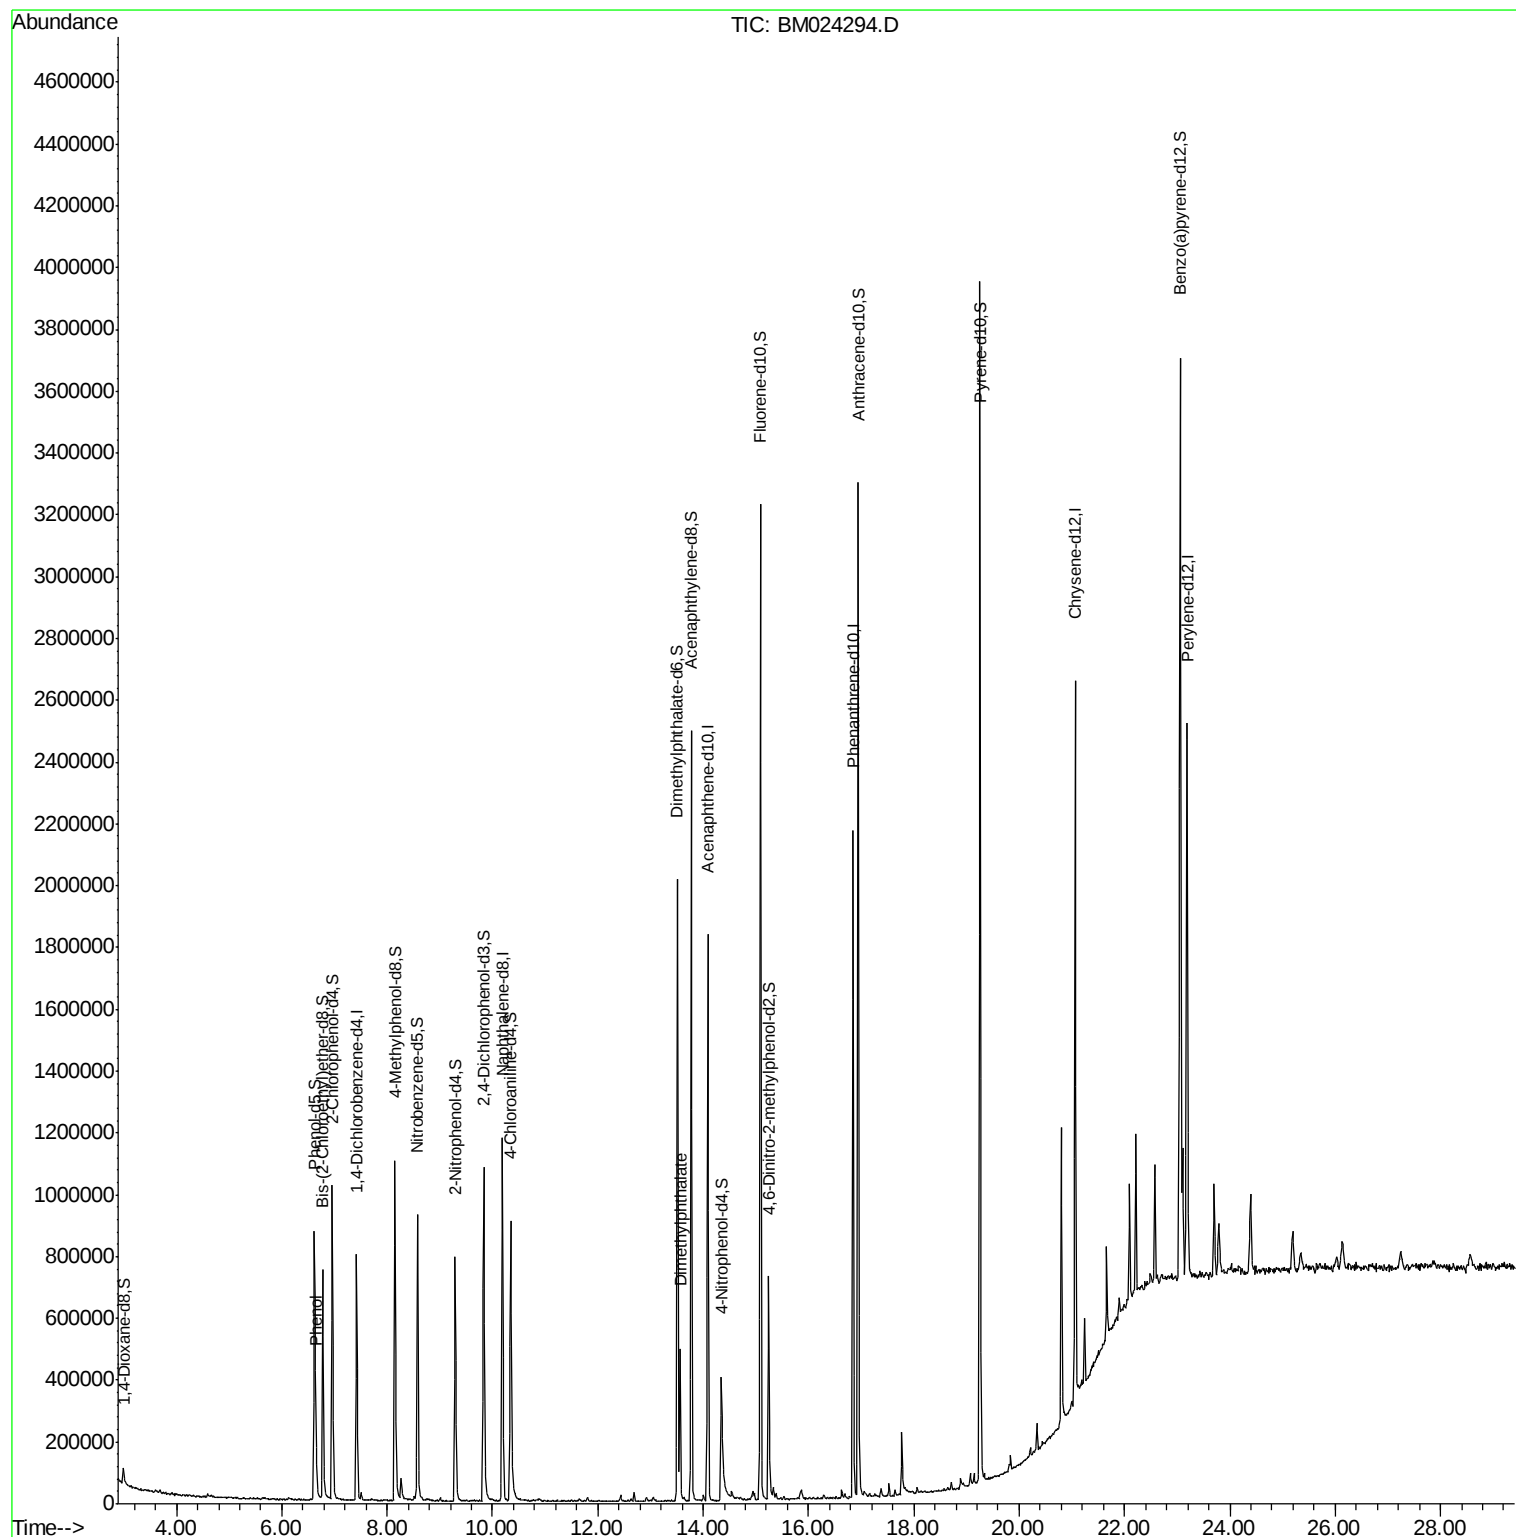

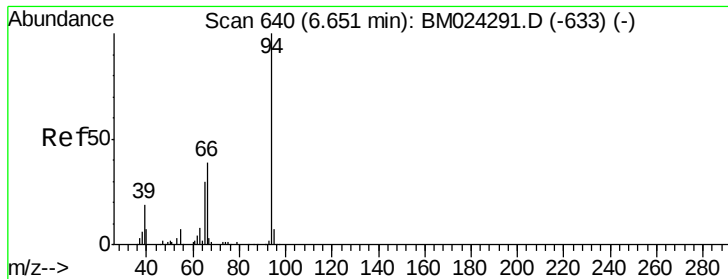

#6

Phenol

Concen: 3.921 ng/ul

RT: 6.65 min Scan# 640

Delta R.T. -0.01 min

Lab File: BM024294.D

Acq: 26 Dec 2019 12:45

Instrument :

BNA_M

ClientSampleID :

ETK79





Tot Ion: 94 Resp: 79105

Ion Ratio Lower Upper

94 100

65 29.4 22.6 33.8

66 44.0 30.7 46.1

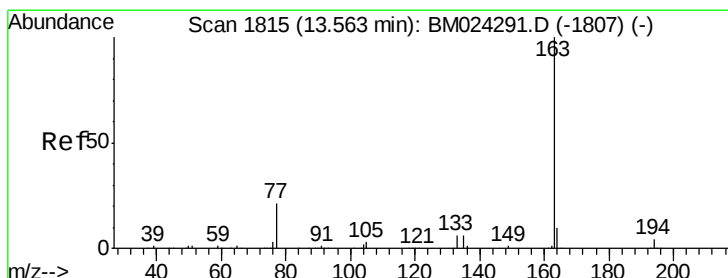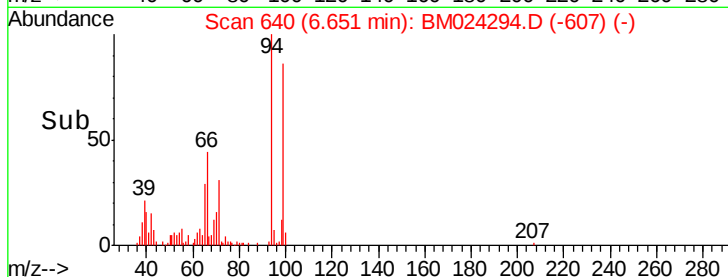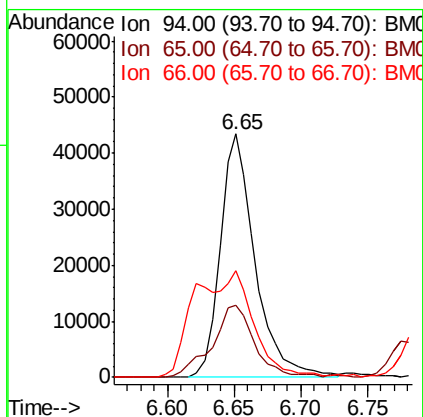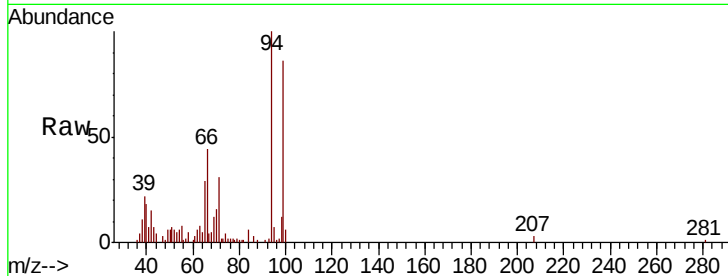

#45

Dimethylphthalate

Concen: 7.069 ng/ul

RT: 13.56 min Scan# 1815

Delta R.T. -0.01 min

Lab File: BM024294.D

Acq: 26 Dec 2019 12:45

Tgt Ion: 163 Resp: 302061

Ion Ratio Lower Upper

163 100

194 3.9 3.2 4.8

164 9.6 7.8 11.6

