

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122619\
 Data File : BM024298.D
 Acq On : 26 Dec 2019 15:10
 Operator : JU
 Sample : K6270-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ETK83

Quant Time: Dec 26 15:49:10 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Dec 26 03:43:38 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.42	152	228992	20.00	ng/ul	0.00
18) Naphthalene-d8	10.19	136	964412	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.09	164	589390	20.00	ng/ul	-0.01
62) Phenanthrene-d10	16.84	188	1154311	20.00	ng/ul	-0.01
78) Chrysene-d12	21.06	240	988150	20.00	ng/ul	0.00
86) Perylene-d12	23.19	264	1204528	20.00	ng/ul	-0.01

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.00	96	15268	2.95	ng/uL	0.00
5) Phenol-d5	6.63	99	272843	12.58	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.78	67	213218	16.40	ng/ul	0.00
9) 2-Chlorophenol-d4	6.96	132	234140	15.14	ng/ul	0.00
13) 4-Methylphenol-d8	8.15	113	227165	12.82	ng/ul	0.00
19) Nitrobenzene-d5	8.58	128	115566	16.68	ng/ul	0.00
22) 2-Nitrophenol-d4	9.30	143	128138	16.82	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.84	165	203532	13.74	ng/ul	0.00
29) 4-Chloroaniline-d4	10.35	131	320170	17.80	ng/ul	0.00
44) Dimethylphthalate-d6	13.52	166	818387	18.78	ng/ul	0.00
47) Acenaphthylene-d8	13.77	160	782382	14.98	ng/ul	0.00
52) 4-Nitrophenol-d4	14.36	143	66913	8.55	ng/ul	0.01
58) Fluorene-d10	15.09	176	606375	15.87	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.25	200	63066	8.96	ng/ul	0.00
71) Anthracene-d10	16.94	188	835430	15.91	ng/ul	0.00
79) Pyrene-d10	19.26	212	837674	17.80	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.06	264	895388	14.97	ng/ul	-0.01


Target Compounds					Ovalue	
6) Phenol	6.66	94	39241	1.753	ng/ul	96
45) Dimethylphthalate	13.56	163	218852	4.832	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122619\
Data File : BM024298.D
Acq On : 26 Dec 2019 15:10
Operator : JU
Sample : K6270-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ETK83

Quant Time: Dec 26 15:49:10 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Dec 26 03:43:38 2019
Response via : Initial Calibration

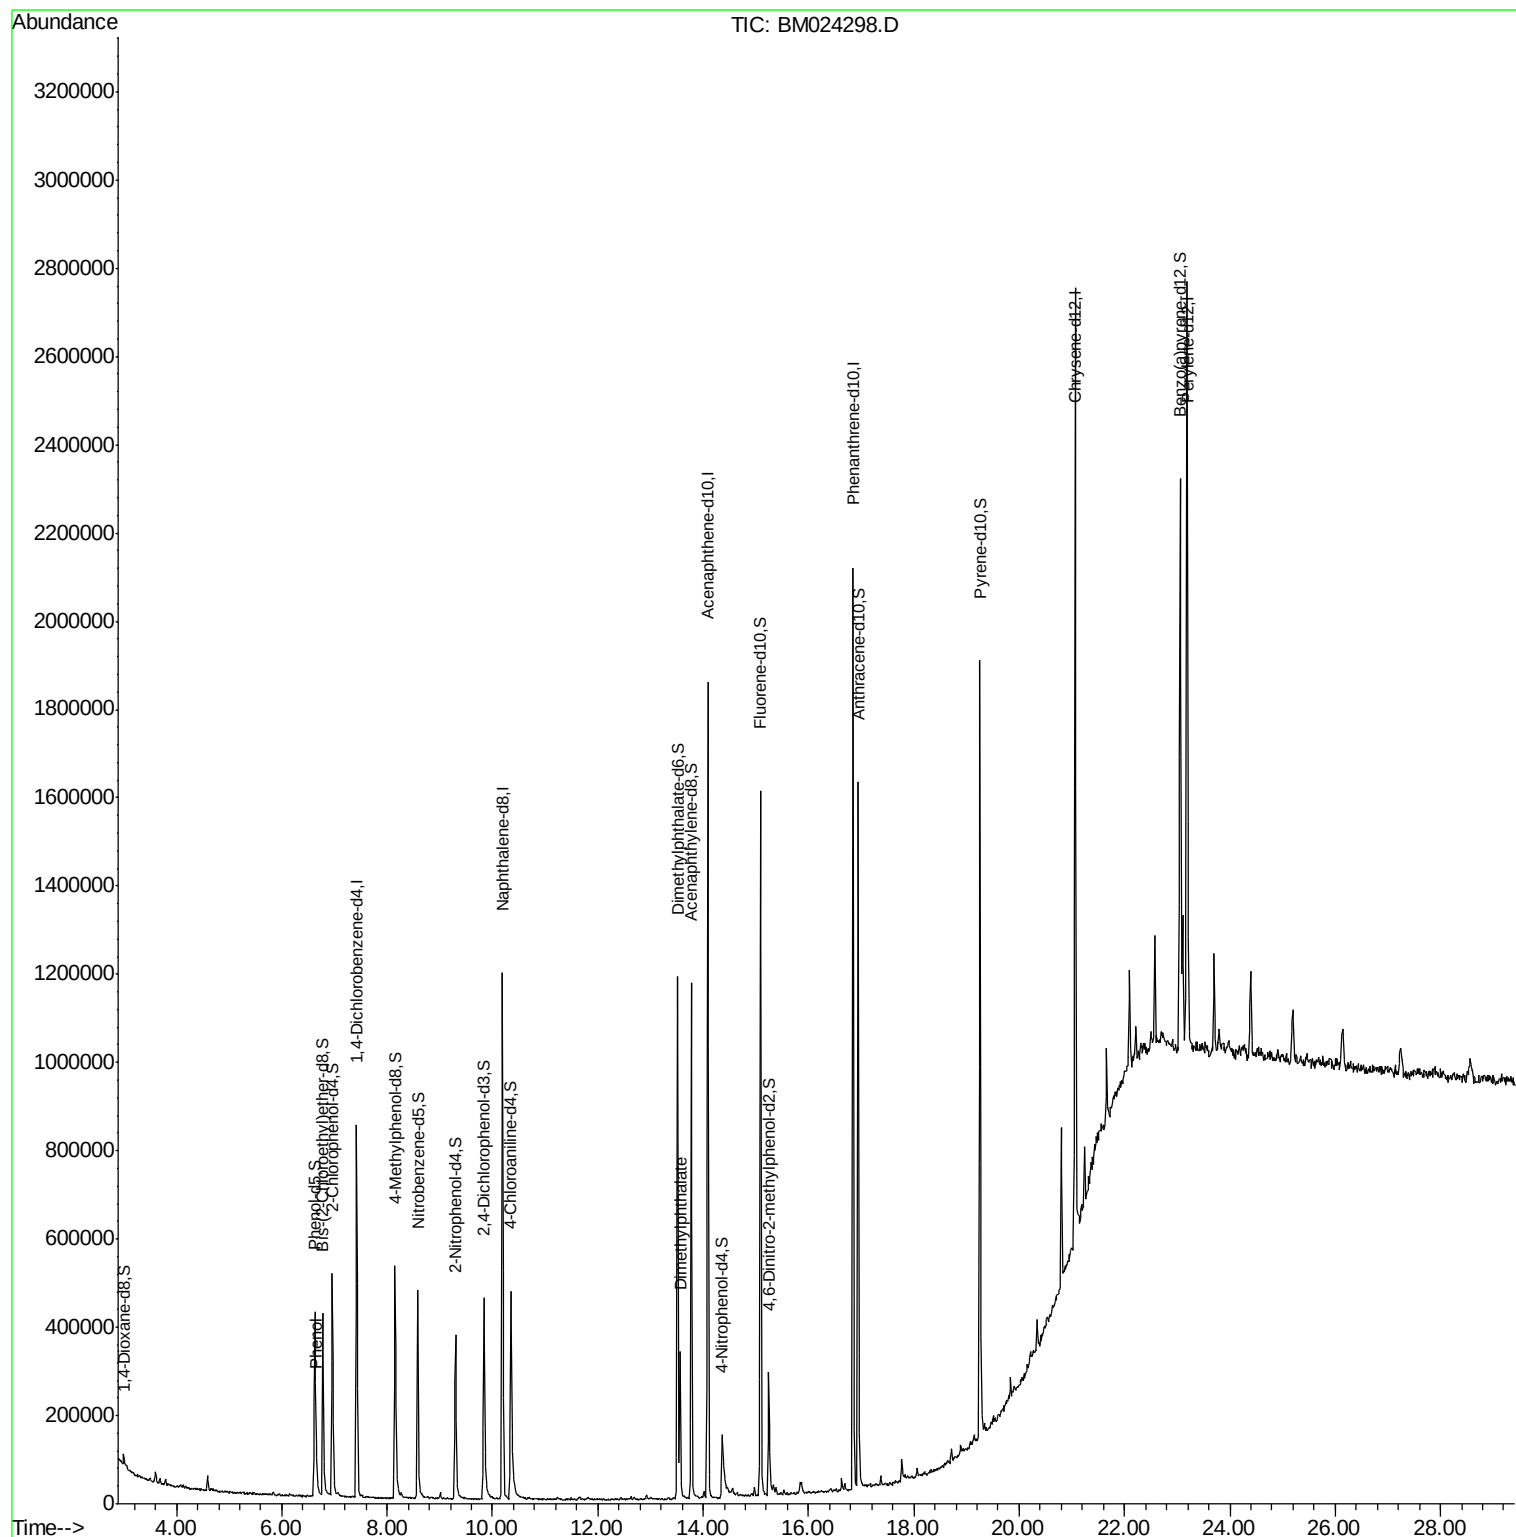

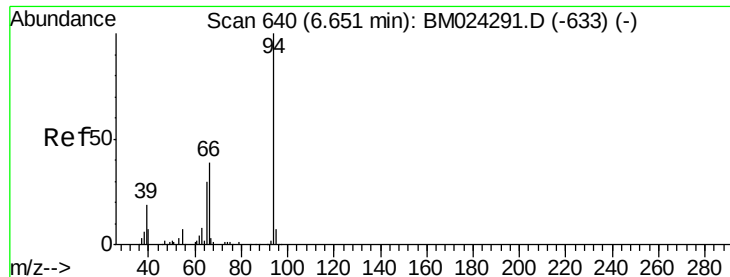





#6

Phenol

Concen: 1.753 ng/ul
 RT: 6.66 min Scan# 641
 Delta R.T. -0.00 min
 Lab File: BM024298.D
 Acq: 26 Dec 2019 15:10

Instrument :
 BNA_M
 ClientSampled :
 ETK83

Tot Ion: 94 Resp: 39241
 Ion Ratio Lower Upper
 94 100
 65 29.5 22.6 33.8
 66 41.8 30.7 46.1

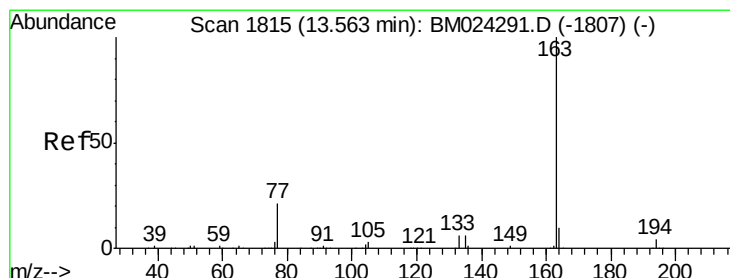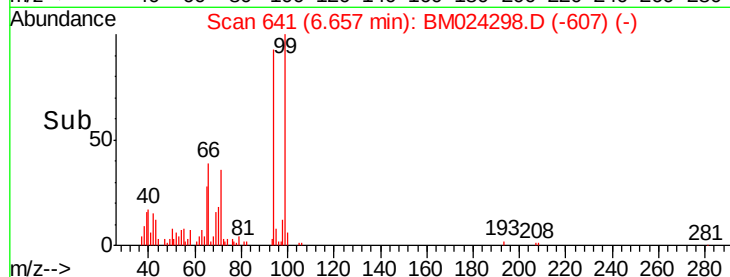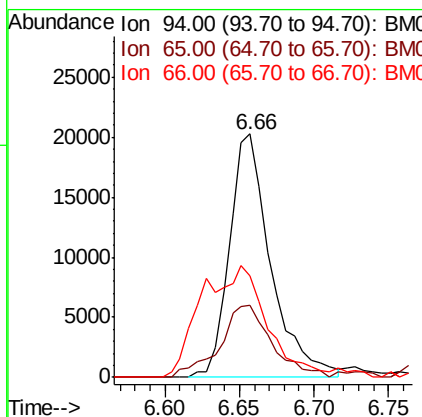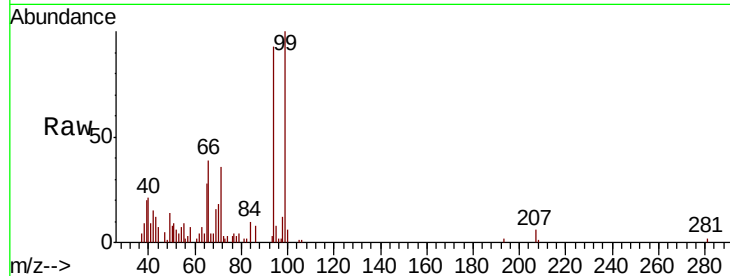

#45

Dimethylphthalate

Concen: 4.832 ng/ul
 RT: 13.56 min Scan# 1815
 Delta R.T. -0.01 min
 Lab File: BM024298.D
 Acq: 26 Dec 2019 15:10

Tgt Ion: 163 Resp: 218852
 Ion Ratio Lower Upper
 163 100
 194 3.9 3.2 4.8
 164 9.8 7.8 11.6

