

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122619\
 Data File : BM024322.D
 Acq On : 27 Dec 2019 06:10
 Operator : JU
 Sample : PB125663BL
 Misc : GCMS CONFIRMATION
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK63

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.675	132	134	135	rBV	3836	2503	0.22%	0.041%
2	3.875	166	168	171	rBV4	3291	3576	0.31%	0.059%
3	3.934	177	178	181	rBV3	3972	3973	0.34%	0.066%
4	4.199	219	223	227	rBV5	3028	5979	0.51%	0.099%
5	4.246	230	231	234	rBV2	3977	3678	0.32%	0.061%
6	4.316	242	243	245	rVB2	4333	2888	0.25%	0.048%
7	4.340	245	247	249	rBV3	2012	2225	0.19%	0.037%
8	4.422	259	261	266	rVB6	3313	4465	0.38%	0.074%
9	4.463	266	268	270	rBV3	2800	3136	0.27%	0.052%
10	4.498	272	274	277	rBV4	3346	2744	0.24%	0.045%
11	4.581	286	288	290	rVB2	3615	1926	0.17%	0.032%
12	4.940	346	349	351	rVB4	2344	2772	0.24%	0.046%
13	4.981	354	356	358	rVB3	2629	2081	0.18%	0.034%
14	5.269	402	405	407	rBV3	3215	2711	0.23%	0.045%
15	5.463	436	438	441	rVB3	2223	2007	0.17%	0.033%
16	5.540	448	451	453	rBV2	1989	2282	0.20%	0.038%
17	5.663	470	472	475	rVB4	2719	3134	0.27%	0.052%
18	5.693	475	477	479	rBV2	2678	2822	0.24%	0.047%
19	5.763	487	489	490	rBV	2820	2076	0.18%	0.034%
20	6.022	531	533	537	rBV3	2312	3666	0.32%	0.061%
21	6.245	570	571	573	rBV2	2668	2050	0.18%	0.034%
22	6.563	623	625	630	rVB4	1991	2208	0.19%	0.036%
23	6.634	635	637	640	rVB2	2405	2247	0.19%	0.037%
24	6.998	696	699	700	rBV3	2154	2206	0.19%	0.036%
25	7.345	754	758	760	rVB3	2715	3699	0.32%	0.061%
26	7.363	760	761	764	rBV3	2375	2487	0.21%	0.041%
27	7.422	764	771	790	rBV	400792	725960	62.40%	11.984%
28	7.639	807	808	812	rVB3	3048	3025	0.26%	0.050%
29	7.681	812	815	817	rBV3	2704	2706	0.23%	0.045%
30	7.781	830	832	835	rVV2	2097	2043	0.18%	0.034%
31	7.834	837	841	844	rVB5	1743	2344	0.20%	0.039%
32	7.881	844	849	851	rBV5	2434	3766	0.32%	0.062%
33	7.904	851	853	859	rVB5	1592	2526	0.22%	0.042%
34	8.098	884	886	889	rVV3	2747	2369	0.20%	0.039%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122619\
 Data File : BM024322.D
 Acq On : 27 Dec 2019 06:10
 Operator : JU
 Sample : PB125663BL
 Misc : GCMS CONFIRMATION
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK63

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
 Title : SVOA CALIBRATION

35	8.139	889	893	894	rVB3	2902	2920	0.25%	0.048%
36	8.163	894	897	899	rBV2	2517	3278	0.28%	0.054%
37	8.234	907	909	914	rVV4	1537	2464	0.21%	0.041%
38	8.286	916	918	921	rVB3	3229	3202	0.28%	0.053%
39	8.416	938	940	944	rBV4	1957	3150	0.27%	0.052%
40	8.469	946	949	951	rBV4	2839	3755	0.32%	0.062%
41	8.857	1012	1015	1018	rVB4	2142	2411	0.21%	0.040%
42	8.969	1027	1034	1035	rVV5	2324	3869	0.33%	0.064%
43	9.034	1042	1045	1050	rVB4	1681	2734	0.23%	0.045%
44	9.104	1054	1057	1062	rVB5	2266	3973	0.34%	0.066%
45	9.322	1089	1094	1097	rBV5	990	1917	0.16%	0.032%
46	9.398	1103	1107	1108	rBV2	2469	2269	0.20%	0.037%
47	9.410	1108	1109	1113	rVV3	2024	1966	0.17%	0.032%
48	9.539	1128	1131	1133	rVB2	2335	2204	0.19%	0.036%
49	9.563	1133	1135	1136	rBV2	2194	1871	0.16%	0.031%
50	9.781	1167	1172	1175	rVB3	1680	2815	0.24%	0.046%
51	9.810	1175	1177	1180	rBV3	1998	1945	0.17%	0.032%
52	9.933	1195	1198	1201	rVB3	1870	2095	0.18%	0.035%
53	9.963	1201	1203	1206	rBV2	2169	2278	0.20%	0.038%
54	10.186	1234	1241	1255	rBV	503264	942914	81.04%	15.566%
55	10.316	1261	1263	1266	rVB3	3052	3372	0.29%	0.056%
56	10.586	1308	1309	1312	rVB3	2332	1905	0.16%	0.031%
57	10.792	1342	1344	1347	rVB3	2228	2394	0.21%	0.040%
58	10.816	1347	1348	1351	rBV2	2267	2171	0.19%	0.036%
59	10.857	1351	1355	1357	rVB3	1501	1942	0.17%	0.032%
60	11.575	1475	1477	1480	rVB4	1845	2040	0.18%	0.034%
61	12.104	1564	1567	1573	rVB3	1787	3274	0.28%	0.054%
62	12.739	1671	1675	1676	rBV2	1910	2436	0.21%	0.040%
63	12.780	1678	1682	1684	rBV2	1841	2049	0.18%	0.034%
64	13.257	1755	1763	1766	rVB4	2262	4953	0.43%	0.082%
65	13.292	1766	1769	1770	rBV	1999	2053	0.18%	0.034%
66	13.374	1782	1783	1789	rVB3	2364	2371	0.20%	0.039%
67	13.839	1860	1862	1866	rVV2	1560	1934	0.17%	0.032%
68	13.974	1884	1885	1891	rBV2	1254	2048	0.18%	0.034%
69	14.086	1897	1904	1922	rBV	695696	1163466	100.00%	19.207%
70	14.545	1981	1982	1985	rVV3	2078	1904	0.16%	0.031%
71	14.580	1985	1988	1990	rVB2	1977	1974	0.17%	0.033%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122619\
 Data File : BM024322.D
 Acq On : 27 Dec 2019 06:10
 Operator : JU
 Sample : PB125663BL
 Misc : GCMS CONFIRMATION
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK63

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
 Title : SVOA CALIBRATION

72	14.774	2019	2021	2023	rBV3	2588	2102	0.18%	0.035%
73	14.863	2033	2036	2040	rBV3	2307	3226	0.28%	0.053%
74	14.910	2040	2044	2047	rBV4	1298	2125	0.18%	0.035%
75	15.004	2057	2060	2062	rBV3	1778	2206	0.19%	0.036%
76	15.121	2078	2080	2084	rBV3	2618	2042	0.18%	0.034%
77	15.286	2105	2108	2109	rBV3	2284	2145	0.18%	0.035%
78	15.298	2109	2110	2114	rVB	2520	2230	0.19%	0.037%
79	15.327	2114	2115	2117	rBV	2370	1918	0.16%	0.032%
80	15.415	2127	2130	2131	rVV2	2598	2167	0.19%	0.036%
81	15.486	2139	2142	2146	rVB3	1870	2605	0.22%	0.043%
82	15.521	2146	2148	2151	rBV4	1720	2080	0.18%	0.034%
83	15.574	2154	2157	2159	rBV	2339	1911	0.16%	0.032%
84	15.639	2164	2168	2170	rBV3	1900	1901	0.16%	0.031%
85	15.839	2199	2202	2204	rBV4	1368	1946	0.17%	0.032%
86	15.992	2225	2228	2230	rVB3	2429	2356	0.20%	0.039%
87	16.174	2256	2259	2262	rVV2	3824	3874	0.33%	0.064%
88	16.633	2336	2337	2340	rBV3	1912	2071	0.18%	0.034%
89	16.698	2345	2348	2349	rBV3	2174	2127	0.18%	0.035%
90	16.845	2367	2373	2389	rBV	619195	1082885	93.07%	17.877%
91	17.233	2436	2439	2441	rVV3	3025	3708	0.32%	0.061%
92	17.256	2441	2443	2446	rVV4	2223	2511	0.22%	0.041%
93	17.298	2449	2450	2454	rVB4	3099	3242	0.28%	0.054%
94	17.327	2454	2455	2457	rBV2	3286	2201	0.19%	0.036%
95	17.598	2499	2501	2504	rVB4	2867	2262	0.19%	0.037%
96	17.633	2504	2507	2508	rBV3	2384	3066	0.26%	0.051%
97	18.021	2569	2573	2577	rBV6	4357	7962	0.68%	0.131%
98	18.898	2720	2722	2723	rBV	5002	3632	0.31%	0.060%
99	21.062	3085	3090	3097	rBV	593509	930007	79.93%	15.353%
100	23.186	3446	3451	3460	rVB	494628	958417	82.38%	15.822%


Sum of corrected areas: 6057521

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122619\
Data File : BM024322.D
Acq On : 27 Dec 2019 06:10
Operator : JU
Sample : PB125663BL
Misc : GCMS CONFIRMATION
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK63

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

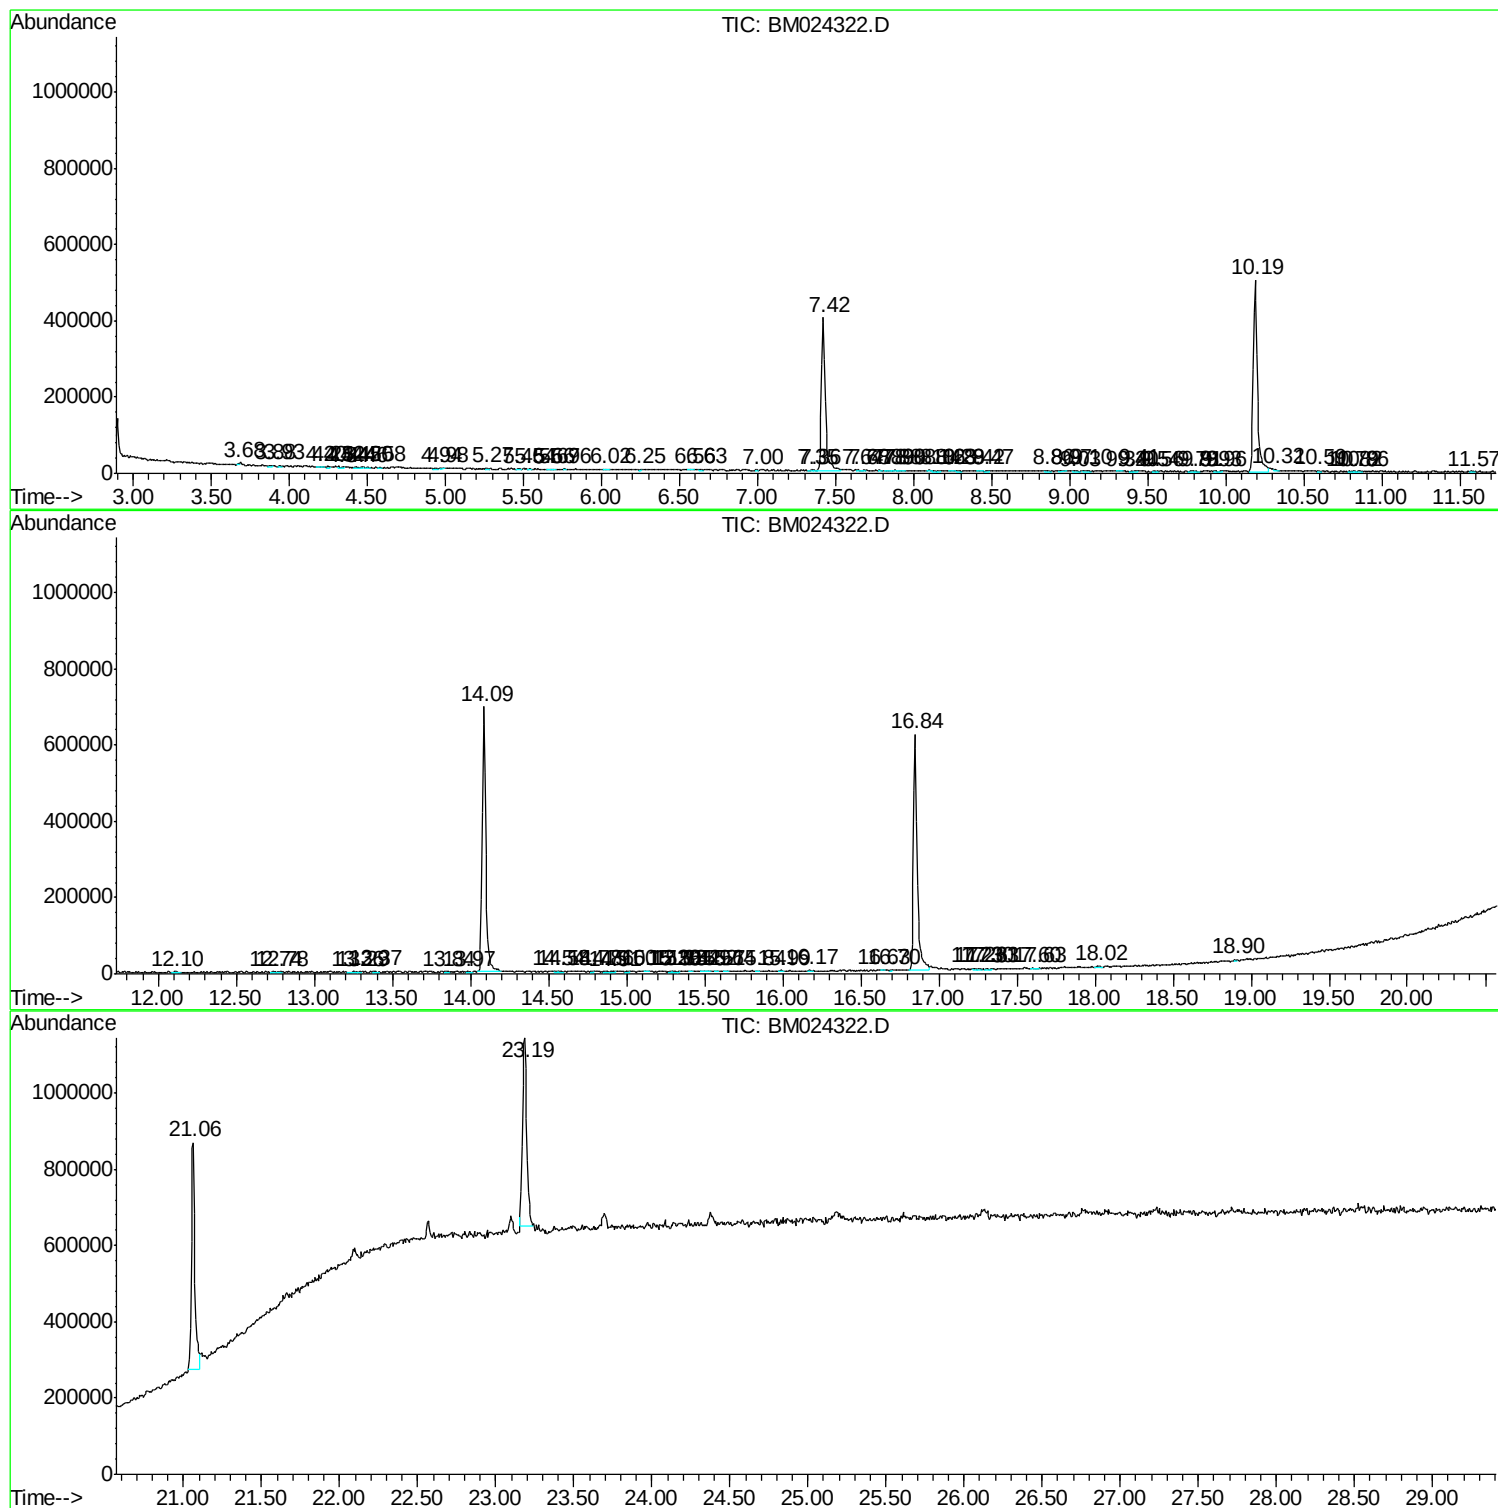

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM122619\
Data_File : BM024322.D
Acq_On : 27 Dec 2019 06:100
Operator : JUJ
Sample : PB125663BLL
Misc : GCMS_CONFIRMATIONN
ALS_Vial : 31 Sample_Multiplier: 11

Instrument :
BNA_M
ClientSampleId :
SBLK63

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.MM
Quant_Title : SVOA_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
