

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
 Data File : BM043599.D
 Acq On : 27 Dec 2023 09:17
 Operator : MA/JU
 Sample : 06020-01
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3N9

Quant Time: Dec 27 21:40:56 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 26 22:58:31 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.967	152	5486	0.400	ng/ul	0.00
4) Naphthalene-d8	10.774	136	16533	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.601	164	7487	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.443	188	1277818	0.400	ng/ul	# 0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.53
23) Perylene-d12	23.936	264	12732	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	31763	4.582	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.368	152	6710	0.286	ng/ul	0.00
18) Fluoranthene-d10	19.371	212	10438	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.410	88	480	0.069	ng/ul#	68
26) Benzo(a)pyrene	23.781	252	5023	0.105	ng/ul#	47


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
Data File : BM043599.D
Acq On : 27 Dec 2023 09:17
Operator : MA/JU
Sample : 06020-01
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3N9

Quant Time: Dec 27 21:40:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 26 22:58:31 2023
Response via : Initial Calibration




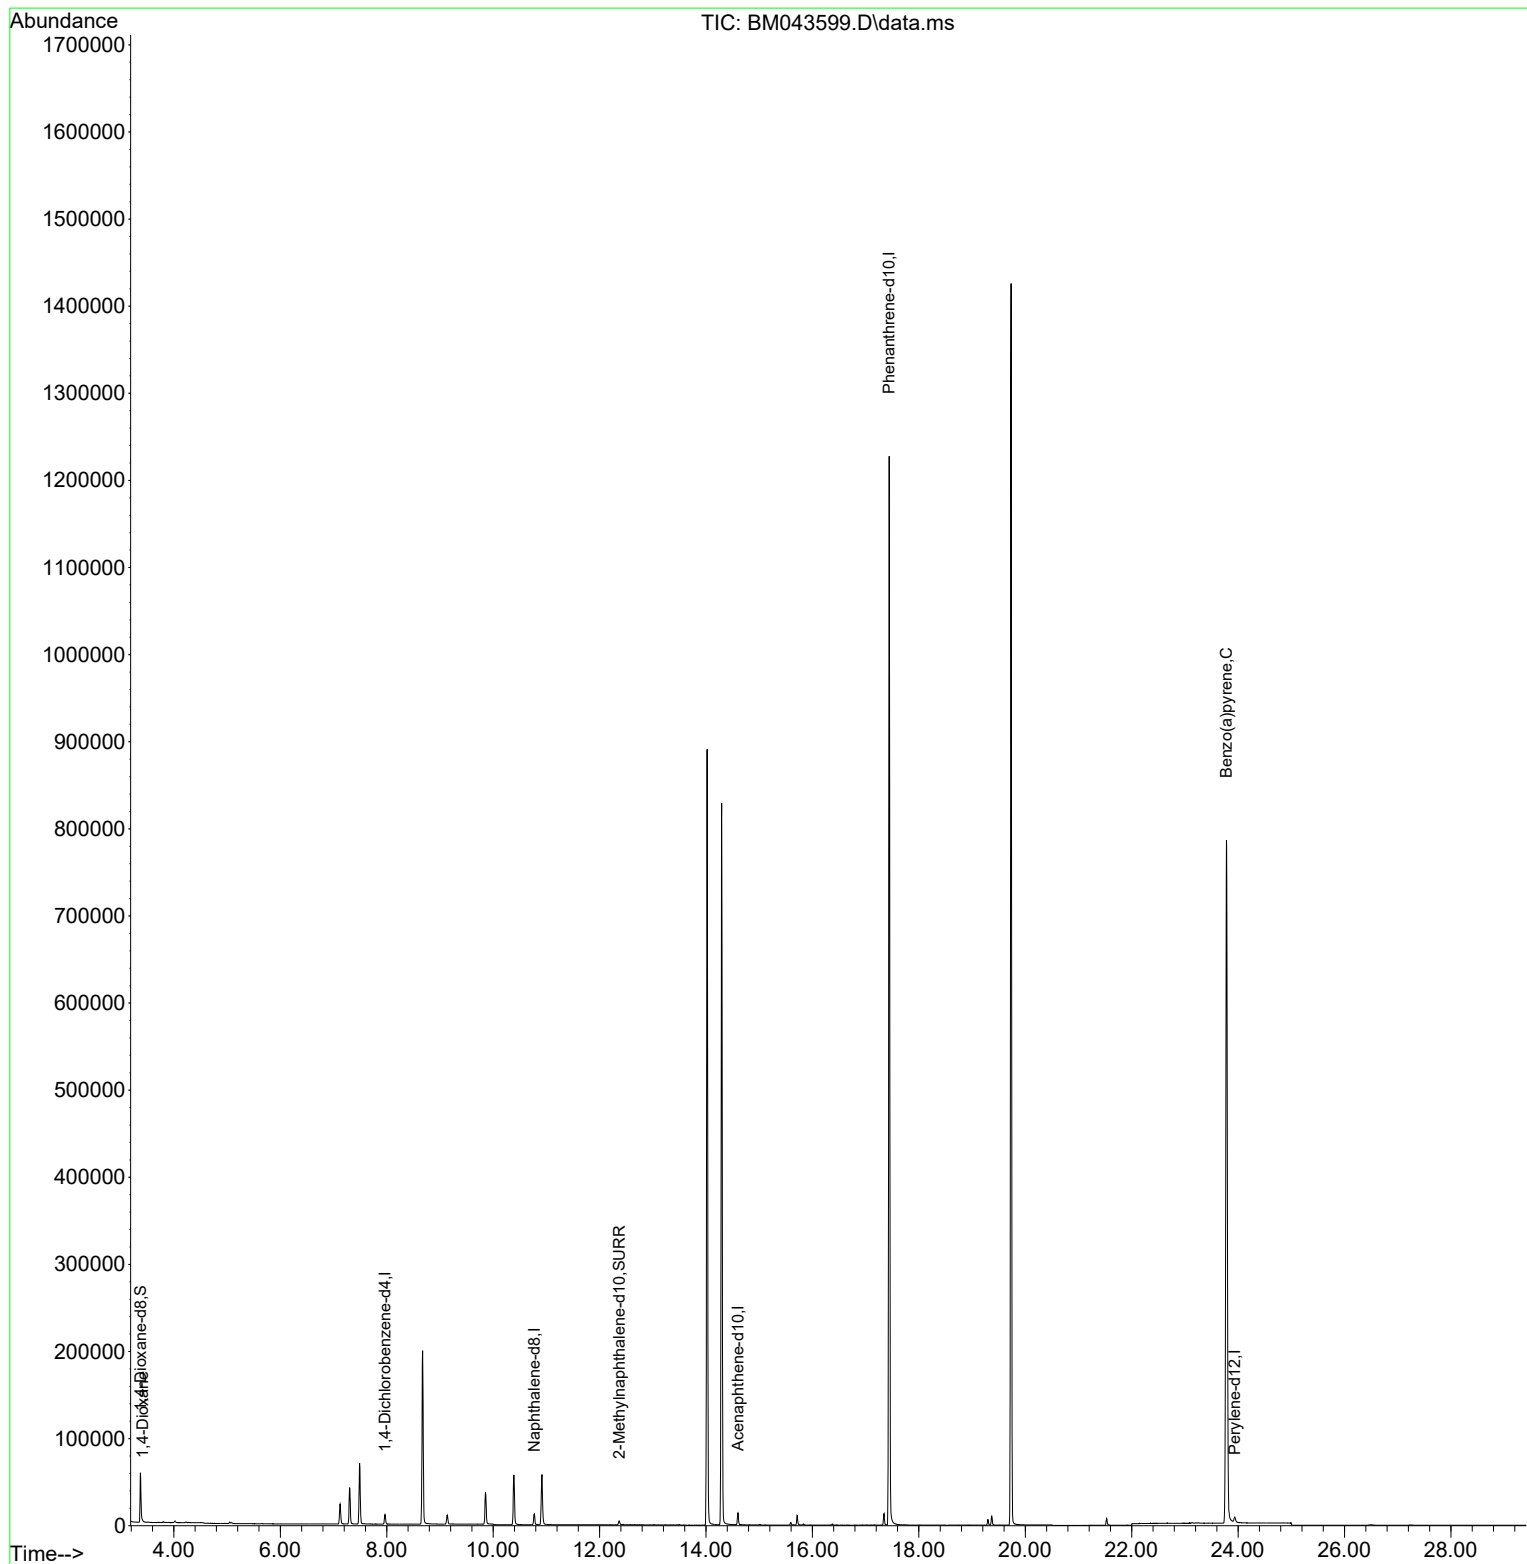


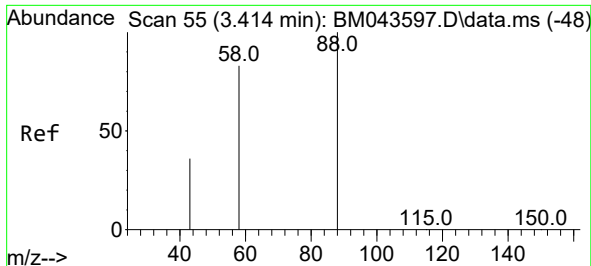

#2
1,4-Dioxane
Concen: 0.069 ng/ul
RT: 3.410 min Scan# 54
Delta R.T. -0.004 min
Lab File: BM043599.D
Acq: 27 Dec 2023 09:17

Instrument :
BNA_M
ClientSampleId :
BH3N9

Tgt Ion: 88 Resp: 480
Ion Ratio Lower Upper
88 100
43 36.1 27.9 41.9
58 17.2 43.4 65.2#

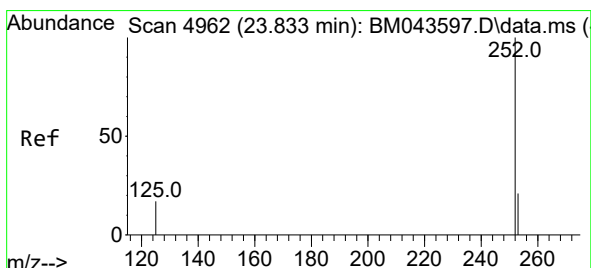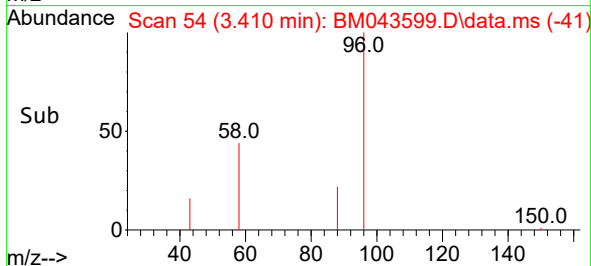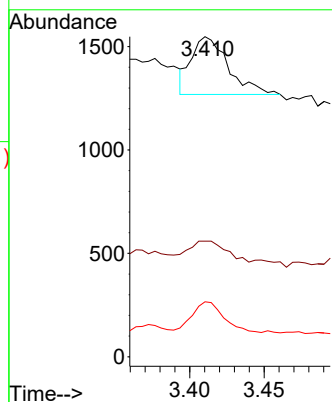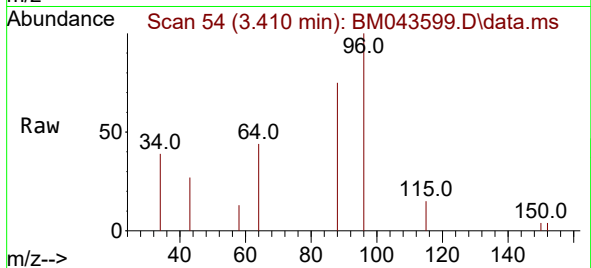

#26
Benzo(a)pyrene
Concen: 0.105 ng/ul
RT: 23.781 min Scan# 4944
Delta R.T. -0.052 min
Lab File: BM043599.D
Acq: 27 Dec 2023 09:17

Tgt Ion: 252 Resp: 5023
Ion Ratio Lower Upper
252 100
253 45.8 20.2 30.2#
125 48.0 13.5 20.3#

