

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
 Data File : BM043608.D
 Acq On : 27 Dec 2023 14:44
 Operator : MA/JU
 Sample : 06020-09
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH7X0

Quant Time: Dec 27 21:41:58 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 26 22:58:31 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.971	152	5013	0.400	ng/ul	0.00
4) Naphthalene-d8	10.773	136	15128	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.601	164	6833	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.451	188	1387938	0.400	ng/ul	# 0.10
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.53
23) Perylene-d12	23.936	264	12263	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	32131	5.073	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.363	152	7680	0.358	ng/ul	0.00
18) Fluoranthene-d10	19.371	212	12418	0.000	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.410	88	3469	0.546	ng/ul#	75
12) Fluorene	15.596	166	2806	0.090	ng/ul#	14
26) Benzo(a)pyrene	23.781	252	4889	0.106	ng/ul#	47


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
Data File : BM043608.D
Acq On : 27 Dec 2023 14:44
Operator : MA/JU
Sample : 06020-09
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH7X0

Quant Time: Dec 27 21:41:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 26 22:58:31 2023
Response via : Initial Calibration




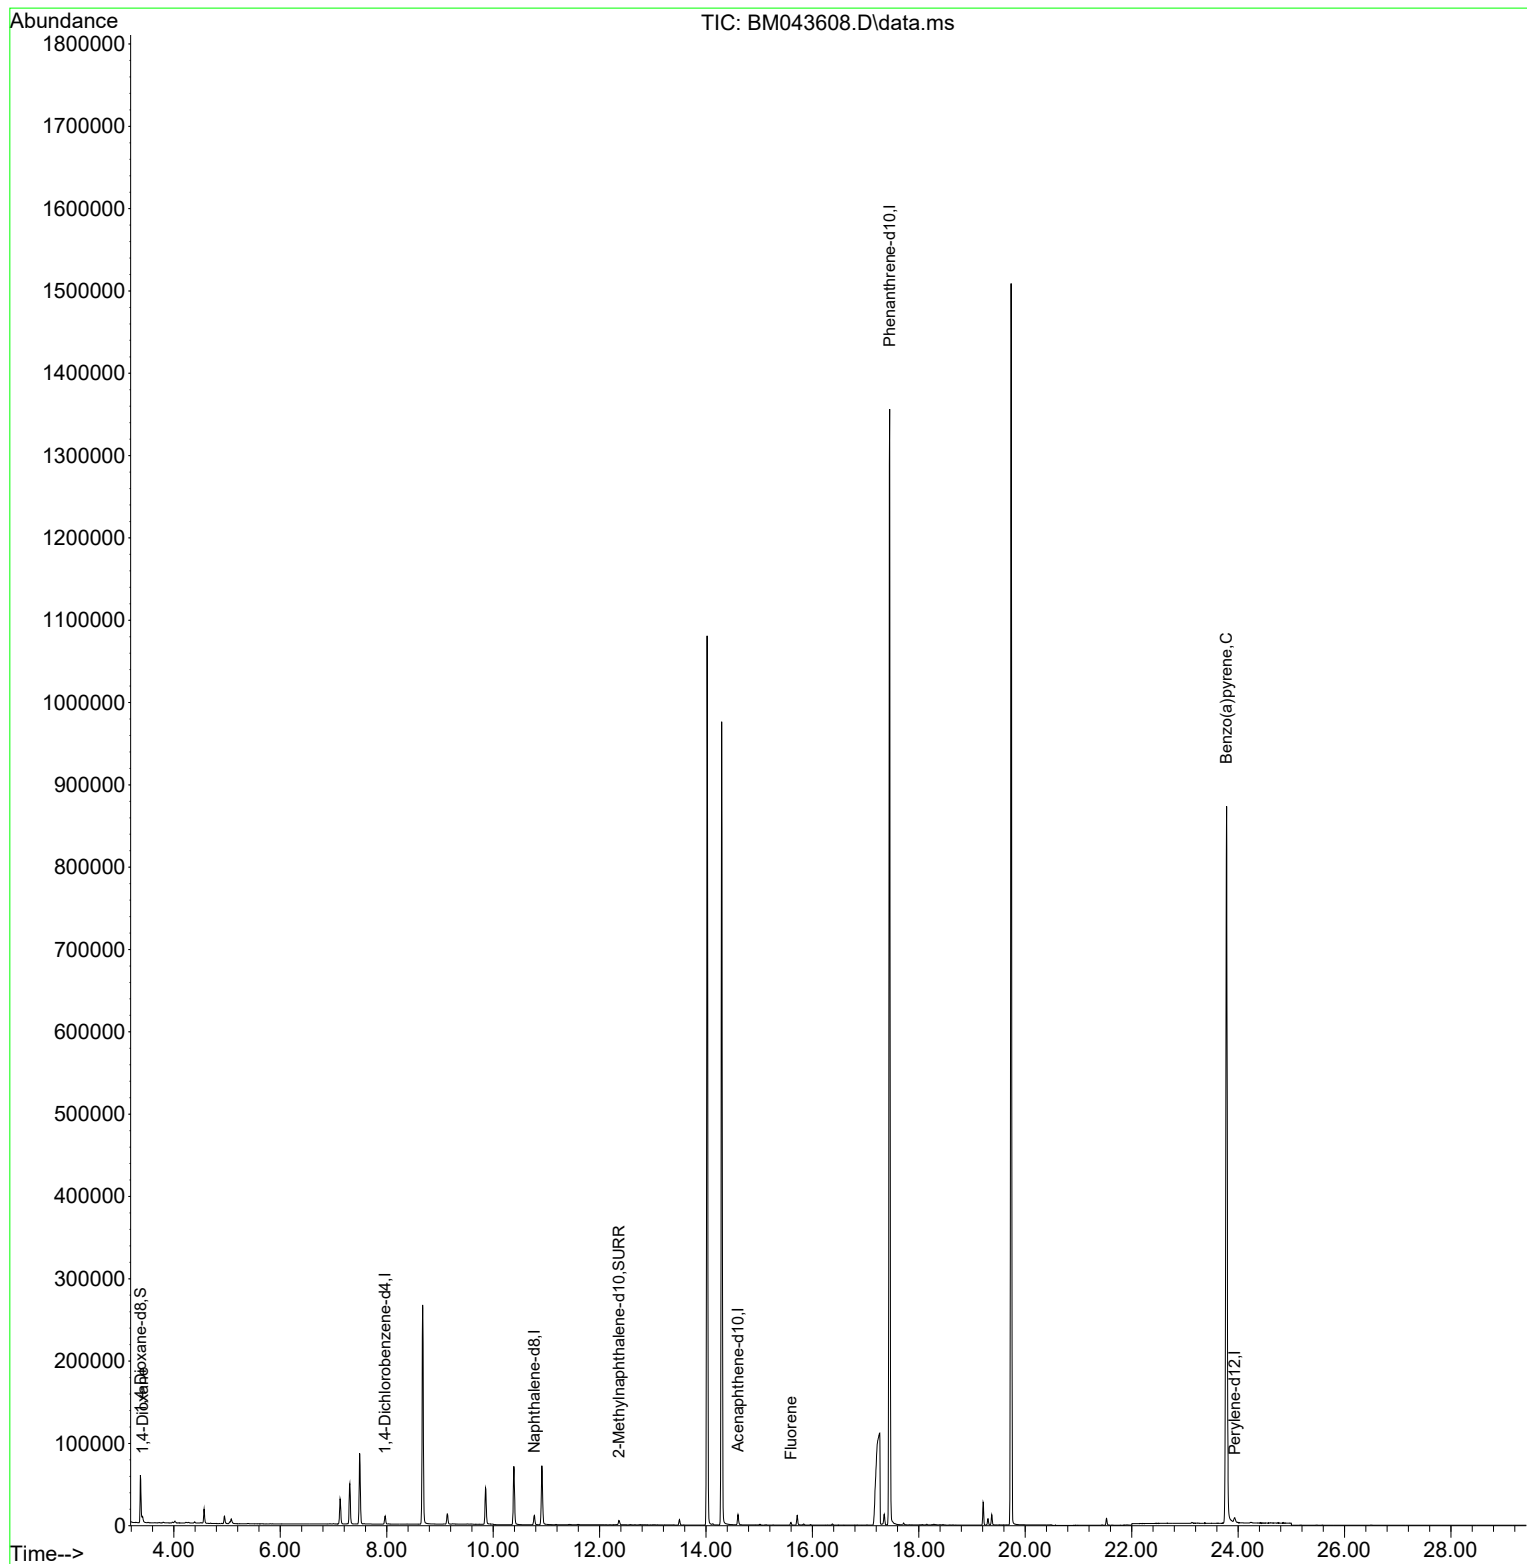


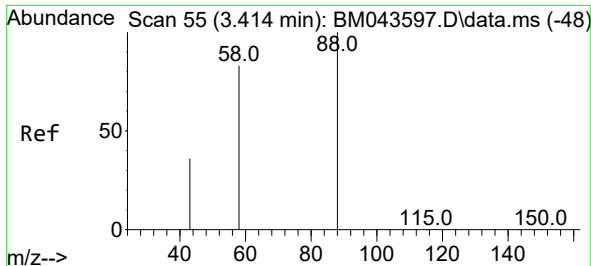

#2
1,4-Dioxane
Concen: 0.546 ng/ul
RT: 3.410 min Scan# 54
Delta R.T. -0.004 min
Lab File: BM043608.D
Acq: 27 Dec 2023 14:44




Instrument :
BNA_M
ClientSampleId :
BH7X0


Tgt Ion: 88 Resp: 3469
Ion Ratio Lower Upper
88 100
43 55.0 27.9 41.9#
58 68.3 43.4 65.2#

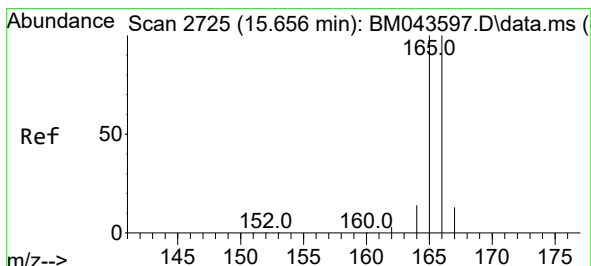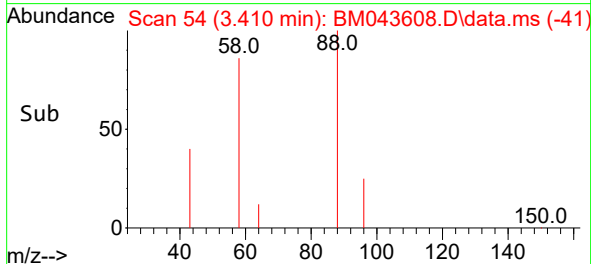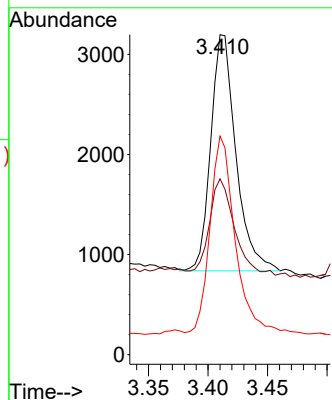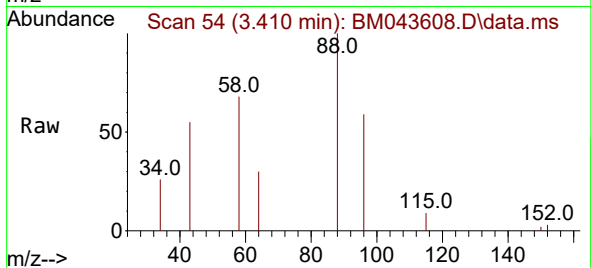

#12
Fluorene
Concen: 0.090 ng/ul
RT: 15.596 min Scan# 2712
Delta R.T. -0.060 min
Lab File: BM043608.D
Acq: 27 Dec 2023 14:44


Tgt Ion: 166 Resp: 2806
Ion Ratio Lower Upper
166 100
165 9.1 80.3 120.5#
167 34.3 10.8 16.2#

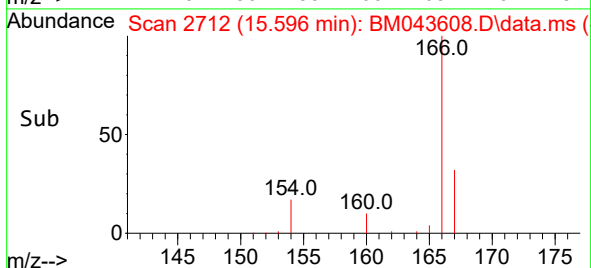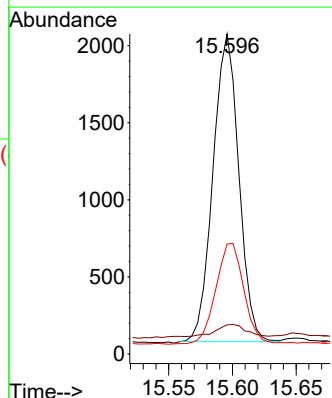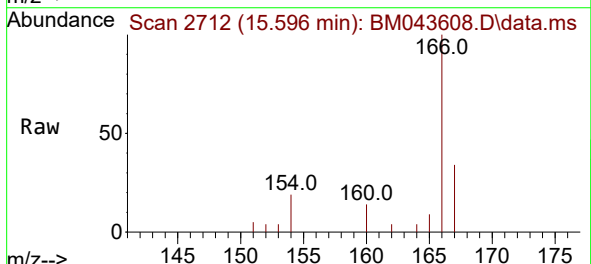

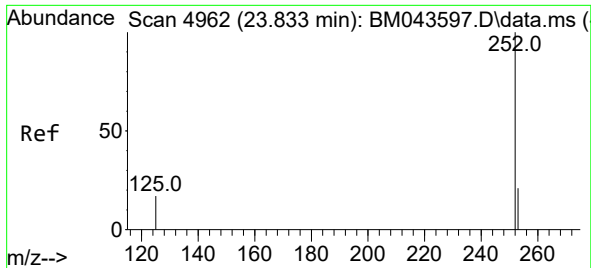

#26
Benzo(a)pyrene
Concen: 0.106 ng/ul
RT: 23.781 min Scan# 4944
Delta R.T. -0.053 min
Lab File: BM043608.D
Acq: 27 Dec 2023 14:44

Instrument :
BNA_M
ClientSampleId :
BH7X0

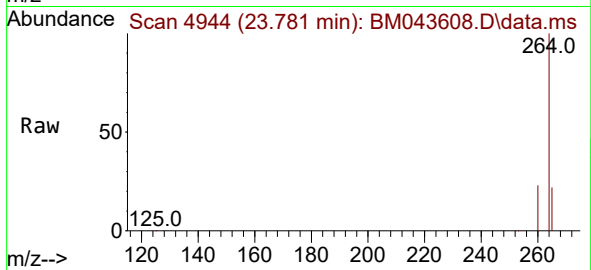

Tgt Ion:252 Resp: 4889
Ion Ratio Lower Upper
252 100
253 44.8 20.2 30.2#
125 48.5 13.5 20.3#

