

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
 Data File : BM043611.D
 Acq On : 27 Dec 2023 16:33
 Operator : MA/JU
 Sample : PB158069BL
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK069

Quant Time: Dec 27 21:42:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 26 22:58:31 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.971	152	5035	0.400	ng/ul	0.00
4) Naphthalene-d8	10.774	136	15157	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.601	164	6679	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.443	188	806774	0.400	ng/ul	# 0.09
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.53
23) Perylene-d12	23.941	264	11185	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	37915	5.960	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.368	152	5256	0.245	ng/ul	0.00
18) Fluoranthene-d10	19.371	212	6454	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.591	166	1729	0.057	ng/ul#	16
26) Benzo(a)pyrene	23.784	252	2933	0.070	ng/ul#	31


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
Data File : BM043611.D
Acq On : 27 Dec 2023 16:33
Operator : MA/JU
Sample : PB158069BL
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK069

Quant Time: Dec 27 21:42:24 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 26 22:58:31 2023
Response via : Initial Calibration




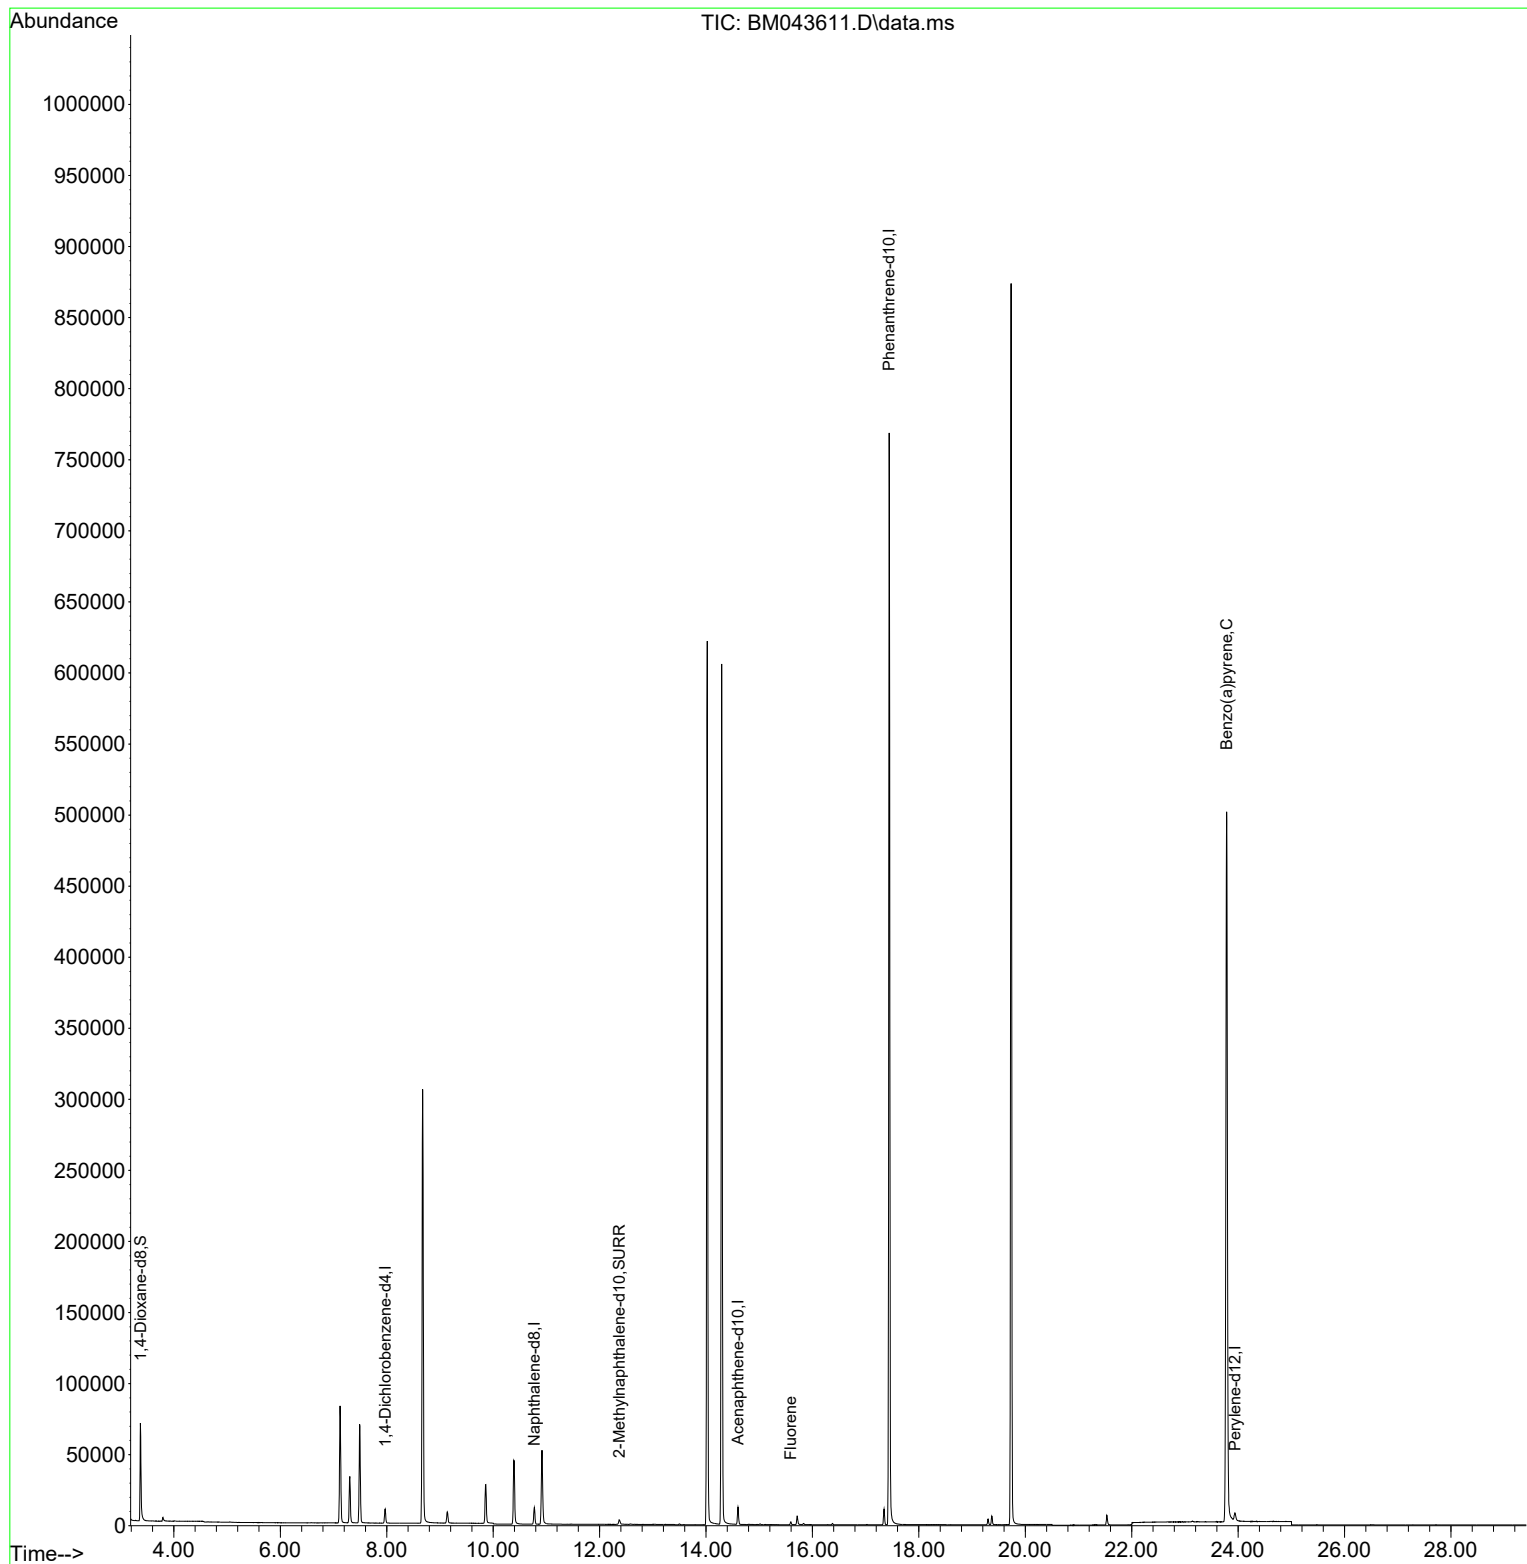


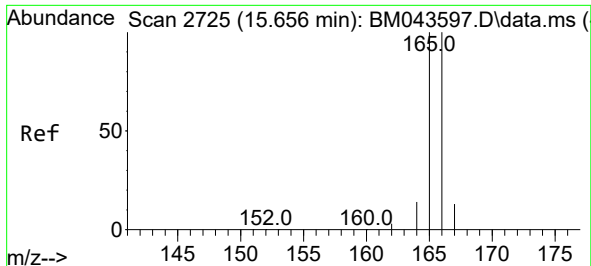

#12
Fluorene
Concen: 0.057 ng/ul
RT: 15.591 min Scan# 21
Delta R.T. -0.065 min
Lab File: BM043611.D
Acq: 27 Dec 2023 16:33

Instrument :
BNA_M
ClientSampleId :
SBLK069

Tgt Ion:166 Resp: 1729
Ion Ratio Lower Upper
166 100
165 11.5 80.3 120.5#
167 33.3 10.8 16.2#

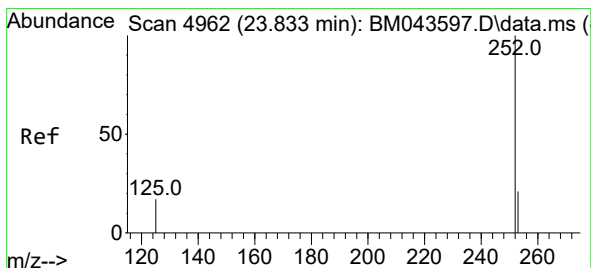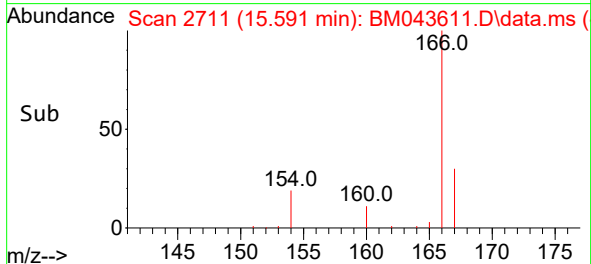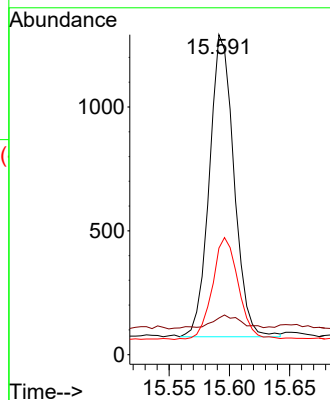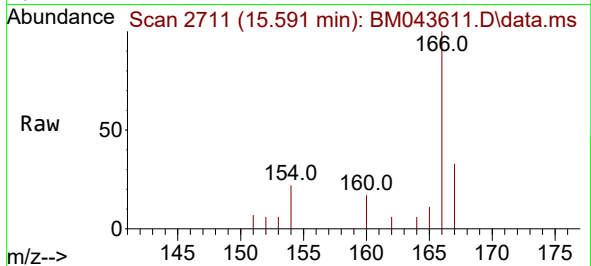

#26
Benzo(a)pyrene
Concen: 0.070 ng/ul
RT: 23.784 min Scan# 4945
Delta R.T. -0.050 min
Lab File: BM043611.D
Acq: 27 Dec 2023 16:33

Tgt Ion:252 Resp: 2933
Ion Ratio Lower Upper
252 100
253 52.7 20.2 30.2#
125 56.4 13.5 20.3#

