

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
 Data File : BM043613.D
 Acq On : 27 Dec 2023 18:22
 Operator : MA/JU
 Sample : PB158067BL
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK067

Quant Time: Dec 27 21:42:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 26 22:58:31 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.971	152	5645	0.400	ng/ul	0.00
4) Naphthalene-d8	10.774	136	17096	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.601	164	7631	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.447	188	835497	0.400	ng/ul	# 0.10
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.53
23) Perylene-d12	23.939	264	11935	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	39424	5.527	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.368	152	5487	0.226	ng/ul	0.00
18) Fluoranthene-d10	19.371	212	6514	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.596	166	1820	0.053	ng/ul#	15
26) Benzo(a)pyrene	23.781	252	2960	0.066	ng/ul#	33


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
Data File : BM043613.D
Acq On : 27 Dec 2023 18:22
Operator : MA/JU
Sample : PB158067BL
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK067

Quant Time: Dec 27 21:42:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 26 22:58:31 2023
Response via : Initial Calibration

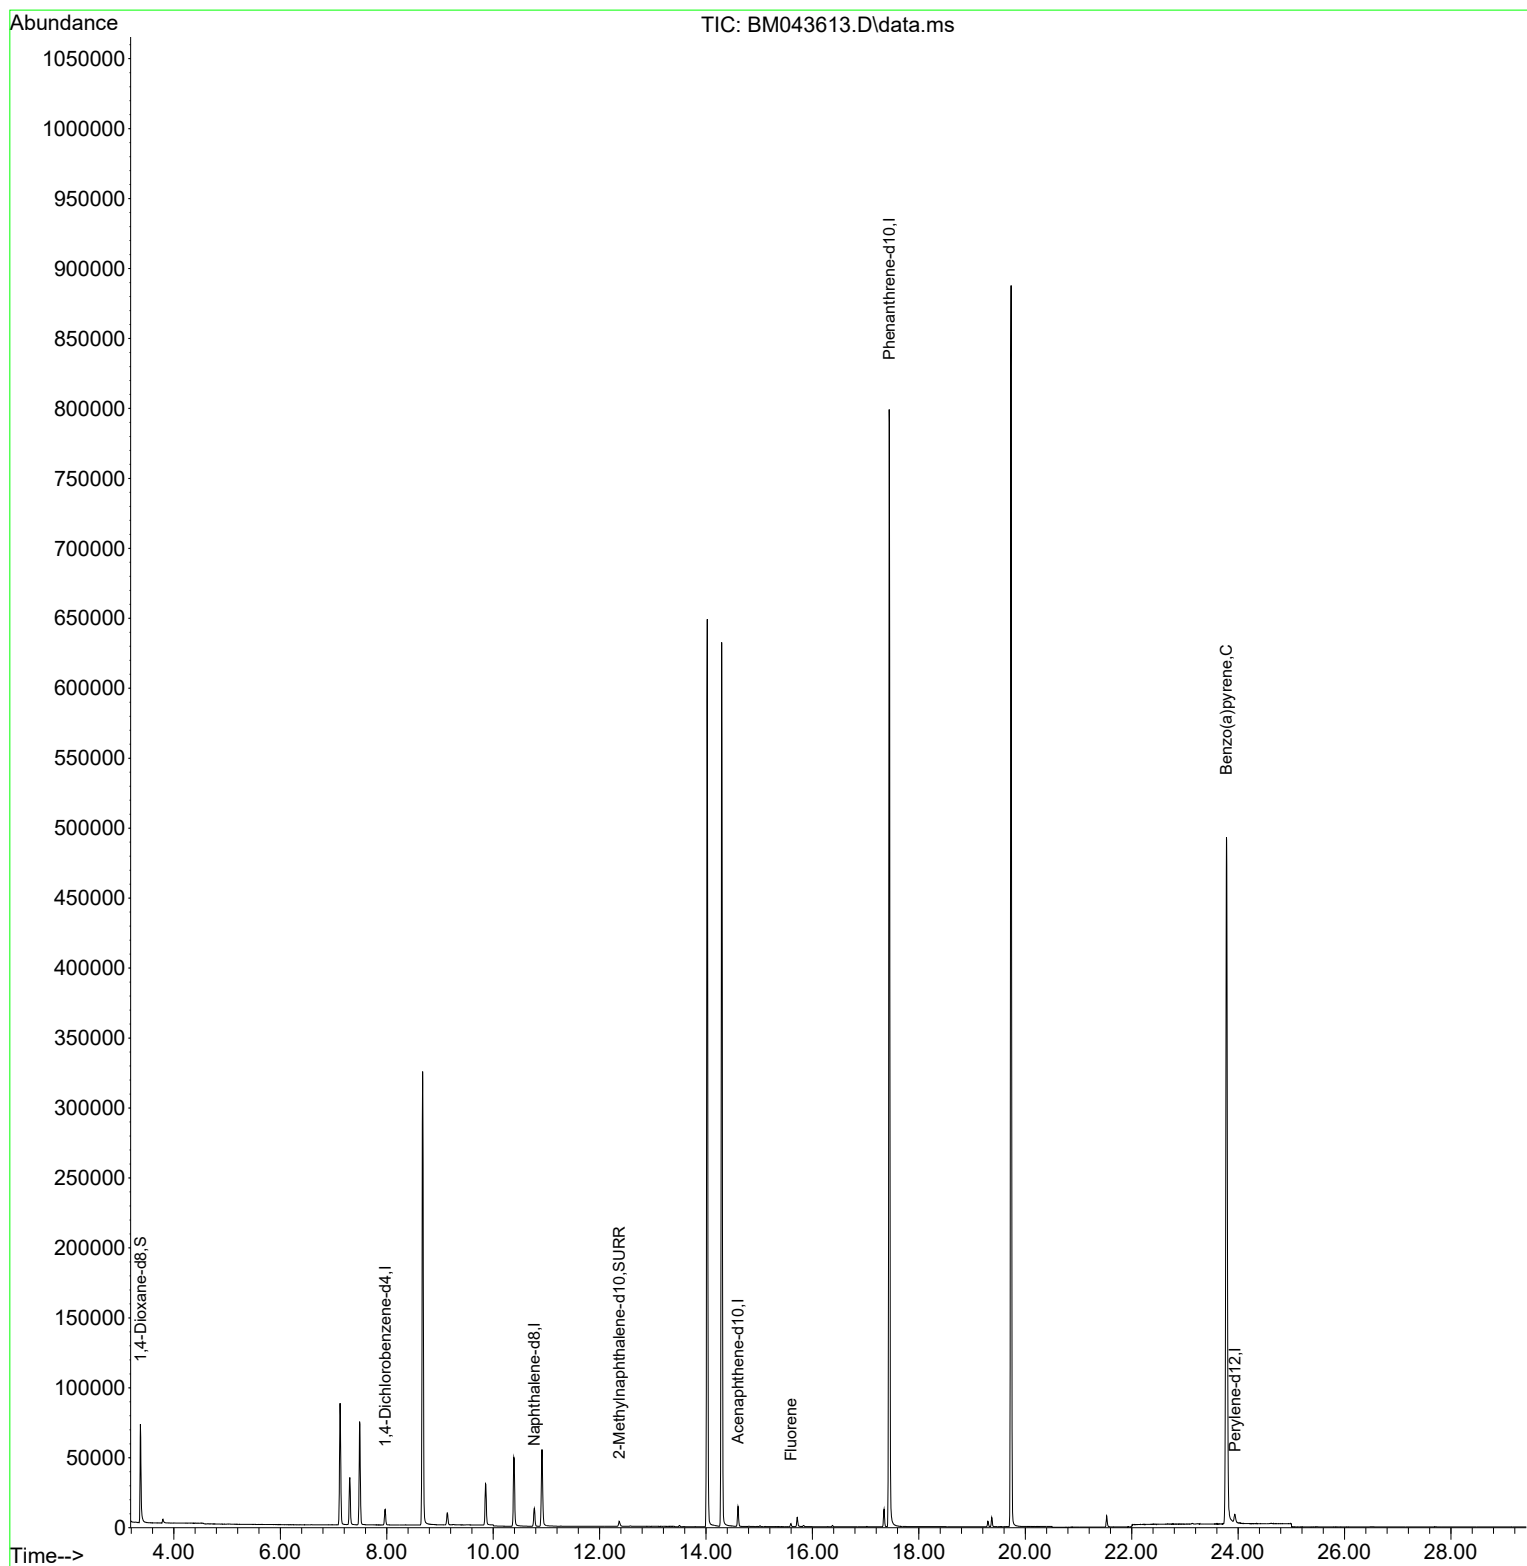

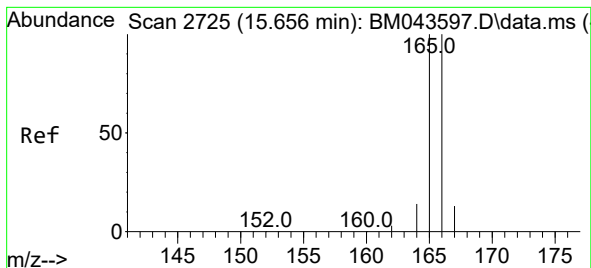

#12

Fluorene

Concen: 0.053 ng/ul

RT: 15.596 min Scan# 21

Delta R.T. -0.060 min

Lab File: BM043613.D

Acq: 27 Dec 2023 18:22

Instrument :

BNA_M

ClientSampleId :

SBLK067





Tgt Ion:166 Resp: 1820

Ion Ratio Lower Upper

166 100

165 11.7 80.3 120.5#

167 35.9 10.8 16.2#

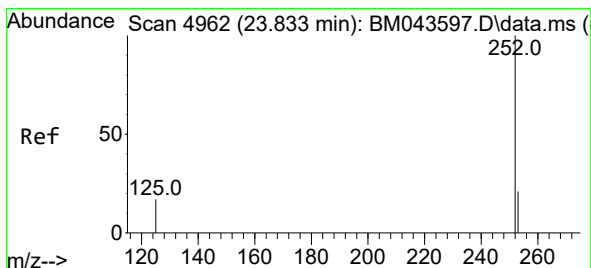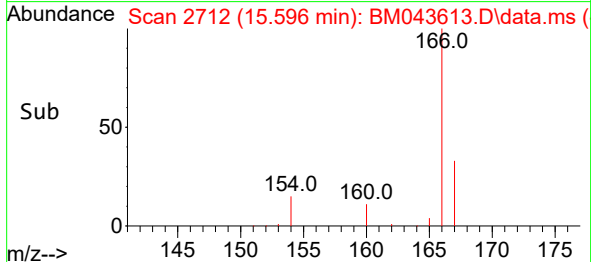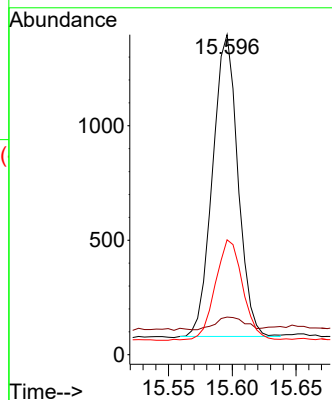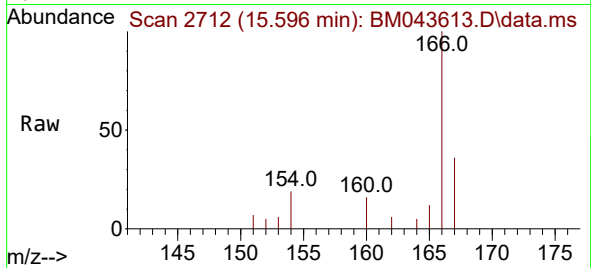

#26

Benzo(a)pyrene

Concen: 0.066 ng/ul

RT: 23.781 min Scan# 4944

Delta R.T. -0.053 min

Lab File: BM043613.D

Acq: 27 Dec 2023 18:22

Tgt Ion:252 Resp: 2960

Ion Ratio Lower Upper

252 100

253 50.7 20.2 30.2#

125 56.2 13.5 20.3#

