

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
 Data File : BM043616.D
 Acq On : 27 Dec 2023 20:11
 Operator : MA/JU
 Sample : 06020-12
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH7X7

Quant Time: Dec 27 21:43:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 26 22:58:31 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.971	152	5408	0.400	ng/ul	0.00
4) Naphthalene-d8	10.774	136	16486	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.601	164	7409	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.447	188	1399498	0.400	ng/ul	# 0.10
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.53
23) Perylene-d12	23.933	264	12611	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.372	96	34479	5.046	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.368	152	7751	0.332	ng/ul	0.00
18) Fluoranthene-d10	19.371	212	11345	0.000	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.410	88	563	0.082	ng/ul#	59
12) Fluorene	15.591	166	2907	0.086	ng/ul#	14
26) Benzo(a)pyrene	23.781	252	5116	0.108	ng/ul#	47


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
Data File : BM043616.D
Acq On : 27 Dec 2023 20:11
Operator : MA/JU
Sample : 06020-12
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH7X7

Quant Time: Dec 27 21:43:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 26 22:58:31 2023
Response via : Initial Calibration




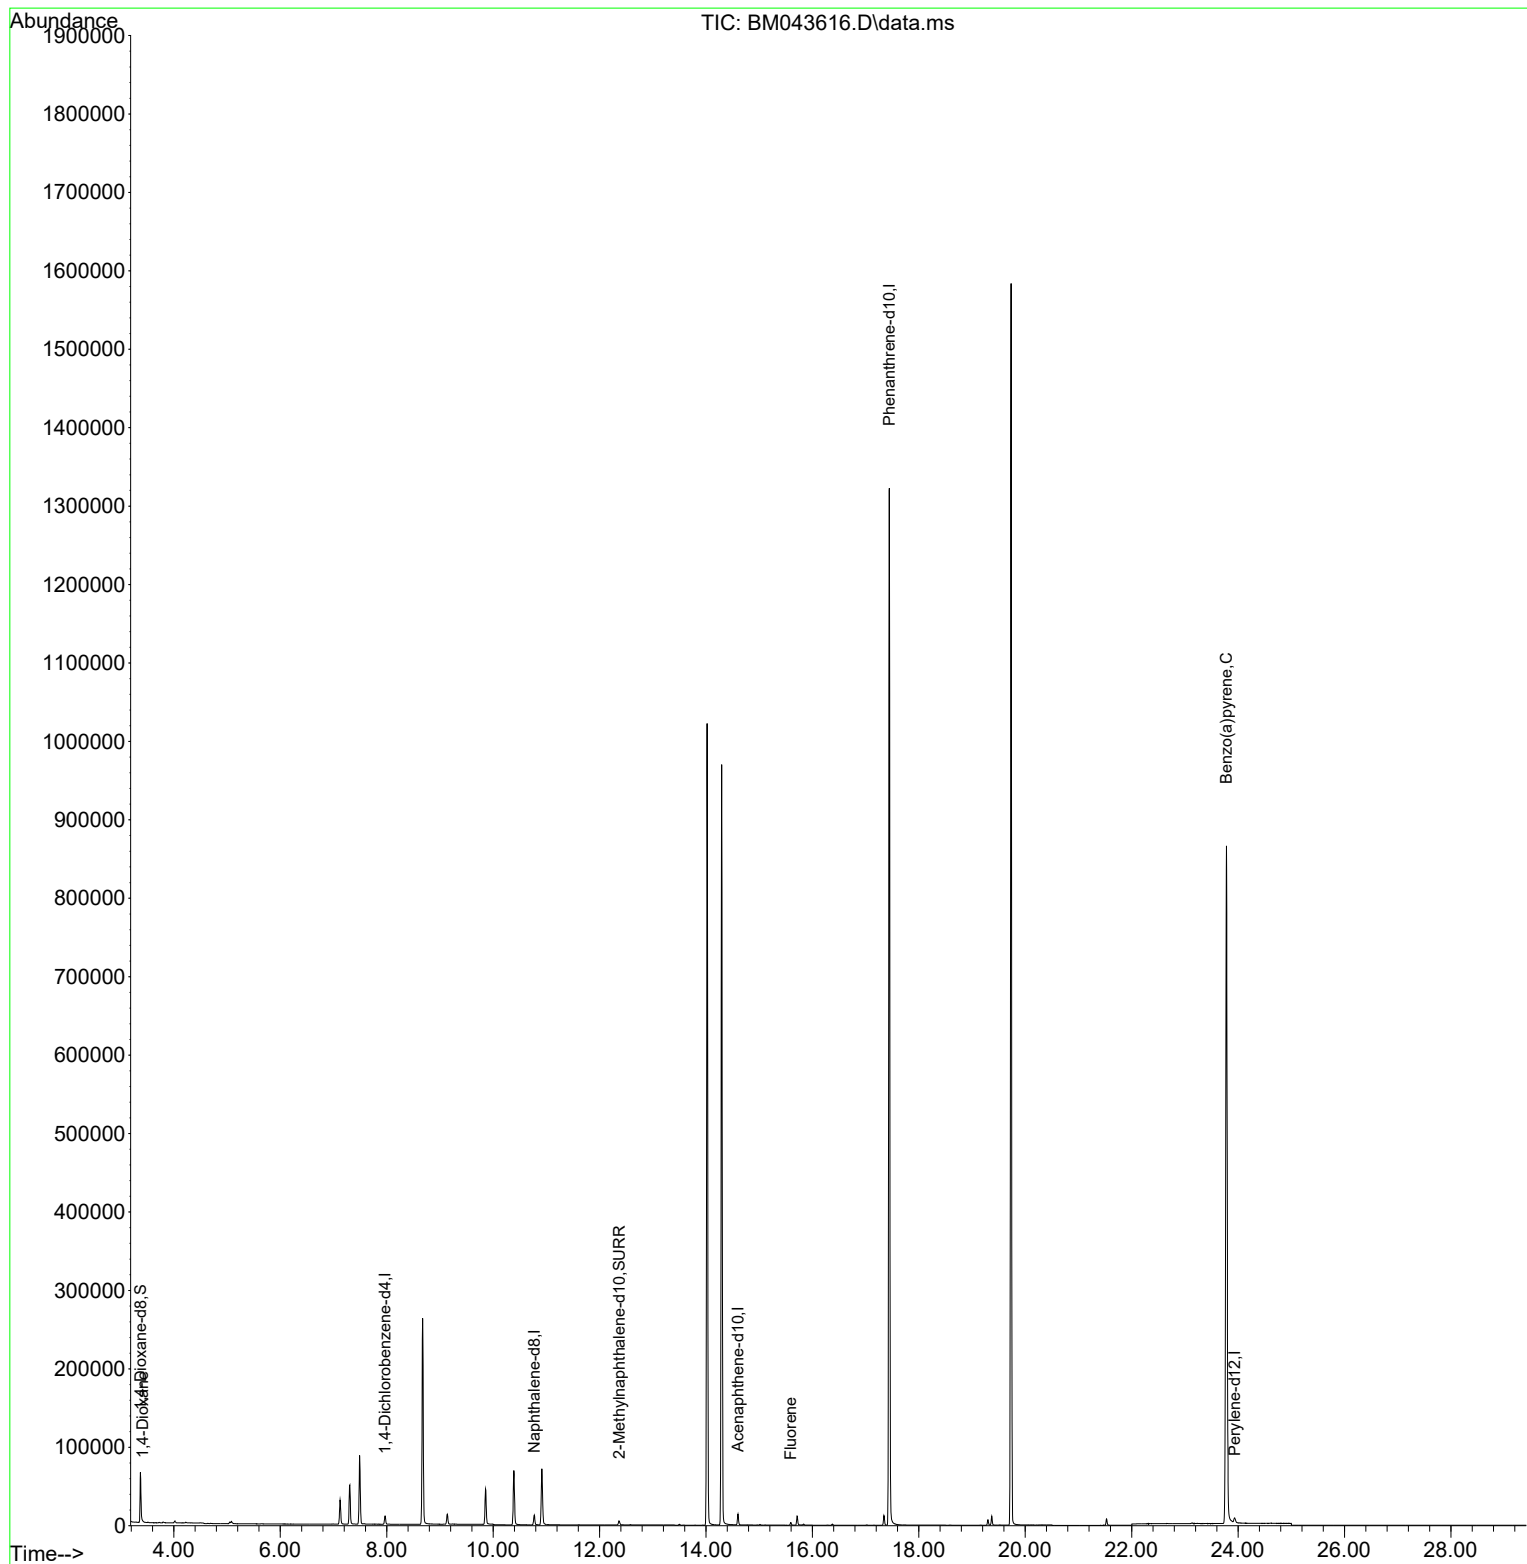


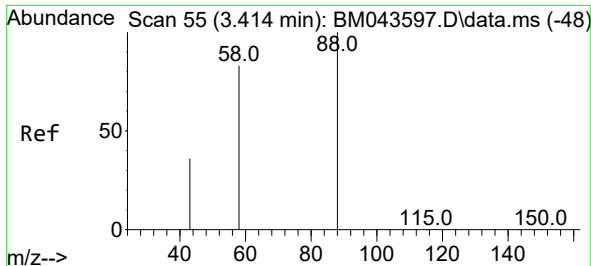

#2
1,4-Dioxane
Concen: 0.082 ng/ul
RT: 3.410 min Scan# 54
Delta R.T. -0.004 min
Lab File: BM043616.D
Acq: 27 Dec 2023 20:11




Instrument :
BNA_M
ClientSampleId :
BH7X7


Tgt Ion: 88 Resp: 563
Ion Ratio Lower Upper
88 100
43 55.9 27.9 41.9#
58 23.0 43.4 65.2#

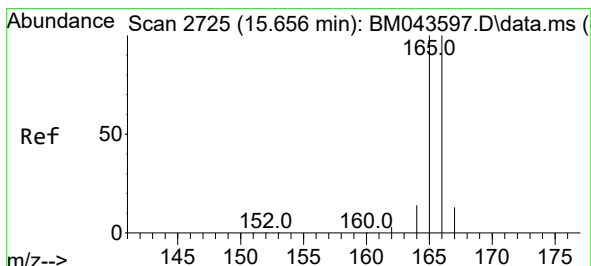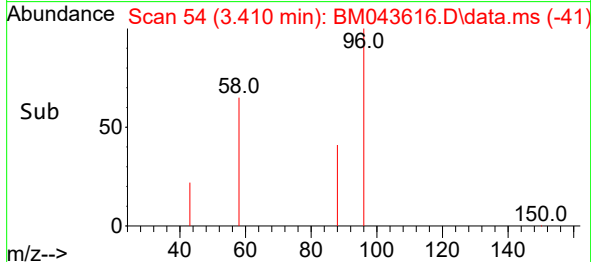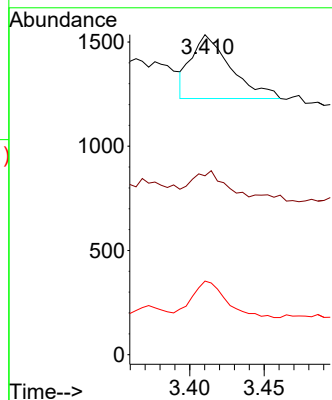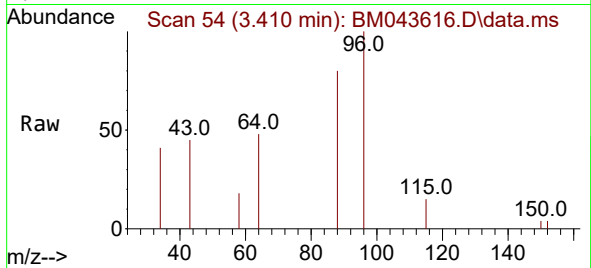

#12
Fluorene
Concen: 0.086 ng/ul
RT: 15.591 min Scan# 2711
Delta R.T. -0.065 min
Lab File: BM043616.D
Acq: 27 Dec 2023 20:11


Tgt Ion: 166 Resp: 2907
Ion Ratio Lower Upper
166 100
165 8.1 80.3 120.5#
167 30.9 10.8 16.2#

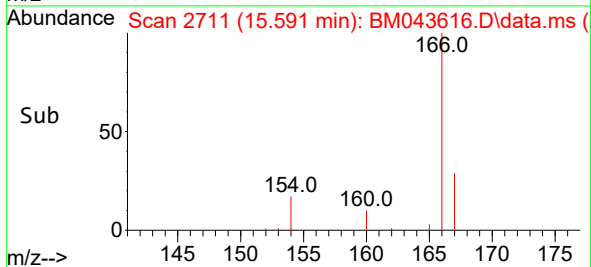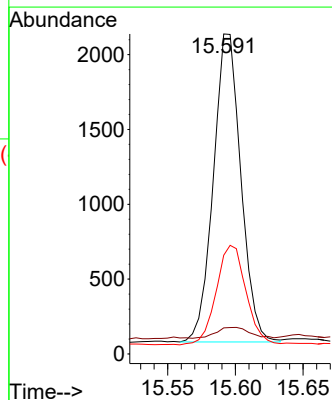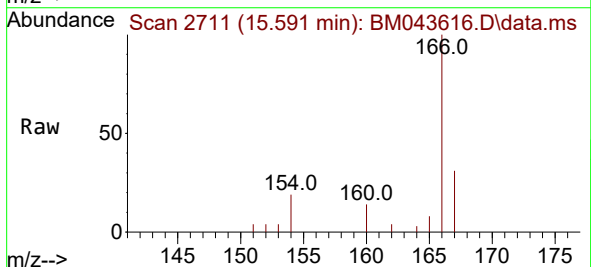

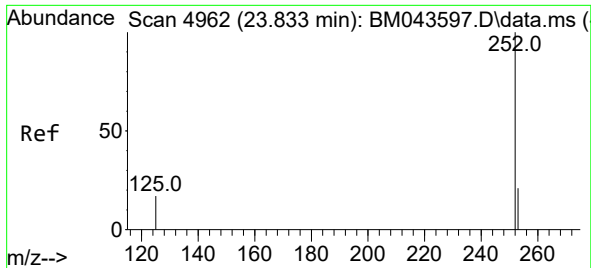

#26
 Benzo(a)pyrene
 Concen: 0.108 ng/ul
 RT: 23.781 min Scan# 4962
 Delta R.T. -0.052 min
 Lab File: BM043616.D
 Acq: 27 Dec 2023 20:11

Instrument :
 BNA_M
 ClientSampleId :
 BH7X7

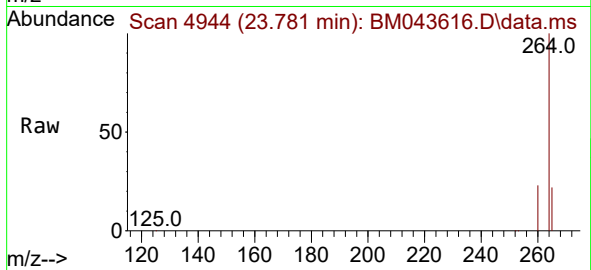

Tgt Ion:252 Resp: 5116
 Ion Ratio Lower Upper
 252 100
 253 45.7 20.2 30.2#
 125 47.9 13.5 20.3#

