




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
 Data File : BM043568.D
 Acq On : 26 Dec 2023 12:04
 Operator : MA/JU
 Sample : 05927-12
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3P3

Manual IntegrationsAPPROVED

Quant Time: Dec 26 12:52:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 19 23:32:46 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/28/2023
 Supervised By :mohammad ahmed 12/29/2023

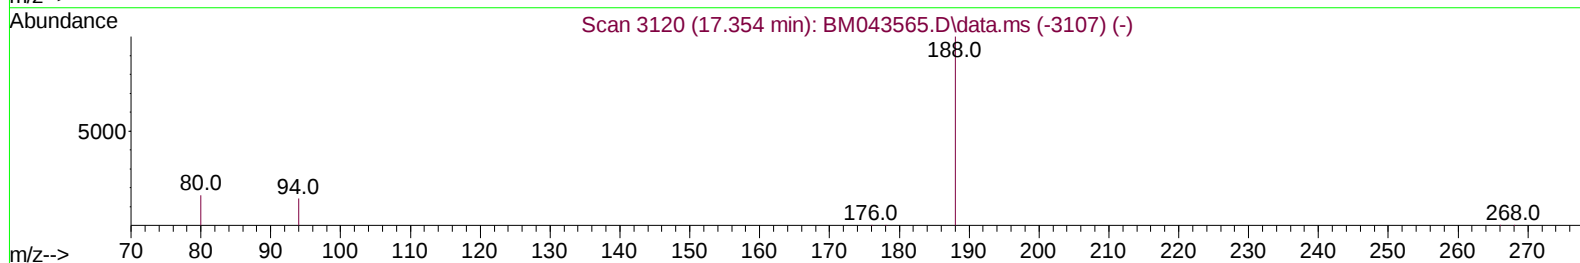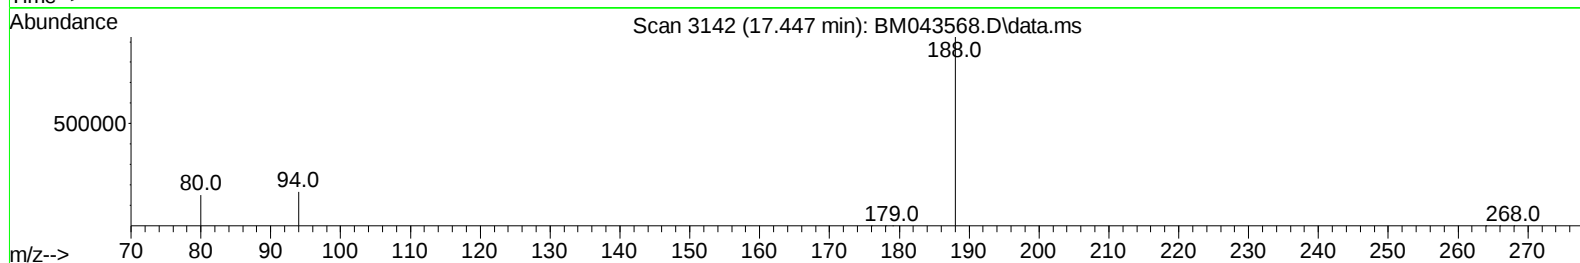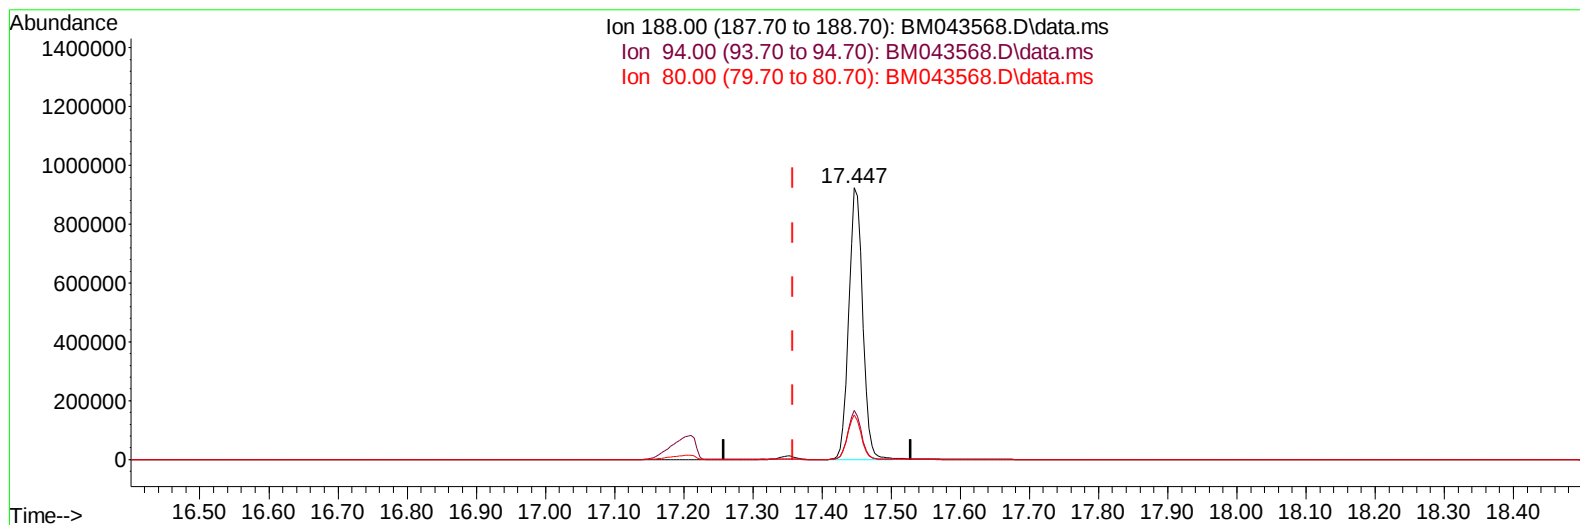

TIC: BM043568.D\data.ms

(13) Phenanthrene-d10 (I)

17.447min (+ 0.089) 0.40 ng/u1

response 1277242

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.30	18.07#
80.00	13.20	16.36#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
Data File : BM043568.D
Acq On : 26 Dec 2023 12:04
Operator : MA/JU
Sample : 05927-12
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3P3

Manual IntegrationsAPPROVED

Quant Time: Dec 26 12:52:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 19 23:32:46 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/28/2023
Supervised By :mohammad ahmed 12/29/2023

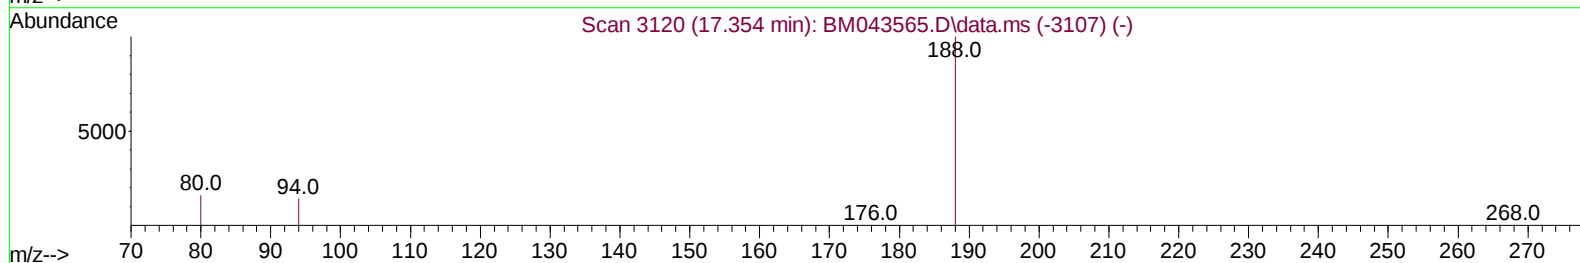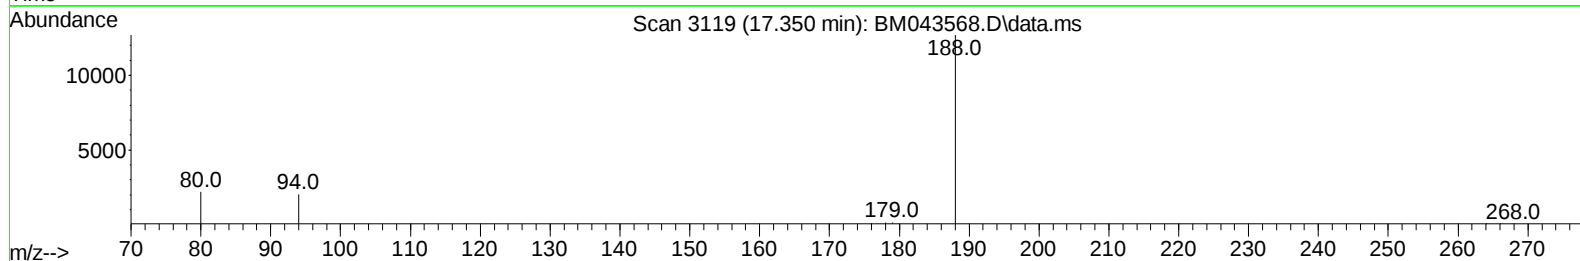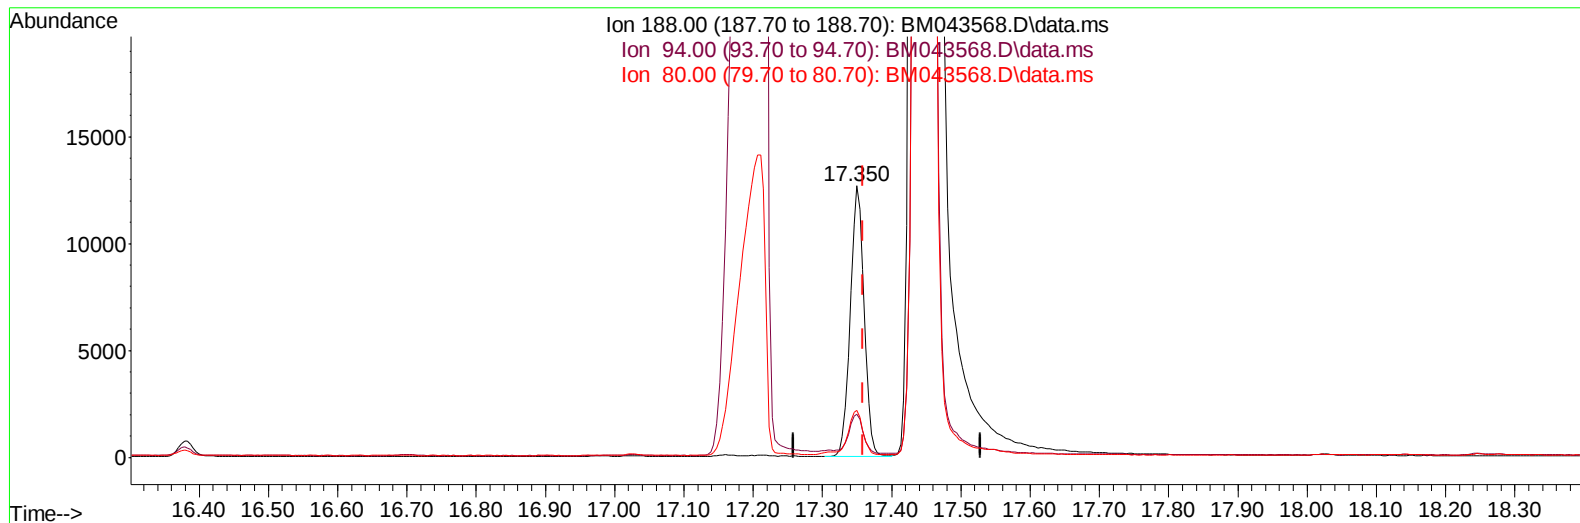

TIC: BM043568.D\data.ms

(13) Phenanthrene-d10 (I)

17.350min (-0.008) 0.40 ng/u1 m

response 17581

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.30	16.01#
80.00	13.20	17.31#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
 Data File : BM043568.D
 Acq On : 26 Dec 2023 12:04
 Operator : MA/JU
 Sample : 05927-12
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3P3

Manual IntegrationsAPPROVED

Quant Time: Dec 26 12:52:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 19 23:32:46 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/28/2023
 Supervised By :mohammad ahmed 12/29/2023

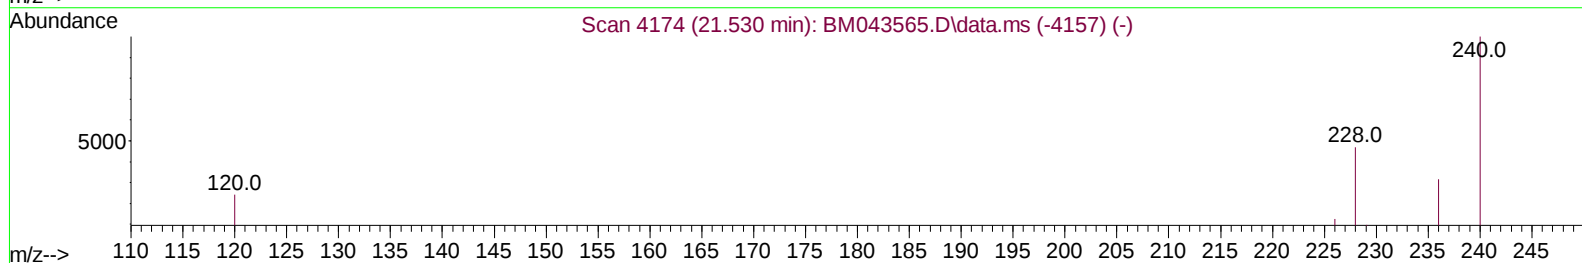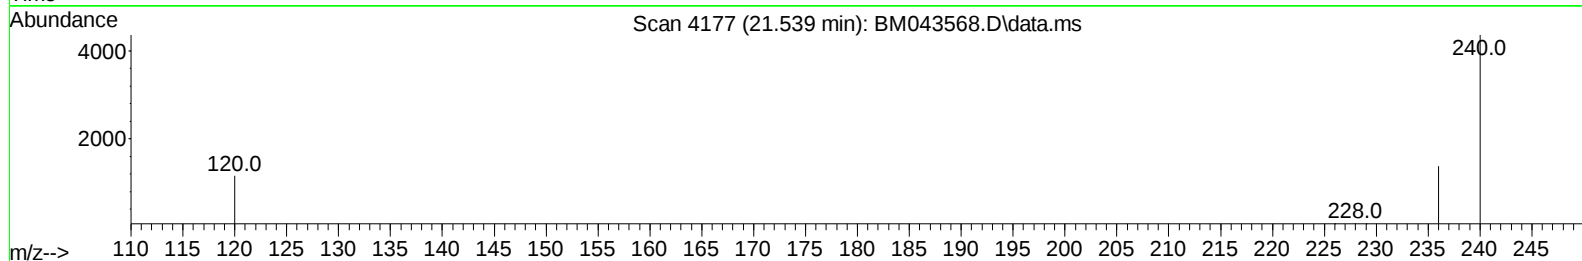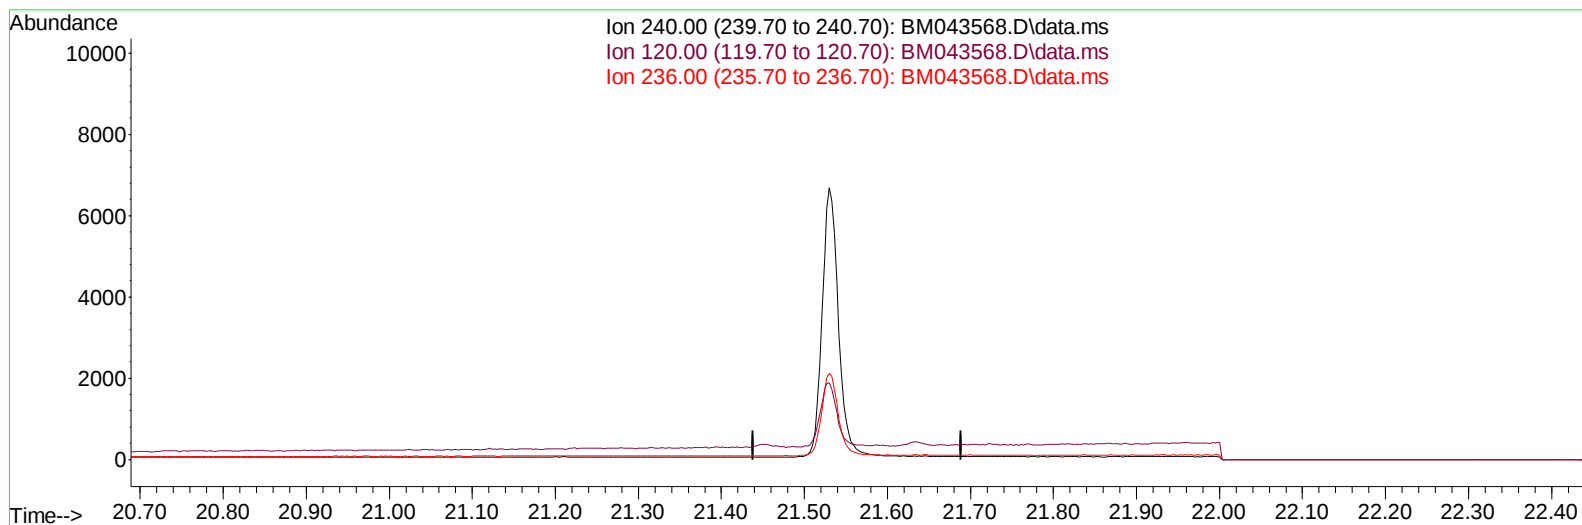

TIC: BM043568.D\data.ms

(17) Chrysene-d12

21.539min (-21.539) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	20.60	0.00#
236.00	31.10	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
 Data File : BM043568.D
 Acq On : 26 Dec 2023 12:04
 Operator : MA/JU
 Sample : 05927-12
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3P3

Manual IntegrationsAPPROVED

Quant Time: Dec 26 12:52:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 19 23:32:46 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/28/2023
 Supervised By :mohammad ahmed 12/29/2023

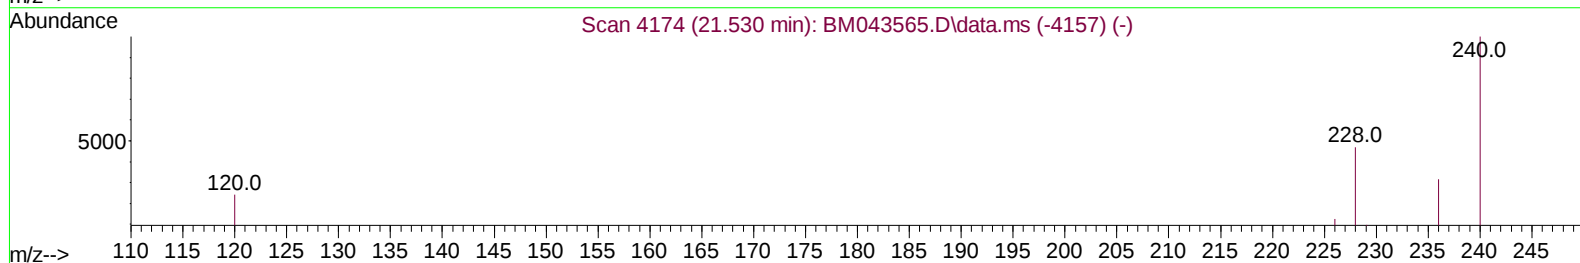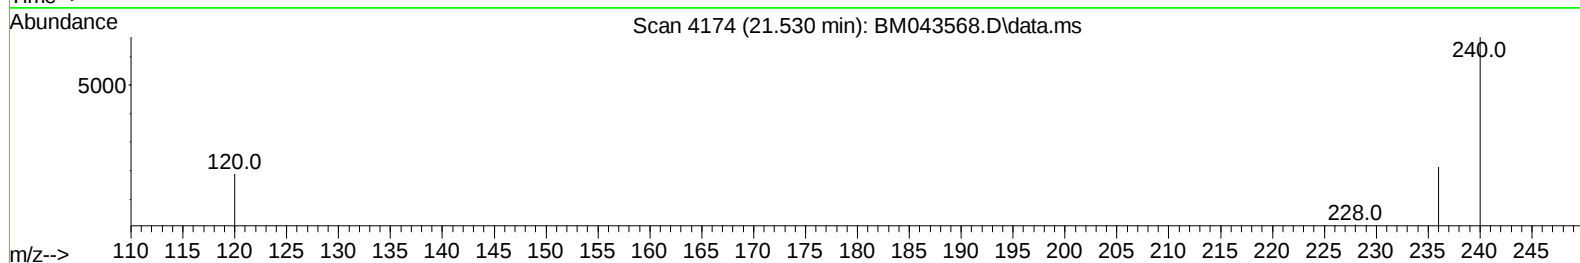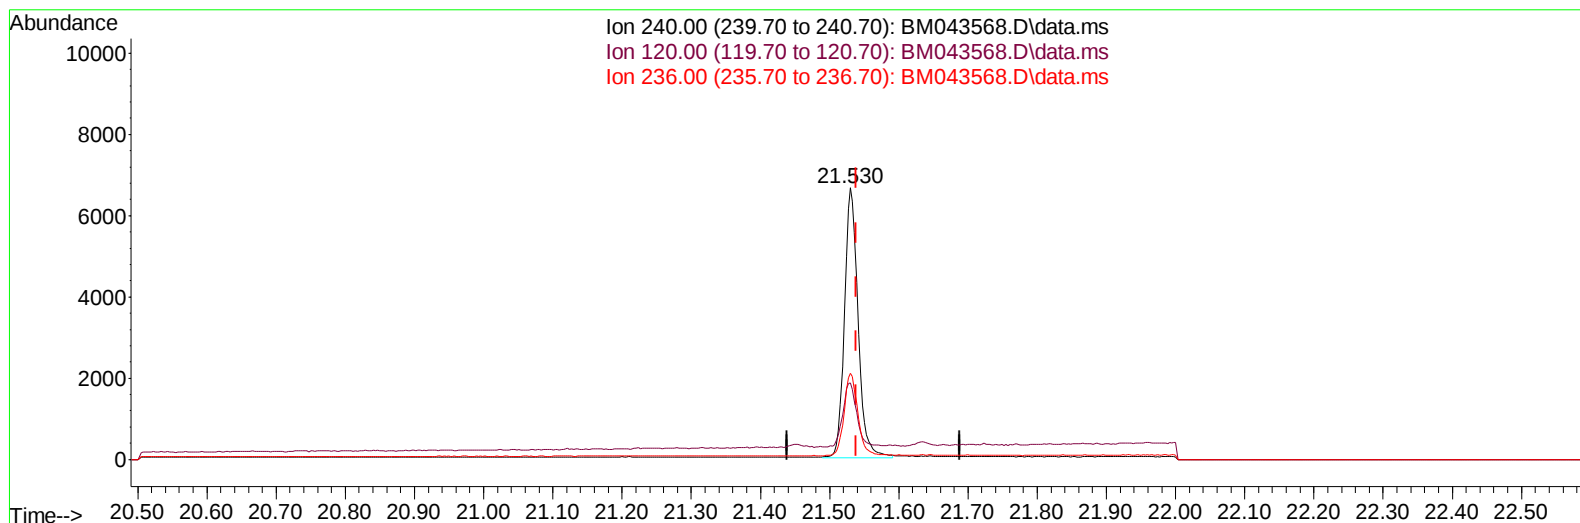

TIC: BM043568.D\data.ms

(17) Chrysene-d12

21.530min (-0.009) 0.40 ng/ul m

response 9151

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	20.60	28.20#
236.00	31.10	31.79
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
Data File : BM043568.D
Acq On : 26 Dec 2023 12:04
Operator : MA/JU
Sample : 05927-12
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3P3

Manual IntegrationsAPPROVED

Quant Time: Dec 26 12:52:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 19 23:32:46 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/28/2023
Supervised By :mohammad ahmed 12/29/2023

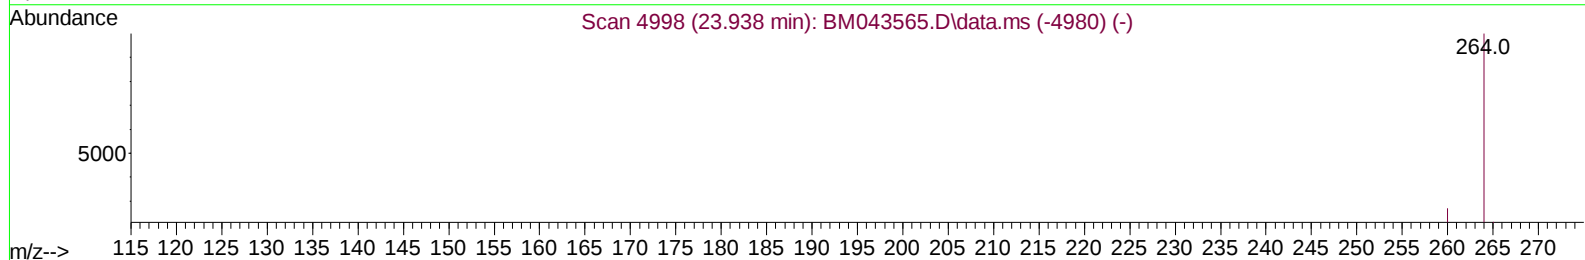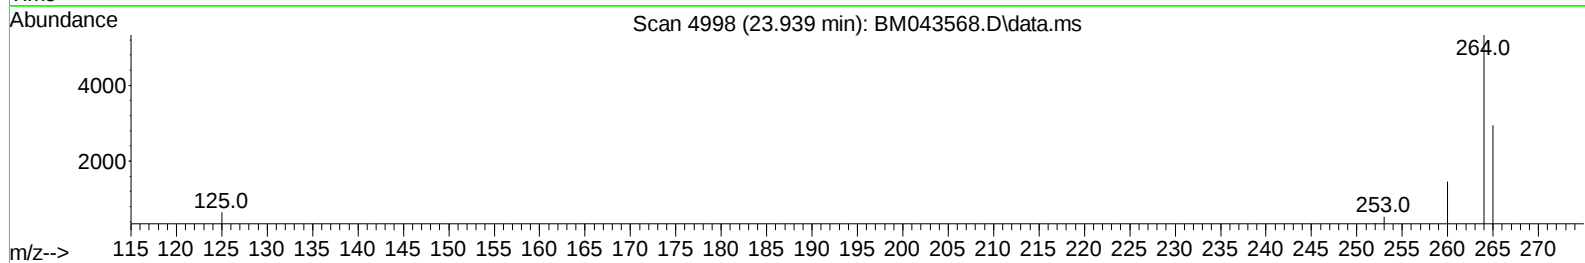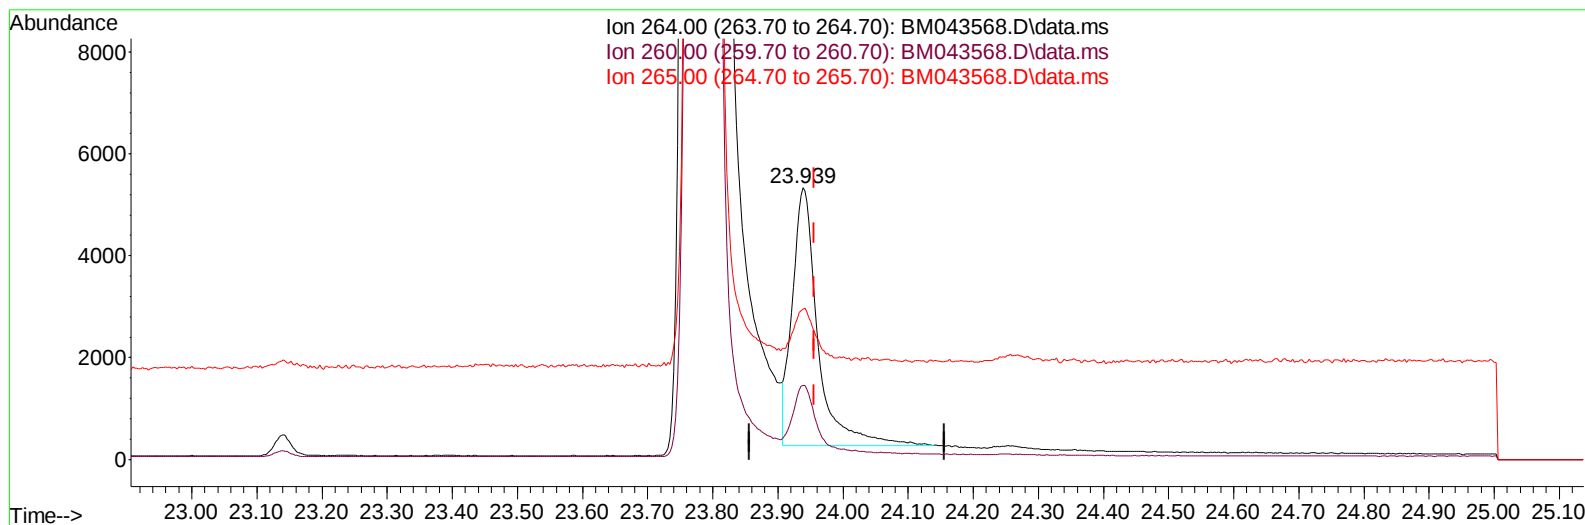

TIC: BM043568.D\data.ms

(23) Perylene-d12 (I)

23.939min (-0.017) 0.40 ng/u1

response 13877

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	28.30	27.33
265.00	39.10	55.34#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
 Data File : BM043568.D
 Acq On : 26 Dec 2023 12:04
 Operator : MA/JU
 Sample : 05927-12
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3P3

Manual IntegrationsAPPROVED

Quant Time: Dec 26 12:52:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 19 23:32:46 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/28/2023
 Supervised By :mohammad ahmed 12/29/2023

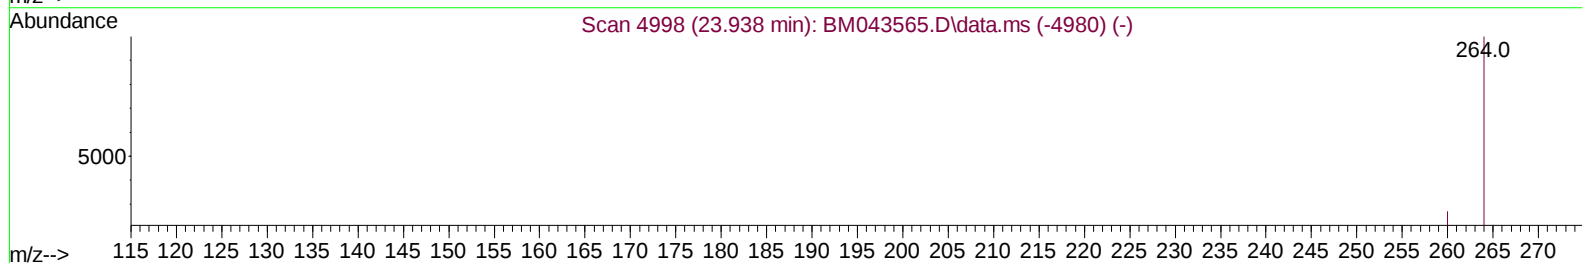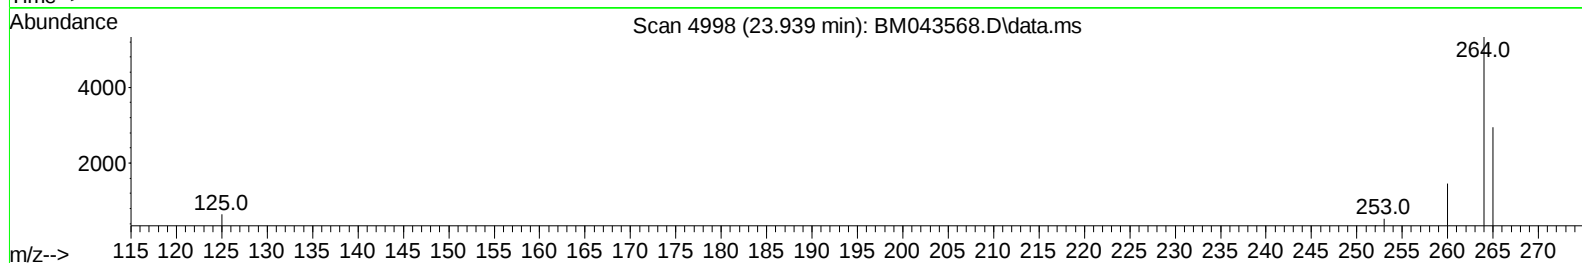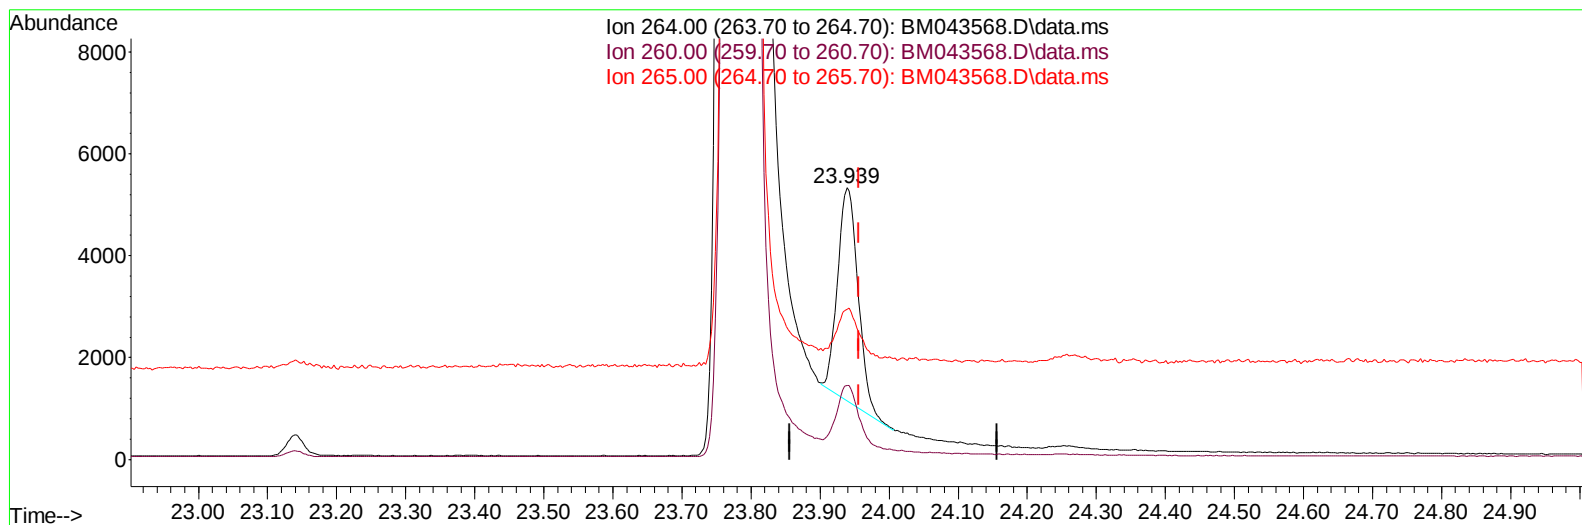

TIC: BM043568.D\data.ms

(23) Perylene-d12 (I)

23.939min (-0.017) 0.40 ng/ul m

response 8582

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	28.30	27.33
265.00	39.10	55.34#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
 Data File : BM043568.D
 Acq On : 26 Dec 2023 12:04
 Operator : MA/JU
 Sample : 05927-12
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3P3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/28/2023
 Supervised By :mohammad ahmed 12/29/2023

Quant Time: Dec 26 12:52:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 19 23:32:46 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.971	152		6688	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.779	136		19658	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.606	164		8778	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.350	188		17581m	0.400	ng/ul	0.00
17) Chrysene-d12	21.530	240		9151m	0.400	ng/ul	0.00
23) Perylene-d12	23.939	264		8582m	0.400	ng/ul	-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.377	96		33181	3.927	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.368	152		6738	0.242	ng/ul	-0.01
18) Fluoranthene-d10	19.371	212		10715	0.328	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.414	88		631	0.074	ng/ul#	69

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
Data File : BM043568.D
Acq On : 26 Dec 2023 12:04
Operator : MA/JU
Sample : 05927-12
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH3P3

Manual IntegrationsAPPROVED

Quant Time: Dec 26 12:52:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 19 23:32:46 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/28/2023
Supervised By :mohammad ahmed 12/29/2023

