




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
 Data File : BM043575.D
 Acq On : 26 Dec 2023 16:19
 Operator : MA/JU
 Sample : 05976-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH7W2

Manual IntegrationsAPPROVED

Quant Time: Dec 26 18:03:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 19 23:32:46 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/28/2023
 Supervised By :mohammad ahmed 12/29/2023

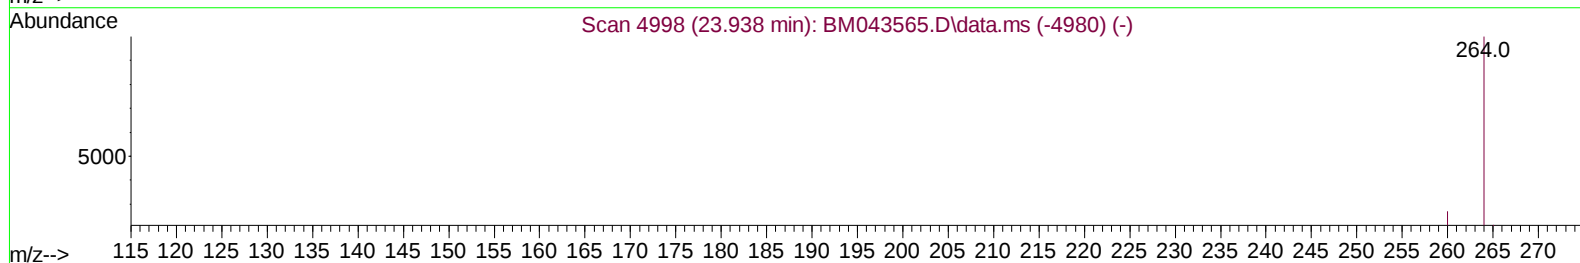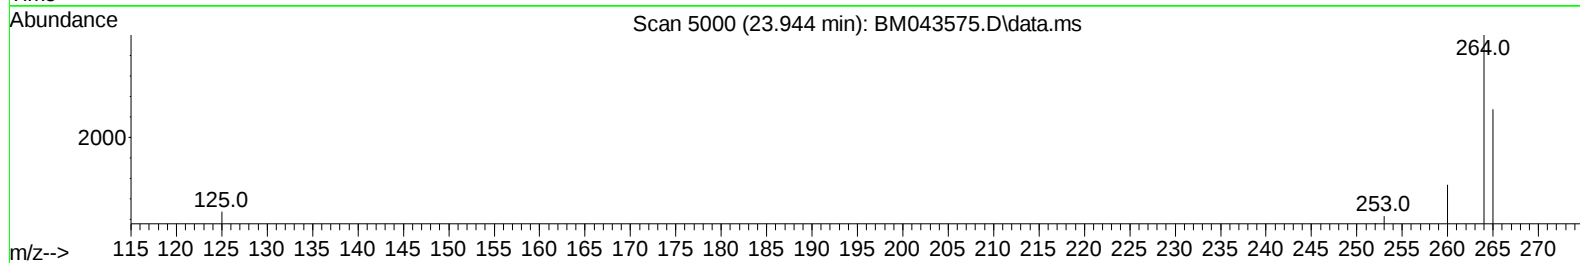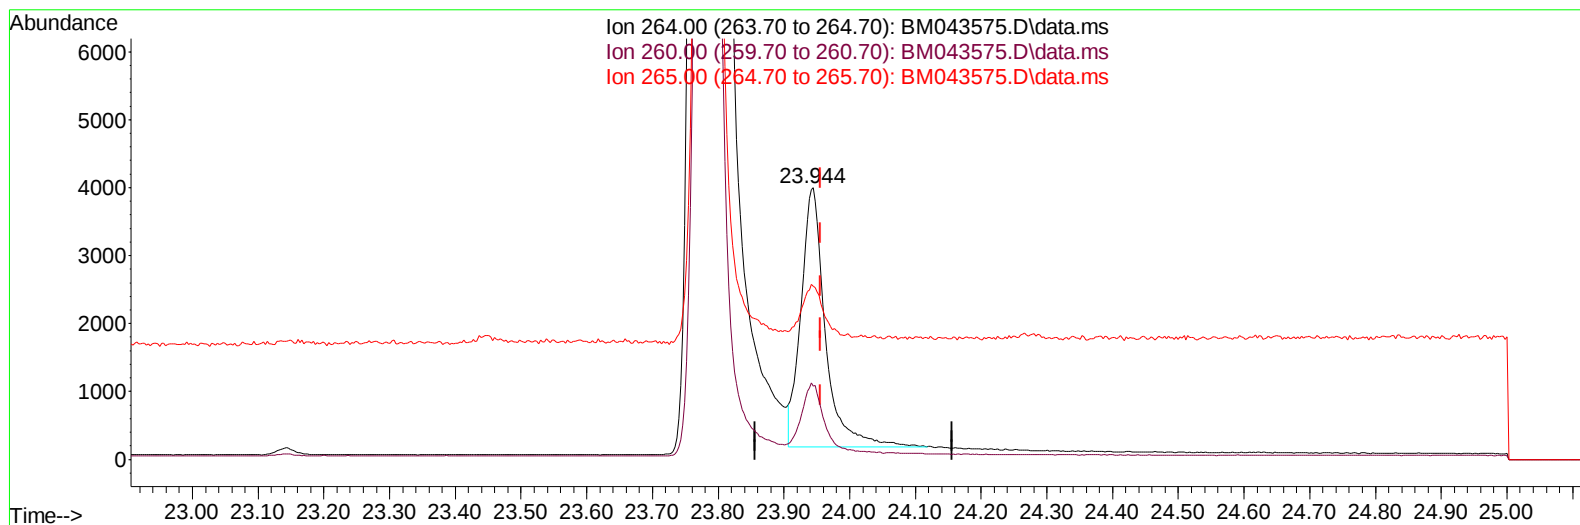

TIC: BM043575.D\data.ms

(23) Perylene-d12 (I)

23.944min (-0.012) 0.40 ng/u1

response 9926

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	28.30	27.03
265.00	39.10	63.74#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
 Data File : BM043575.D
 Acq On : 26 Dec 2023 16:19
 Operator : MA/JU
 Sample : 05976-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH7W2

Manual IntegrationsAPPROVED

Quant Time: Dec 26 18:03:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 19 23:32:46 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/28/2023
 Supervised By :mohammad ahmed 12/29/2023

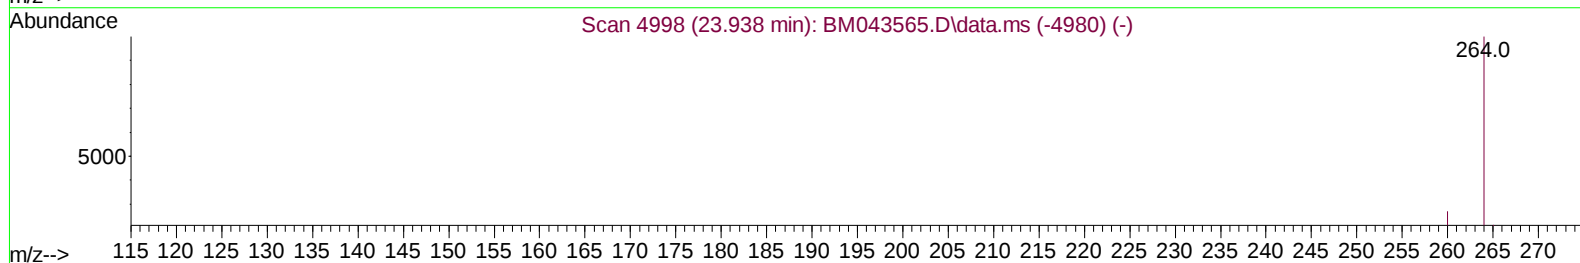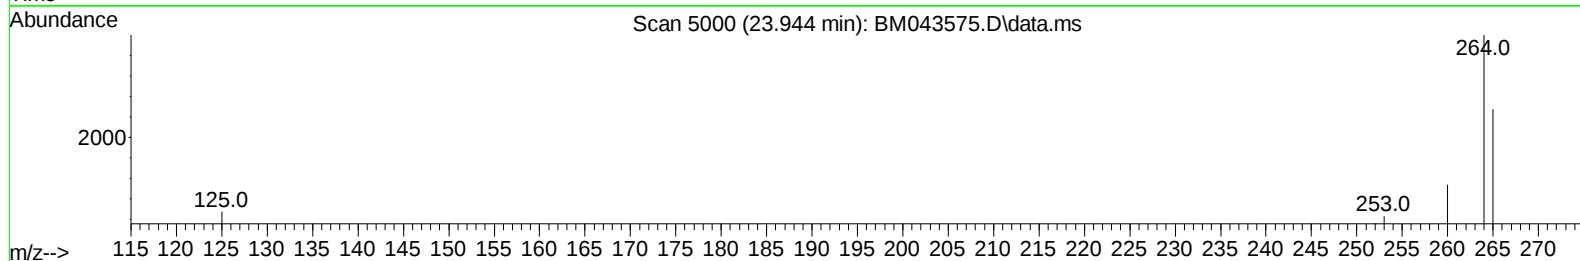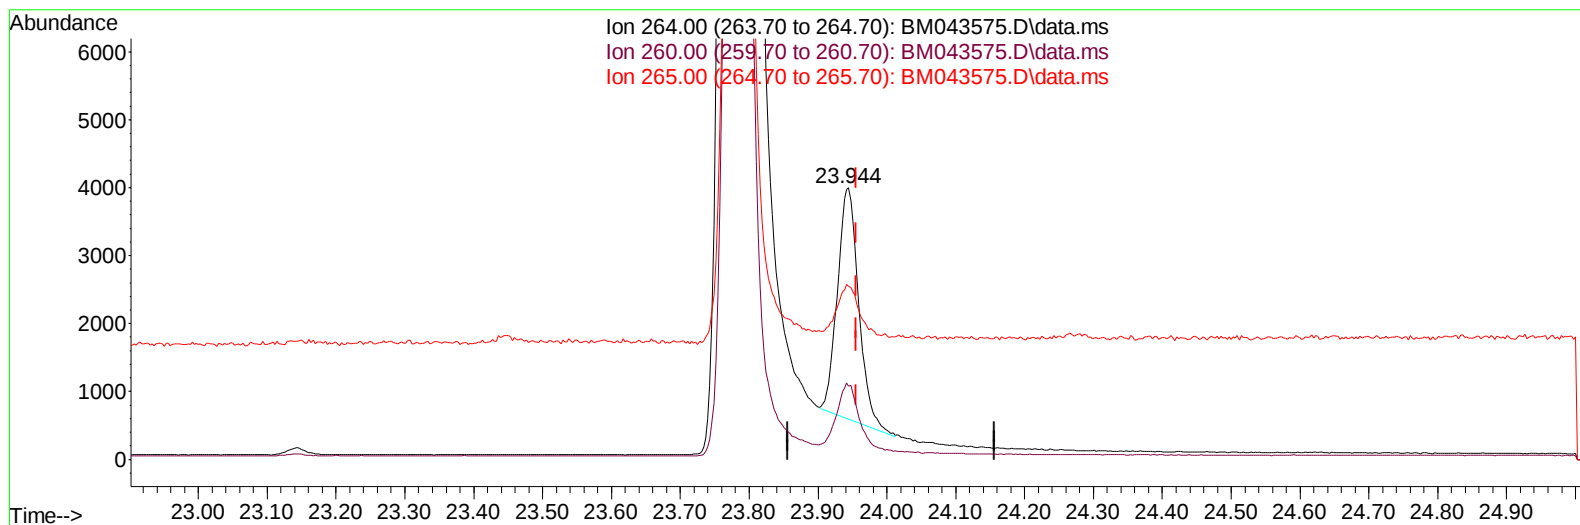

TIC: BM043575.D\data.ms

(23) Perylene-d12 (I)

23.944min (-0.012) 0.40 ng/ul m

response 7274

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	28.30	27.03
265.00	39.10	63.74#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
 Data File : BM043575.D
 Acq On : 26 Dec 2023 16:19
 Operator : MA/JU
 Sample : 05976-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH7W2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/28/2023
 Supervised By :mohammad ahmed 12/29/2023

Quant Time: Dec 26 18:03:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 19 23:32:46 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.975	152	5139	0.400	ng/ul	0.00
4) Naphthalene-d8	10.779	136	15279	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.606	164	6851	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.350	188	12854	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.533	240	7283	0.400	ng/ul	# 0.00
23) Perylene-d12	23.944	264	7274m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.377	96	24434	3.763	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.379	152	1964	0.091	ng/ul	0.00
18) Fluoranthene-d10	19.376	212	2521	0.097	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
Data File : BM043575.D
Acq On : 26 Dec 2023 16:19
Operator : MA/JU
Sample : 05976-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH7W2

Manual IntegrationsAPPROVED

Quant Time: Dec 26 18:03:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 19 23:32:46 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/28/2023
Supervised By :mohammad ahmed 12/29/2023

