




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
 Data File : BM043592.D
 Acq On : 27 Dec 2023 03:10
 Operator : MA/JU
 Sample : 06021-13
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH7Z5

Manual IntegrationsAPPROVED

Quant Time: Dec 27 03:43:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 26 22:58:31 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/28/2023
 Supervised By :mohammad ahmed 12/29/2023

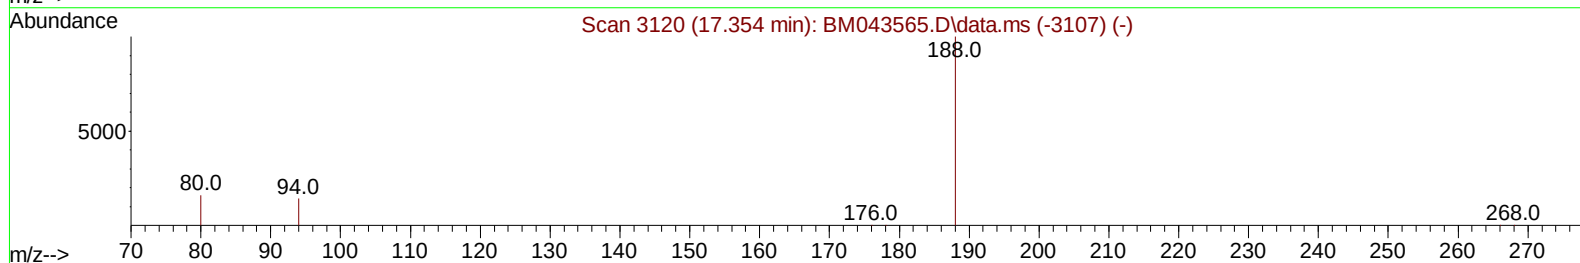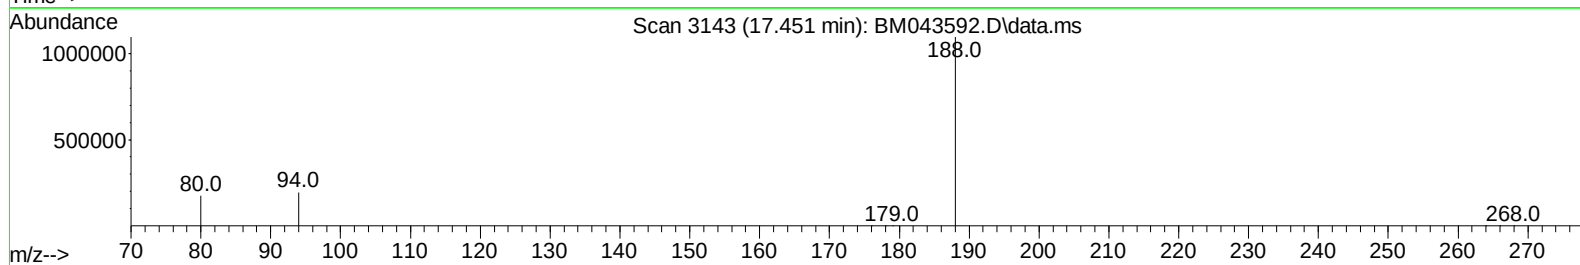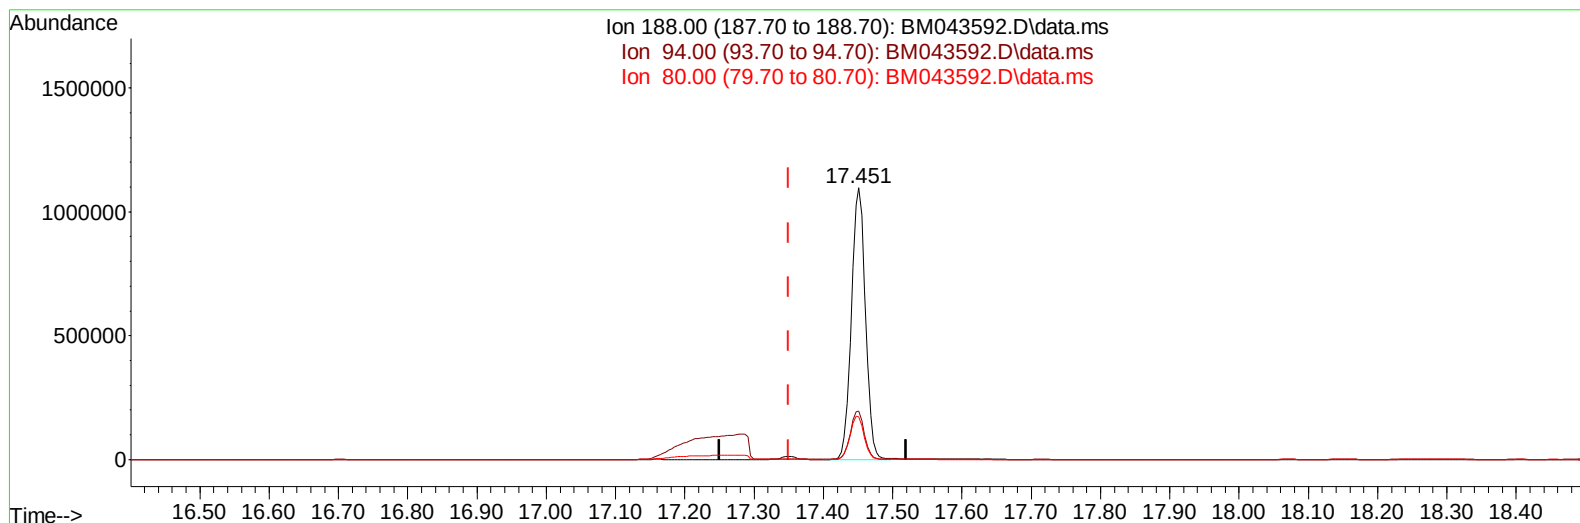

TIC: BM043592.D\data.ms

(13) Phenanthrene-d10 (I)

17.451min (+ 0.101) 0.40 ng/u1

response 1544518

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.30	17.73#
80.00	13.20	15.81
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
Data File : BM043592.D
Acq On : 27 Dec 2023 03:10
Operator : MA/JU
Sample : 06021-13
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH7Z5

Manual IntegrationsAPPROVED

Quant Time: Dec 27 03:43:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 26 22:58:31 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/28/2023
Supervised By :mohammad ahmed 12/29/2023

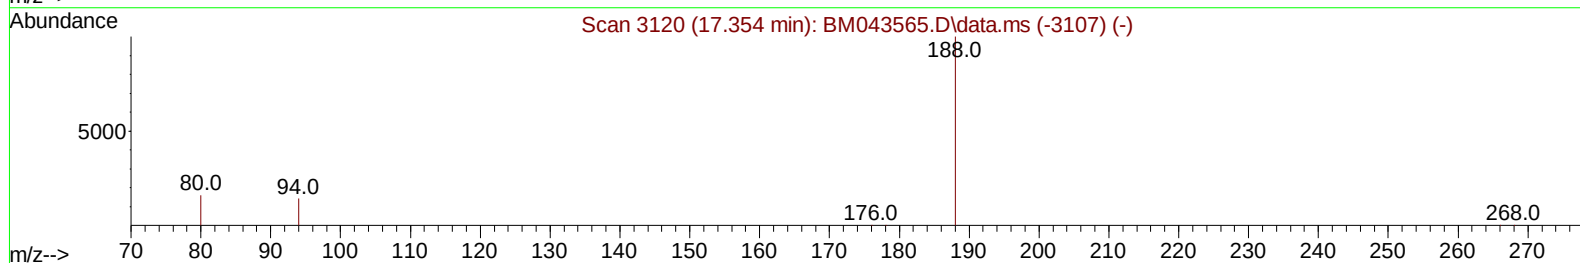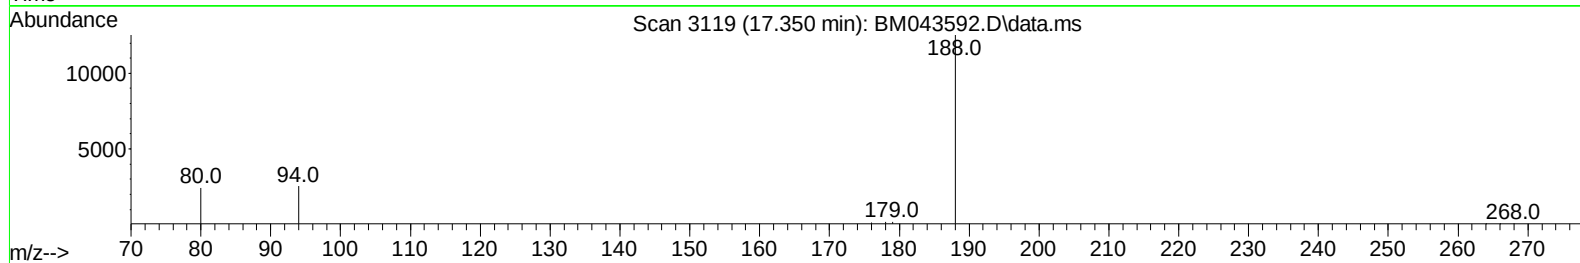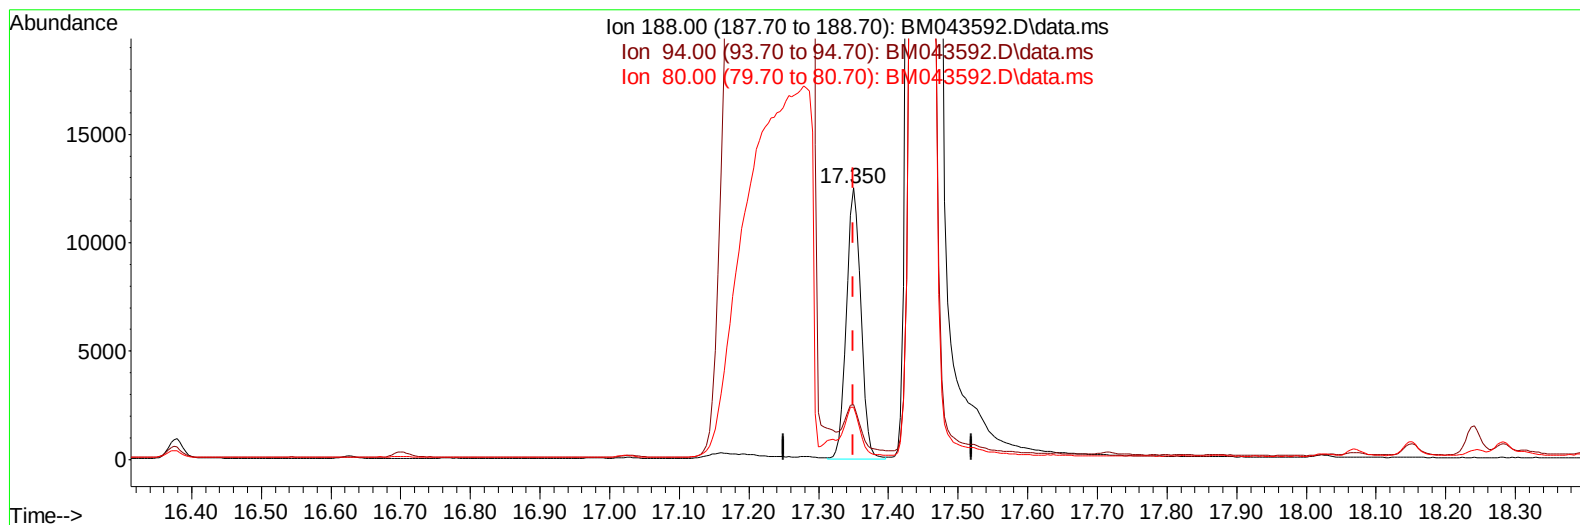

TIC: BM043592.D\data.ms

(13) Phenanthrene-d10 (I)

17.350min (+ 0.000) 0.40 ng/ul m

response 18036

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	12.30	20.18#
80.00	13.20	19.20#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
Data File : BM043592.D
Acq On : 27 Dec 2023 03:10
Operator : MA/JU
Sample : 06021-13
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH7Z5

Manual IntegrationsAPPROVED

Quant Time: Dec 27 03:43:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 26 22:58:31 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/28/2023
Supervised By :mohammad ahmed 12/29/2023

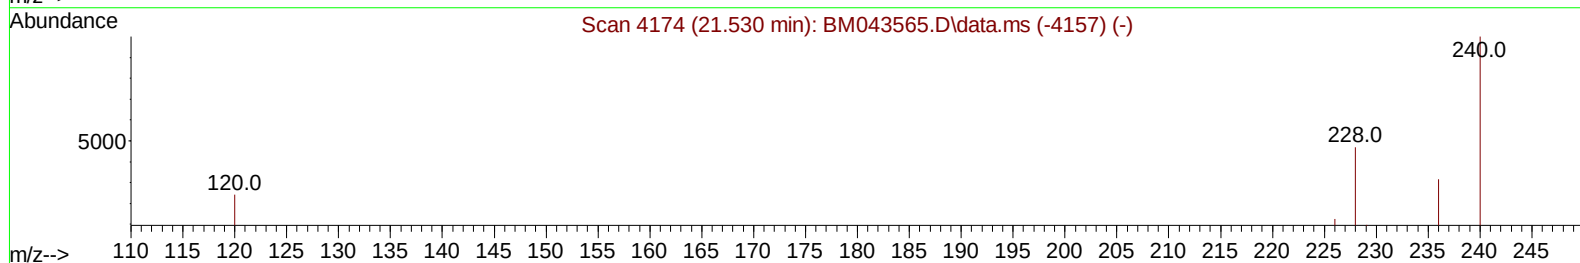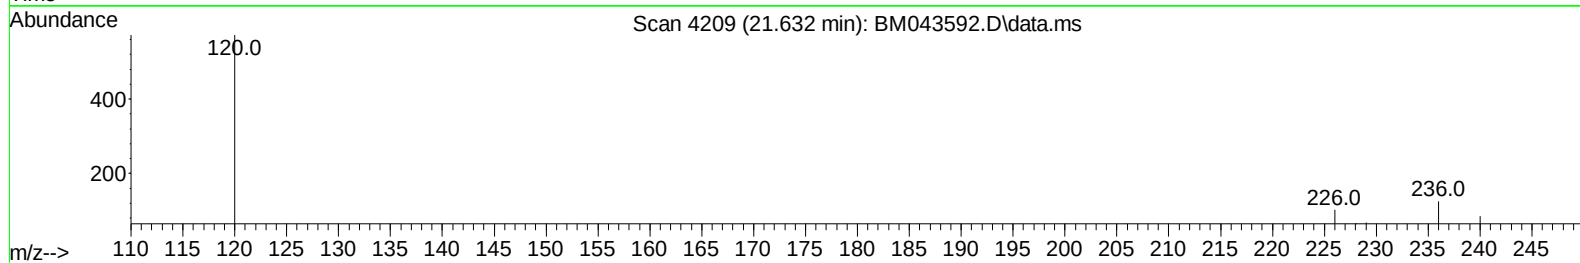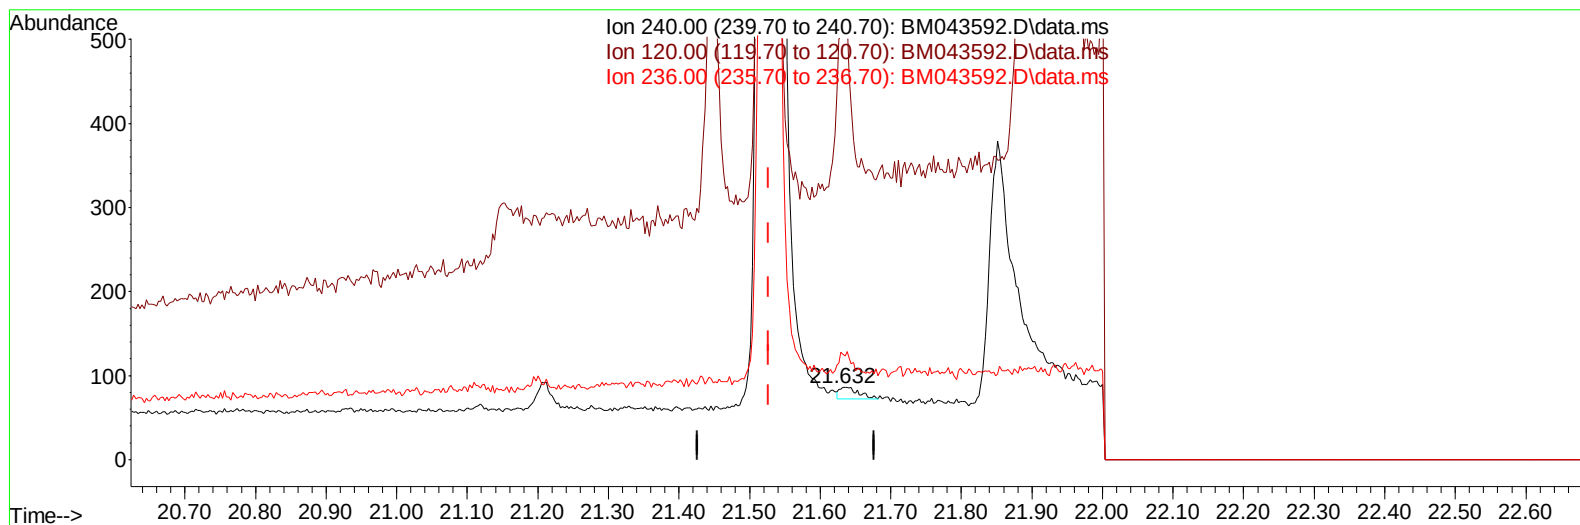

TIC: BM043592.D\data.ms

(17) Chrysene-d12

21.632min (+ 0.105) 0.40 ng/u1

response 27

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	20.60	665.12#
236.00	31.10	146.51#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
 Data File : BM043592.D
 Acq On : 27 Dec 2023 03:10
 Operator : MA/JU
 Sample : 06021-13
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH7Z5

Manual IntegrationsAPPROVED

Quant Time: Dec 27 03:43:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 26 22:58:31 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/28/2023
 Supervised By :mohammad ahmed 12/29/2023

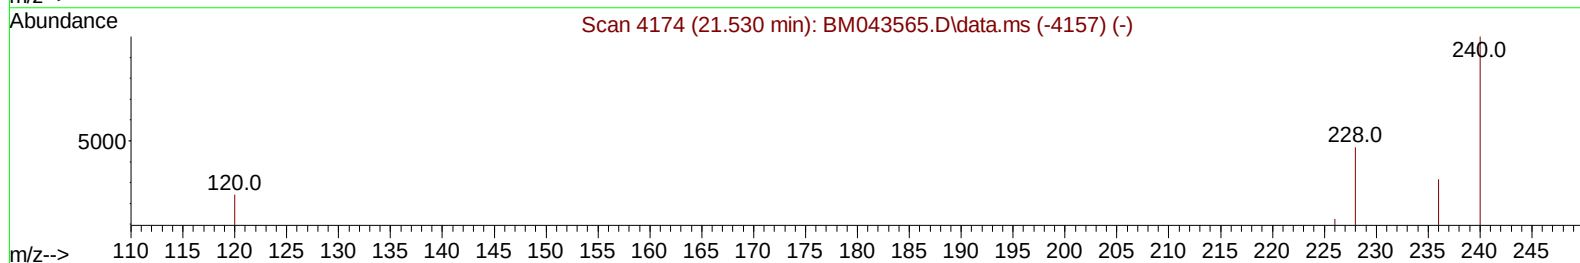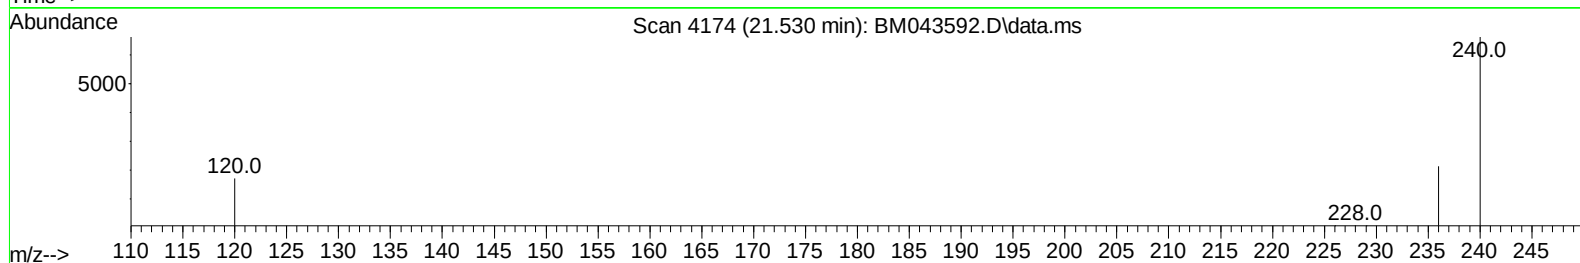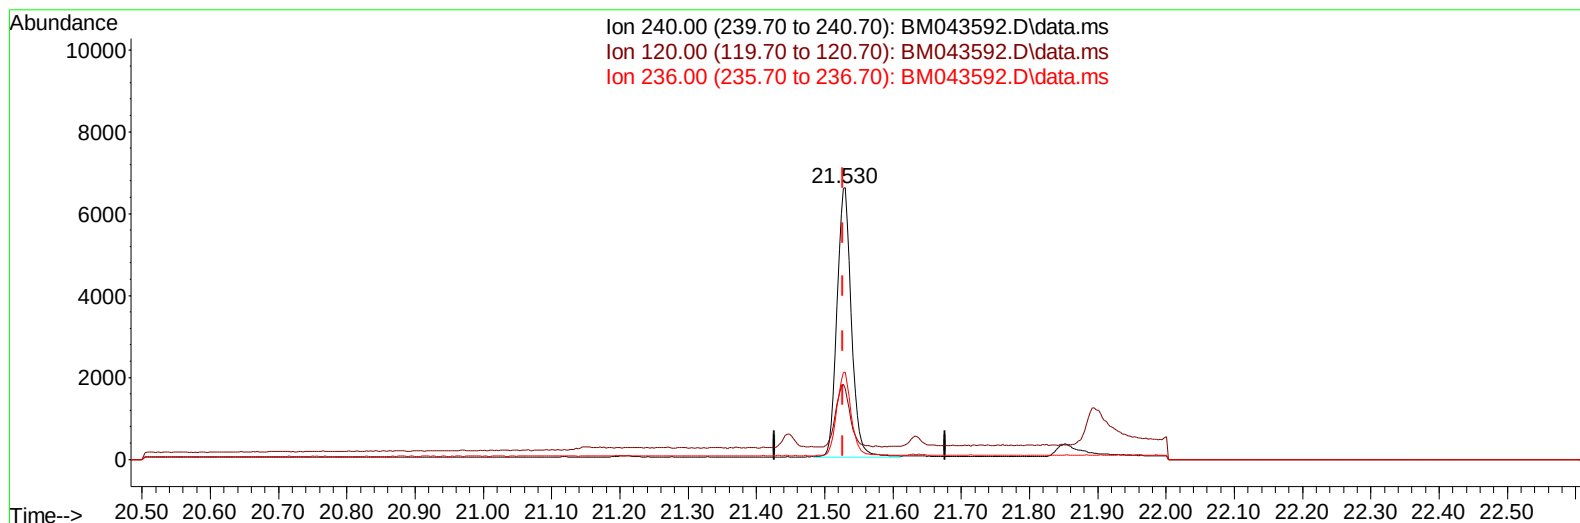

TIC: BM043592.D\data.ms

(17) Chrysene-d12

21.530min (+ 0.003) 0.40 ng/ul m

response 9614

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	20.60	26.03#
236.00	31.10	32.12
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
 Data File : BM043592.D
 Acq On : 27 Dec 2023 03:10
 Operator : MA/JU
 Sample : 06021-13
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH7Z5

Manual IntegrationsAPPROVED

Quant Time: Dec 27 03:43:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 26 22:58:31 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/28/2023
 Supervised By :mohammad ahmed 12/29/2023

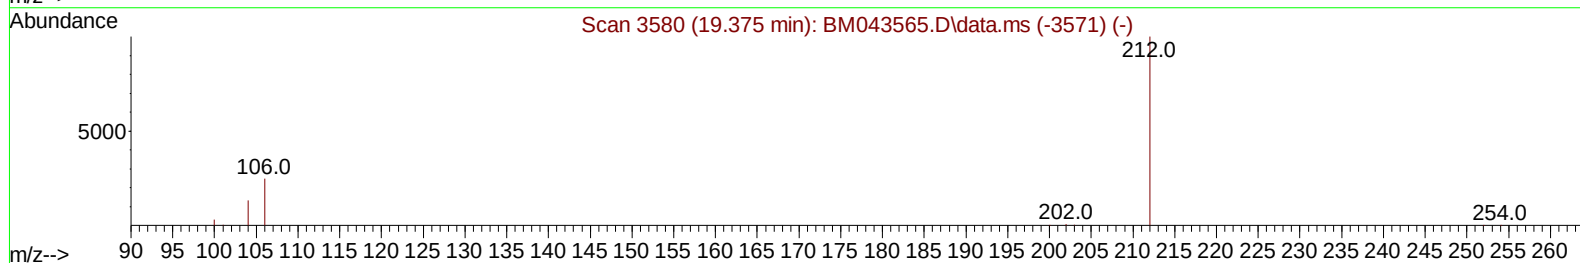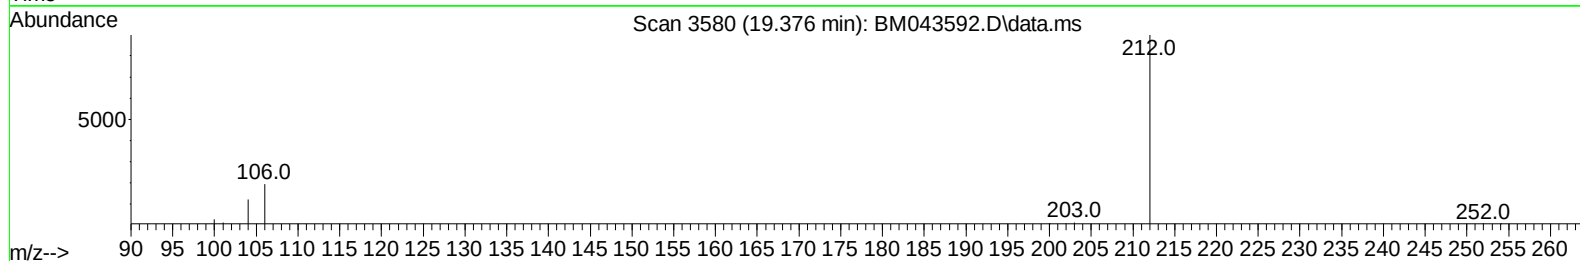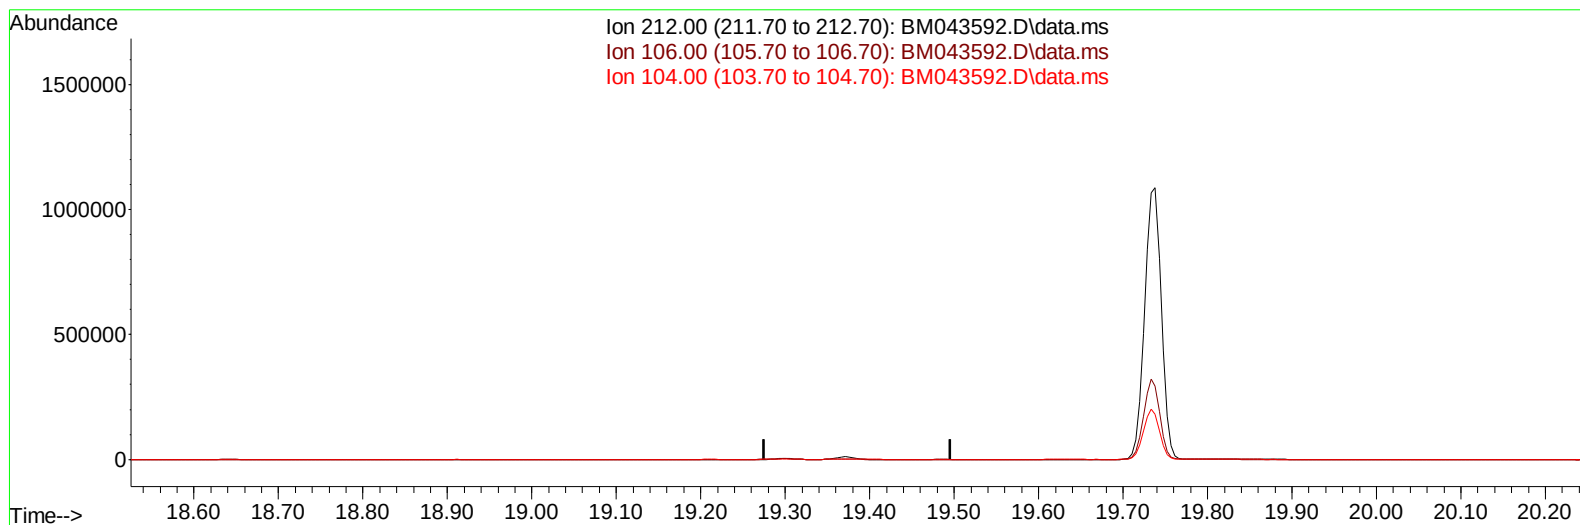

TIC: BM043592.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.375min (-19.375) 0.00 ng/u1

response 0

Ion	Exp%	Act%
212.00	100.00	0.00
106.00	19.40	0.00#
104.00	11.00	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
 Data File : BM043592.D
 Acq On : 27 Dec 2023 03:10
 Operator : MA/JU
 Sample : 06021-13
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH7Z5

Manual IntegrationsAPPROVED

Quant Time: Dec 27 03:43:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 26 22:58:31 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/28/2023
 Supervised By :mohammad ahmed 12/29/2023

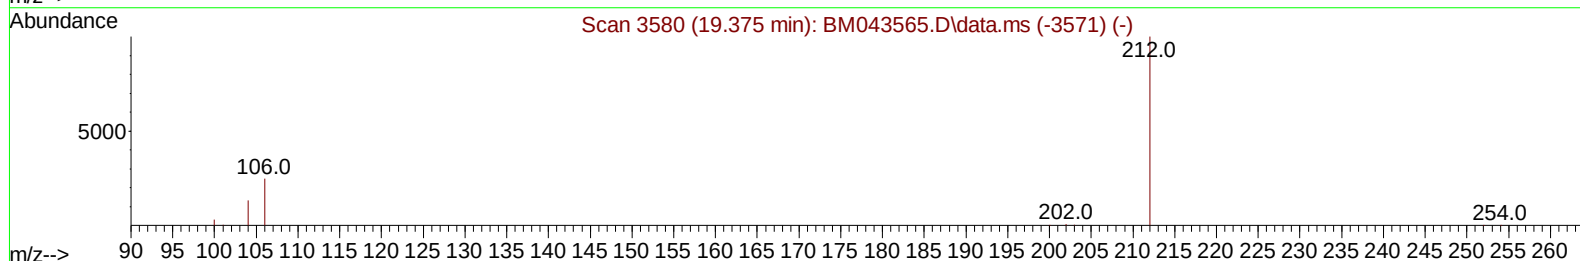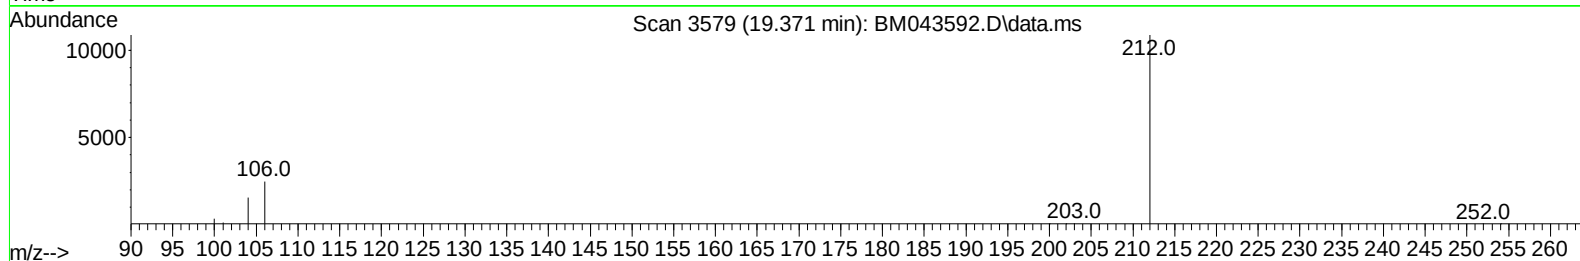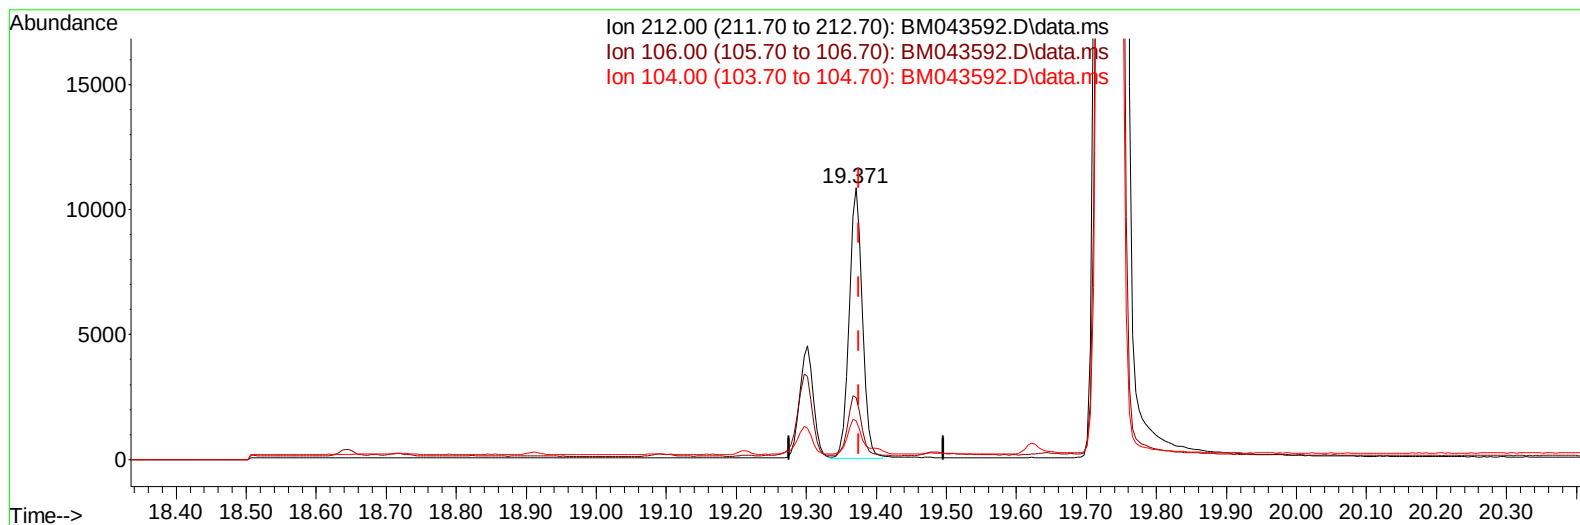

TIC: BM043592.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.371min (-0.004) 0.42 ng/ul m

response 14368

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	19.40	0.00#
104.00	11.00	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
 Data File : BM043592.D
 Acq On : 27 Dec 2023 03:10
 Operator : MA/JU
 Sample : 06021-13
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH7Z5

Manual IntegrationsAPPROVED

Quant Time: Dec 27 03:43:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 26 22:58:31 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/28/2023
 Supervised By :mohammad ahmed 12/29/2023

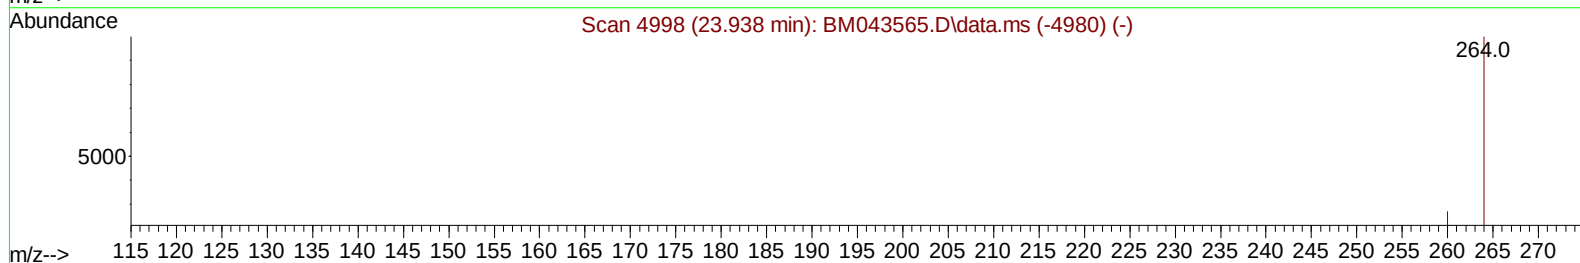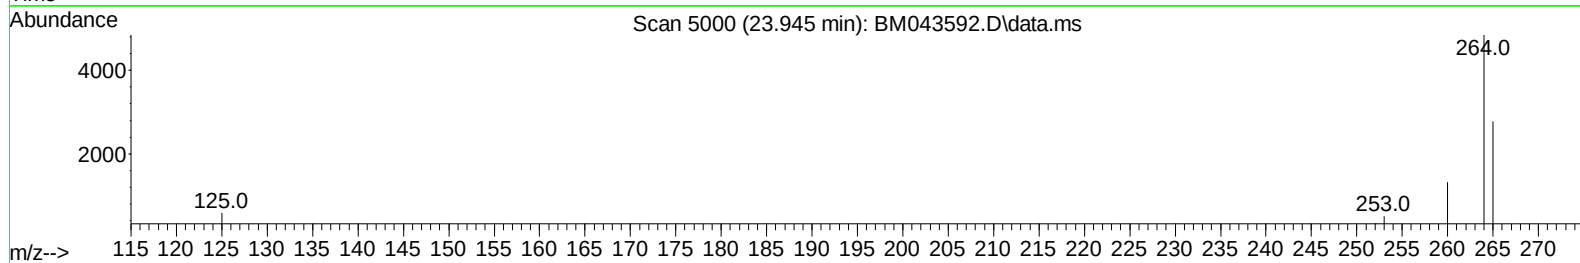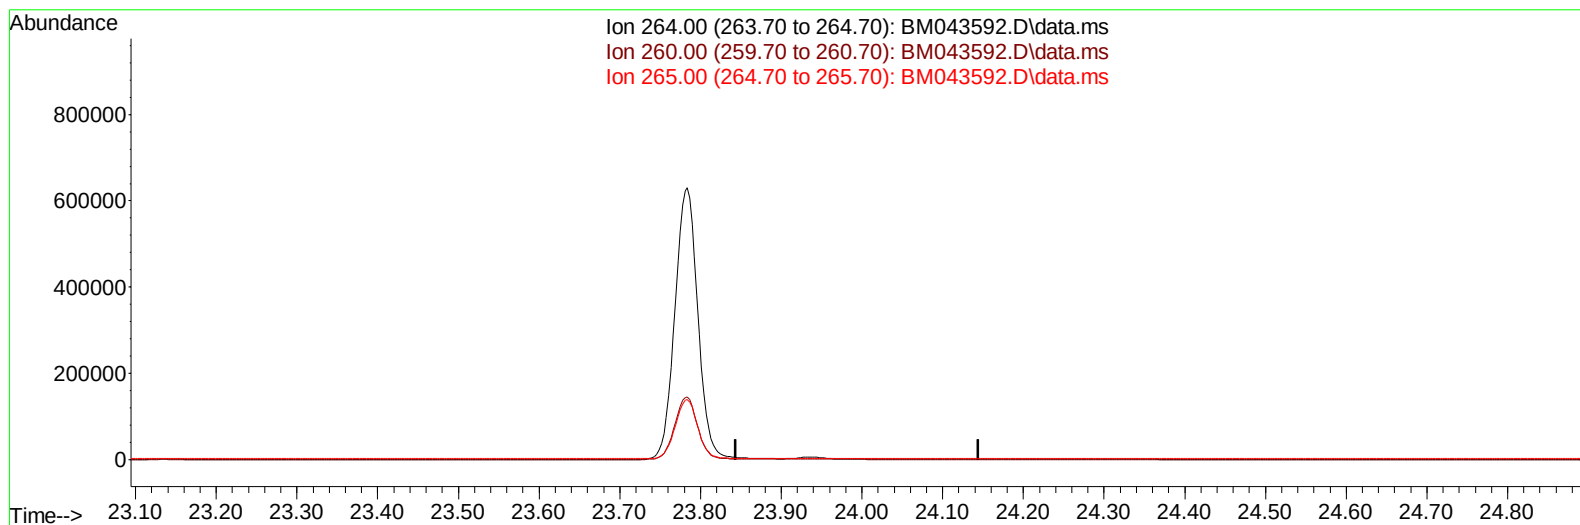

TIC: BM043592.D\data.ms

(23) Perylene-d12 (I)

23.944min (-23.944) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	28.30	0.00#
265.00	39.10	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
 Data File : BM043592.D
 Acq On : 27 Dec 2023 03:10
 Operator : MA/JU
 Sample : 06021-13
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH7Z5

Manual IntegrationsAPPROVED

Quant Time: Dec 27 03:43:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 26 22:58:31 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/28/2023
 Supervised By :mohammad ahmed 12/29/2023

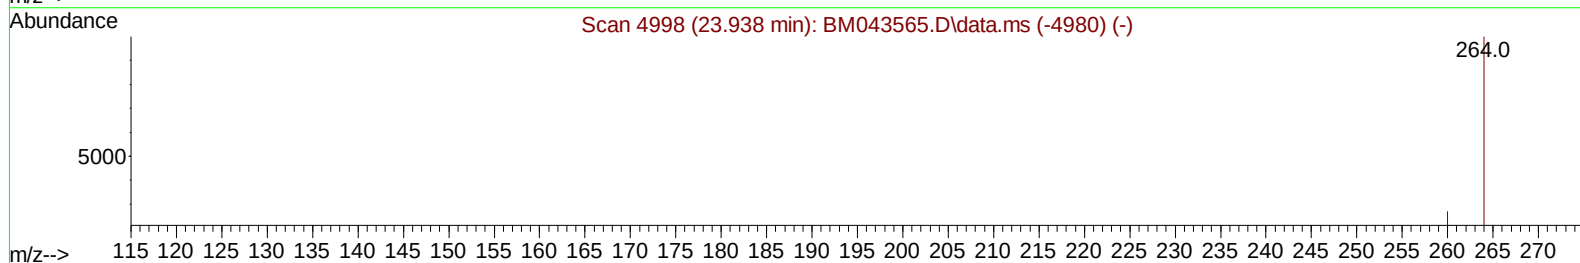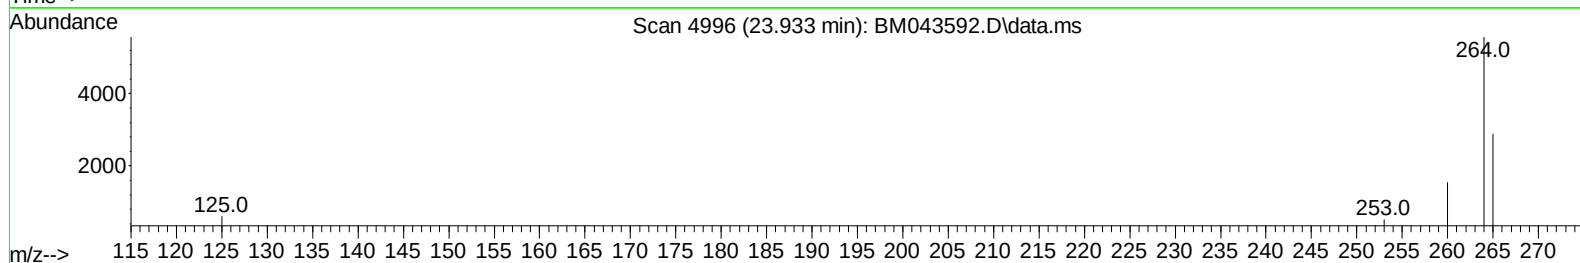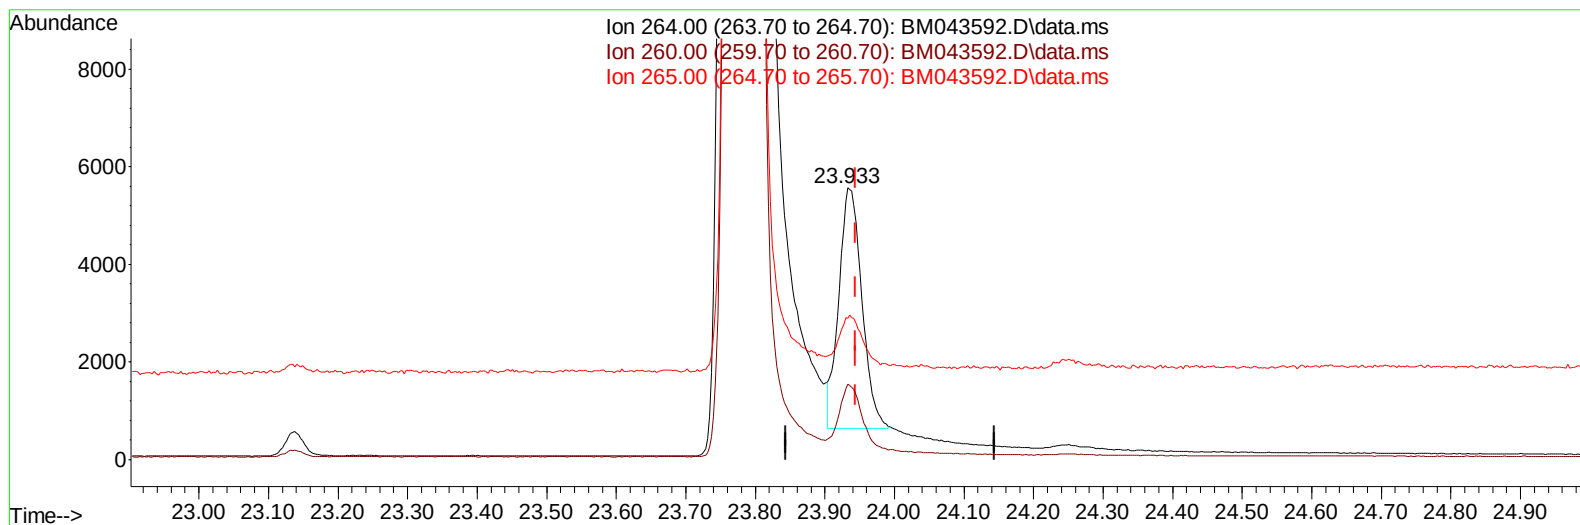

TIC: BM043592.D\data.ms

(23) Perylene-d12 (I)

23.933min (-0.012) 0.40 ng/ul m

response 11343

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	28.30	27.79
265.00	39.10	52.12#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
 Data File : BM043592.D
 Acq On : 27 Dec 2023 03:10
 Operator : MA/JU
 Sample : 06021-13
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH7Z5

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/28/2023
 Supervised By :mohammad ahmed 12/29/2023

Quant Time: Dec 27 03:43:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 26 22:58:31 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.971	152		6523	0.400	ng/ul	0.00
4) Naphthalene-d8	10.774	136		19993	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.601	164		9264	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.350	188		18036m	0.400	ng/ul	0.00
17) Chrysene-d12	21.530	240		9614m	0.400	ng/ul	0.00
23) Perylene-d12	23.933	264		11343m	0.400	ng/ul	-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.372	96		37097	4.501	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.363	152		8406	0.297	ng/ul	0.00
18) Fluoranthene-d10	19.371	212		14368m	0.418	ng/ul	0.00
Target Compounds							Qvalue
2) 1,4-Dioxane	3.410	88		5761	0.697	ng/ul#	82

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
Data File : BM043592.D
Acq On : 27 Dec 2023 03:10
Operator : MA/JU
Sample : 06021-13
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BH7Z5

Manual IntegrationsAPPROVED

Quant Time: Dec 27 03:43:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 26 22:58:31 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/28/2023
Supervised By :mohammad ahmed 12/29/2023

