

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
 Data File : BM043569.D
 Acq On : 26 Dec 2023 12:40
 Operator : MA/JU
 Sample : 05927-13
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH3P6

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/28/2023
 Supervised By :mohammad ahmed 12/29/2023

Quant Time: Dec 26 14:06:40 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 19 23:32:46 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.971	152	6398	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.779	136	19099	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.606	164	8707	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.350	188	17734m	0.400	ng/ul	0.00
17) Chrysene-d12	21.530	240	9761m	0.400	ng/ul	0.00
23) Perylene-d12	23.941	264	9460m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.376	96	32382	4.006	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.368	152	7207	0.266	ng/ul	-0.01
18) Fluoranthene-d10	19.371	212	11249	0.323	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.414	88	604	0.074	ng/ul#	63

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
Data File : BM043569.D
Acq On : 26 Dec 2023 12:40
Operator : MA/JU
Sample : 05927-13
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BH3P6

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/28/2023
Supervised By :mohammad ahmed 12/29/2023


Quant Time: Dec 26 14:06:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 19 23:32:46 2023
Response via : Initial Calibration

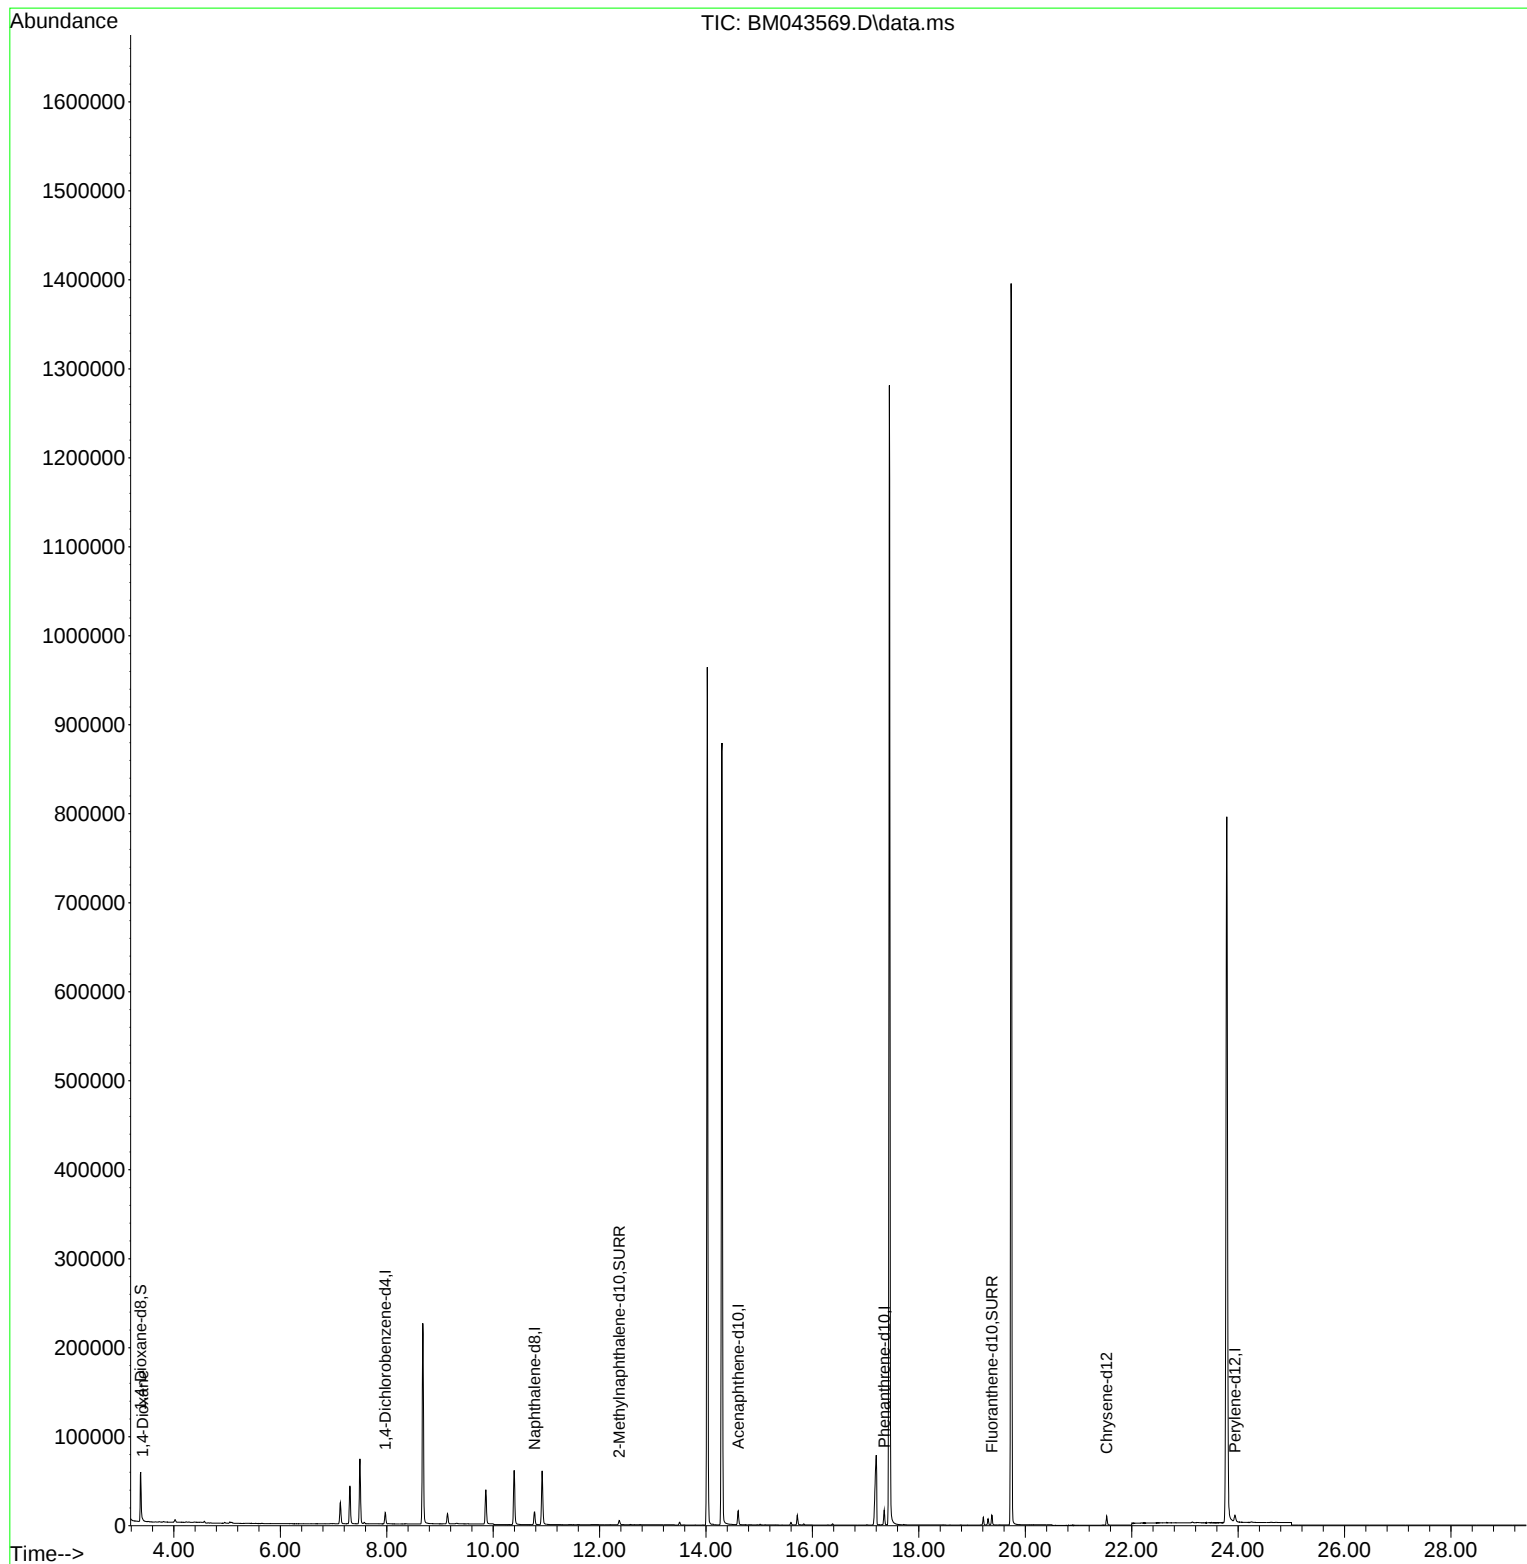

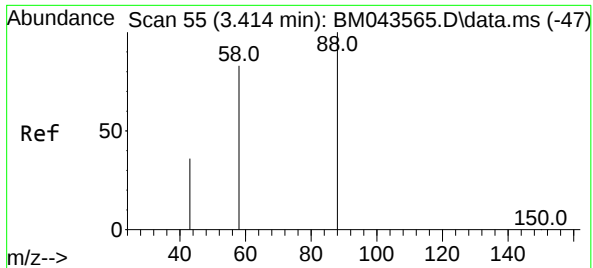

#2
 1,4-Dioxane
 Concen: 0.074 ng/ul
 RT: 3.414 min Scan# 51
 Delta R.T. -0.004 min
 Lab File: BM043569.D
 Acq: 26 Dec 2023 12:40

Instrument :
 BNA_M
 ClientSampleId :
 BH3P6

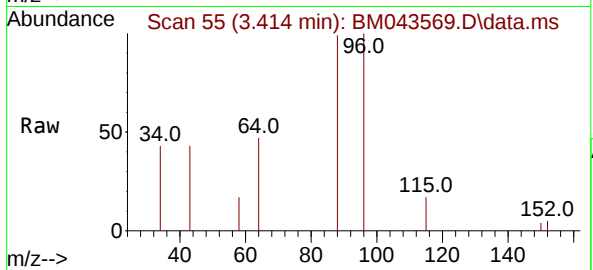

Tgt Ion: 88 Resp: 604

Ion	Ratio	Lower	Upper
88	100		
43	43.1	27.9	41.9
58	16.8	43.4	65.2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/28/2023
 Supervised By :mohammad ahmed 12/29/2023

