

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
 Data File : BM043609.D
 Acq On : 27 Dec 2023 15:20
 Operator : MA/JU
 Sample : 06020-10
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BH7X1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/28/2023
 Supervised By :mohammad ahmed 12/29/2023

Quant Time: Dec 27 21:42:05 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 26 22:58:31 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.971	152	4843	0.400	ng/ul	0.00
4) Naphthalene-d8	10.773	136	14890	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.601	164	6938	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.345	188	15096m	0.400	ng/ul	0.00
17) Chrysene-d12	21.530	240	8958m	0.400	ng/ul	0.00
23) Perylene-d12	23.938	264	14050	0.400	ng/ul #	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.376	96	28911	4.725	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.368	152	6456	0.306	ng/ul	0.00
18) Fluoranthene-d10	19.371	212	12781	0.399	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.414	88	946	0.154	ng/ul#	65

(#) = qualifier out of range (m) = manual integration (+) = signals summed


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\  
Data File : BM043609.D  
Acq On    : 27 Dec 2023   15:20  
Operator  : MA/JU  
Sample    : 06020-10  
Misc      :  
ALS Vial  : 48    Sample Multiplier: 1
```


Instrument :
BNA_M
ClientSampleId :
BH7X1

Manual Integrations

Reviewed By :Yogesh Patel 12/28/2023
Supervised By :mohammad ahmed 12/29/2023


Quant Time: Dec 27 21:42:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 26 22:58:31 2023
Response via : Initial Calibration

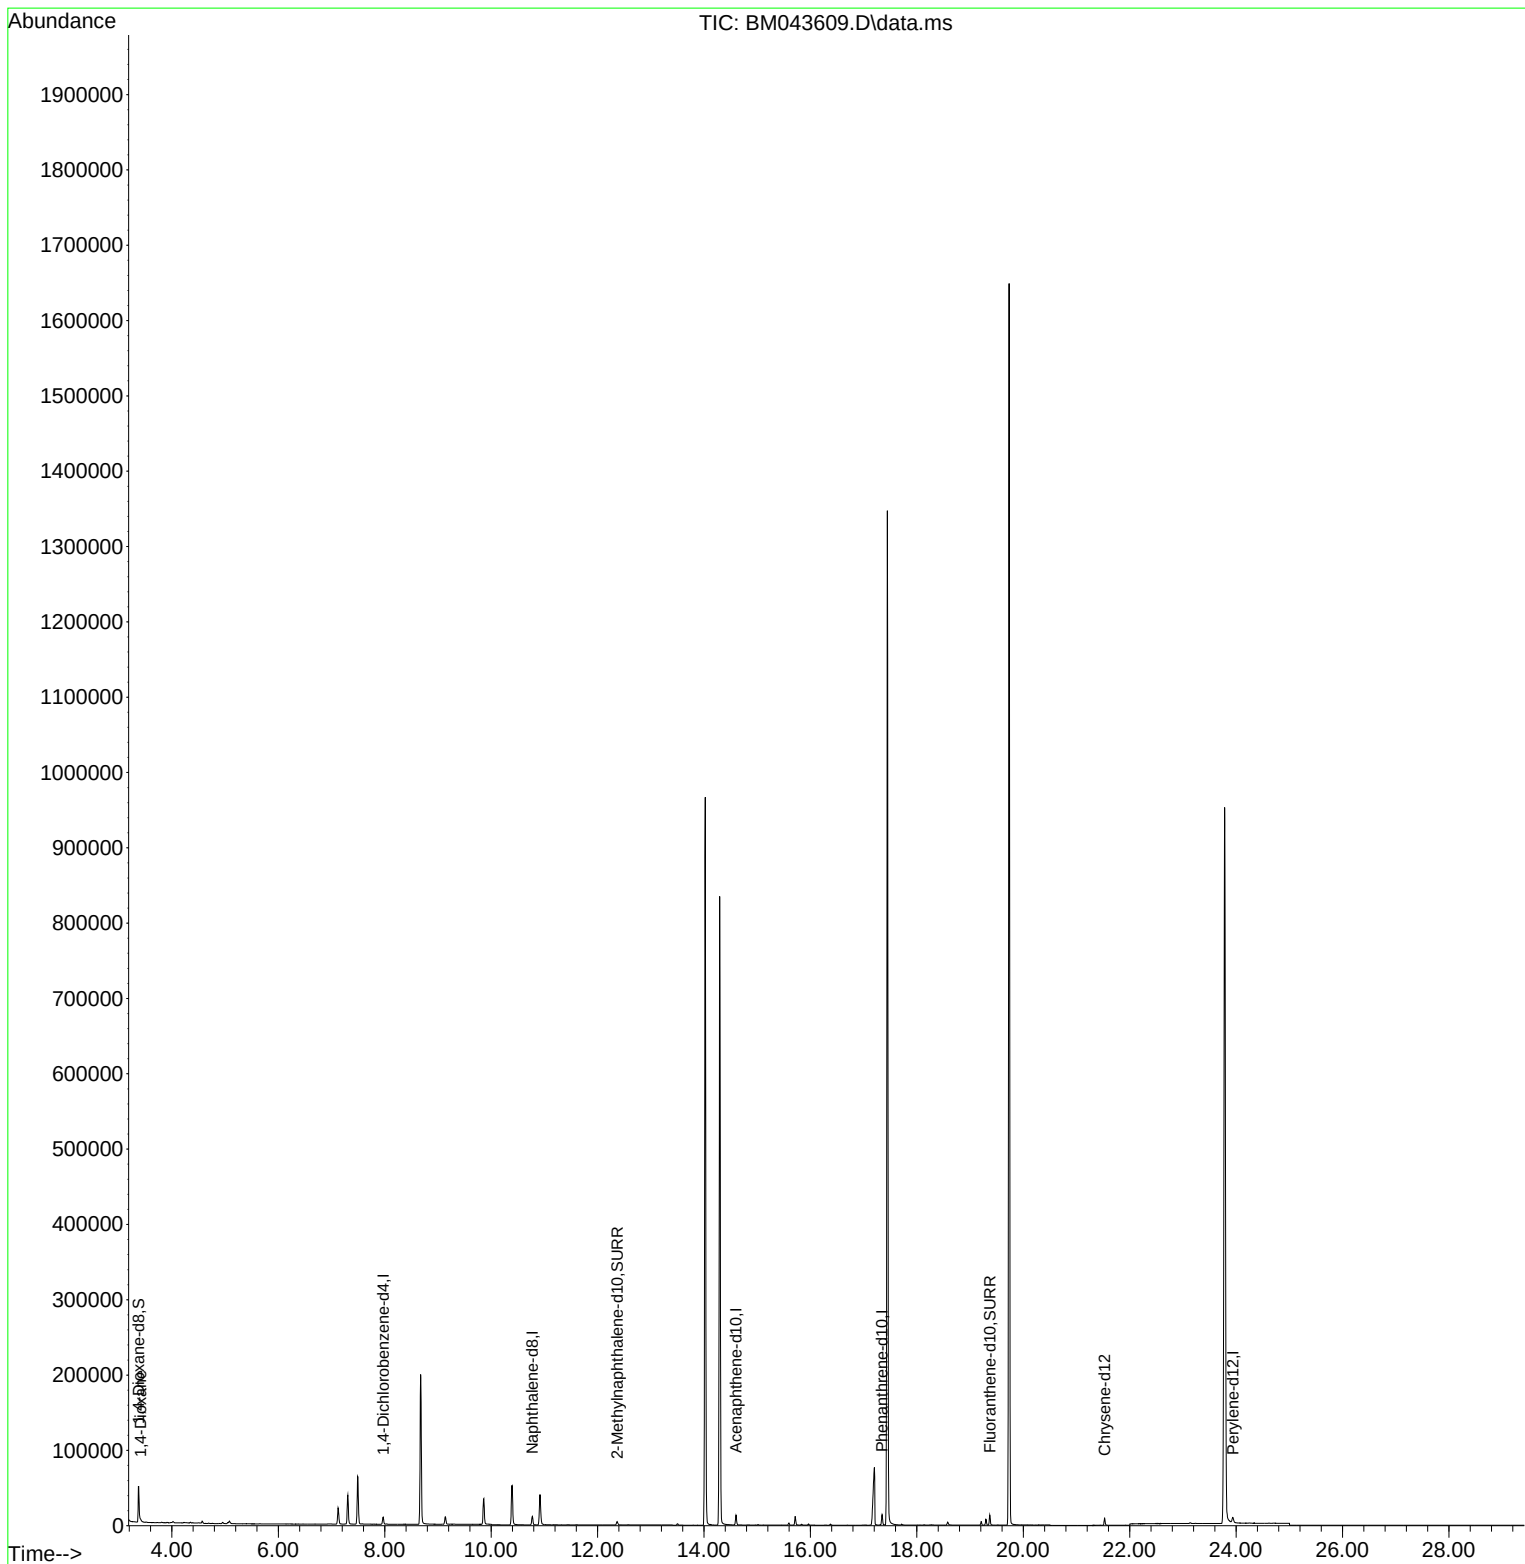

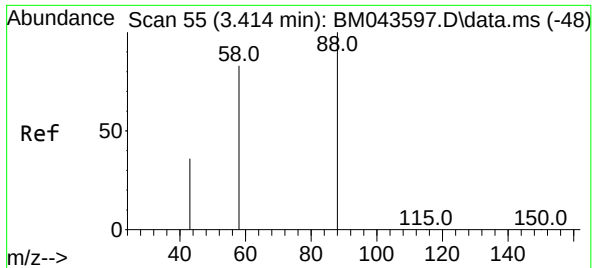

#2
 1,4-Dioxane
 Concen: 0.154 ng/ul
 RT: 3.414 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: BM043609.D
 Acq: 27 Dec 2023 15:20

Instrument :
 BNA_M
 ClientSampleId :
 BH7X1

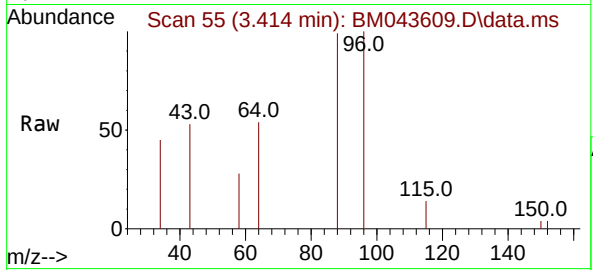

Tgt Ion: 88 Resp: 940

Ion	Ratio	Lower	Upper
88	100		
43	53.8	27.9	41.9
58	28.0	43.4	65.2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/28/2023
 Supervised By :mohammad ahmed 12/29/2023

