

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
 Data File : BM043641.D
 Acq On : 28 Dec 2023 15:16
 Operator : MA/JU
 Sample : PB157780BL
 Misc : GCMS CONFIRMATION
 ALS Vial : 82 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK780

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM043641.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.216	3	5	7	rVV2	27620	21974	1.16%	0.192%
2	3.240	7	9	12	rVB	54004	52687	2.78%	0.461%
3	3.281	12	16	27	rVB	1231026	1279896	67.63%	11.197%
4	3.622	72	74	82	rVB4	21439	30938	1.63%	0.271%
5	4.110	154	157	163	rVB	22252	31020	1.64%	0.271%
6	4.263	180	183	187	rBV3	14745	19352	1.02%	0.169%
7	4.316	189	192	198	rVB	19609	25907	1.37%	0.227%
8	4.416	206	209	213	rBV2	18493	23757	1.26%	0.208%
9	4.457	213	216	225	rVB2	23447	36425	1.92%	0.319%
10	6.051	484	487	494	rVB8	4034	7318	0.39%	0.064%
11	6.287	526	527	529	rVB2	4306	1941	0.10%	0.017%
12	6.316	529	532	535	rBV5	3688	5479	0.29%	0.048%
13	6.404	545	547	548	rBV	2975	2044	0.11%	0.018%
14	6.498	561	563	566	rBV4	2476	2092	0.11%	0.018%
15	6.587	574	578	585	rVB3	15652	25281	1.34%	0.221%
16	6.734	598	603	609	rBV	19922	35305	1.87%	0.309%
17	7.039	652	655	662	rVB8	6301	10680	0.56%	0.093%
18	7.598	749	750	752	rBV2	2594	2012	0.11%	0.018%
19	7.863	793	795	796	rBV2	2669	2503	0.13%	0.022%
20	7.957	804	811	824	rBV	846934	1393758	73.65%	12.193%
21	8.116	835	838	841	rBV5	1611	2170	0.11%	0.019%
22	8.139	841	842	846	rVB4	2850	2937	0.16%	0.026%
23	8.951	979	980	982	rBV	3560	3092	0.16%	0.027%
24	9.286	1035	1037	1042	rVB6	2044	2829	0.15%	0.025%
25	9.333	1042	1045	1047	rBV3	1897	1977	0.10%	0.017%
26	9.598	1089	1090	1094	rVB3	2686	2464	0.13%	0.022%
27	9.775	1119	1120	1123	rBV3	1914	2002	0.11%	0.018%
28	9.927	1141	1146	1148	rBV6	2165	2529	0.13%	0.022%
29	10.016	1158	1161	1165	rBV5	2282	3460	0.18%	0.030%
30	10.151	1179	1184	1187	rBV6	2055	3497	0.18%	0.031%
31	10.345	1216	1217	1221	rVB4	2325	2170	0.11%	0.019%
32	10.380	1221	1223	1224	rBV2	2574	2307	0.12%	0.020%
33	10.539	1248	1250	1253	rVB4	2278	2234	0.12%	0.020%
34	10.769	1281	1289	1301	rBV	1044468	1789461	94.56%	15.655%
35	11.157	1352	1355	1357	rBV4	1754	2102	0.11%	0.018%
36	11.721	1447	1451	1455	rBV7	1553	2408	0.13%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
 Data File : BM043641.D
 Acq On : 28 Dec 2023 15:16
 Operator : MA/JU
 Sample : PB157780BL
 Misc : GCMS CONFIRMATION
 ALS Vial : 82 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK780

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
 Title : SVOA CALIBRATION

37	11.921	1480	1485	1486	rVB5	2937	3000	0.16%	0.026%
38	12.410	1563	1568	1571	rVB7	2136	3235	0.17%	0.028%
39	12.674	1610	1613	1616	rBV5	2800	3752	0.20%	0.033%
40	13.168	1693	1697	1699	rBV5	1633	2664	0.14%	0.023%
41	13.198	1701	1702	1706	rBV4	1784	1920	0.10%	0.017%
42	13.780	1799	1801	1805	rVB5	2063	2324	0.12%	0.020%
43	13.845	1809	1812	1813	rBV3	2381	2176	0.11%	0.019%
44	13.992	1832	1837	1838	rBV5	2596	3657	0.19%	0.032%
45	14.104	1855	1856	1861	rVB4	1752	1962	0.10%	0.017%
46	14.186	1867	1870	1871	rBV3	1981	2098	0.11%	0.018%
47	14.304	1889	1890	1894	rVB4	2516	2545	0.13%	0.022%
48	14.374	1900	1902	1905	rVB3	1966	1948	0.10%	0.017%
49	14.598	1933	1940	1958	rBV	1273252	1892464	100.00%	16.556%
50	14.910	1990	1993	1997	rBV5	1676	2977	0.16%	0.026%
51	15.057	2015	2018	2020	rBV4	2423	3102	0.16%	0.027%
52	15.327	2062	2064	2066	rBV3	1996	2096	0.11%	0.018%
53	15.657	2116	2120	2122	rBV5	1855	2078	0.11%	0.018%
54	15.727	2126	2132	2134	rBV6	1977	3406	0.18%	0.030%
55	16.098	2191	2195	2197	rBV5	1993	2415	0.13%	0.021%
56	16.256	2219	2222	2224	rBV3	2168	2585	0.14%	0.023%
57	16.509	2262	2265	2267	rVV4	2310	2337	0.12%	0.020%
58	17.051	2353	2357	2359	rBV5	1726	2599	0.14%	0.023%
59	17.133	2366	2371	2376	rBV7	3083	6556	0.35%	0.057%
60	17.345	2400	2407	2423	rBV	1180258	1863999	98.50%	16.307%
61	17.833	2487	2490	2494	rVB5	2316	3689	0.19%	0.032%
62	17.874	2494	2497	2500	rBV5	2596	4205	0.22%	0.037%
63	18.074	2529	2531	2533	rBV3	2094	2149	0.11%	0.019%
64	18.233	2553	2558	2560	rBV5	2402	3518	0.19%	0.031%
65	18.421	2588	2590	2593	rVB3	2678	2936	0.16%	0.026%
66	18.456	2593	2596	2597	rBV3	2248	2006	0.11%	0.018%
67	18.833	2656	2660	2661	rBV3	2096	1997	0.11%	0.017%
68	19.003	2688	2689	2692	rBV3	2036	2342	0.12%	0.020%
69	19.139	2709	2712	2713	rBV2	2395	2059	0.11%	0.018%
70	19.580	2785	2787	2789	rBV3	2579	2661	0.14%	0.023%
71	19.674	2800	2803	2807	rBV6	4827	7688	0.41%	0.067%
72	20.309	2910	2911	2914	rBV3	5923	7179	0.38%	0.063%
73	21.521	3112	3117	3127	rBV	987404	1345175	71.08%	11.768%
74	23.932	3520	3527	3543	rVB2	667443	1387125	73.30%	12.135%

Sum of corrected areas: 11430632

Instrument :

BNA_M

ClientSampleId :




SBLK780

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
Data File : BM043641.D
Acq On : 28 Dec 2023 15:16
Operator : MA/JU
Sample : PB157780BL
Misc : GCMS CONFIRMATION
ALS Vial : 82 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK780

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

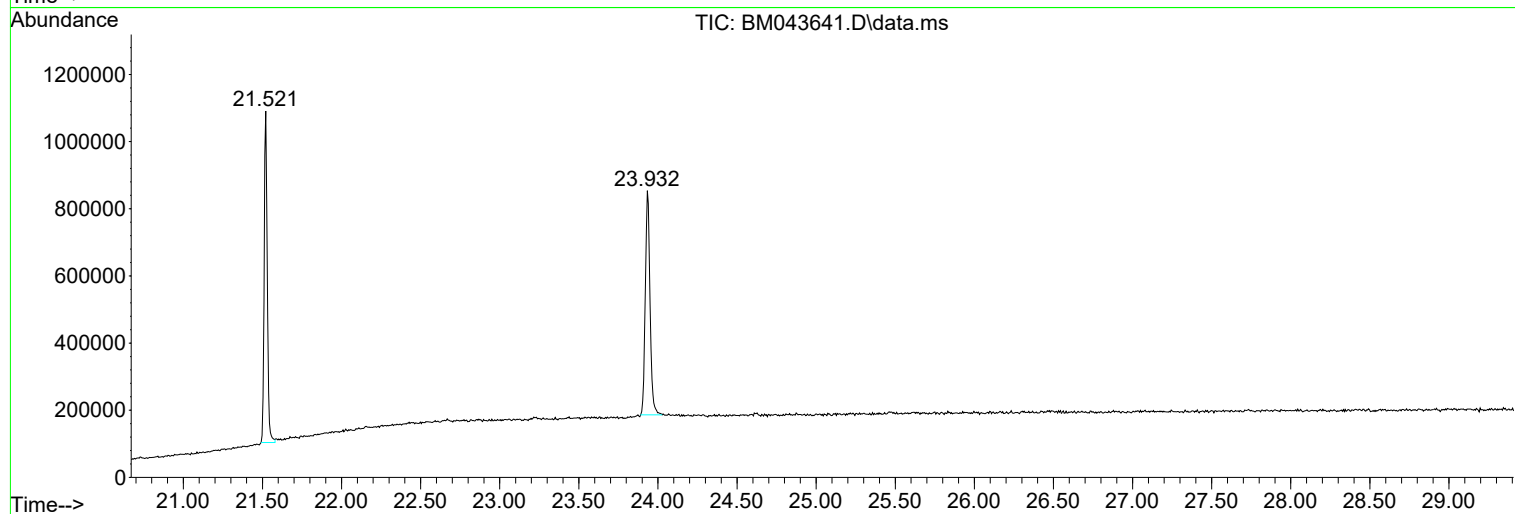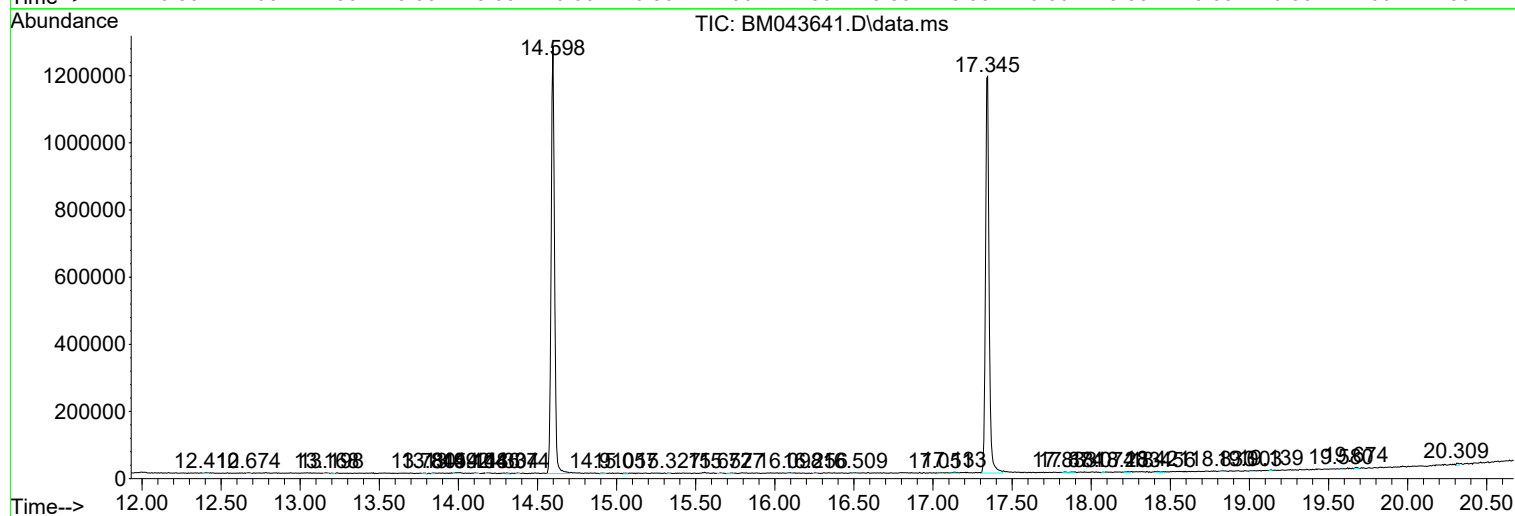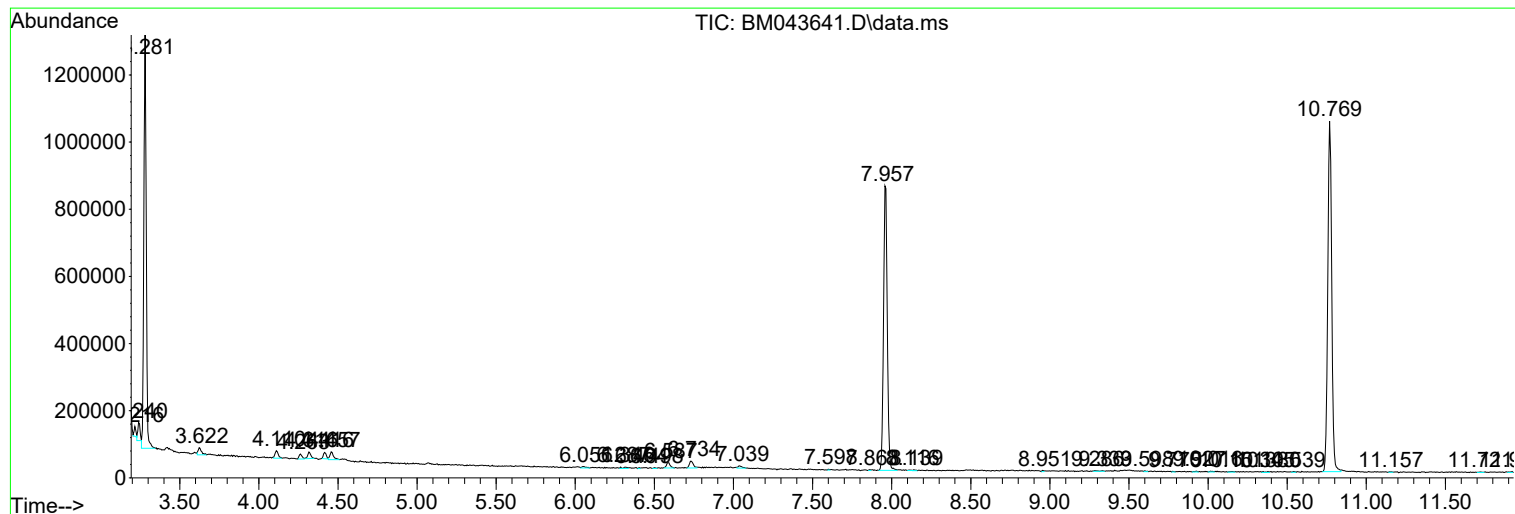

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
Data File : BM043641.D
Acq On : 28 Dec 2023 15:16
Operator : MA/JU
Sample : PB157780BL
Misc : GCMS CONFIRMATION
ALS Vial : 82 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK780










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.281	18.37 ng/ul	1279900	1,4-Dichlorobenzene-d4	7.963

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Heptane			100	C7H16	000142-82-5	94
2	Heptane			100	C7H16	000142-82-5	91
3	Heptane			100	C7H16	000142-82-5	91
4	Heptane			100	C7H16	000142-82-5	72
5	Hexane, 3-methyl-			100	C7H16	000589-34-4	42

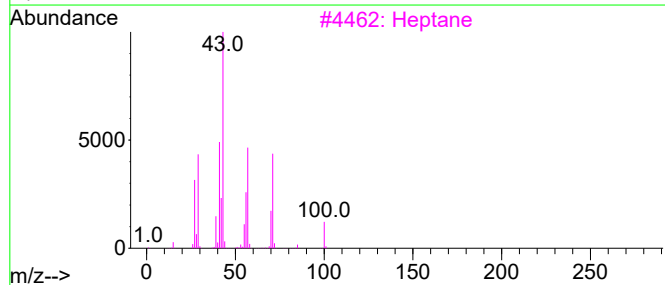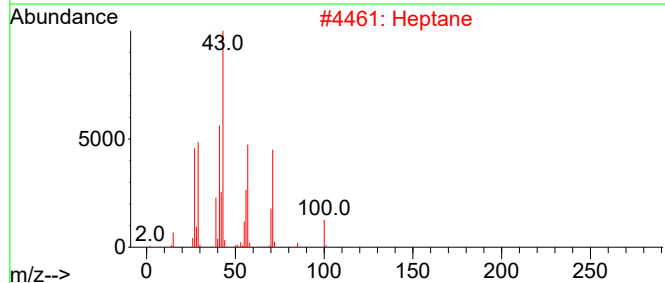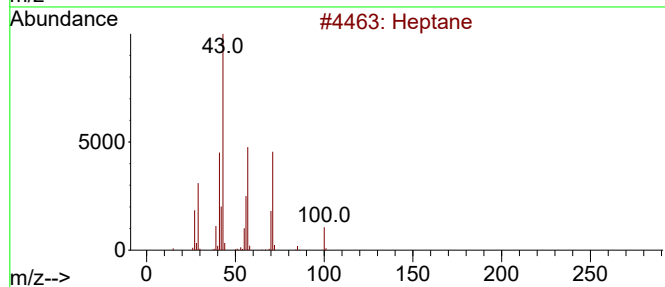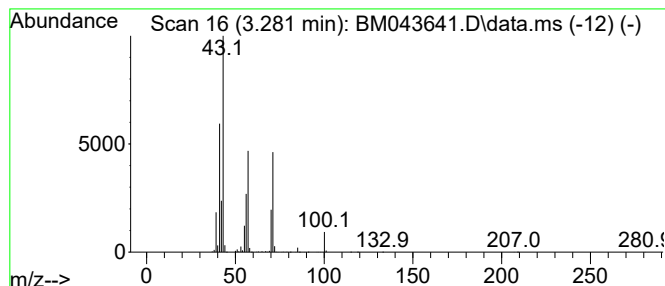

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122623\
Data File : BM043641.D
Acq On : 28 Dec 2023 15:16
Operator : MA/JU
Sample : PB157780BL
Misc : GCMS CONFIRMATION
ALS Vial : 82 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK780

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM121523.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	3.281	18.4	ng/ul	1279900	1	7.963	1393760	20.0