

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122624\
 Data File : BM049235.D
 Acq On : 26 Dec 2024 21:08
 Operator : RC/JU
 Sample : PB165752BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK752

Quant Time: Dec 26 21:59:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 26 11:35:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.543	152	3986	0.400	ng/ul	0.00
4) Naphthalene-d8	10.304	136	11977	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.183	164	7066	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.031	188	1103208	0.400	ng/ul	# 0.10
17) Chrysene-d12	0.000	240	0	0.000	ng/ul	-21.13
23) Perylene-d12	23.288	264	19525	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.134	96	25850	5.623	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.915	152	4664	0.290	ng/ul	0.00
18) Fluoranthene-d10	18.969	212	11811	0.000	ng/ul	0.00
Target Compounds						
26) Benzo(a)pyrene	23.150	252	4645	0.078	ng/ul#	Qvalue 70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122624\
Data File : BM049235.D
Acq On : 26 Dec 2024 21:08
Operator : RC/JU
Sample : PB165752BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK752


Quant Time: Dec 26 21:59:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 26 11:35:38 2024
Response via : Initial Calibration

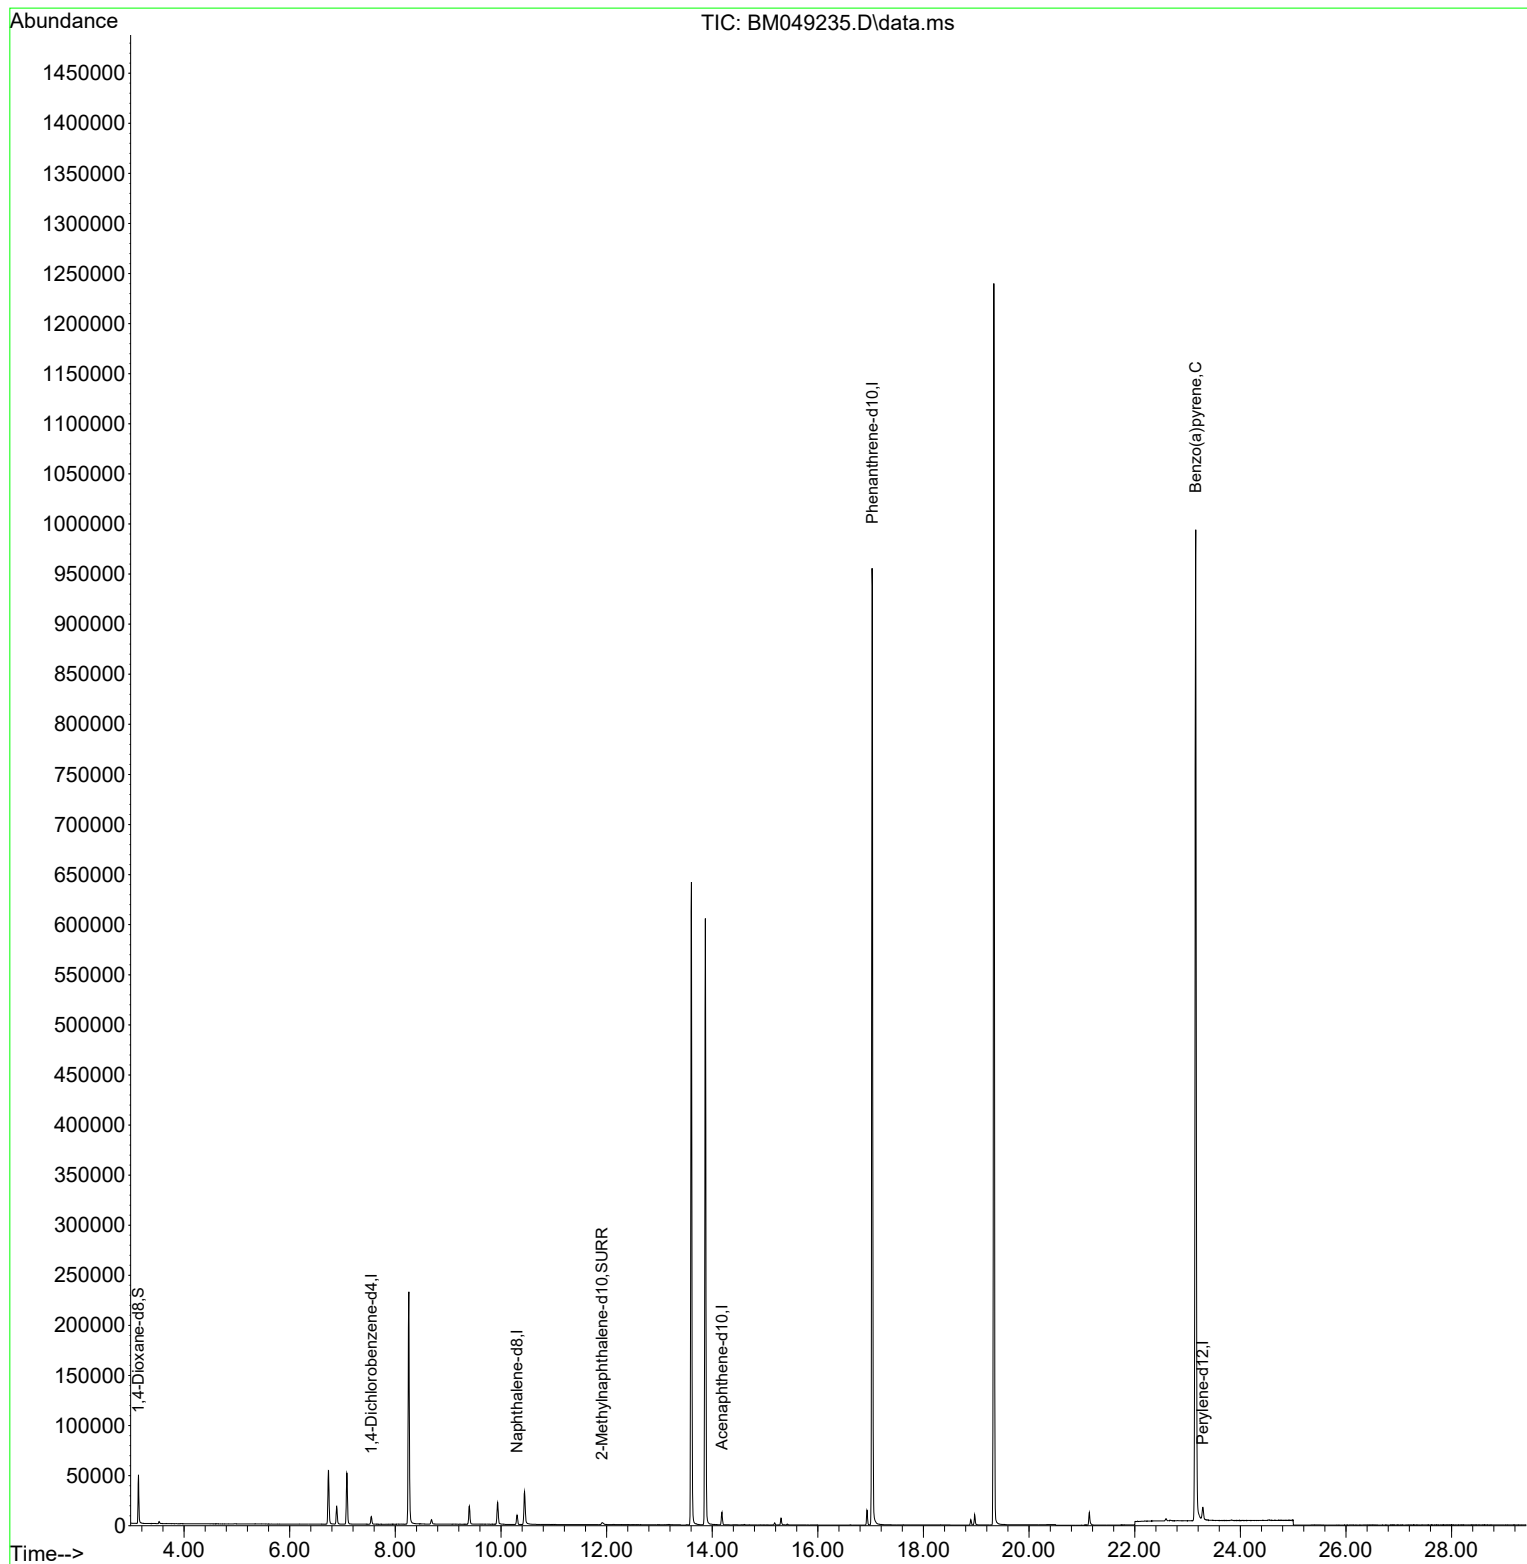

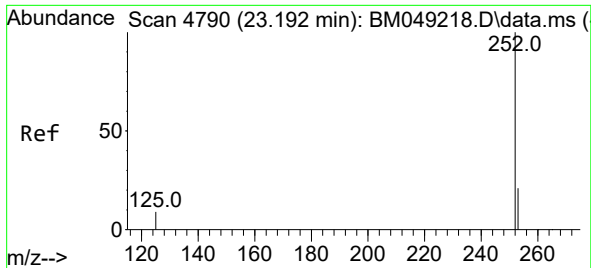

#26
Benzo(a)pyrene
Concen: 0.078 ng/ul
RT: 23.150 min Scan# 41
Delta R.T. -0.041 min
Lab File: BM049235.D
Acq: 26 Dec 2024 21:08

Instrument :
BNA_M
ClientSampleId :
SBLK752

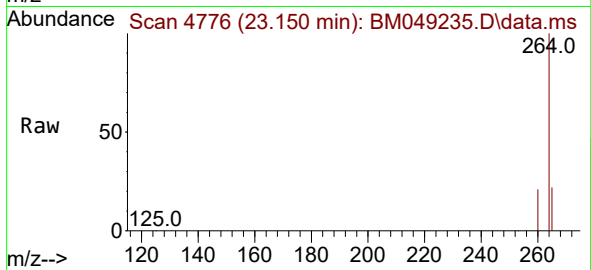

Tgt Ion:252 Resp: 4645
Ion Ratio Lower Upper
252 100
253 43.7 22.4 33.6#
125 31.6 14.8 22.2#

