




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122624\
Data File : BM049238.D
Acq On : 26 Dec 2024 22:56
Operator : RC/JU
Sample : P5333-14DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2916DL

Manual IntegrationsAPPROVED

Quant Time: Dec 27 00:46:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 26 11:35:38 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/27/2024
Supervised By :mohammad ahmed 12/30/2024

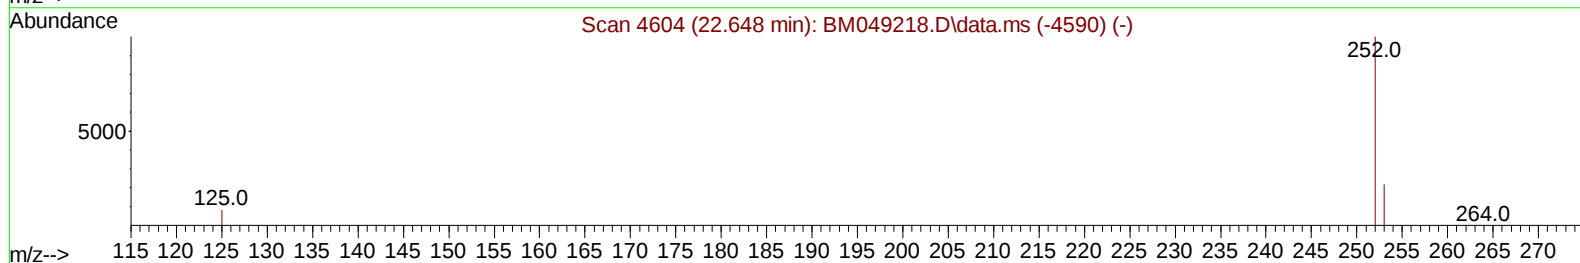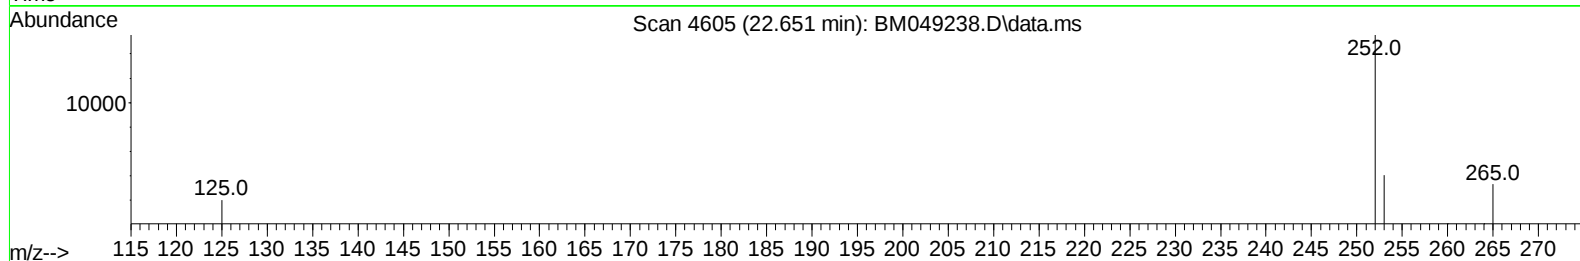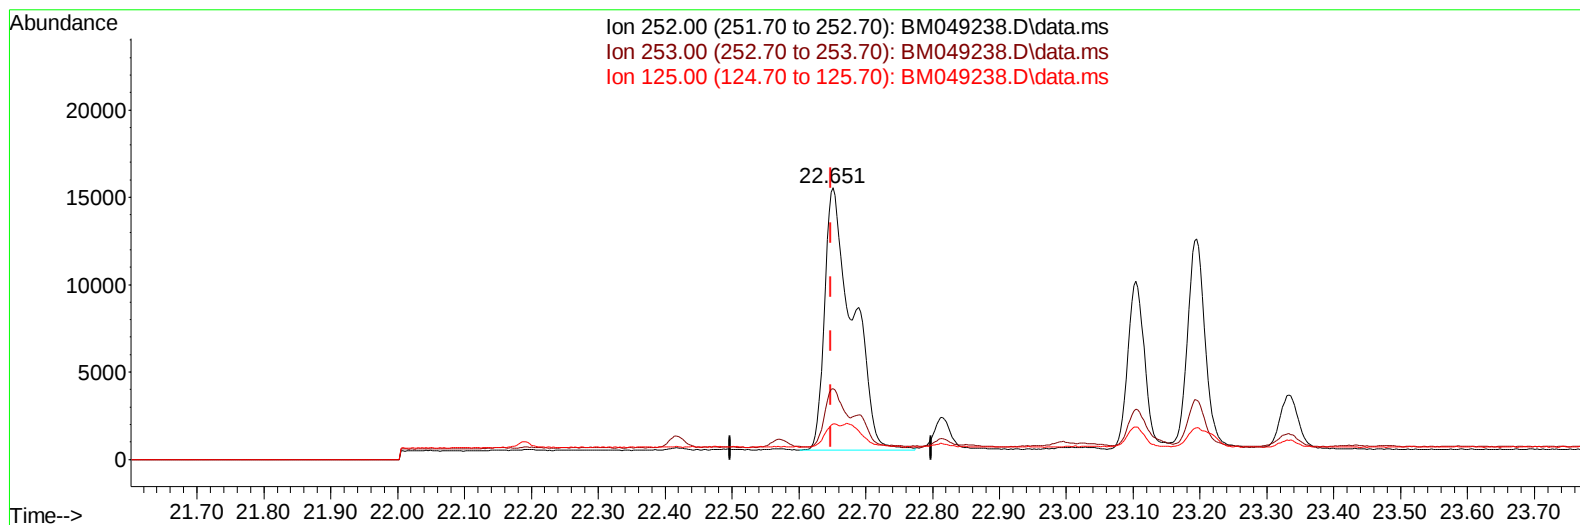

TIC: BM049238.D\data.ms

(24) Benzo(b)fluoranthene

22.651min (+ 0.003) 0.66 ng/u1

response 43803

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	26.30	26.11
125.00	15.40	13.06
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122624\
Data File : BM049238.D
Acq On : 26 Dec 2024 22:56
Operator : RC/JU
Sample : P5333-14DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2916DL

Manual IntegrationsAPPROVED

Quant Time: Dec 27 00:46:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 26 11:35:38 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/27/2024
Supervised By :mohammad ahmed 12/30/2024

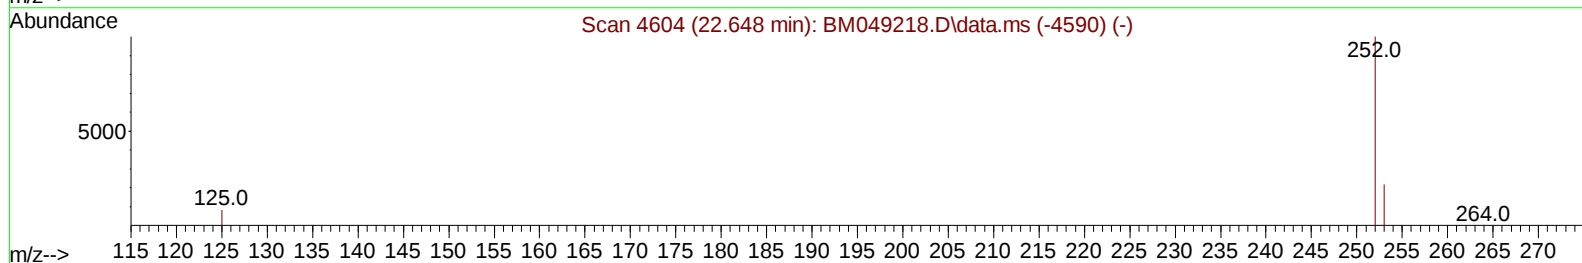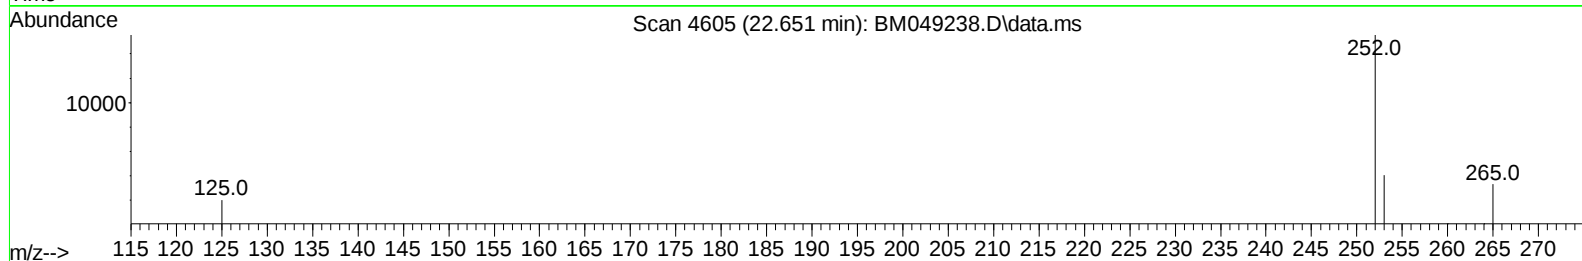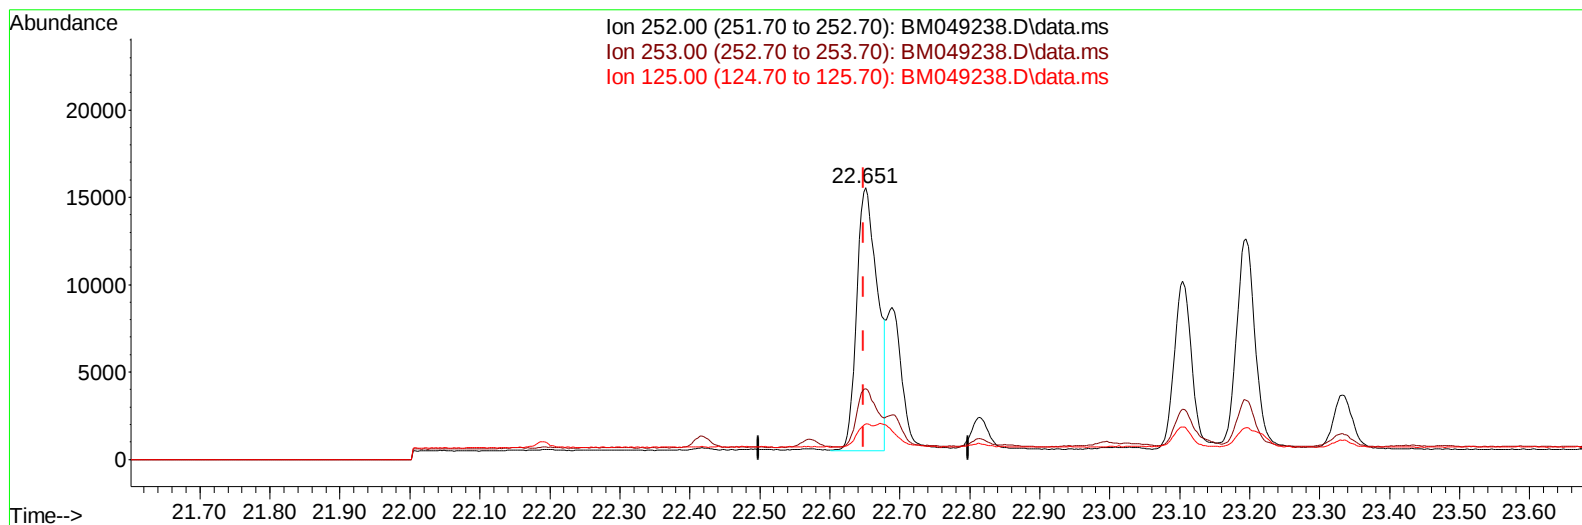

TIC: BM049238.D\data.ms

(24) Benzo(b)fluoranthene

22.651min (+ 0.003) 0.46 ng/u1 m

response 30941

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	26.30	26.11
125.00	15.40	13.06
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122624\
Data File : BM049238.D
Acq On : 26 Dec 2024 22:56
Operator : RC/JU
Sample : P5333-14DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2916DL

Manual IntegrationsAPPROVED

Quant Time: Dec 27 00:46:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 26 11:35:38 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/27/2024
Supervised By :mohammad ahmed 12/30/2024

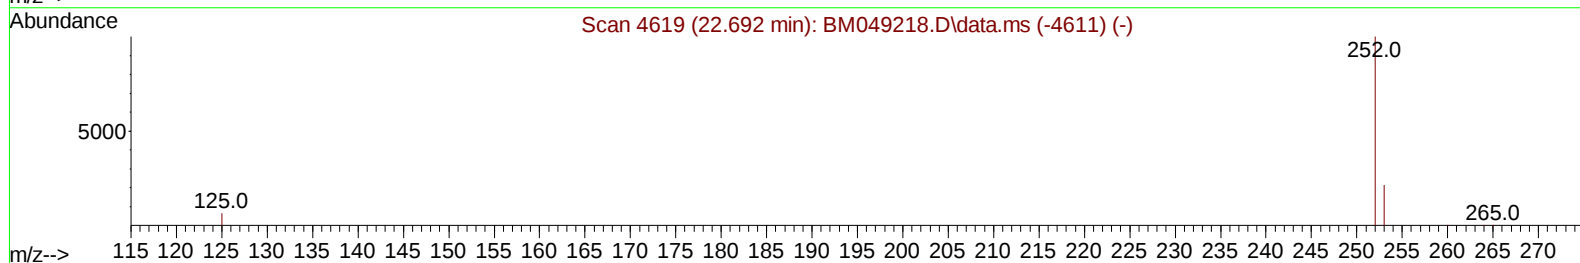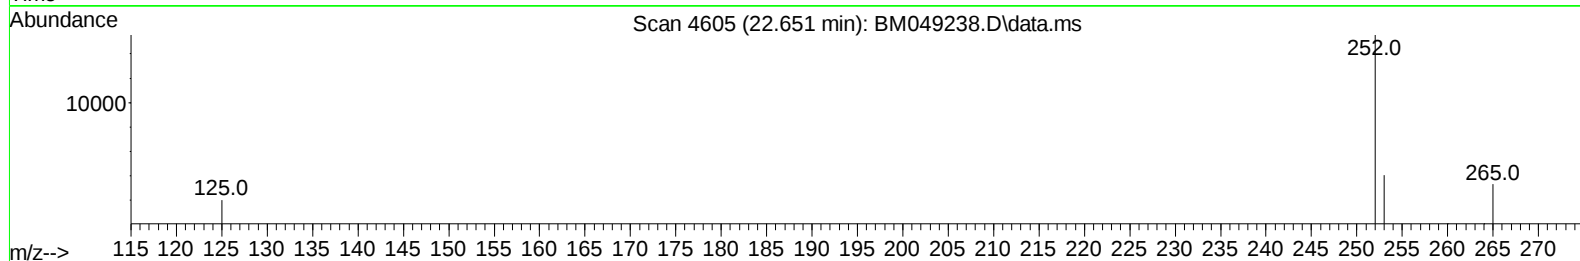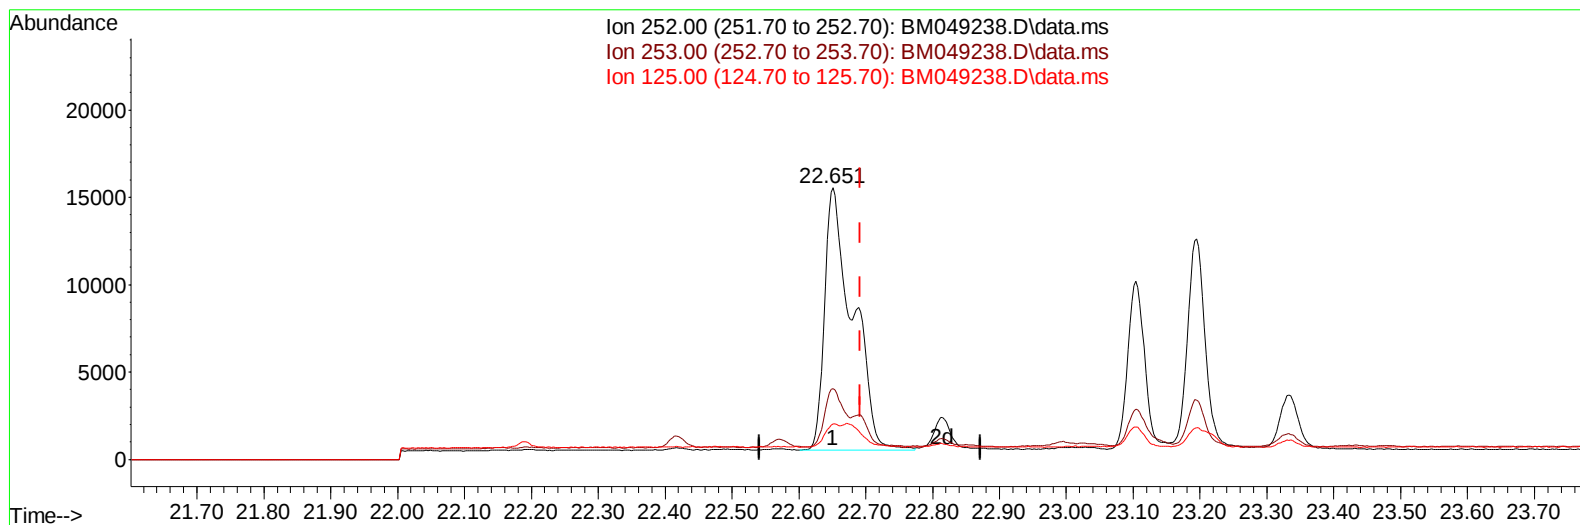

TIC: BM049238.D\data.ms

(25) Benzo(k)fluoranthene

22.651min (-0.041) 0.60 ng/u1

response 43803

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	26.60	26.11
125.00	15.70	13.06
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122624\
Data File : BM049238.D
Acq On : 26 Dec 2024 22:56
Operator : RC/JU
Sample : P5333-14DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2916DL

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/27/2024
Supervised By :mohammad ahmed 12/30/2024

Quant Time: Dec 27 00:46:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 26 11:35:38 2024
Response via : Initial Calibration

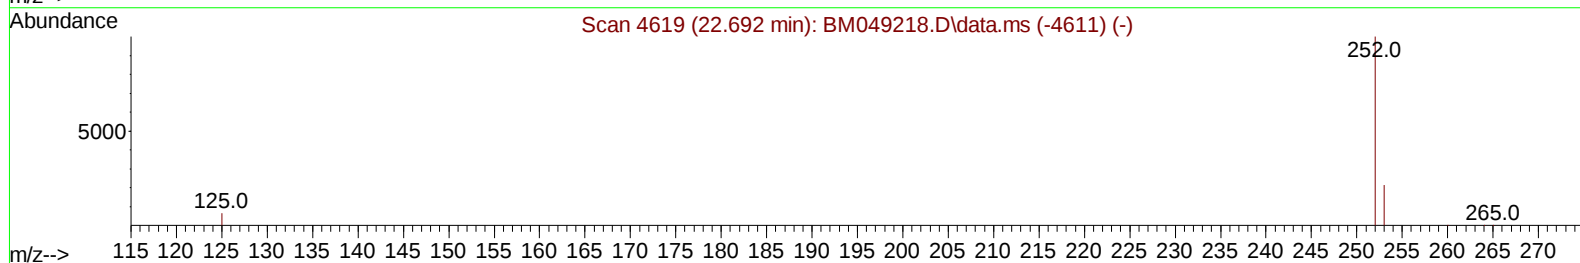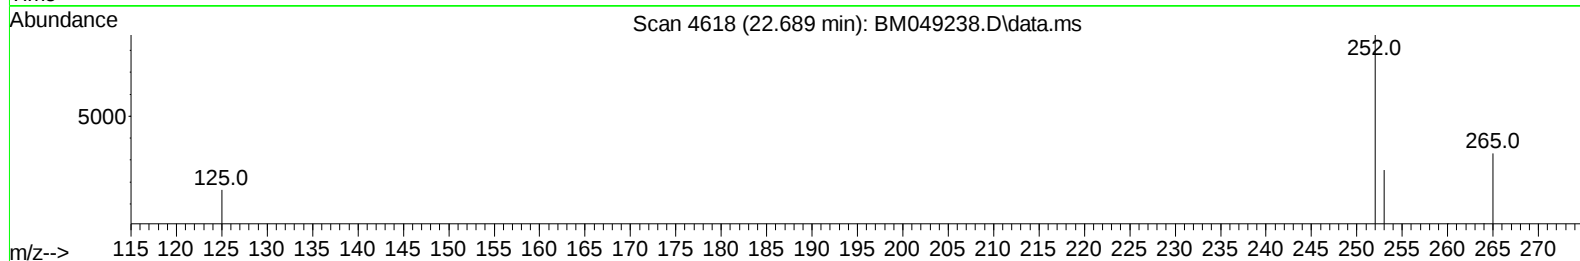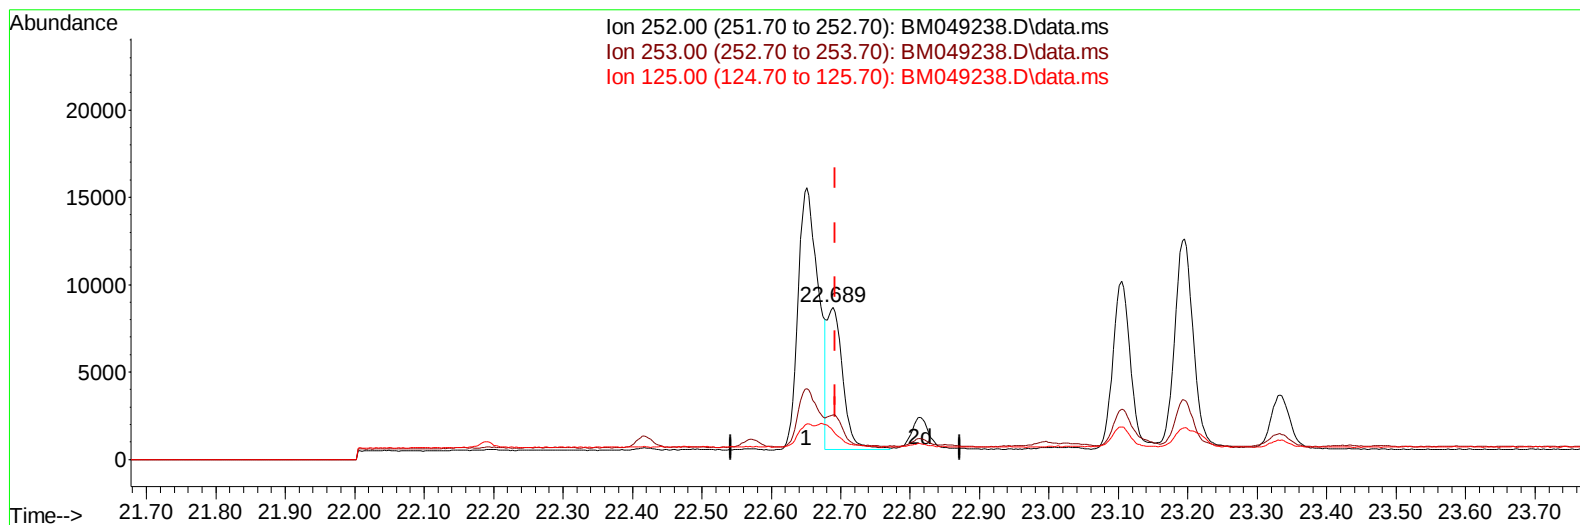

TIC: BM049238.D\data.ms

(25) Benzo(k)fluoranthene

22.689min (-0.003) 0.17 ng/u1 m

response 12752

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	26.60	29.18
125.00	15.70	18.69
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122624\
Data File : BM049238.D
Acq On : 26 Dec 2024 22:56
Operator : RC/JU
Sample : P5333-14DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2916DL

Manual IntegrationsAPPROVED

Quant Time: Dec 27 00:46:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 26 11:35:38 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/27/2024
Supervised By :mohammad ahmed 12/30/2024

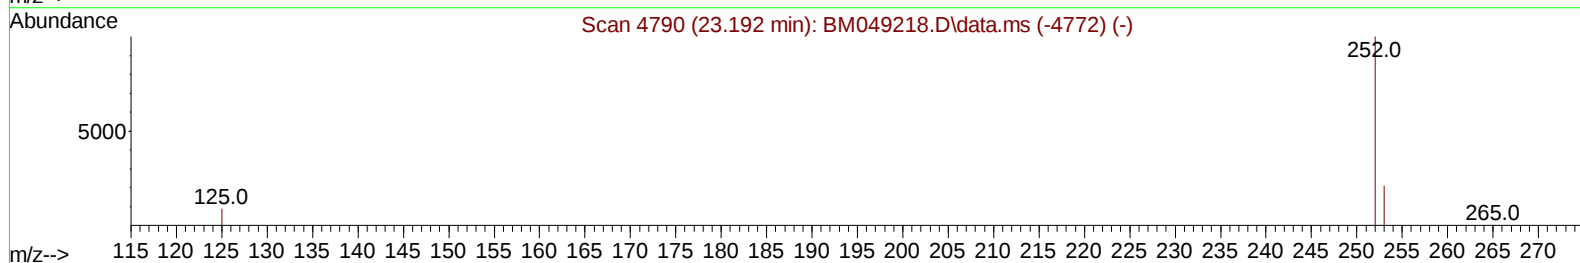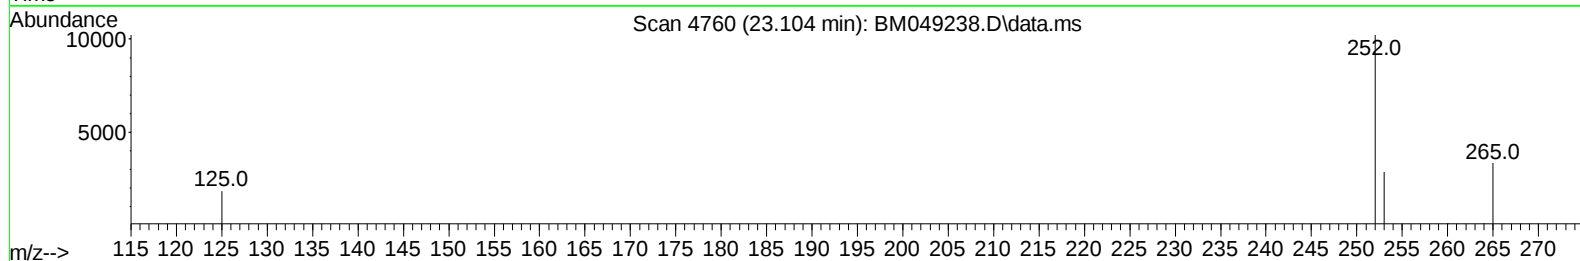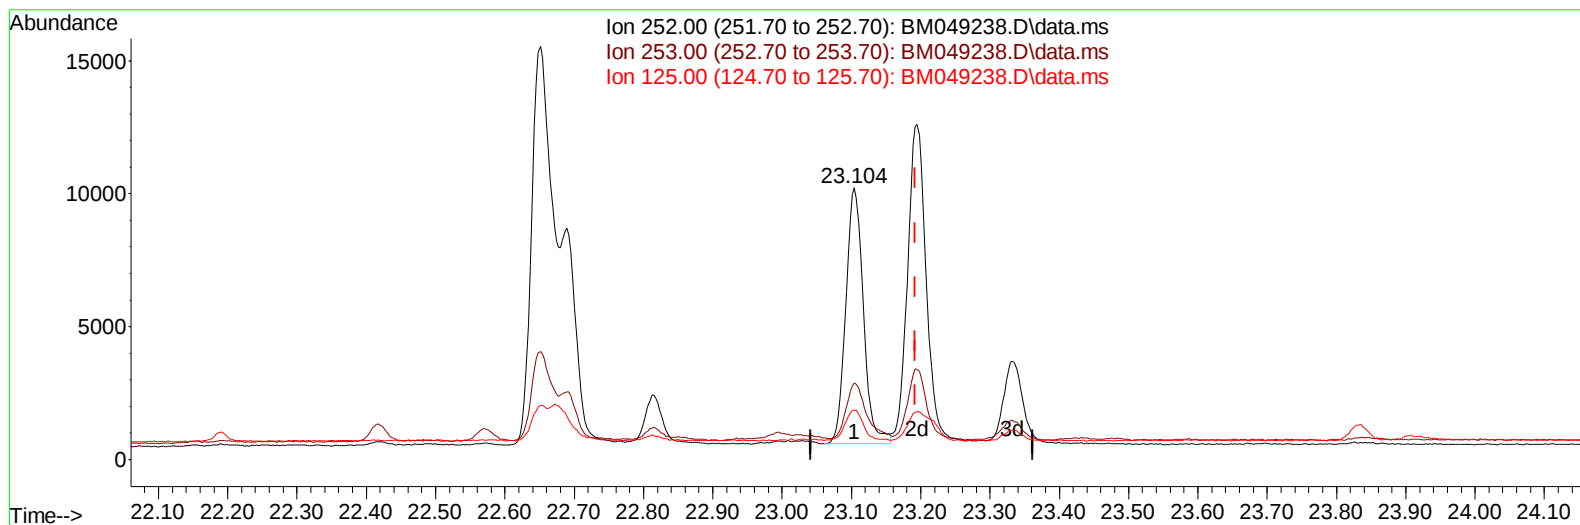

TIC: BM049238.D\data.ms

(26) Benzo(a)pyrene (C)

23.104min (-0.088) 0.27 ng/u1

response 17065

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	28.00	28.18
125.00	18.50	18.07
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122624\
Data File : BM049238.D
Acq On : 26 Dec 2024 22:56
Operator : RC/JU
Sample : P5333-14DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2916DL

Manual IntegrationsAPPROVED

Quant Time: Dec 27 00:46:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 26 11:35:38 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/27/2024
Supervised By :mohammad ahmed 12/30/2024

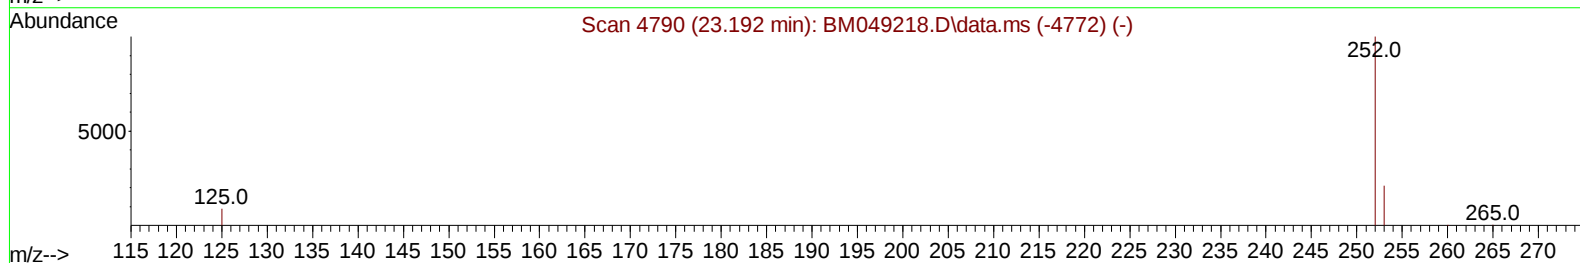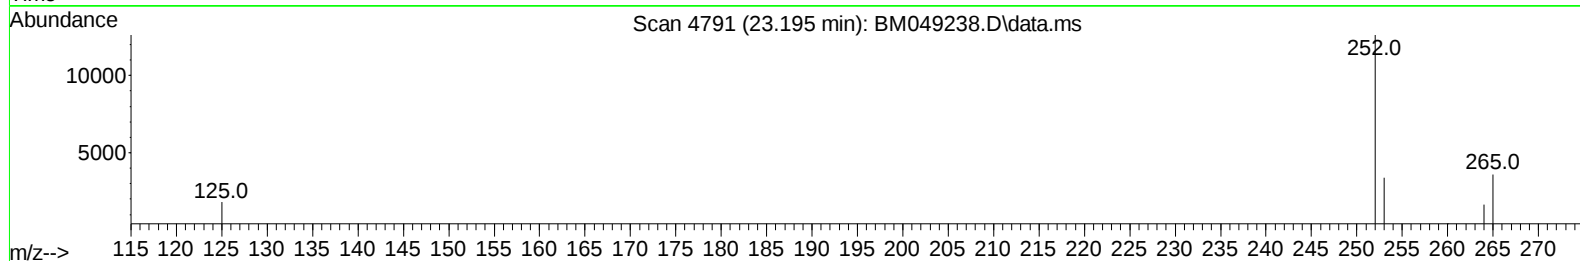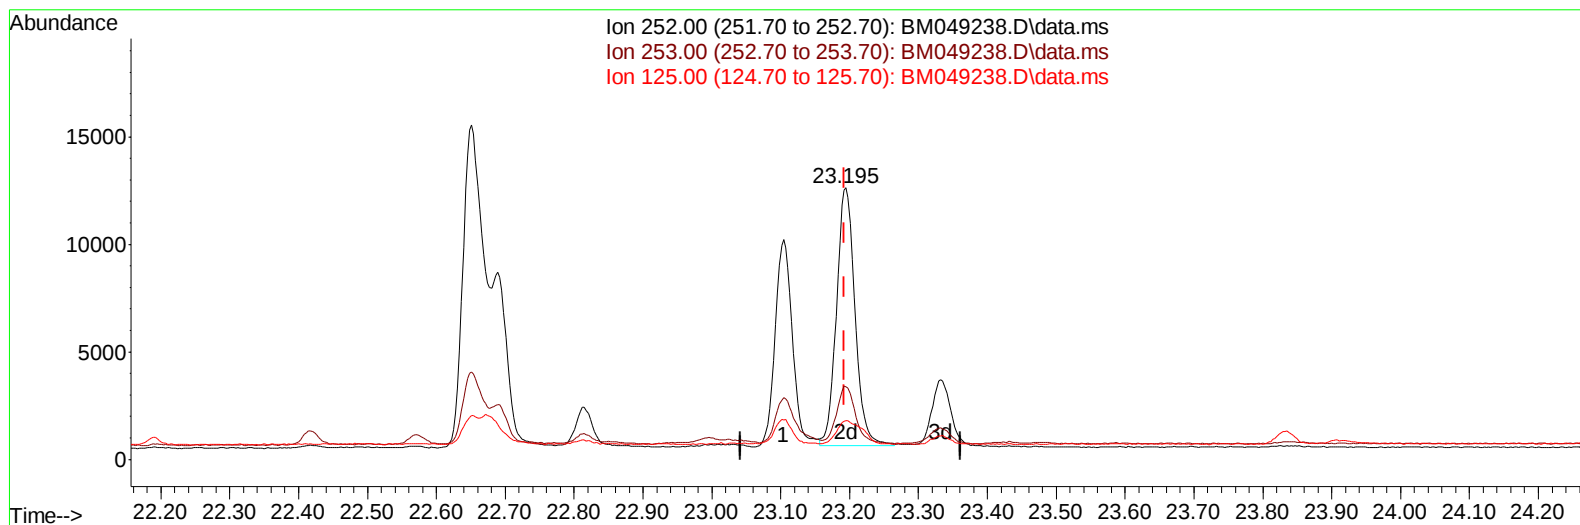

TIC: BM049238.D\data.ms

(26) Benzo(a)pyrene (C)

23.195min (+ 0.003) 0.35 ng/u1 m

response 22279

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	28.00	26.85
125.00	18.50	14.30#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122624\
 Data File : BM049238.D
 Acq On : 26 Dec 2024 22:56
 Operator : RC/JU
 Sample : P5333-14DL 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E2916DL

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 12/27/2024
 Supervised By :mohammad ahmed 12/30/2024

Quant Time: Dec 27 00:46:48 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 26 11:35:38 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.544	152		5384	0.400	ng/ul	0.00
4) Naphthalene-d8	10.308	136		16715	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.182	164		10451	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.933	188		23044	0.400	ng/ul	0.00
17) Chrysene-d12	21.135	240		19057	0.400	ng/ul	0.00
23) Perylene-d12	23.288	264		20829	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.139	96		3945	0.635	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.914	152		804	0.036	ng/ul	0.00
18) Fluoranthene-d10	18.968	212		1759	0.033	ng/ul	0.00
Target Compounds							
							Qvalue
5) Naphthalene	10.358	128		1363	0.033	ng/ul#	81
7) 2-Methylnaphthalene	11.991	142		934	0.035	ng/ul	94
15) Phenanthrene	16.971	178		9273	0.154	ng/ul	99
16) Anthracene	17.064	178		1876	0.034	ng/ul#	85
19) Fluoranthene	18.996	202		25547	0.371	ng/ul	99
20) Pyrene	19.359	202		26335	0.358	ng/ul	99
21) Benzo(a)anthracene	21.120	228		15932	0.240	ng/ul	98
22) Chrysene	21.170	228		19924	0.280	ng/ul	97
24) Benzo(b)fluoranthene	22.651	252		30941m	0.465	ng/ul	
25) Benzo(k)fluoranthene	22.689	252		12752m	0.175	ng/ul	
26) Benzo(a)pyrene	23.195	252		22279m	0.349	ng/ul	
27) Indeno(1,2,3-cd)pyrene	25.420	276		18637	0.206	ng/ul#	90
28) Dibenzo(a,h)anthracene	25.427	278		3972	0.057	ng/ul#	80
29) Benzo(g,h,i)perylene	26.064	276		19339	0.266	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM122624\
Data File : BM049238.D
Acq On : 26 Dec 2024 22:56
Operator : RC/JU
Sample : P5333-14DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E2916DL

Manual IntegrationsAPPROVED

Quant Time: Dec 27 00:46:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM121824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 26 11:35:38 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 12/27/2024
Supervised By :mohammad ahmed 12/30/2024

